

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051625\
 Data File : PL095729.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2025 15:41
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 01:57:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
 Quant Title : GC Extractables
 QLast Update : Tue May 13 14:38:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.591	2.908	77988938	91752894	19.087	19.588
28)	SA Decachlor...	9.114	8.085	72651882	85251060	21.416	20.668
Target Compounds							
8)	B Heptachlo...	5.723	0.000	106.4E6	0	20.528	N.D. #
13)	MA Dieldrin	0.000	5.552f	0	25832842	N.D.	4.199 #
14)	MA Endrin	0.000	5.810	0	25499592	N.D.	4.786 #
15)	B Endosulfa...	6.810f	6.091	9844822	7958342	2.362	1.453 #
16)	A 4,4'-DDD	6.730f	0.000	11217092	0	2.887	N.D. #
17)	MA 4,4'-DDT	7.080f	0.000	20987726	0	5.833	N.D. #
24)	Chlordane-2	0.000	4.498	0	3537983	N.D.	13.294 #
27)	Chlordane-5	0.000	6.091	0	7958342	N.D.	27.708 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051625\
Data File : PL095729.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2025 15:41
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 01:57:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
Quant Title : GC Extractables
QLast Update : Tue May 13 14:38:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

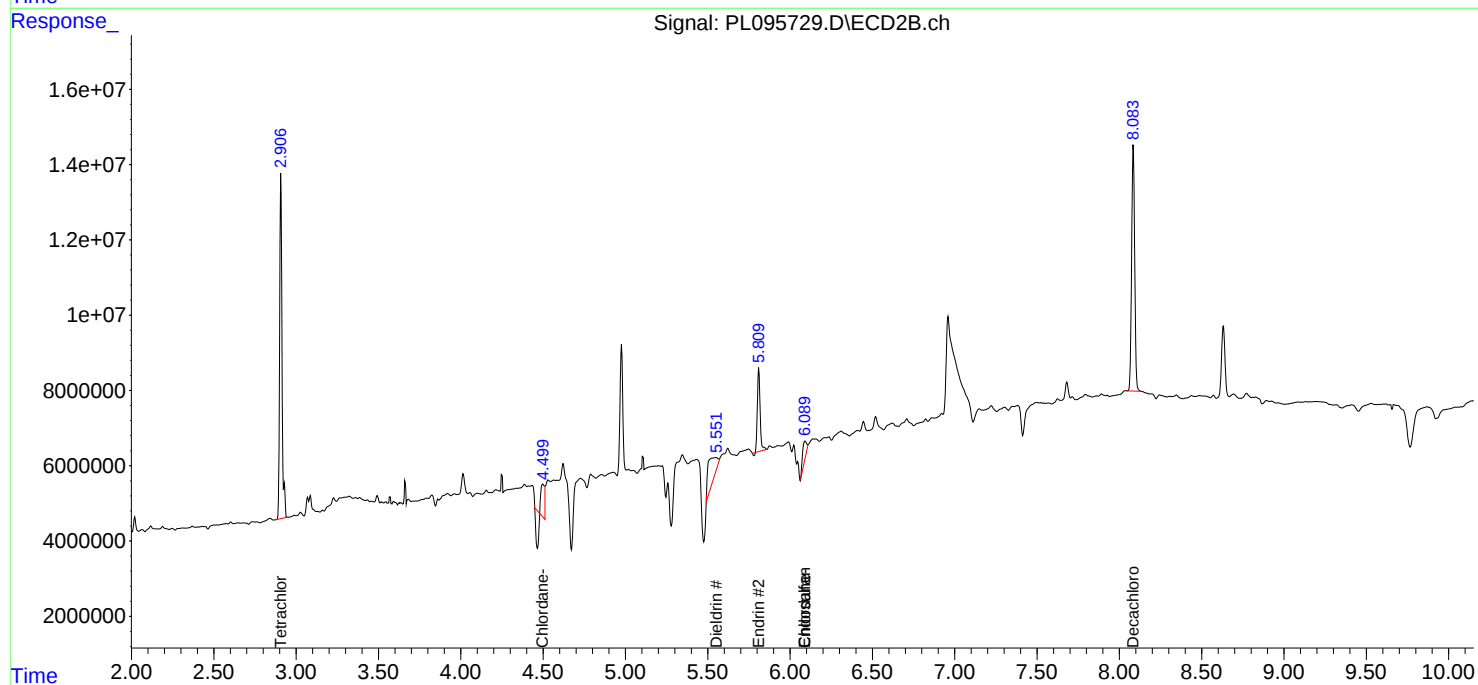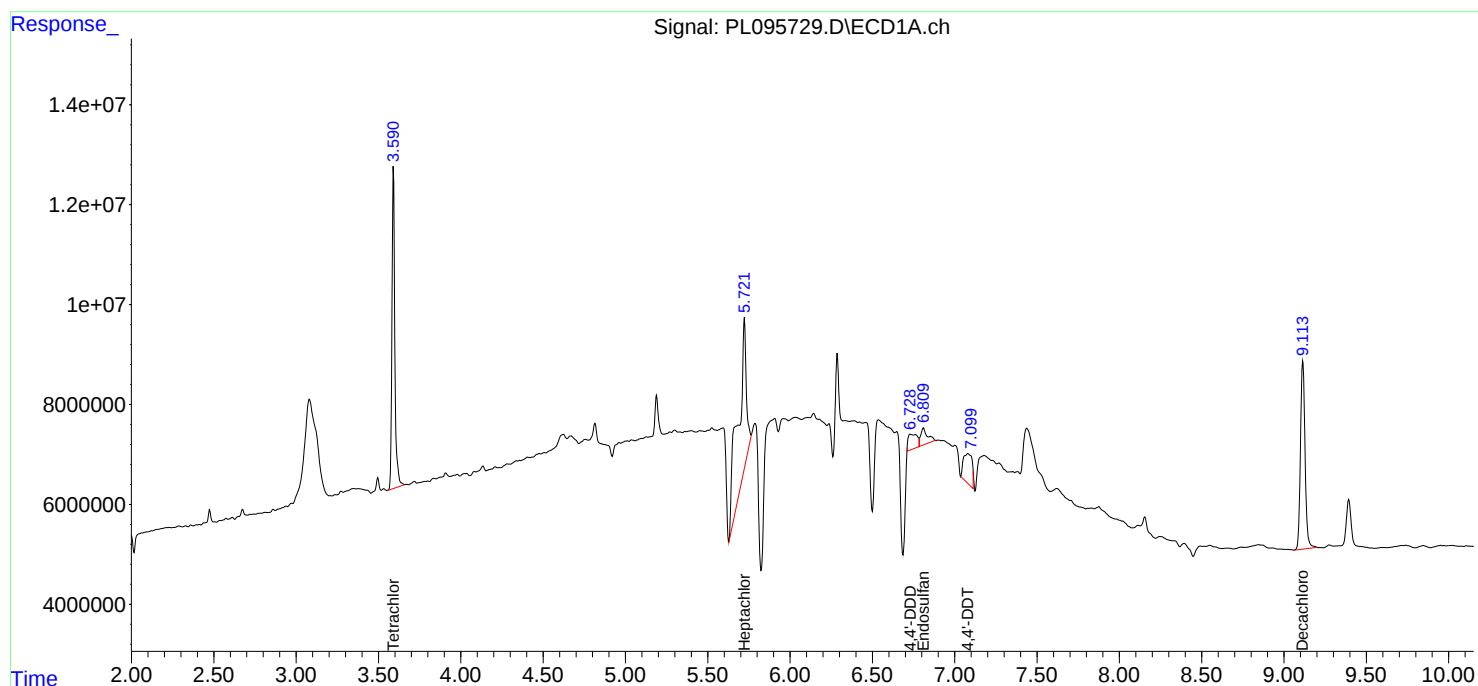


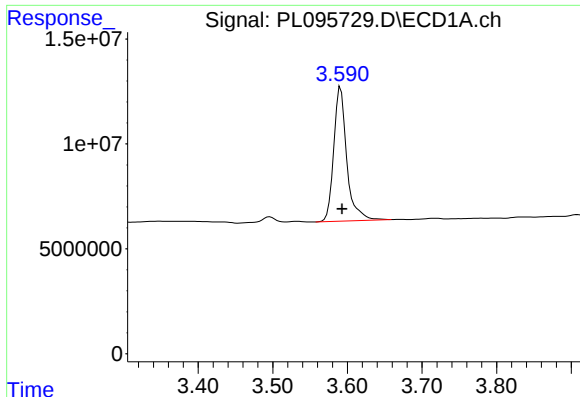

#1 Tetrachloro-m-xylene


R.T.: 3.591 min
Delta R.T.: -0.002 min
Response: 77988938
Conc: 19.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

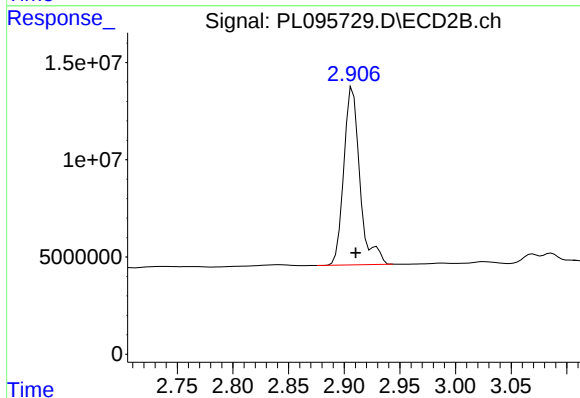


#1 Tetrachloro-m-xylene

R.T.: 2.908 min
Delta R.T.: -0.003 min
Response: 91752894
Conc: 19.59 ng/ml

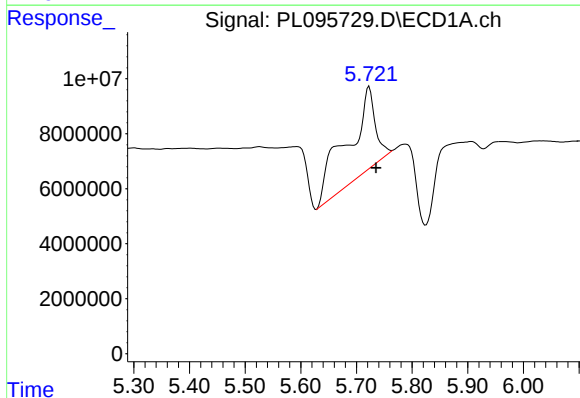


#8 Heptachlor epoxide

R.T.: 5.723 min
Delta R.T.: -0.012 min
Response: 106376489
Conc: 20.53 ng/ml

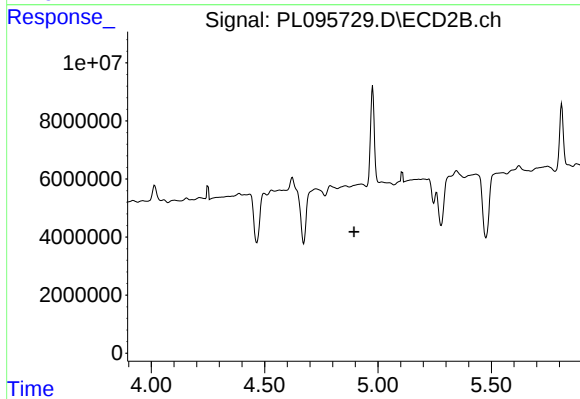

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.895 min
Response: 0
Conc: N.D.

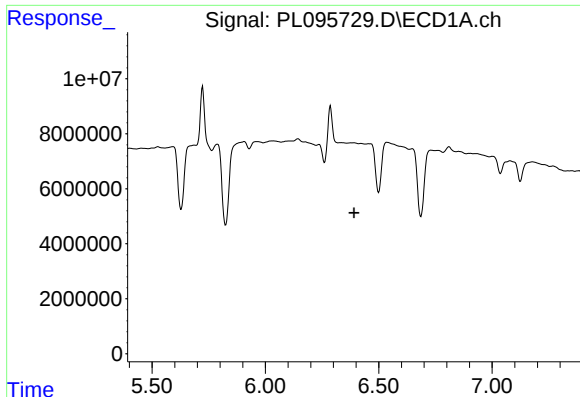

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

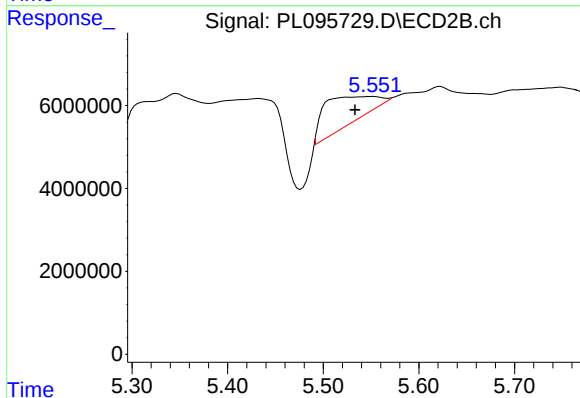


#13 Dieldrin

R.T.: 5.552 min
Delta R.T.: 0.019 min
Response: 25832842
Conc: 4.20 ng/ml

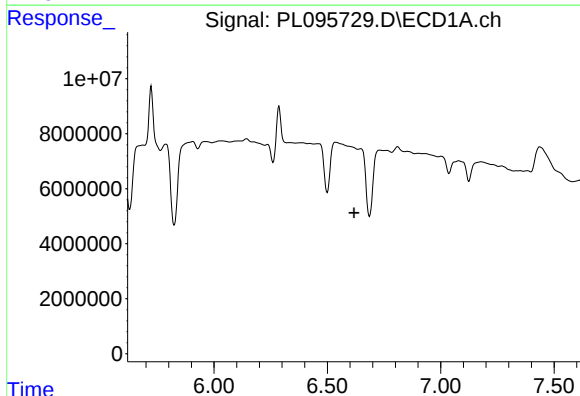


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.619 min
Response: 0
Conc: N.D.

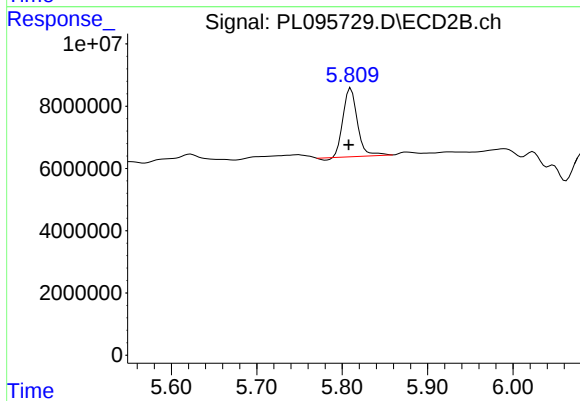

#14 Endrin


R.T.: 5.810 min
Delta R.T.: 0.002 min
Response: 25499592
Conc: 4.79 ng/ml

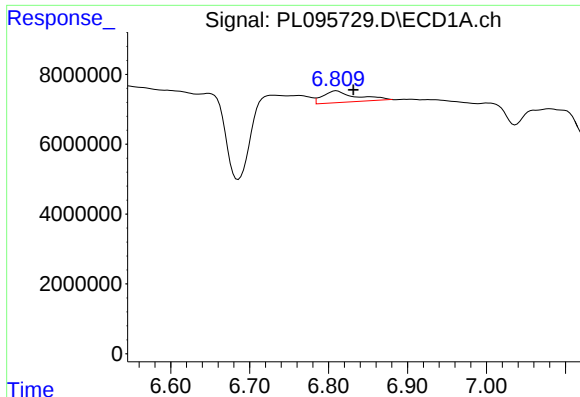

#15 Endosulfan II


R.T.: 6.810 min
Delta R.T.: -0.021 min
Response: 9844822
Conc: 2.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

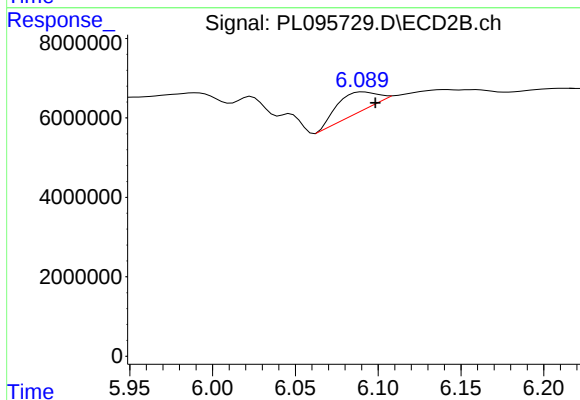


#15 Endosulfan II

R.T.: 6.091 min
Delta R.T.: -0.007 min
Response: 7958342
Conc: 1.45 ng/ml

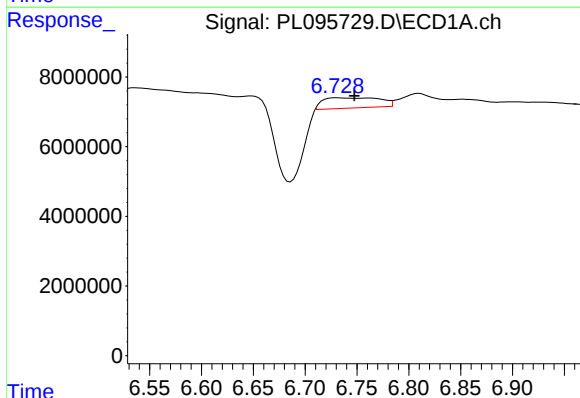


#16 4,4'-DDD

R.T.: 6.730 min
Delta R.T.: -0.018 min
Response: 11217092
Conc: 2.89 ng/ml

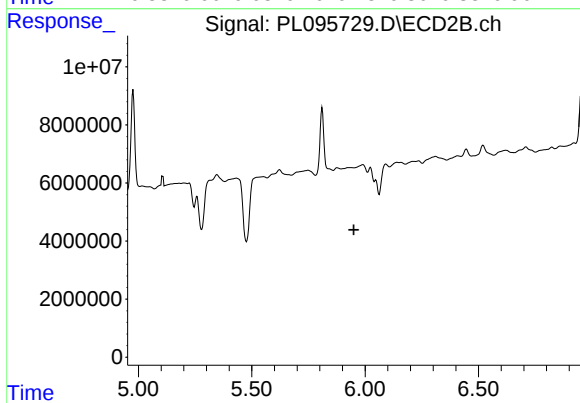

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.949 min
Response: 0
Conc: N.D.

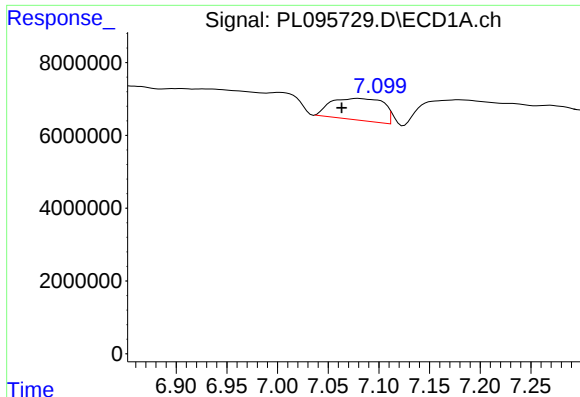

#17 4,4'-DDT


R.T.: 7.080 min
Delta R.T.: 0.016 min
Response: 20987726
Conc: 5.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

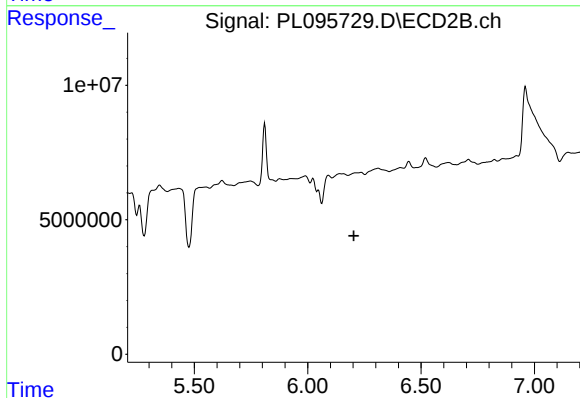


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.203 min
Response: 0
Conc: N.D.

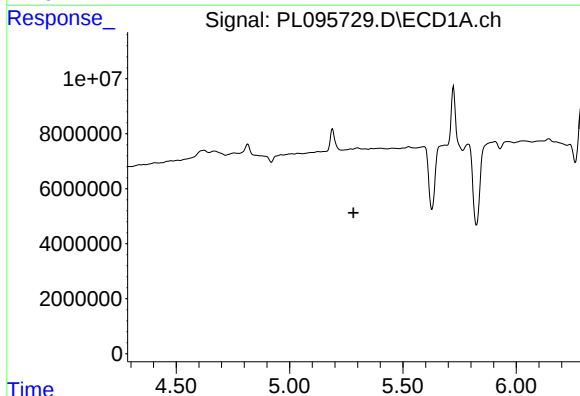


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.282 min
Response: 0
Conc: N.D.

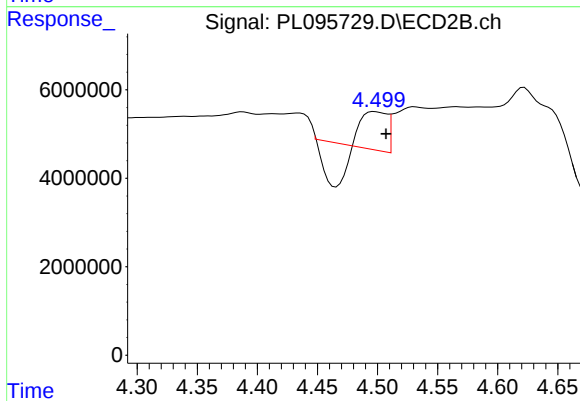

#24 Chlordane-2


R.T.: 4.498 min
Delta R.T.: -0.010 min
Response: 3537983
Conc: 13.29 ng/ml

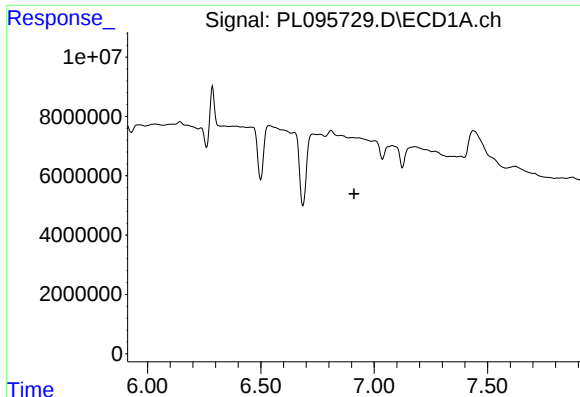

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.911 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

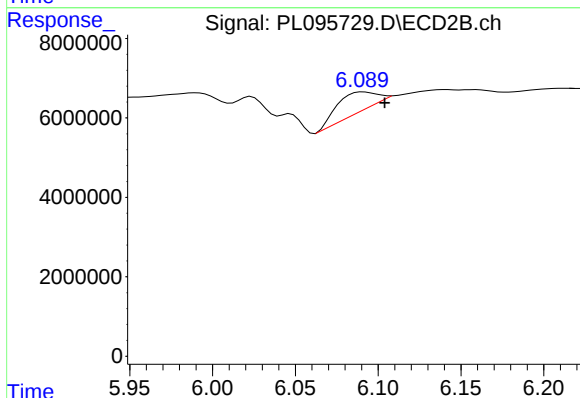


#27 Chlordane-5

R.T.: 6.091 min
Delta R.T.: -0.013 min
Response: 7958342
Conc: 27.71 ng/ml

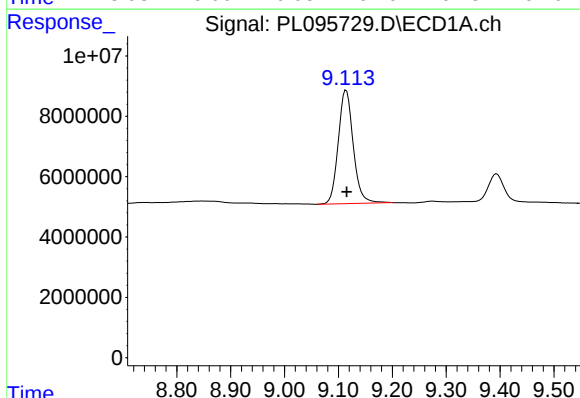

#28 Decachlorobiphenyl

R.T.: 9.114 min
Delta R.T.: 0.000 min
Response: 72651882
Conc: 21.42 ng/ml

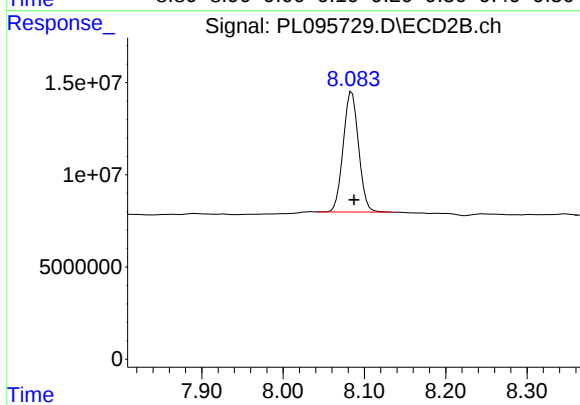

#28 Decachlorobiphenyl

R.T.: 8.085 min
Delta R.T.: -0.003 min
Response: 85251060
Conc: 20.67 ng/ml