

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051719\
 Data File : PL048611.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2019 21:26
 Operator : SM\AJ
 Sample : K2866-07
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RO-COMP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 01:08:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.327	3.940	115.9E6	23298302	11.968	9.353
28)	SA Decachlor...	7.995	8.978	110.9E6	32011222	11.030	12.060
Target Compounds							
10)	B gamma-Chl...	5.192f	0.000	6034388	0	0.452	N.D. #
13)	MA Dieldrin	5.561	0.000	23990330	0	1.842	N.D. #
14)	MA Endrin	5.817	6.629	9846341	2475781	0.809	0.950
15)	B Endosulfa...	6.076	0.000	4535340	0	0.393	N.D. #
16)	A 4,4'-DDD	0.000	6.764	0	8322676	N.D.	3.709 #
17)	MA 4,4'-DDT	6.178	7.029f	28874623	8774909	2.874	3.739 #
18)	B Endrin al...	6.270	0.000	10174592	0	1.047	N.D. #
19)	B Endosulfa...	6.460	7.163f	19362091	3068946	1.804	1.186 #
20)	A Methoxychlor	6.706f	0.000	57919942	0	10.638	N.D. #
21)	B Endrin ke...	6.976f	0.000	8727446	0	0.749	N.D. #
25)	Chlordane-3	5.192f	0.000	6034388	0	3.832	N.D. #
27)	Chlordane-5	6.076f	0.000	4535340	0	9.659	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051719\
Data File : PL048611.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2019 21:26
Operator : SM\AJ
Sample : K2866-07
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
RO-COMP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 01:08:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

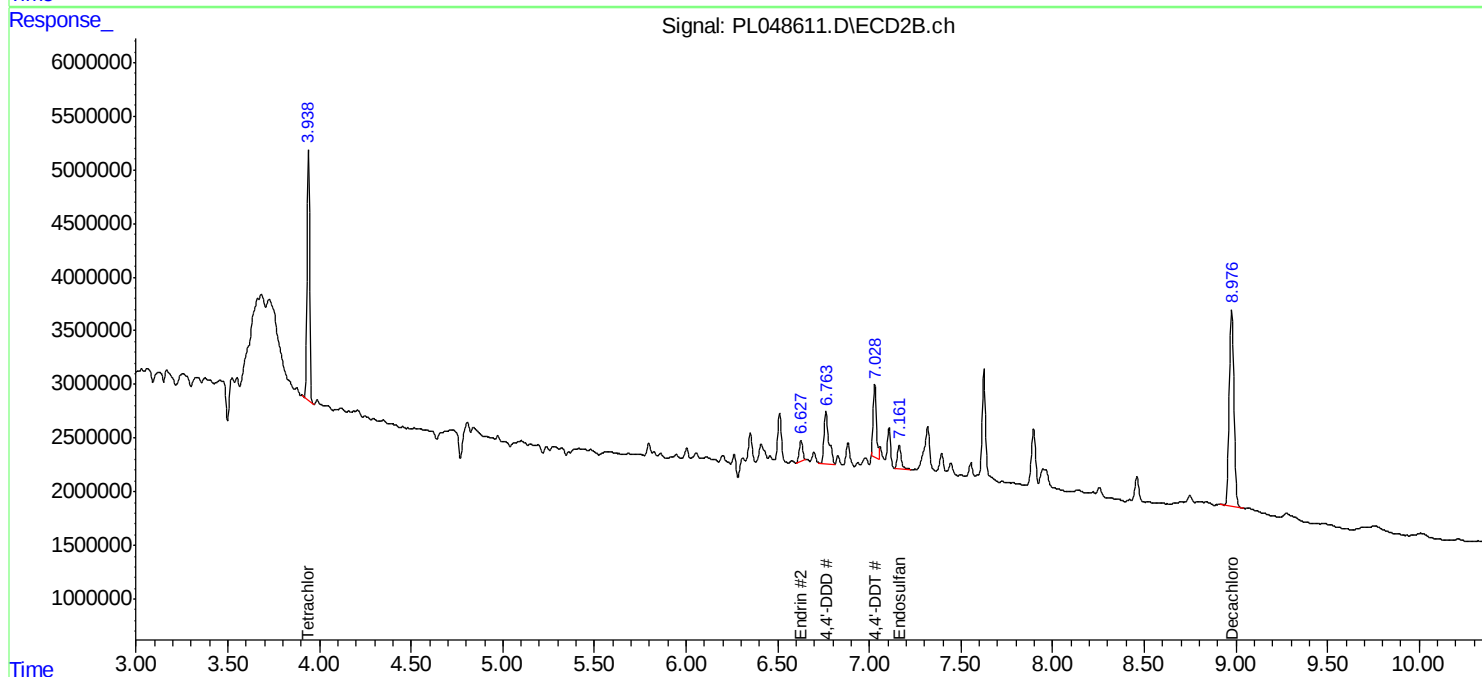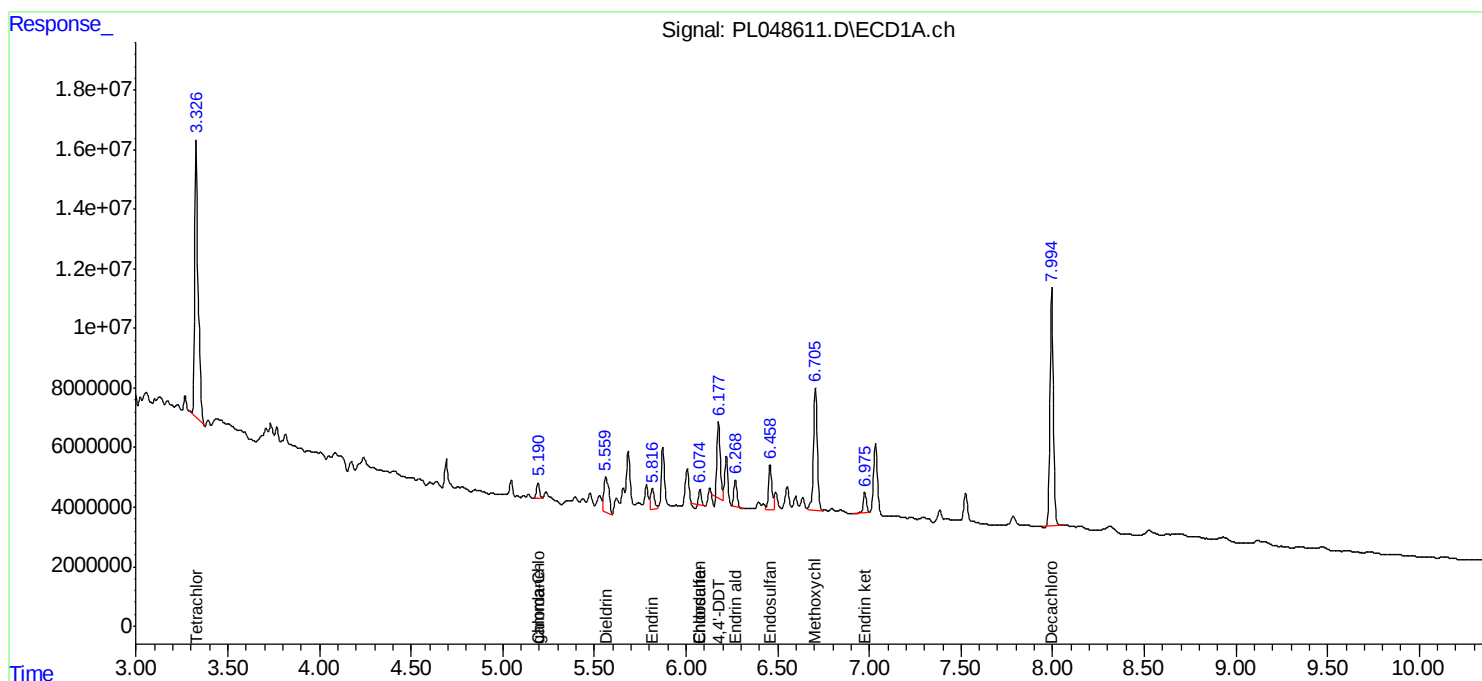


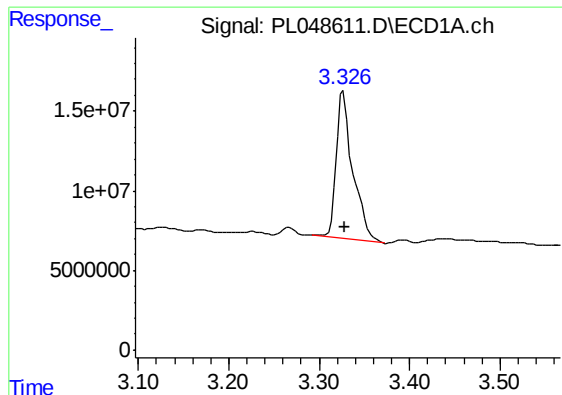

#1 Tetrachloro-m-xylene


R.T.: 3.327 min
Delta R.T.: 0.000 min
Response: 115933590
Conc: 11.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-COMP-3

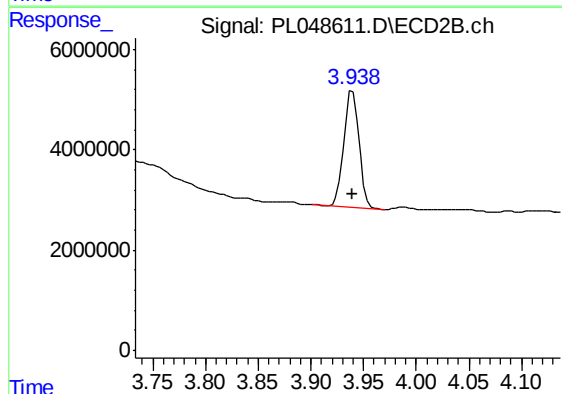


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 23298302
Conc: 9.35 ng/ml

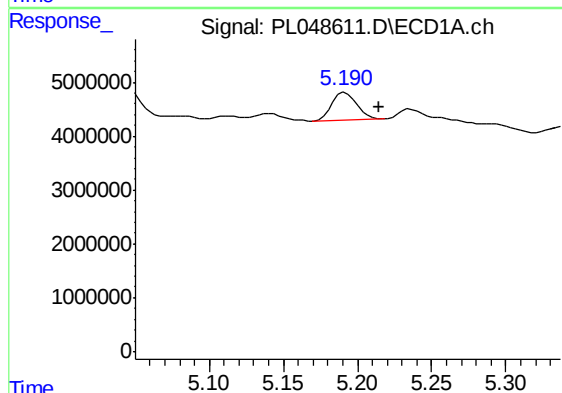


#10 gamma-Chlordane

R.T.: 5.192 min
Delta R.T.: -0.023 min
Response: 6034388
Conc: 0.45 ng/ml

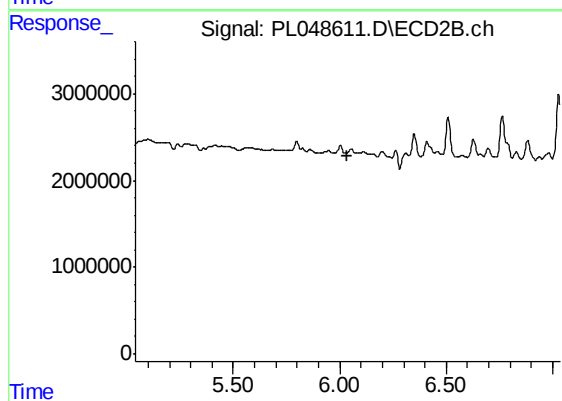

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.



#13 Dieldrin


R.T.: 5.561 min
Delta R.T.: -0.001 min
Response: 23990330
Conc: 1.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-COMP-3

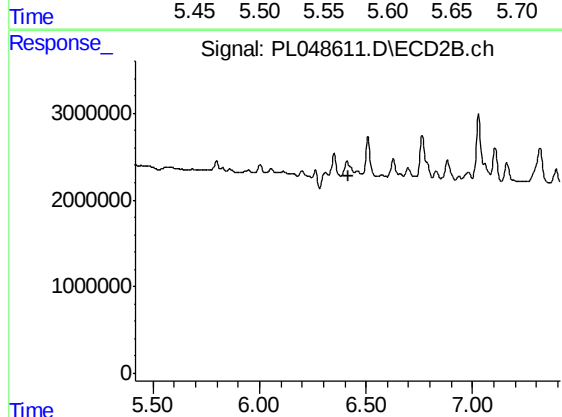


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

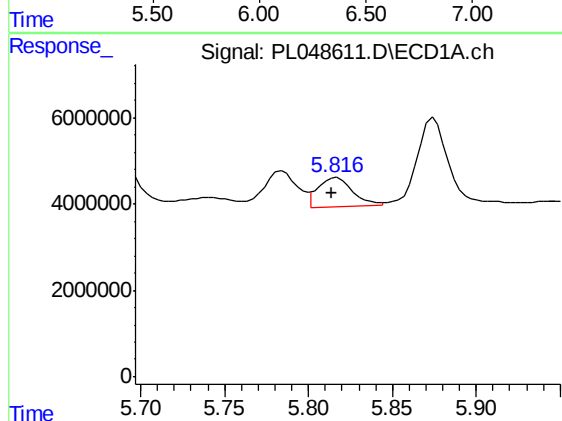


#14 Endrin

R.T.: 5.817 min
Delta R.T.: 0.003 min
Response: 9846341
Conc: 0.81 ng/ml

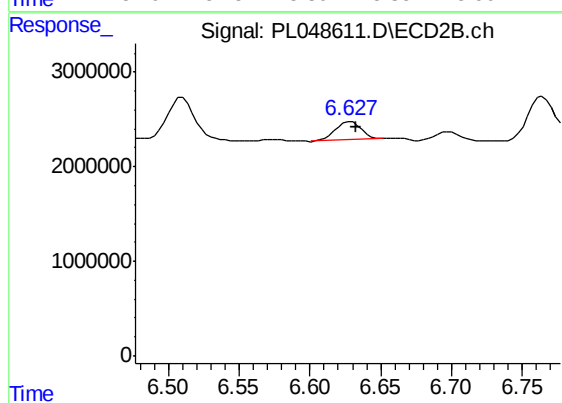

#14 Endrin


R.T.: 6.629 min
Delta R.T.: -0.004 min
Response: 2475781
Conc: 0.95 ng/ml



#15 Endosulfan II


R.T.: 6.076 min
Delta R.T.: -0.013 min
Response: 4535340
Conc: 0.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-COMP-3

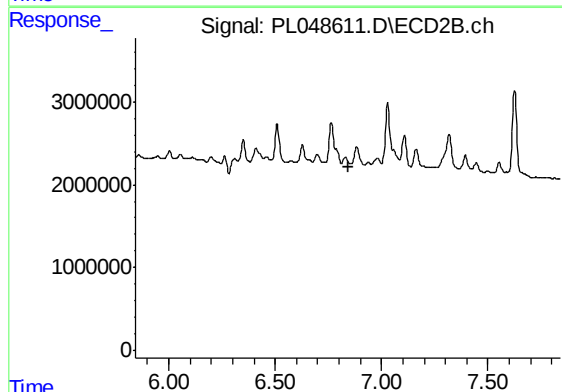


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.843 min
Response: 0
Conc: N.D.




#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

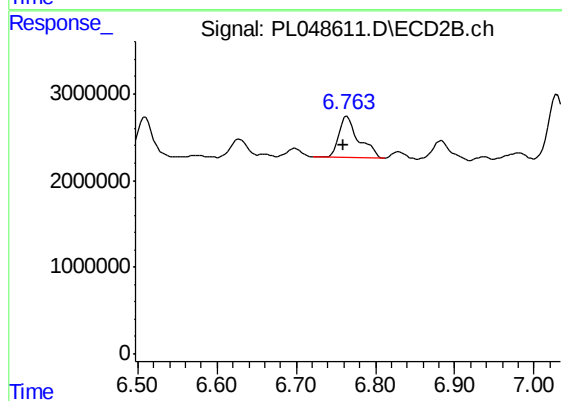

#16 4,4'-DDD


R.T.: 6.764 min
Delta R.T.: 0.005 min
Response: 8322676
Conc: 3.71 ng/ml



#17 4,4'-DDT


R.T.: 6.178 min
Delta R.T.: -0.006 min
Response: 28874623
Conc: 2.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-COMP-3

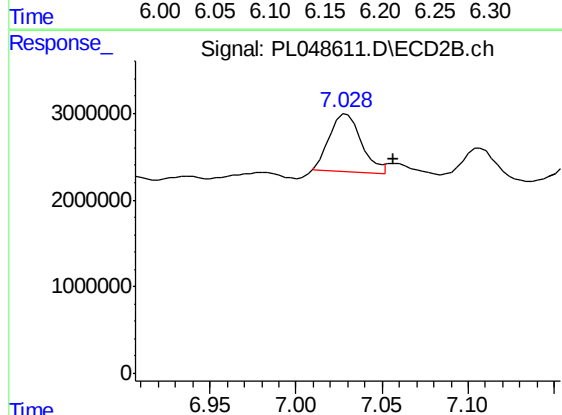


#17 4,4'-DDT

R.T.: 7.029 min
Delta R.T.: -0.027 min
Response: 8774909
Conc: 3.74 ng/ml

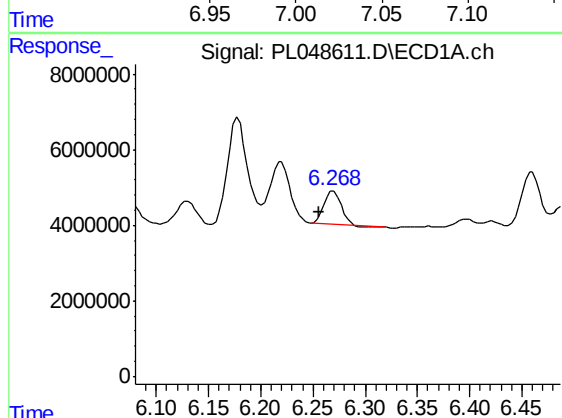


#18 Endrin aldehyde

R.T.: 6.270 min
Delta R.T.: 0.014 min
Response: 10174592
Conc: 1.05 ng/ml

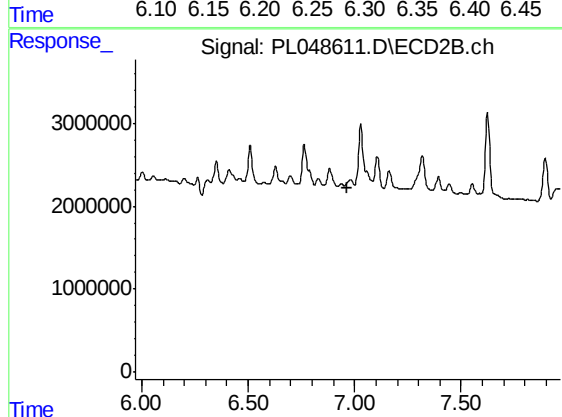

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.967 min
Response: 0
Conc: N.D.



#19 Endosulfan Sulfate


R.T.: 6.460 min
Delta R.T.: -0.008 min
Response: 19362091
Conc: 1.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-COMP-3

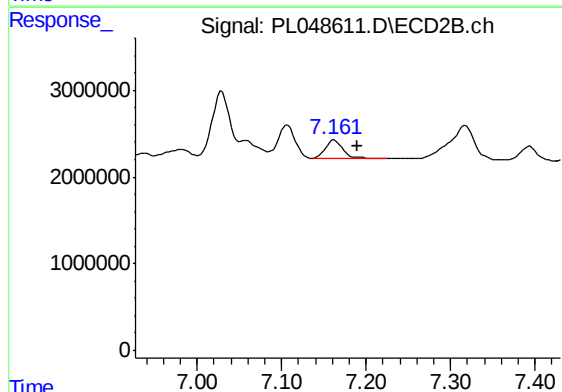


#19 Endosulfan Sulfate

R.T.: 7.163 min
Delta R.T.: -0.027 min
Response: 3068946
Conc: 1.19 ng/ml




#20 Methoxychlor

R.T.: 6.706 min
Delta R.T.: -0.022 min
Response: 57919942
Conc: 10.64 ng/ml

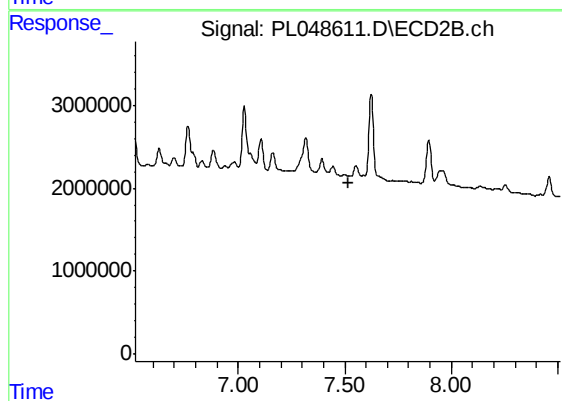

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.516 min
Response: 0
Conc: N.D.



#21 Endrin ketone


R.T.: 6.976 min
Delta R.T.: 0.027 min
Response: 8727446
Conc: 0.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-COMP-3

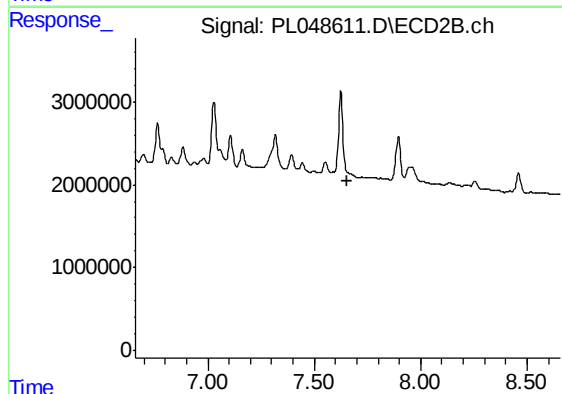


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.658 min
Response: 0
Conc: N.D.




#25 Chlordane-3

R.T.: 5.192 min
Delta R.T.: -0.024 min
Response: 6034388
Conc: 3.83 ng/ml

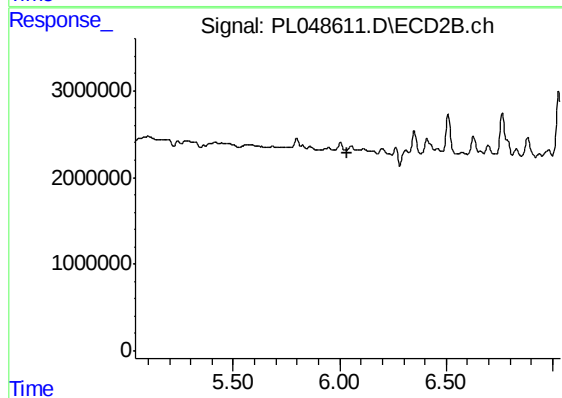

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.



#27 Chlordane-5


R.T.: 6.076 min
Delta R.T.: -0.015 min
Response: 4535340
Conc: 9.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-COMP-3

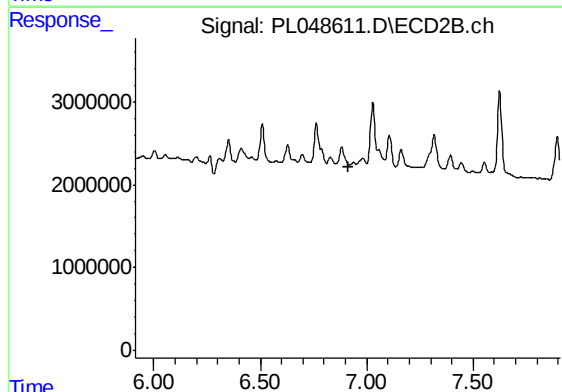


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.913 min
Response: 0
Conc: N.D.



#28 Decachlorobiphenyl

R.T.: 7.995 min
Delta R.T.: 0.000 min
Response: 110896884
Conc: 11.03 ng/ml

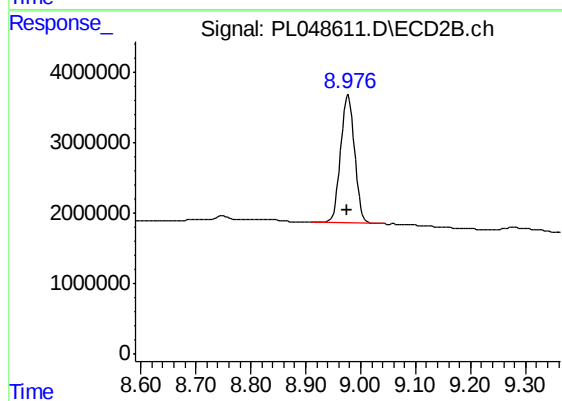

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: 0.003 min
Response: 32011222
Conc: 12.06 ng/ml