

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051719\
 Data File : PL048625.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 May 2019 00:57
 Operator : SM\AJ
 Sample : K2865-08
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-22-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 04:04:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.327	3.940	182.5E6	50653249	18.843	20.335
28)	SA Decachlor...	7.996	8.978	134.9E6	37477779	13.420	14.120
Target Compounds							
7)	B delta-BHC	0.000	4.975f	0	4135245	N.D.	1.462 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051719\
Data File : PL048625.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2019 00:57
Operator : SM\AJ
Sample : K2865-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-22-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 04:04:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

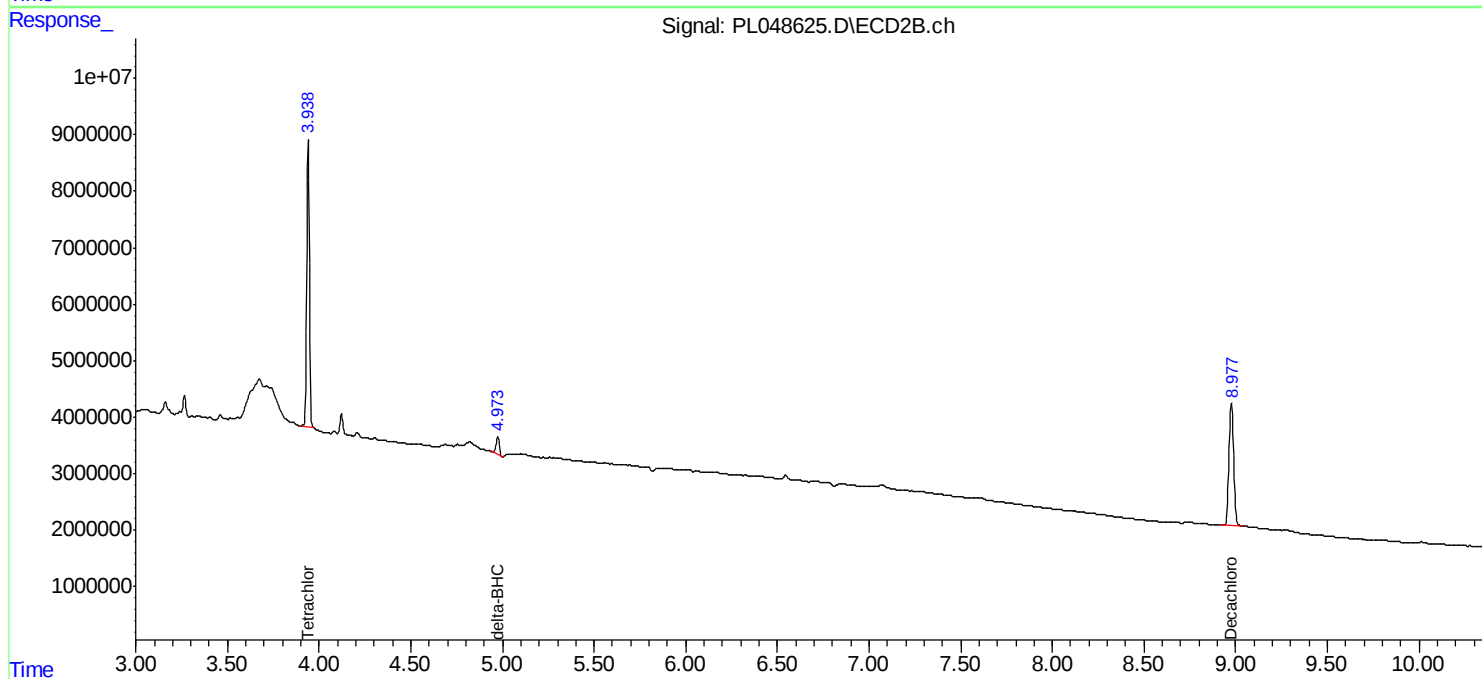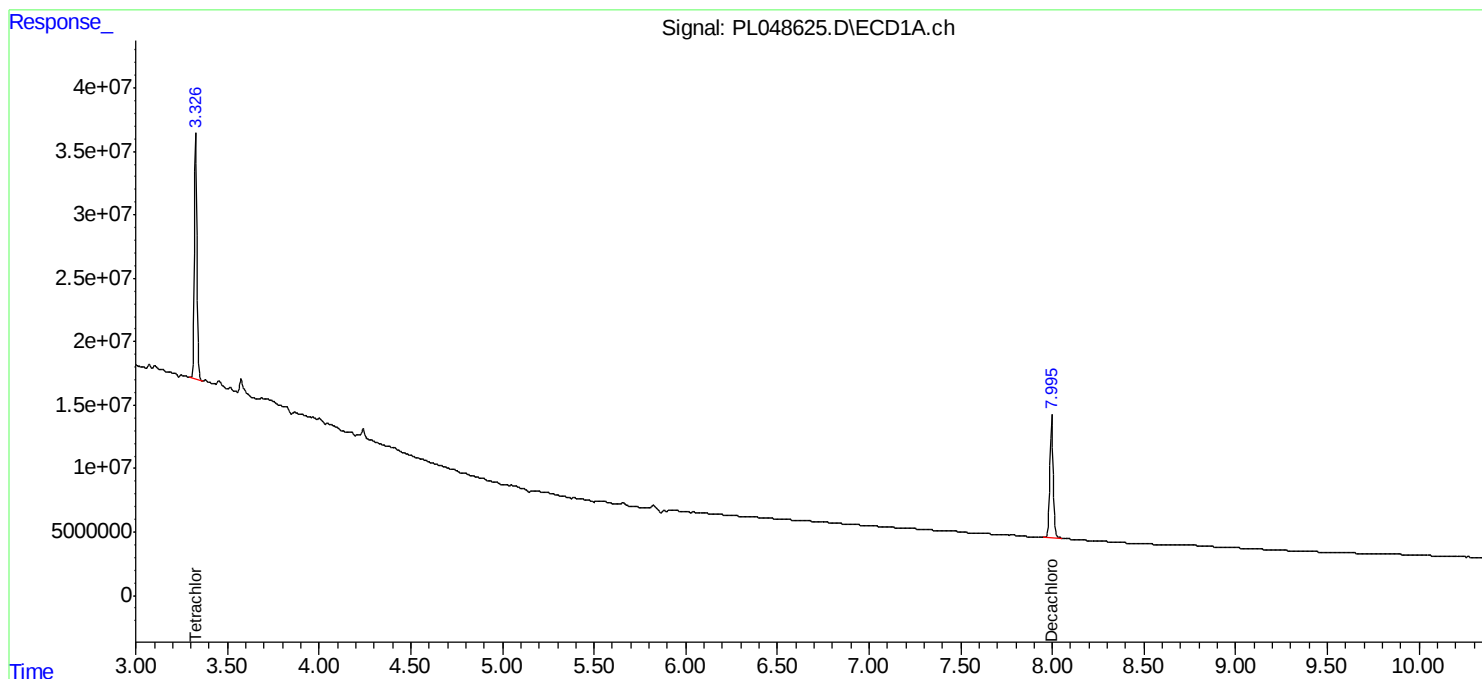


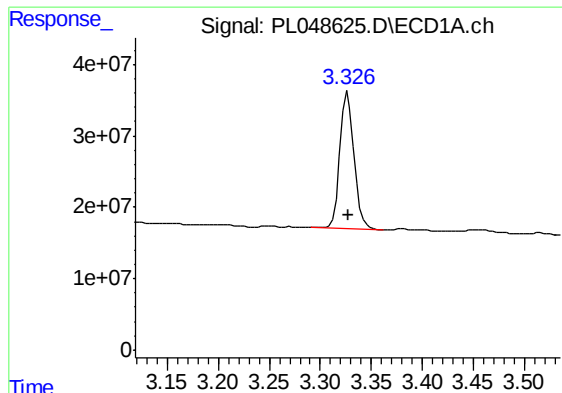

#1 Tetrachloro-m-xylene


R.T.: 3.327 min
Delta R.T.: 0.000 min
Response: 182527209
Conc: 18.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-22-S

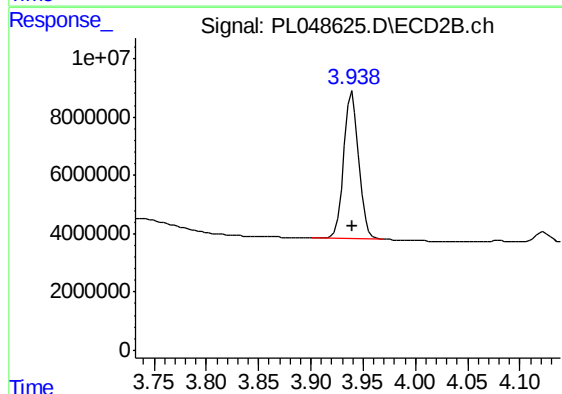


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 50653249
Conc: 20.34 ng/ml

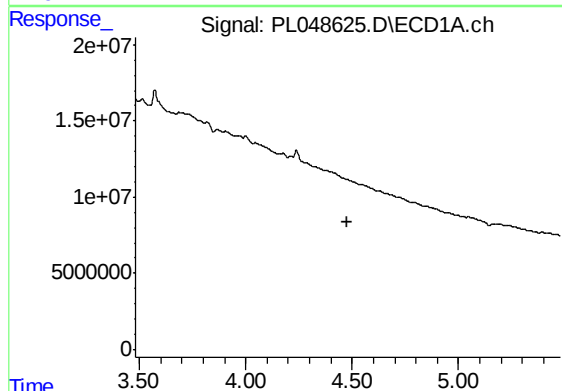


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

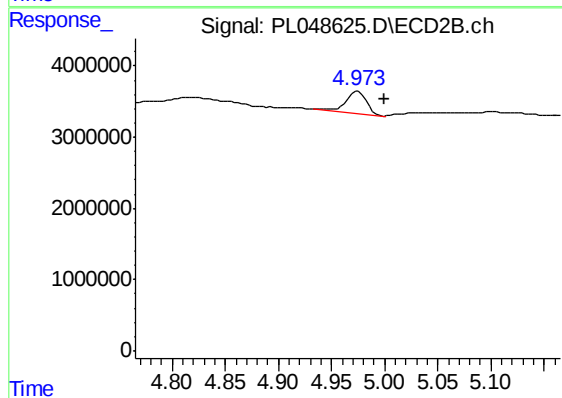

#7 delta-BHC


R.T.: 4.975 min
Delta R.T.: -0.025 min
Response: 4135245
Conc: 1.46 ng/ml

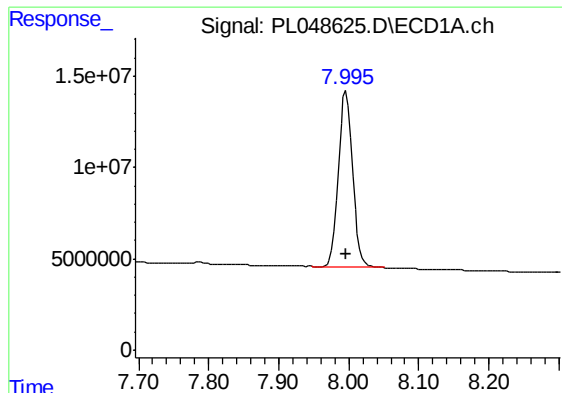

#28 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: 0.000 min
Response: 134927956
Conc: 13.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-22-S

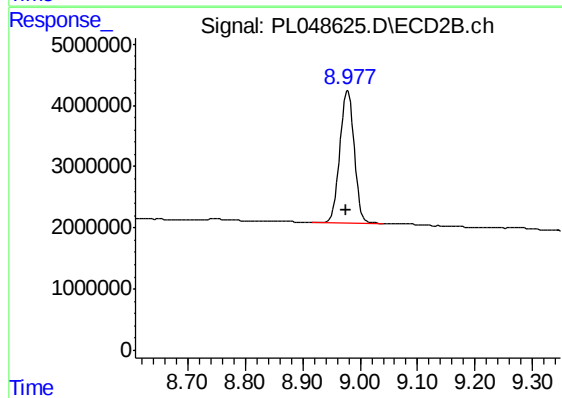

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: 0.003 min
Response: 37477779
Conc: 14.12 ng/ml