

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051719\
 Data File : PL048606.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2019 20:11
 Operator : SM\AJ
 Sample : K2865-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-21-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 01:07:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.327	3.939	84901956	23403614	8.765	9.396
28)	SA Decachlor...	7.996	8.977	94915051	28217495	9.440	10.631
Target Compounds							
12)	B 4,4'-DDE	5.437	6.270	15051648	3960520	1.187	1.434



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051719\
Data File : PL048606.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2019 20:11
Operator : SM\AJ
Sample : K2865-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-21-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 01:07:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

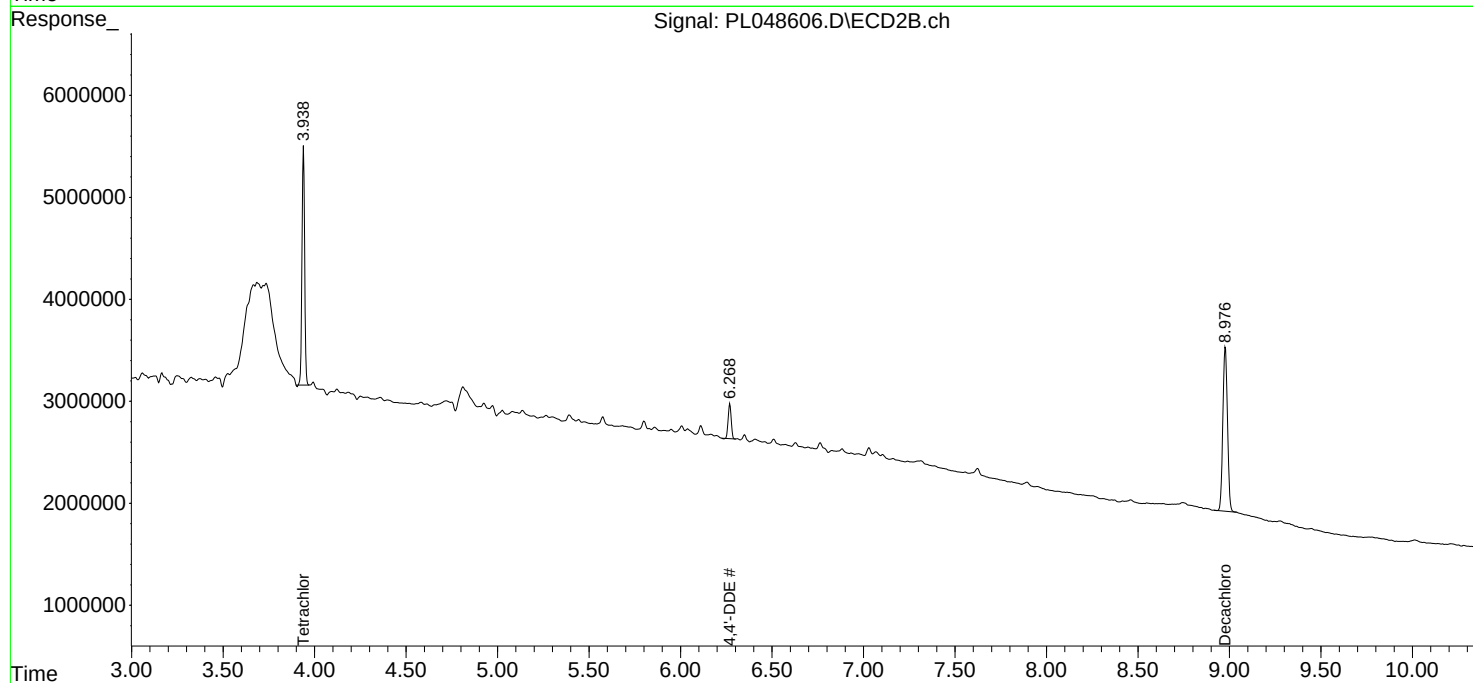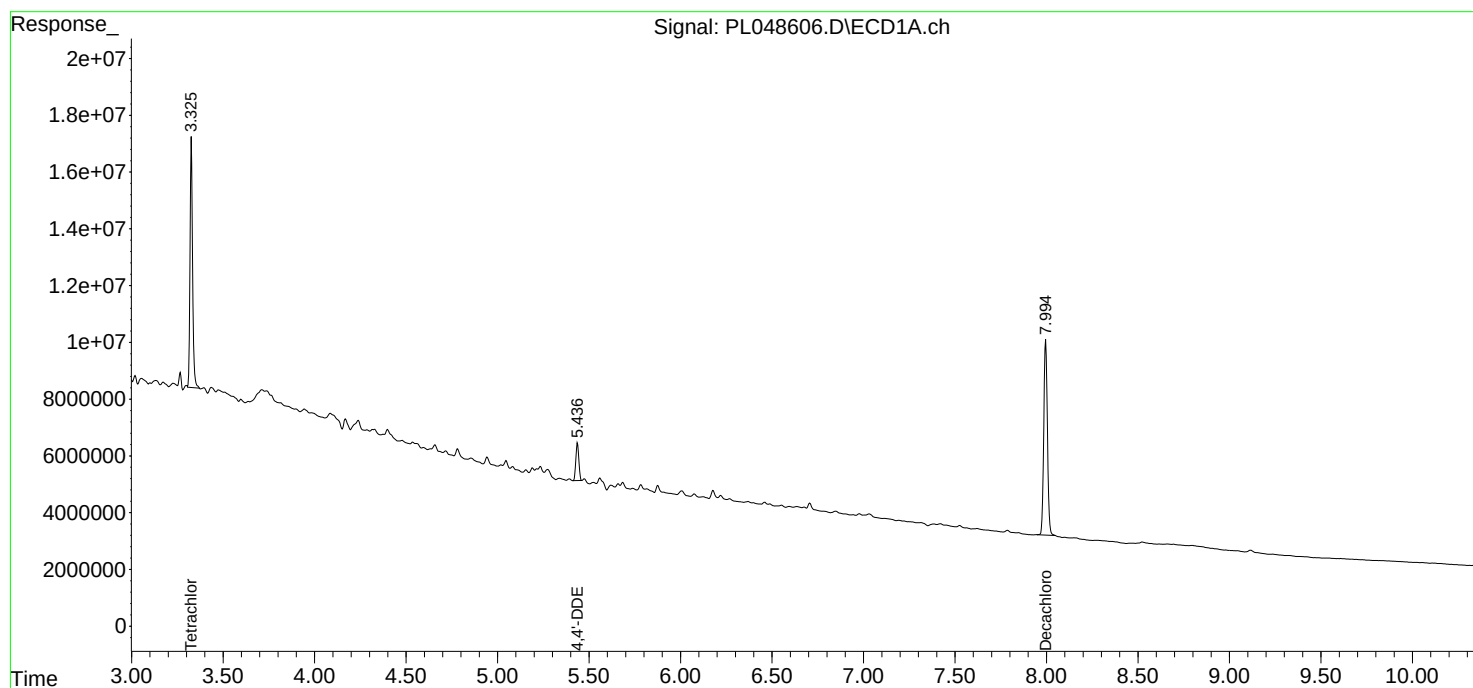


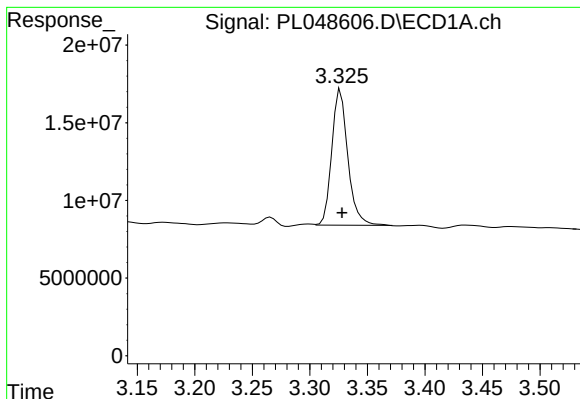

#1 Tetrachloro-m-xylene


R.T.: 3.327 min
Delta R.T.: -0.001 min
Response: 84901956
Conc: 8.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-21-S

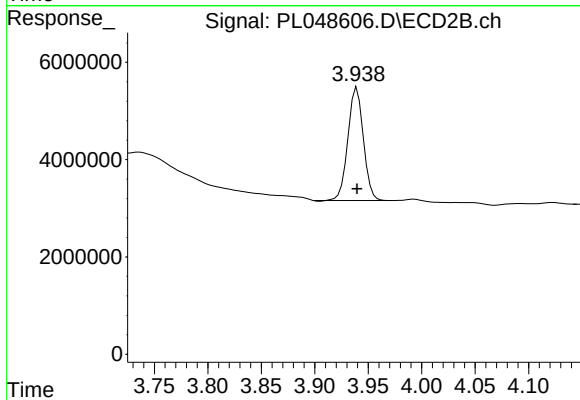


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 23403614
Conc: 9.40 ng/ml

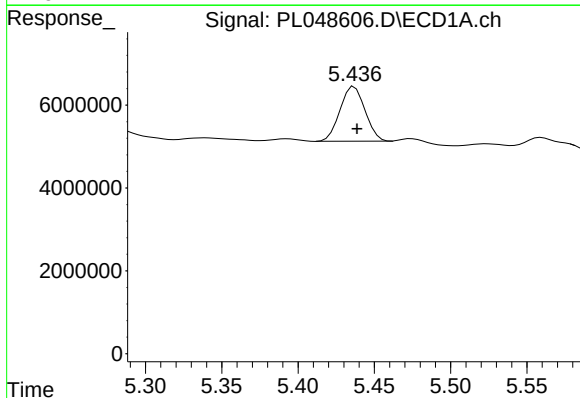


#12 4,4'-DDE

R.T.: 5.437 min
Delta R.T.: -0.002 min
Response: 15051648
Conc: 1.19 ng/ml

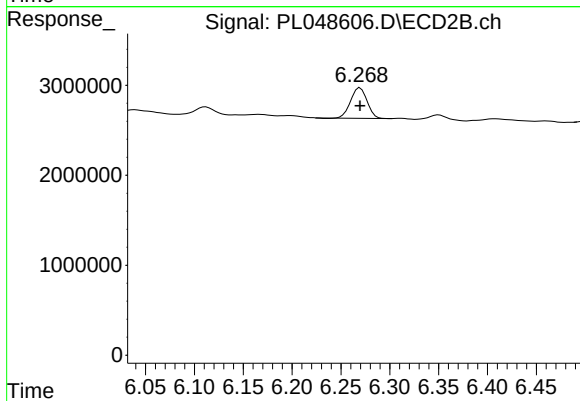

#12 4,4'-DDE

R.T.: 6.270 min
Delta R.T.: 0.000 min
Response: 3960520
Conc: 1.43 ng/ml

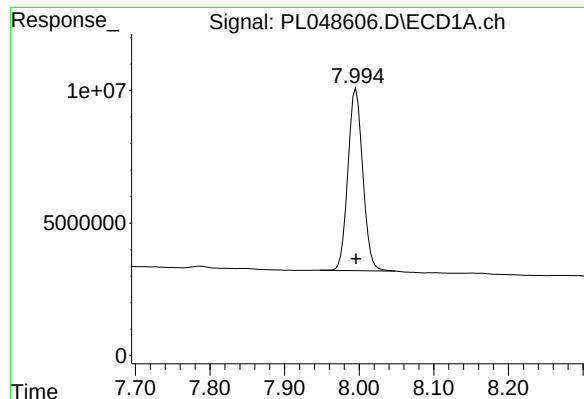

#28 Decachlorobiphenyl


R.T.: 7.996 min

Delta R.T.: 0.000 min

Response: 94915051

Conc: 9.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-21-S

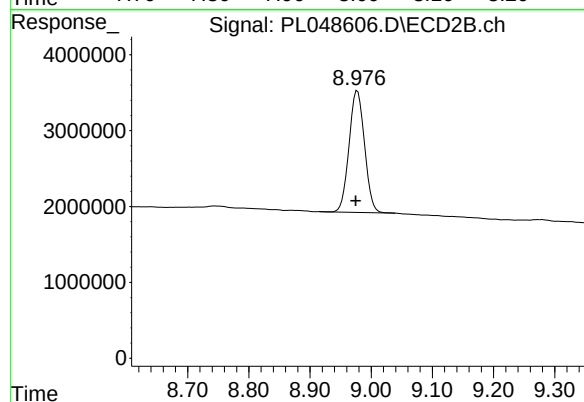

#28 Decachlorobiphenyl

R.T.: 8.977 min

Delta R.T.: 0.002 min

Response: 28217495

Conc: 10.63 ng/ml