

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051719\
 Data File : PL048614.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2019 22:12
 Operator : SM\AJ
 Sample : K2644-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-01-051519-A

Manual Integrations
 APPROVED

Ankita
 5/17/2019 12:27:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 01:09:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.326	3.939	133.4E6	33505749	13.773	13.451
28)	SA Decachlor...	7.996	8.977	128.6E6	39557355	12.789	14.903
Target Compounds							
12)	B 4,4'-DDE	5.435	6.264	6591097	1214757	0.520m	0.440m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051719\
Data File : PL048614.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2019 22:12
Operator : SM\AJ
Sample : K2644-01
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
EO-01-051519-A


Manual Integrations
APPROVED

Ankita
5/17/2019 12:27:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 01:09:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

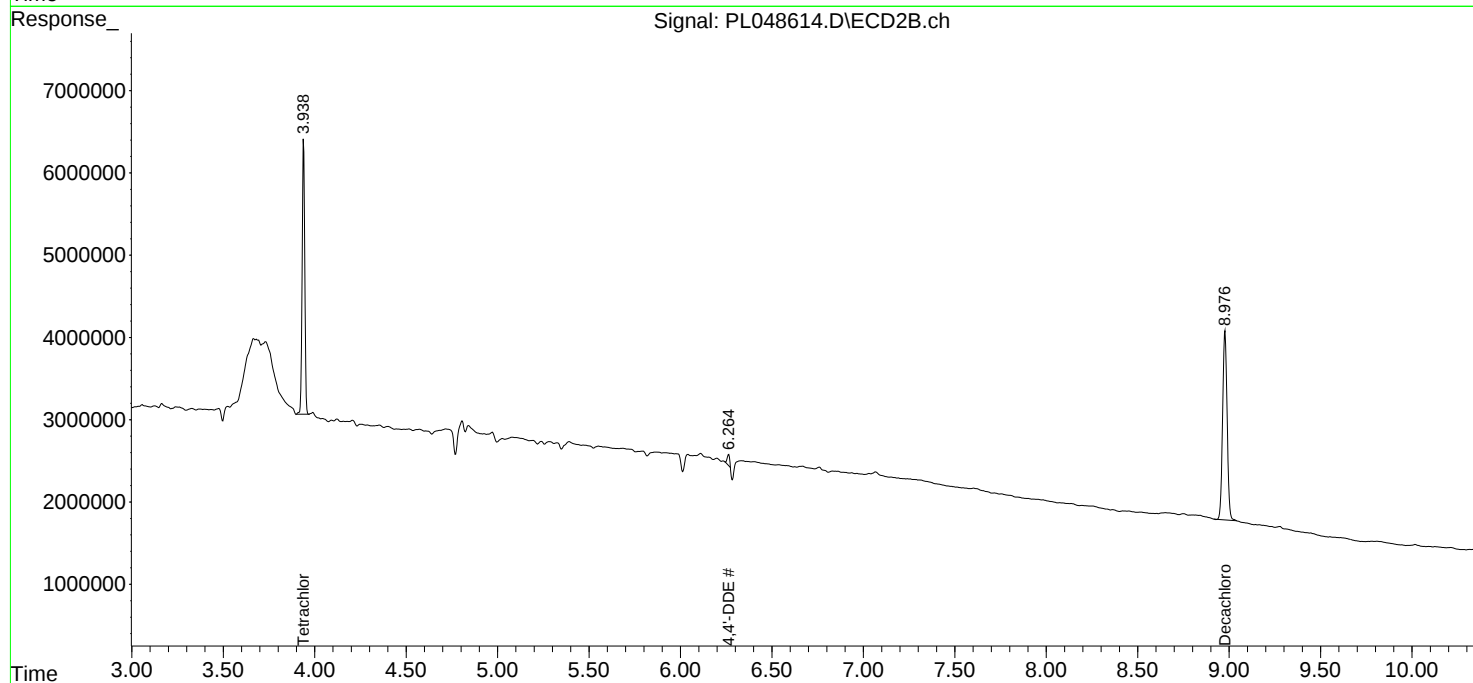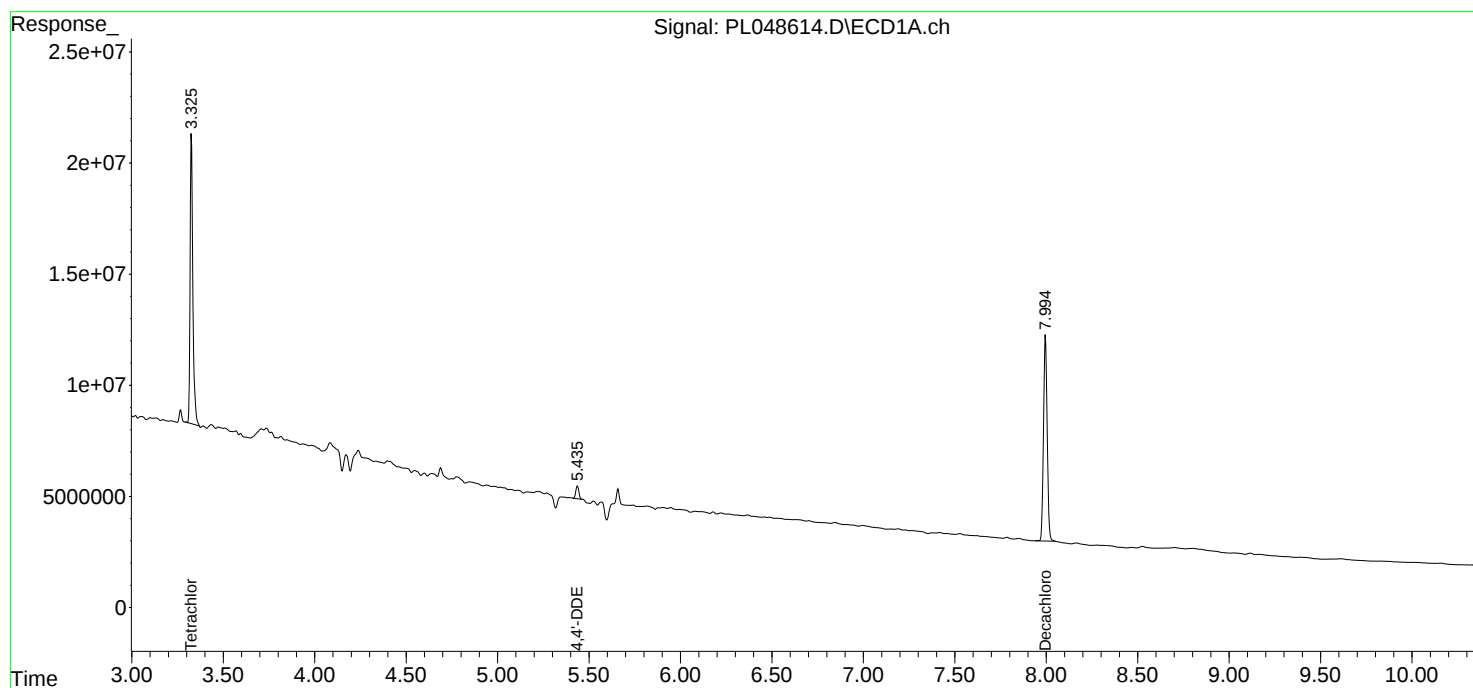

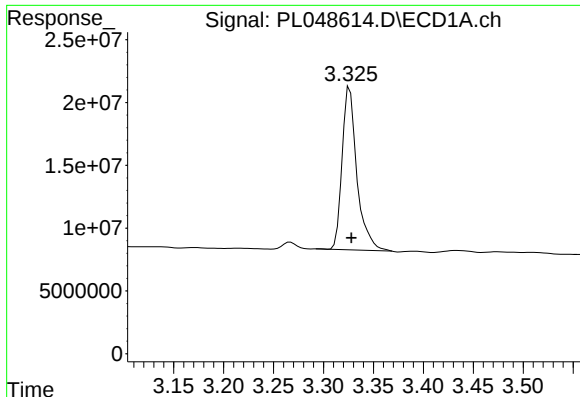


#1 Tetrachloro-m-xylene

R.T.: 3.326 min
Delta R.T.: -0.002 min
Response: 133417475
Conc: 13.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-01-051519-A


Manual Integrations
APPROVED

Ankita
5/17/2019 12:27:52 PM

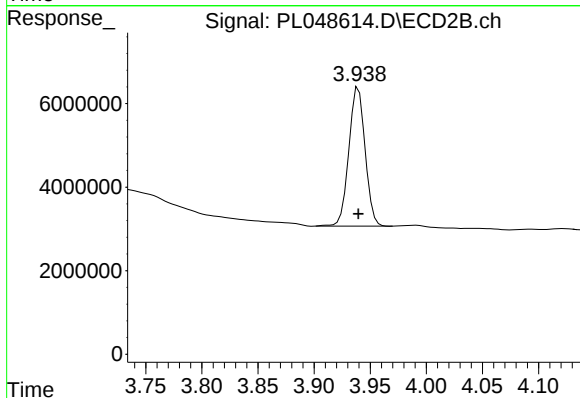


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 33505749
Conc: 13.45 ng/ml

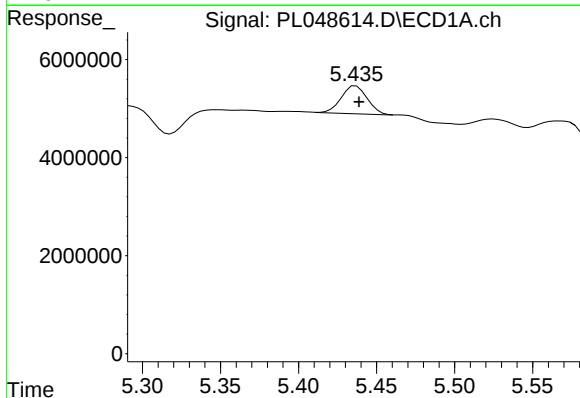


#12 4,4'-DDE

R.T.: 5.435 min
Delta R.T.: -0.003 min
Response: 6591097
Conc: 0.52 ng/ml m

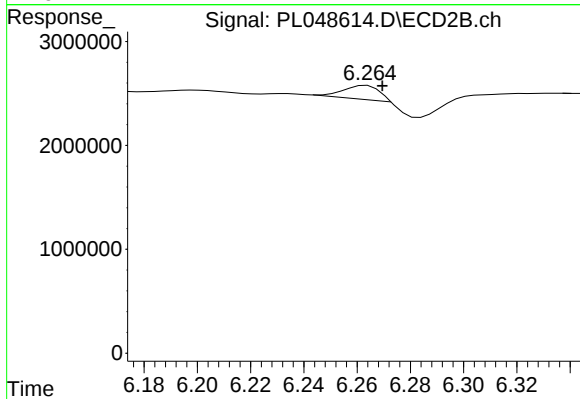

#12 4,4'-DDE

R.T.: 6.264 min
Delta R.T.: -0.006 min
Response: 1214757
Conc: 0.44 ng/ml m

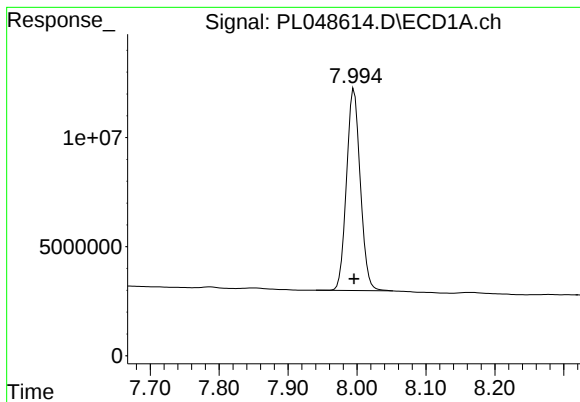


#28 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: 0.000 min
Response: 128583807
Conc: 12.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-01-051519-A

Manual Integrations
APPROVED

Ankita
5/17/2019 12:27:52 PM

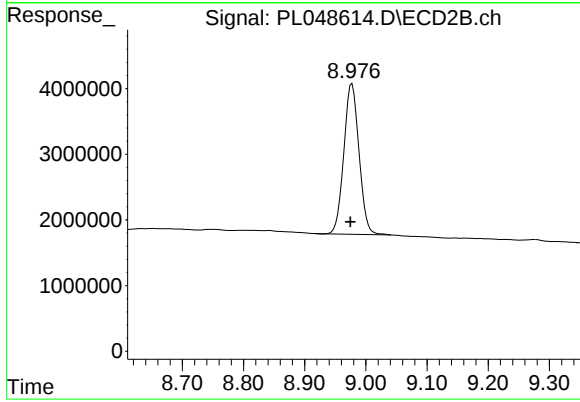

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: 0.002 min
Response: 39557355
Conc: 14.90 ng/ml