

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051723\
 Data File : PL082771.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 May 2023 18:39
 Operator : AR\AJ
 Sample : 02798-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WATERWITCH-AVE-SAMPLE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/18/2023
 Supervised By :Ankita Jodhani 05/18/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 21:31:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.320	2.641	48077854	40104212	17.999	17.311
28) SA Decachlor...	8.736	7.746	37126325	39352922	19.447	17.241m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051723\
Data File : PL082771.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2023 18:39
Operator : AR\AJ
Sample : 02798-02
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WATERWITCH-AVE-SAMPLE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/18/2023
Supervised By : Ankita Jodhani 05/18/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 21:31:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

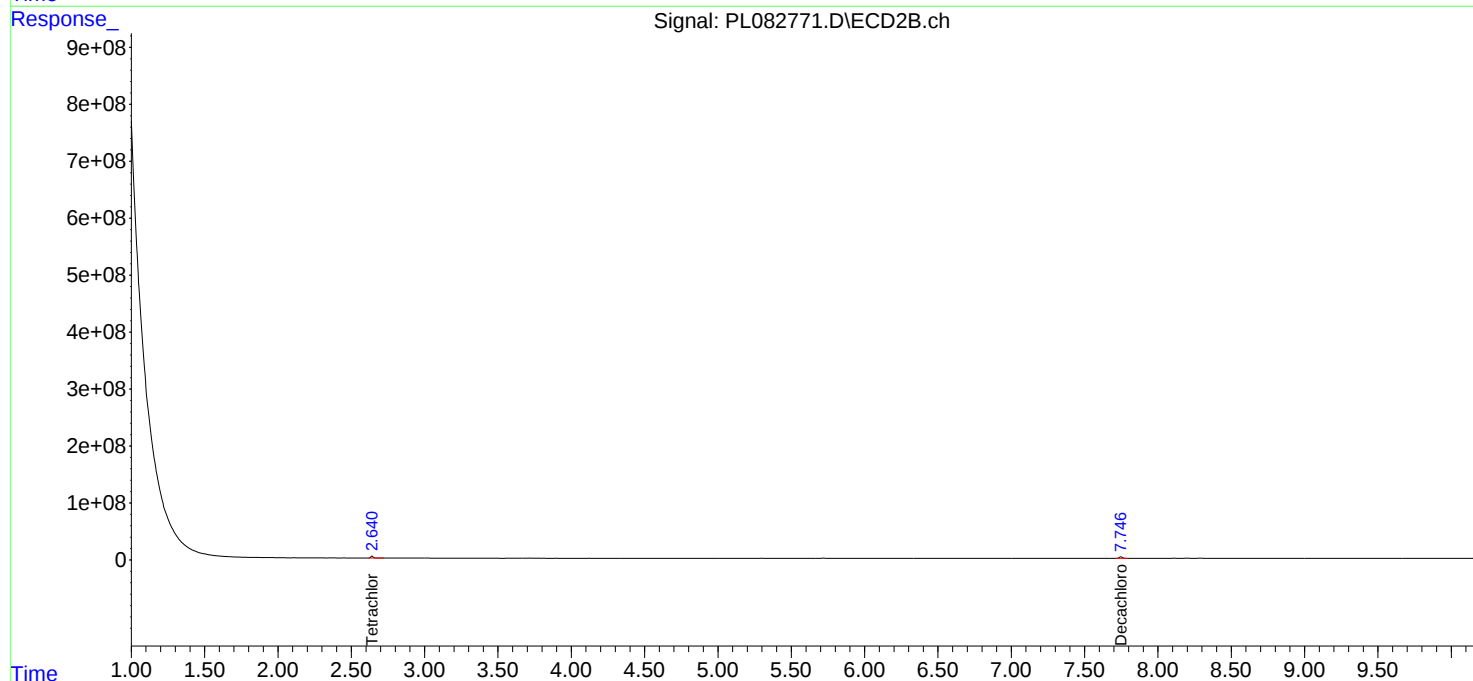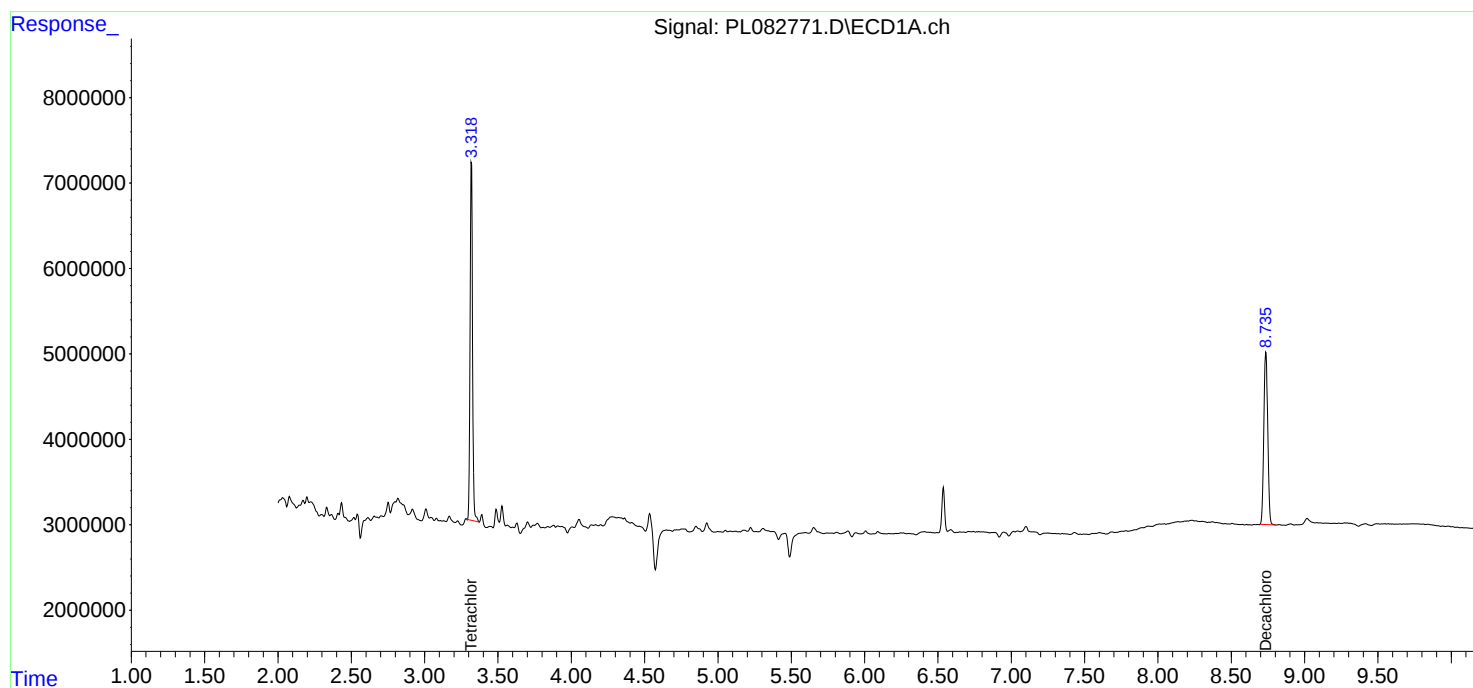

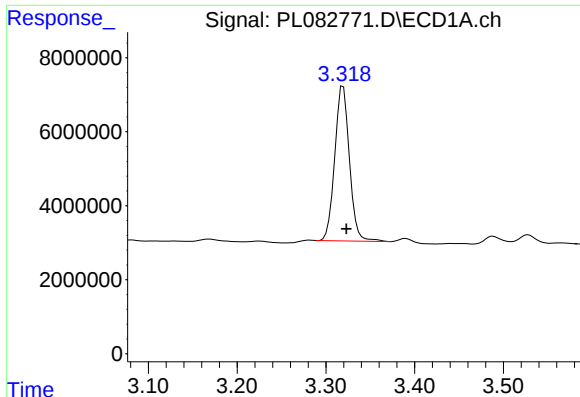


#1 Tetrachloro-m-xylene

R.T.: 3.320 min
Delta R.T.: -0.003 min
Response: 48077854
Conc: 18.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
WATERWITCH-AVE-SAMPLE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/18/2023
Supervised By :Ankita Jodhani 05/18/2023

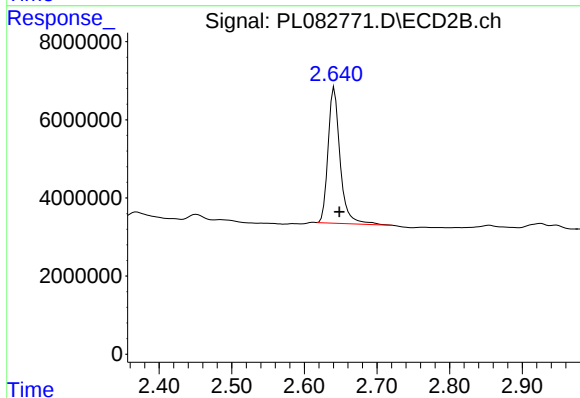


#1 Tetrachloro-m-xylene

R.T.: 2.641 min
Delta R.T.: -0.007 min
Response: 40104212
Conc: 17.31 ng/ml

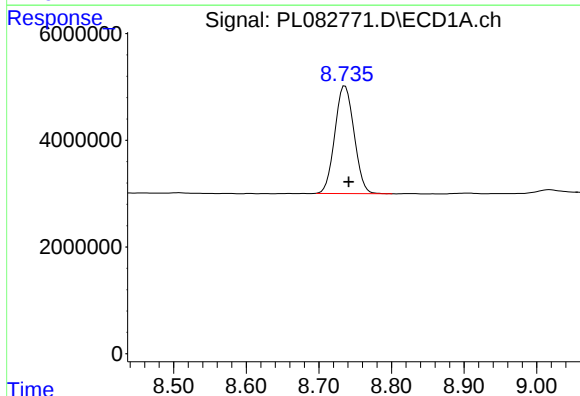

#28 Decachlorobiphenyl

R.T.: 8.736 min
Delta R.T.: -0.005 min
Response: 37126325
Conc: 19.45 ng/ml

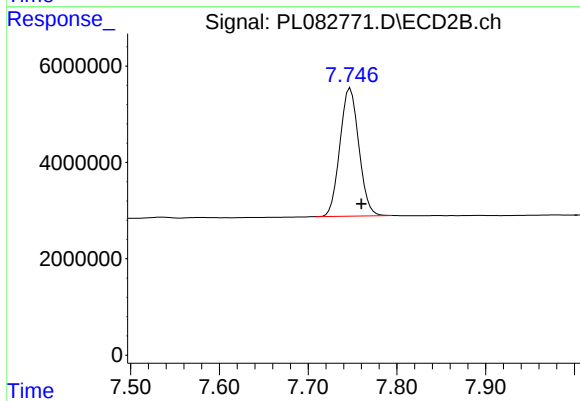

#28 Decachlorobiphenyl

R.T.: 7.746 min
Delta R.T.: -0.014 min
Response: 39352922
Conc: 17.24 ng/ml m