

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051724\
 Data File : PL089577.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 May 2024 11:07
 Operator : AR\AJ
 Sample : TOXAPH201
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 14:54:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 14:45:09 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.812	20506856	12478371	10.657	9.627
27)	SA Decachlor...	9.066	7.963	14233302	6065975	21.423	9.935 #
Target Compounds							
22)	Toxaphene-1	5.862	5.049	7981525	7368371	1120.848	867.925
23)	Toxaphene-2	6.452	5.374	21053075	6574850	1096.968	805.787 #
24)	Toxaphene-3	7.069	6.649	43578695	25042025	1005.779	850.483
25)	Toxaphene-4	7.161	6.777	33299770	36405168	1017.614	894.665
26)	Toxaphene-5	7.580	7.089	23394968	24111903	1008.844	926.409

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051724\
Data File : PL089577.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2024 11:07
Operator : AR\AJ
Sample : TOXAPH201
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 14:54:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051724CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 14:45:09 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

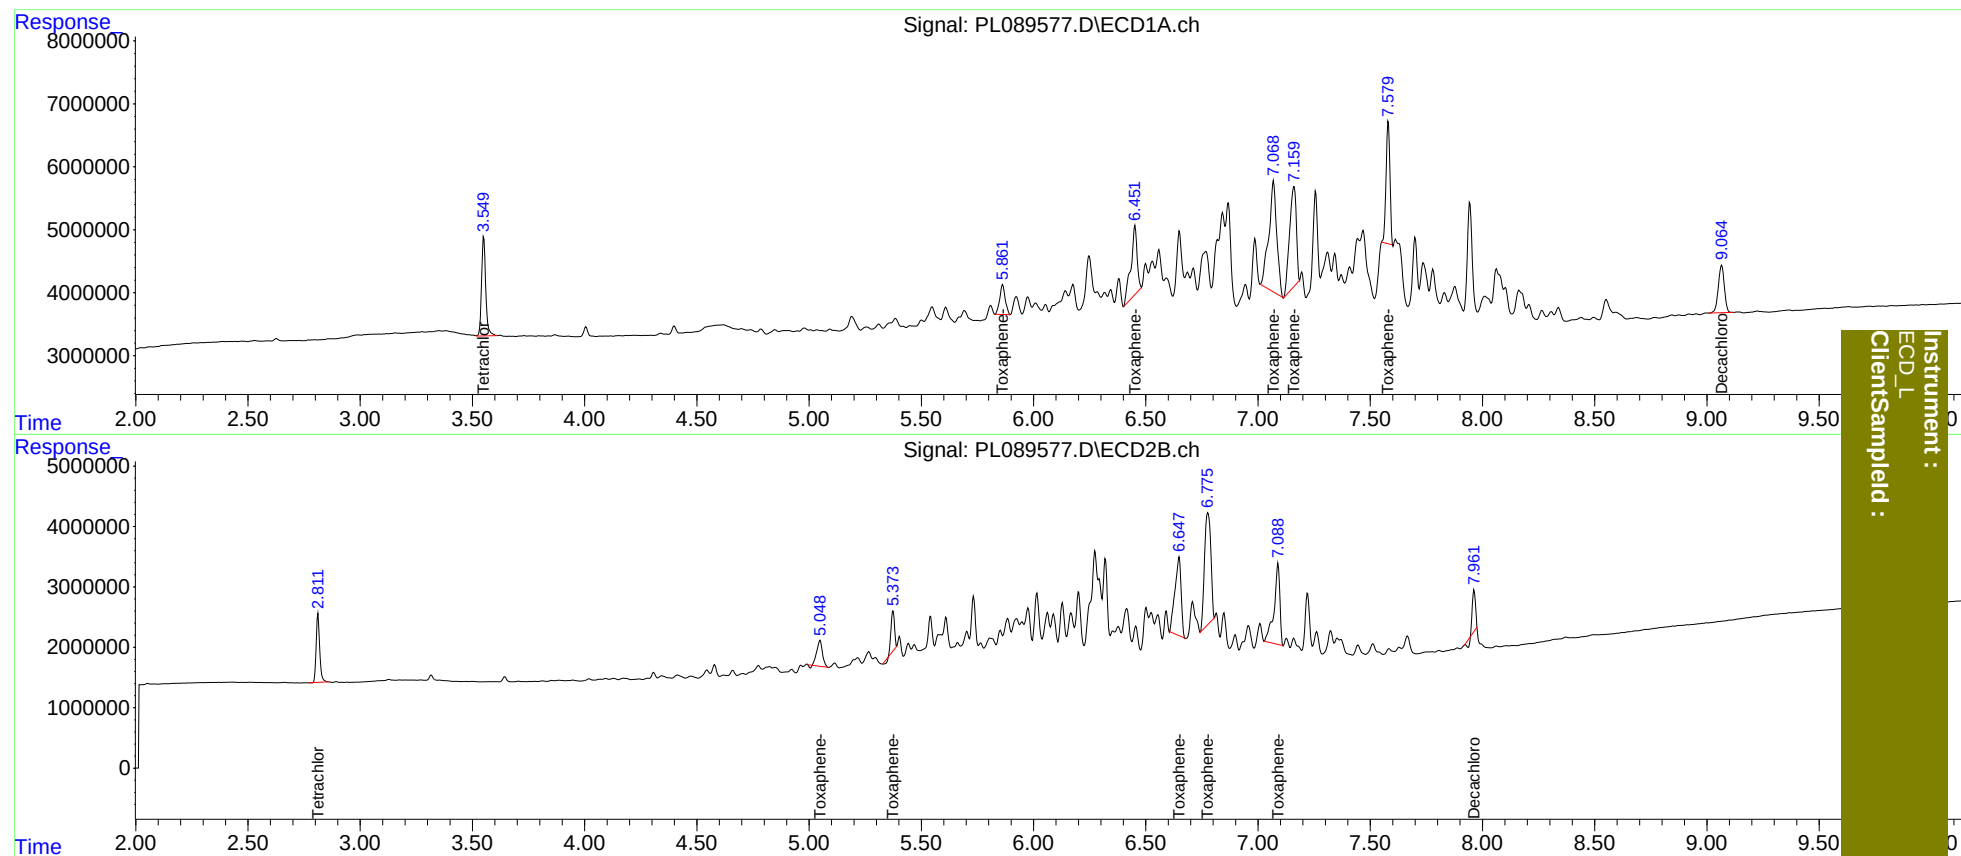

Instrument :
ECD_L
ClientSampled :
PL051724CLP.M