

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051819\
 Data File : PL048667.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 May 2019 18:38
 Operator : SM\AJ
 Sample : K2880-04
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 339

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 23:19:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.327	3.939	117.6E6	33374536	12.135	13.399
28)	SA Decachlor...	7.997	8.977	86887918	23692910	8.642	8.926
Target Compounds							
3)	MA gamma-BHC...	4.038	0.000	40208254	0	2.830	N.D. #
4)	MA Heptachlor	4.309	0.000	39696050	0	2.698	N.D. #
6)	B beta-BHC	4.309f	0.000	39696050	0	6.726	N.D. #
7)	B delta-BHC	0.000	4.983f	0	10454728	N.D.	3.697 #
9)	A Endosulfan I	5.351f	0.000	41238245	0	3.428	N.D. #
10)	B gamma-Chl...	5.245f	6.029	25760343	4002498	1.929	1.300 #
11)	B alpha-Chl...	5.245f	0.000	25760343	0	1.970	N.D. #
13)	MA Dieldrin	5.551	0.000	33883767	0	2.602	N.D. #
25)	Chlordane-3	5.245f	6.029	25760343	4002498	16.360	9.133 #
26)	Chlordane-4	5.245f	0.000	25760343	0	17.743	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051819\
Data File : PL048667.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2019 18:38
Operator : SM\AJ
Sample : K2880-04
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
339

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 23:19:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

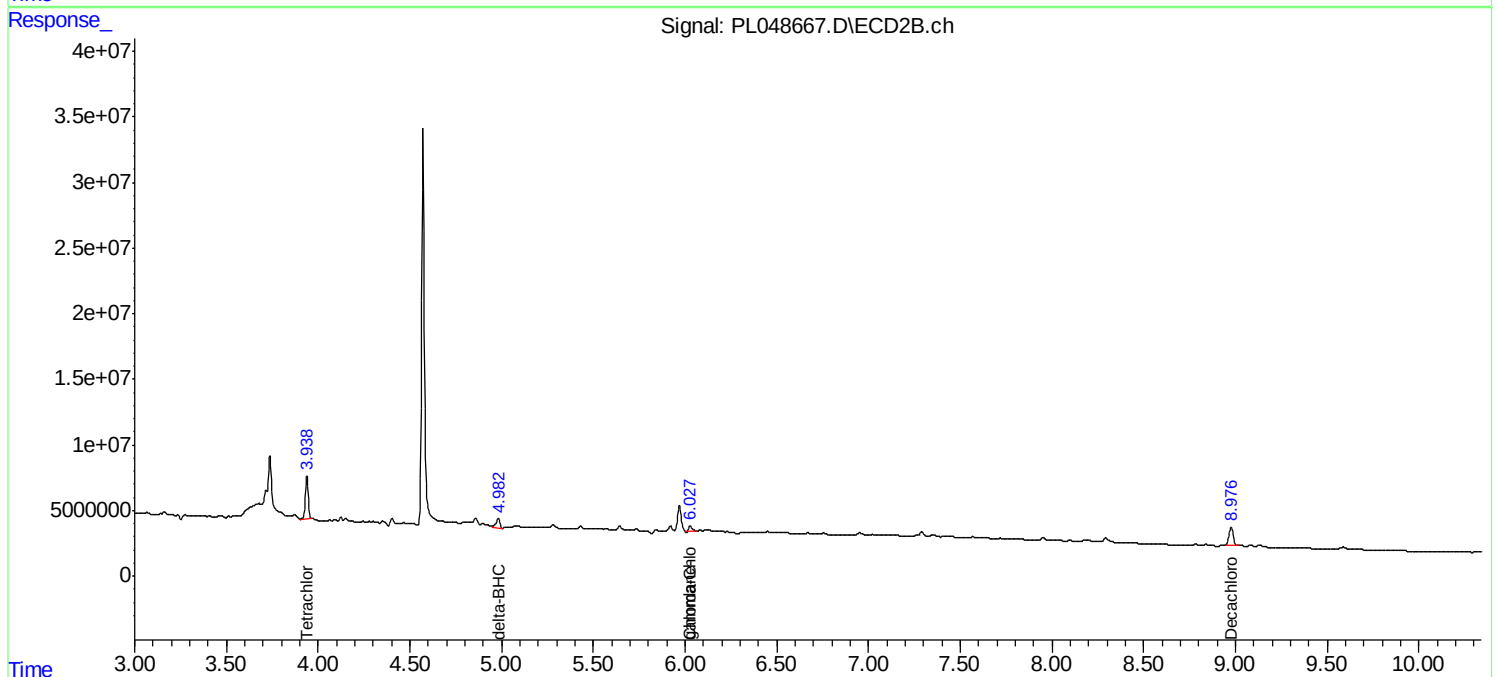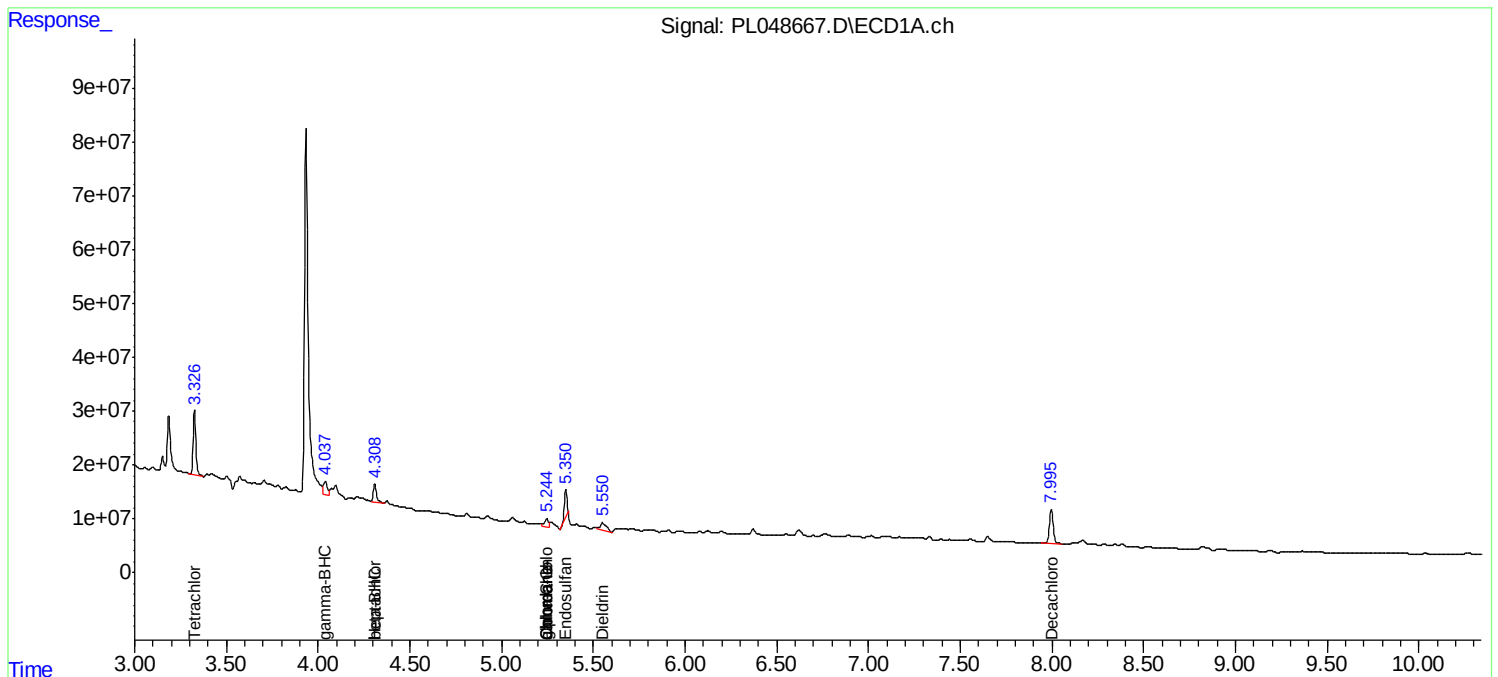


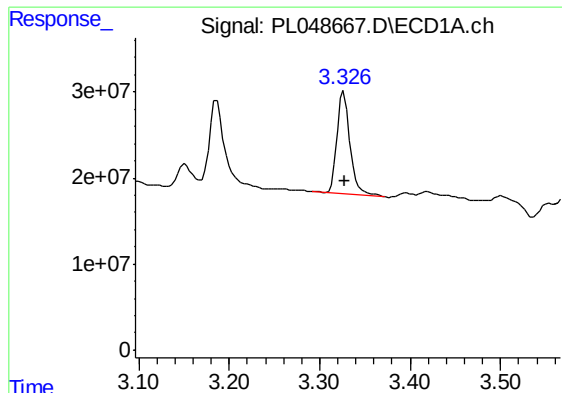

#1 Tetrachloro-m-xylene


R.T.: 3.327 min
Delta R.T.: -0.001 min
Response: 117550941
Conc: 12.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
339

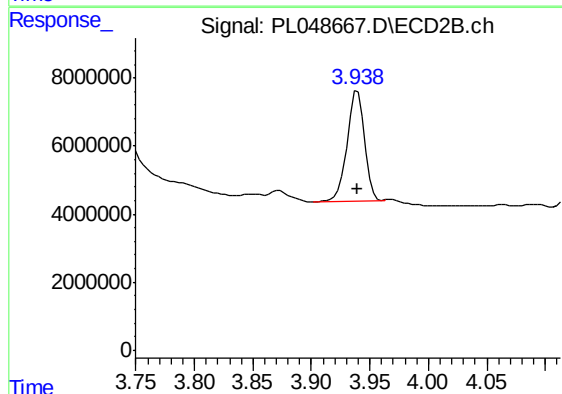


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 33374536
Conc: 13.40 ng/ml

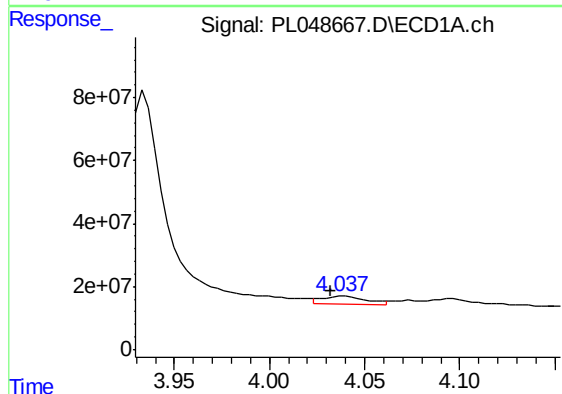


#3 gamma-BHC (Lindane)

R.T.: 4.038 min
Delta R.T.: 0.006 min
Response: 40208254
Conc: 2.83 ng/ml

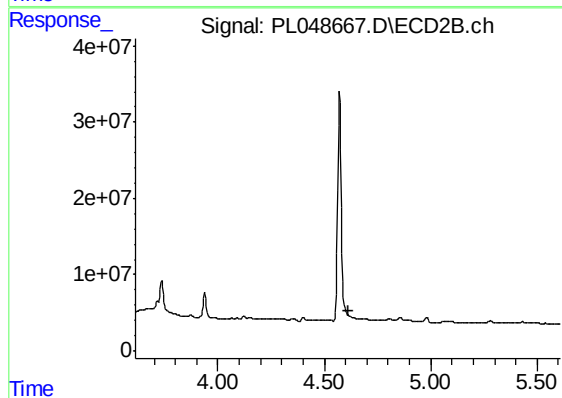

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.612 min
Response: 0
Conc: N.D.

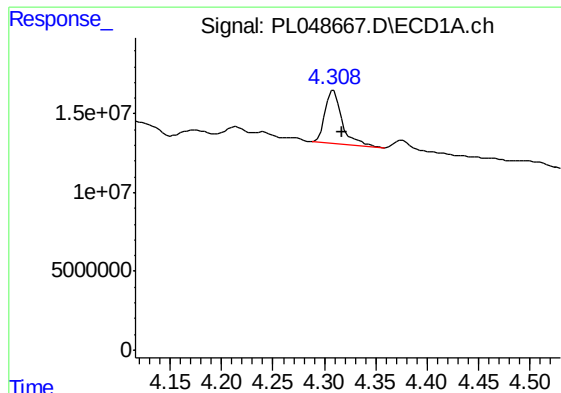

#4 Heptachlor


R.T.: 4.309 min
Delta R.T.: -0.008 min
Response: 39696050
Conc: 2.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
339

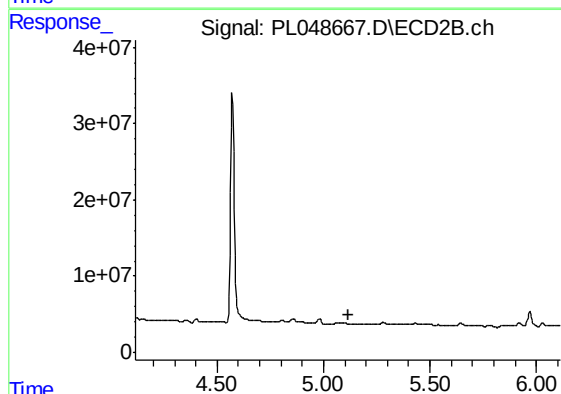


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.116 min
Response: 0
Conc: N.D.

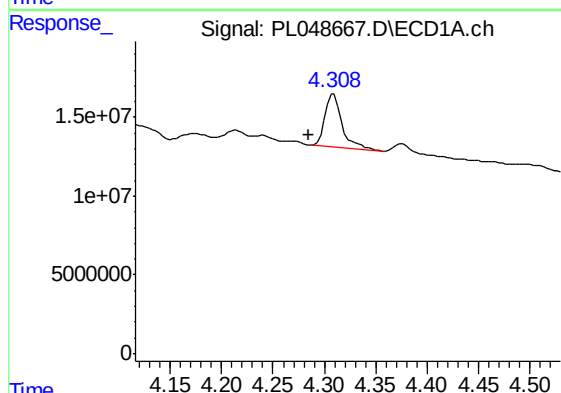


#6 beta-BHC

R.T.: 4.309 min
Delta R.T.: 0.024 min
Response: 39696050
Conc: 6.73 ng/ml

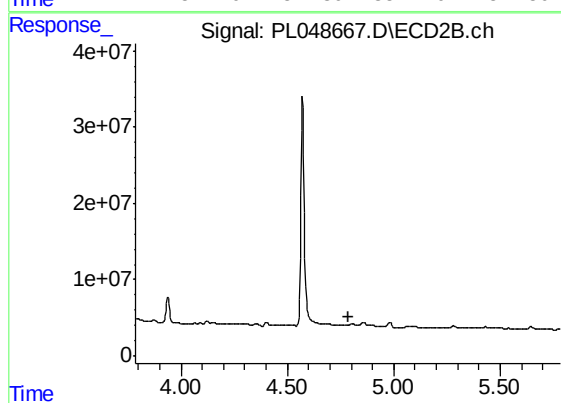

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.786 min
Response: 0
Conc: N.D.

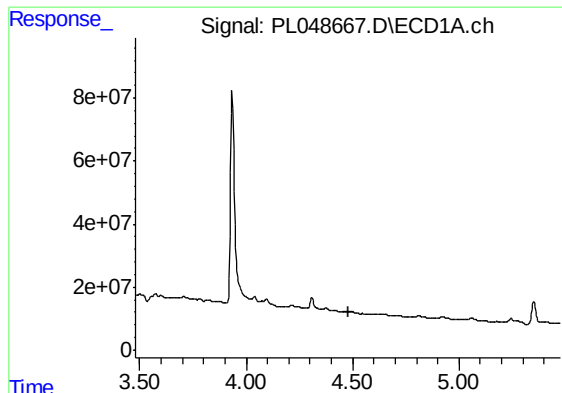

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
339

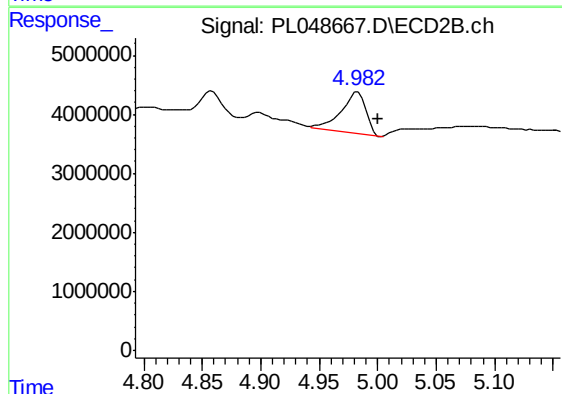


#7 delta-BHC

R.T.: 4.983 min
Delta R.T.: -0.017 min
Response: 10454728
Conc: 3.70 ng/ml

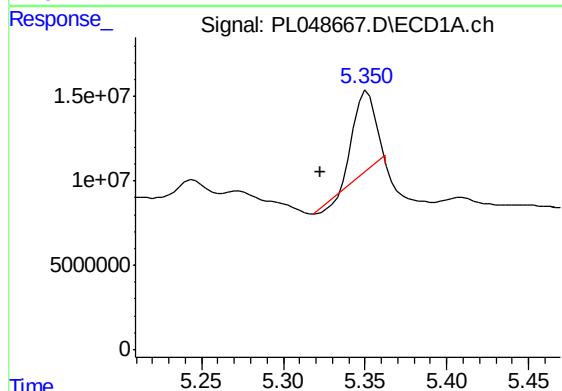


#9 Endosulfan I

R.T.: 5.351 min
Delta R.T.: 0.029 min
Response: 41238245
Conc: 3.43 ng/ml

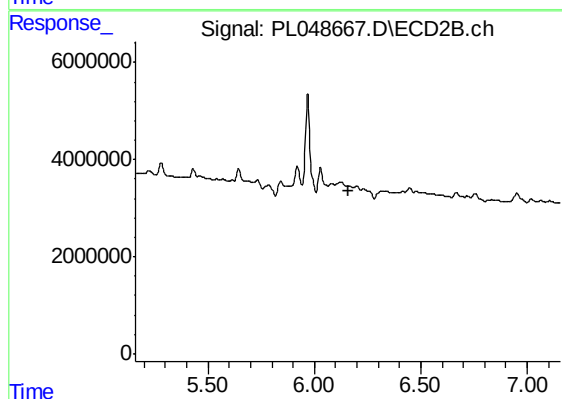

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.159 min
Response: 0
Conc: N.D.

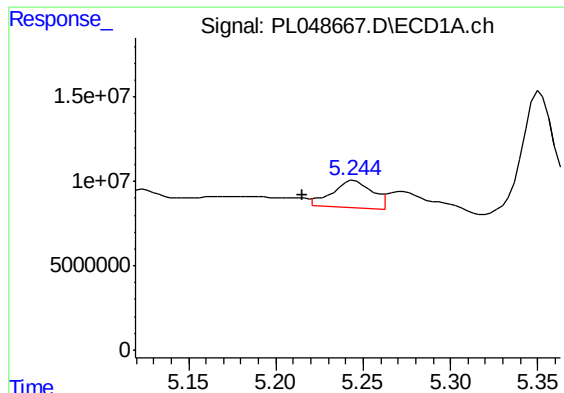

#10 gamma-Chlordane


R.T.: 5.245 min
Delta R.T.: 0.030 min
Response: 25760343
Conc: 1.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
339

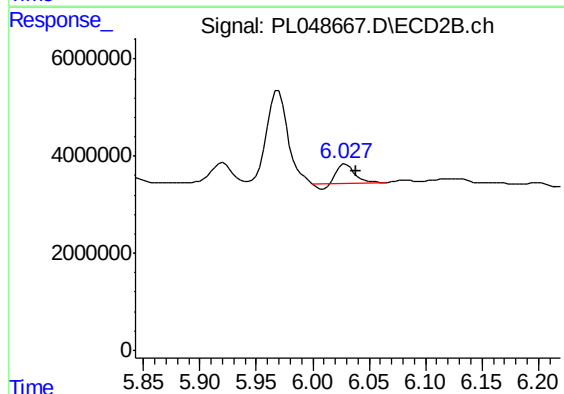


#10 gamma-Chlordane

R.T.: 6.029 min
Delta R.T.: -0.010 min
Response: 4002498
Conc: 1.30 ng/ml

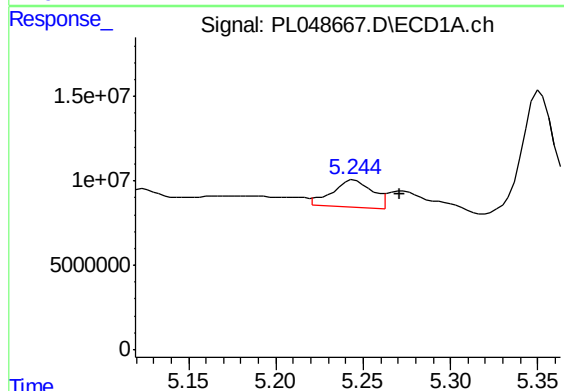


#11 alpha-Chlordane

R.T.: 5.245 min
Delta R.T.: -0.026 min
Response: 25760343
Conc: 1.97 ng/ml

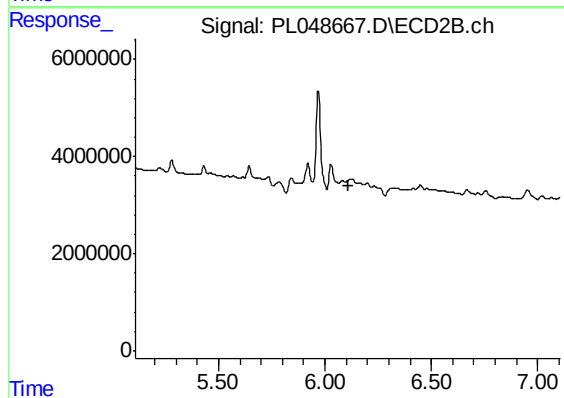

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.109 min
Response: 0
Conc: N.D.

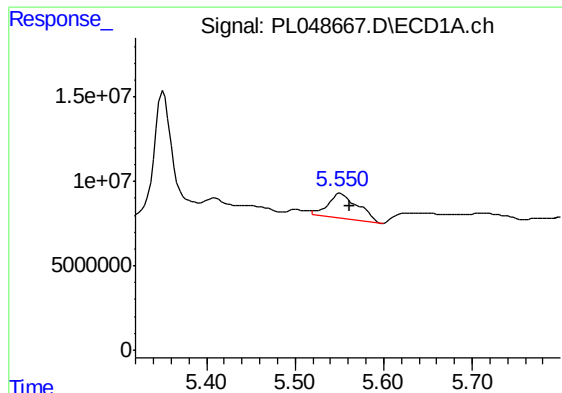

#13 Dieldrin


R.T.: 5.551 min
Delta R.T.: -0.011 min
Response: 33883767
Conc: 2.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
339

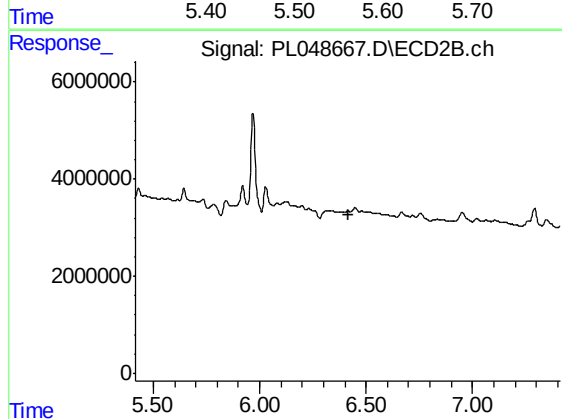


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

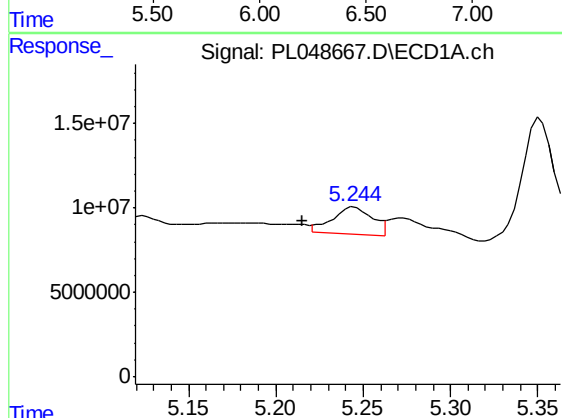


#25 Chlordane-3

R.T.: 5.245 min
Delta R.T.: 0.029 min
Response: 25760343
Conc: 16.36 ng/ml

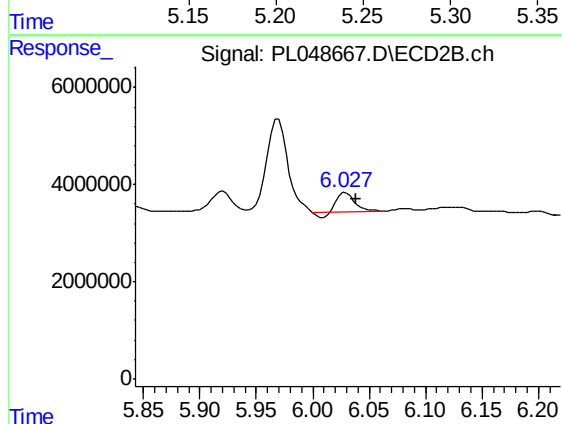

#25 Chlordane-3


R.T.: 6.029 min
Delta R.T.: -0.009 min
Response: 4002498
Conc: 9.13 ng/ml

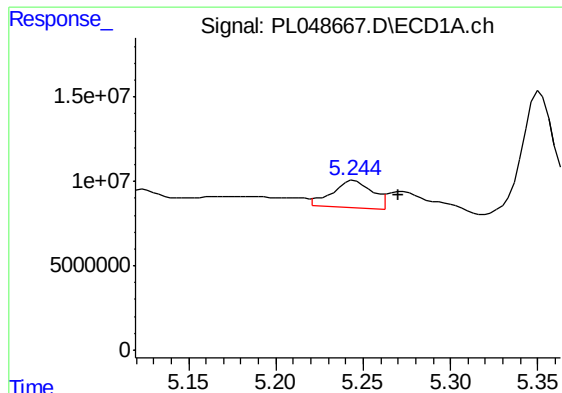

#26 Chlordane-4


R.T.: 5.245 min
Delta R.T.: -0.025 min
Response: 25760343
Conc: 17.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
339

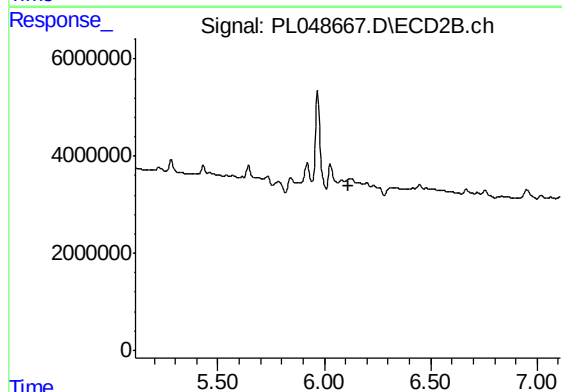


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.111 min
Response: 0
Conc: N.D.

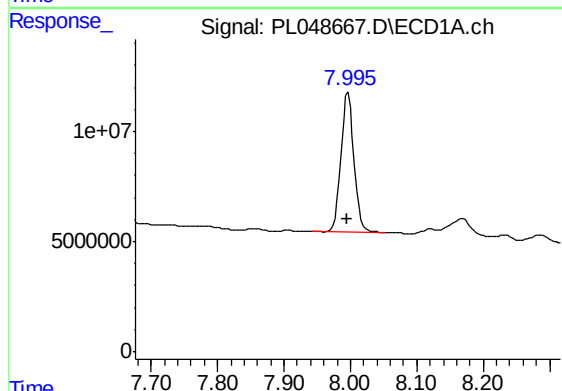

#28 Decachlorobiphenyl

R.T.: 7.997 min
Delta R.T.: 0.000 min
Response: 86887918
Conc: 8.64 ng/ml

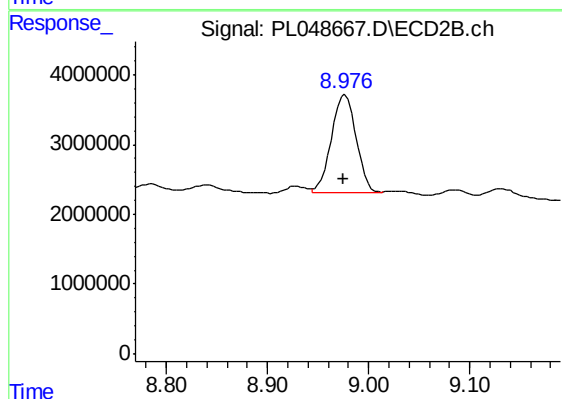

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: 0.002 min
Response: 23692910
Conc: 8.93 ng/ml