

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051819\
 Data File : PL048686.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2019 00:26
 Operator : SM\AJ
 Sample : K2881-01
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-PS-01-047

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 01:30:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.327	3.939	194.9E6	53703680	20.116	21.560
28)	SA Decachlor...	7.996	8.976	143.3E6	42988537	14.252	16.196
Target Compounds							
10)	B gamma-Chl...	5.213	0.000	6295215	0	0.471	N.D. #
11)	B alpha-Chl...	0.000	6.111	0	2826923	N.D.	0.921 #
25)	Chlordane-3	5.213	0.000	6295215	0	3.998	N.D. #
26)	Chlordane-4	0.000	6.111	0	2826923	N.D.	5.389 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051819\
Data File : PL048686.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2019 00:26
Operator : SM\AJ
Sample : K2881-01
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-047

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 01:30:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

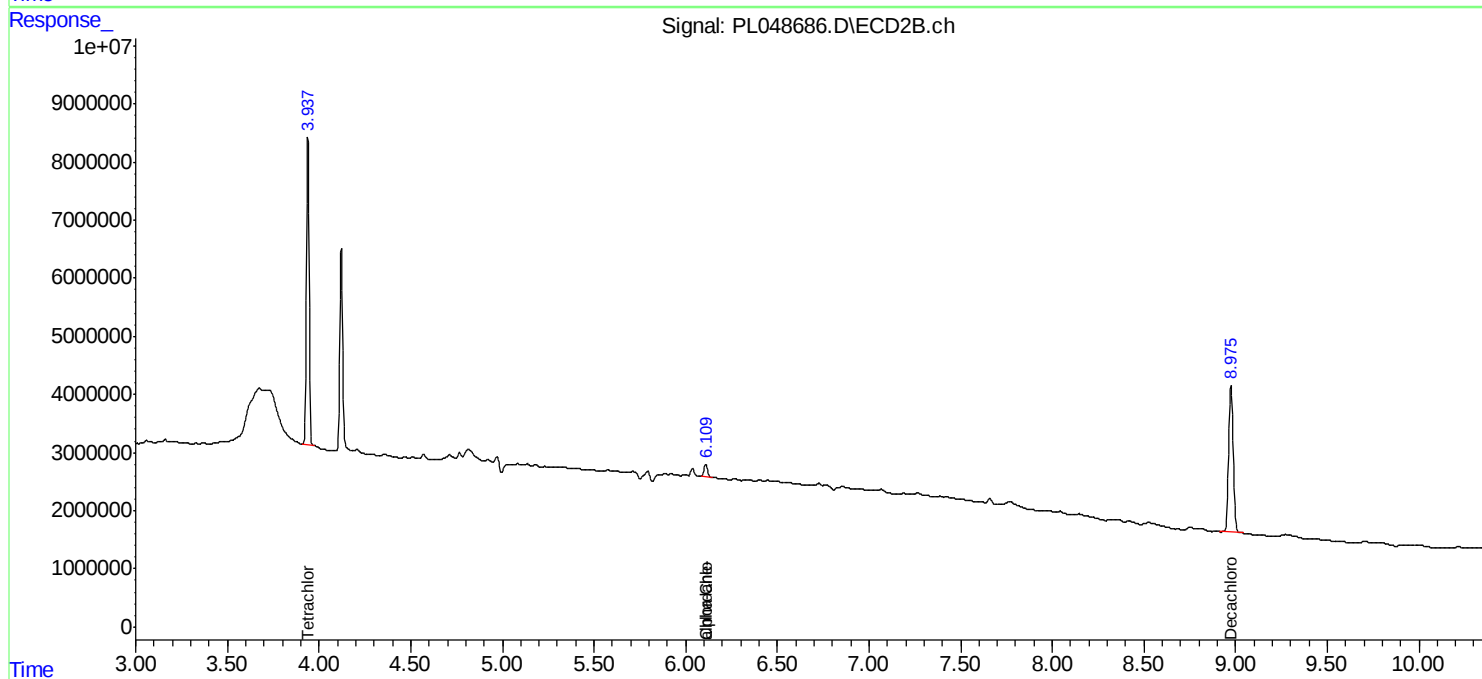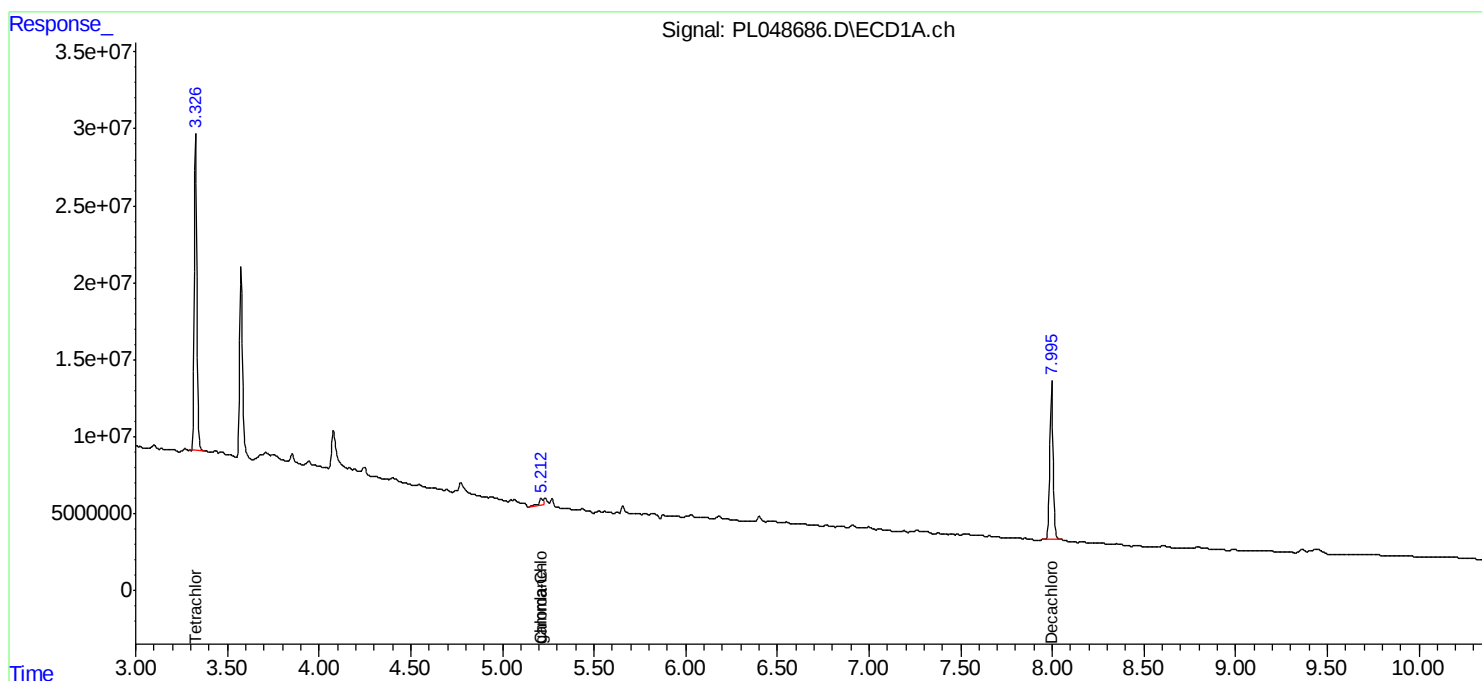


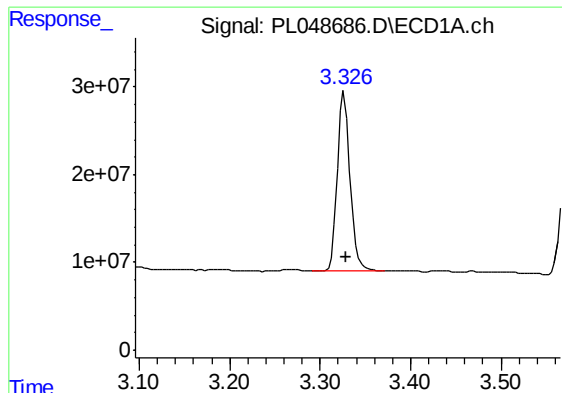

#1 Tetrachloro-m-xylene


R.T.: 3.327 min
Delta R.T.: 0.000 min
Response: 194862876
Conc: 20.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-047

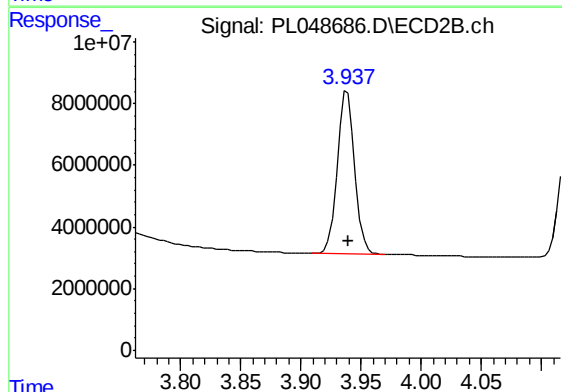


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: -0.001 min
Response: 53703680
Conc: 21.56 ng/ml

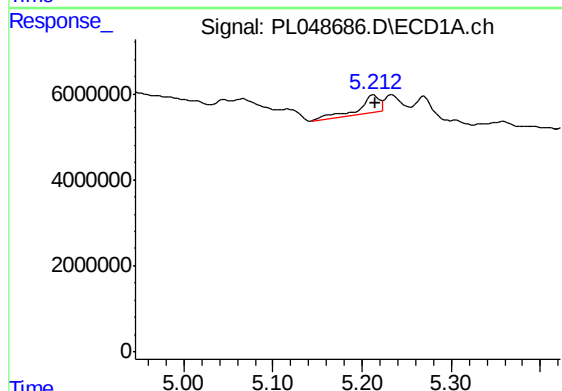


#10 gamma-Chlordane

R.T.: 5.213 min
Delta R.T.: -0.002 min
Response: 6295215
Conc: 0.47 ng/ml

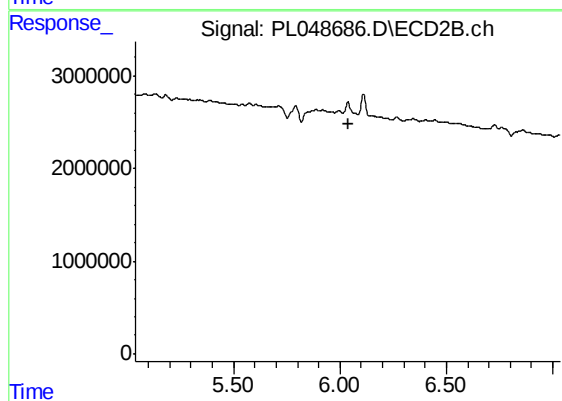

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

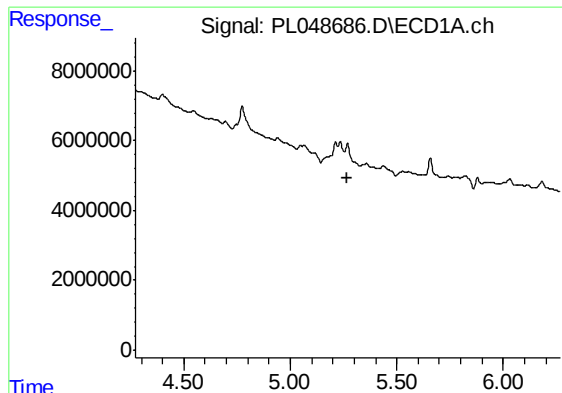

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.271 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-047

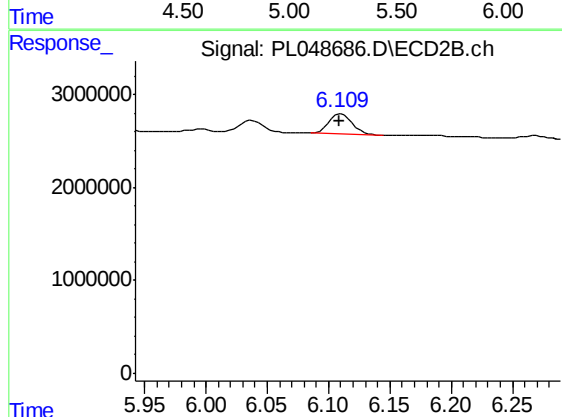


#11 alpha-Chlordane

R.T.: 6.111 min
Delta R.T.: 0.001 min
Response: 2826923
Conc: 0.92 ng/ml

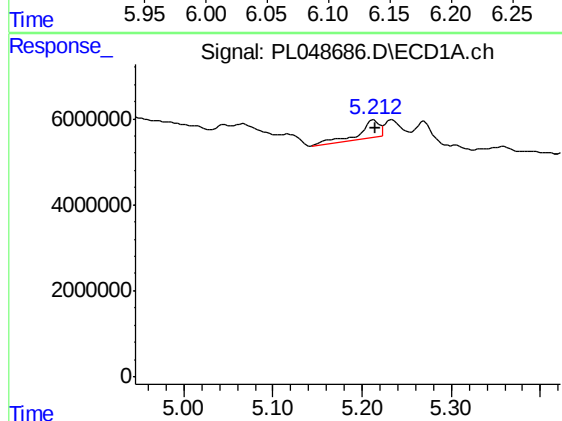


#25 Chlordane-3

R.T.: 5.213 min
Delta R.T.: -0.002 min
Response: 6295215
Conc: 4.00 ng/ml

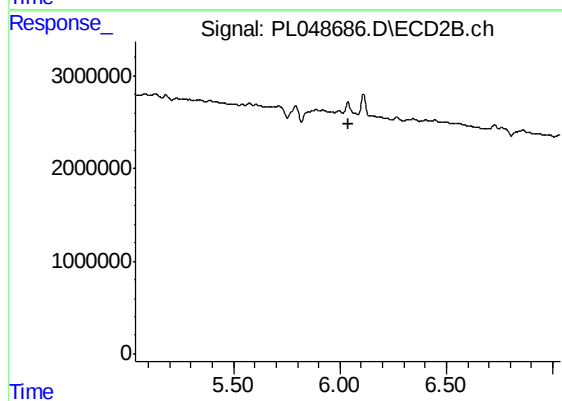

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

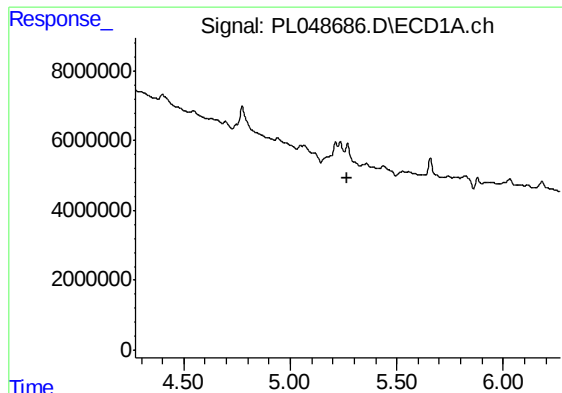

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.270 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-047

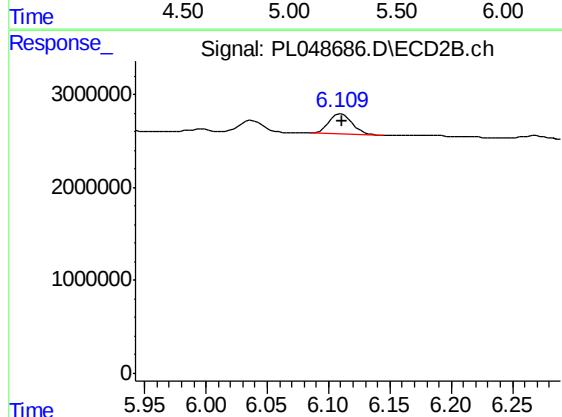


#26 Chlordane-4

R.T.: 6.111 min
Delta R.T.: 0.000 min
Response: 2826923
Conc: 5.39 ng/ml

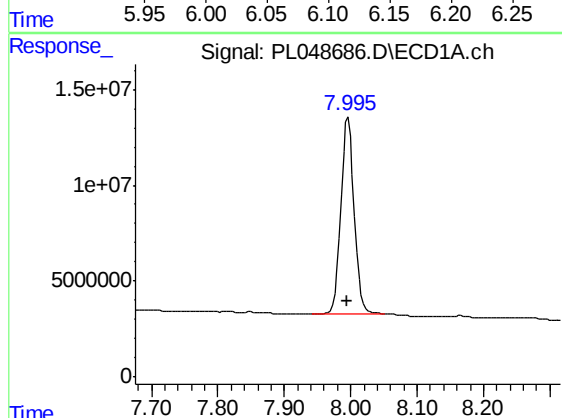

#28 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: 0.000 min
Response: 143296172
Conc: 14.25 ng/ml

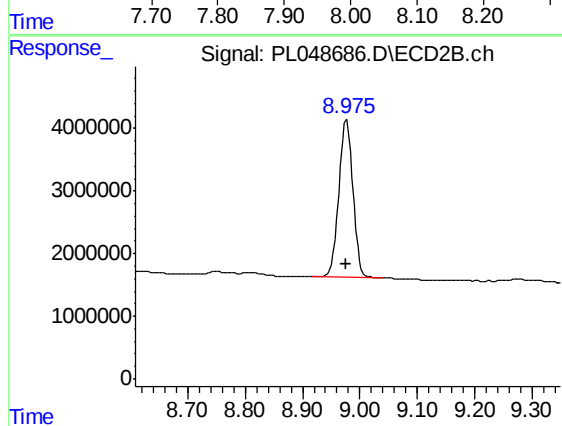

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: 0.001 min
Response: 42988537
Conc: 16.20 ng/ml