

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051819\
 Data File : PL048690.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2019 01:26
 Operator : SM\AJ
 Sample : K2866-09
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RO-COMP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 02:00:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.327	3.940	195.3E6	55608745	20.162	22.325
28)	SA Decachlor...	7.996	8.976	171.8E6	52318741	17.091	19.711
Target Compounds							
3)	MA gamma-BHC...	4.038	4.593f	61409462	20841183	4.322	6.381 #
7)	B delta-BHC	0.000	4.975f	0	10714654	N.D.	3.789 #
9)	A Endosulfan I	5.352f	0.000	3285306	0	0.273	N.D. #
10)	B gamma-Chl...	0.000	6.026	0	2485377	N.D.	0.807 #
13)	MA Dieldrin	5.573	0.000	15589649	0	1.197	N.D. #
25)	Chlordane-3	0.000	6.026	0	2485377	N.D.	5.671 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051819\
Data File : PL048690.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2019 01:26
Operator : SM\AJ
Sample : K2866-09
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RO-COMP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 02:00:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

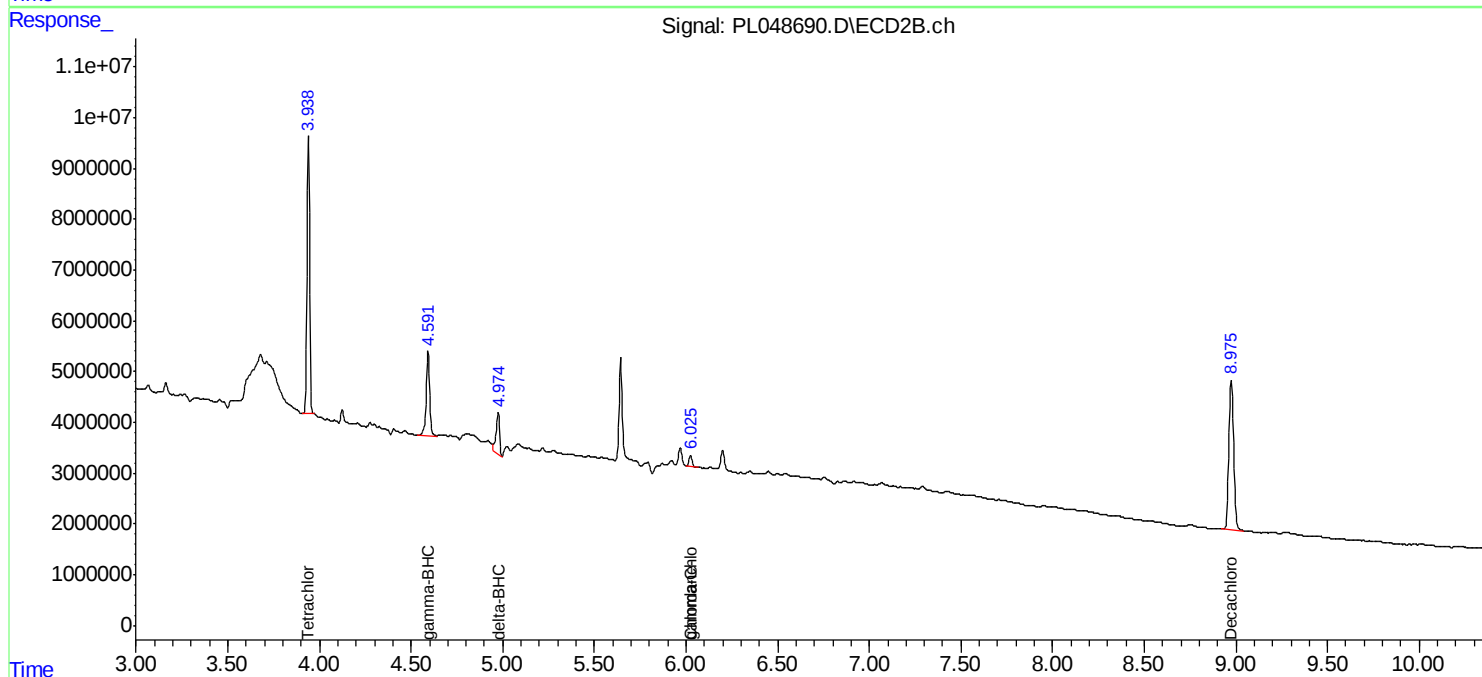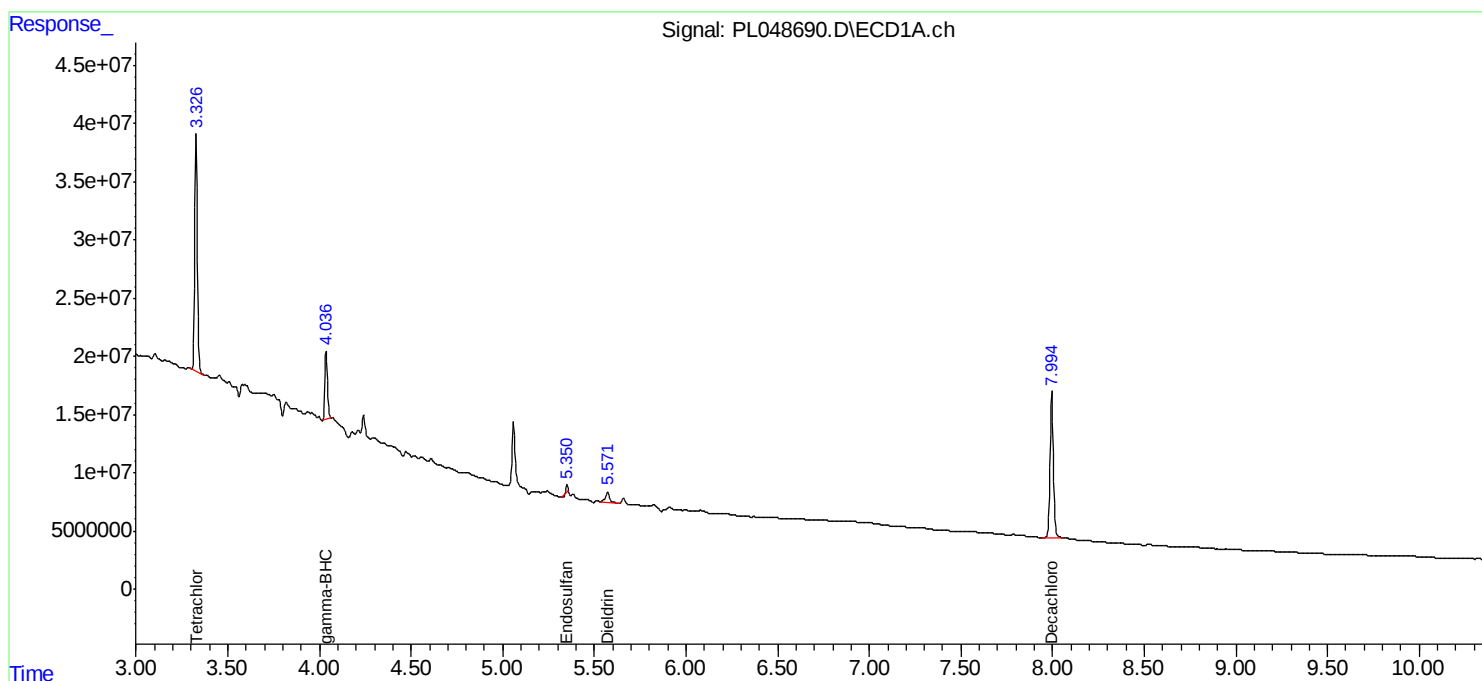


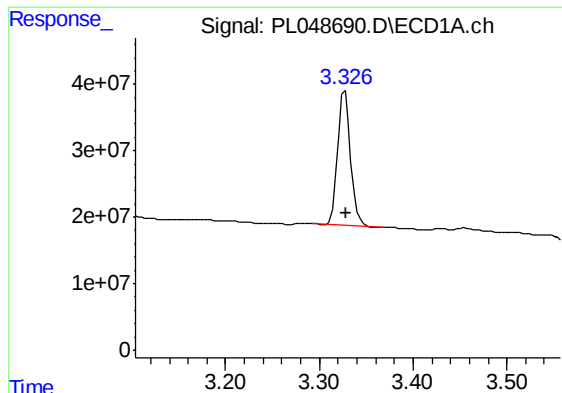

#1 Tetrachloro-m-xylene


R.T.: 3.327 min
Delta R.T.: 0.000 min
Response: 195303047
Conc: 20.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-COMP-3

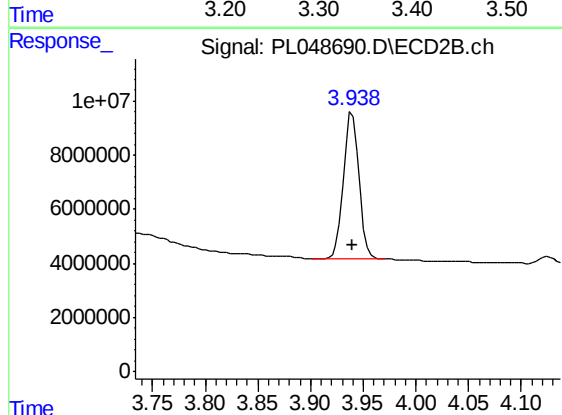


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 55608745
Conc: 22.32 ng/ml

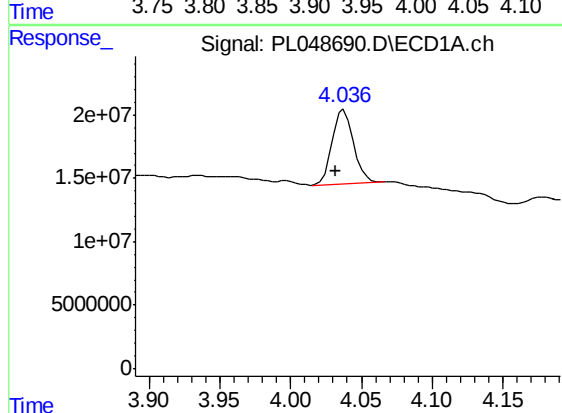


#3 gamma-BHC (Lindane)

R.T.: 4.038 min
Delta R.T.: 0.006 min
Response: 61409462
Conc: 4.32 ng/ml

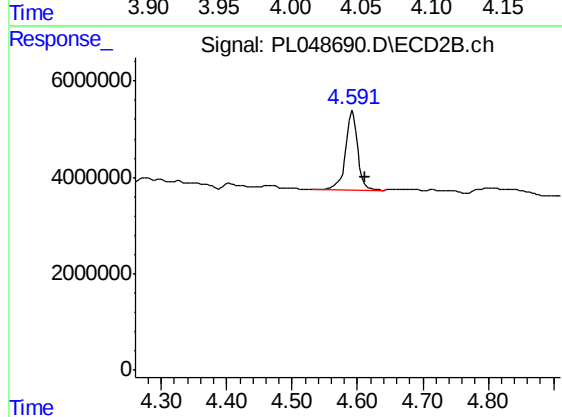

#3 gamma-BHC (Lindane)


R.T.: 4.593 min
Delta R.T.: -0.019 min
Response: 20841183
Conc: 6.38 ng/ml

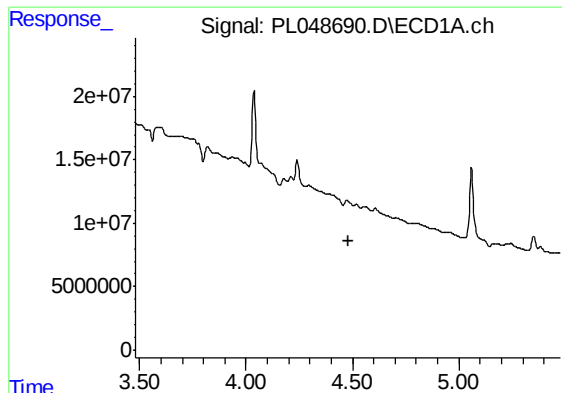

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
RO-COMP-3

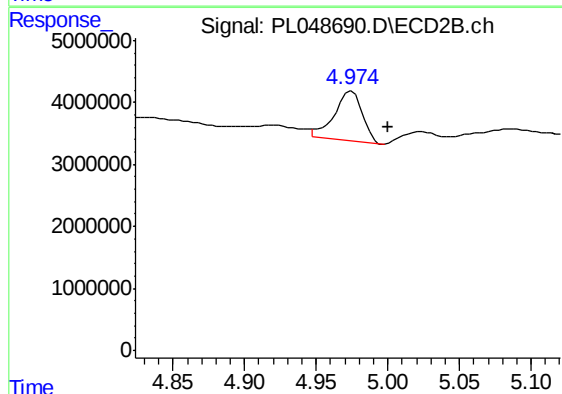


#7 delta-BHC

R.T.: 4.975 min
Delta R.T.: -0.025 min
Response: 10714654
Conc: 3.79 ng/ml

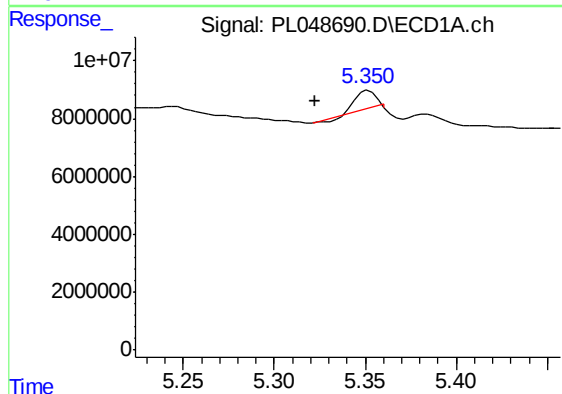


#9 Endosulfan I

R.T.: 5.352 min
Delta R.T.: 0.029 min
Response: 3285306
Conc: 0.27 ng/ml

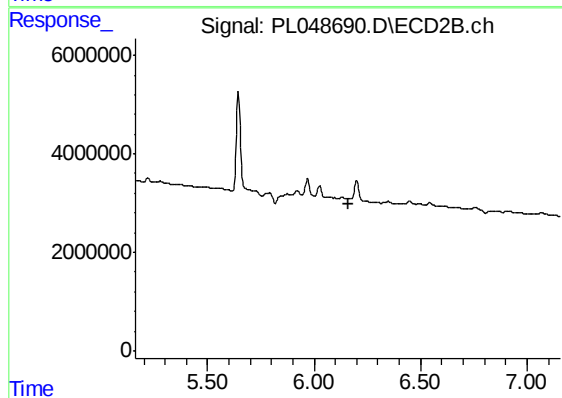

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.159 min
Response: 0
Conc: N.D.

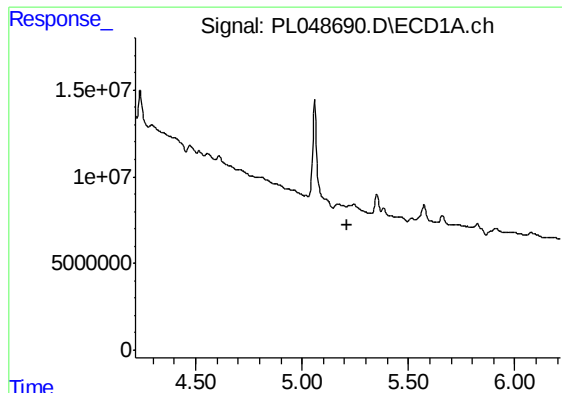

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.215 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
RO-COMP-3

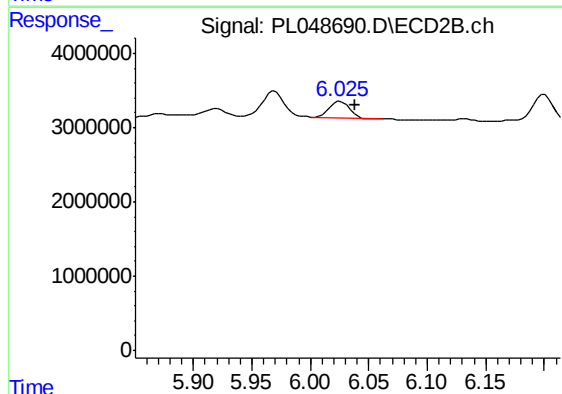


#10 gamma-Chlordane

R.T.: 6.026 min
Delta R.T.: -0.012 min
Response: 2485377
Conc: 0.81 ng/ml

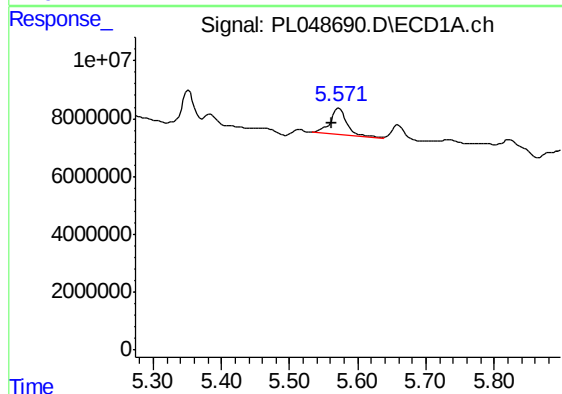


#13 Dieldrin

R.T.: 5.573 min
Delta R.T.: 0.011 min
Response: 15589649
Conc: 1.20 ng/ml

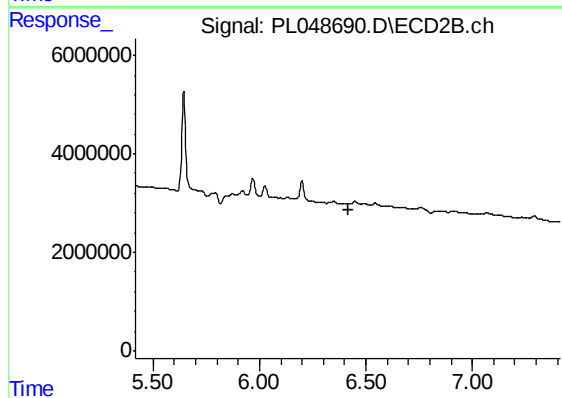

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

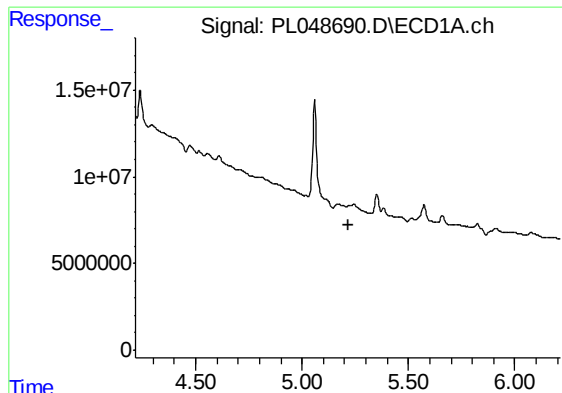

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.216 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
RO-COMP-3

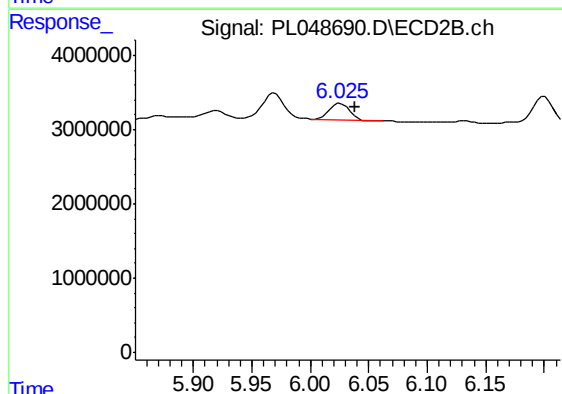


#25 Chlordane-3

R.T.: 6.026 min
Delta R.T.: -0.012 min
Response: 2485377
Conc: 5.67 ng/ml

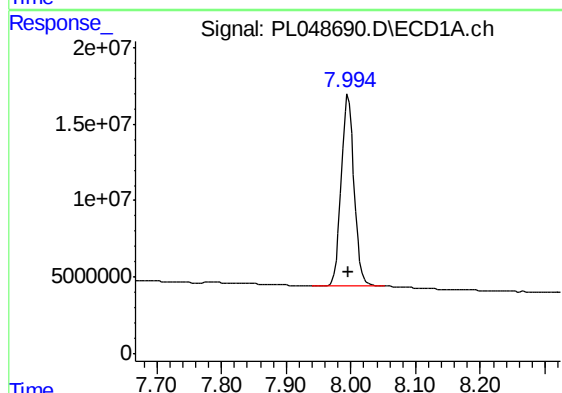

#28 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: 0.000 min
Response: 171838312
Conc: 17.09 ng/ml

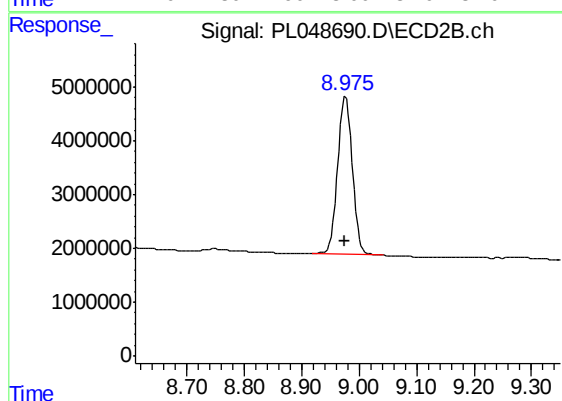

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: 0.001 min
Response: 52318741
Conc: 19.71 ng/ml