

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051819\
 Data File : PL048644.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 May 2019 12:49
 Operator : SM\AJ
 Sample : K2865-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-21-S

Manual Integrations
 APPROVED

Ankita
 5/20/2019 2:03:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 23:14:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.327	3.939	85552463	24159691	8.832	9.699
28) SA Decachlor...	7.997	8.977	97323911	29142064	9.680	10.979
Target Compounds						
12) B 4,4'-DDE	5.436	6.268	17792183	3850429	1.403m	1.395

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051819\
Data File : PL048644.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2019 12:49
Operator : SM\AJ
Sample : K2865-03
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-21-S


Manual Integrations
APPROVED

Ankita
5/20/2019 2:03:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 23:14:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

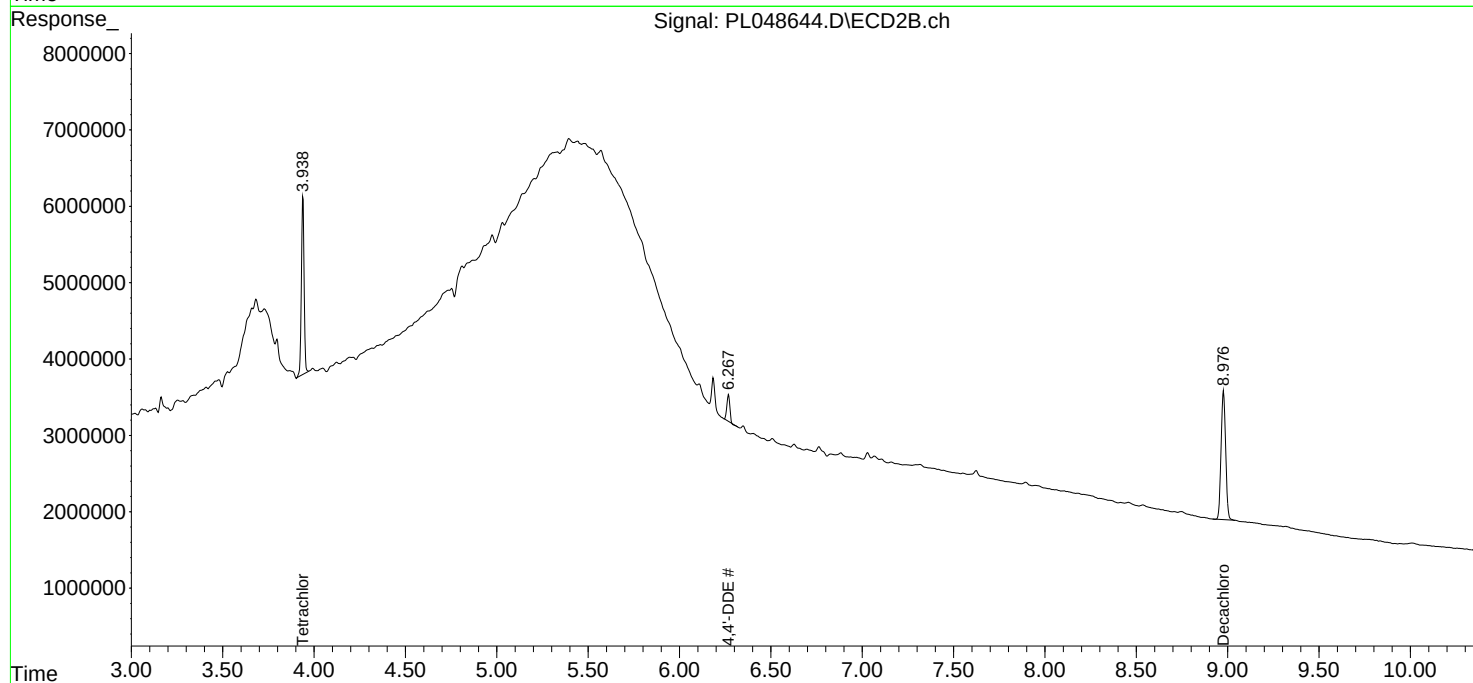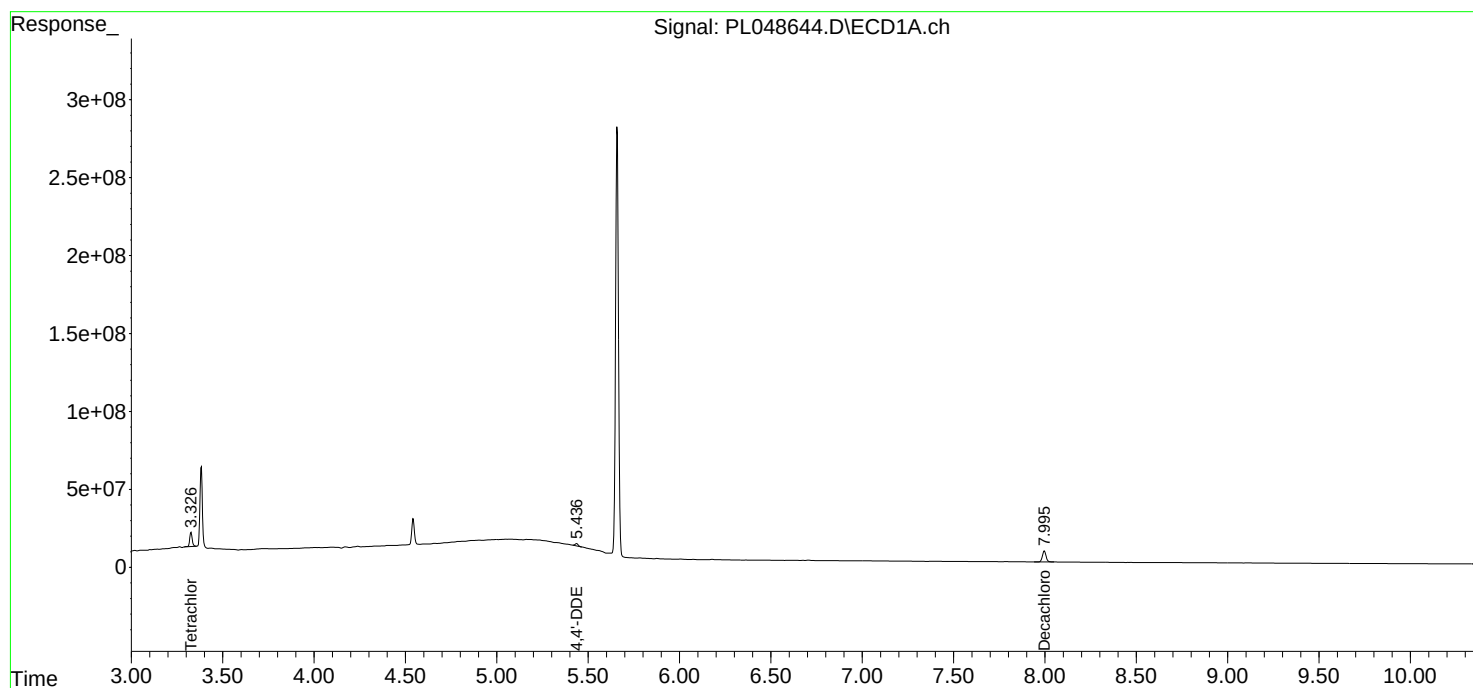

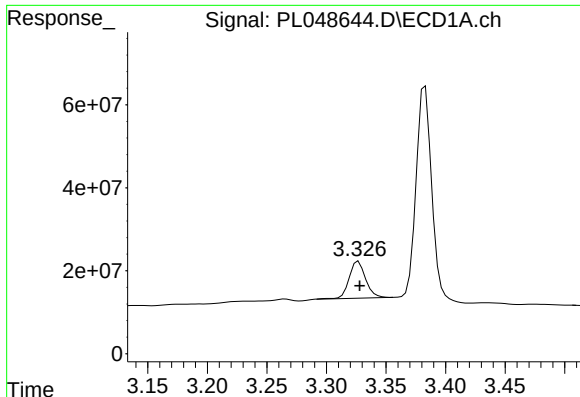


#1 Tetrachloro-m-xylene

R.T.: 3.327 min
Delta R.T.: 0.000 min
Response: 85552463
Conc: 8.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-21-S


Manual Integrations
APPROVED

Ankita
5/20/2019 2:03:22 PM

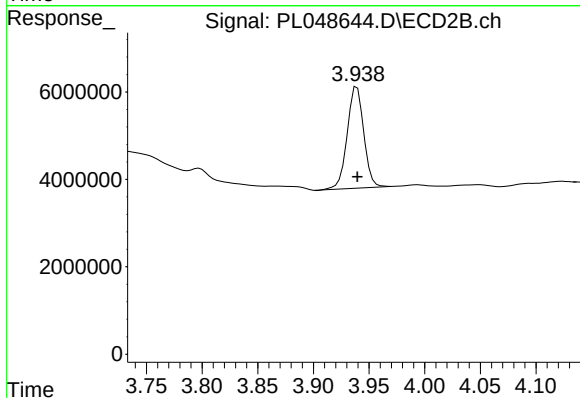


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 24159691
Conc: 9.70 ng/ml

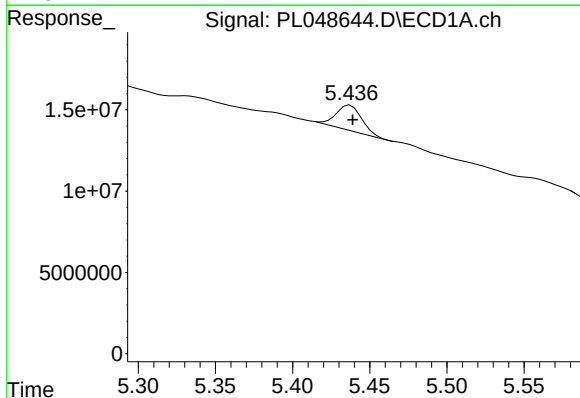


#12 4,4'-DDE

R.T.: 5.436 min
Delta R.T.: -0.002 min
Response: 17792183
Conc: 1.40 ng/ml m

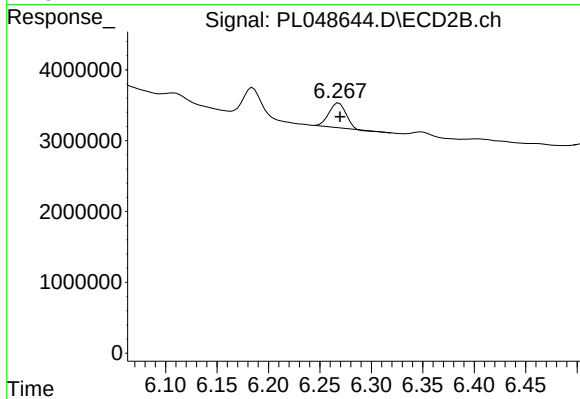

#12 4,4'-DDE

R.T.: 6.268 min
Delta R.T.: 0.000 min
Response: 3850429
Conc: 1.39 ng/ml

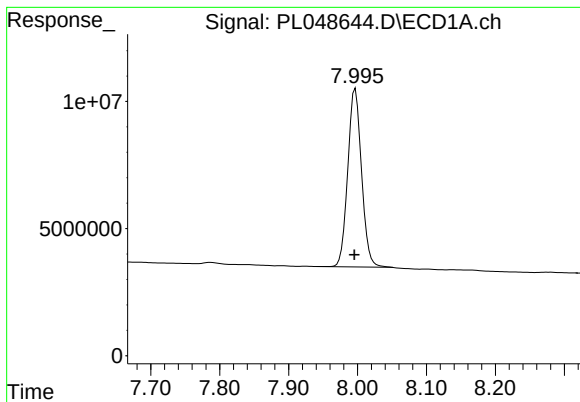

#28 Decachlorobiphenyl

R.T.: 7.997 min

Delta R.T.: 0.001 min


Response: 97323911

Conc: 9.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-21-S

Manual Integrations
APPROVED

Ankita
5/20/2019 2:03:22 PM

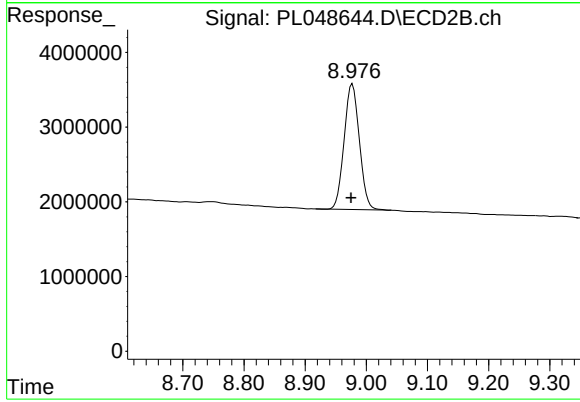

#28 Decachlorobiphenyl

R.T.: 8.977 min

Delta R.T.: 0.002 min

Response: 29142064

Conc: 10.98 ng/ml