

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051819\
 Data File : PL048686.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2019 00:26
 Operator : SM\AJ
 Sample : K2881-01
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-PS-01-047

Manual Integrations
 APPROVED

Ankita
 5/20/2019 2:03:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 01:45:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.327	3.939	194.9E6	53703680	20.116	21.560
2) SA Decachlor...	7.996	8.976	143.3E6	42988537	14.252	16.196
Target Compounds						
10) B gamma-Chl...	5.212	6.036	5336444	1682841	0.400m	0.547m#
11) B alpha-Chl...	5.268	6.111	7288357	2826923	0.557m	0.921 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051819\
Data File : PL048686.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2019 00:26
Operator : SM\AJ
Sample : K2881-01
Misc :
ALS Vial : 51 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FK-PS-01-047


Manual Integrations
APPROVED

Ankita
5/20/2019 2:03:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 01:45:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

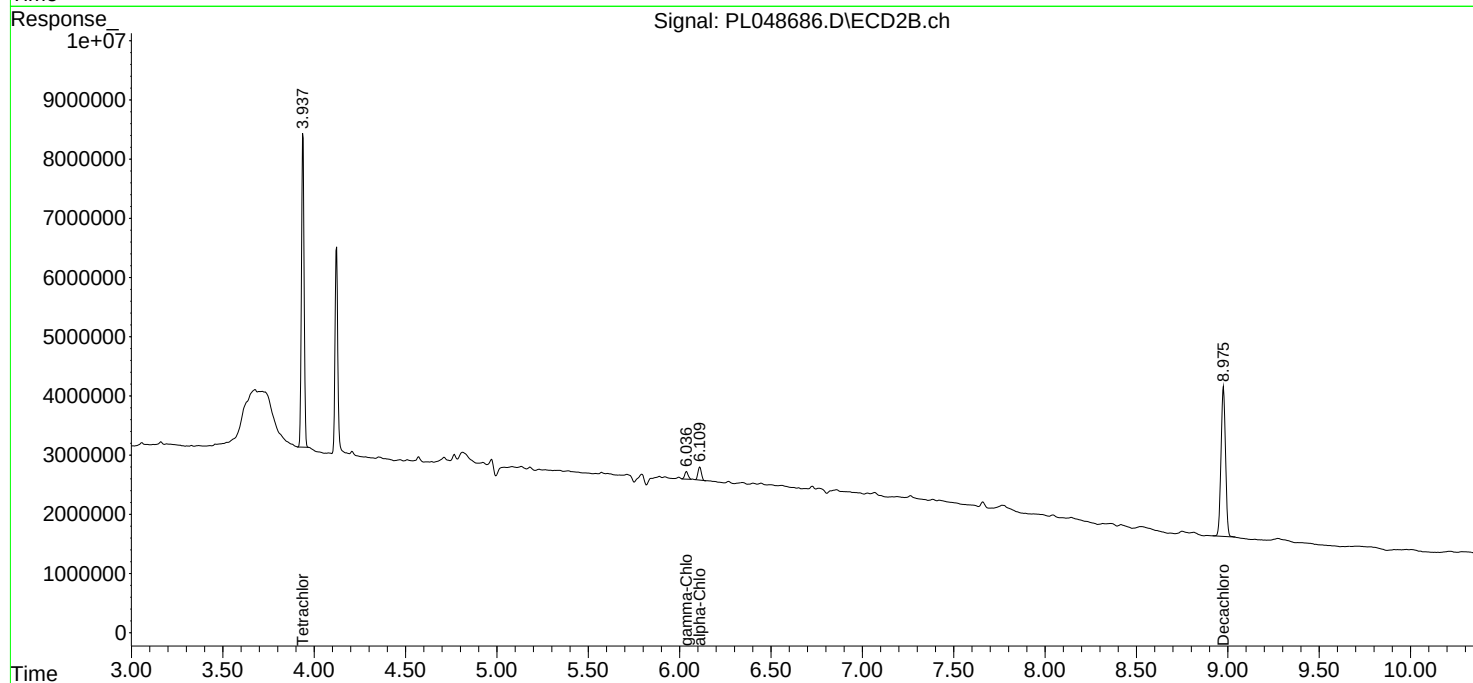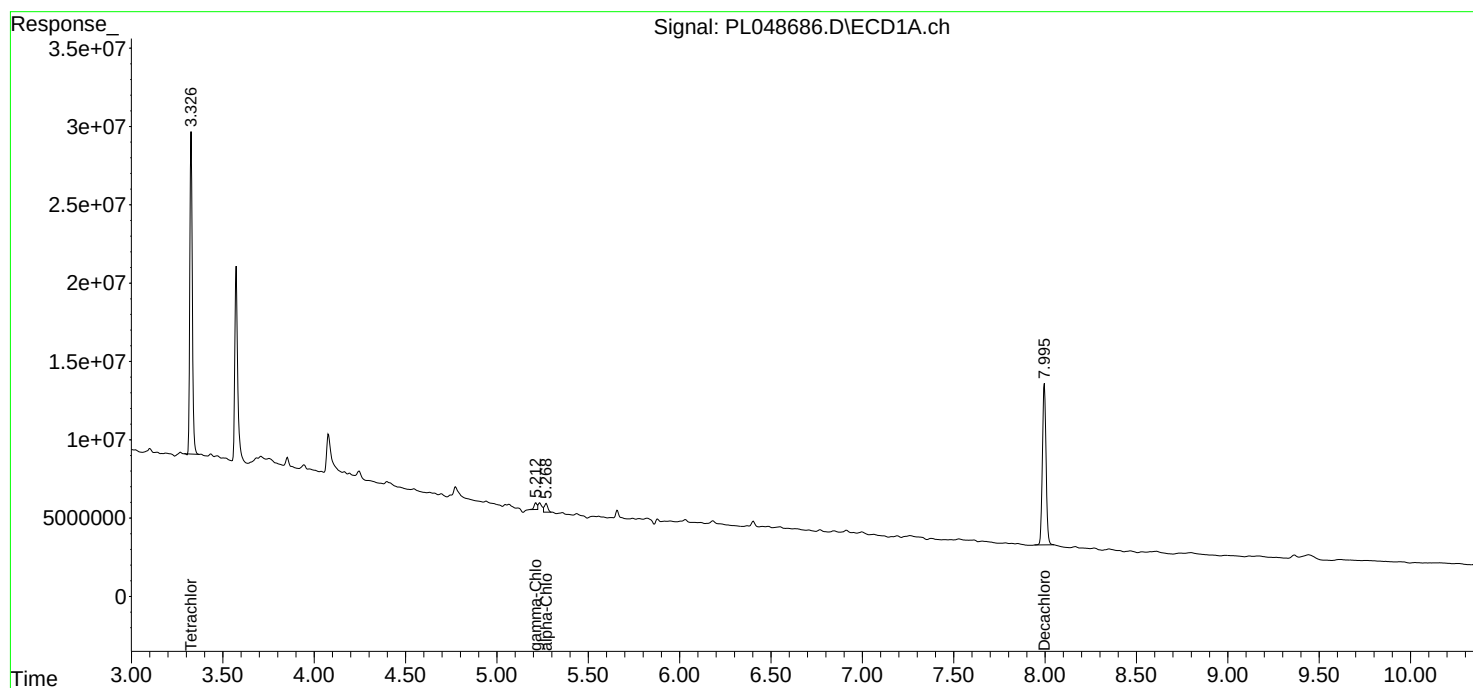

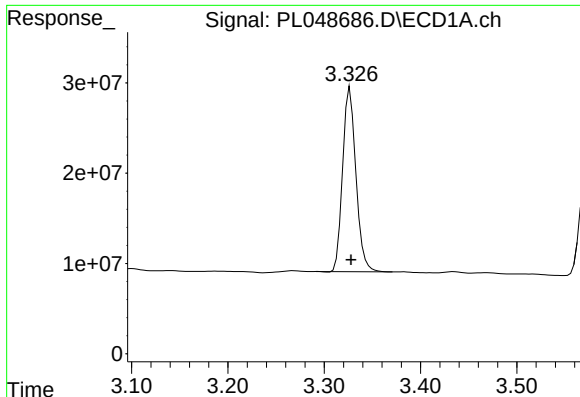


#1 Tetrachloro-m-xylene

R.T.: 3.327 min
Delta R.T.: 0.000 min
Response: 194862876
Conc: 20.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-047


Manual Integrations
APPROVED

Ankita
5/20/2019 2:03:51 PM

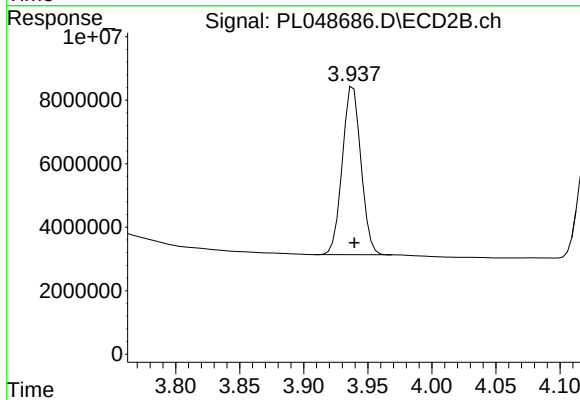


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: -0.001 min
Response: 53703680
Conc: 21.56 ng/ml

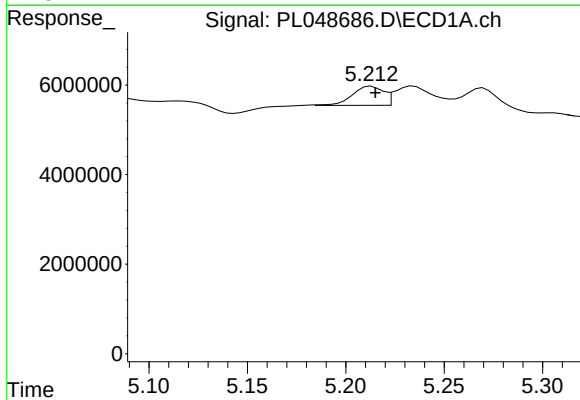


#10 gamma-Chlordane

R.T.: 5.212 min
Delta R.T.: -0.003 min
Response: 5336444
Conc: 0.40 ng/ml m

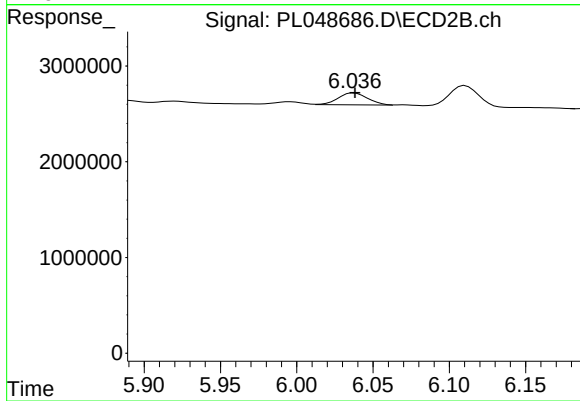

#10 gamma-Chlordane

R.T.: 6.036 min
Delta R.T.: -0.002 min
Response: 1682841
Conc: 0.55 ng/ml m

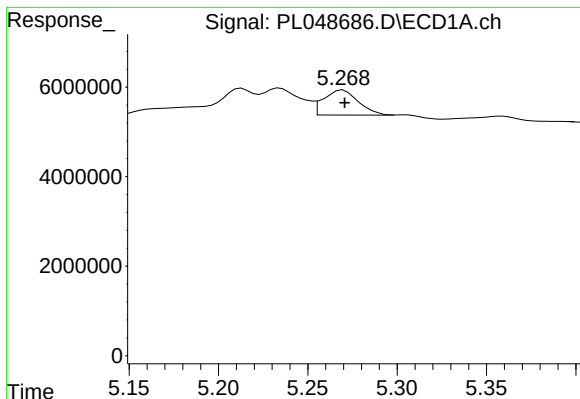


#11 alpha-Chlordane

R.T.: 5.268 min
Delta R.T.: -0.002 min
Response: 7288357
Conc: 0.56 ng/ml m

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-047


Manual Integrations
APPROVED

Ankita
5/20/2019 2:03:51 PM

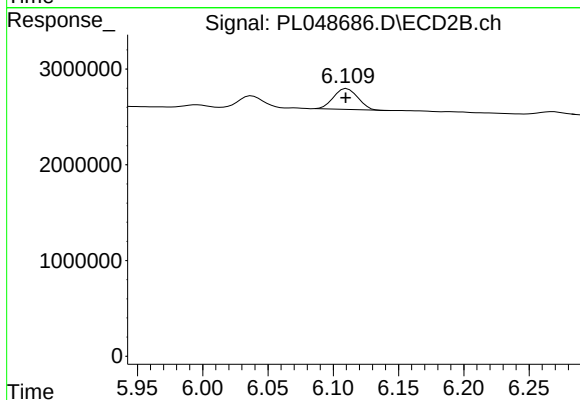


#11 alpha-Chlordane

R.T.: 6.111 min
Delta R.T.: 0.001 min
Response: 2826923
Conc: 0.92 ng/ml

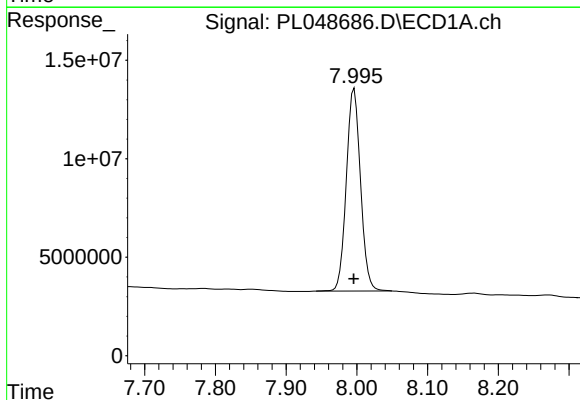

#28 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: 0.000 min
Response: 143296172
Conc: 14.25 ng/ml

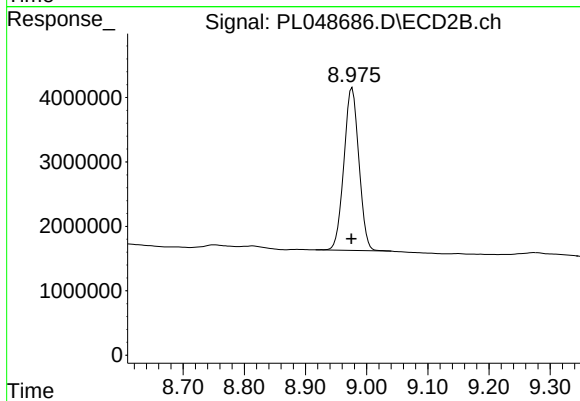

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: 0.001 min
Response: 42988537
Conc: 16.20 ng/ml