

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051820\
 Data File : PL058762.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2020 14:11
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 23:08:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
 Quant Title : GC Extractables
 QLast Update : Fri May 15 06:18:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.530	4.077	36670898	56284270	22.322	26.002
28)	SA Decachlor...	8.315	9.189	32405287	53197797	24.817	30.101
Target Compounds							
4)	MA Heptachlor	0.000	5.269	0	448726	N.D.	0.160 #
8)	B Heptachlo...	0.000	5.955	0	492536	N.D.	0.205 #
9)	A Endosulfan I	0.000	6.315	0	712886	N.D.	0.331 #
14)	MA Endrin	0.000	6.828f	0	450048	N.D.	0.248 #
15)	B Endosulfa...	0.000	7.011	0	1094017	N.D.	0.548 #
16)	A 4,4'-DDD	0.000	6.944f	0	66826	N.D.	0.038 #
22)	Mirex	7.465	0.000	1287149	0	1.053	N.D. #
27)	Chlordane-5	0.000	7.078	0	396188	N.D.	6.346 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051820\
Data File : PL058762.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2020 14:11
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 23:08:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
Quant Title : GC Extractables
QLast Update : Fri May 15 06:18:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

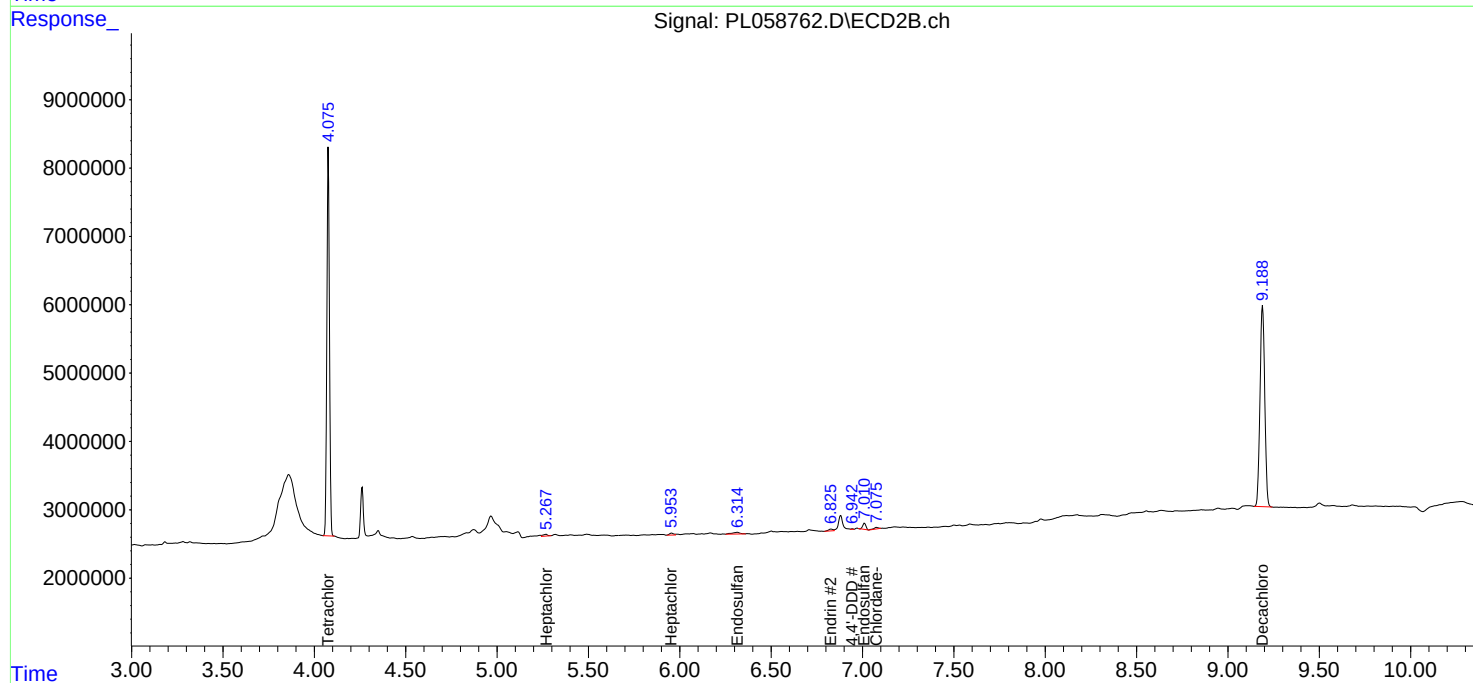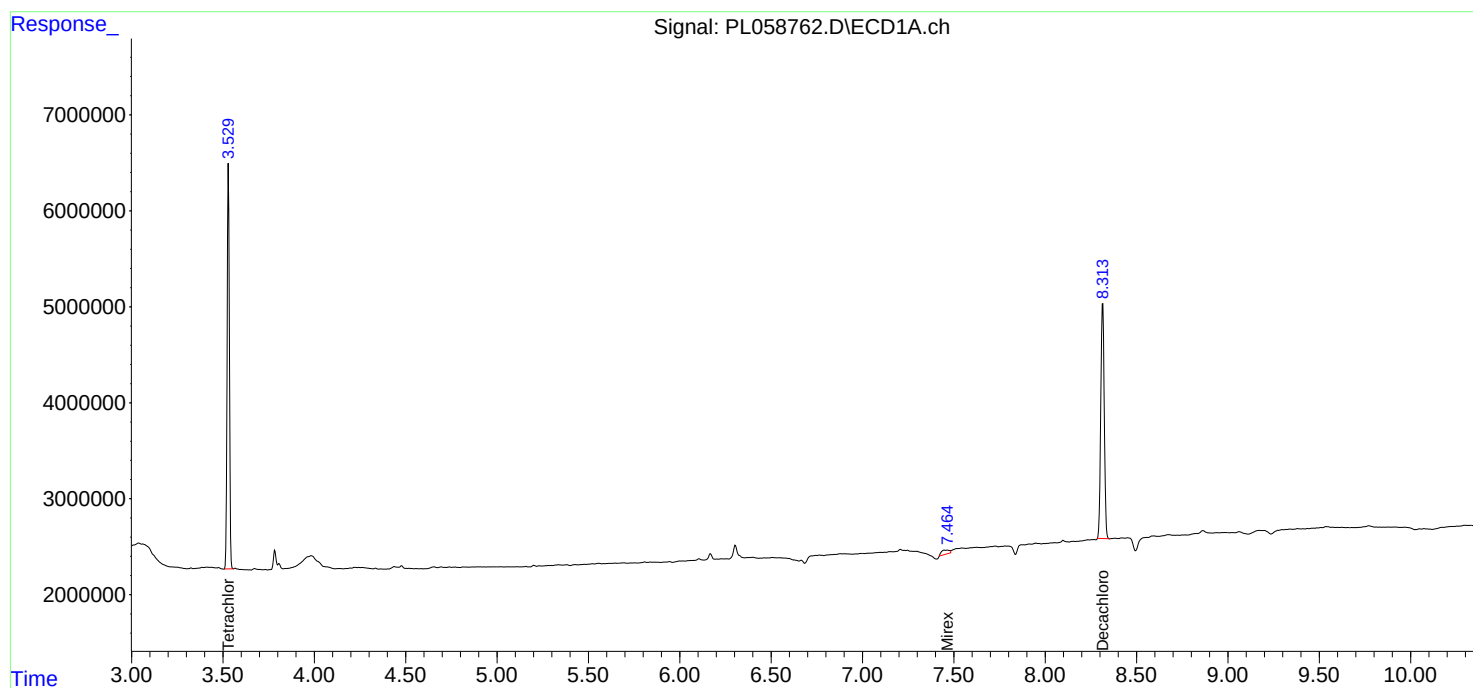


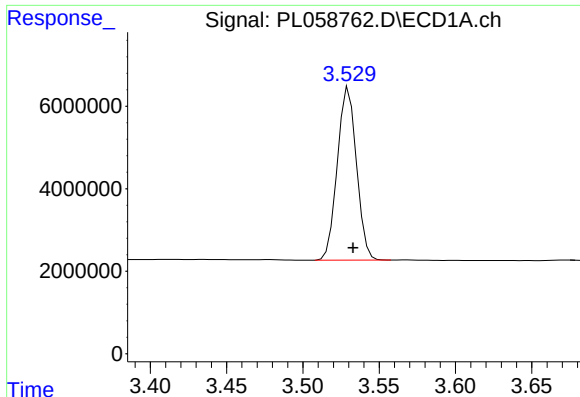

#1 Tetrachloro-m-xylene


R.T.: 3.530 min
Delta R.T.: -0.003 min
Response: 36670898
Conc: 22.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

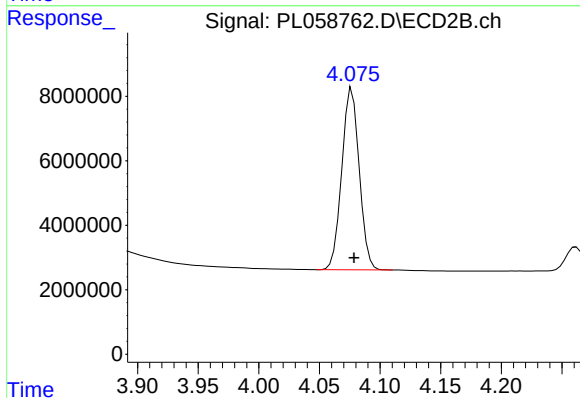


#1 Tetrachloro-m-xylene

R.T.: 4.077 min
Delta R.T.: -0.002 min
Response: 56284270
Conc: 26.00 ng/ml

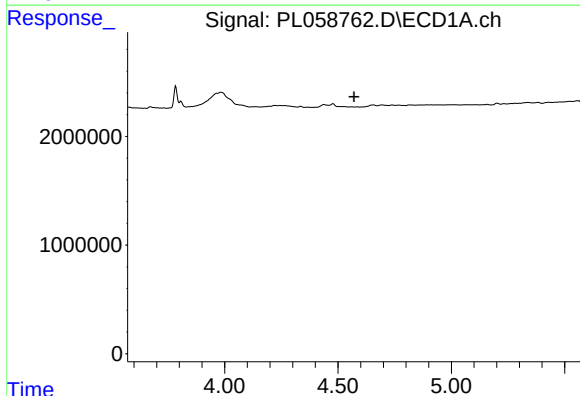


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.571 min
Response: 0
Conc: N.D.

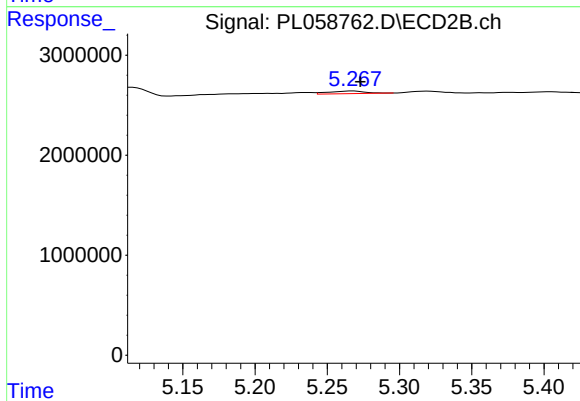

#4 Heptachlor


R.T.: 5.269 min
Delta R.T.: -0.004 min
Response: 448726
Conc: 0.16 ng/ml

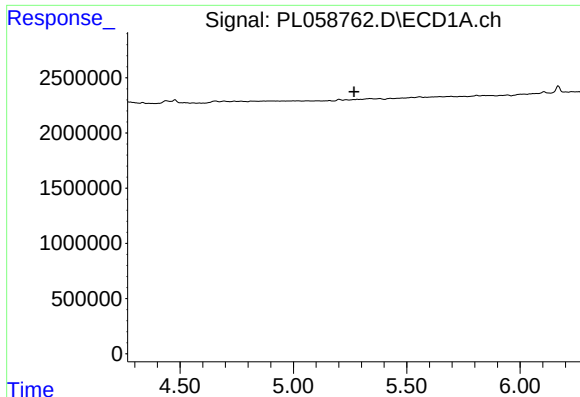

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

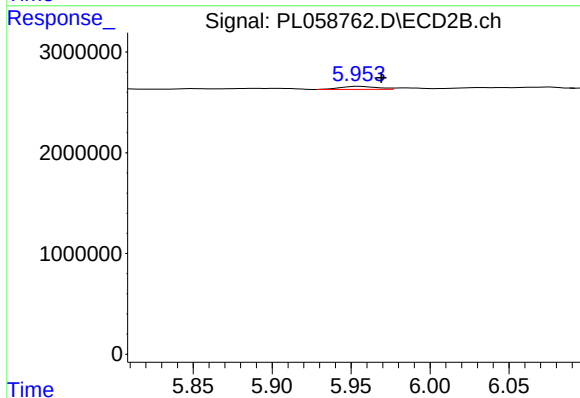


#8 Heptachlor epoxide

R.T.: 5.955 min
Delta R.T.: -0.014 min
Response: 492536
Conc: 0.21 ng/ml

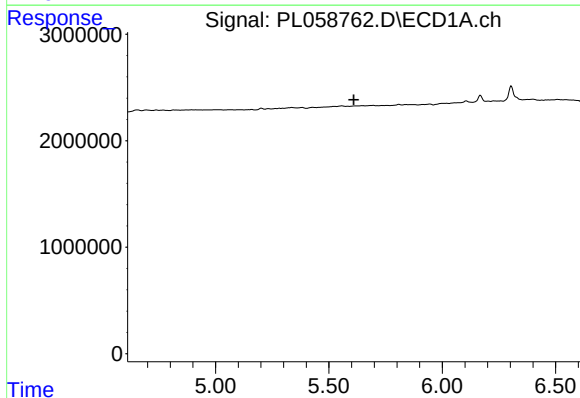


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.609 min
Response: 0
Conc: N.D.

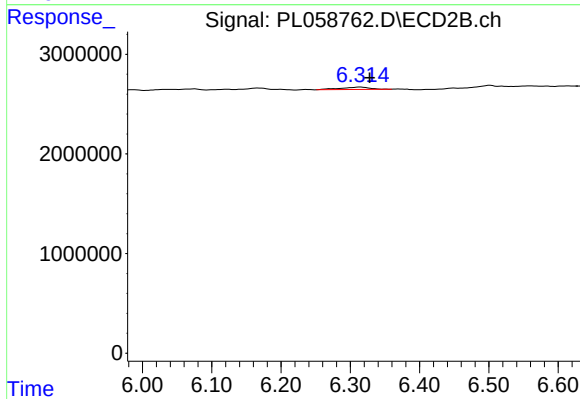

#9 Endosulfan I


R.T.: 6.315 min
Delta R.T.: -0.013 min
Response: 712886
Conc: 0.33 ng/ml

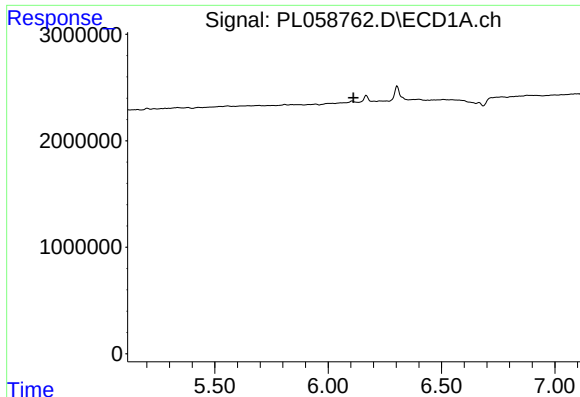

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.112 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

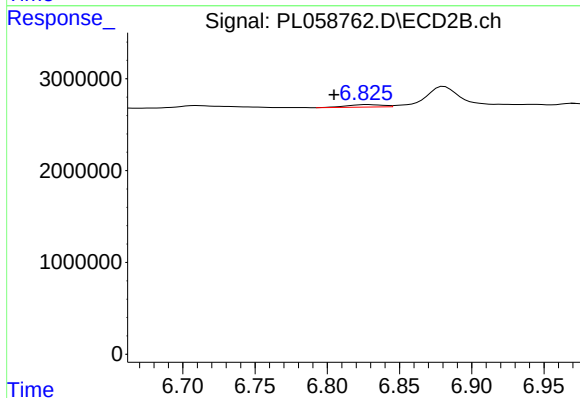


#14 Endrin

R.T.: 6.828 min
Delta R.T.: 0.024 min
Response: 450048
Conc: 0.25 ng/ml

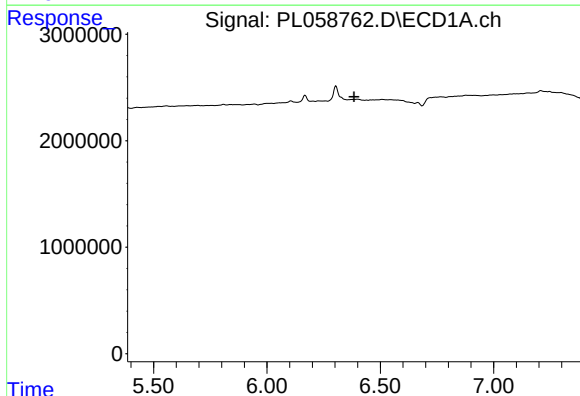


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.385 min
Response: 0
Conc: N.D.

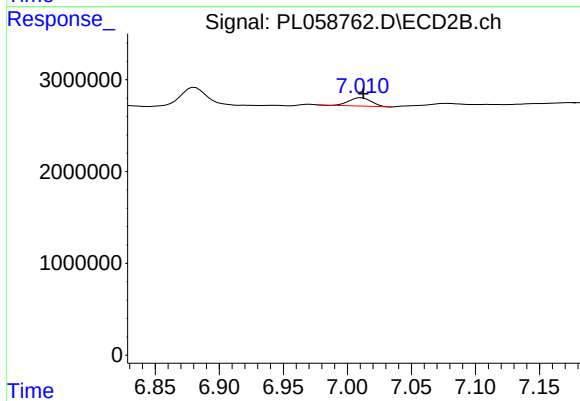

#15 Endosulfan II


R.T.: 7.011 min
Delta R.T.: -0.001 min
Response: 1094017
Conc: 0.55 ng/ml

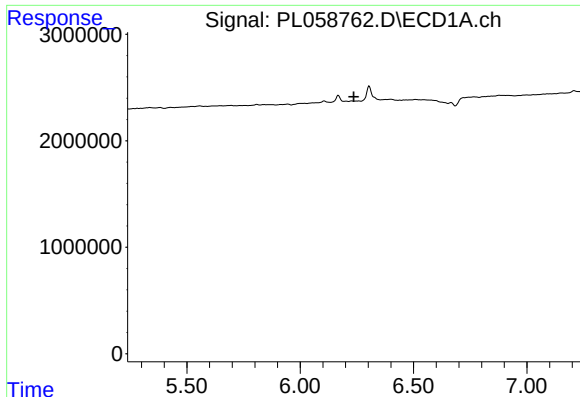

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.237 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

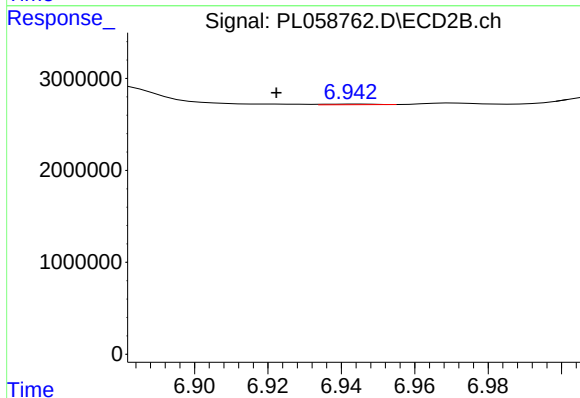


#16 4,4'-DDD

R.T.: 6.944 min
Delta R.T.: 0.022 min
Response: 66826
Conc: 0.04 ng/ml

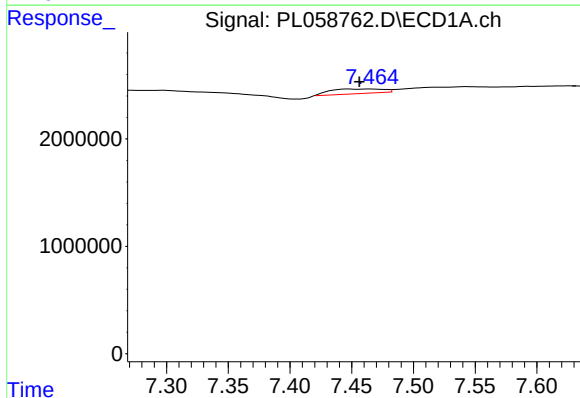


#22 Mirex

R.T.: 7.465 min
Delta R.T.: 0.009 min
Response: 1287149
Conc: 1.05 ng/ml

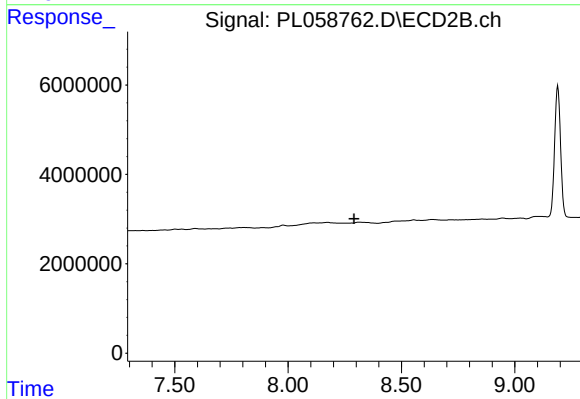

#22 Mirex

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

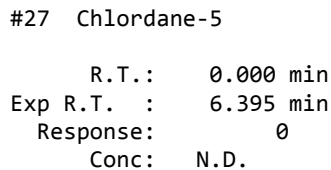

Instrument :
ECD_L
ClientSampleId :

