

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051820\
 Data File : PL058771.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2020 16:43
 Operator : AJ\MA
 Sample : PB128948BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 23:10:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
 Quant Title : GC Extractables
 QLast Update : Fri May 15 06:18:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.531	4.077	33157253	52509700	20.183	24.258
28)	SA Decachlor...	8.315	9.191	27710143	52470873	21.221	29.690 #
Target Compounds							
4)	MA Heptachlor	0.000	5.264	0	512511	N.D.	0.183 #
7)	B delta-BHC	0.000	5.119f	0	1516937	N.D.	0.535 #
8)	B Heptachlo...	0.000	5.956	0	3965487	N.D.	1.651 #
10)	B gamma-Chl...	5.503	0.000	6554595	0	4.219	N.D. #
15)	B Endosulfa...	0.000	7.013	0	1178085	N.D.	0.590 #
16)	A 4,4'-DDD	6.242	6.934	20421952	507476	17.316	0.290 #
17)	MA 4,4'-DDT	0.000	7.227	0	178010	N.D.	0.105 #
25)	Chlordane-3	5.503	0.000	6554595	0	46.851	N.D. #
27)	Chlordane-5	0.000	7.081	0	1076122	N.D.	17.237 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051820\
Data File : PL058771.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2020 16:43
Operator : AJ\MA
Sample : PB128948BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 23:10:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
Quant Title : GC Extractables
QLast Update : Fri May 15 06:18:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

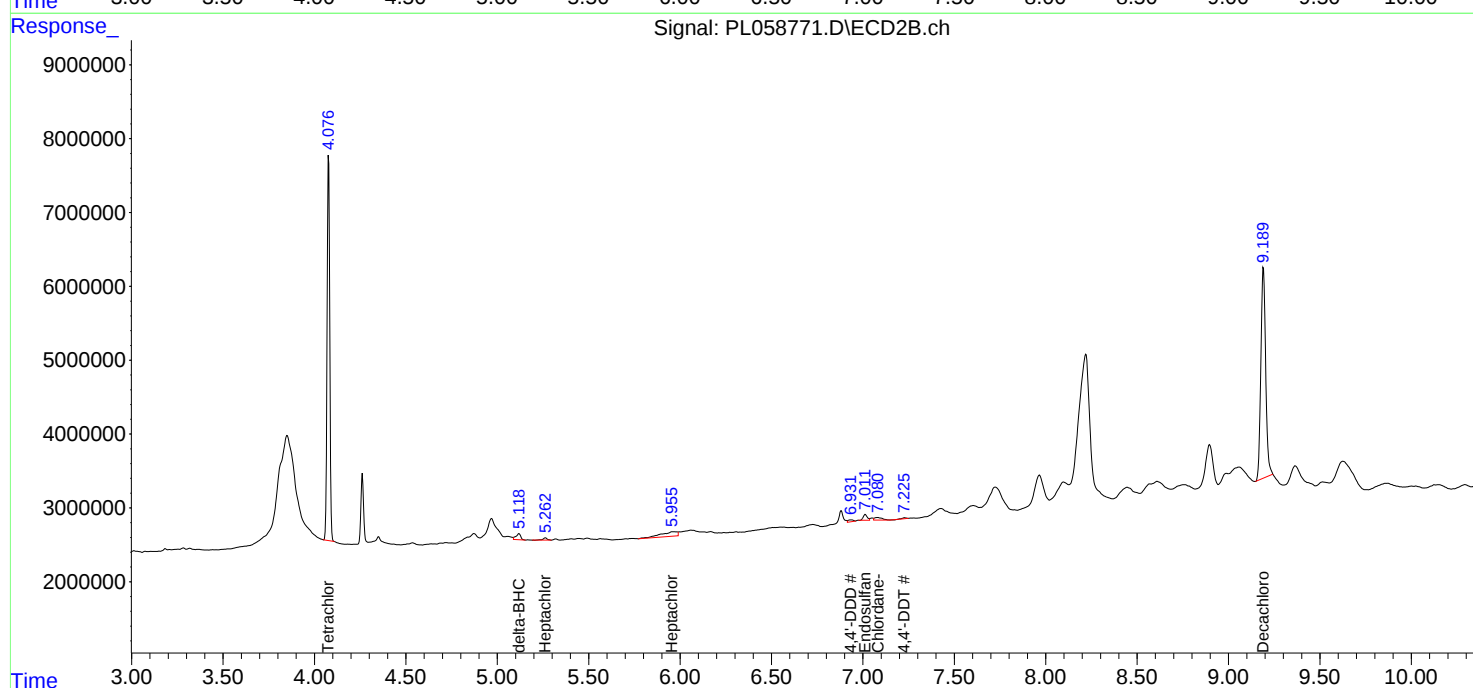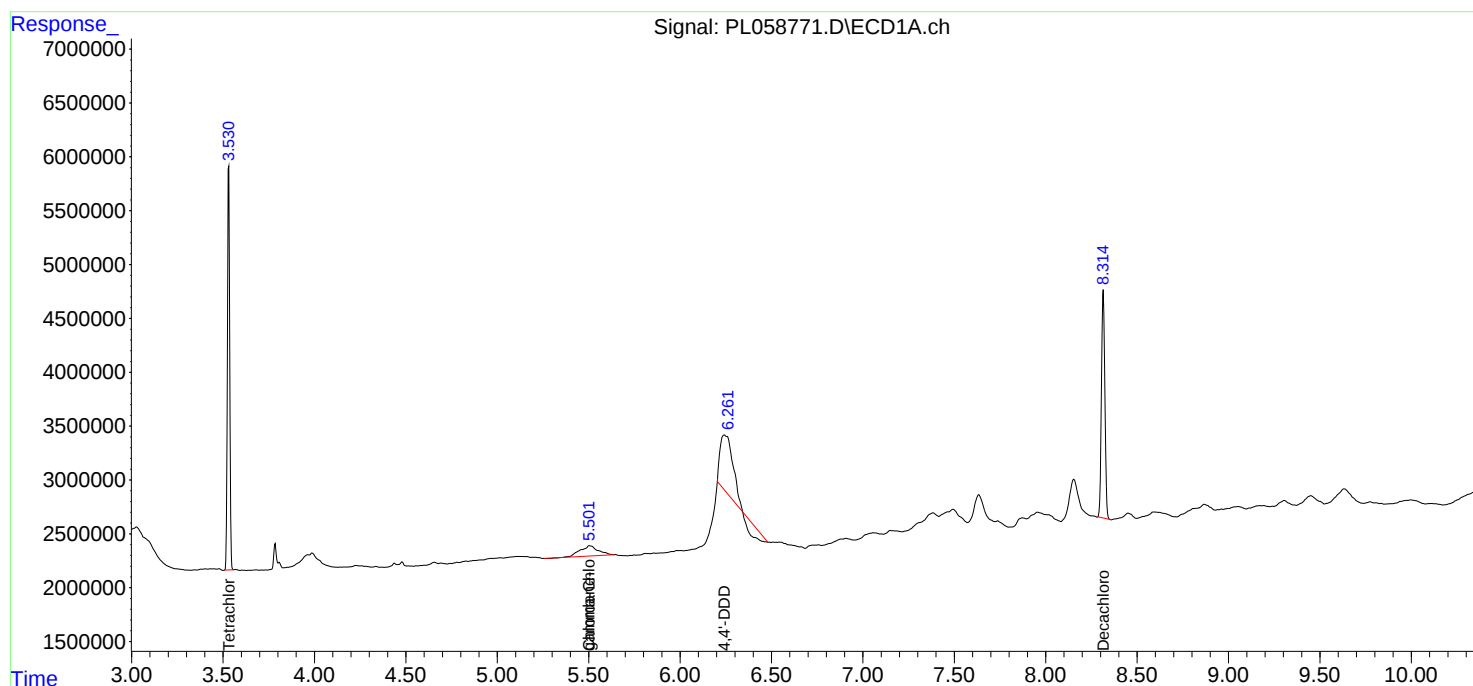


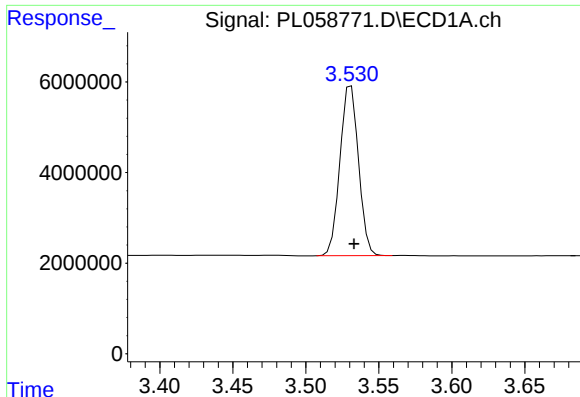

#1 Tetrachloro-m-xylene


R.T.: 3.531 min
Delta R.T.: -0.002 min
Response: 33157253
Conc: 20.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

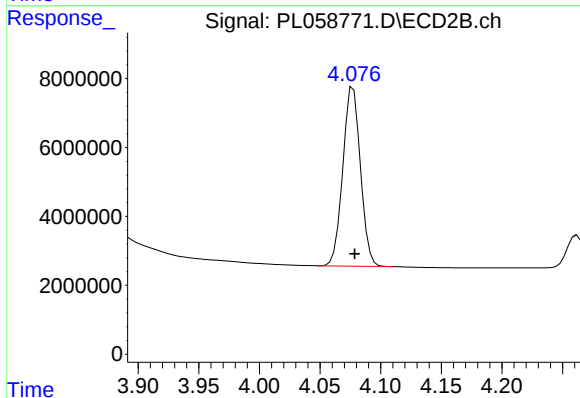


#1 Tetrachloro-m-xylene

R.T.: 4.077 min
Delta R.T.: -0.001 min
Response: 52509700
Conc: 24.26 ng/ml

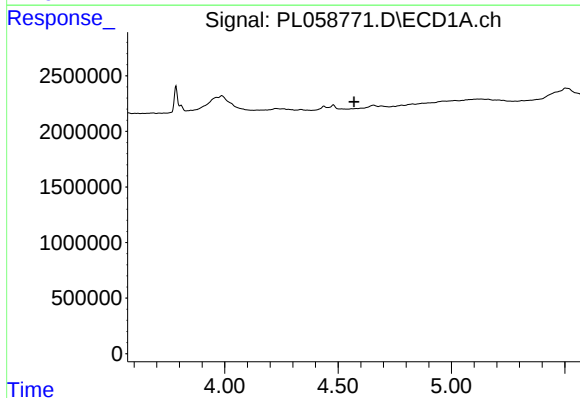


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.571 min
Response: 0
Conc: N.D.

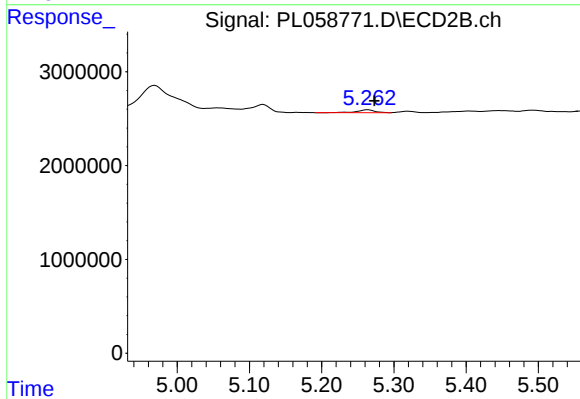

#4 Heptachlor


R.T.: 5.264 min
Delta R.T.: -0.009 min
Response: 512511
Conc: 0.18 ng/ml

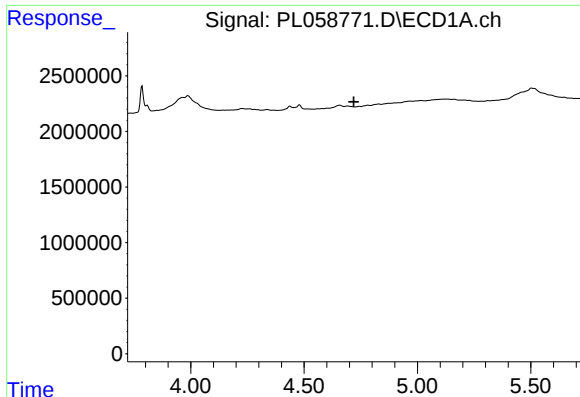

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.719 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

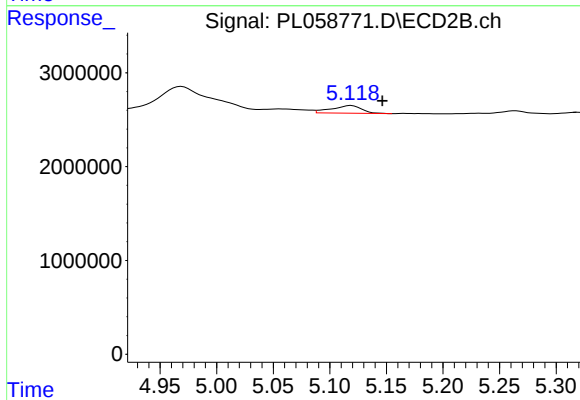


#7 delta-BHC

R.T.: 5.119 min
Delta R.T.: -0.027 min
Response: 1516937
Conc: 0.53 ng/ml

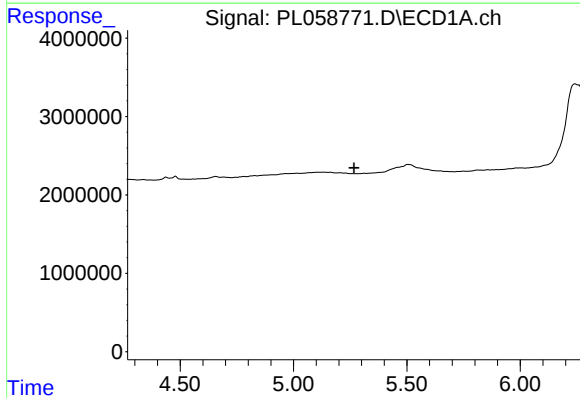


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.268 min
Response: 0
Conc: N.D.

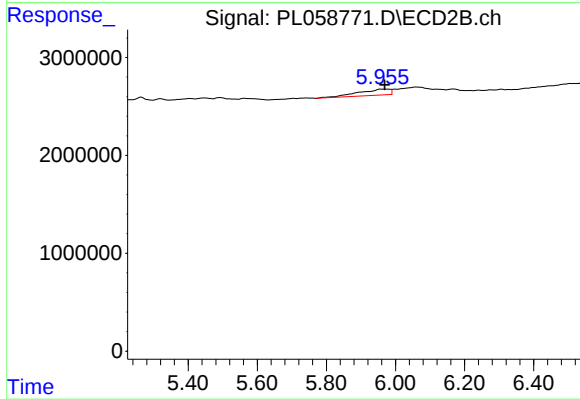

#8 Heptachlor epoxide


R.T.: 5.956 min
Delta R.T.: -0.013 min
Response: 3965487
Conc: 1.65 ng/ml

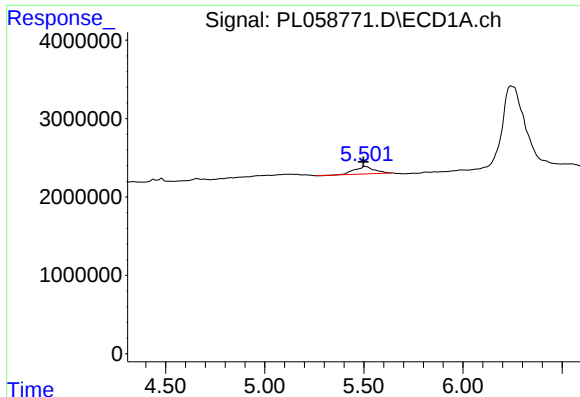

#10 gamma-Chlordane


R.T.: 5.503 min
Delta R.T.: 0.006 min
Response: 6554595
Conc: 4.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

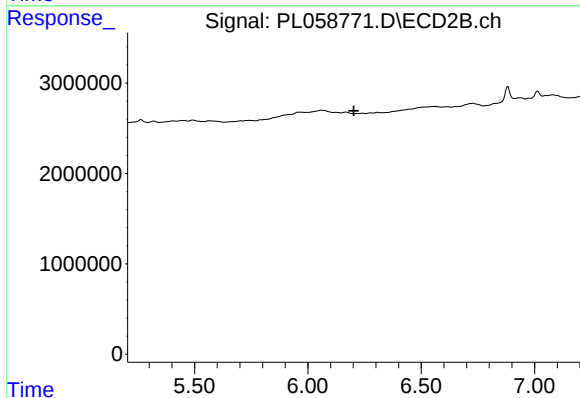


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.203 min
Response: 0
Conc: N.D.

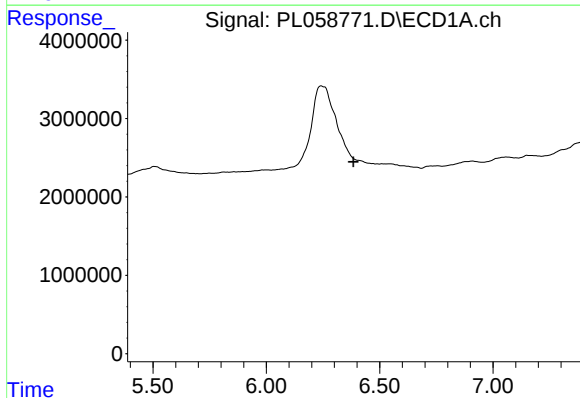


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.385 min
Response: 0
Conc: N.D.

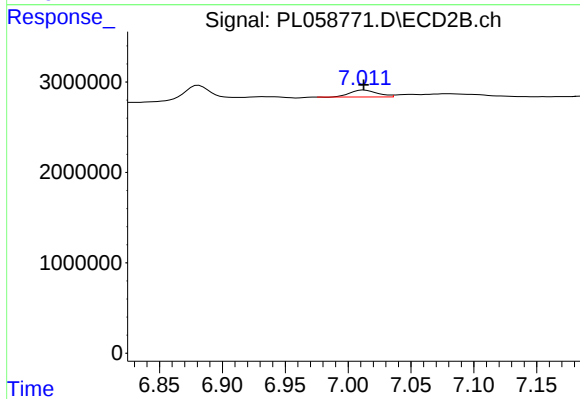

#15 Endosulfan II


R.T.: 7.013 min
Delta R.T.: 0.000 min
Response: 1178085
Conc: 0.59 ng/ml

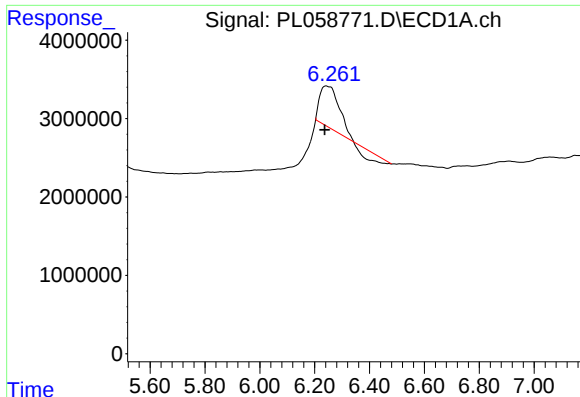

#16 4,4'-DDD


R.T.: 6.242 min
Delta R.T.: 0.005 min
Response: 20421952
Conc: 17.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

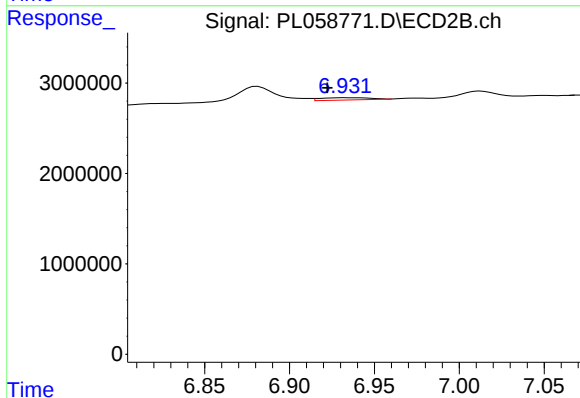


#16 4,4'-DDD

R.T.: 6.934 min
Delta R.T.: 0.012 min
Response: 507476
Conc: 0.29 ng/ml

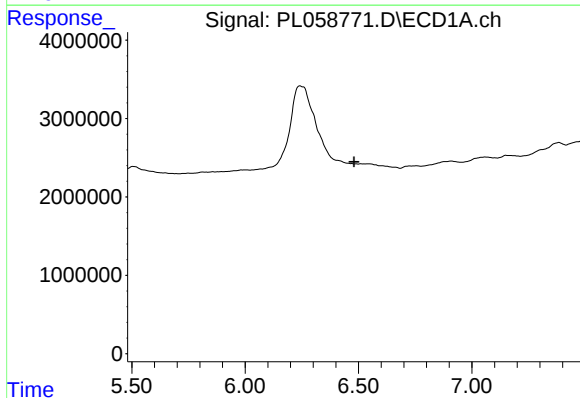


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.480 min
Response: 0
Conc: N.D.

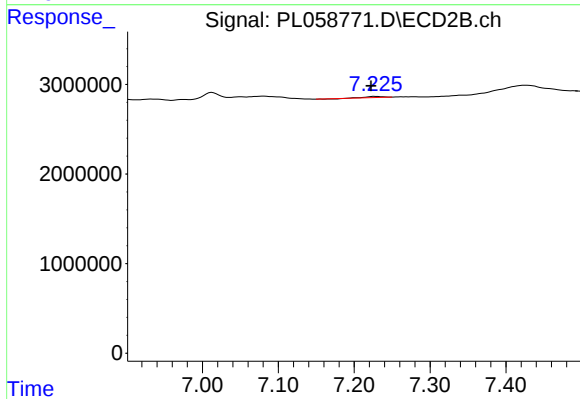

#17 4,4'-DDT


R.T.: 7.227 min
Delta R.T.: 0.005 min
Response: 178010
Conc: 0.11 ng/ml

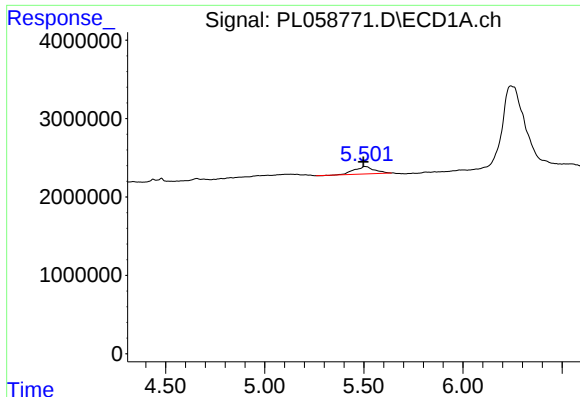

#25 Chlordane-3


R.T.: 5.503 min
Delta R.T.: 0.006 min
Response: 6554595
Conc: 46.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

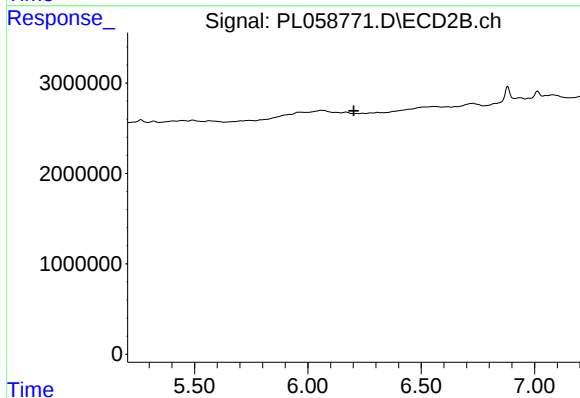


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.203 min
Response: 0
Conc: N.D.

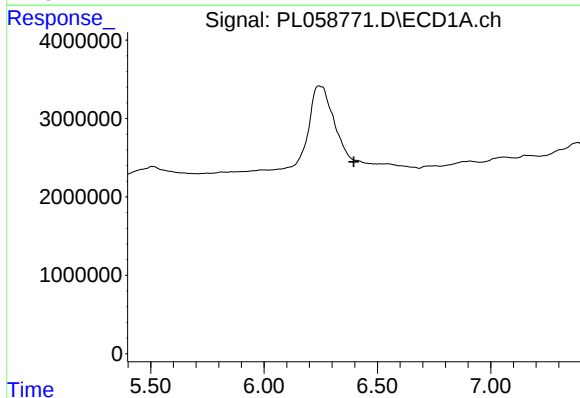


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.395 min
Response: 0
Conc: N.D.

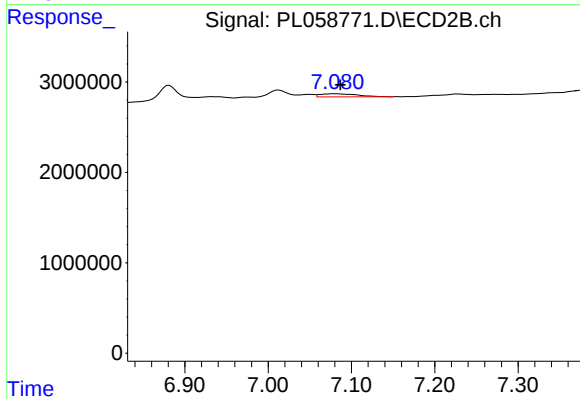

#27 Chlordane-5


R.T.: 7.081 min
Delta R.T.: -0.006 min
Response: 1076122
Conc: 17.24 ng/ml

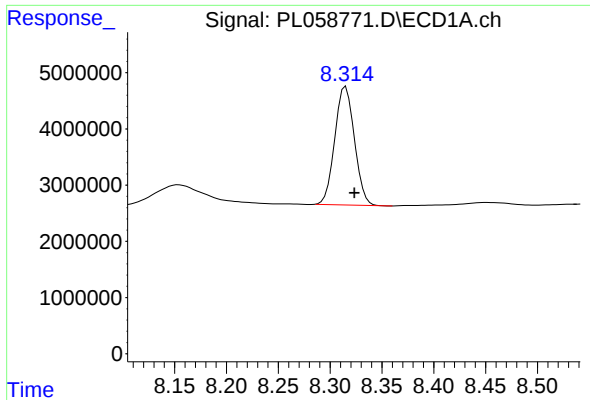

#28 Decachlorobiphenyl

R.T.: 8.315 min
Delta R.T.: -0.008 min
Response: 27710143
Conc: 21.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

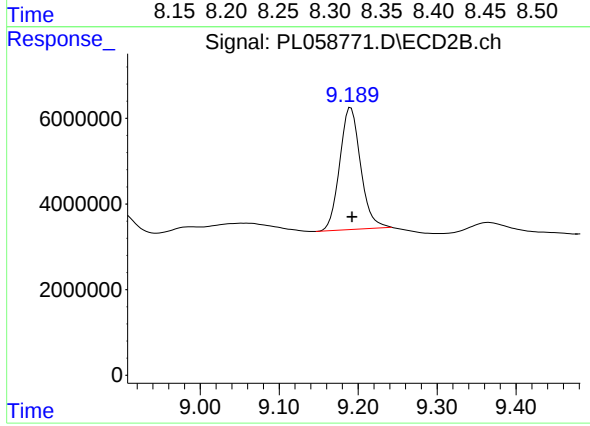

#28 Decachlorobiphenyl

R.T.: 9.191 min
Delta R.T.: -0.002 min
Response: 52470873
Conc: 29.69 ng/ml