

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051820\
 Data File : PL058775.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2020 17:39
 Operator : AJ\MA
 Sample : PB128958BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 23:10:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
 Quant Title : GC Extractables
 QLast Update : Fri May 15 06:18:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.531	4.078	31051042	51311133	18.901	23.705 #
28)	SA Decachlor...	8.316	9.190	28906950	49225967	22.138	27.854 #
Target Compounds							
4)	MA Heptachlor	0.000	5.265	0	633871	N.D.	0.226 #
7)	B delta-BHC	0.000	5.119f	0	1226382	N.D.	0.432 #
10)	B gamma-Chl...	0.000	6.174f	0	164018	N.D.	0.070 #
11)	B alpha-Chl...	0.000	6.274	0	66731	N.D.	0.028 #
13)	MA Dieldrin	5.832f	0.000	1338473	0	0.899	N.D. #
14)	MA Endrin	0.000	6.822f	0	1254550	N.D.	0.692 #
15)	B Endosulfa...	0.000	7.012	0	986632	N.D.	0.494 #
25)	Chlordane-3	0.000	6.174f	0	164018	N.D.	0.542 #
26)	Chlordane-4	0.000	6.274	0	66731	N.D.	0.183 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051820\
Data File : PL058775.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2020 17:39
Operator : AJ\MA
Sample : PB128958BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 23:10:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
Quant Title : GC Extractables
QLast Update : Fri May 15 06:18:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

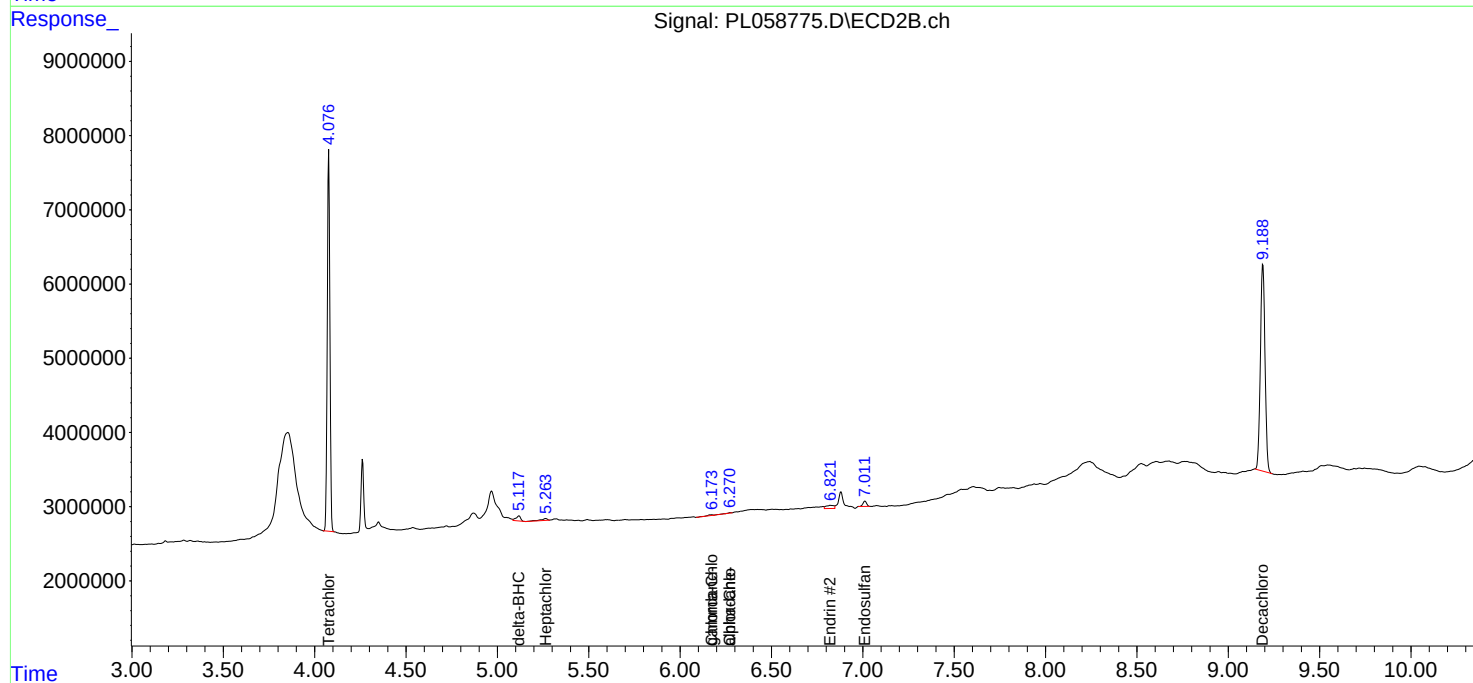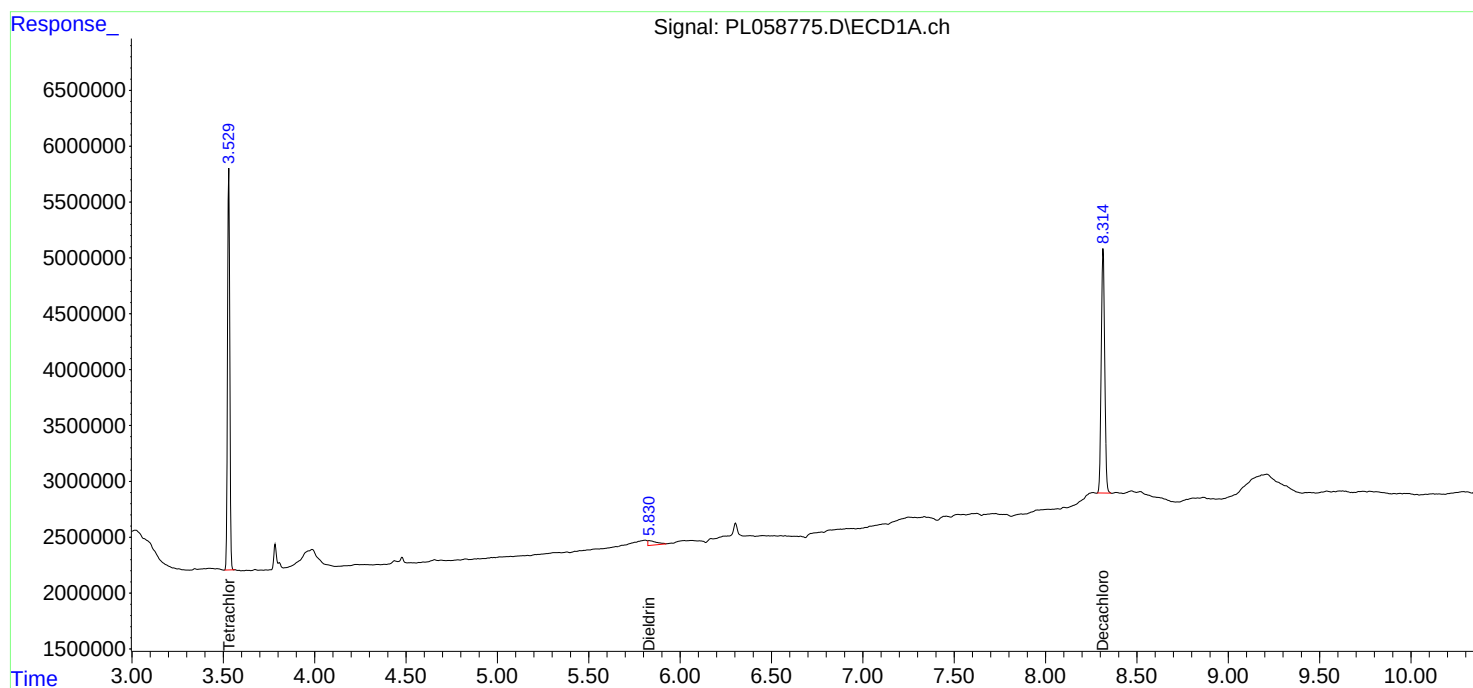


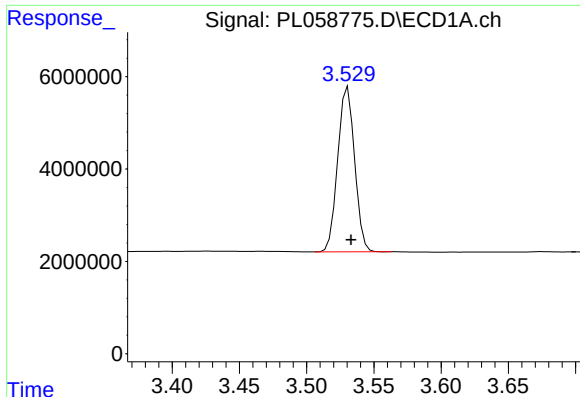

#1 Tetrachloro-m-xylene


R.T.: 3.531 min
Delta R.T.: -0.002 min
Response: 31051042
Conc: 18.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

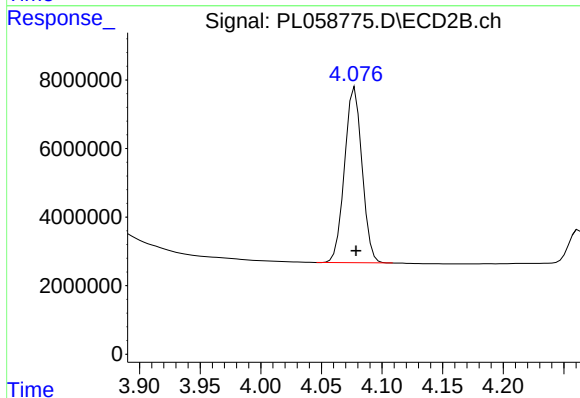


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 51311133
Conc: 23.70 ng/ml

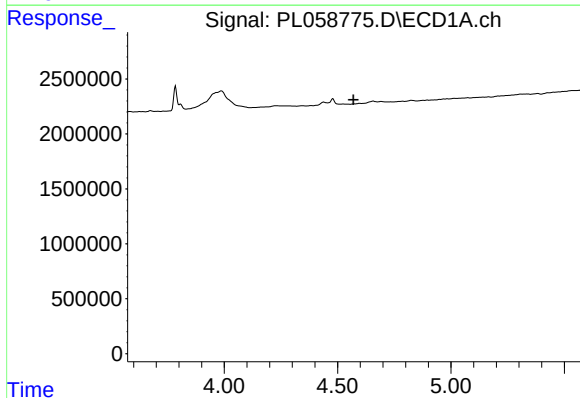


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.571 min
Response: 0
Conc: N.D.

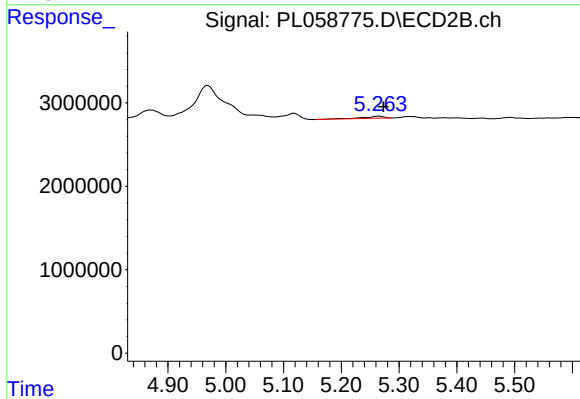

#4 Heptachlor


R.T.: 5.265 min
Delta R.T.: -0.008 min
Response: 633871
Conc: 0.23 ng/ml

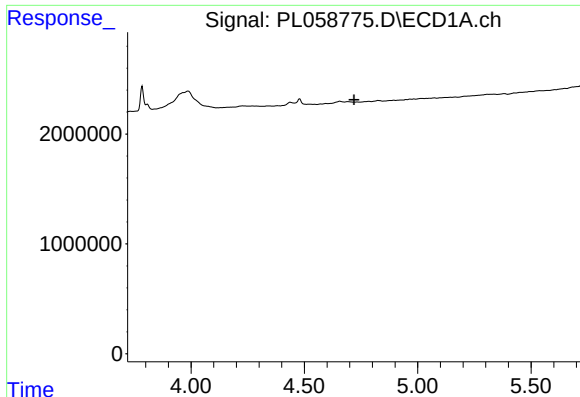

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.719 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

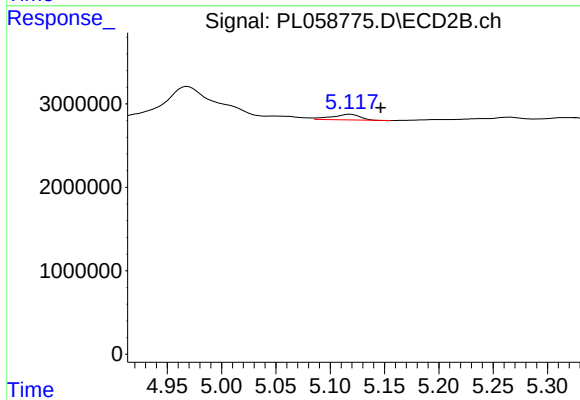


#7 delta-BHC

R.T.: 5.119 min
Delta R.T.: -0.028 min
Response: 1226382
Conc: 0.43 ng/ml

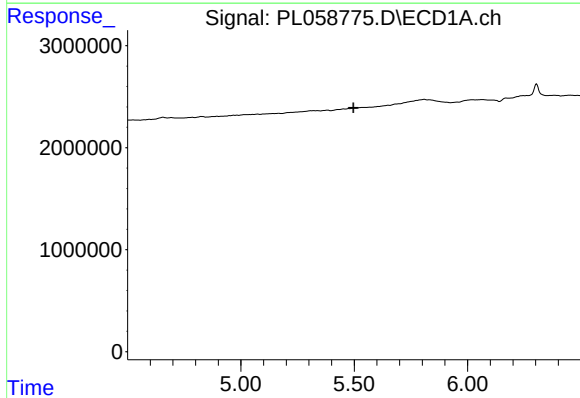


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

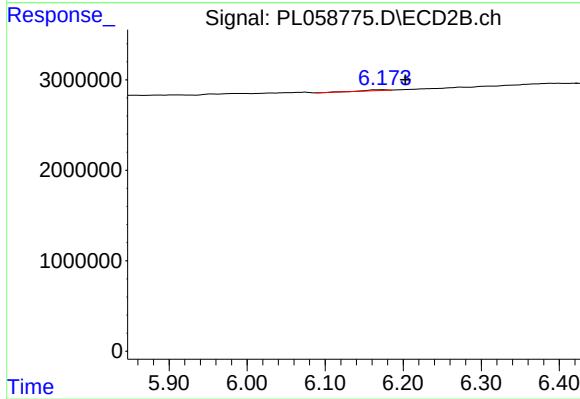

#10 gamma-Chlordane


R.T.: 6.174 min
Delta R.T.: -0.029 min
Response: 164018
Conc: 0.07 ng/ml

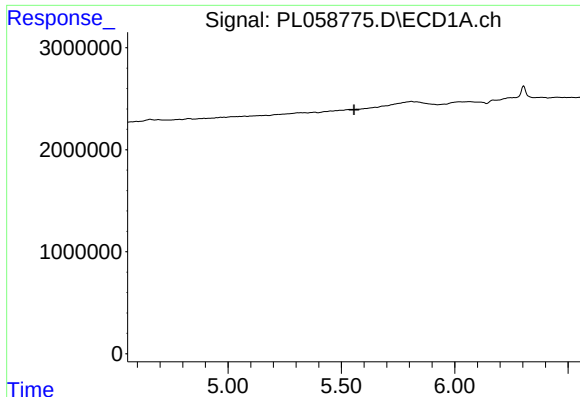

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.556 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

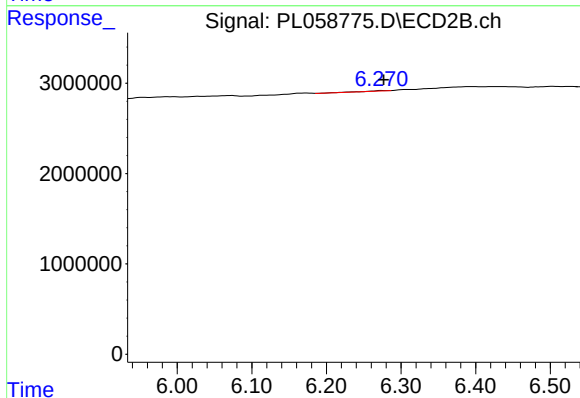


#11 alpha-Chlordane

R.T.: 6.274 min
Delta R.T.: -0.003 min
Response: 66731
Conc: 0.03 ng/ml

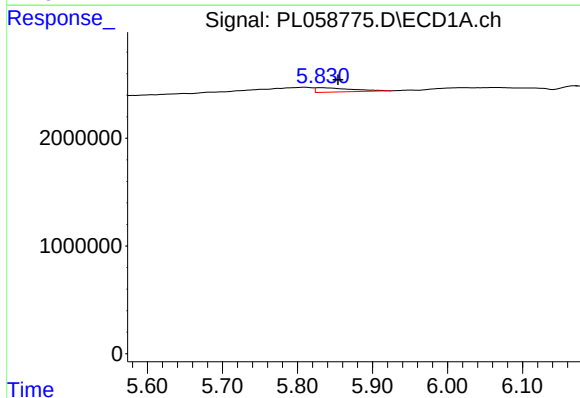


#13 Dieldrin

R.T.: 5.832 min
Delta R.T.: -0.022 min
Response: 1338473
Conc: 0.90 ng/ml

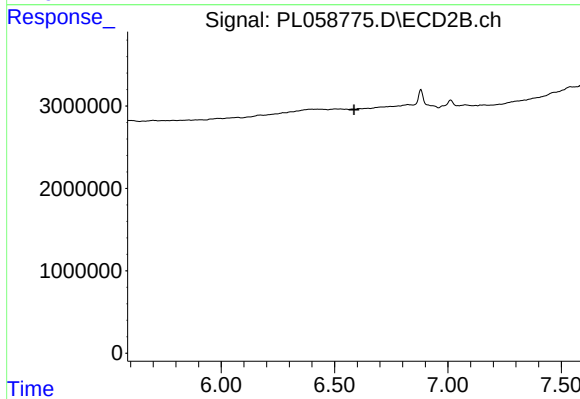

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.586 min
Response: 0
Conc: N.D.

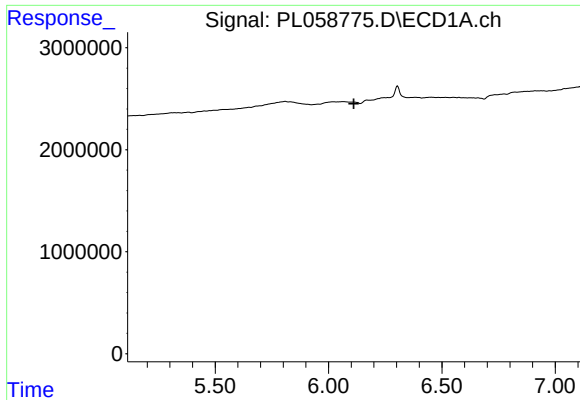

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.112 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

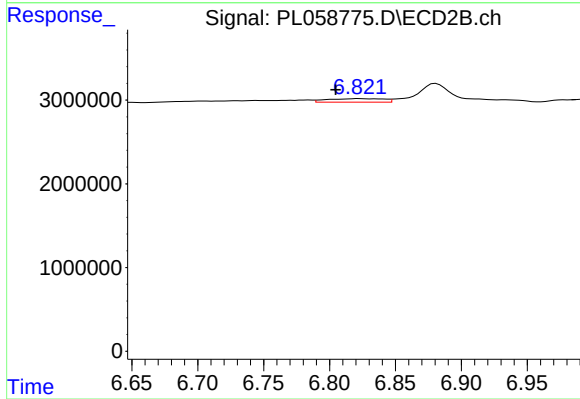


#14 Endrin

R.T.: 6.822 min
Delta R.T.: 0.018 min
Response: 1254550
Conc: 0.69 ng/ml

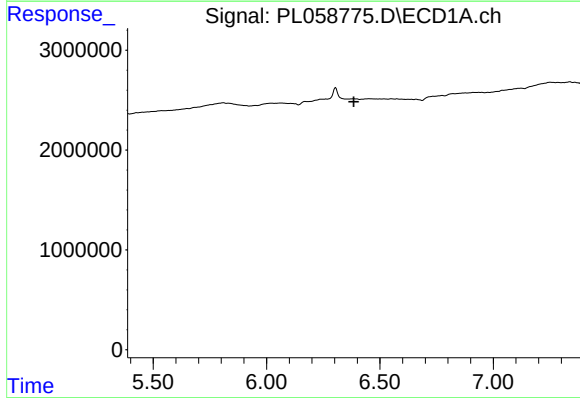


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.385 min
Response: 0
Conc: N.D.

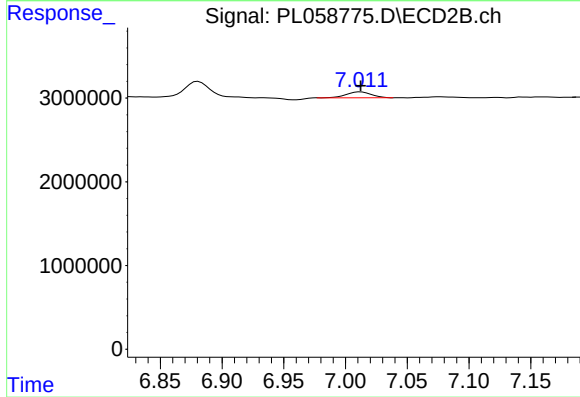

#15 Endosulfan II


R.T.: 7.012 min
Delta R.T.: 0.000 min
Response: 986632
Conc: 0.49 ng/ml

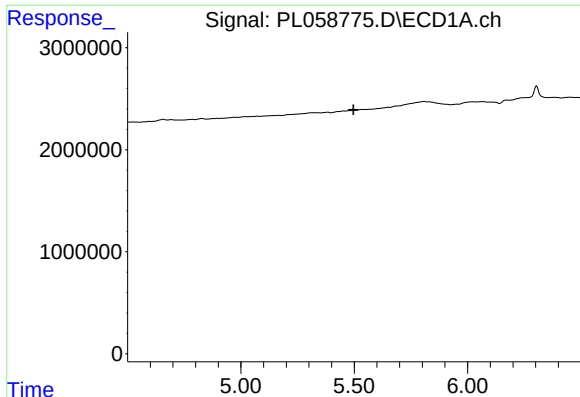

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

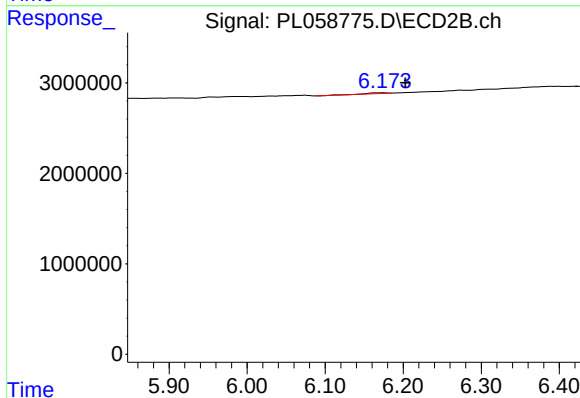


#25 Chlordane-3

R.T.: 6.174 min
Delta R.T.: -0.028 min
Response: 164018
Conc: 0.54 ng/ml

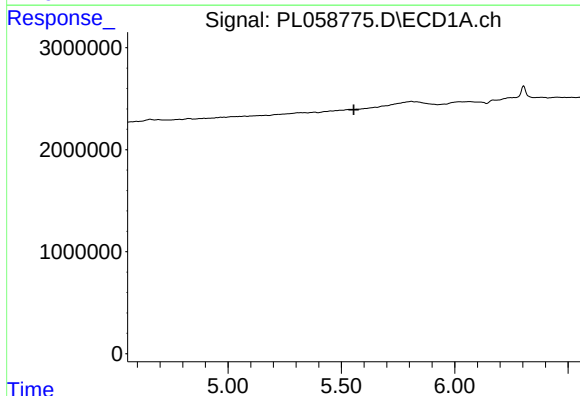


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.555 min
Response: 0
Conc: N.D.

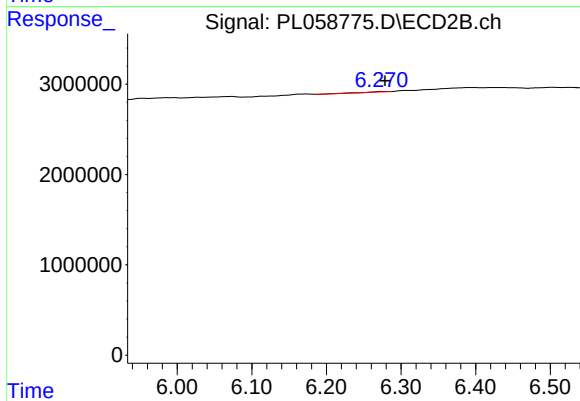

#26 Chlordane-4


R.T.: 6.274 min
Delta R.T.: -0.005 min
Response: 66731
Conc: 0.18 ng/ml

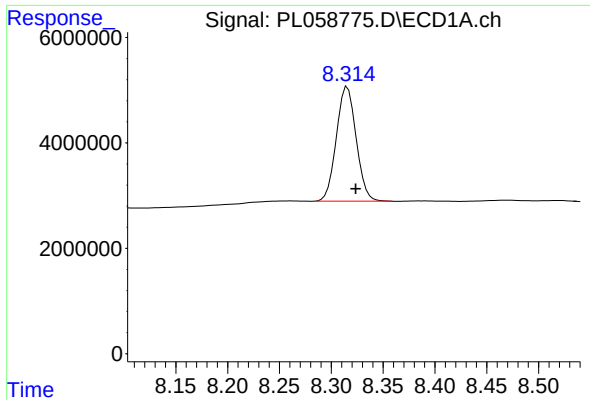

#28 Decachlorobiphenyl

R.T.: 8.316 min
Delta R.T.: -0.008 min
Response: 28906950
Conc: 22.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

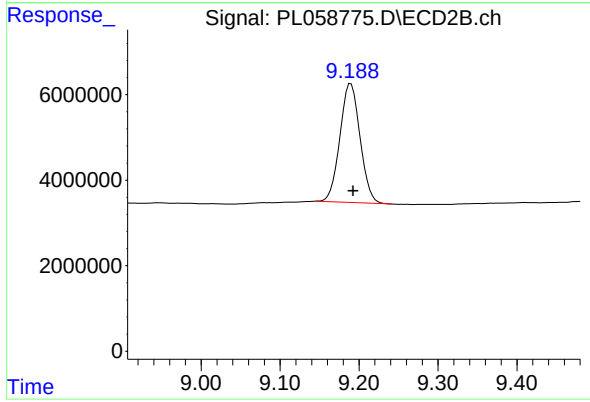

#28 Decachlorobiphenyl

R.T.: 9.190 min
Delta R.T.: -0.003 min
Response: 49225967
Conc: 27.85 ng/ml