

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051822\
 Data File : PL074775.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2022 10:19
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 03:10:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
4) MA	Heptachlor	7.310f	6.167f	444831	314972	0.689 0.208 #
5) MB	Aldrin	0.000	6.533f	0	80254	N.D. 0.053 #
6) B	beta-BHC	0.000	6.167	0	314972	N.D. 0.397 #
8) B	Heptachlo...	8.128	0.000	19389524	0	34.092 N.D. #
9) A	Endosulfan I	0.000	7.517f	0	399088	N.D. 0.319 #
10) B	gamma-Chl...	0.000	7.359	0	1154216	N.D. 0.833 #
11) B	alpha-Chl...	8.501f	7.421	2302243	2421767	3.771 1.791 #
14) MA	Endrin	0.000	8.082f	0	11236995	N.D. 10.638 #
24)	Chlordane-2	0.000	6.642f	0	2558274	N.D. 46.074 #
25)	Chlordane-3	0.000	7.359	0	1154216	N.D. 8.893 #
26)	Chlordane-4	8.501f	7.421	2302243	2421767	23.897 17.666 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051822\
Data File : PL074775.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2022 10:19
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 03:10:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

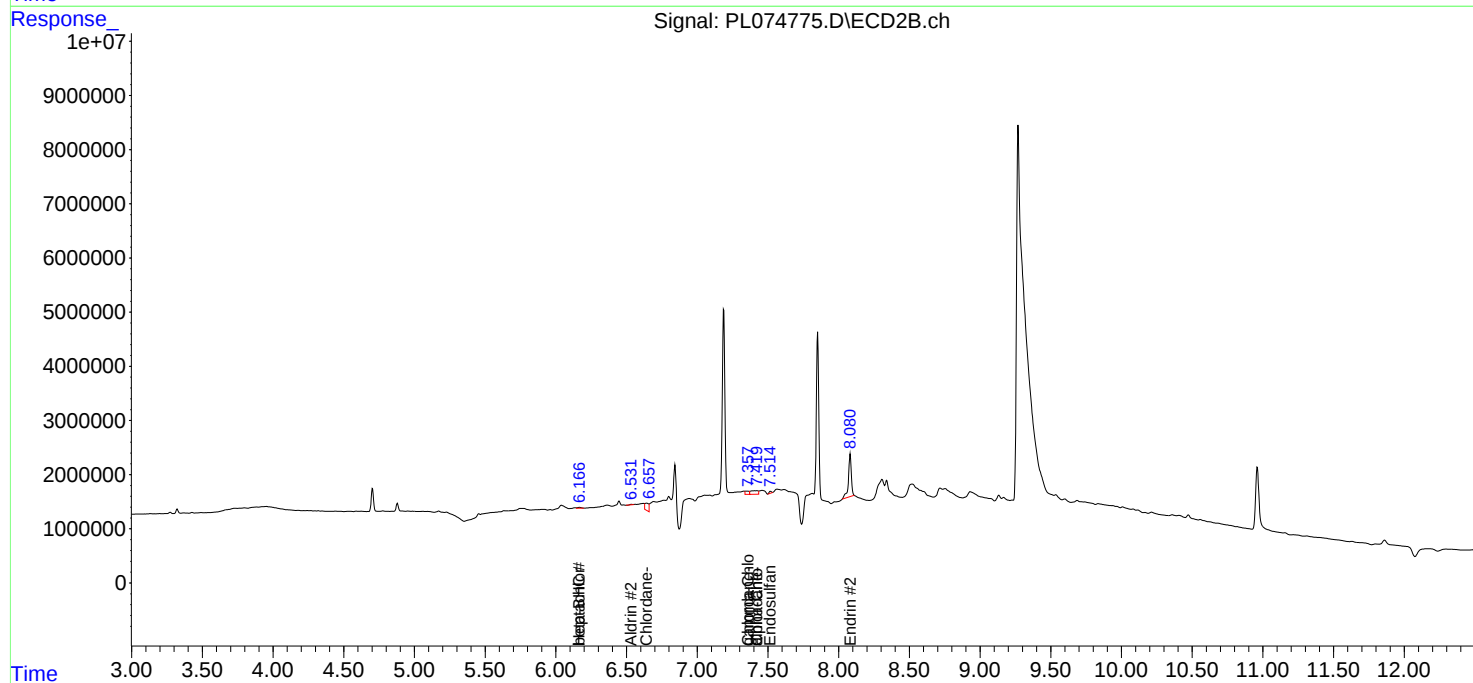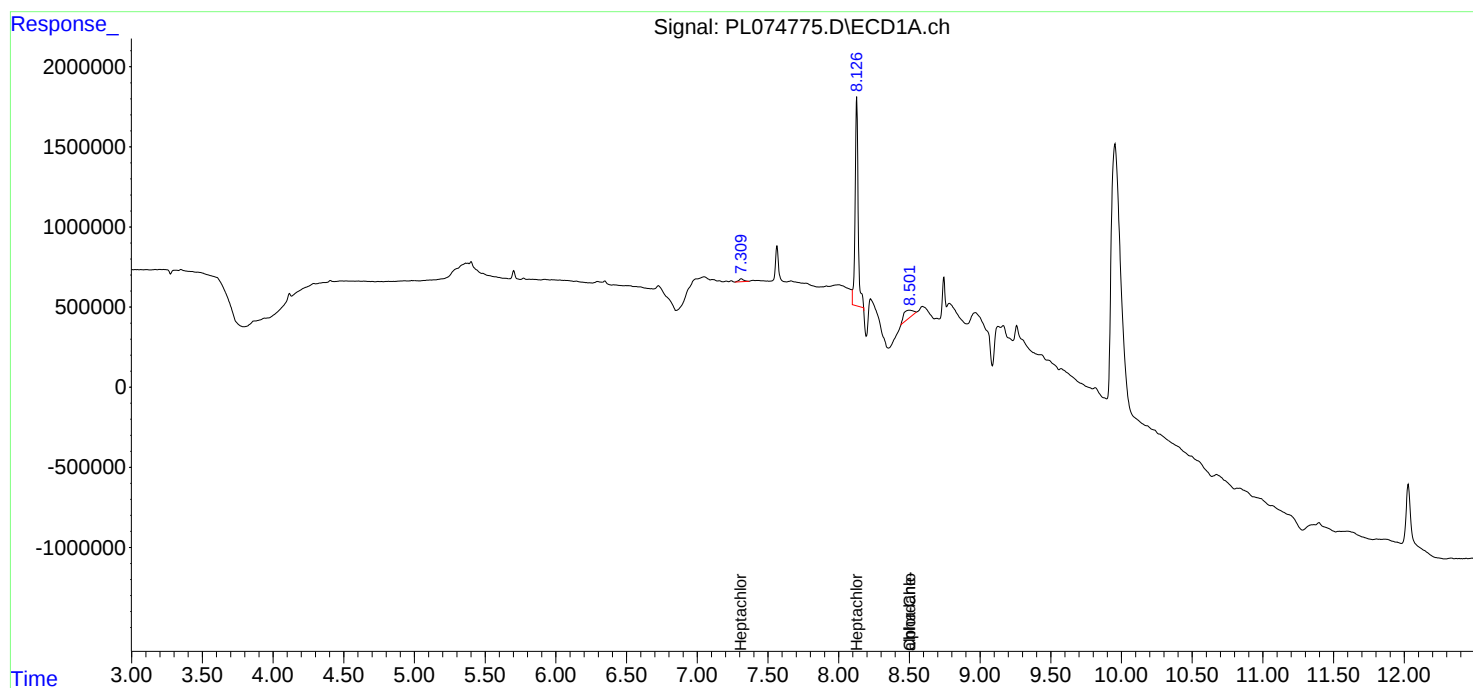


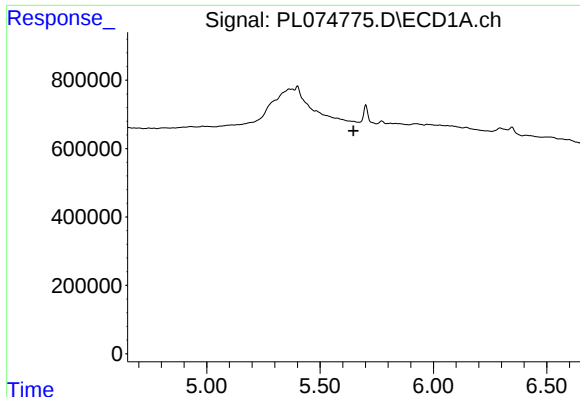

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 5.648 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

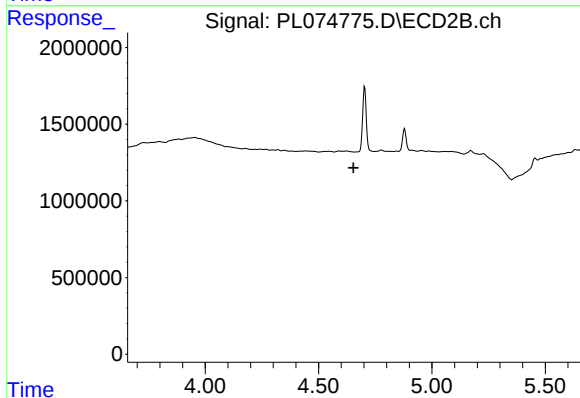


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.654 min
Response: 0
Conc: N.D.

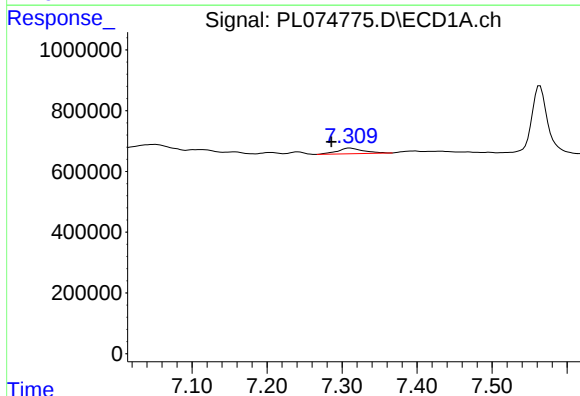


#4 Heptachlor

R.T.: 7.310 min
Delta R.T.: 0.025 min
Response: 444831
Conc: 0.69 ng/ml

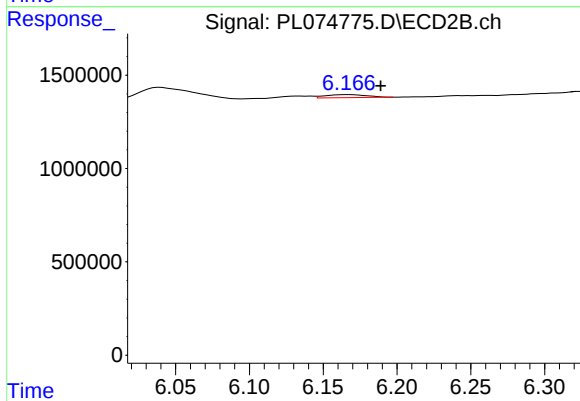

#4 Heptachlor


R.T.: 6.167 min
Delta R.T.: -0.022 min
Response: 314972
Conc: 0.21 ng/ml

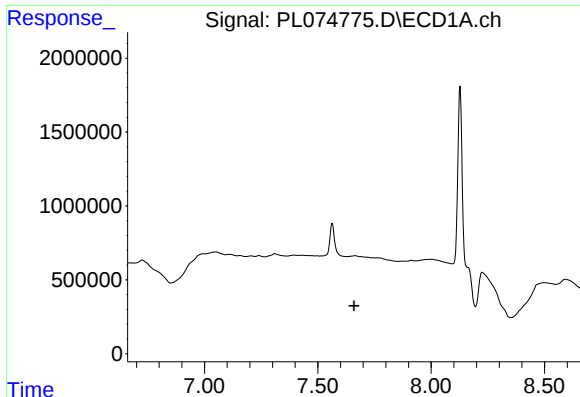

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 7.660 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

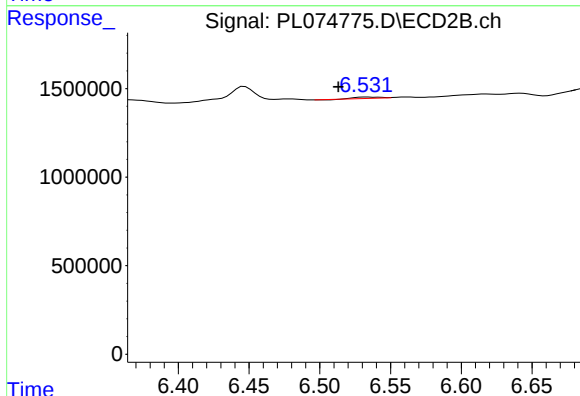


#5 Aldrin

R.T.: 6.533 min
Delta R.T.: 0.020 min
Response: 80254
Conc: 0.05 ng/ml

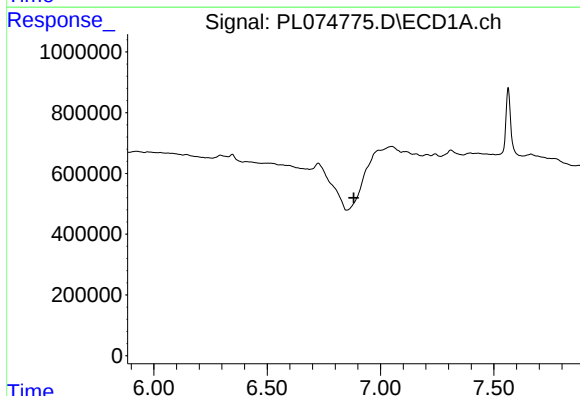


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 6.882 min
Response: 0
Conc: N.D.

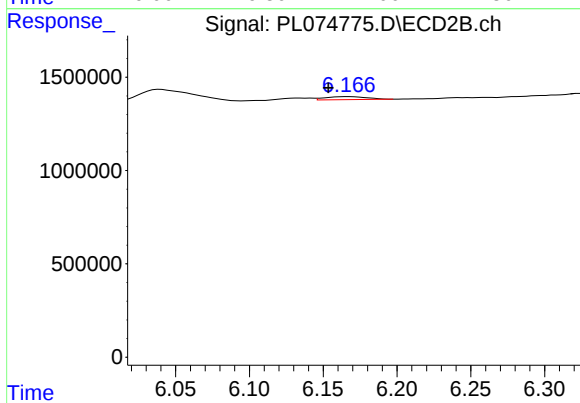

#6 beta-BHC


R.T.: 6.167 min
Delta R.T.: 0.014 min
Response: 314972
Conc: 0.40 ng/ml

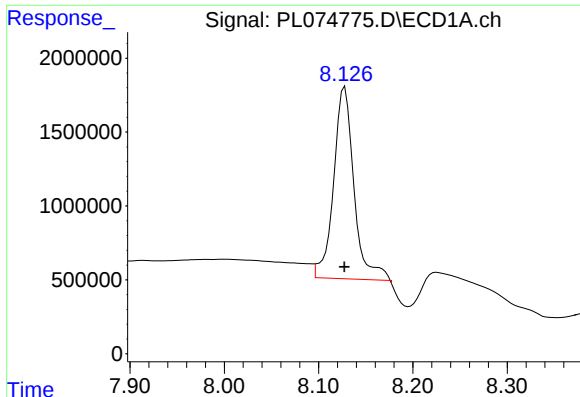

#8 Heptachlor epoxide


R.T.: 8.128 min
Delta R.T.: 0.000 min
Response: 19389524
Conc: 34.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

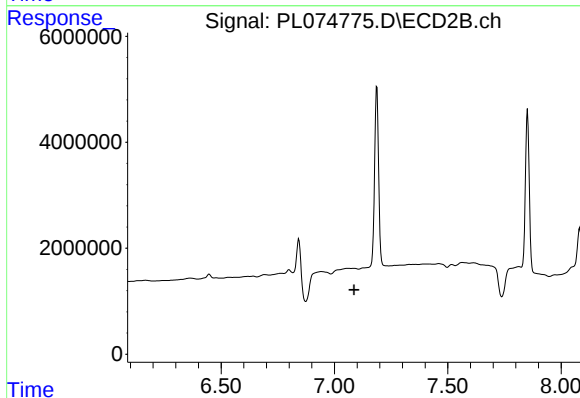


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.087 min
Response: 0
Conc: N.D.

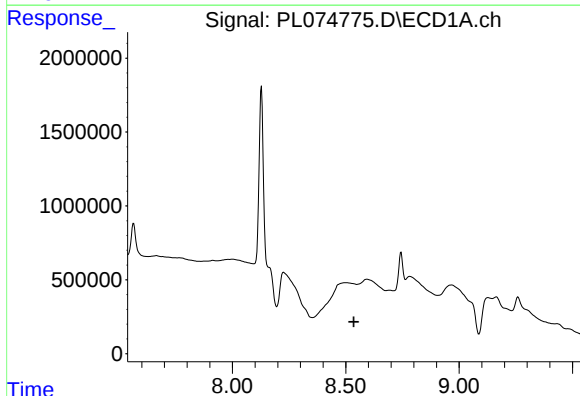


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 8.536 min
Response: 0
Conc: N.D.

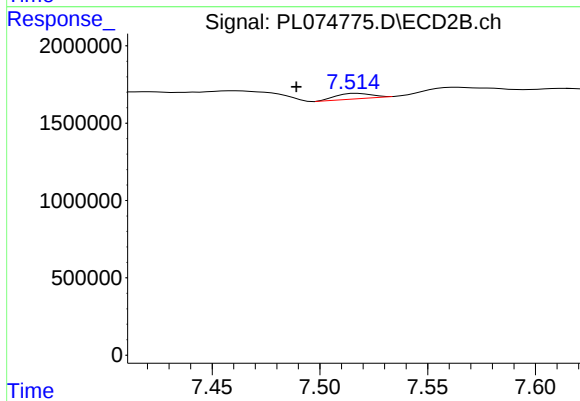

#9 Endosulfan I


R.T.: 7.517 min
Delta R.T.: 0.028 min
Response: 399088
Conc: 0.32 ng/ml

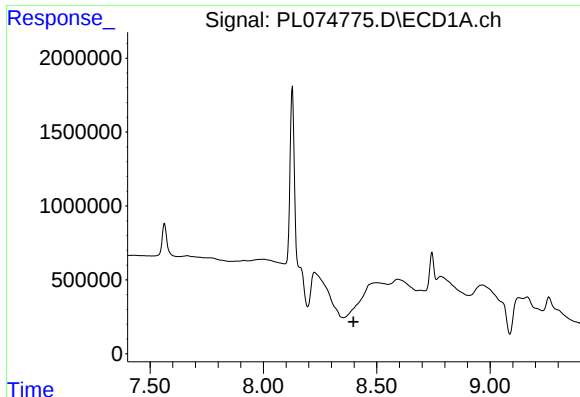

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

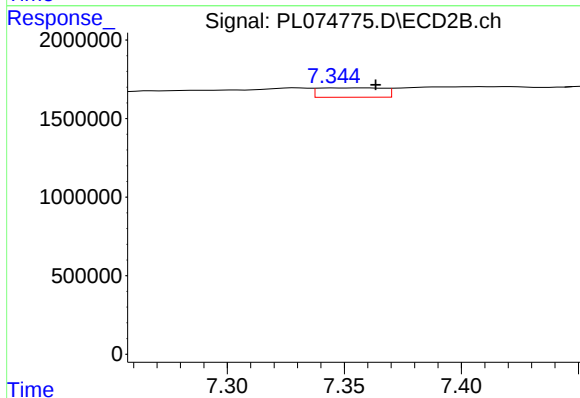


#10 gamma-Chlordane

R.T.: 7.359 min
Delta R.T.: -0.005 min
Response: 1154216
Conc: 0.83 ng/ml

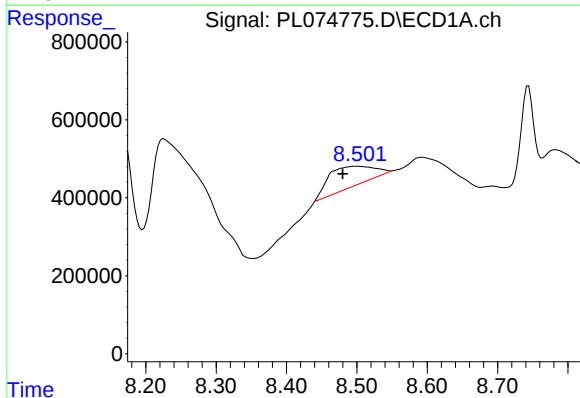


#11 alpha-Chlordane

R.T.: 8.501 min
Delta R.T.: 0.021 min
Response: 2302243
Conc: 3.77 ng/ml

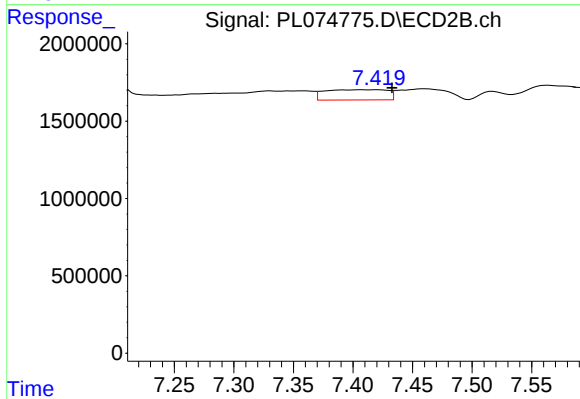

#11 alpha-Chlordane


R.T.: 7.421 min
Delta R.T.: -0.012 min
Response: 2421767
Conc: 1.79 ng/ml

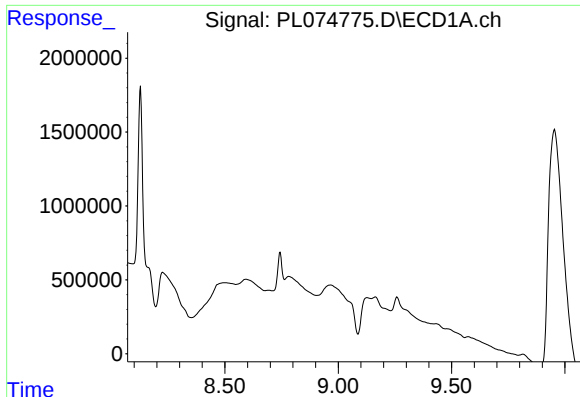

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

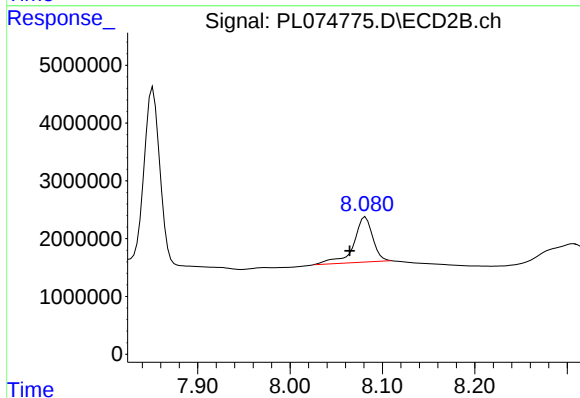


#14 Endrin

R.T.: 8.082 min
Delta R.T.: 0.017 min
Response: 11236995
Conc: 10.64 ng/ml

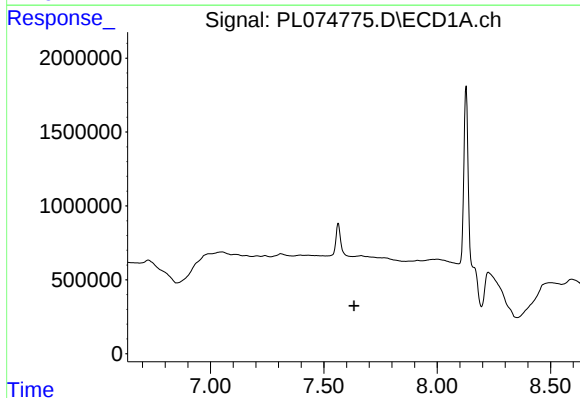


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 7.634 min
Response: 0
Conc: N.D.

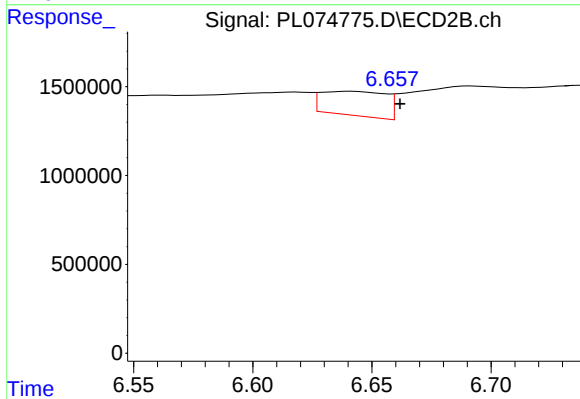

#24 Chlordane-2


R.T.: 6.642 min
Delta R.T.: -0.020 min
Response: 2558274
Conc: 46.07 ng/ml

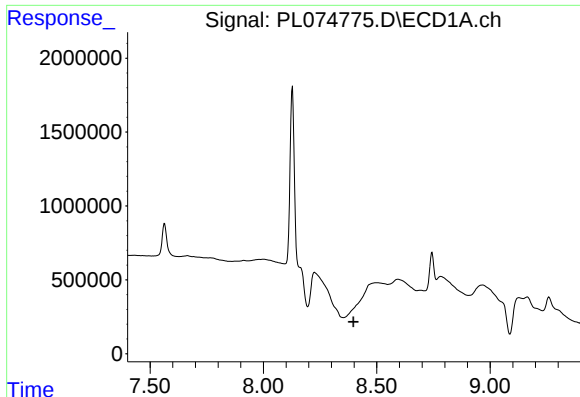

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

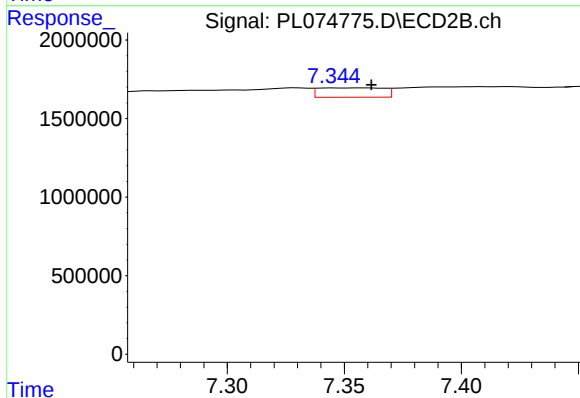


#25 Chlordane-3

R.T.: 7.359 min
Delta R.T.: -0.003 min
Response: 1154216
Conc: 8.89 ng/ml

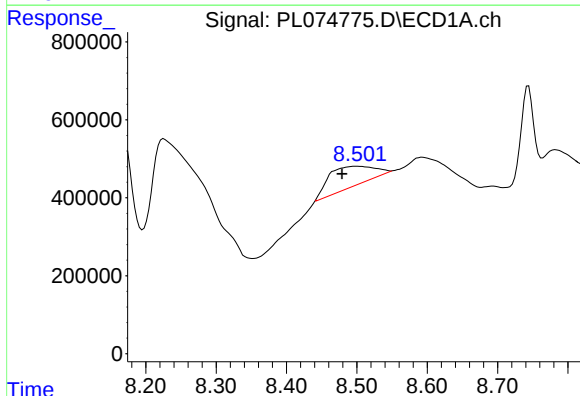


#26 Chlordane-4

R.T.: 8.501 min
Delta R.T.: 0.022 min
Response: 2302243
Conc: 23.90 ng/ml

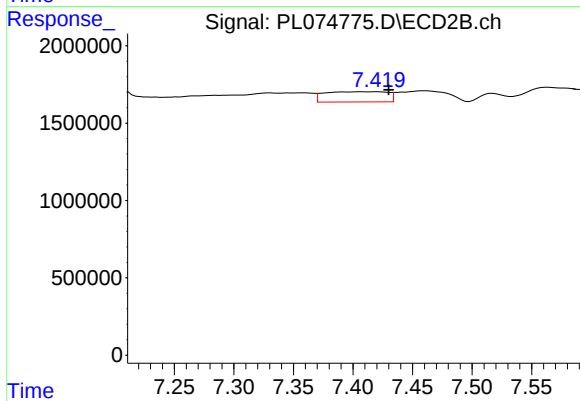

#26 Chlordane-4


R.T.: 7.421 min
Delta R.T.: -0.009 min
Response: 2421767
Conc: 17.67 ng/ml

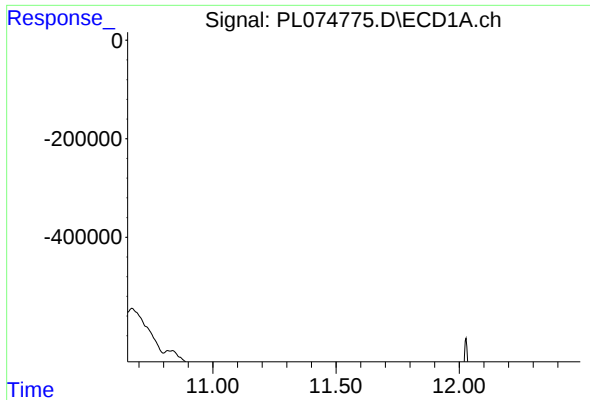

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.651 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

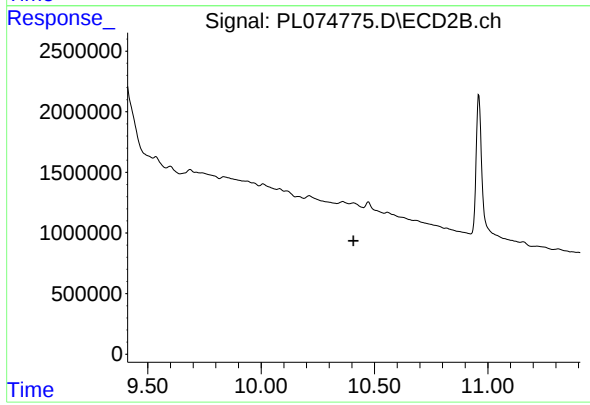

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.408 min
Response: 0
Conc: N.D.