

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051822\
 Data File : PL074789.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2022 16:01
 Operator : AR\AJ
 Sample : N2881-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 03:13:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.645	4.650	10997339	28825723	21.659	21.002
28)	SA Decachlor...	11.645	10.402	9301875	23117924	20.829	22.523
Target Compounds							
5)	MB Aldrin	0.000	6.503	0	388340	N.D.	0.259 #
6)	B beta-BHC	0.000	6.124f	0	3168239	N.D.	3.990 #
7)	B delta-BHC	7.128f	0.000	355734	0	0.567	N.D. #
8)	B Heptachlo...	0.000	7.083	0	286860	N.D.	0.206 #
9)	A Endosulfan I	8.520f	0.000	2550995	0	4.425	N.D. #
11)	B alpha-Chl...	8.502f	0.000	2580477	0	4.227	N.D. #
14)	MA Endrin	0.000	8.082f	0	62219	N.D.	0.059 #
21)	B Endrin ke...	0.000	9.339f	0	342213	N.D.	0.307 #
26)	Chlordane-4	8.502f	0.000	2580477	0	26.785	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051822\
Data File : PL074789.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2022 16:01
Operator : AR\AJ
Sample : N2881-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 03:13:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

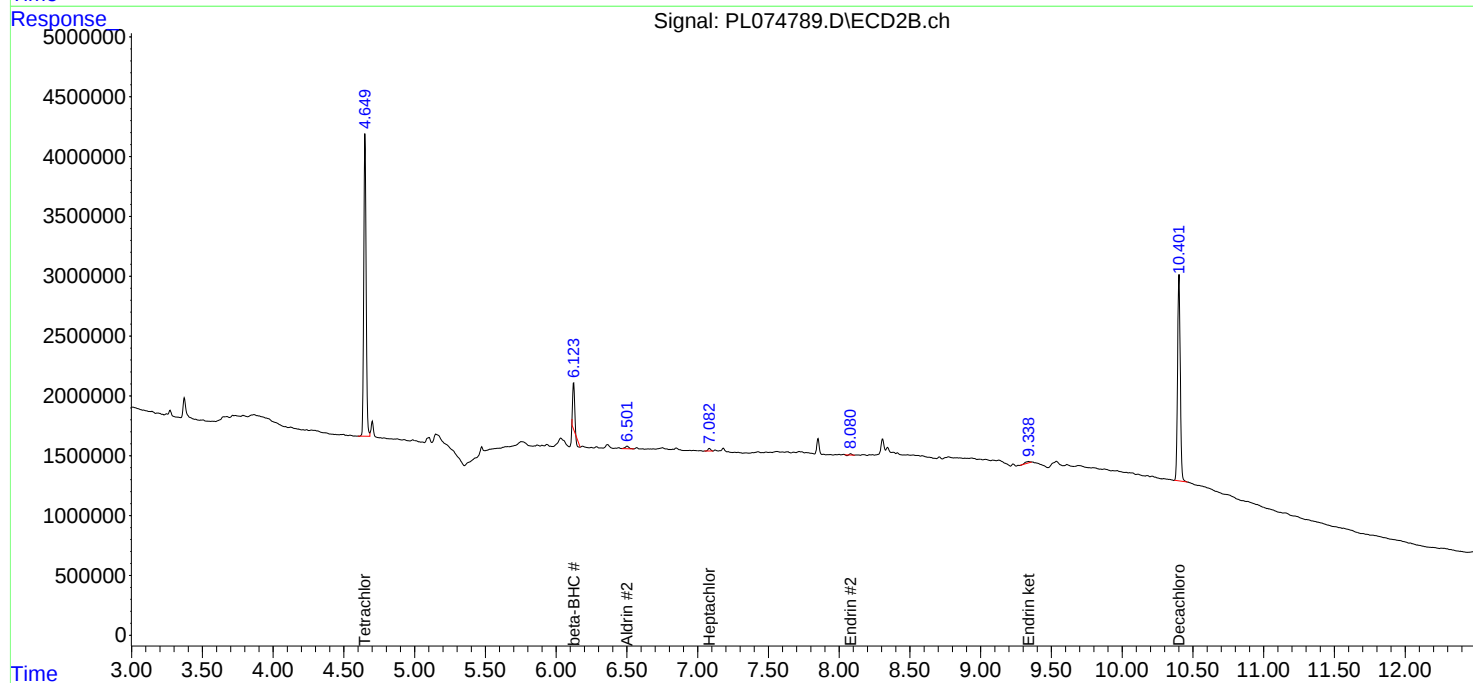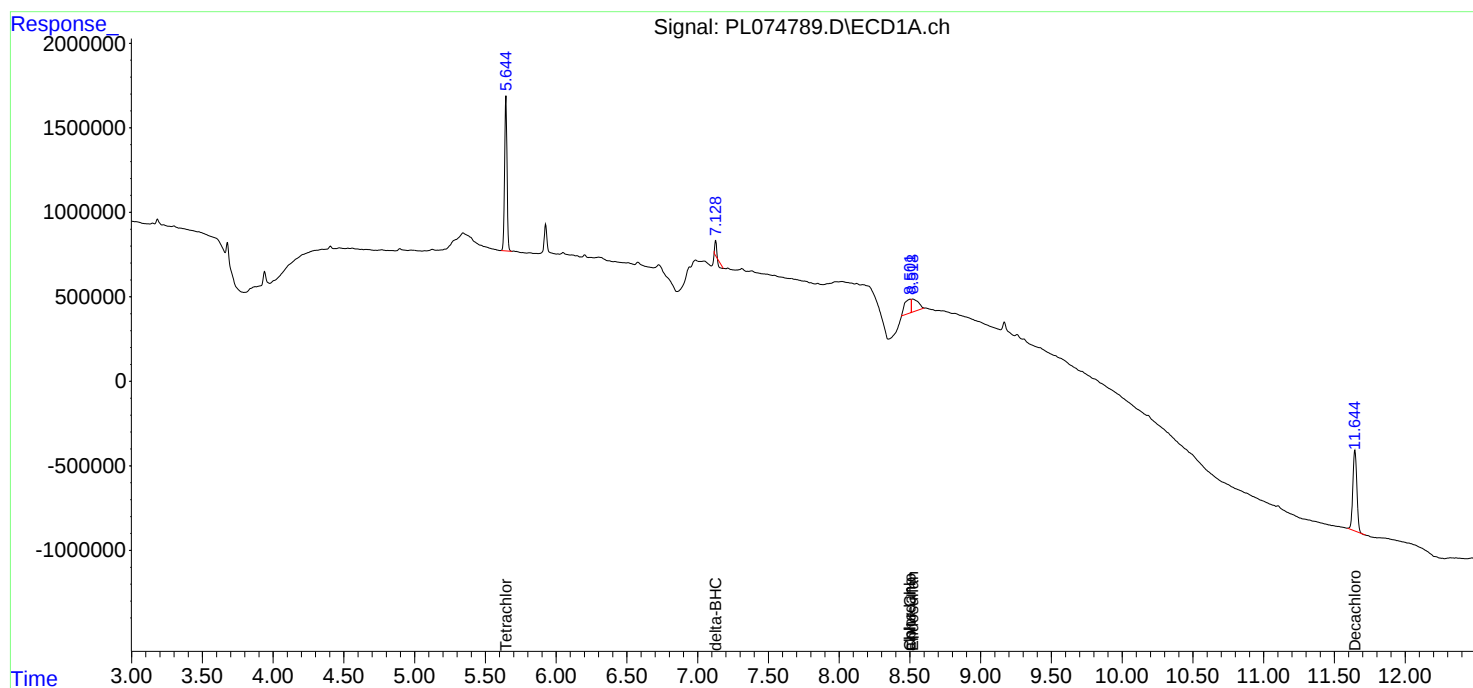


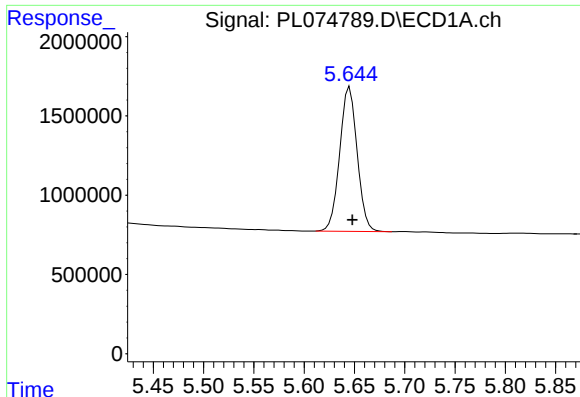

#1 Tetrachloro-m-xylene


R.T.: 5.645 min
Delta R.T.: -0.003 min
Response: 10997339
Conc: 21.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

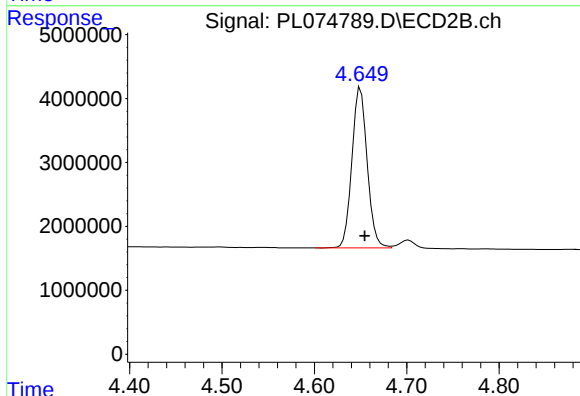


#1 Tetrachloro-m-xylene

R.T.: 4.650 min
Delta R.T.: -0.004 min
Response: 28825723
Conc: 21.00 ng/ml

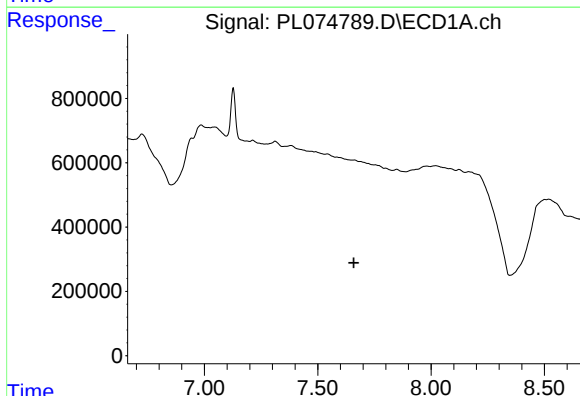


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.660 min
Response: 0
Conc: N.D.

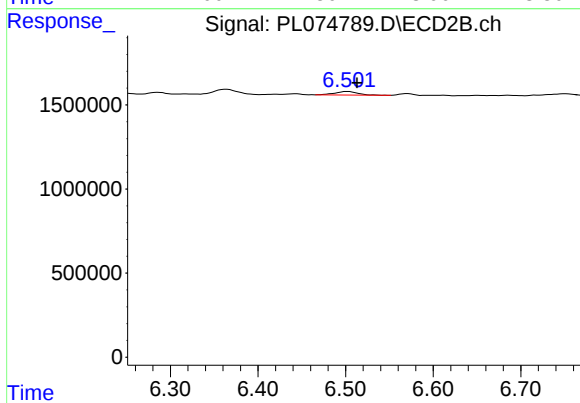

#5 Aldrin


R.T.: 6.503 min
Delta R.T.: -0.011 min
Response: 388340
Conc: 0.26 ng/ml

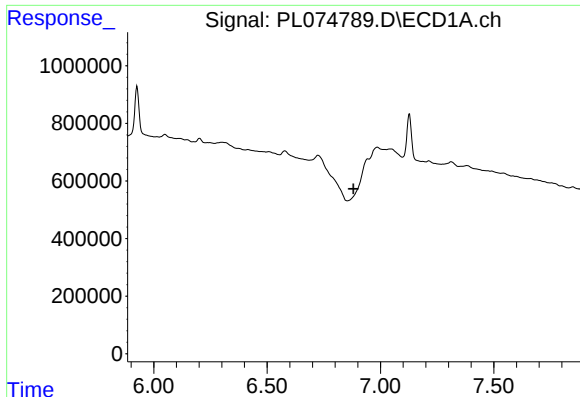

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.882 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

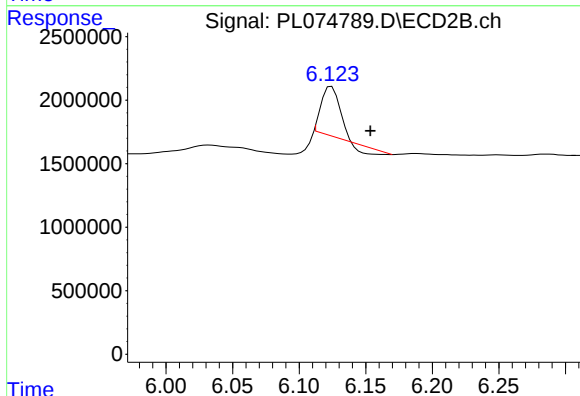


#6 beta-BHC

R.T.: 6.124 min
Delta R.T.: -0.029 min
Response: 3168239
Conc: 3.99 ng/ml

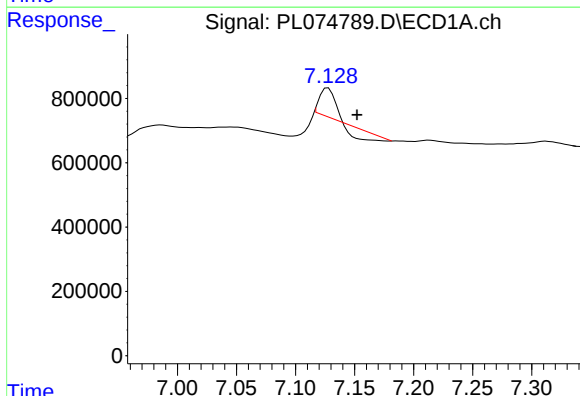


#7 delta-BHC

R.T.: 7.128 min
Delta R.T.: -0.025 min
Response: 355734
Conc: 0.57 ng/ml

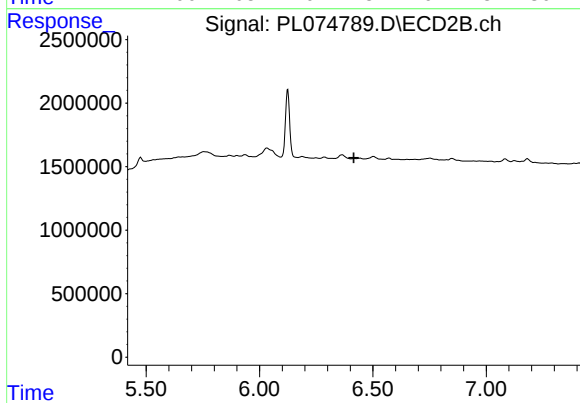

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.415 min
Response: 0
Conc: N.D.

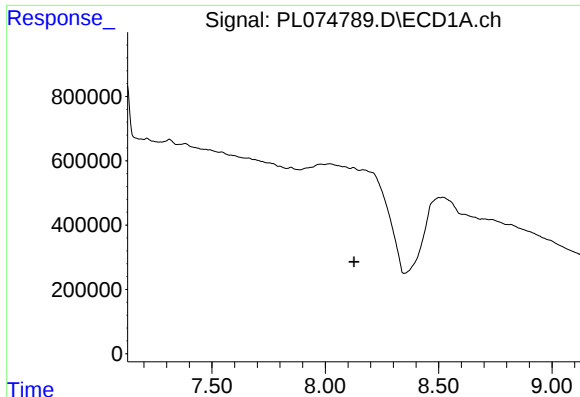

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 8.127 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

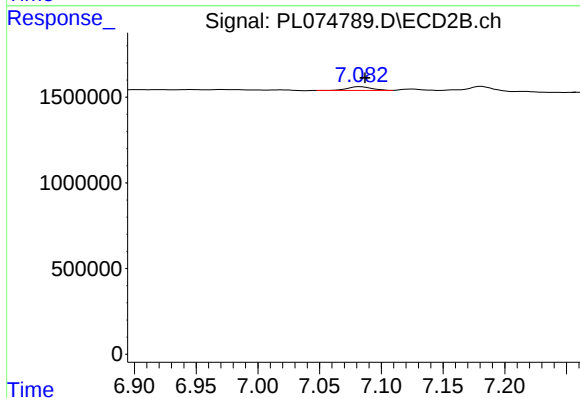


#8 Heptachlor epoxide

R.T.: 7.083 min
Delta R.T.: -0.004 min
Response: 286860
Conc: 0.21 ng/ml

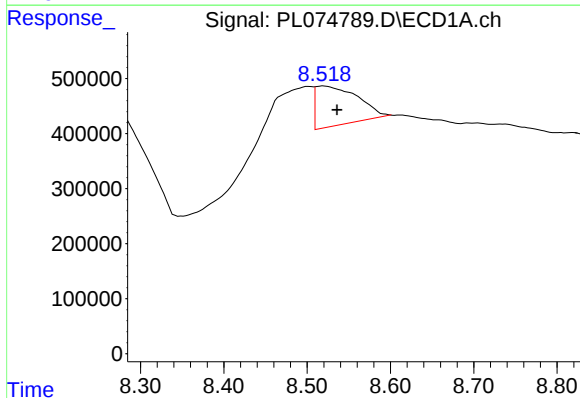


#9 Endosulfan I

R.T.: 8.520 min
Delta R.T.: -0.016 min
Response: 2550995
Conc: 4.42 ng/ml

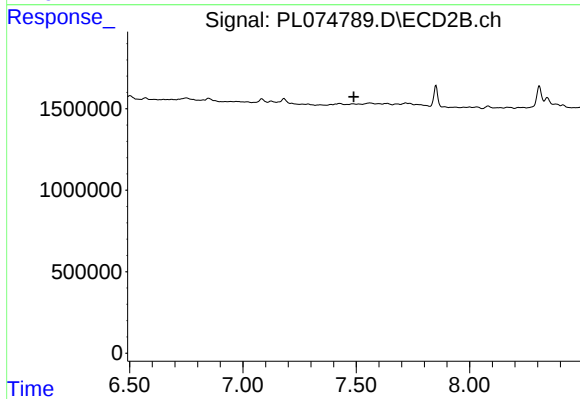

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.489 min
Response: 0
Conc: N.D.

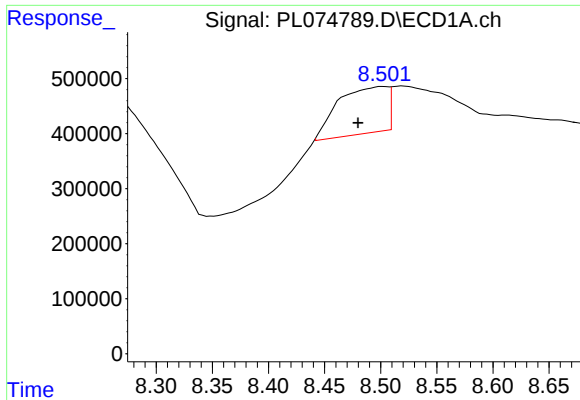

#11 alpha-Chlordane


R.T.: 8.502 min
Delta R.T.: 0.022 min
Response: 2580477
Conc: 4.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

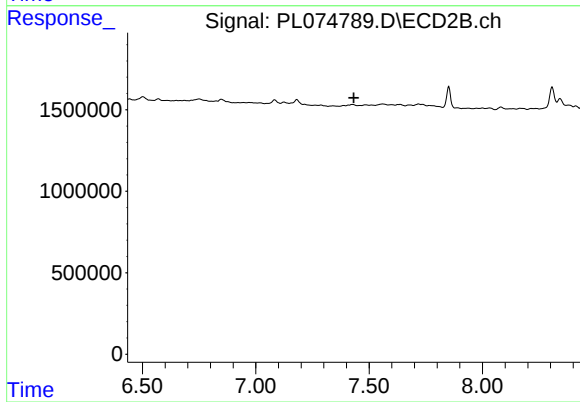


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.433 min
Response: 0
Conc: N.D.

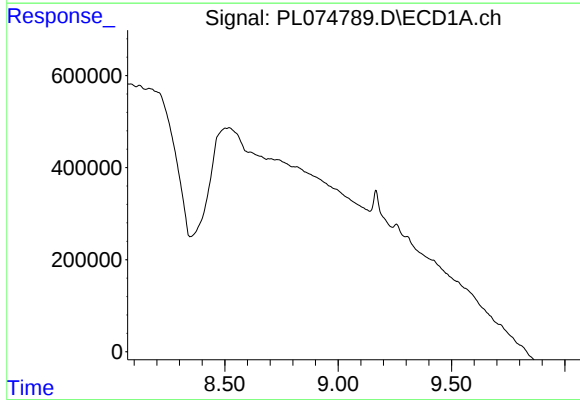


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.068 min
Response: 0
Conc: N.D.

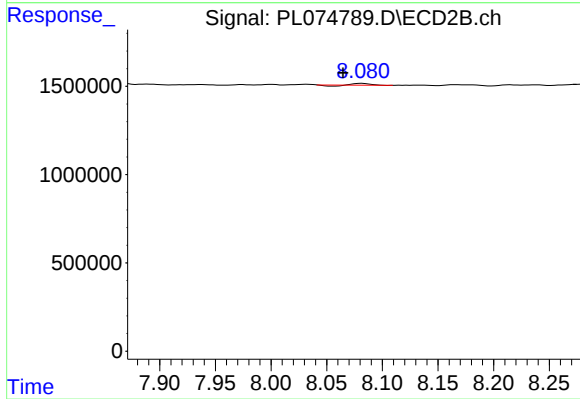

#14 Endrin


R.T.: 8.082 min
Delta R.T.: 0.017 min
Response: 62219
Conc: 0.06 ng/ml

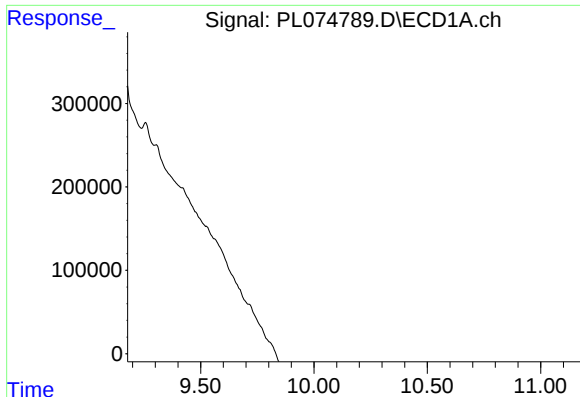

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 10.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

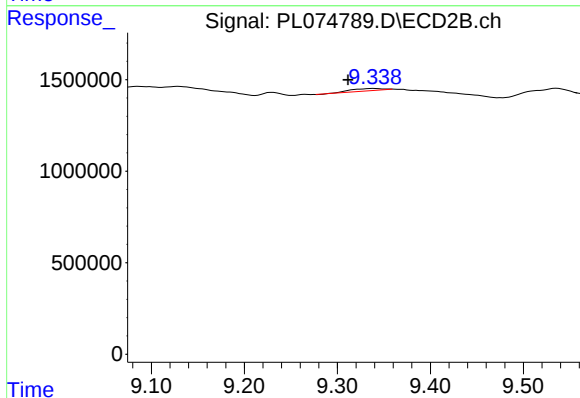


#21 Endrin ketone

R.T.: 9.339 min
Delta R.T.: 0.028 min
Response: 342213
Conc: 0.31 ng/ml

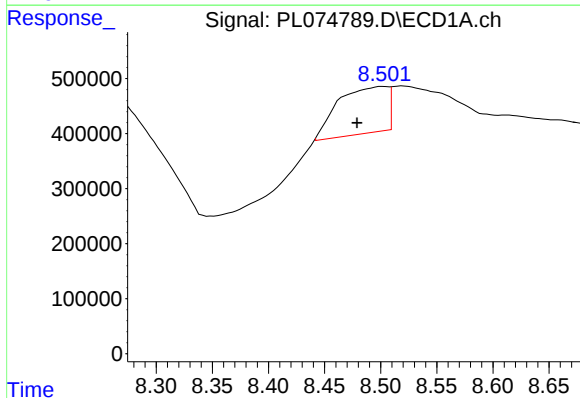


#26 Chlordane-4

R.T.: 8.502 min
Delta R.T.: 0.023 min
Response: 2580477
Conc: 26.79 ng/ml

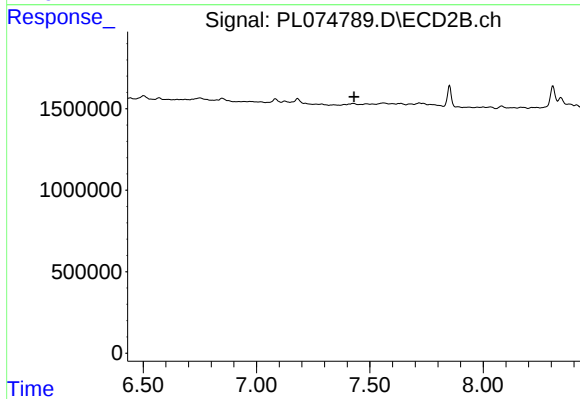

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

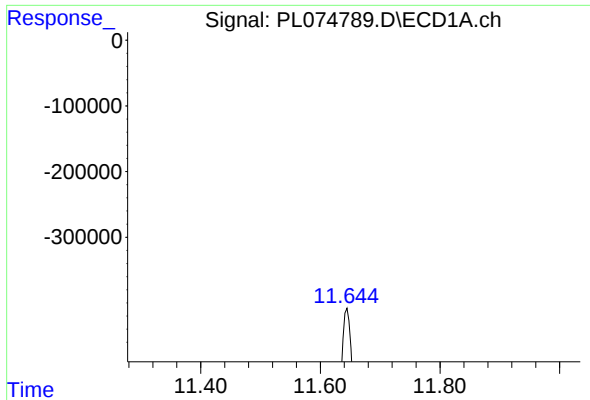

#28 Decachlorobiphenyl

R.T.: 11.645 min
Delta R.T.: -0.006 min
Response: 9301875
Conc: 20.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

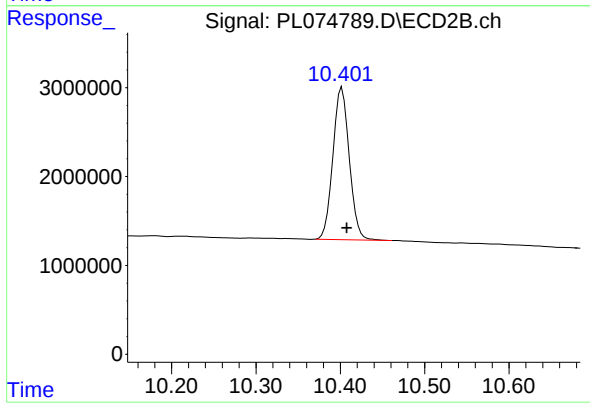

#28 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: -0.006 min
Response: 23117924
Conc: 22.52 ng/ml