

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051822\
 Data File : PL074791.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2022 16:34
 Operator : AR\AJ
 Sample : N2863-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 03:13:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.646	4.650	10270625	28092625	20.228	20.468
28)	SA Decachlor...	11.646	10.402	6826578	17739979	15.286	17.283
Target Compounds							
6)	B beta-BHC	0.000	6.124f	0	589473	N.D.	0.742 #
9)	A Endosulfan I	8.522	0.000	5304727	0	9.202	N.D. #
13)	MA Dieldrin	0.000	7.777	0	233382	N.D.	0.183 #
14)	MA Endrin	0.000	8.077	0	896970	N.D.	0.849 #
16)	A 4,4'-DDD	9.206	0.000	564194	0	1.248	N.D. #
17)	MA 4,4'-DDT	0.000	8.476	0	4119029	N.D.	4.117 #
19)	B Endosulfa...	0.000	8.789	0	3646592	N.D.	3.350 #
21)	B Endrin ke...	0.000	9.340f	0	3320283	N.D.	2.978 #
27)	Chlordane-5	0.000	8.140	0	1456834	N.D.	39.402 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051822\
Data File : PL074791.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2022 16:34
Operator : AR\AJ
Sample : N2863-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 03:13:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

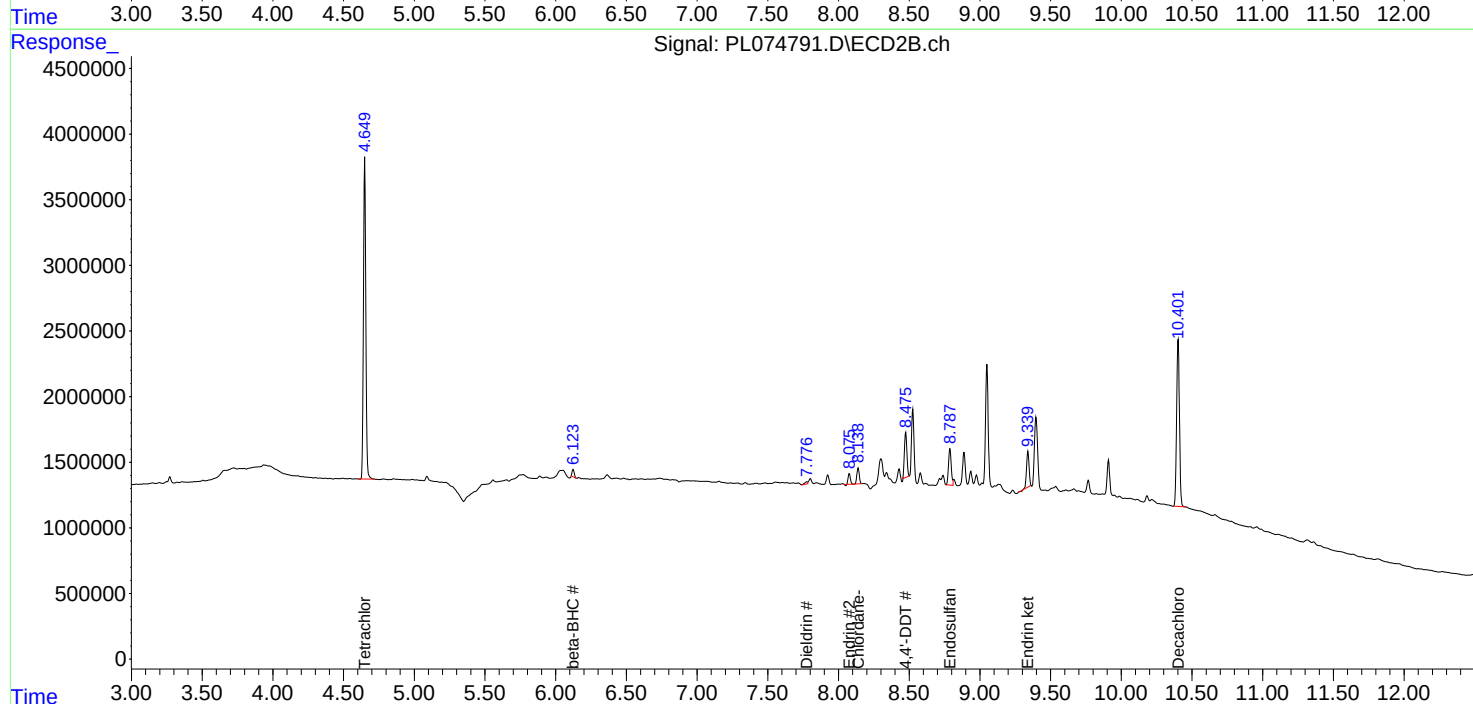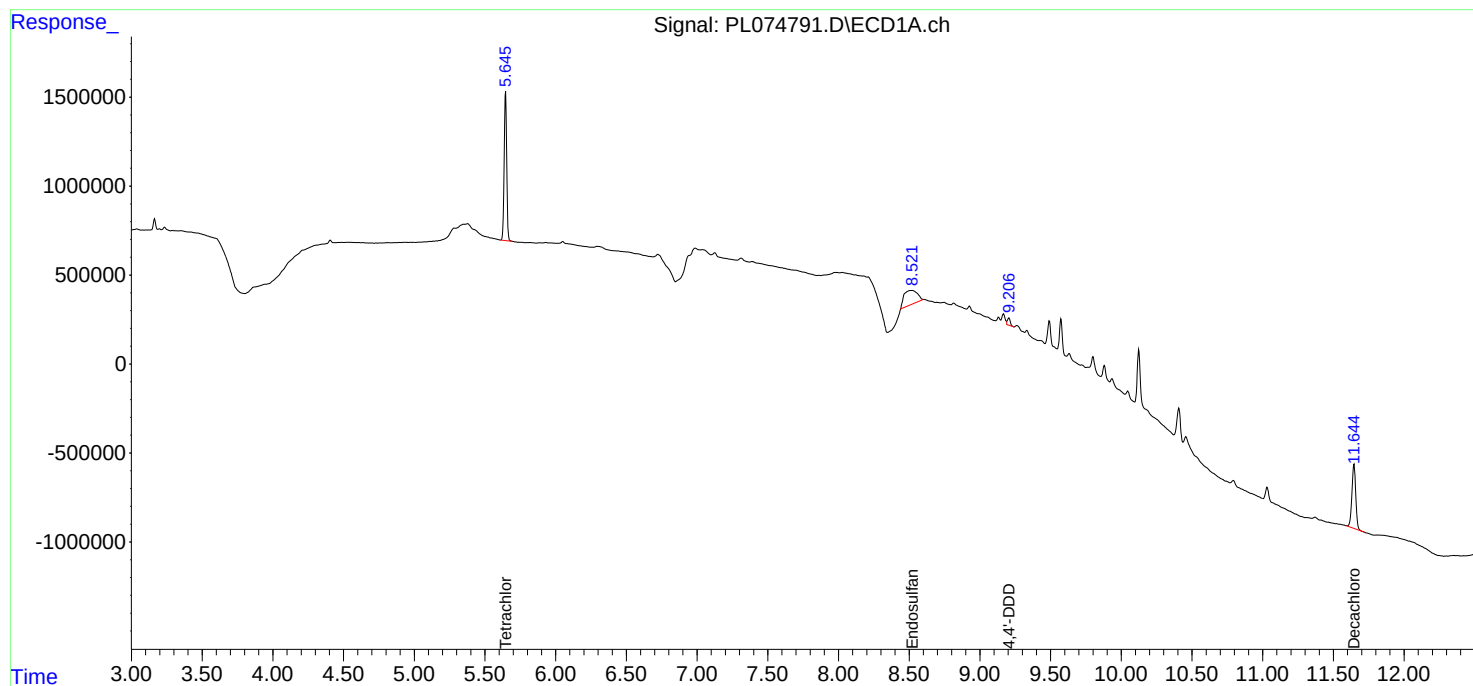


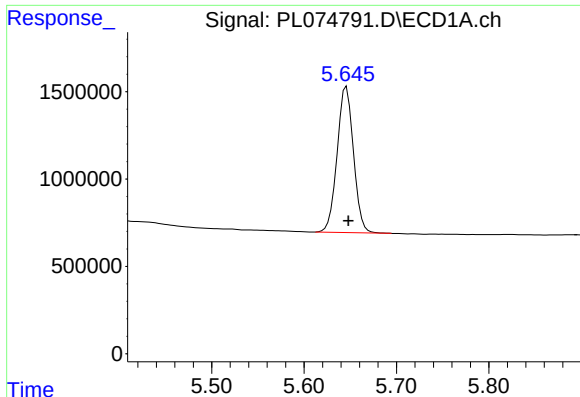

#1 Tetrachloro-m-xylene


R.T.: 5.646 min
Delta R.T.: -0.002 min
Response: 10270625
Conc: 20.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

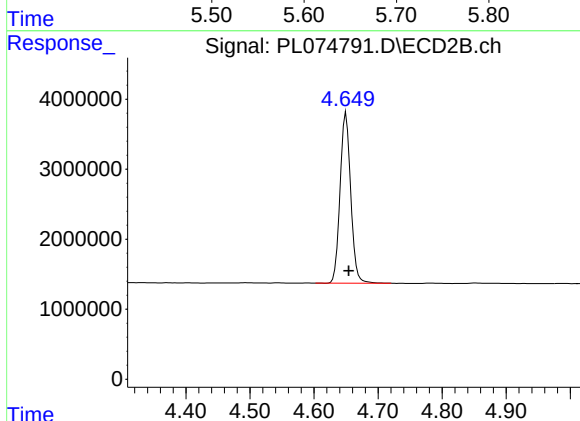


#1 Tetrachloro-m-xylene

R.T.: 4.650 min
Delta R.T.: -0.004 min
Response: 28092625
Conc: 20.47 ng/ml

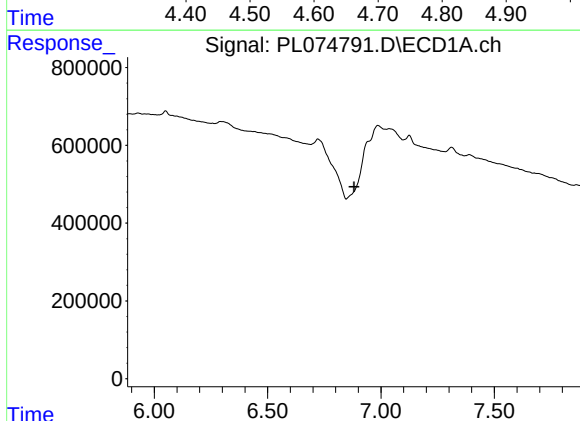


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.882 min
Response: 0
Conc: N.D.

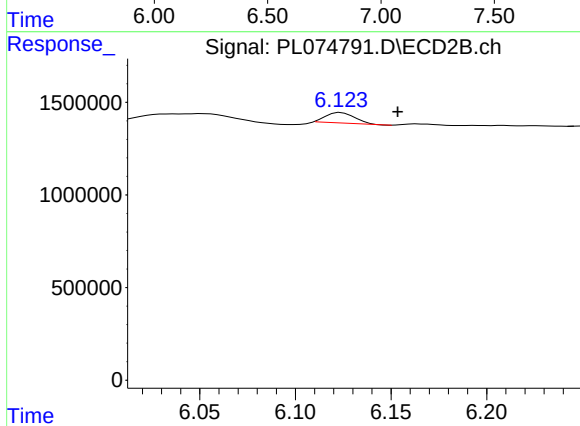

#6 beta-BHC


R.T.: 6.124 min
Delta R.T.: -0.029 min
Response: 589473
Conc: 0.74 ng/ml

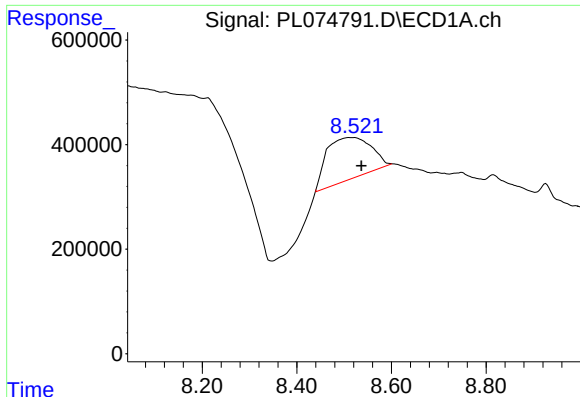

#9 Endosulfan I


R.T.: 8.522 min
Delta R.T.: -0.014 min
Response: 5304727
Conc: 9.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

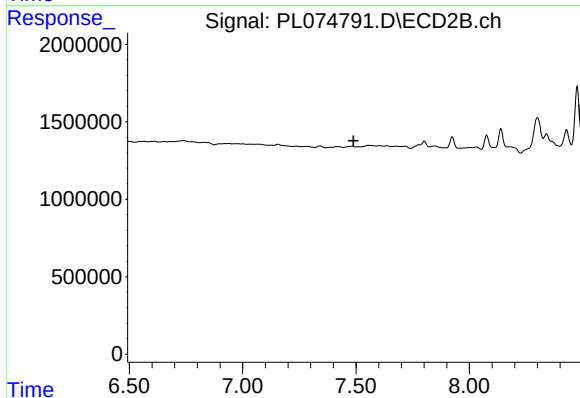


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.489 min
Response: 0
Conc: N.D.

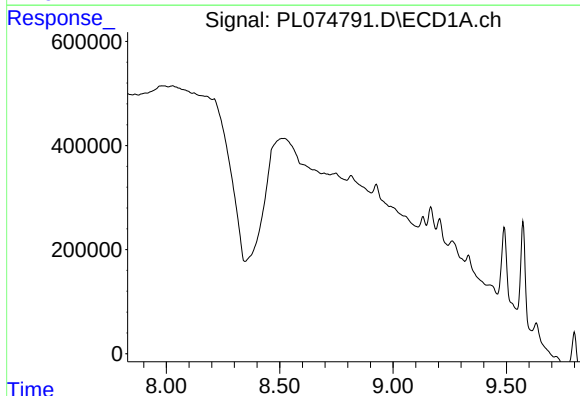


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.827 min
Response: 0
Conc: N.D.

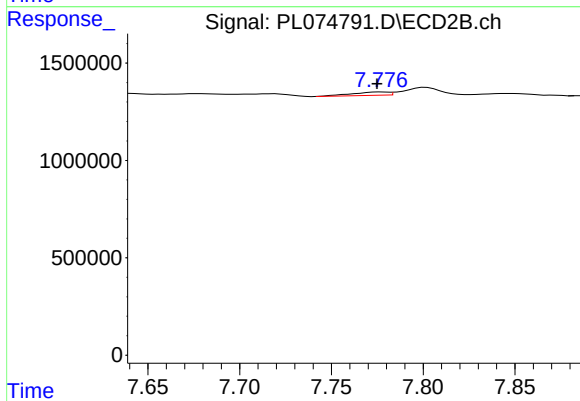

#13 Dieldrin


R.T.: 7.777 min
Delta R.T.: 0.002 min
Response: 233382
Conc: 0.18 ng/ml

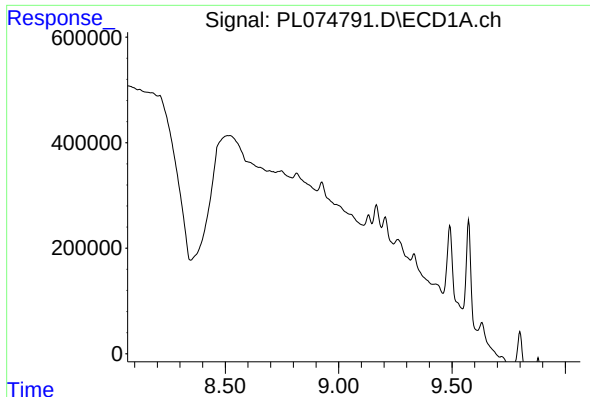

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

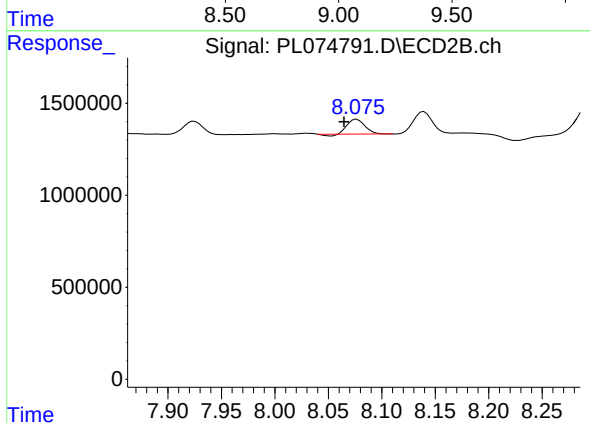


#14 Endrin

R.T.: 8.077 min
Delta R.T.: 0.012 min
Response: 896970
Conc: 0.85 ng/ml

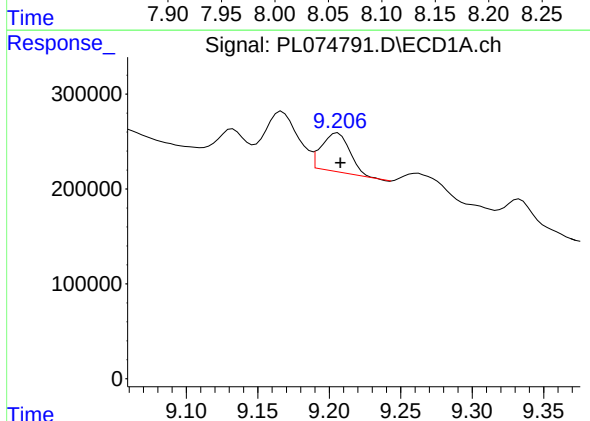


#16 4,4'-DDD

R.T.: 9.206 min
Delta R.T.: -0.002 min
Response: 564194
Conc: 1.25 ng/ml

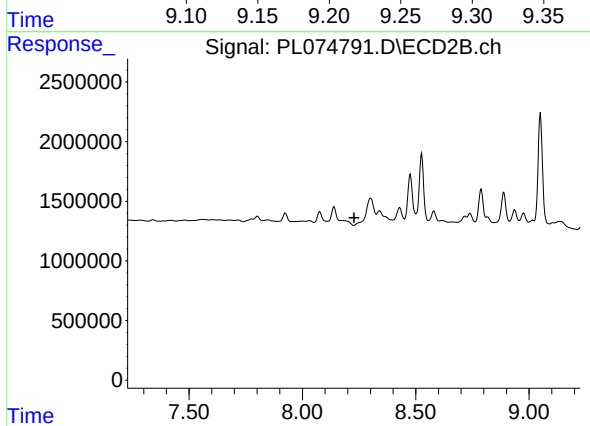

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.229 min
Response: 0
Conc: N.D.

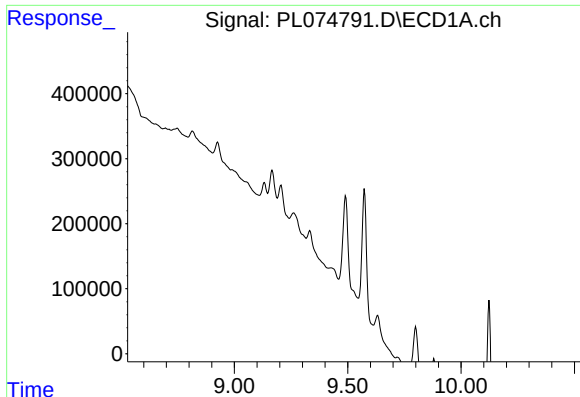

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.527 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

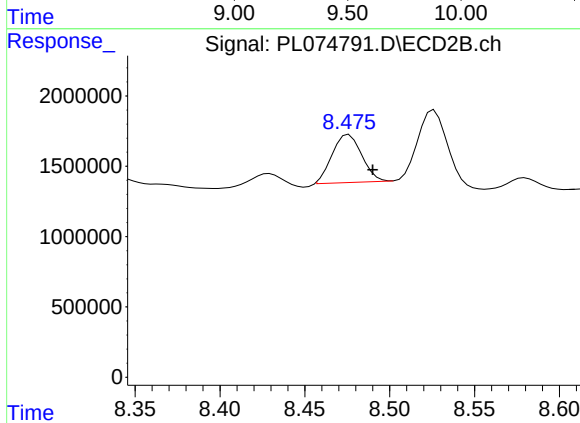


#17 4,4'-DDT

R.T.: 8.476 min
Delta R.T.: -0.014 min
Response: 4119029
Conc: 4.12 ng/ml

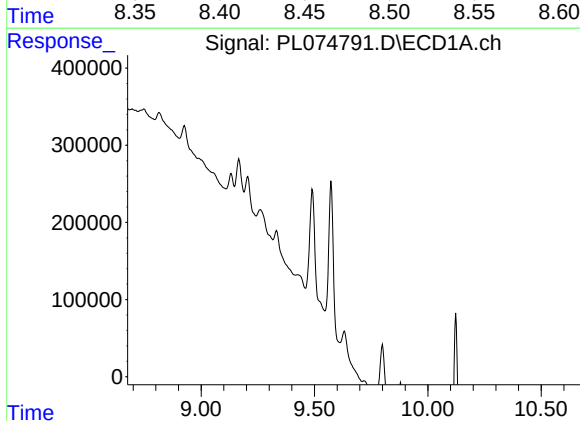


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 9.675 min
Response: 0
Conc: N.D.

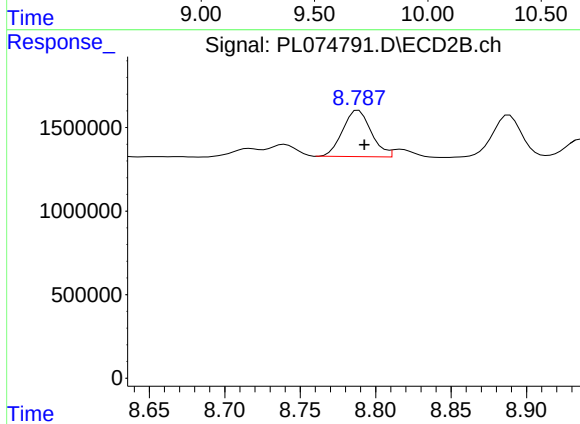

#19 Endosulfan Sulfate


R.T.: 8.789 min
Delta R.T.: -0.004 min
Response: 3646592
Conc: 3.35 ng/ml

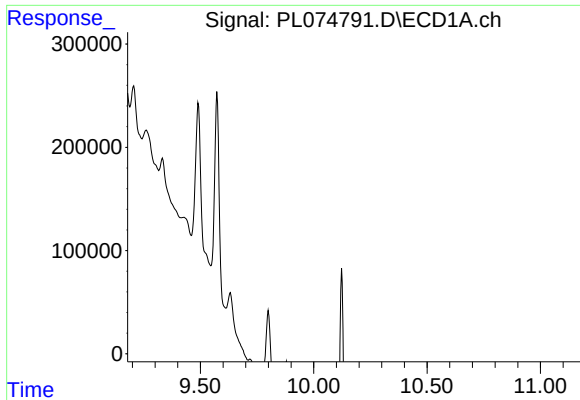

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 10.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

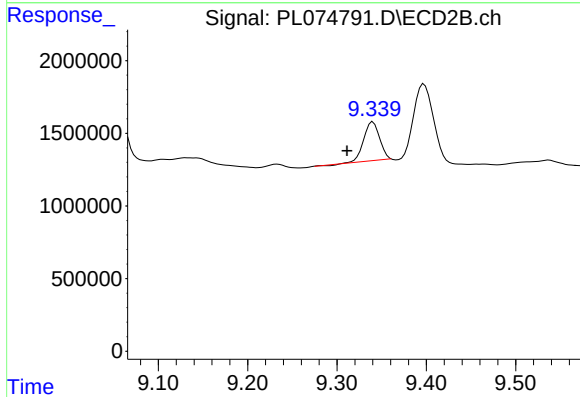


#21 Endrin ketone

R.T.: 9.340 min
Delta R.T.: 0.029 min
Response: 3320283
Conc: 2.98 ng/ml

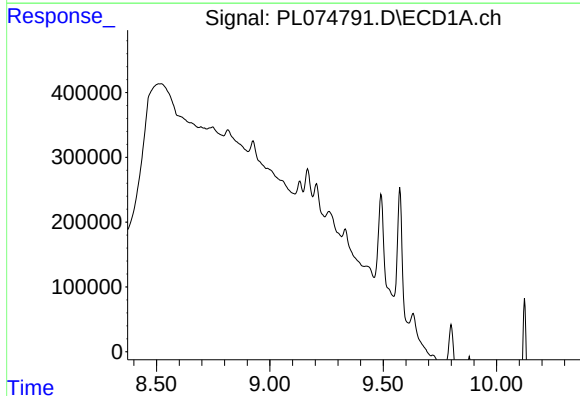


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 9.371 min
Response: 0
Conc: N.D.

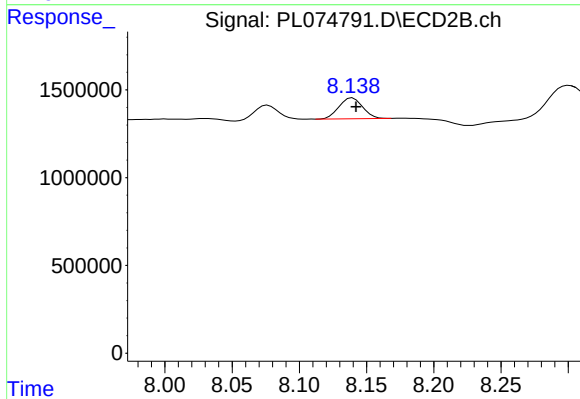

#27 Chlordane-5


R.T.: 8.140 min
Delta R.T.: -0.003 min
Response: 1456834
Conc: 39.40 ng/ml

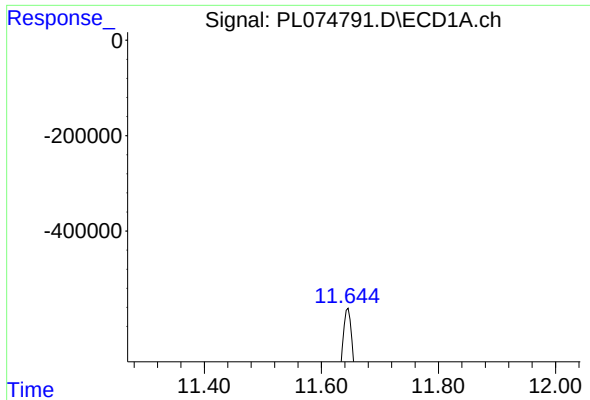

#28 Decachlorobiphenyl

R.T.: 11.646 min
Delta R.T.: -0.005 min
Response: 6826578
Conc: 15.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

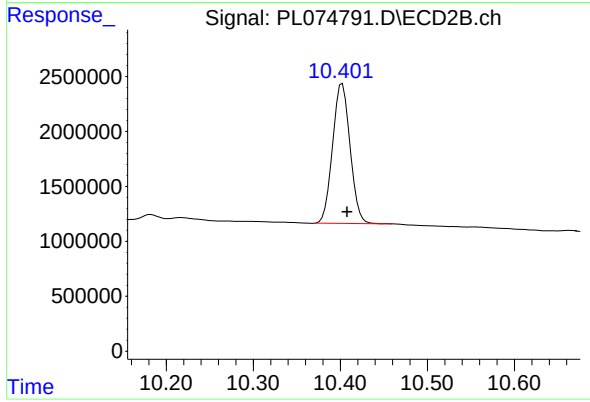

#28 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: -0.006 min
Response: 17739979
Conc: 17.28 ng/ml