

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051822\
 Data File : PL074794.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2022 17:33
 Operator : AR\AJ
 Sample : N2865-24
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 03:14:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.652	4.651	10122731	27758147	19.937	20.224
28)	SA Decachlor...	11.651	10.405	6392510	17393911	14.314	16.946
Target Compounds							
3)	MA gamma-BHC...	0.000	5.795f	0	309907	N.D.	0.188 #
4)	MA Heptachlor	7.292	0.000	1034584	0	1.603	N.D. #
5)	MB Aldrin	0.000	6.499	0	318132	N.D.	0.212 #
6)	B beta-BHC	0.000	6.126f	0	9556841	N.D.	12.037 #
7)	B delta-BHC	7.133f	0.000	4392765	0	7.006	N.D. #
9)	A Endosulfan I	8.526	7.466f	2155075	793570	3.738	0.634 #
11)	B alpha-Chl...	8.507f	7.425	3132212	473764	5.131	0.350 #
23)	Chlordane-1	0.000	6.005f	0	255137	N.D.	5.630 #
26)	Chlordane-4	8.507f	7.425	3132212	473764	32.512	3.456 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051822\
Data File : PL074794.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2022 17:33
Operator : AR\AJ
Sample : N2865-24
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 03:14:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

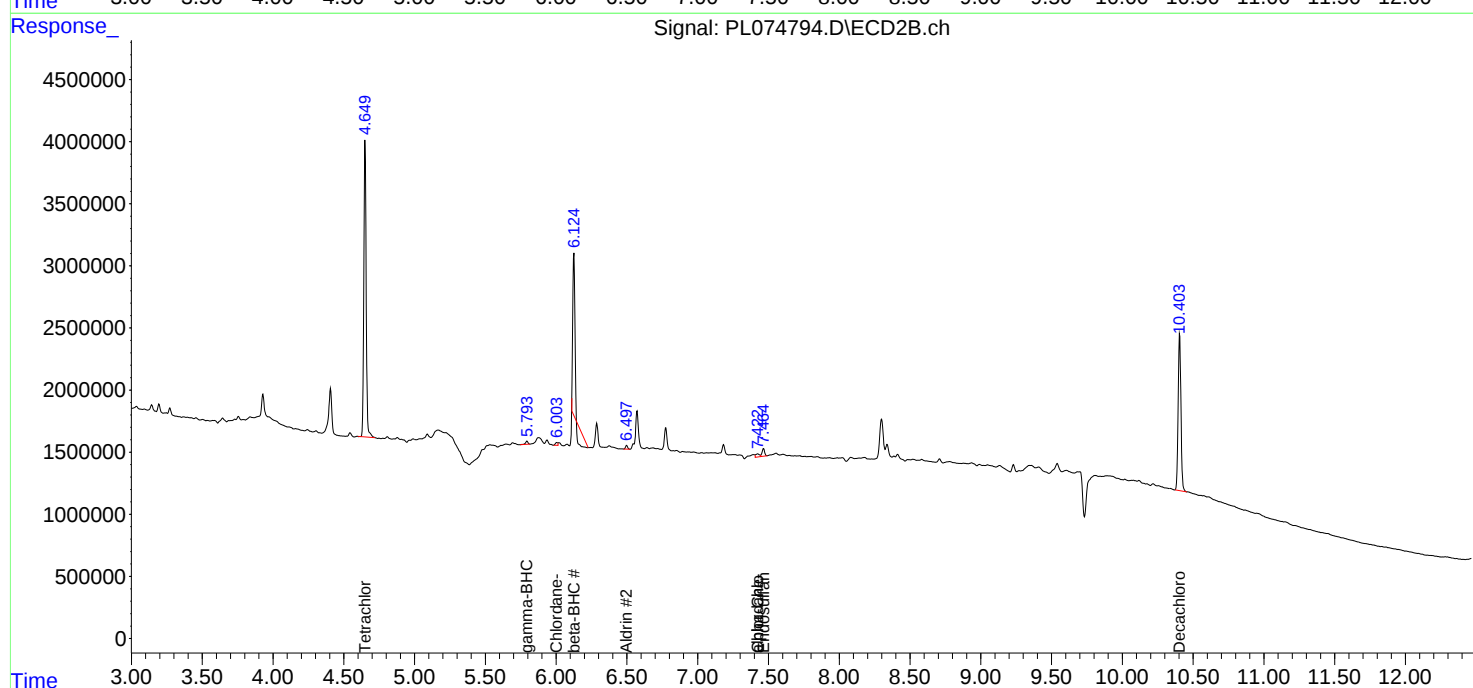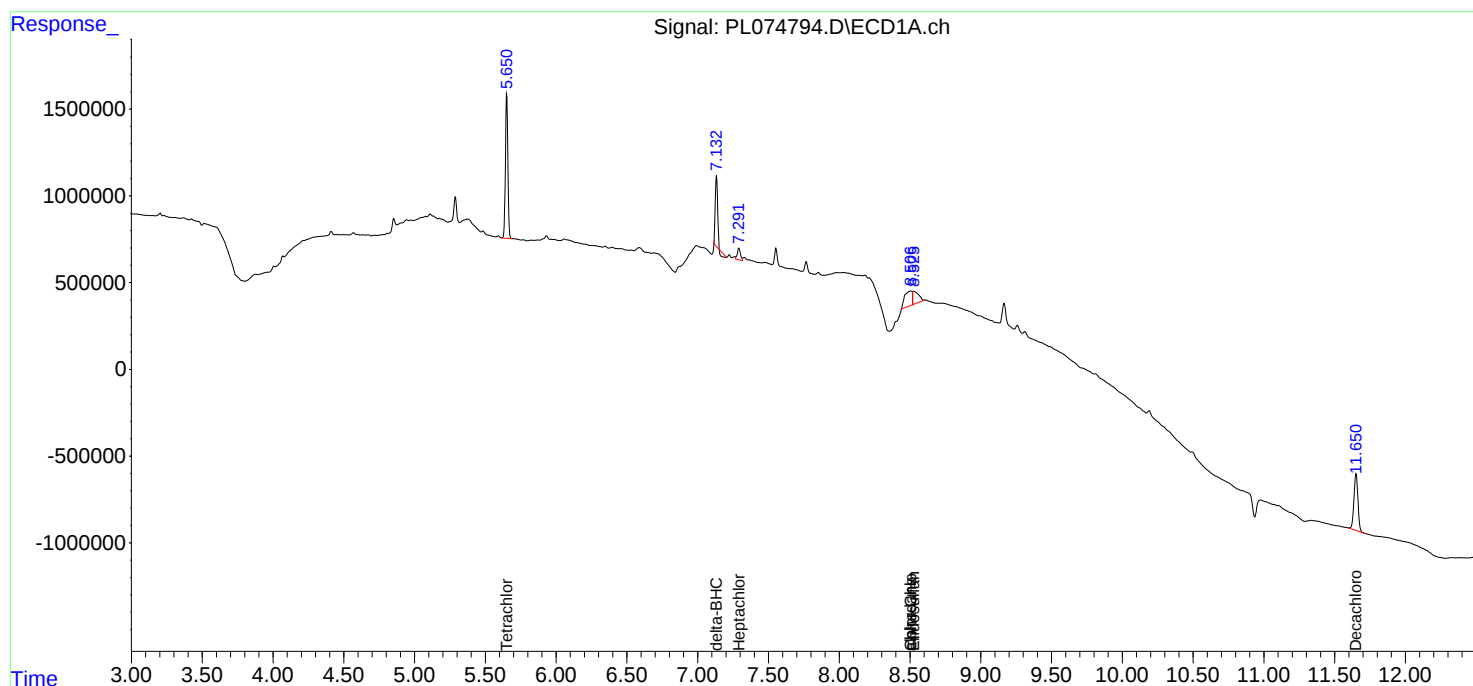


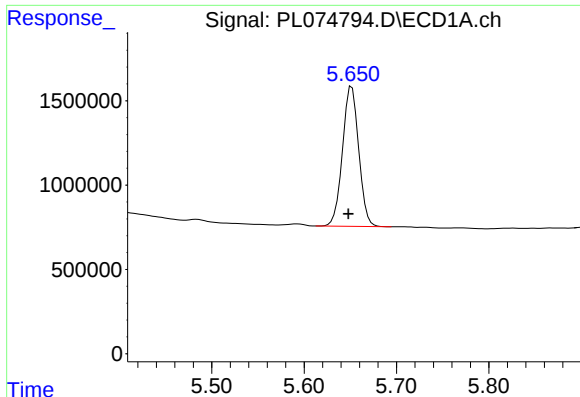

#1 Tetrachloro-m-xylene


R.T.: 5.652 min
Delta R.T.: 0.004 min
Response: 10122731
Conc: 19.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

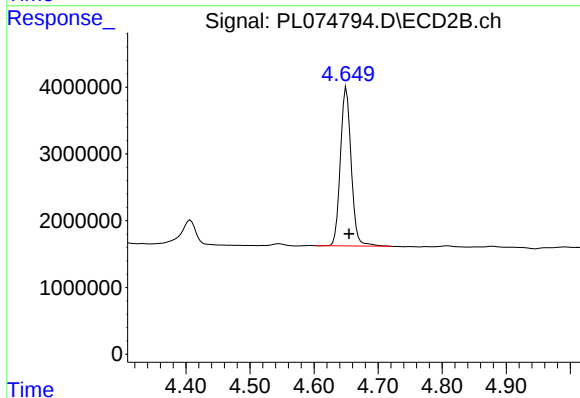


#1 Tetrachloro-m-xylene

R.T.: 4.651 min
Delta R.T.: -0.004 min
Response: 27758147
Conc: 20.22 ng/ml

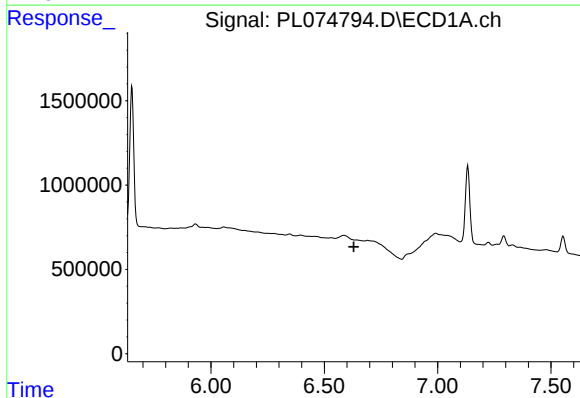


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 6.630 min
Response: 0
Conc: N.D.

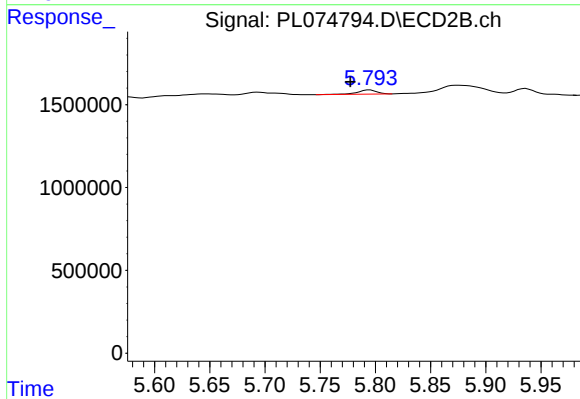

#3 gamma-BHC (Lindane)


R.T.: 5.795 min
Delta R.T.: 0.017 min
Response: 309907
Conc: 0.19 ng/ml

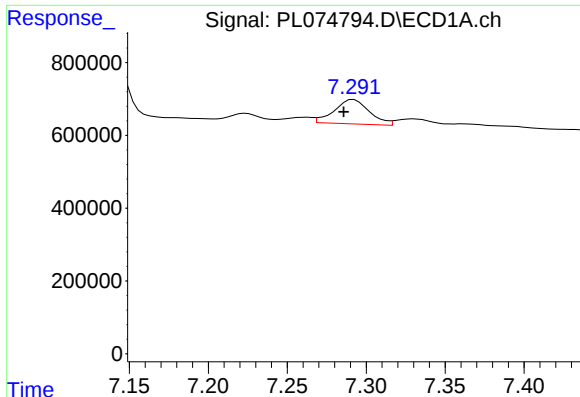

#4 Heptachlor


R.T.: 7.292 min
Delta R.T.: 0.006 min
Response: 1034584
Conc: 1.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

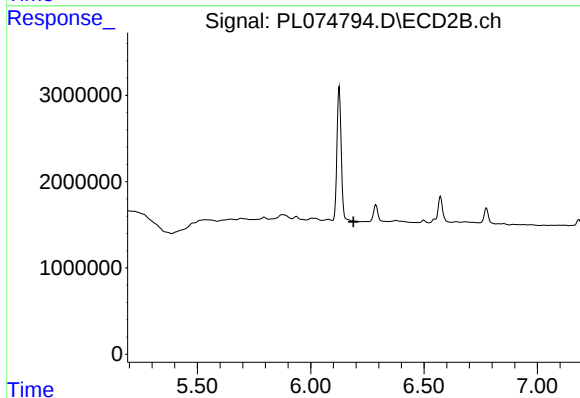


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 6.189 min
Response: 0
Conc: N.D.

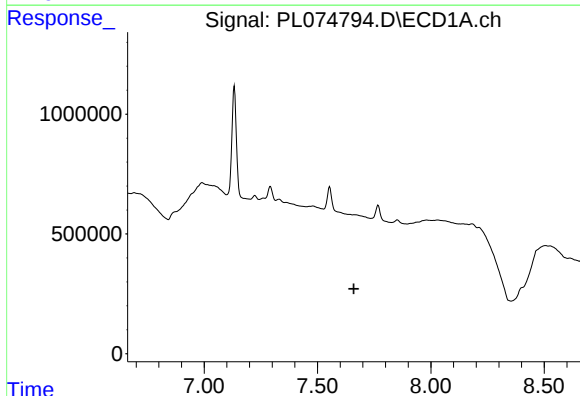


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.660 min
Response: 0
Conc: N.D.

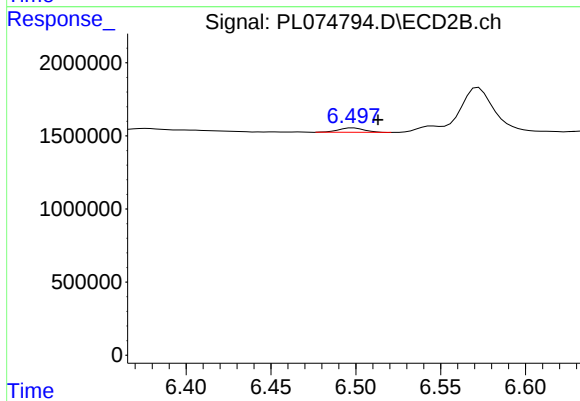

#5 Aldrin


R.T.: 6.499 min
Delta R.T.: -0.015 min
Response: 318132
Conc: 0.21 ng/ml

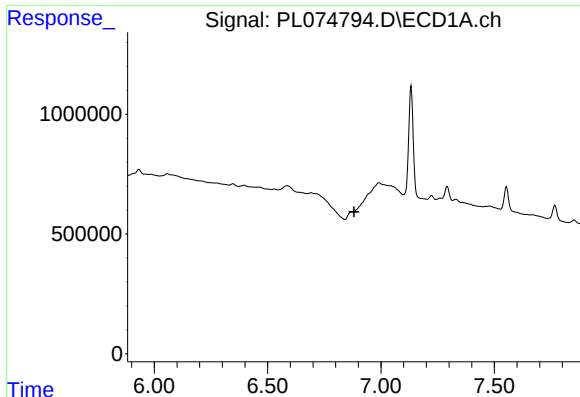

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.882 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

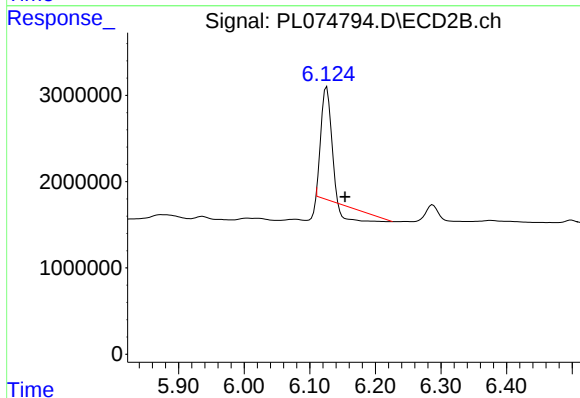


#6 beta-BHC

R.T.: 6.126 min
Delta R.T.: -0.028 min
Response: 9556841
Conc: 12.04 ng/ml

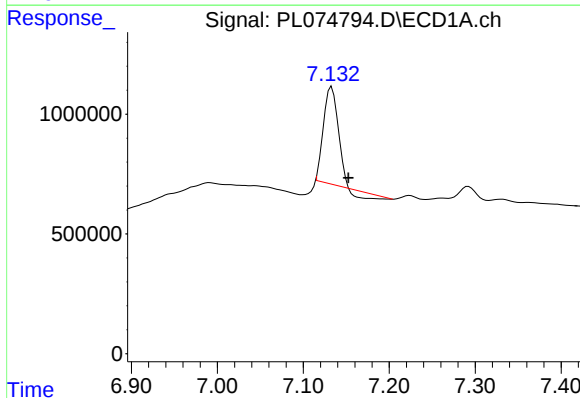


#7 delta-BHC

R.T.: 7.133 min
Delta R.T.: -0.019 min
Response: 4392765
Conc: 7.01 ng/ml

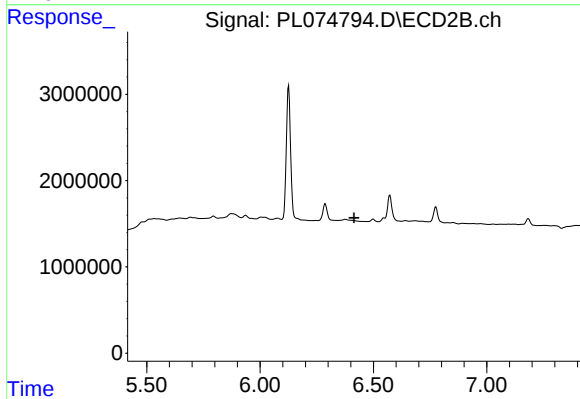

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.415 min
Response: 0
Conc: N.D.

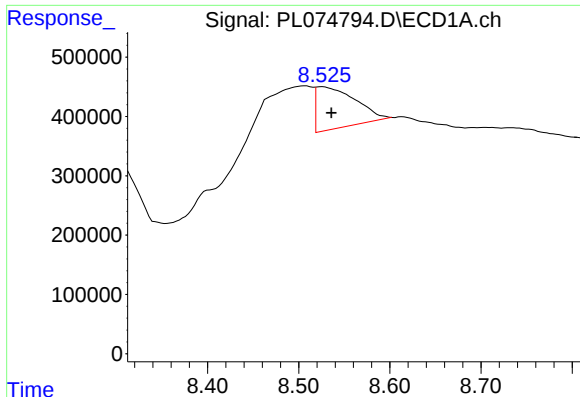

#9 Endosulfan I


R.T.: 8.526 min
Delta R.T.: -0.010 min
Response: 2155075
Conc: 3.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

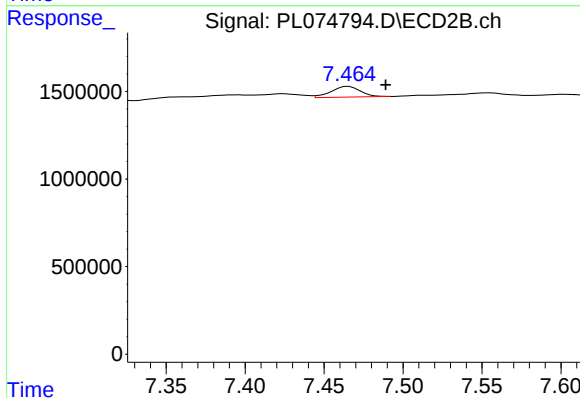


#9 Endosulfan I

R.T.: 7.466 min
Delta R.T.: -0.024 min
Response: 793570
Conc: 0.63 ng/ml

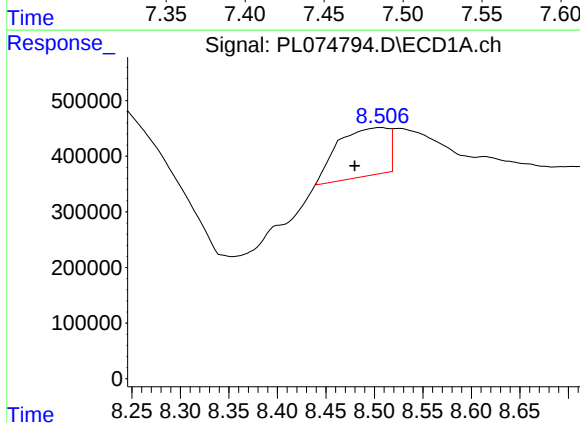


#11 alpha-Chlordane

R.T.: 8.507 min
Delta R.T.: 0.028 min
Response: 3132212
Conc: 5.13 ng/ml

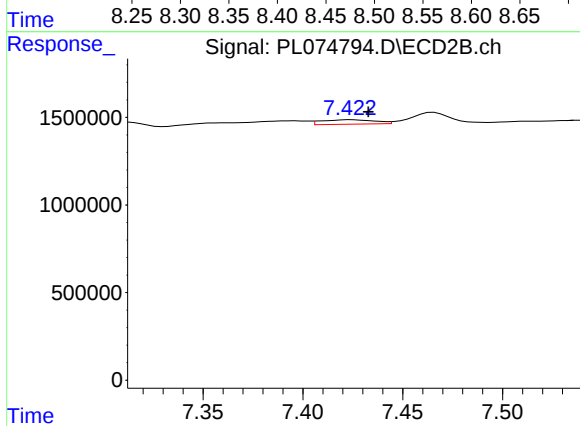

#11 alpha-Chlordane


R.T.: 7.425 min
Delta R.T.: -0.008 min
Response: 473764
Conc: 0.35 ng/ml

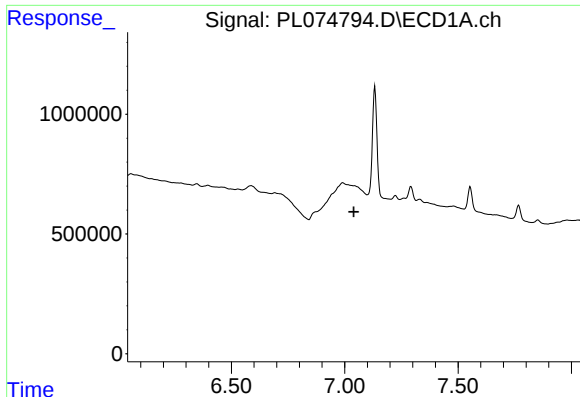

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 7.041 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

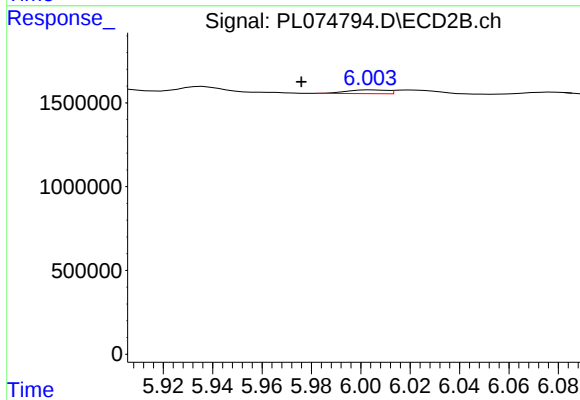


#23 Chlordane-1

R.T.: 6.005 min
Delta R.T.: 0.029 min
Response: 255137
Conc: 5.63 ng/ml

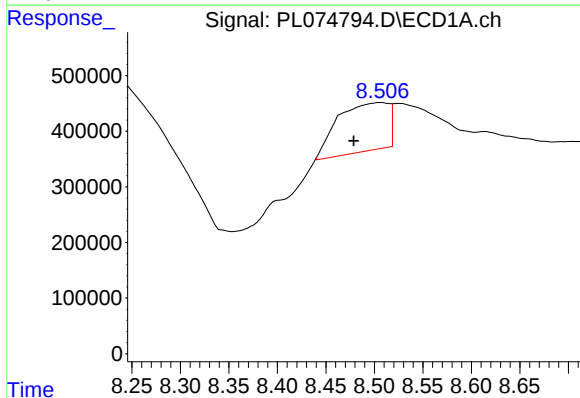


#26 Chlordane-4

R.T.: 8.507 min
Delta R.T.: 0.029 min
Response: 3132212
Conc: 32.51 ng/ml

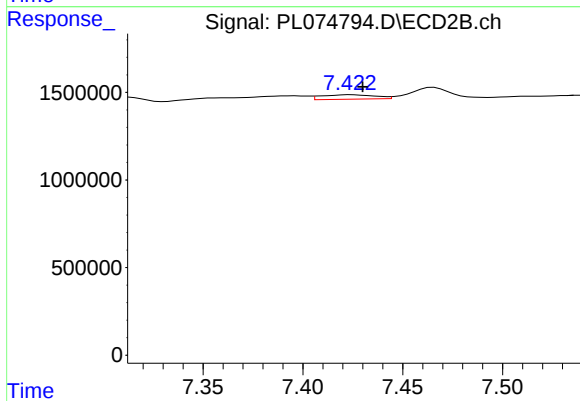

#26 Chlordane-4


R.T.: 7.425 min
Delta R.T.: -0.005 min
Response: 473764
Conc: 3.46 ng/ml

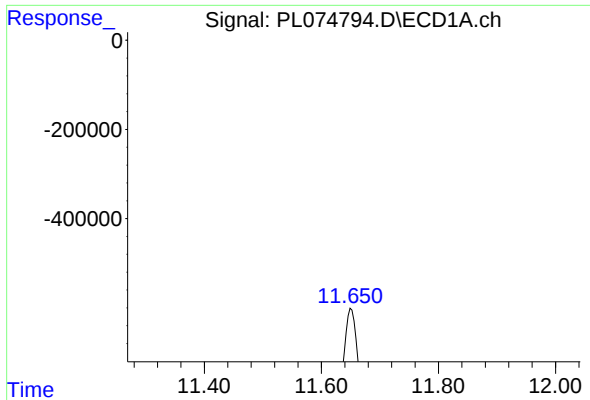

#28 Decachlorobiphenyl

R.T.: 11.651 min
Delta R.T.: 0.000 min
Response: 6392510
Conc: 14.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

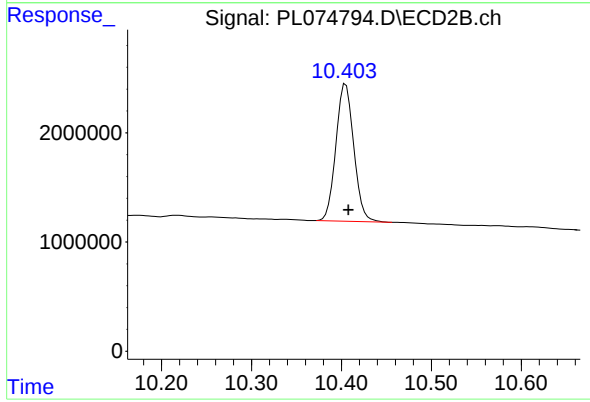

#28 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: -0.003 min
Response: 17393911
Conc: 16.95 ng/ml