

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051822\
 Data File : PL074799.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2022 18:55
 Operator : AR\AJ
 Sample : PB144874TB
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 03:15:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.646	4.650	11217935	30235244	22.094	22.029
28)	SA Decachlor...	11.646	10.402	11453949	29747263	25.648	28.982
Target Compounds							
4)	MA Heptachlor	7.312f	0.000	325344	0	0.504	N.D. #
6)	B beta-BHC	0.000	6.124f	0	373409	N.D.	0.470 #
9)	A Endosulfan I	8.506f	0.000	5270105	0	9.142	N.D. #
11)	B alpha-Chl...	8.506f	0.000	5270105	0	8.632	N.D. #
14)	MA Endrin	0.000	8.082f	0	220584	N.D.	0.209 #
26)	Chlordane-4	8.506f	0.000	5270105	0	54.703	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051822\
Data File : PL074799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2022 18:55
Operator : AR\AJ
Sample : PB144874TB
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 03:15:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

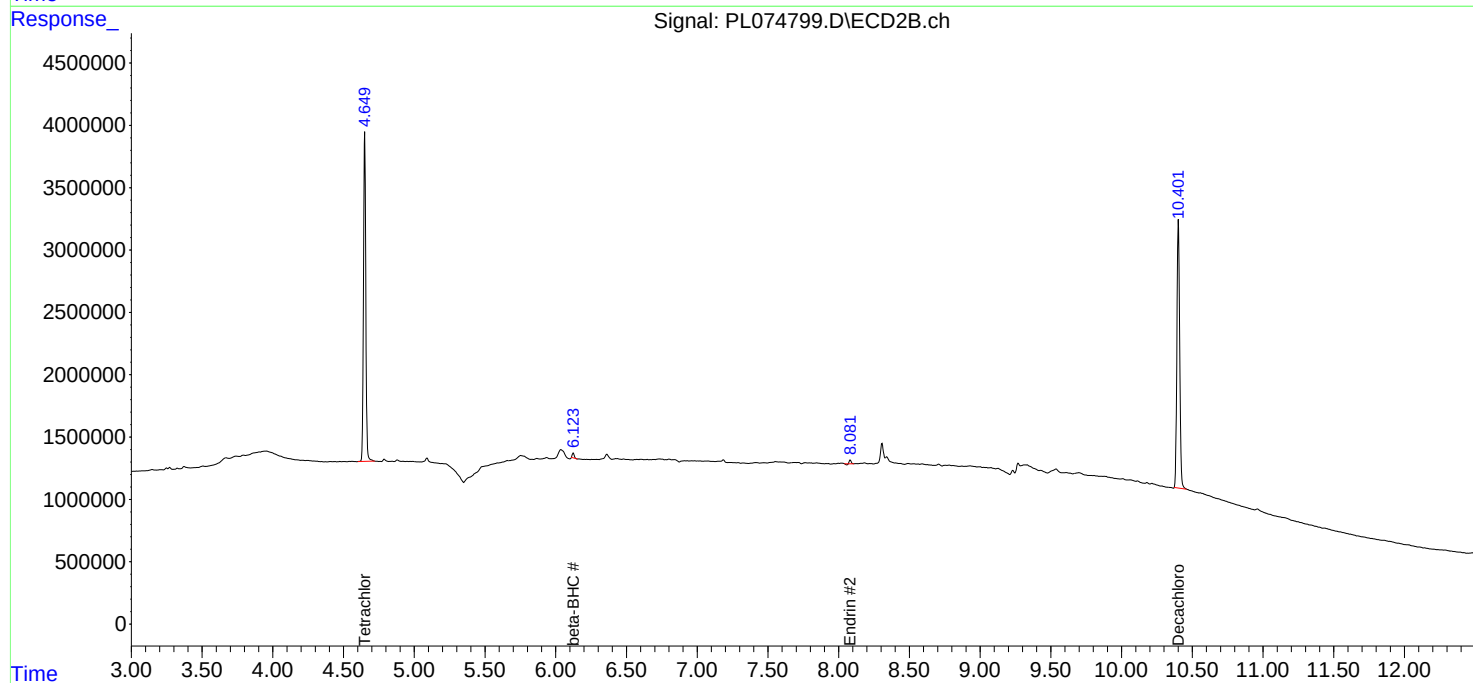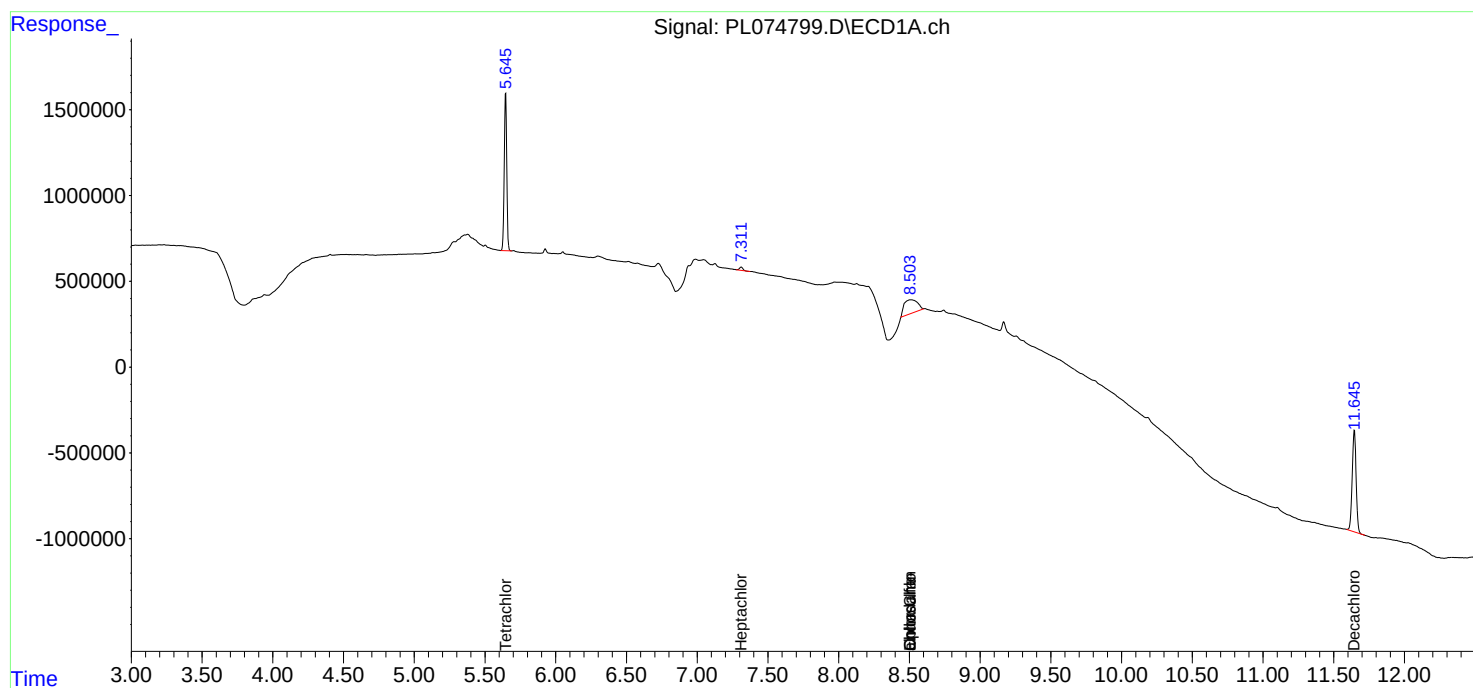


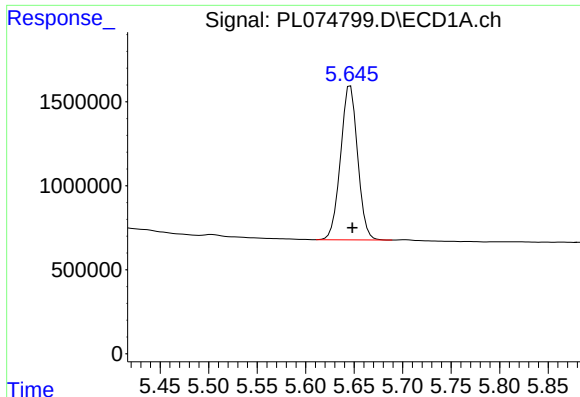

#1 Tetrachloro-m-xylene


R.T.: 5.646 min
Delta R.T.: -0.002 min
Response: 11217935
Conc: 22.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

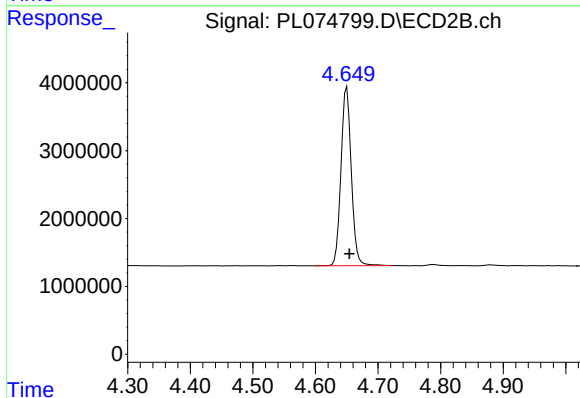


#1 Tetrachloro-m-xylene

R.T.: 4.650 min
Delta R.T.: -0.004 min
Response: 30235244
Conc: 22.03 ng/ml

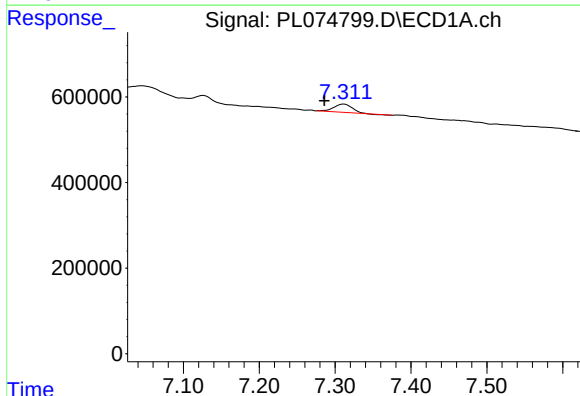


#4 Heptachlor

R.T.: 7.312 min
Delta R.T.: 0.026 min
Response: 325344
Conc: 0.50 ng/ml

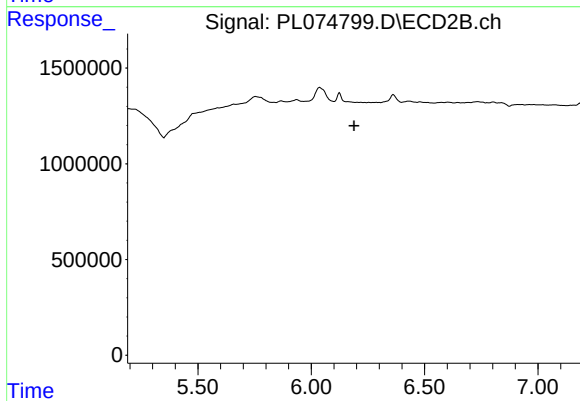

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 6.189 min
Response: 0
Conc: N.D.

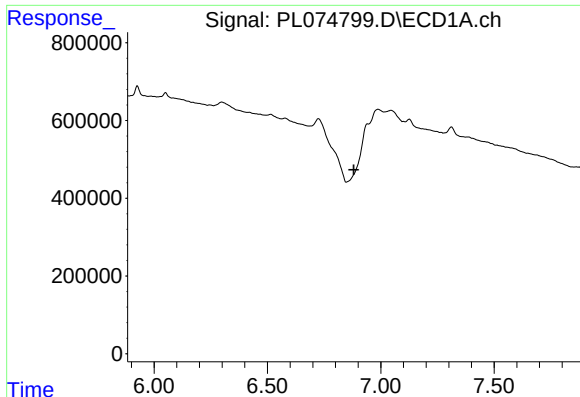

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.882 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

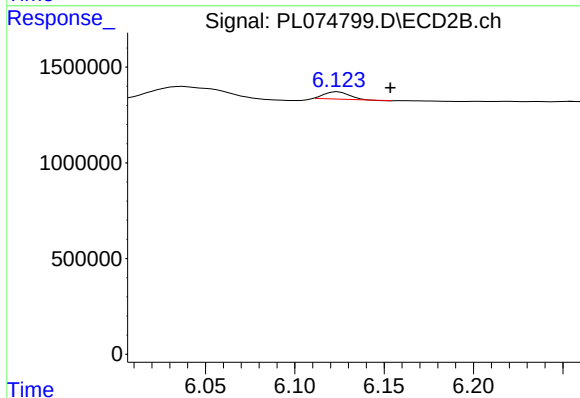


#6 beta-BHC

R.T.: 6.124 min
Delta R.T.: -0.029 min
Response: 373409
Conc: 0.47 ng/ml

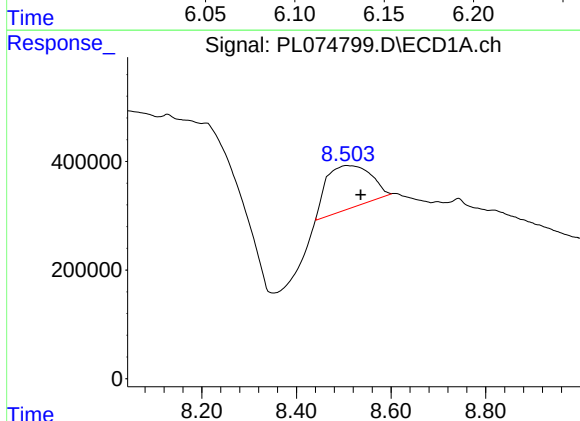


#9 Endosulfan I

R.T.: 8.506 min
Delta R.T.: -0.030 min
Response: 5270105
Conc: 9.14 ng/ml

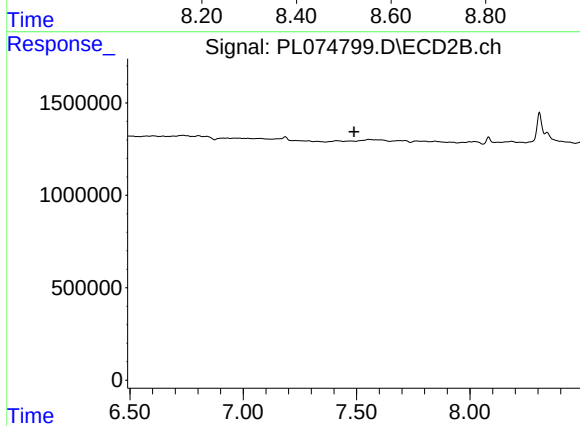

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.489 min
Response: 0
Conc: N.D.

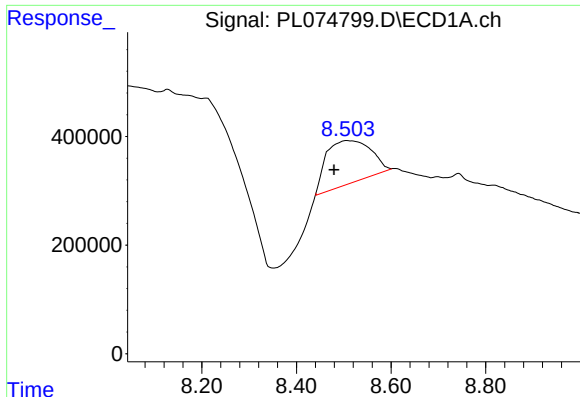

#11 alpha-Chlordane


R.T.: 8.506 min
Delta R.T.: 0.026 min
Response: 5270105
Conc: 8.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

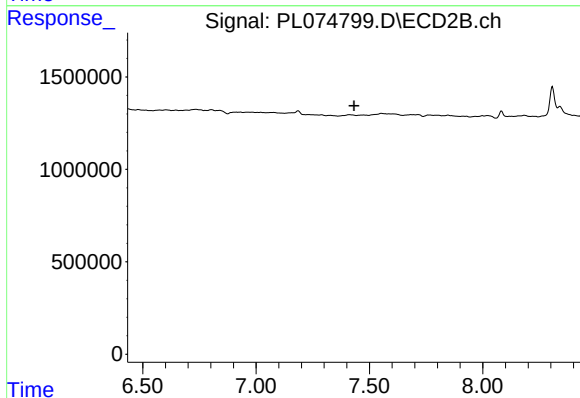


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.433 min
Response: 0
Conc: N.D.

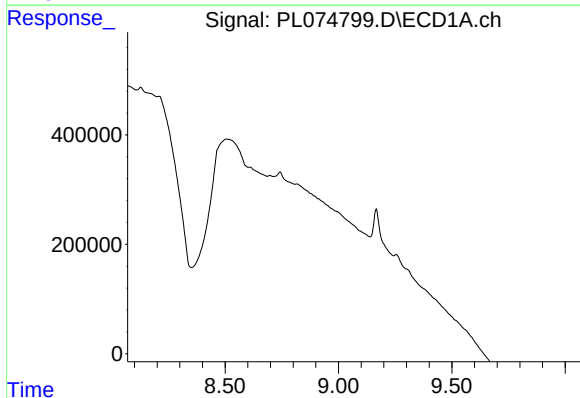


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.068 min
Response: 0
Conc: N.D.

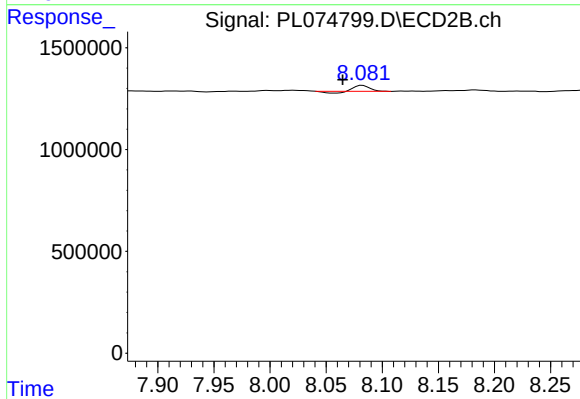

#14 Endrin


R.T.: 8.082 min
Delta R.T.: 0.018 min
Response: 220584
Conc: 0.21 ng/ml

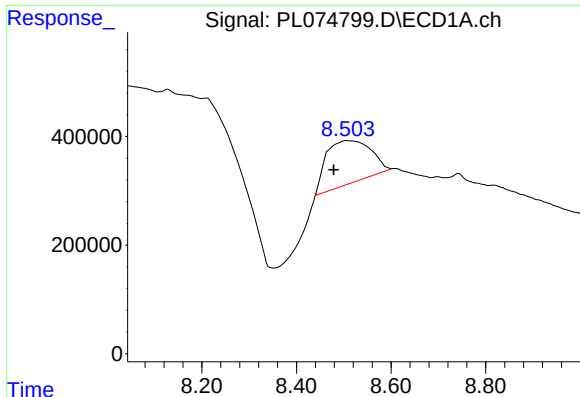

#26 Chlordane-4


R.T.: 8.506 min
Delta R.T.: 0.027 min
Response: 5270105
Conc: 54.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

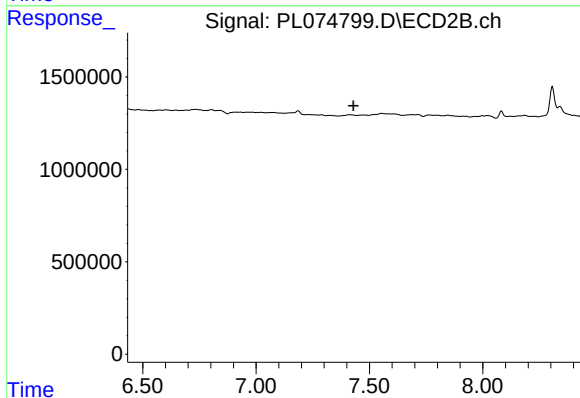


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.430 min
Response: 0
Conc: N.D.

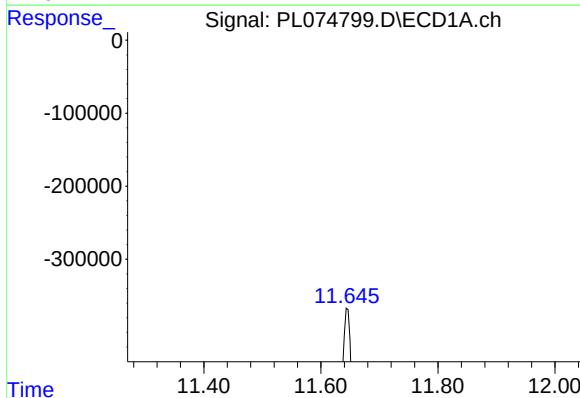

#28 Decachlorobiphenyl

R.T.: 11.646 min
Delta R.T.: -0.005 min
Response: 11453949
Conc: 25.65 ng/ml

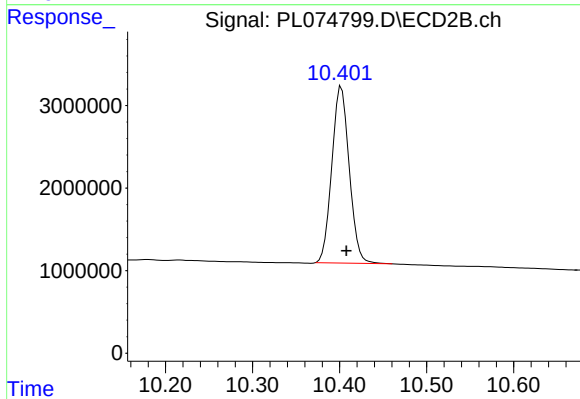

#28 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: -0.006 min
Response: 29747263
Conc: 28.98 ng/ml