

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051822\
 Data File : PL074807.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2022 21:08
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 03:18:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.645	4.650	10703050	29474243	21.080	21.475
28)	SA Decachlor...	11.645	10.403	10706178	27906535	23.973	27.188
Target Compounds							
9)	A Endosulfan I	8.506f	0.000	5036688	0	8.737	N.D. #
11)	B alpha-Chl...	8.506f	0.000	5036688	0	8.250	N.D. #
13)	MA Dieldrin	0.000	7.800f	0	250080	N.D.	0.196 #
14)	MA Endrin	0.000	8.082f	0	120126	N.D.	0.114 #
26)	Chlordane-4	8.506f	0.000	5036688	0	52.280	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051822\
Data File : PL074807.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2022 21:08
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 03:18:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

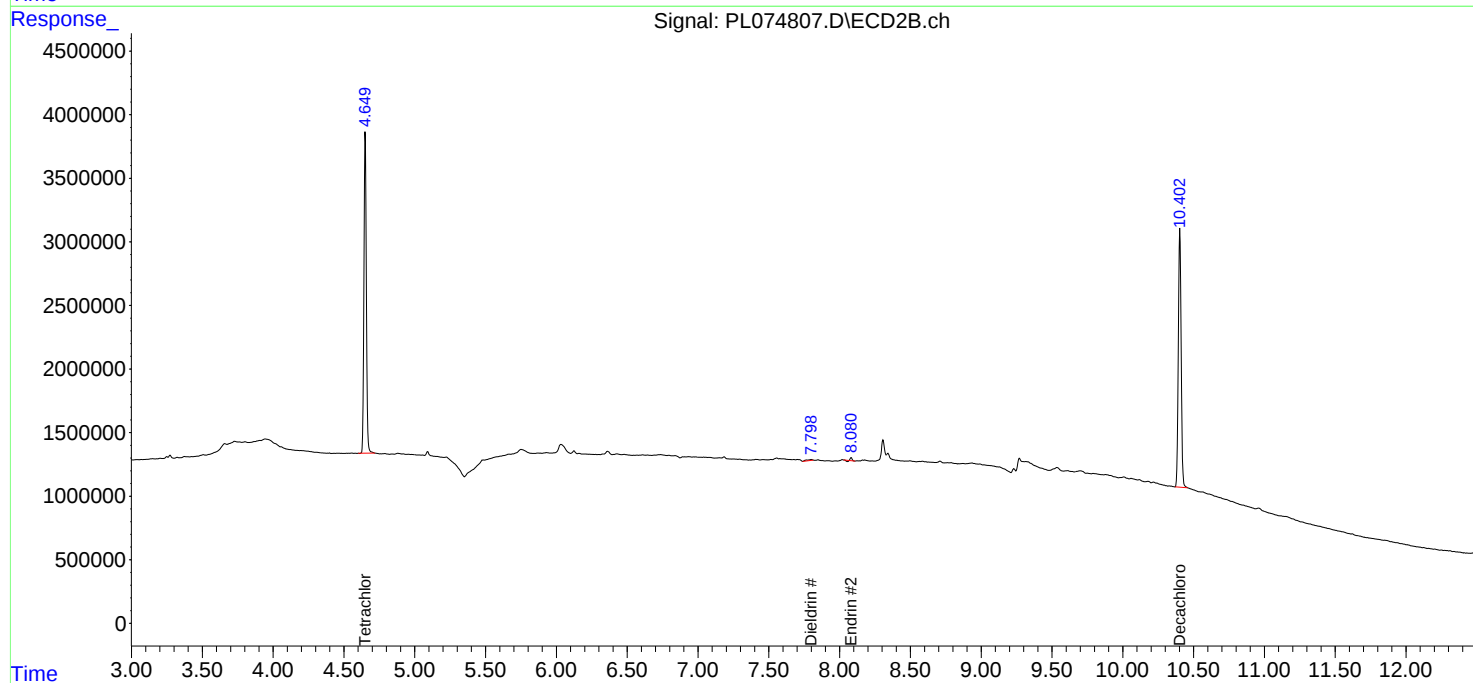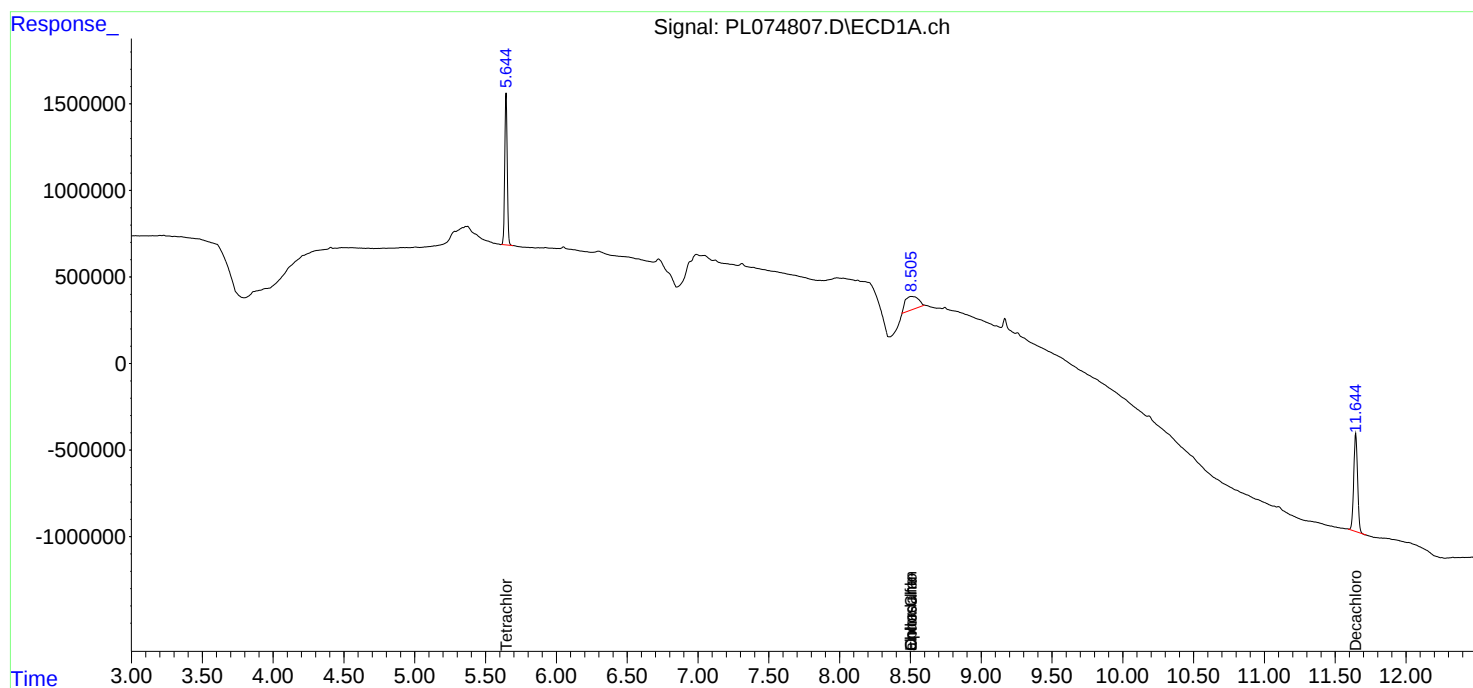


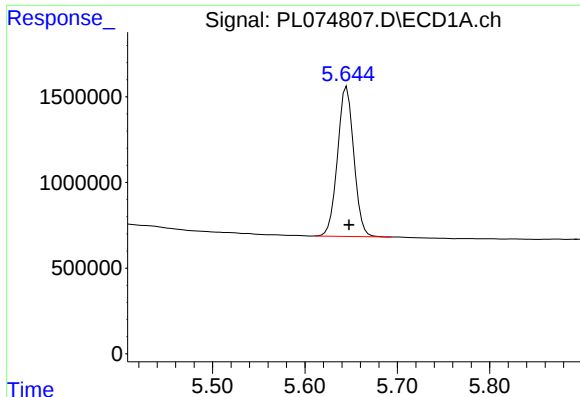

#1 Tetrachloro-m-xylene


R.T.: 5.645 min
Delta R.T.: -0.003 min
Response: 10703050
Conc: 21.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

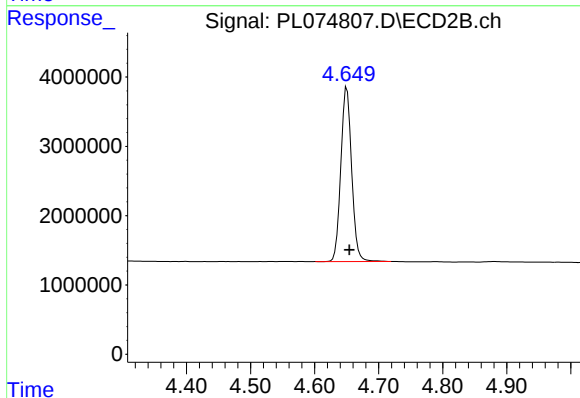


#1 Tetrachloro-m-xylene

R.T.: 4.650 min
Delta R.T.: -0.004 min
Response: 29474243
Conc: 21.47 ng/ml

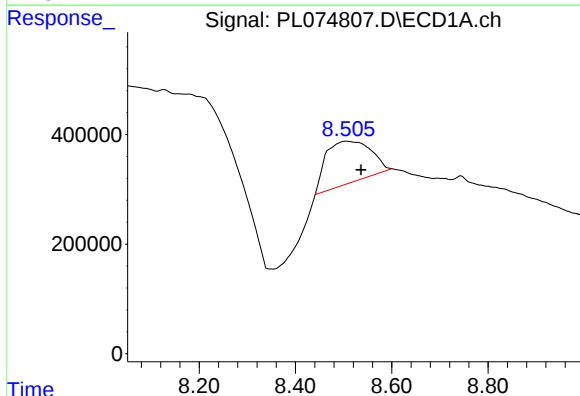


#9 Endosulfan I

R.T.: 8.506 min
Delta R.T.: -0.030 min
Response: 5036688
Conc: 8.74 ng/ml

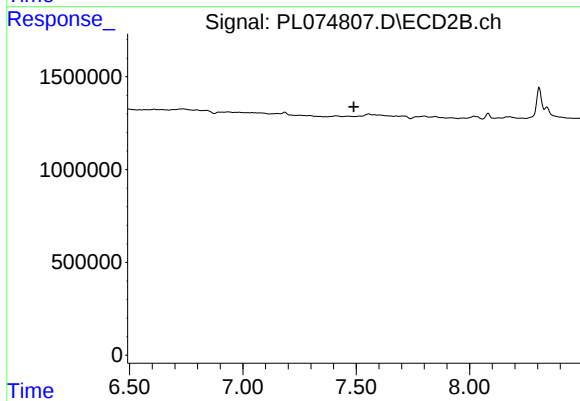

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.489 min
Response: 0
Conc: N.D.

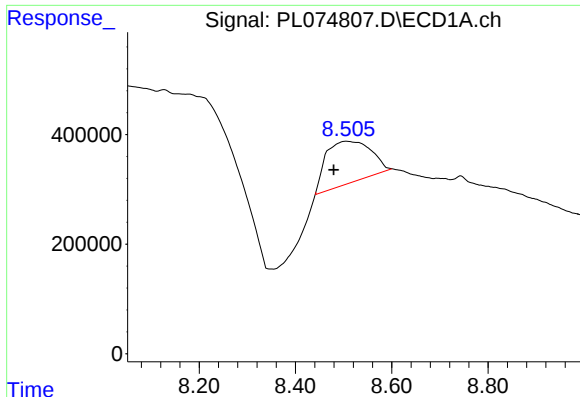

#11 alpha-Chlordane


R.T.: 8.506 min
Delta R.T.: 0.027 min
Response: 5036688
Conc: 8.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

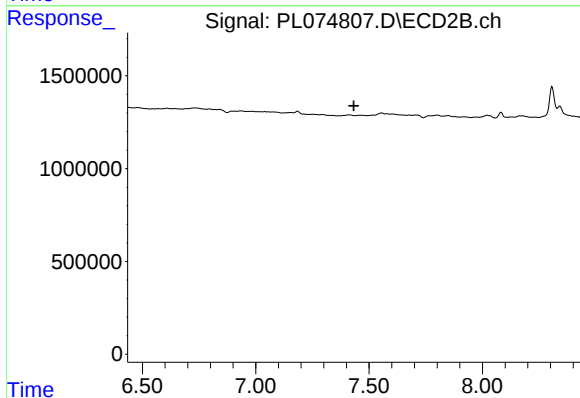


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.433 min
Response: 0
Conc: N.D.

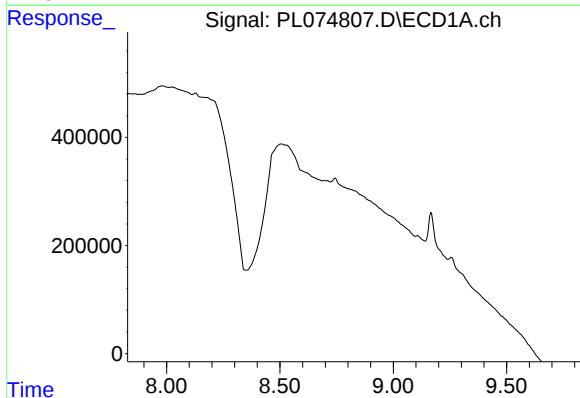


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.827 min
Response: 0
Conc: N.D.

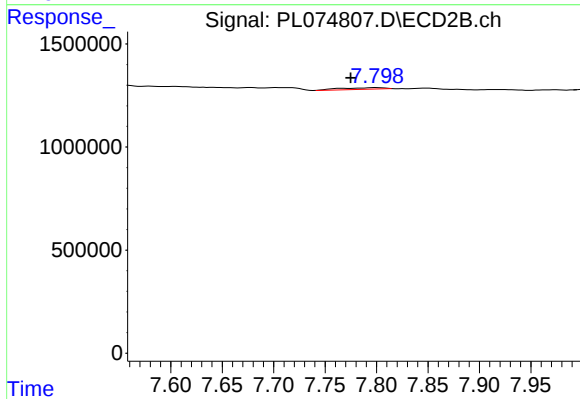

#13 Dieldrin


R.T.: 7.800 min
Delta R.T.: 0.025 min
Response: 250080
Conc: 0.20 ng/ml

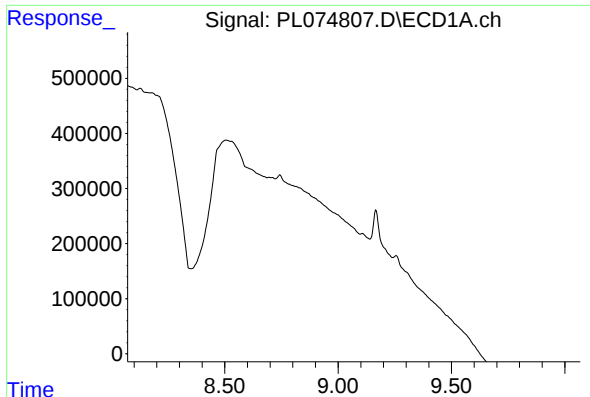

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

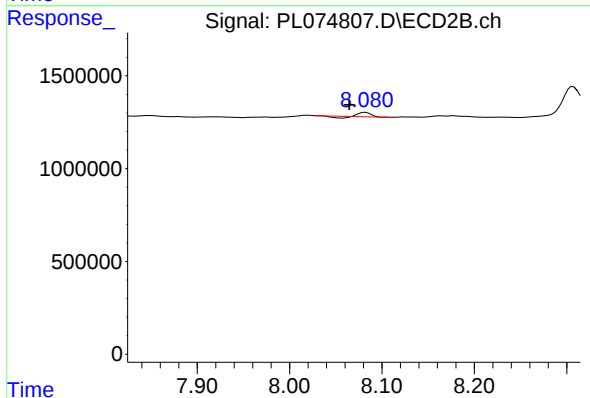


#14 Endrin

R.T.: 8.082 min
Delta R.T.: 0.017 min
Response: 120126
Conc: 0.11 ng/ml

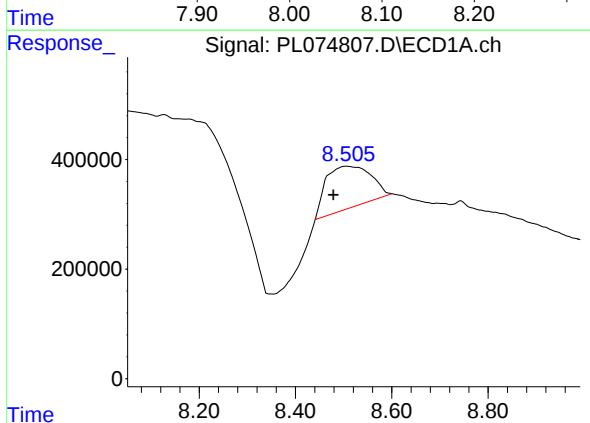


#26 Chlordane-4

R.T.: 8.506 min
Delta R.T.: 0.028 min
Response: 503668
Conc: 52.28 ng/ml

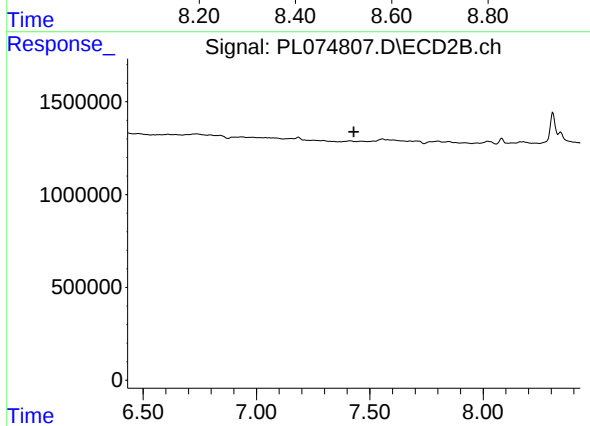

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

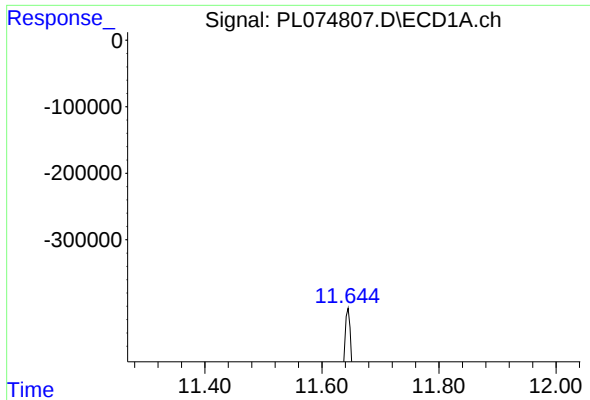

#28 Decachlorobiphenyl

R.T.: 11.645 min
Delta R.T.: -0.006 min
Response: 10706178
Conc: 23.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

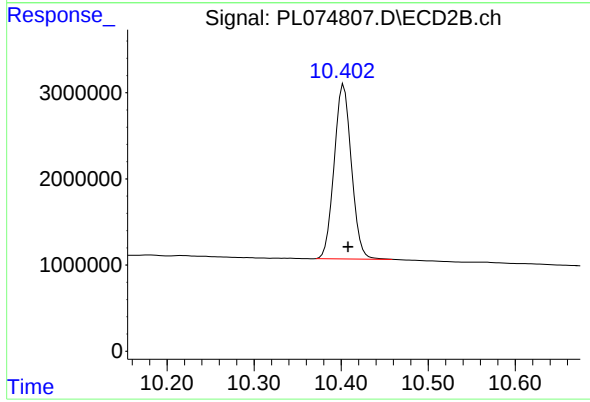

#28 Decachlorobiphenyl

R.T.: 10.403 min
Delta R.T.: -0.005 min
Response: 27906535
Conc: 27.19 ng/ml