

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051823\
 Data File : PL082790.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2023 12:45
 Operator : AR\AJ
 Sample : PB152839TB
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB152839TB

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/19/2023
 Supervised By : Ankita Jodhani 05/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 21:10:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	2.640	43655918	36409684	16.343	15.716
28)	SA Decachlor...	8.735	7.745	33064387	34645746	17.320	15.179m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051823\
Data File : PL082790.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2023 12:45
Operator : AR\AJ
Sample : PB152839TB
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB152839TB


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/19/2023
Supervised By : Ankita Jodhani 05/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 21:10:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

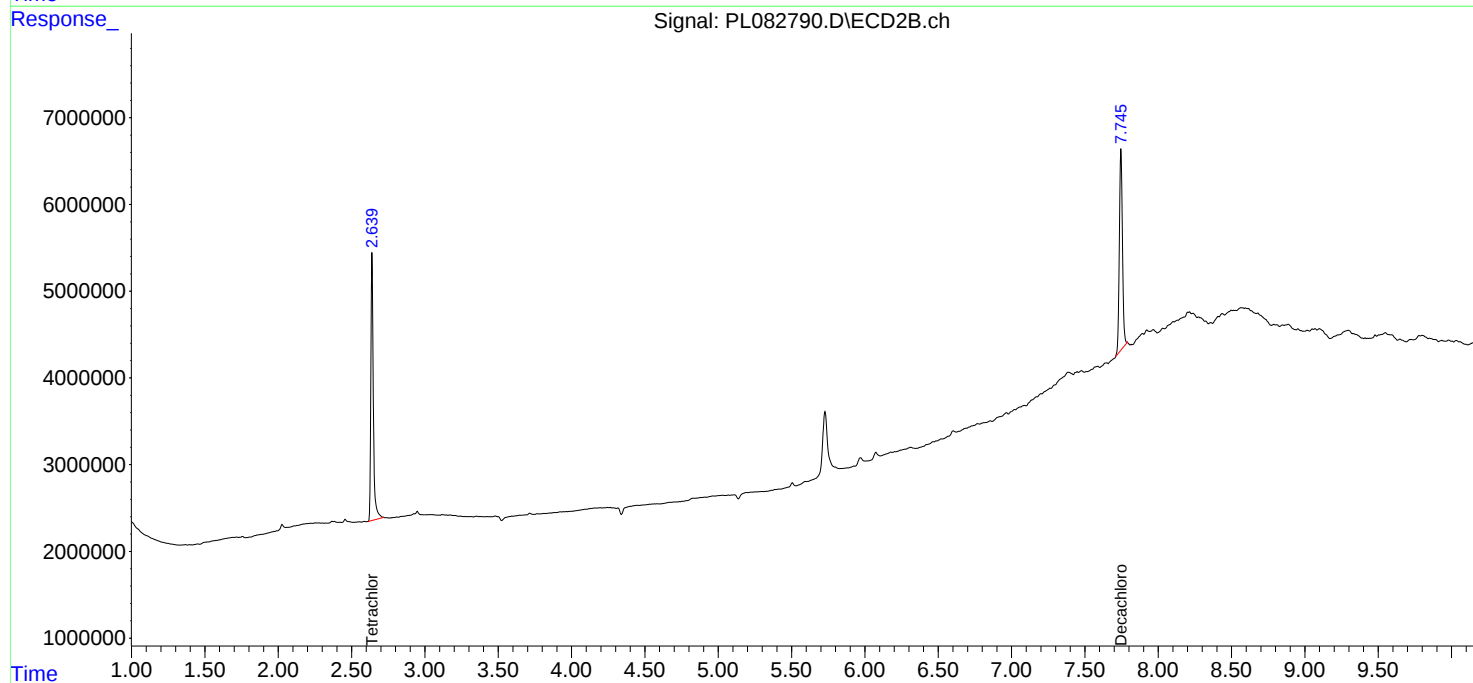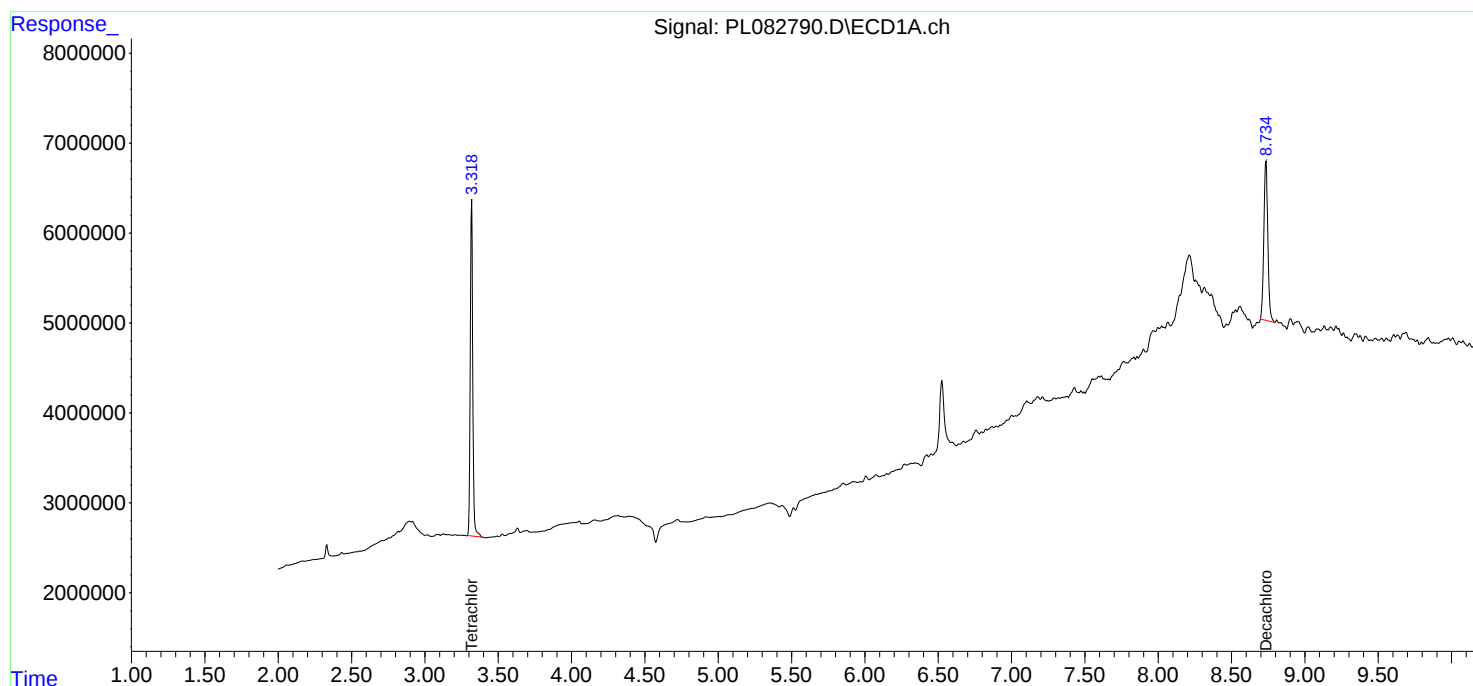

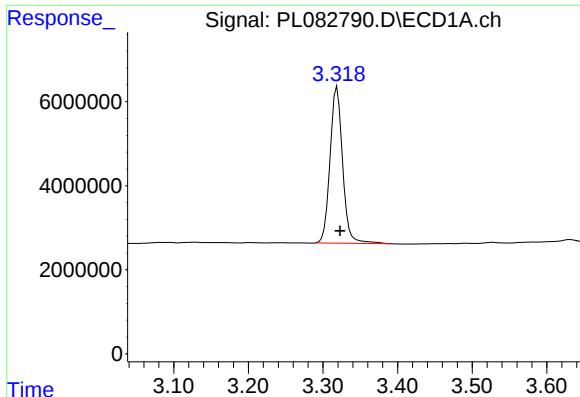


#1 Tetrachloro-m-xylene

R.T.: 3.319 min
Delta R.T.: -0.004 min
Response: 43655918
Conc: 16.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB152839TB


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/19/2023
Supervised By :Ankita Jodhani 05/19/2023

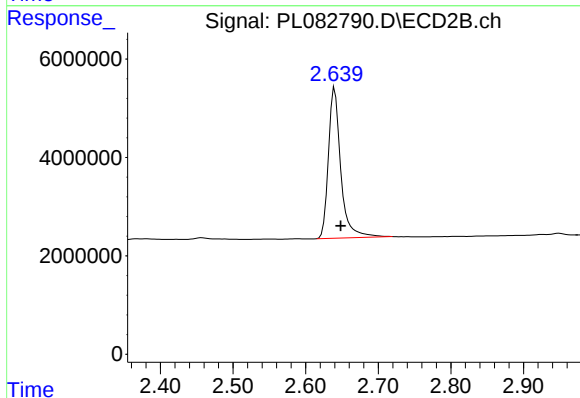


#1 Tetrachloro-m-xylene

R.T.: 2.640 min
Delta R.T.: -0.008 min
Response: 36409684
Conc: 15.72 ng/ml

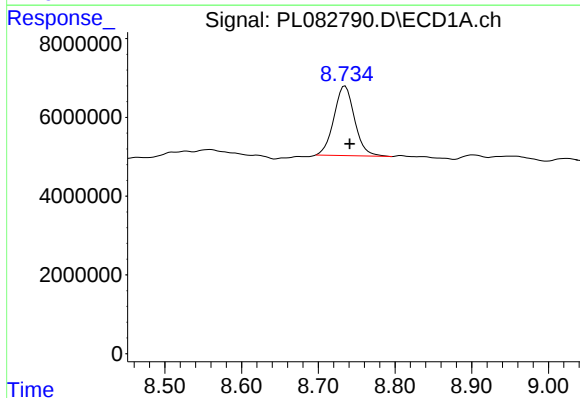

#28 Decachlorobiphenyl

R.T.: 8.735 min
Delta R.T.: -0.006 min
Response: 33064387
Conc: 17.32 ng/ml

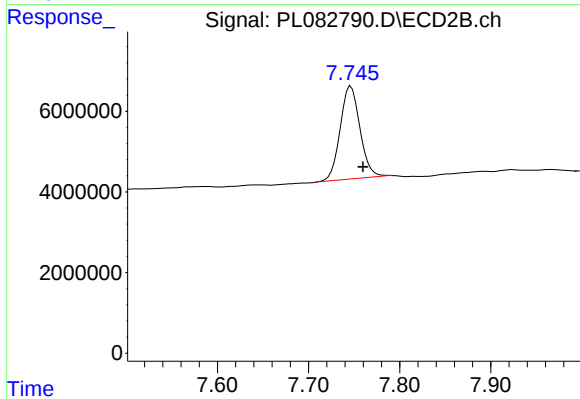

#28 Decachlorobiphenyl

R.T.: 7.745 min
Delta R.T.: -0.015 min
Response: 34645746
Conc: 15.18 ng/ml m