

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051919\
 Data File : PL048721.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2019 10:59
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 04:51:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
4) MA	Heptachlor	0.000	5.089f	0	11322627	N.D. 3.271 #
8) B	Heptachlo...	0.000	5.833f	0	4952517	N.D. 1.698 #
11) B	alpha-Chl...	5.262	0.000	45596990	0	3.488 N.D. #
22)	Mirex	7.123	0.000	7521235	0	0.839 N.D. #
26)	Chlordane-4	5.262	0.000	45596990	0	31.407 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051919\
Data File : PL048721.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2019 10:59
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 04:51:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

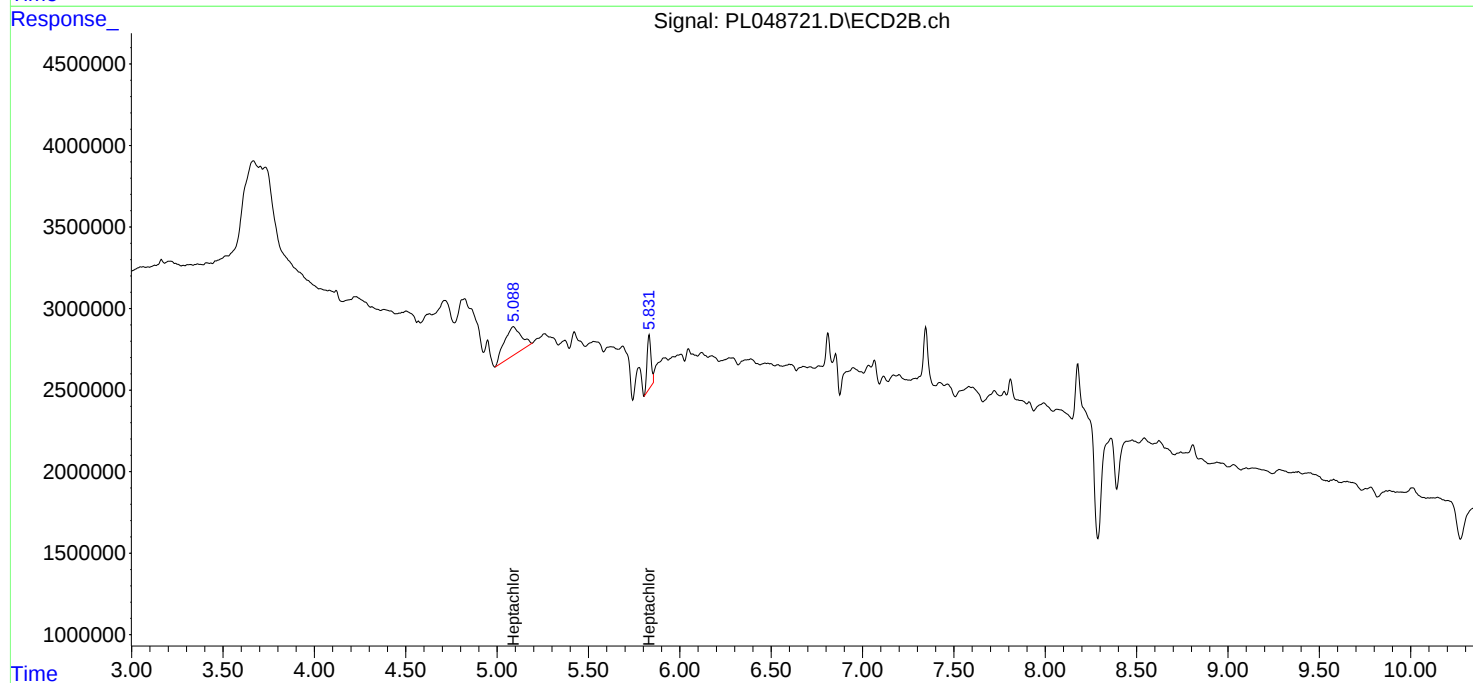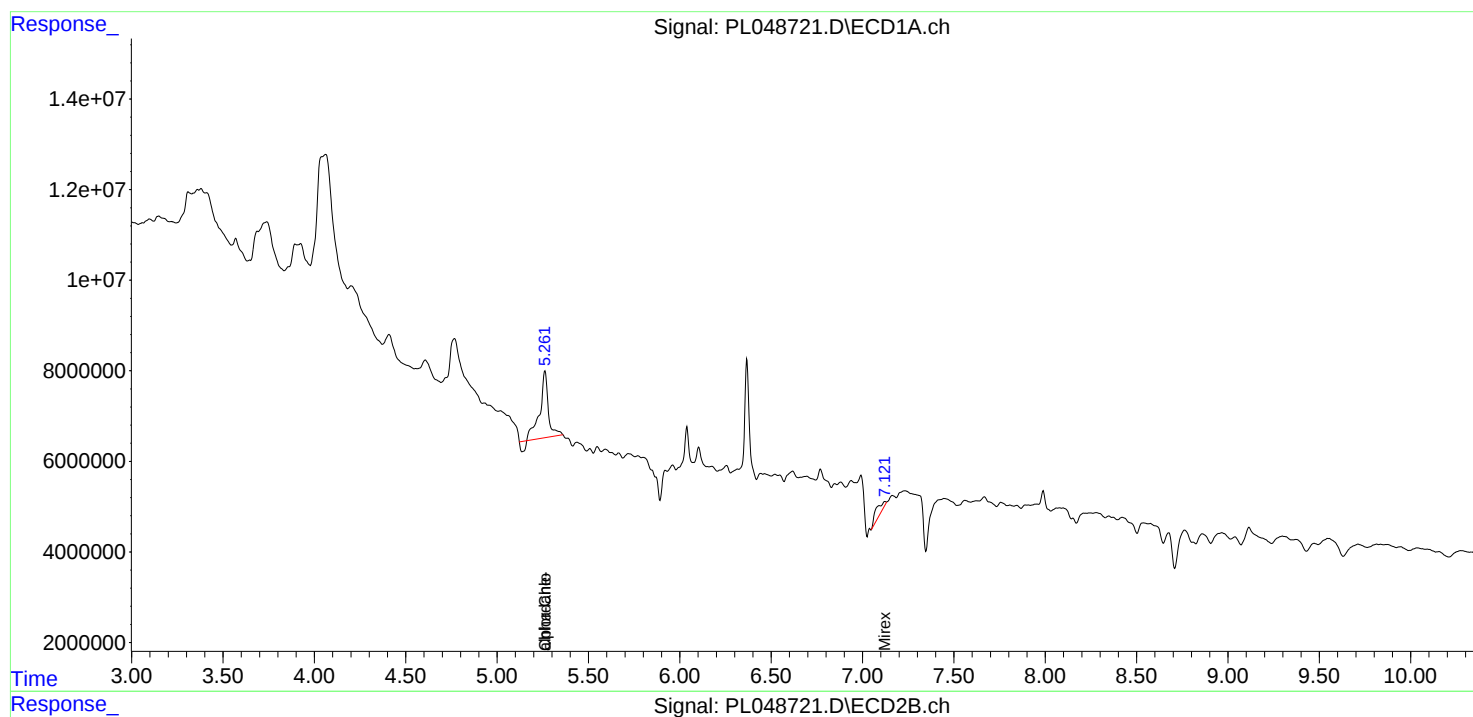


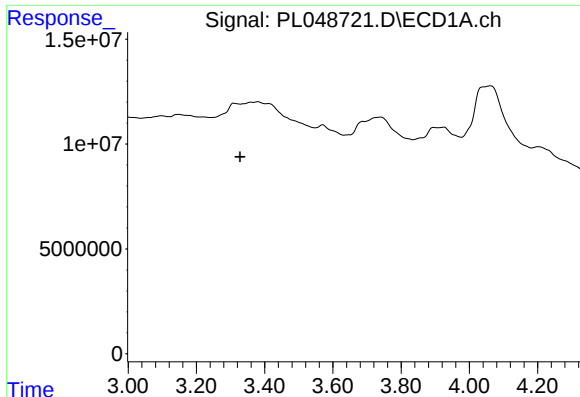

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

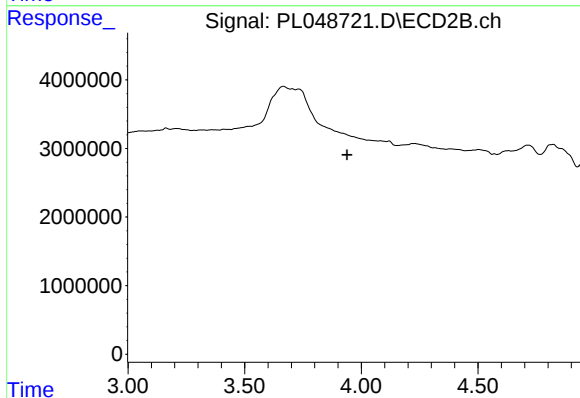


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.940 min
Response: 0
Conc: N.D.

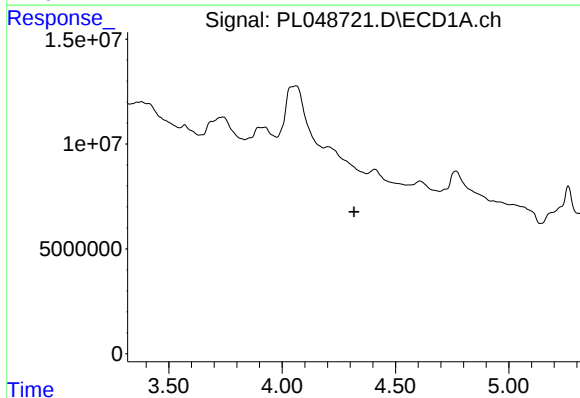


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

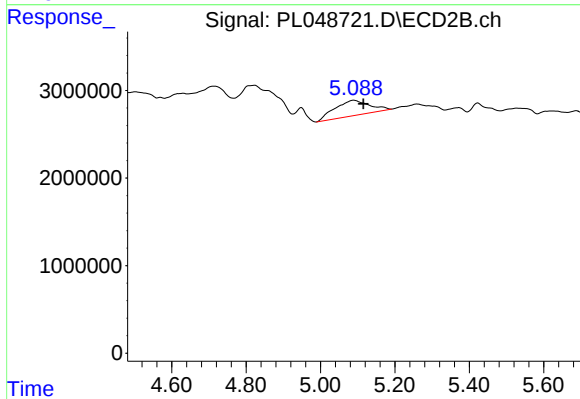

#4 Heptachlor


R.T.: 5.089 min
Delta R.T.: -0.026 min
Response: 11322627
Conc: 3.27 ng/ml

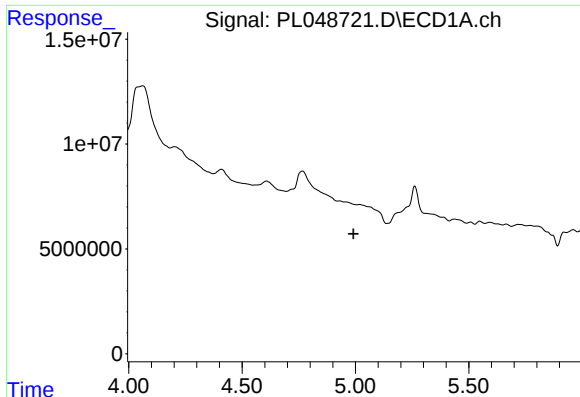

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

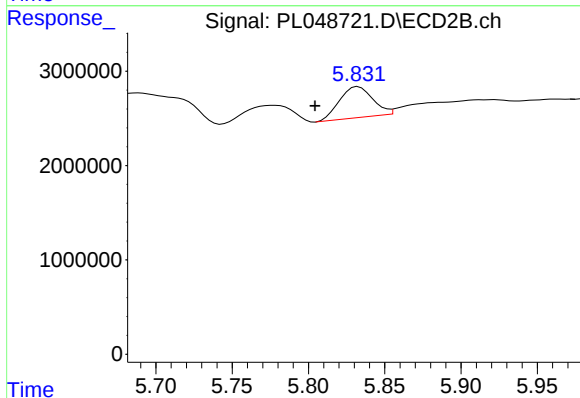


#8 Heptachlor epoxide

R.T.: 5.833 min
Delta R.T.: 0.028 min
Response: 4952517
Conc: 1.70 ng/ml

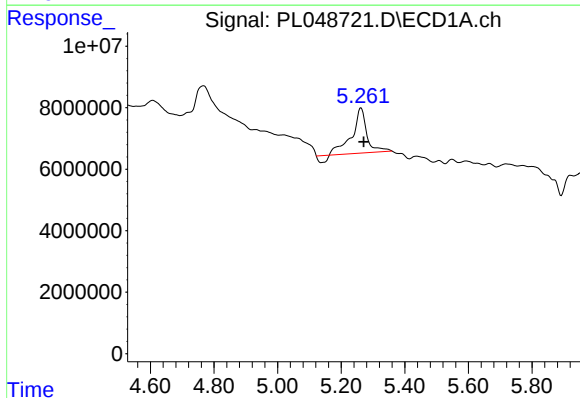


#11 alpha-Chlordane

R.T.: 5.262 min
Delta R.T.: -0.009 min
Response: 45596990
Conc: 3.49 ng/ml

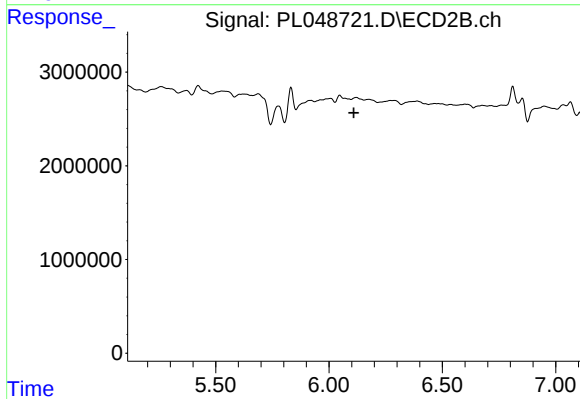

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.109 min
Response: 0
Conc: N.D.

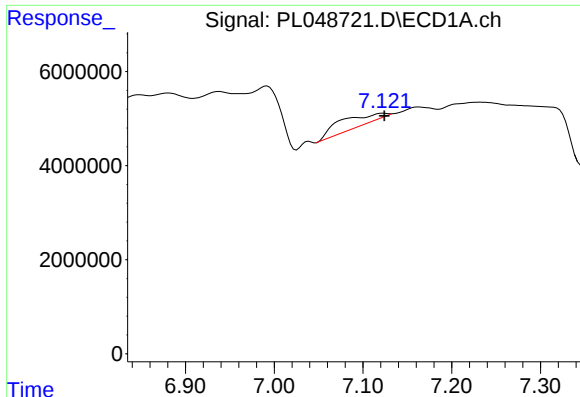

#22 Mirex


R.T.: 7.123 min
Delta R.T.: -0.001 min
Response: 7521235
Conc: 0.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

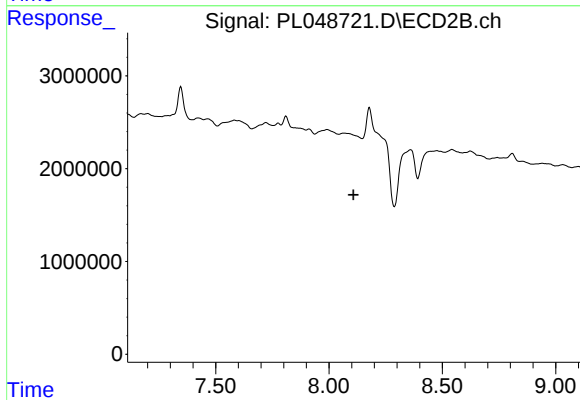


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.109 min
Response: 0
Conc: N.D.

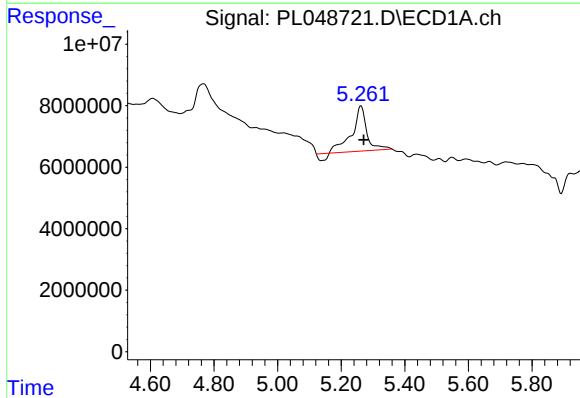


#26 Chlordane-4

R.T.: 5.262 min
Delta R.T.: -0.008 min
Response: 45596990
Conc: 31.41 ng/ml

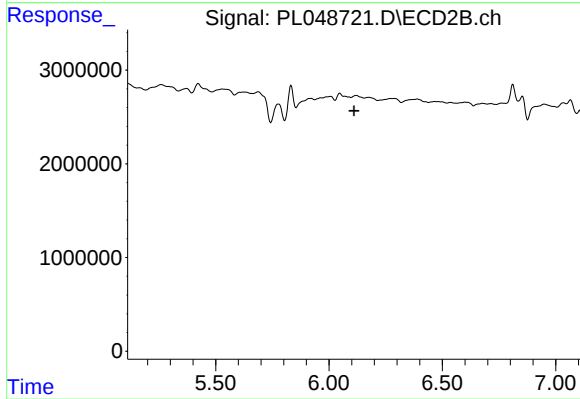

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.111 min
Response: 0
Conc: N.D.

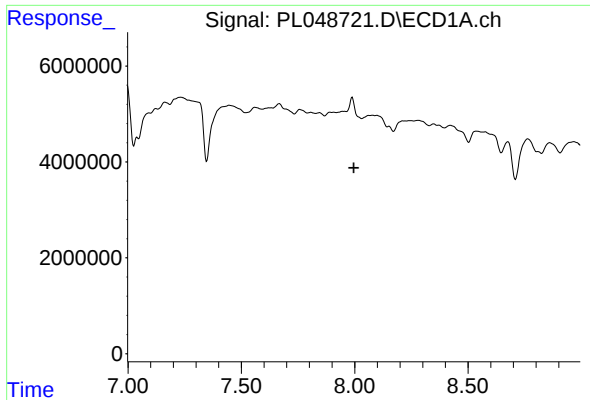

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.996 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

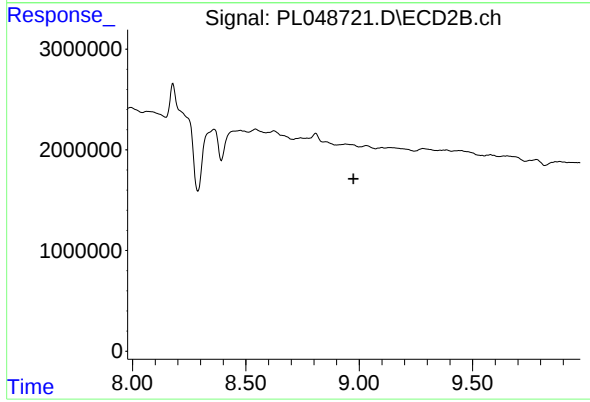

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.975 min
Response: 0
Conc: N.D.