

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051919\
 Data File : PL048742.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2019 17:52
 Operator : SM\AJ
 Sample : K2913-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-17-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 04:54:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	3.939	0	17375400	N.D.	6.976 #
28)	SA Decachlor...	7.994	8.974	116.6E6	30446287	11.596	11.471
Target Compounds							
2)	A alpha-BHC	3.769	4.354f	17598762	-688624	1.138	N.D. #
5)	MB Aldrin	4.543	5.413	3511.5E6	51012927	256.282	16.474 #
9)	A Endosulfan I	5.332	6.184f	684.5E6	69838127	56.899	24.700 #
11)	B alpha-Chl...	5.251f	0.000	1581.3E6	0	120.951	N.D. #
20)	A Methoxychlor	6.706f	0.000	6211821	0	1.141	N.D. #
24)	Chlordane-2	0.000	5.413f	0	51012927	N.D.	394.413 #
26)	Chlordane-4	5.251f	0.000	1581.3E6	0	1089.152	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051919\
Data File : PL048742.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2019 17:52
Operator : SM\AJ
Sample : K2913-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-17-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 04:54:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

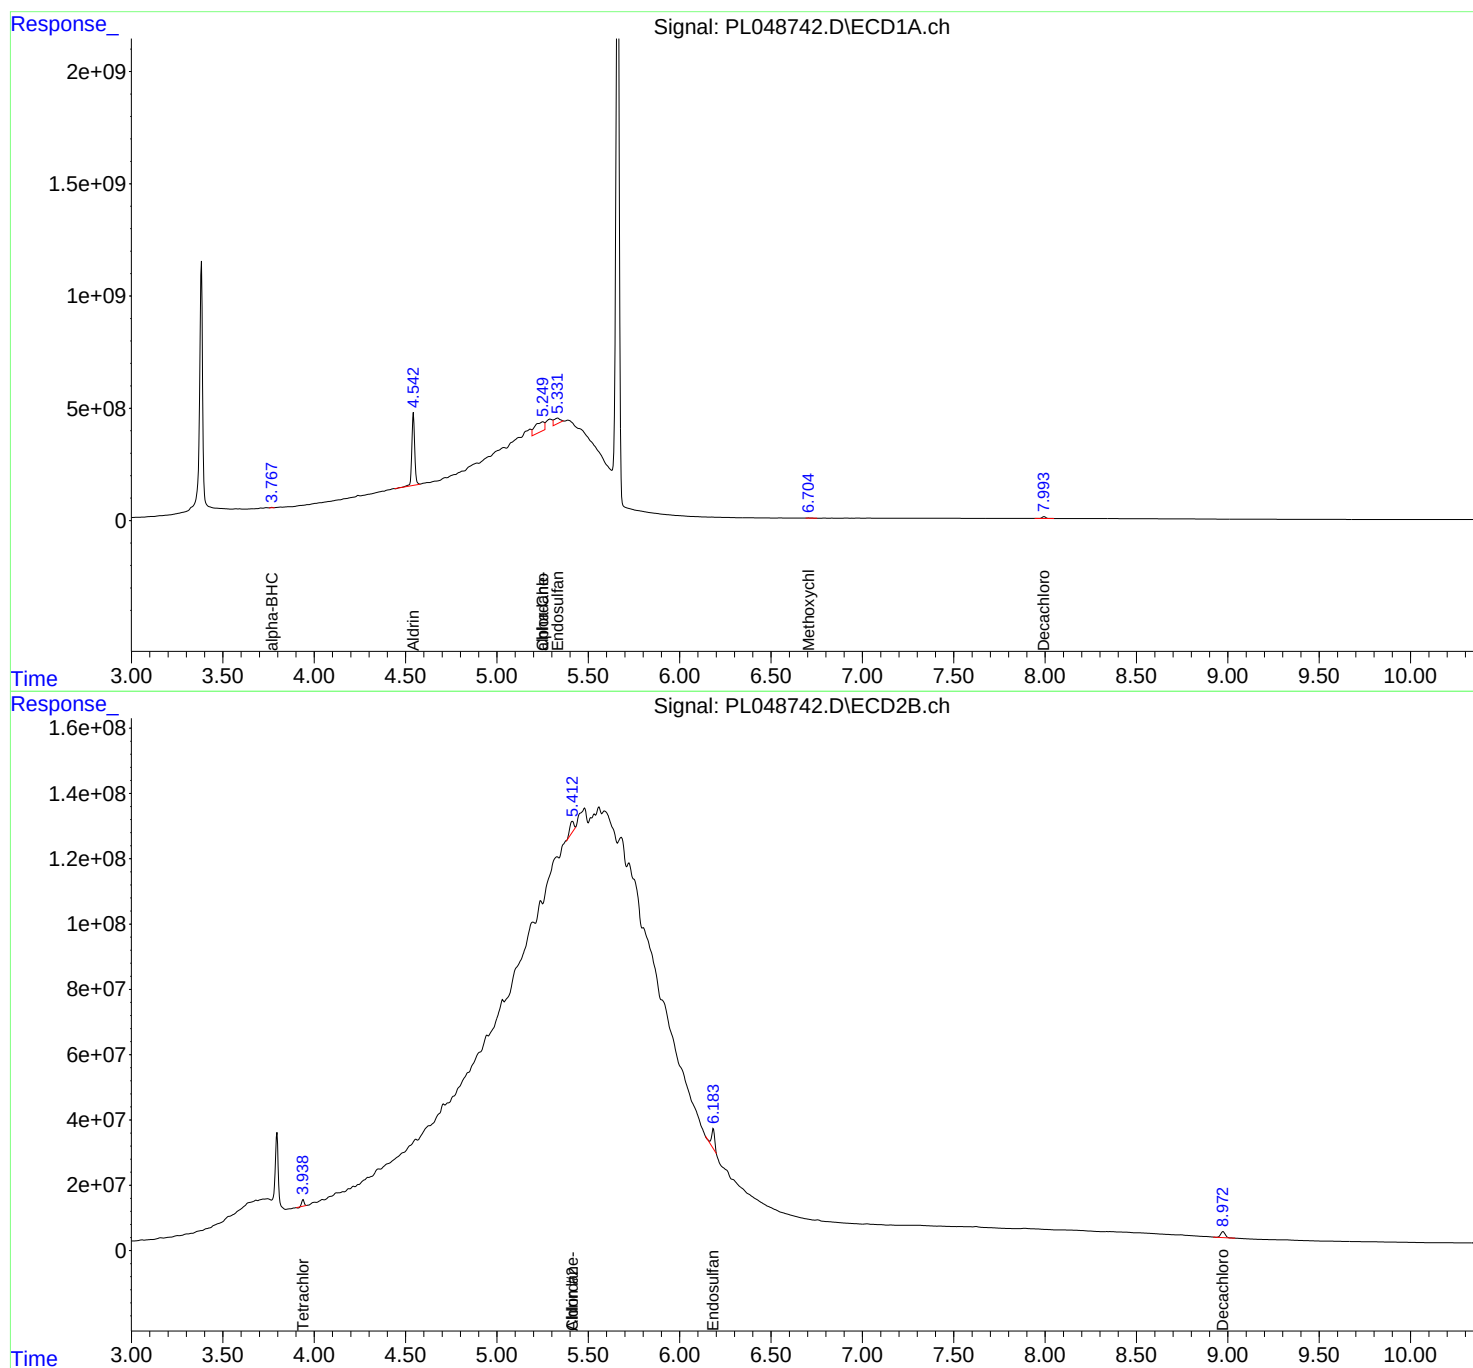


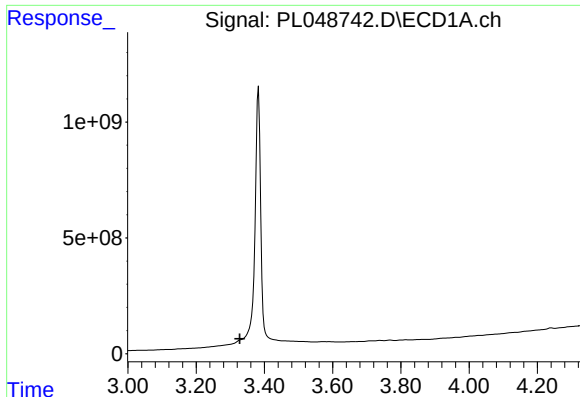

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-17-S

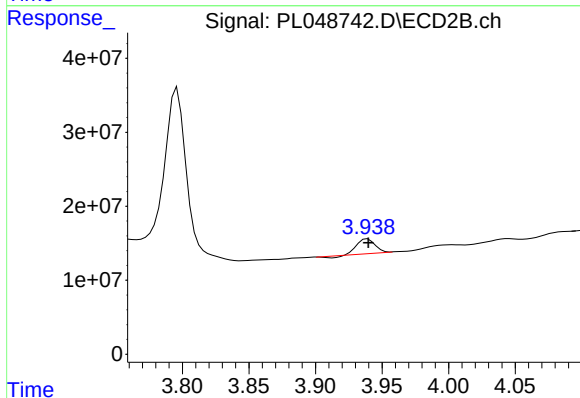


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 17375400
Conc: 6.98 ng/ml

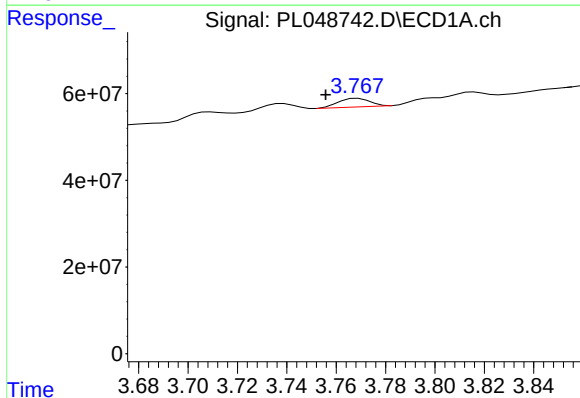


#2 alpha-BHC

R.T.: 3.769 min
Delta R.T.: 0.013 min
Response: 17598762
Conc: 1.14 ng/ml

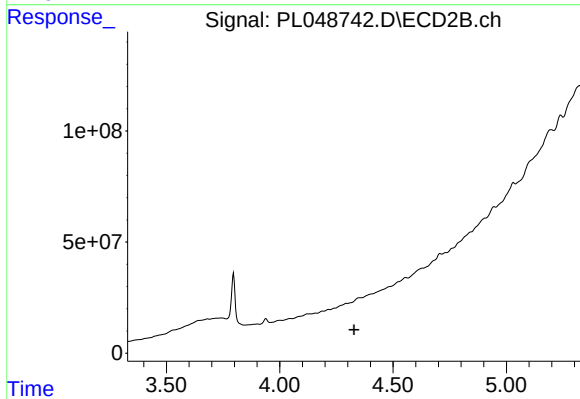

#2 alpha-BHC


R.T.: 4.354 min
Delta R.T.: 0.026 min
Response: -688624
Conc: N.D.

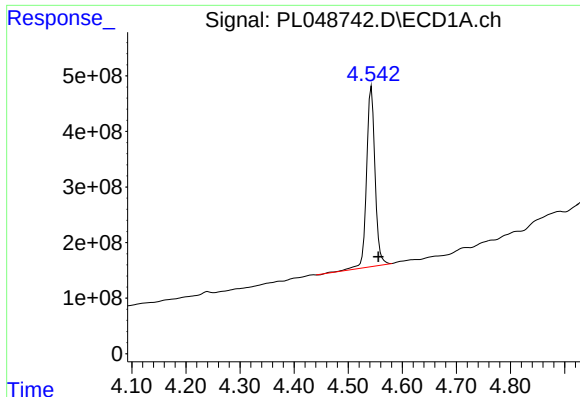

#5 Aldrin


R.T.: 4.543 min
Delta R.T.: -0.013 min
Response: 3511455613
Conc: 256.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-17-S

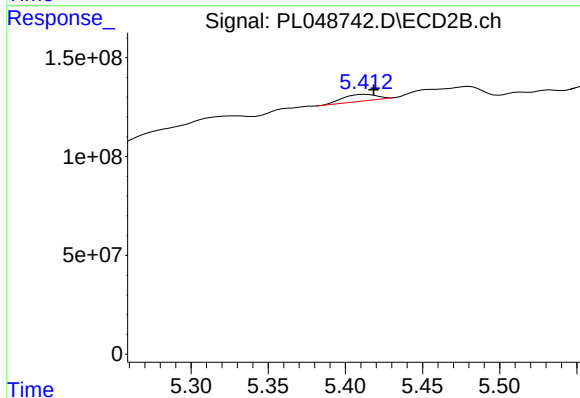


#5 Aldrin

R.T.: 5.413 min
Delta R.T.: -0.005 min
Response: 51012927
Conc: 16.47 ng/ml

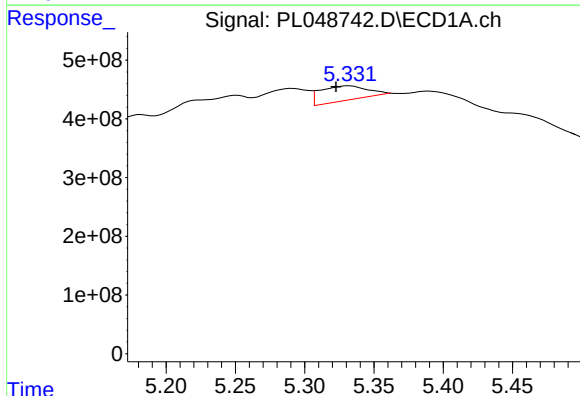


#9 Endosulfan I

R.T.: 5.332 min
Delta R.T.: 0.010 min
Response: 684484416
Conc: 56.90 ng/ml

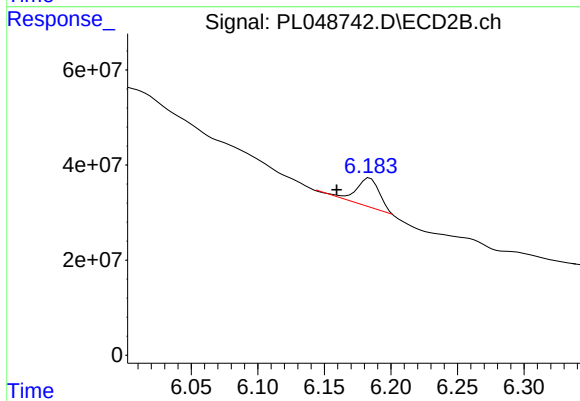

#9 Endosulfan I


R.T.: 6.184 min
Delta R.T.: 0.025 min
Response: 69838127
Conc: 24.70 ng/ml

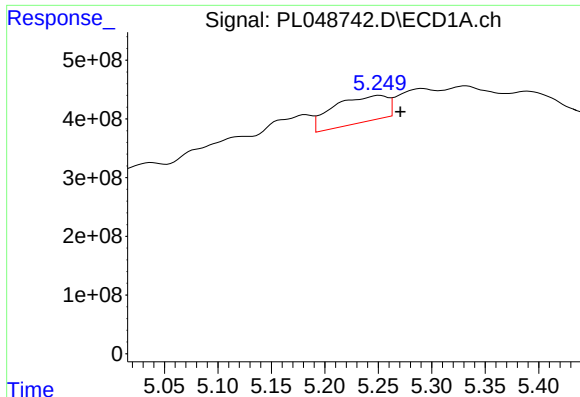

#11 alpha-Chlordane


R.T.: 5.251 min
Delta R.T.: -0.020 min
Response: 1581255808
Conc: 120.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-17-S

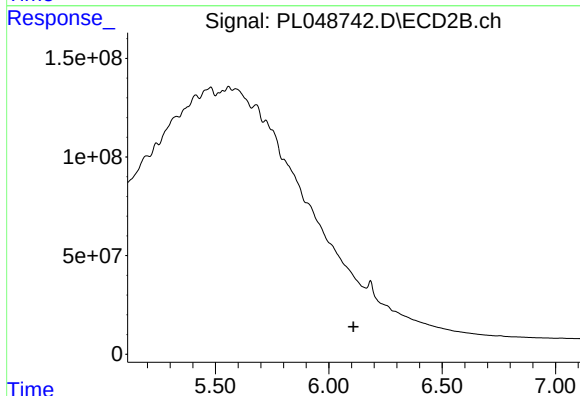


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.109 min
Response: 0
Conc: N.D.

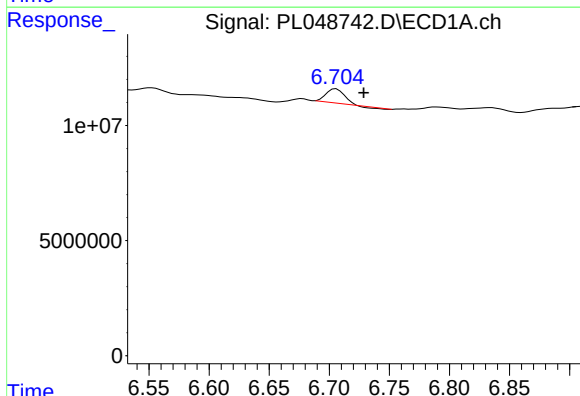


#20 Methoxychlor

R.T.: 6.706 min
Delta R.T.: -0.023 min
Response: 6211821
Conc: 1.14 ng/ml

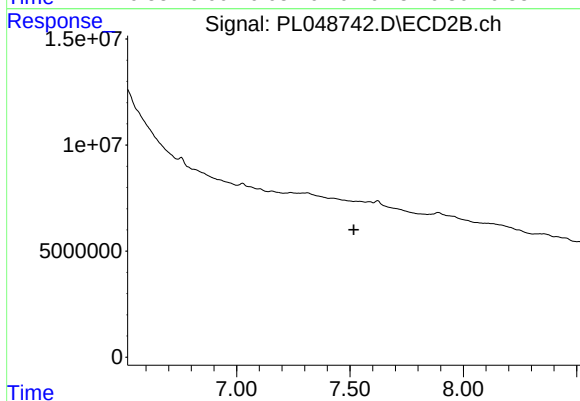

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.516 min
Response: 0
Conc: N.D.

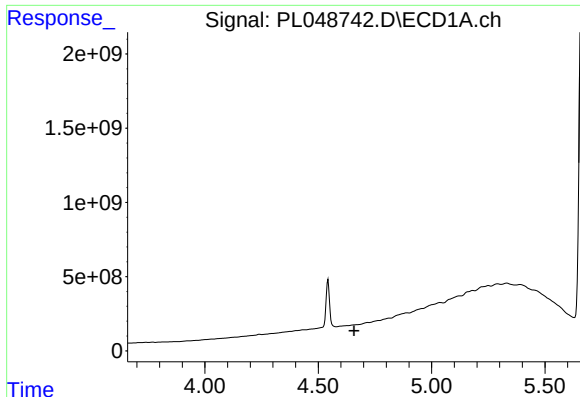

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.658 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-17-S

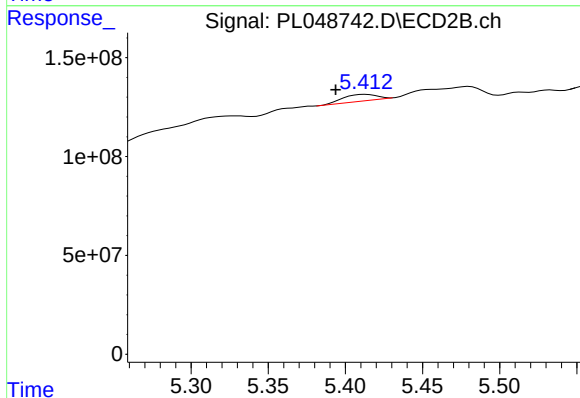


#24 Chlordane-2

R.T.: 5.413 min
Delta R.T.: 0.020 min
Response: 51012927
Conc: 394.41 ng/ml

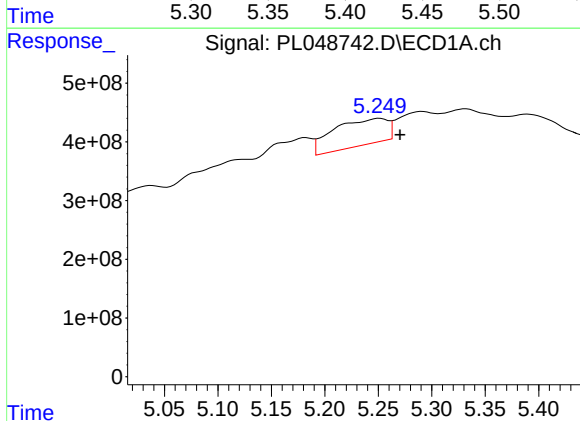


#26 Chlordane-4

R.T.: 5.251 min
Delta R.T.: -0.019 min
Response: 1581255808
Conc: 1089.15 ng/ml

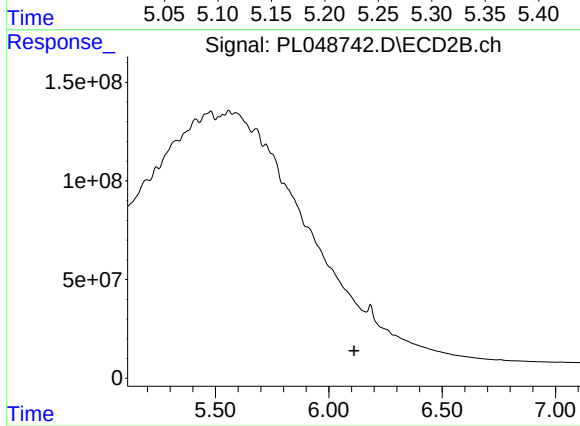

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 6.111 min
Response: 0
Conc: N.D.

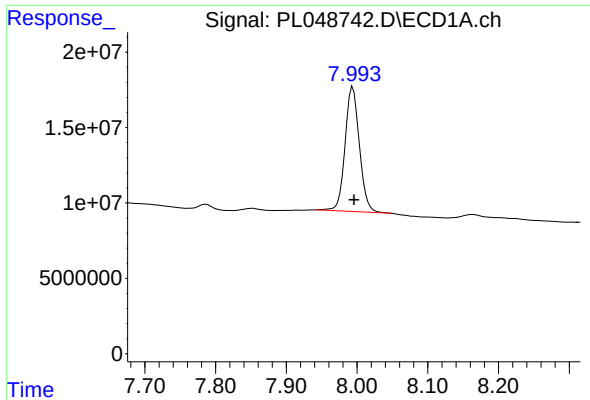

#28 Decachlorobiphenyl

R.T.: 7.994 min
Delta R.T.: -0.002 min
Response: 116587040
Conc: 11.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-17-S

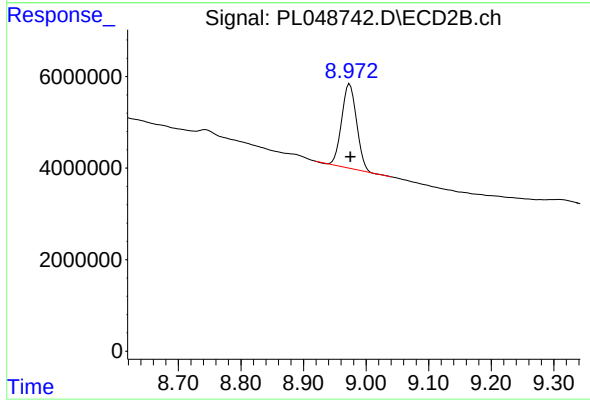

#28 Decachlorobiphenyl

R.T.: 8.974 min
Delta R.T.: -0.001 min
Response: 30446287
Conc: 11.47 ng/ml