

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051919\
 Data File : PL048750.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2019 19:53
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Ankita
 5/20/2019 1:58:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 04:56:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.325	3.939	152.2E6	42553678	15.707m	17.084
28)	SA Decachlor...	7.994	8.974	168.1E6	47969239	16.722	18.072

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051919\
Data File : PL048750.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2019 19:53
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
5/20/2019 1:58:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 04:56:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

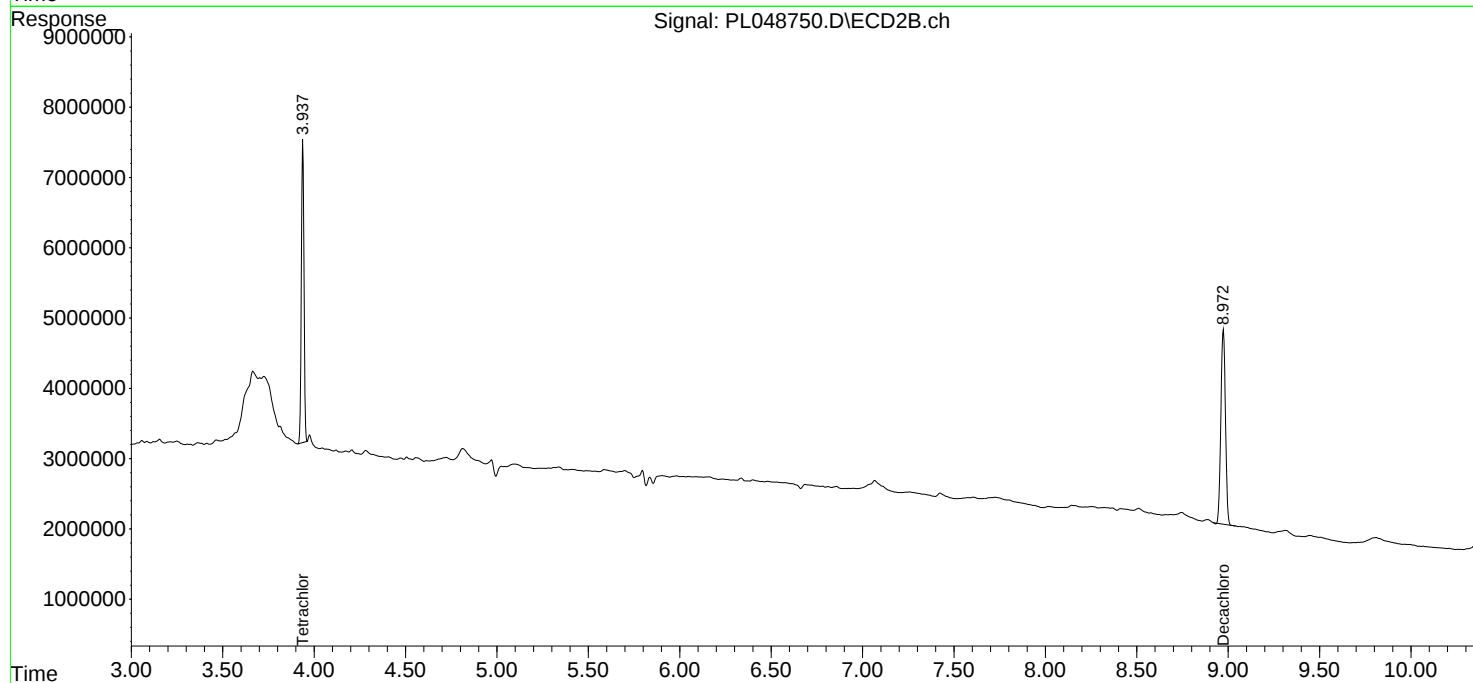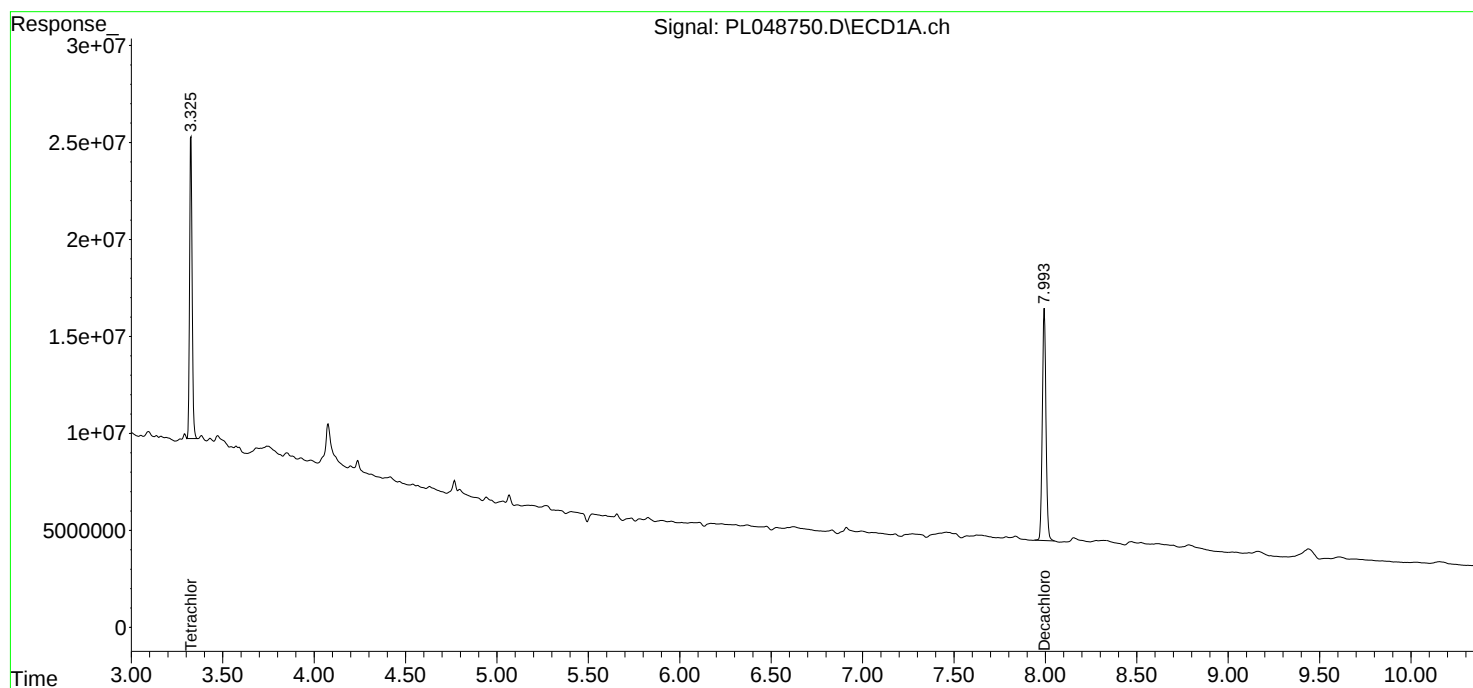

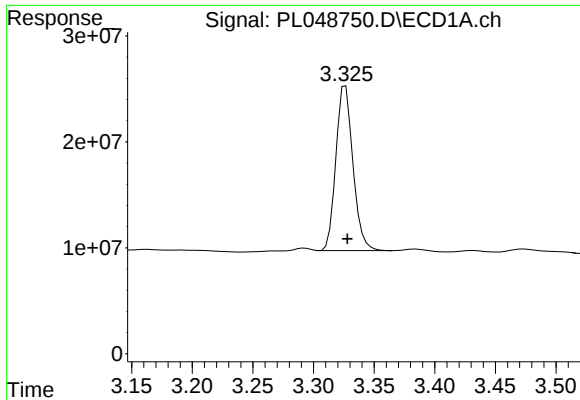

#1 Tetrachloro-m-xylene

R.T.: 3.325 min

Delta R.T.: -0.003 min


Response: 152150192

Conc: 15.71 ng/ml m

Instrument :
ECD_L
ClientSampleId :
I.BLK

Manual Integrations
APPROVED

Ankita
5/20/2019 1:58:43 PM

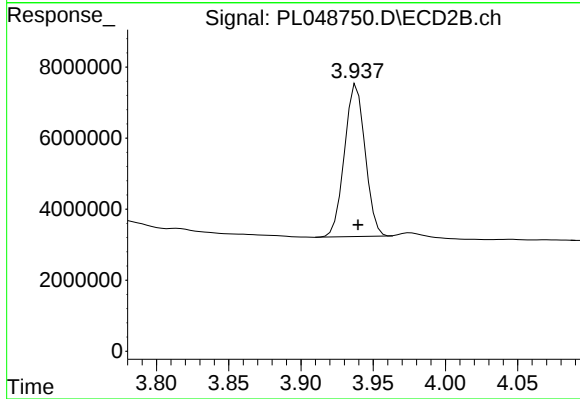


#1 Tetrachloro-m-xylene

R.T.: 3.939 min

Delta R.T.: -0.001 min

Response: 42553678

Conc: 17.08 ng/ml

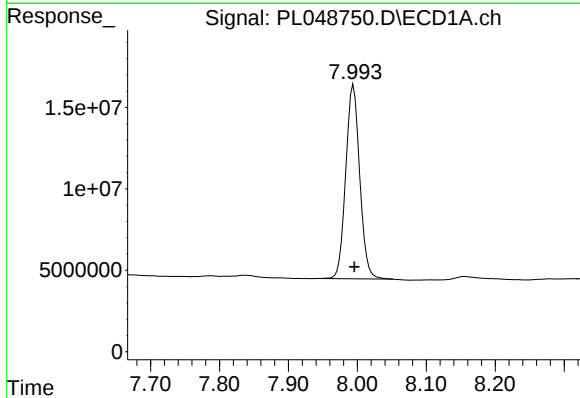


#28 Decachlorobiphenyl

R.T.: 7.994 min

Delta R.T.: -0.001 min

Response: 168126700

Conc: 16.72 ng/ml

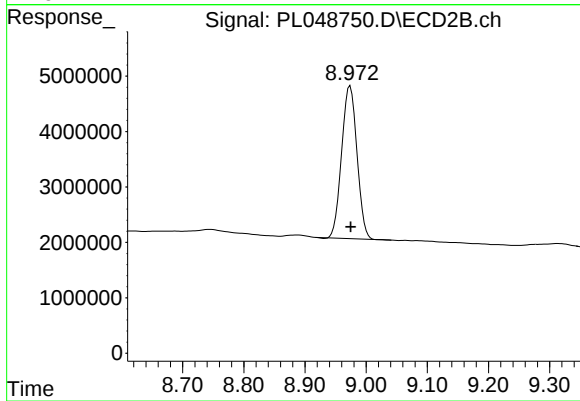

#28 Decachlorobiphenyl

R.T.: 8.974 min

Delta R.T.: -0.001 min

Response: 47969239

Conc: 18.07 ng/ml