

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051922\
 Data File : PL074833.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2022 09:47
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 18:51:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.646	4.650	12813064	34441573	25.236	25.094
28)	SA Decachlor...	11.647	10.404	12709030	32003202	28.458	31.180
Target Compounds							
2)	A alpha-BHC	6.230	5.353	8035038	21162049	11.745	12.575
3)	MA gamma-BHC...	6.628	5.774	7880296	21377190	12.208	12.937
5)	MB Aldrin	0.000	6.532f	0	153558	N.D.	0.102 #
6)	B beta-BHC	6.880	6.151	4070977	12075074	13.640	15.208
8)	B Heptachlo...	8.129	0.000	1455023	0	2.558	N.D. #
9)	A Endosulfan I	8.506f	0.000	5455443	0	9.463	N.D. #
11)	B alpha-Chl...	8.506f	0.000	5455443	0	8.936	N.D. #
12)	B 4,4'-DDE	0.000	7.640	0	422434	N.D.	0.359 #
13)	MA Dieldrin	0.000	7.774	0	2289625	N.D.	1.797 #
14)	MA Endrin	9.065	8.060	28506773	76223132	69.080	72.160
15)	B Endosulfa...	0.000	8.396f	0	302249	N.D.	0.268 #
16)	A 4,4'-DDD	9.204	8.224	1601965	4247984	3.543	4.312
17)	MA 4,4'-DDT	9.524	8.486	57571260	146.3E6	125.255	146.223
18)	B Endrin al...	9.434	8.560	887016	1558750	2.506	1.952
20)	A Methoxychlor	10.010	9.080	76770839	190.4E6	313.462	325.762
21)	B Endrin ke...	10.175	9.307	1500961	2559303	2.927	2.296
26)	Chlordane-4	8.506f	0.000	5455443	0	56.627	N.D. #
27)	Chlordane-5	0.000	8.140	0	182895	N.D.	4.947 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051922\
Data File : PL074833.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2022 09:47
Operator : AR\AJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 18:51:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

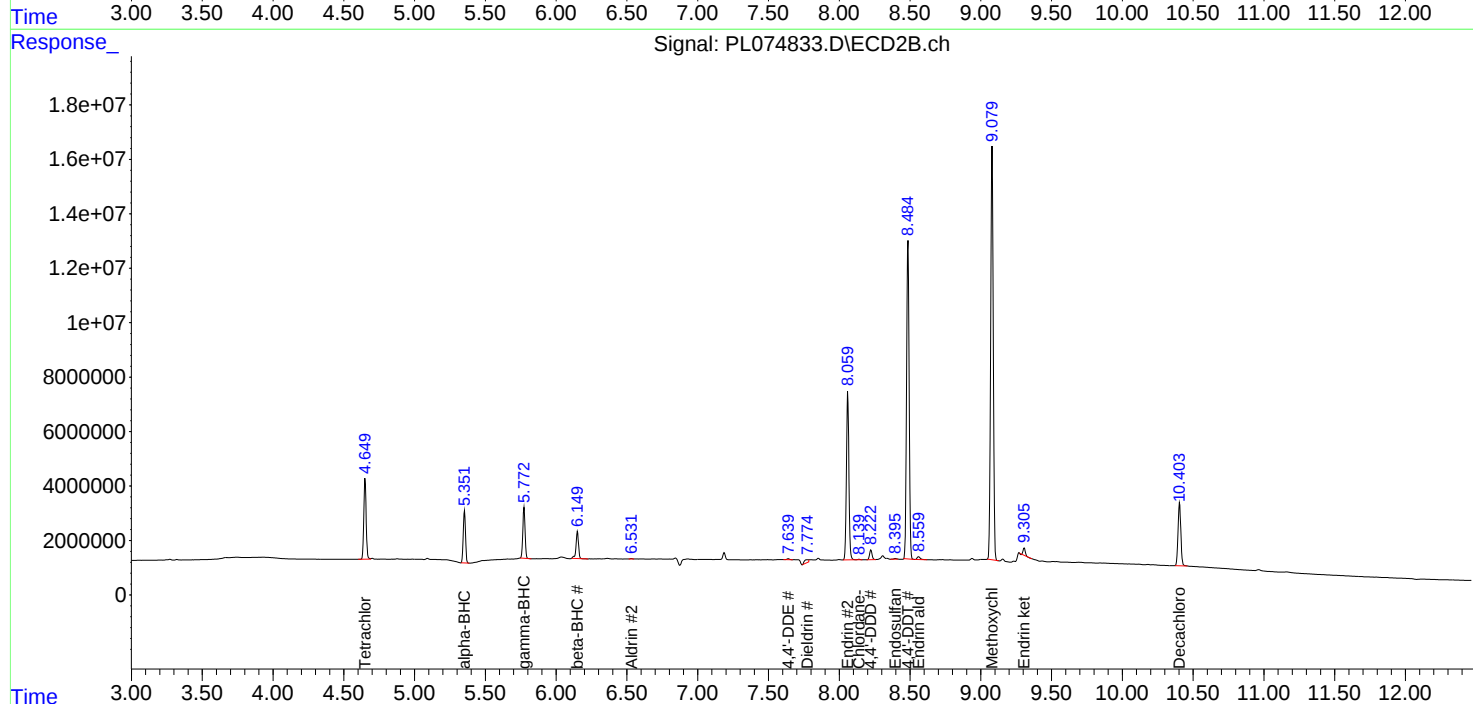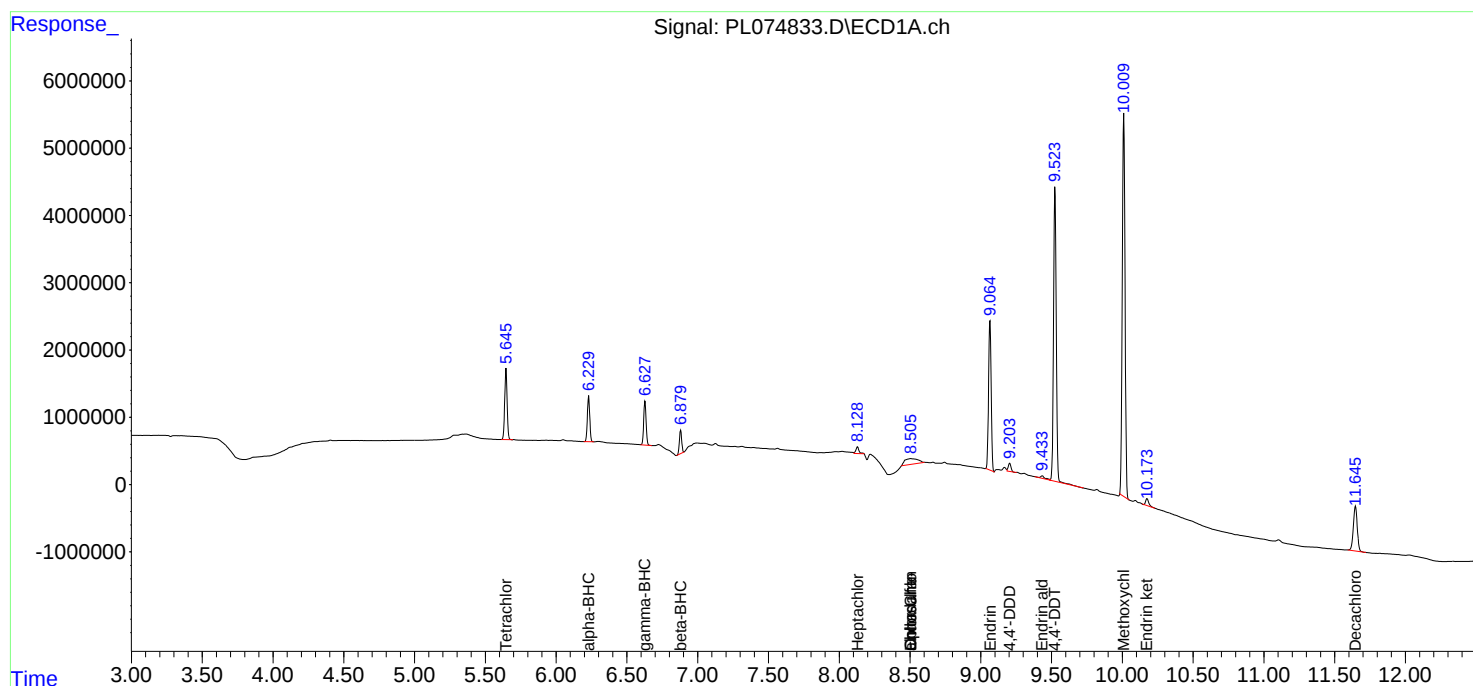


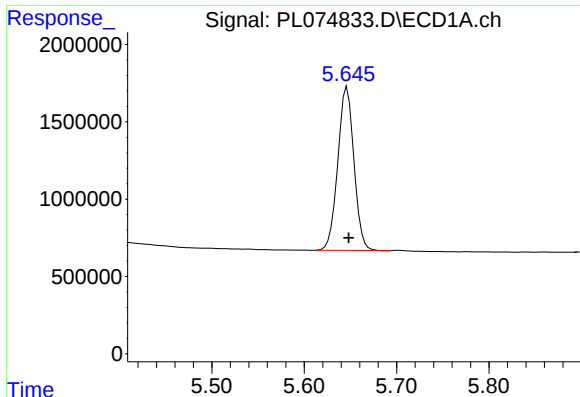

#1 Tetrachloro-m-xylene


R.T.: 5.646 min
Delta R.T.: -0.002 min
Response: 12813064
Conc: 25.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

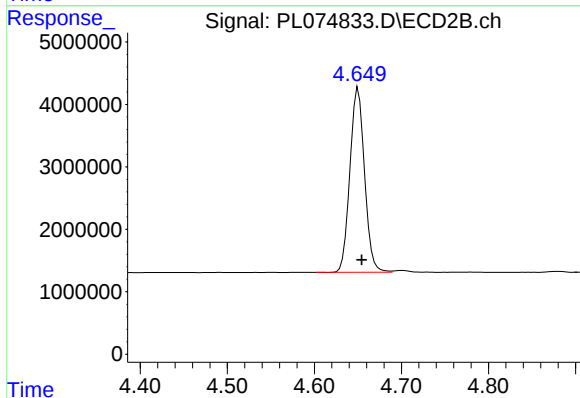


#1 Tetrachloro-m-xylene

R.T.: 4.650 min
Delta R.T.: -0.004 min
Response: 34441573
Conc: 25.09 ng/ml

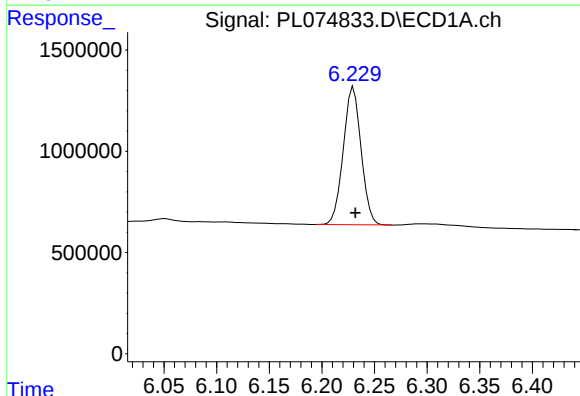


#2 alpha-BHC

R.T.: 6.230 min
Delta R.T.: -0.002 min
Response: 8035038
Conc: 11.74 ng/ml

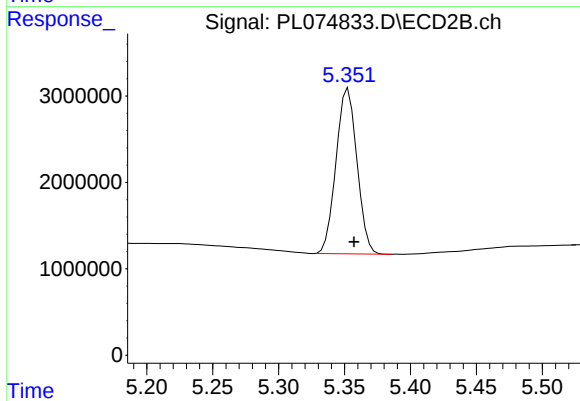

#2 alpha-BHC


R.T.: 5.353 min
Delta R.T.: -0.004 min
Response: 21162049
Conc: 12.57 ng/ml

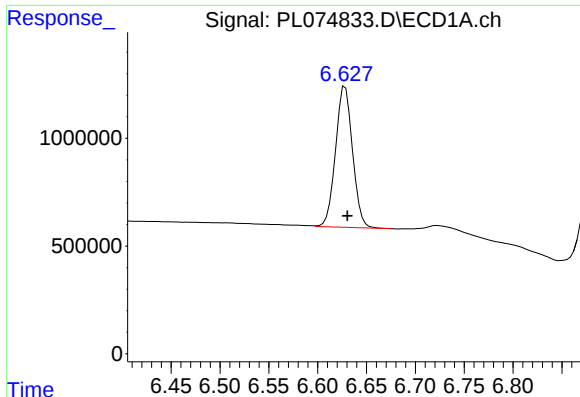

#3 gamma-BHC (Lindane)


R.T.: 6.628 min
Delta R.T.: -0.002 min
Response: 7880296
Conc: 12.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

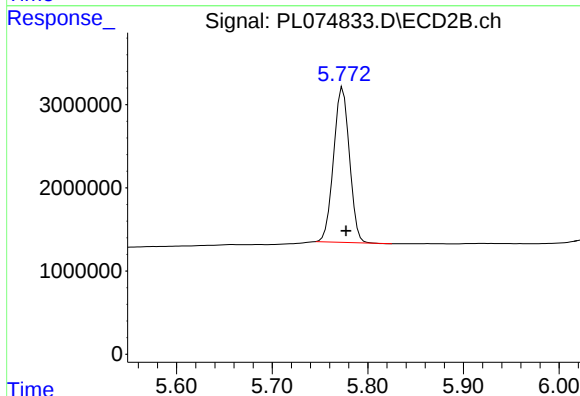


#3 gamma-BHC (Lindane)

R.T.: 5.774 min
Delta R.T.: -0.004 min
Response: 21377190
Conc: 12.94 ng/ml

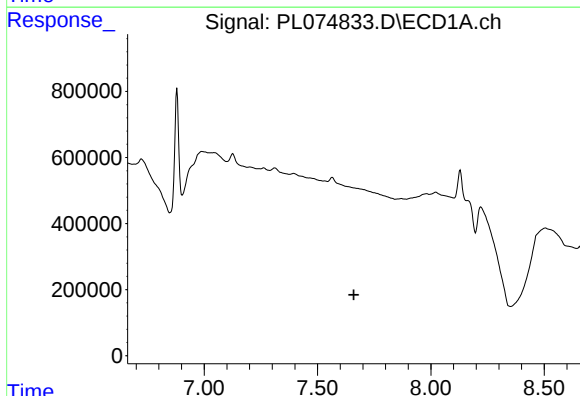


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.660 min
Response: 0
Conc: N.D.

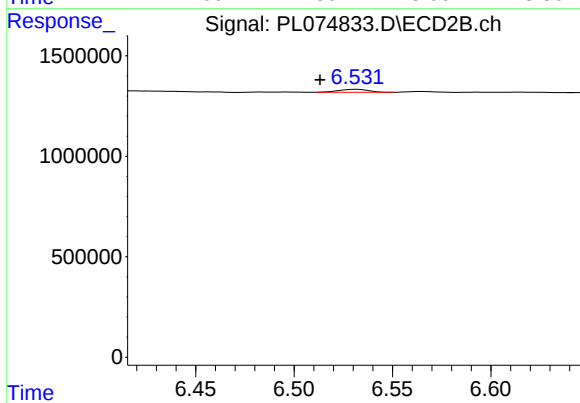

#5 Aldrin


R.T.: 6.532 min
Delta R.T.: 0.019 min
Response: 153558
Conc: 0.10 ng/ml

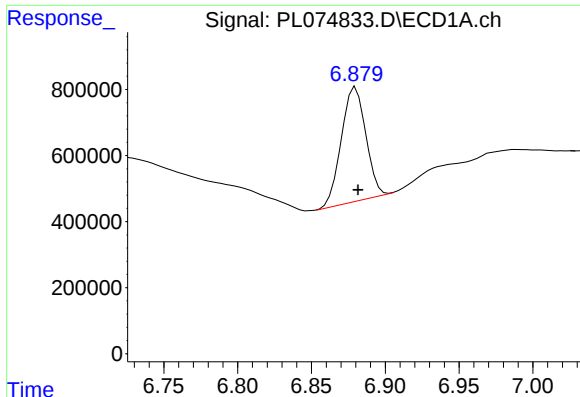

#6 beta-BHC


R.T.: 6.880 min
Delta R.T.: -0.002 min
Response: 4070977
Conc: 13.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

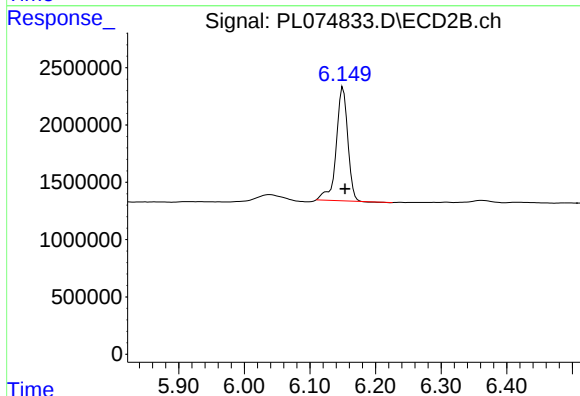


#6 beta-BHC

R.T.: 6.151 min
Delta R.T.: -0.003 min
Response: 12075074
Conc: 15.21 ng/ml

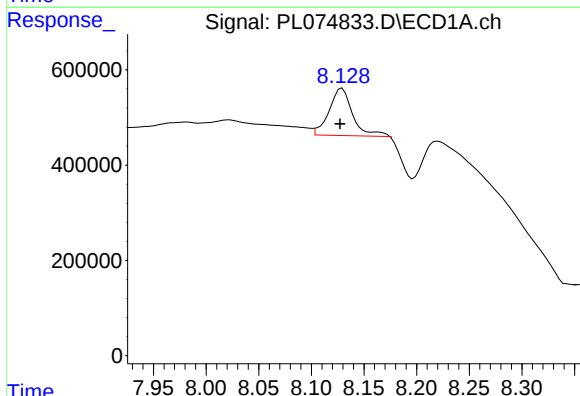


#8 Heptachlor epoxide

R.T.: 8.129 min
Delta R.T.: 0.002 min
Response: 1455023
Conc: 2.56 ng/ml

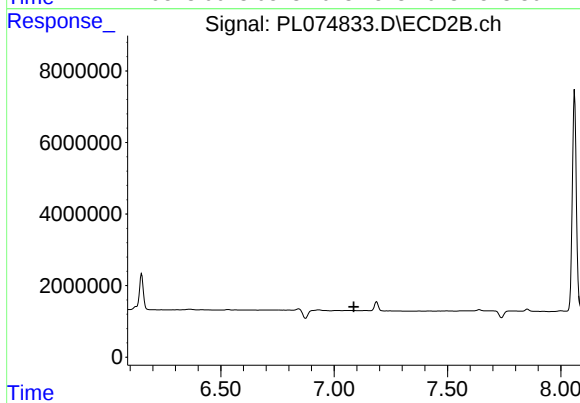

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 7.087 min
Response: 0
Conc: N.D.

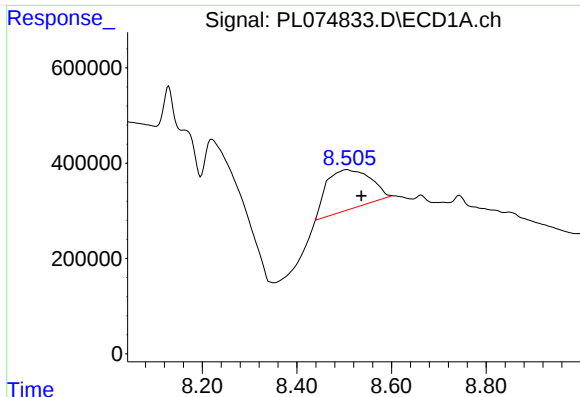

#9 Endosulfan I


R.T.: 8.506 min
Delta R.T.: -0.030 min
Response: 5455443
Conc: 9.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

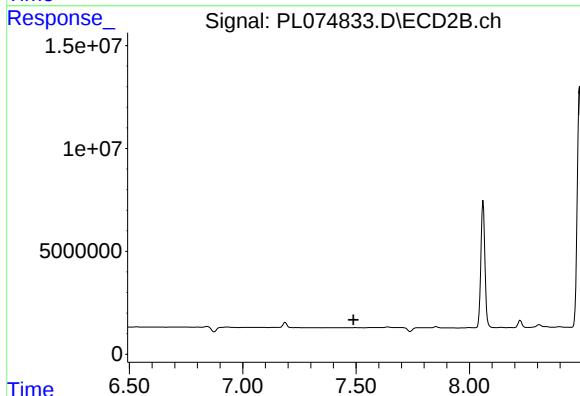


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.489 min
Response: 0
Conc: N.D.

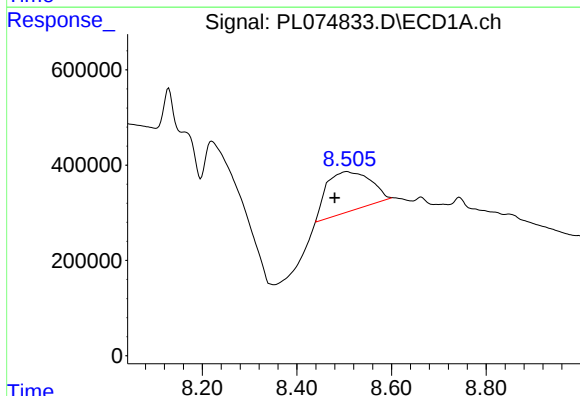


#11 alpha-Chlordane

R.T.: 8.506 min
Delta R.T.: 0.026 min
Response: 5455443
Conc: 8.94 ng/ml

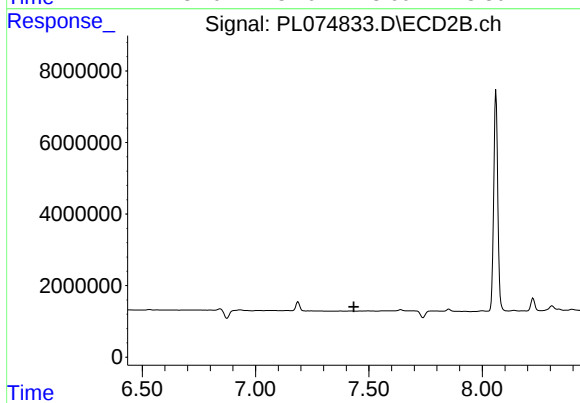

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.433 min
Response: 0
Conc: N.D.

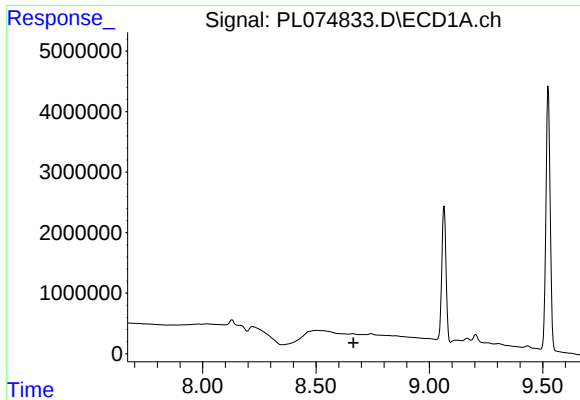

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 8.665 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

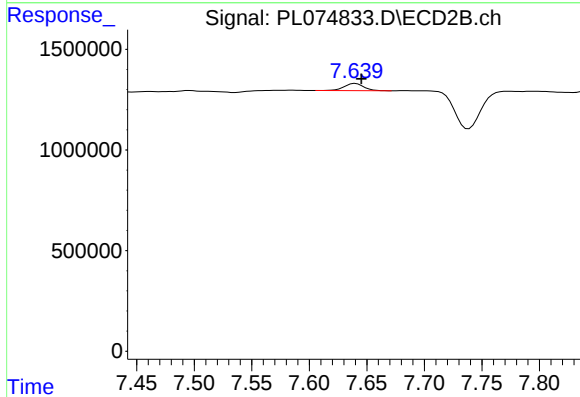


#12 4,4'-DDE

R.T.: 7.640 min
Delta R.T.: -0.005 min
Response: 422434
Conc: 0.36 ng/ml

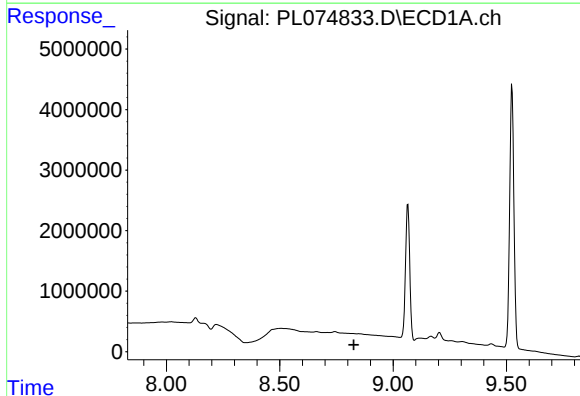


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 8.827 min
Response: 0
Conc: N.D.

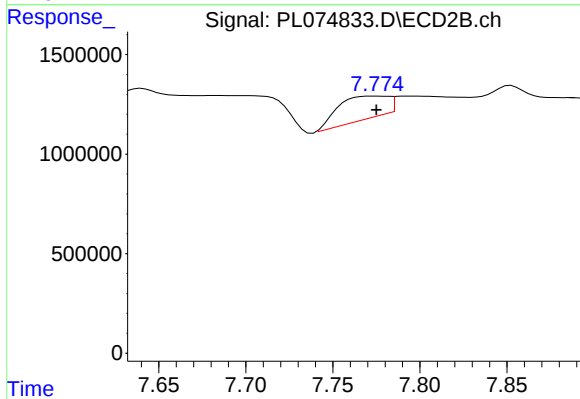

#13 Dieldrin


R.T.: 7.774 min
Delta R.T.: -0.001 min
Response: 2289625
Conc: 1.80 ng/ml

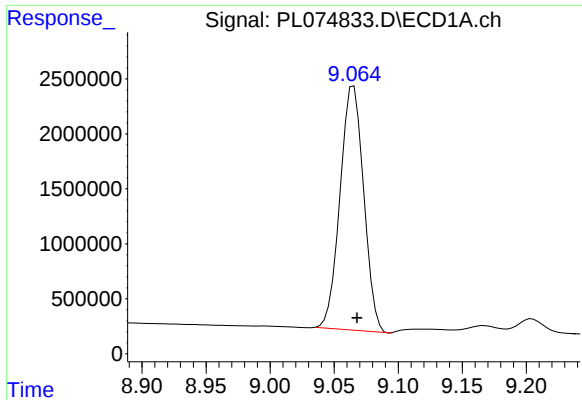

#14 Endrin


R.T.: 9.065 min
Delta R.T.: -0.003 min
Response: 28506773
Conc: 69.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

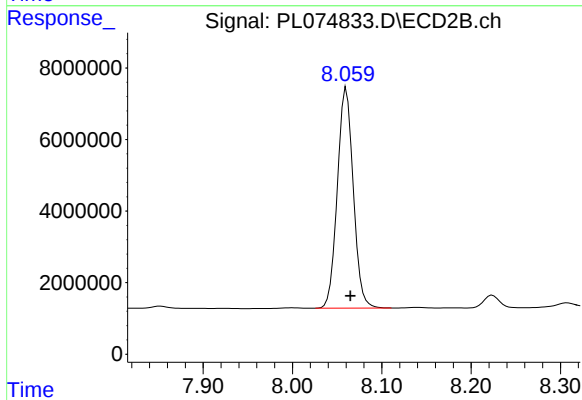


#14 Endrin

R.T.: 8.060 min
Delta R.T.: -0.004 min
Response: 76223132
Conc: 72.16 ng/ml

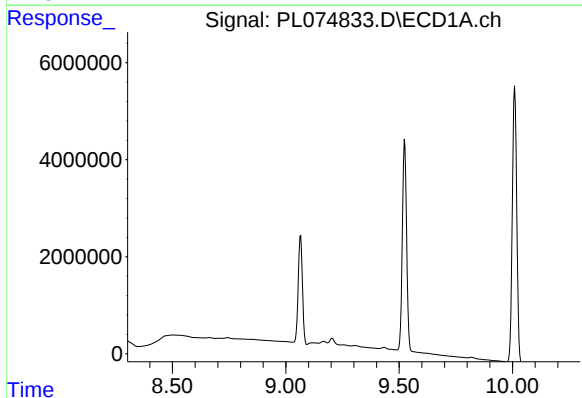


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 9.302 min
Response: 0
Conc: N.D.

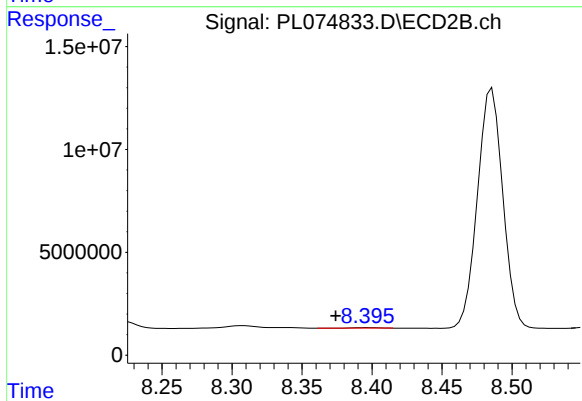

#15 Endosulfan II


R.T.: 8.396 min
Delta R.T.: 0.022 min
Response: 302249
Conc: 0.27 ng/ml

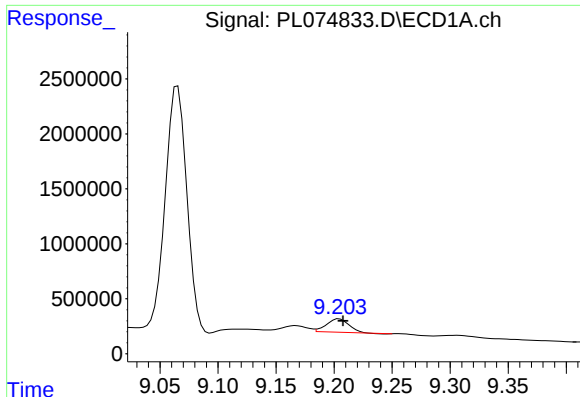

#16 4,4'-DDD


R.T.: 9.204 min
Delta R.T.: -0.003 min
Response: 1601965
Conc: 3.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

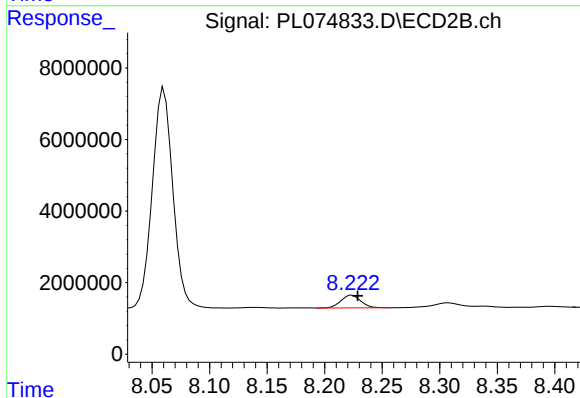


#16 4,4'-DDD

R.T.: 8.224 min
Delta R.T.: -0.005 min
Response: 4247984
Conc: 4.31 ng/ml

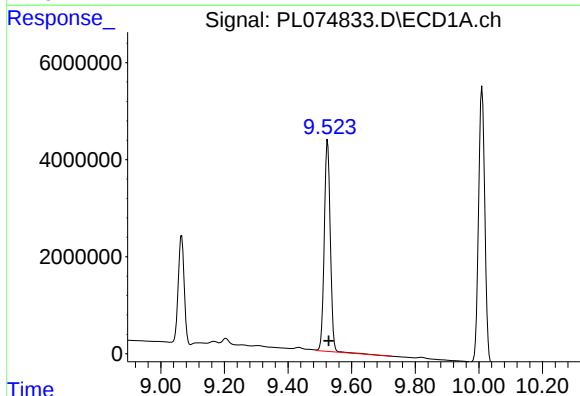


#17 4,4'-DDT

R.T.: 9.524 min
Delta R.T.: -0.003 min
Response: 57571260
Conc: 125.26 ng/ml

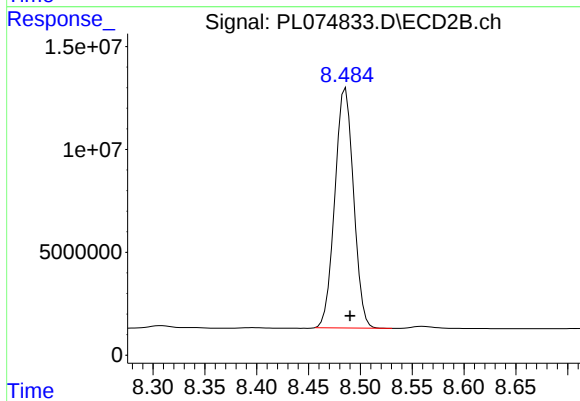

#17 4,4'-DDT


R.T.: 8.486 min
Delta R.T.: -0.004 min
Response: 146298388
Conc: 146.22 ng/ml

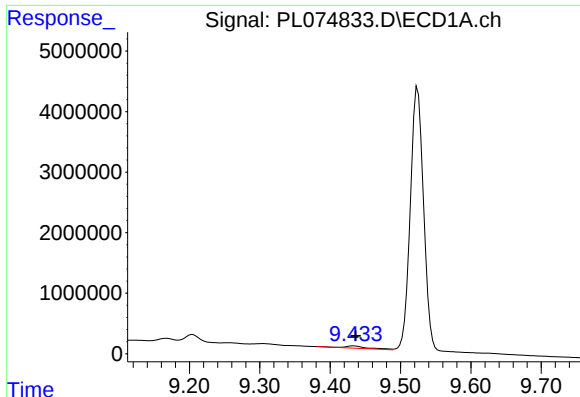

#18 Endrin aldehyde


R.T.: 9.434 min
Delta R.T.: -0.002 min
Response: 887016
Conc: 2.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

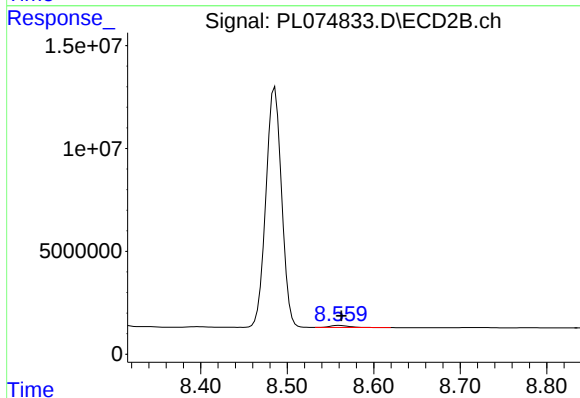


#18 Endrin aldehyde

R.T.: 8.560 min
Delta R.T.: -0.002 min
Response: 1558750
Conc: 1.95 ng/ml

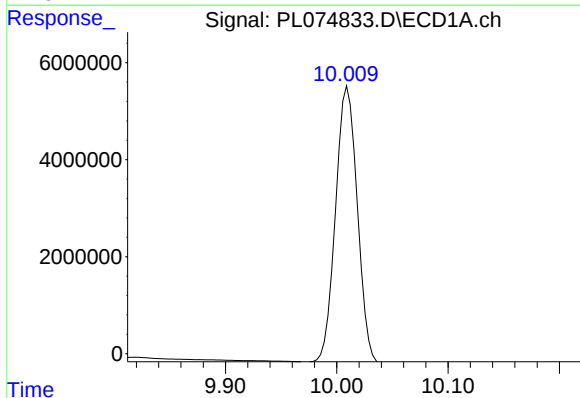


#20 Methoxychlor

R.T.: 10.010 min
Delta R.T.: -0.003 min
Response: 76770839
Conc: 313.46 ng/ml

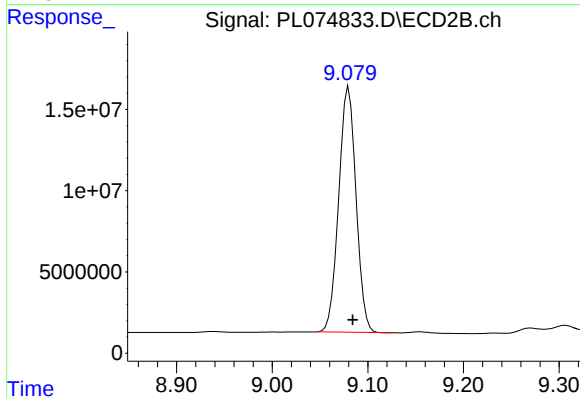

#20 Methoxychlor


R.T.: 9.080 min
Delta R.T.: -0.004 min
Response: 190373028
Conc: 325.76 ng/ml

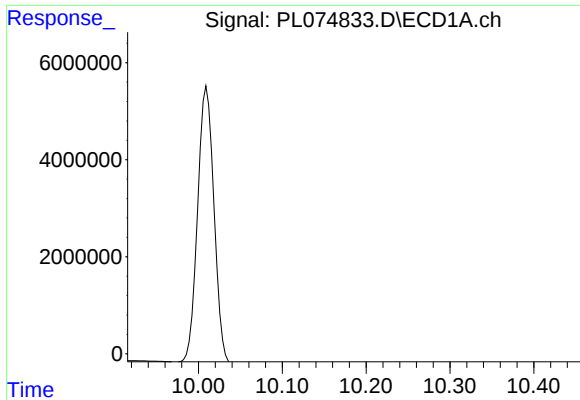

#21 Endrin ketone


R.T.: 10.175 min
Delta R.T.: -0.002 min
Response: 1500961
Conc: 2.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

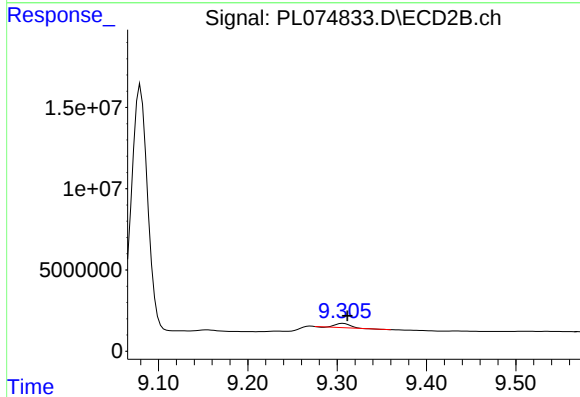


#21 Endrin ketone

R.T.: 9.307 min
Delta R.T.: -0.005 min
Response: 2559303
Conc: 2.30 ng/ml

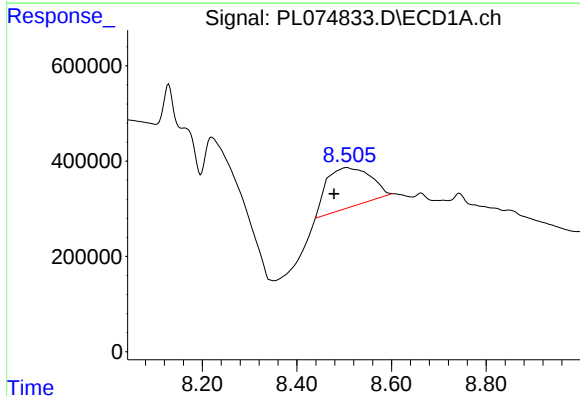


#26 Chlordane-4

R.T.: 8.506 min
Delta R.T.: 0.027 min
Response: 5455443
Conc: 56.63 ng/ml

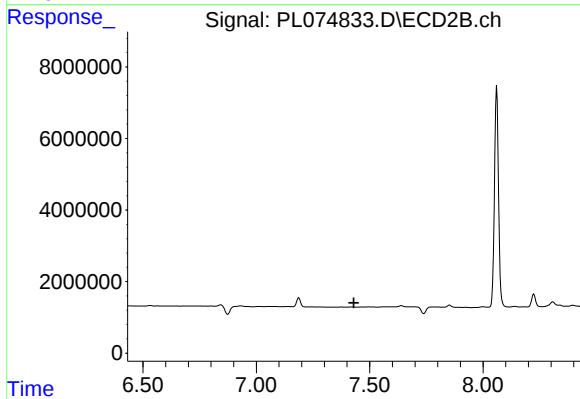

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 7.430 min
Response: 0
Conc: N.D.

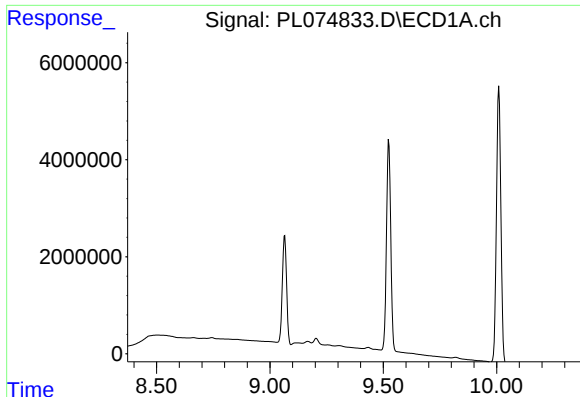

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.371 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

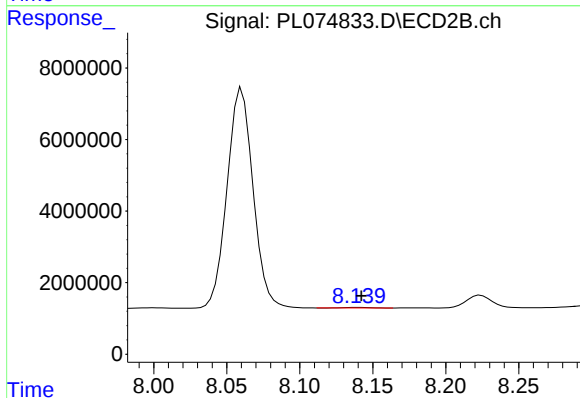


#27 Chlordane-5

R.T.: 8.140 min
Delta R.T.: -0.002 min
Response: 182895
Conc: 4.95 ng/ml

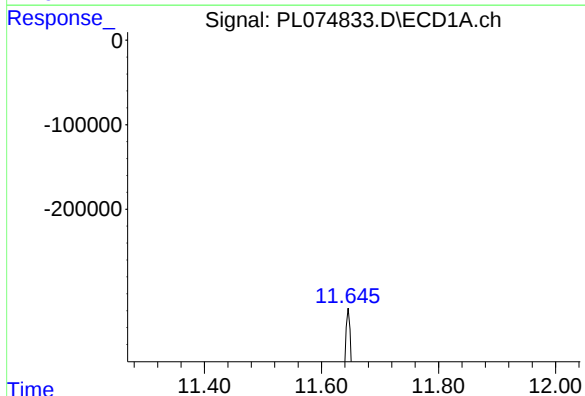

#28 Decachlorobiphenyl

R.T.: 11.647 min
Delta R.T.: -0.004 min
Response: 12709030
Conc: 28.46 ng/ml

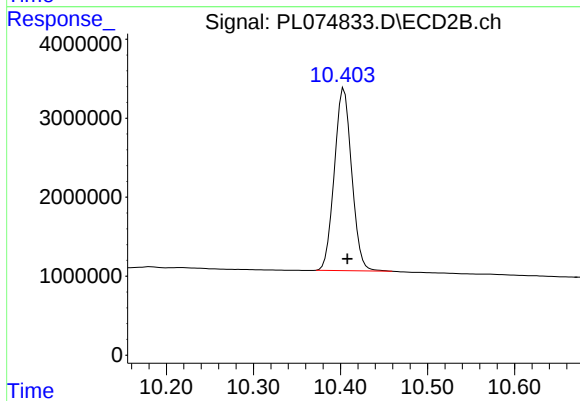

#28 Decachlorobiphenyl

R.T.: 10.404 min
Delta R.T.: -0.004 min
Response: 32003202
Conc: 31.18 ng/ml