

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051922\
 Data File : PL074844.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2022 15:54
 Operator : AR\AJ
 Sample : N2900-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 02:42:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.646	4.651	4364373	11519013	8.596	8.393
28)	SA Decachlor...	11.646	10.403	6653635	16388009	14.899	15.966
Target Compounds							
5)	MB Aldrin	7.669	6.509	752781	320302	1.215	0.213 #
8)	B Heptachlo...	8.152f	0.000	214670	0	0.377	N.D. #
9)	A Endosulfan I	8.521	7.482	2277529	392720	3.951	0.314 #
11)	B alpha-Chl...	8.509f	7.407f	2950133	711535	4.832	0.526 #
12)	B 4,4'-DDE	8.662	7.640	716049	2196903	1.547	1.867
14)	MA Endrin	0.000	8.081f	0	186034	N.D.	0.176 #
17)	MA 4,4'-DDT	0.000	8.484	0	323436	N.D.	0.323 #
26)	Chlordane-4	0.000	7.407f	0	711535	N.D.	5.190 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051922\
Data File : PL074844.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2022 15:54
Operator : AR\AJ
Sample : N2900-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 02:42:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

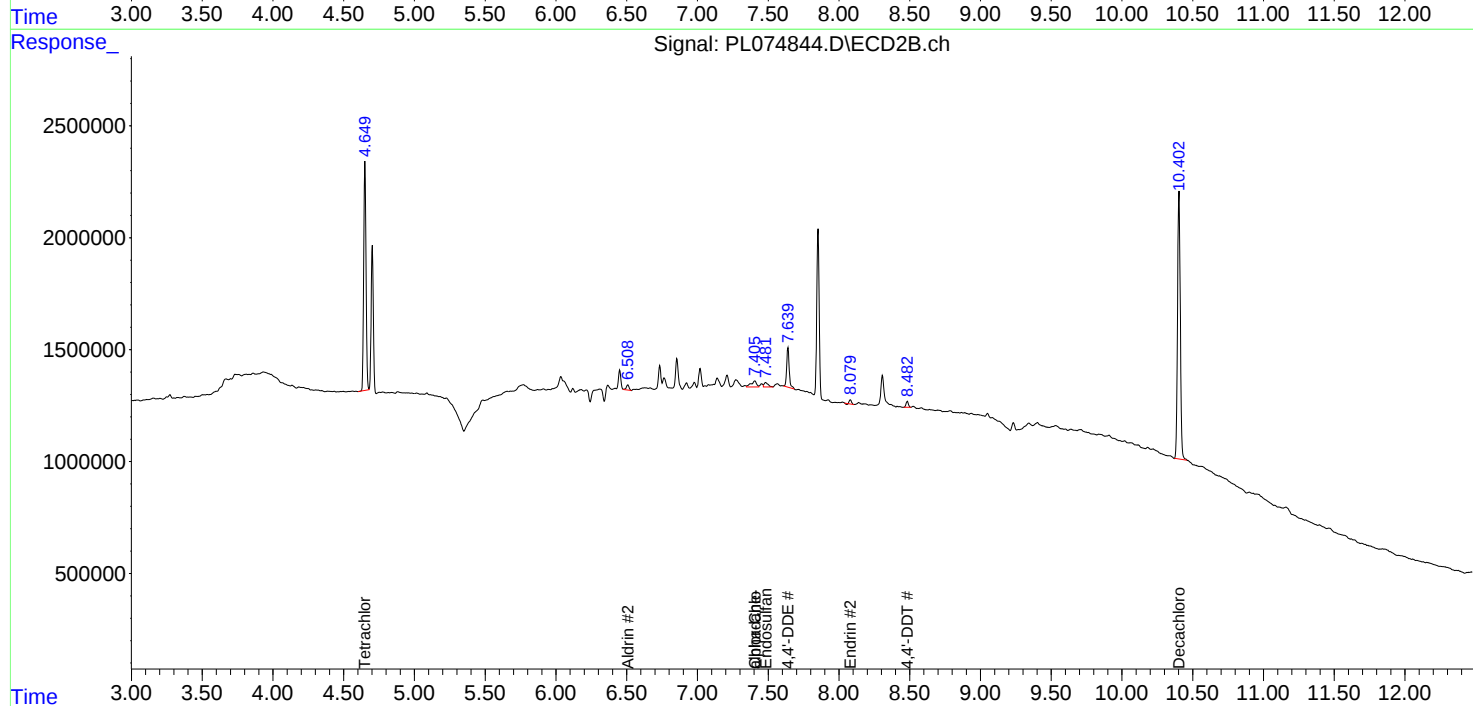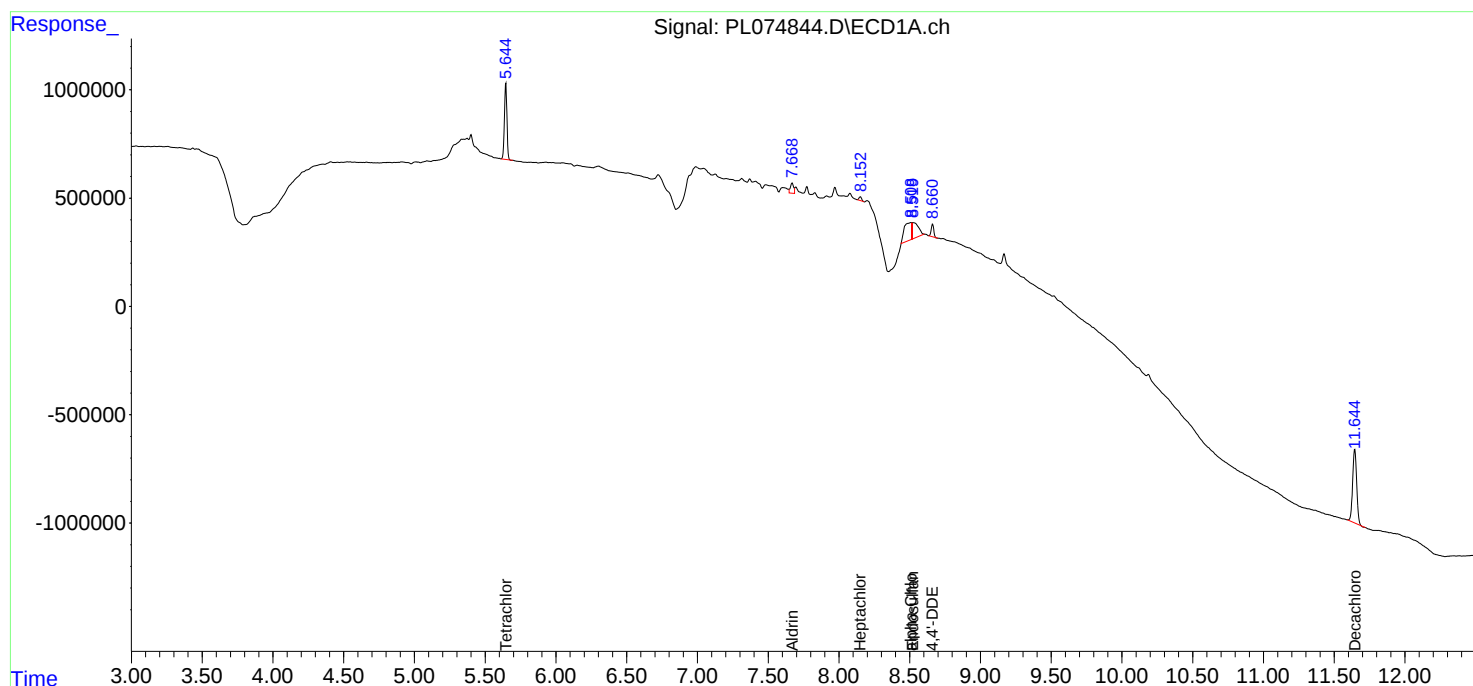


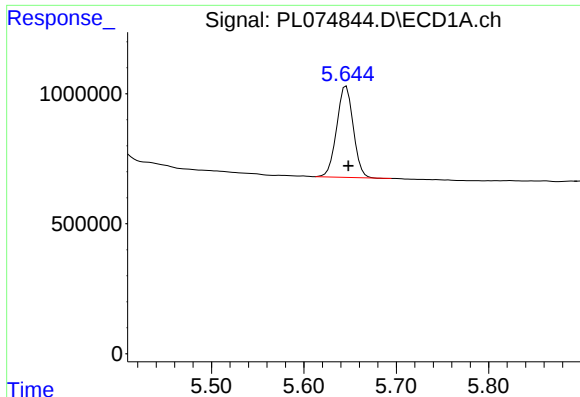

#1 Tetrachloro-m-xylene


R.T.: 5.646 min
Delta R.T.: -0.002 min
Response: 4364373
Conc: 8.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

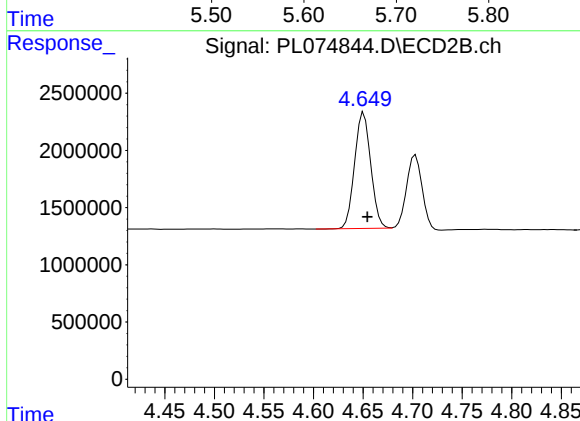


#1 Tetrachloro-m-xylene

R.T.: 4.651 min
Delta R.T.: -0.004 min
Response: 11519013
Conc: 8.39 ng/ml

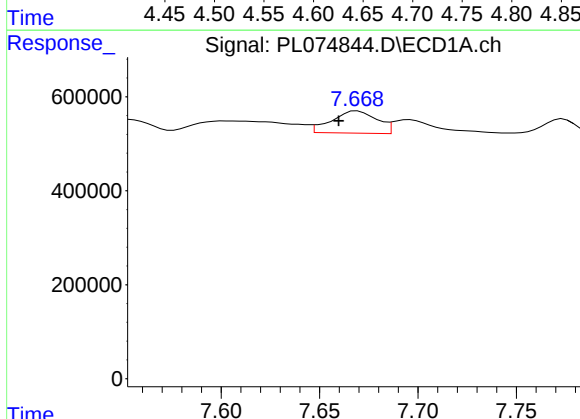


#5 Aldrin

R.T.: 7.669 min
Delta R.T.: 0.009 min
Response: 752781
Conc: 1.22 ng/ml

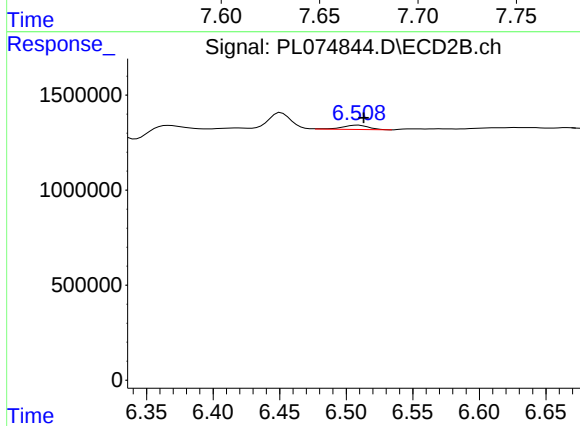

#5 Aldrin


R.T.: 6.509 min
Delta R.T.: -0.005 min
Response: 320302
Conc: 0.21 ng/ml

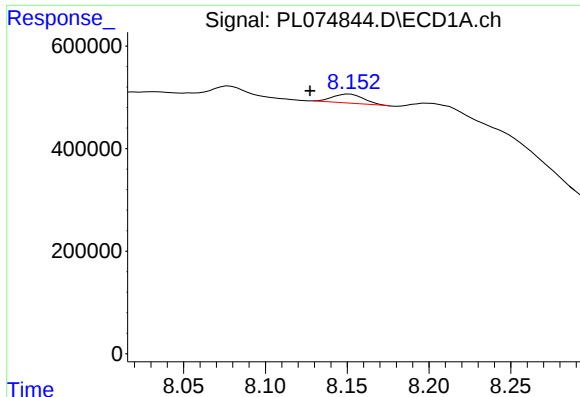

#8 Heptachlor epoxide


R.T.: 8.152 min
Delta R.T.: 0.024 min
Response: 214670
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

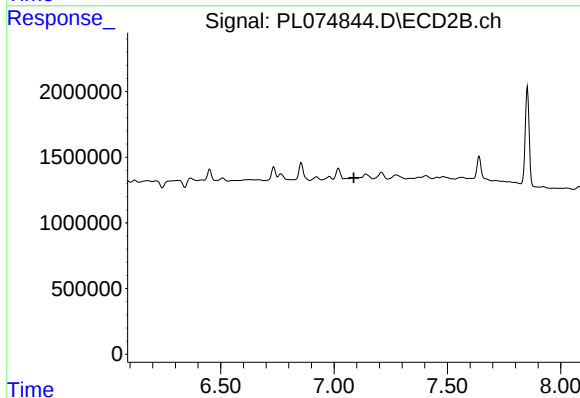


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.087 min
Response: 0
Conc: N.D.

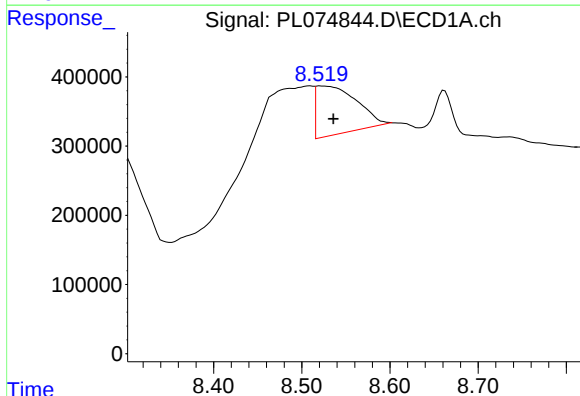


#9 Endosulfan I

R.T.: 8.521 min
Delta R.T.: -0.015 min
Response: 2277529
Conc: 3.95 ng/ml

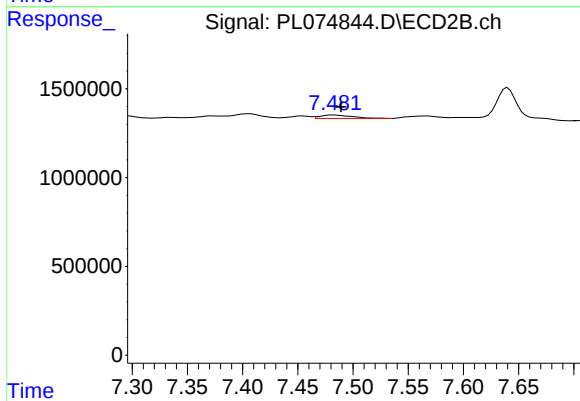

#9 Endosulfan I


R.T.: 7.482 min
Delta R.T.: -0.007 min
Response: 392720
Conc: 0.31 ng/ml

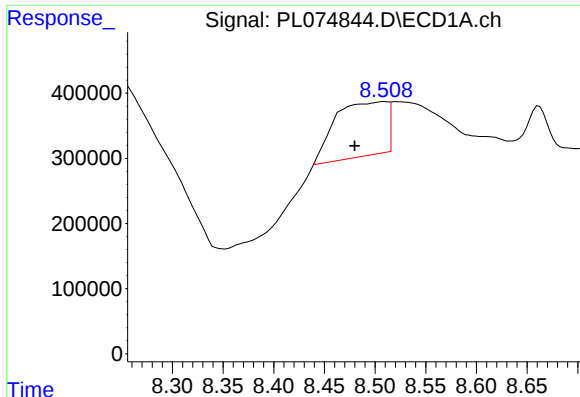

#11 alpha-Chlordane


R.T.: 8.509 min
Delta R.T.: 0.030 min
Response: 2950133
Conc: 4.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

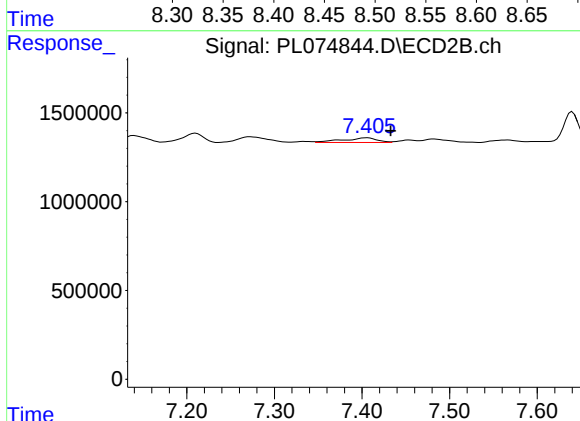


#11 alpha-Chlordane

R.T.: 7.407 min
Delta R.T.: -0.026 min
Response: 711535
Conc: 0.53 ng/ml

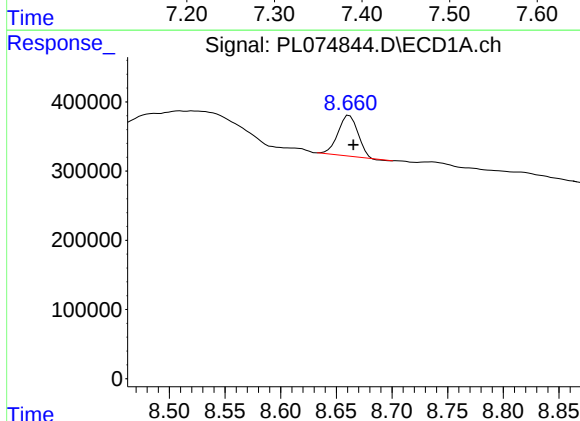


#12 4,4'-DDE

R.T.: 8.662 min
Delta R.T.: -0.004 min
Response: 716049
Conc: 1.55 ng/ml

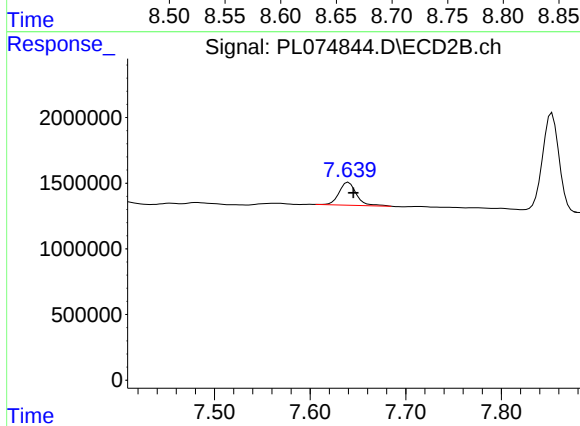

#12 4,4'-DDE


R.T.: 7.640 min
Delta R.T.: -0.005 min
Response: 2196903
Conc: 1.87 ng/ml

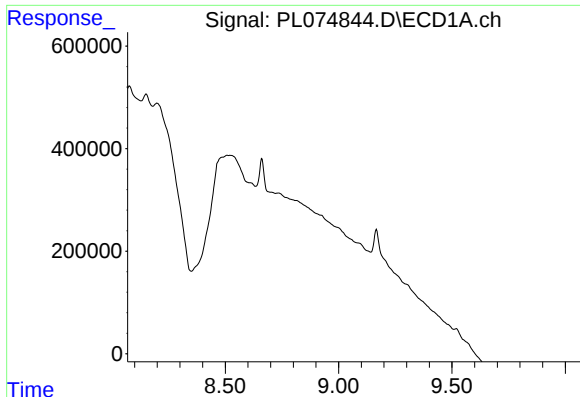

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

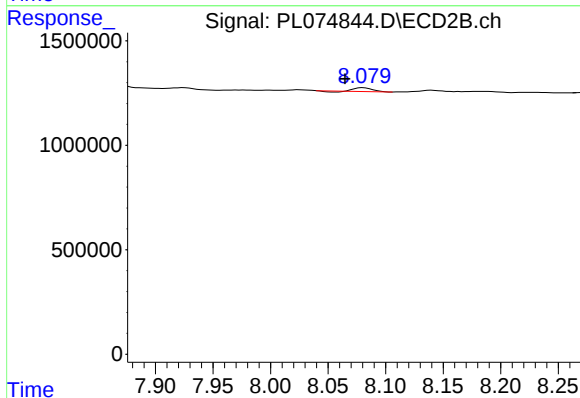


#14 Endrin

R.T.: 8.081 min
Delta R.T.: 0.016 min
Response: 186034
Conc: 0.18 ng/ml

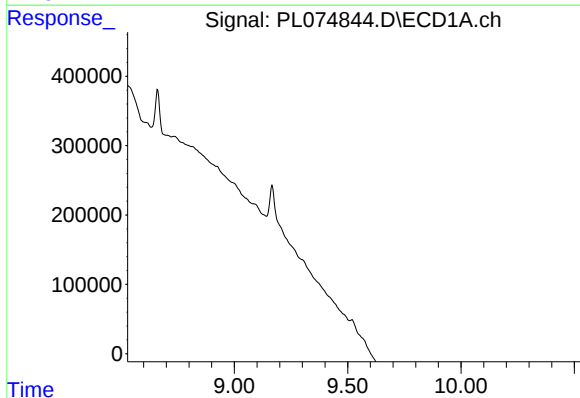


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 9.527 min
Response: 0
Conc: N.D.

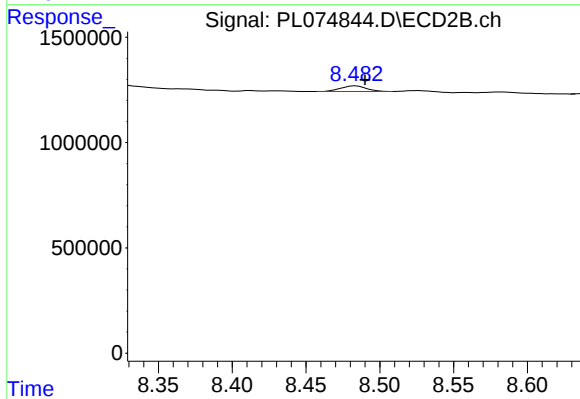

#17 4,4'-DDT


R.T.: 8.484 min
Delta R.T.: -0.006 min
Response: 323436
Conc: 0.32 ng/ml

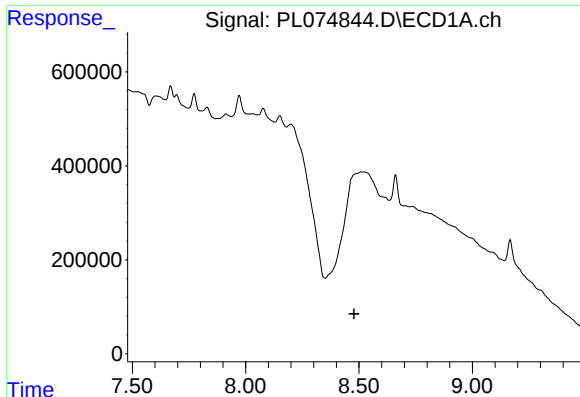

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 8.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

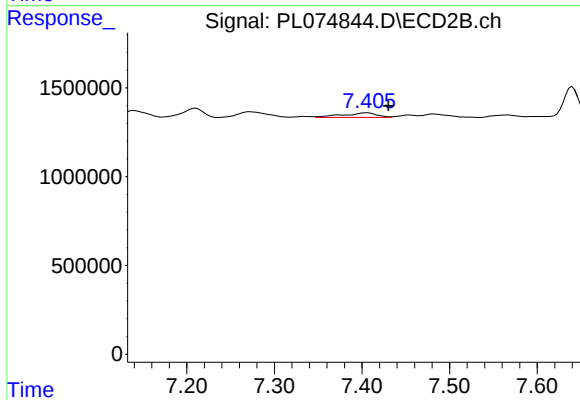


#26 Chlordane-4

R.T.: 7.407 min
Delta R.T.: -0.023 min
Response: 711535
Conc: 5.19 ng/ml

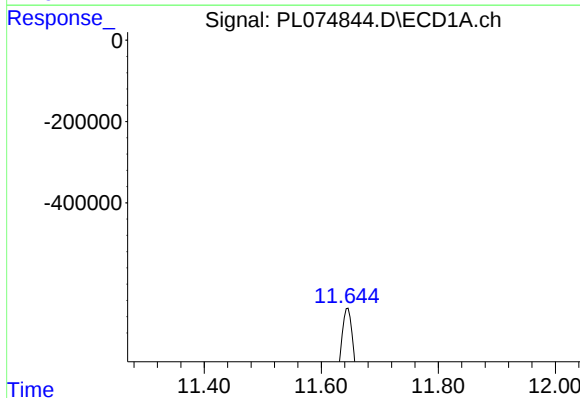

#28 Decachlorobiphenyl

R.T.: 11.646 min
Delta R.T.: -0.005 min
Response: 6653635
Conc: 14.90 ng/ml

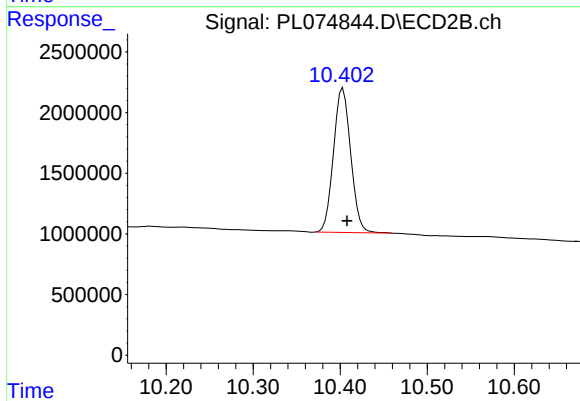

#28 Decachlorobiphenyl

R.T.: 10.403 min
Delta R.T.: -0.005 min
Response: 16388009
Conc: 15.97 ng/ml