

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051922\
 Data File : PL074862.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2022 21:31
 Operator : AR\AJ
 Sample : N2907-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 02:50:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.646	4.650	10049589	26974968	19.793	19.654
2)	SA Decachlor...	11.643	10.401	7429250	18514477	16.636	18.038
Target Compounds							
6)	B beta-BHC	0.000	6.124f	0	344824	N.D.	0.434 #
9)	A Endosulfan I	8.509f	0.000	5347843	0	9.276	N.D. #
11)	B alpha-Chl...	8.509f	0.000	5347843	0	8.760	N.D. #
12)	B 4,4'-DDE	8.661	7.639	3789855	10571302	8.187	8.984
13)	MA Dieldrin	0.000	7.770	0	229075	N.D.	0.180 #
14)	MA Endrin	0.000	8.078	0	684102	N.D.	0.648 #
15)	B Endosulfa...	0.000	8.367	0	234617	N.D.	0.208 #
16)	A 4,4'-DDD	9.202	8.223	699661	1287011	1.547	1.306
17)	MA 4,4'-DDT	9.523	8.484	1167503	3447639	2.540	3.446 #
18)	B Endrin al...	0.000	8.555	0	394002	N.D.	0.493 #
22)	Mirex	0.000	9.519f	0	488115	N.D.	0.504 #
26)	Chlordane-4	8.509f	0.000	5347843	0	55.510	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051922\
Data File : PL074862.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2022 21:31
Operator : AR\AJ
Sample : N2907-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 02:50:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

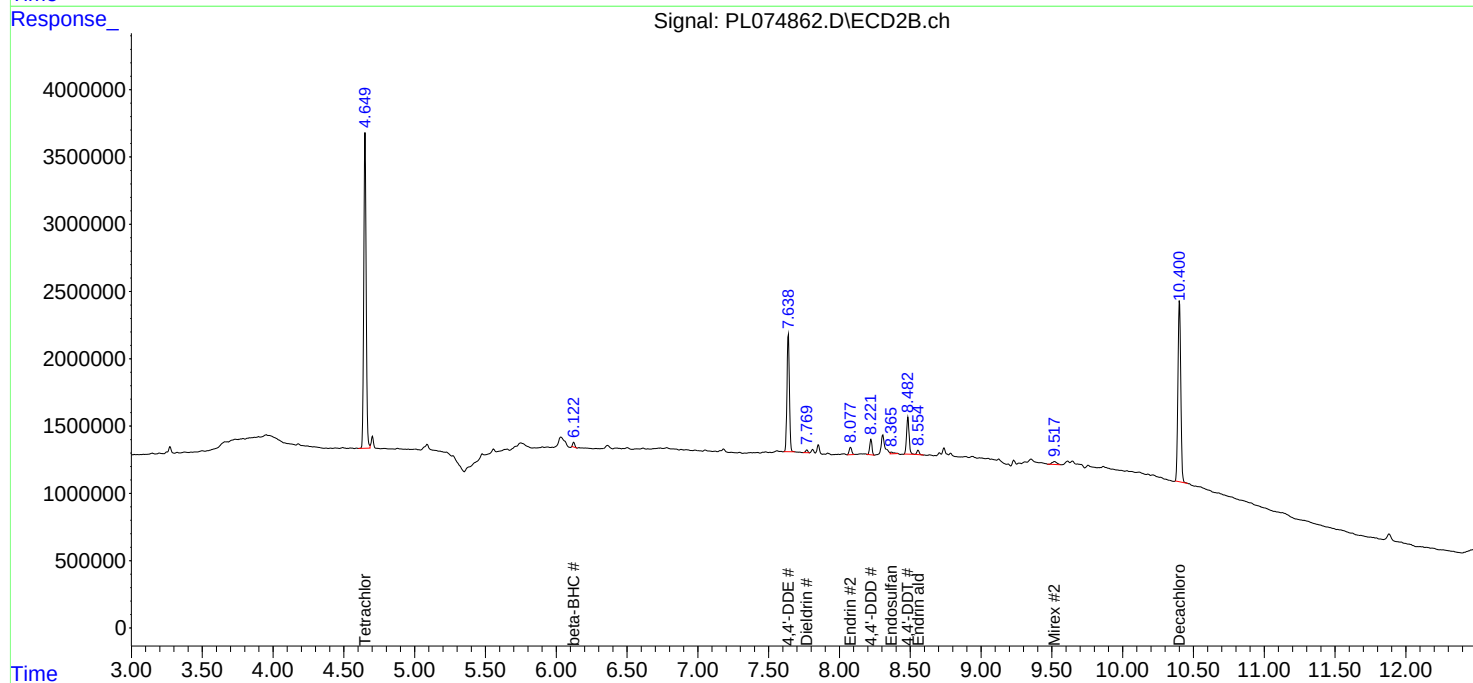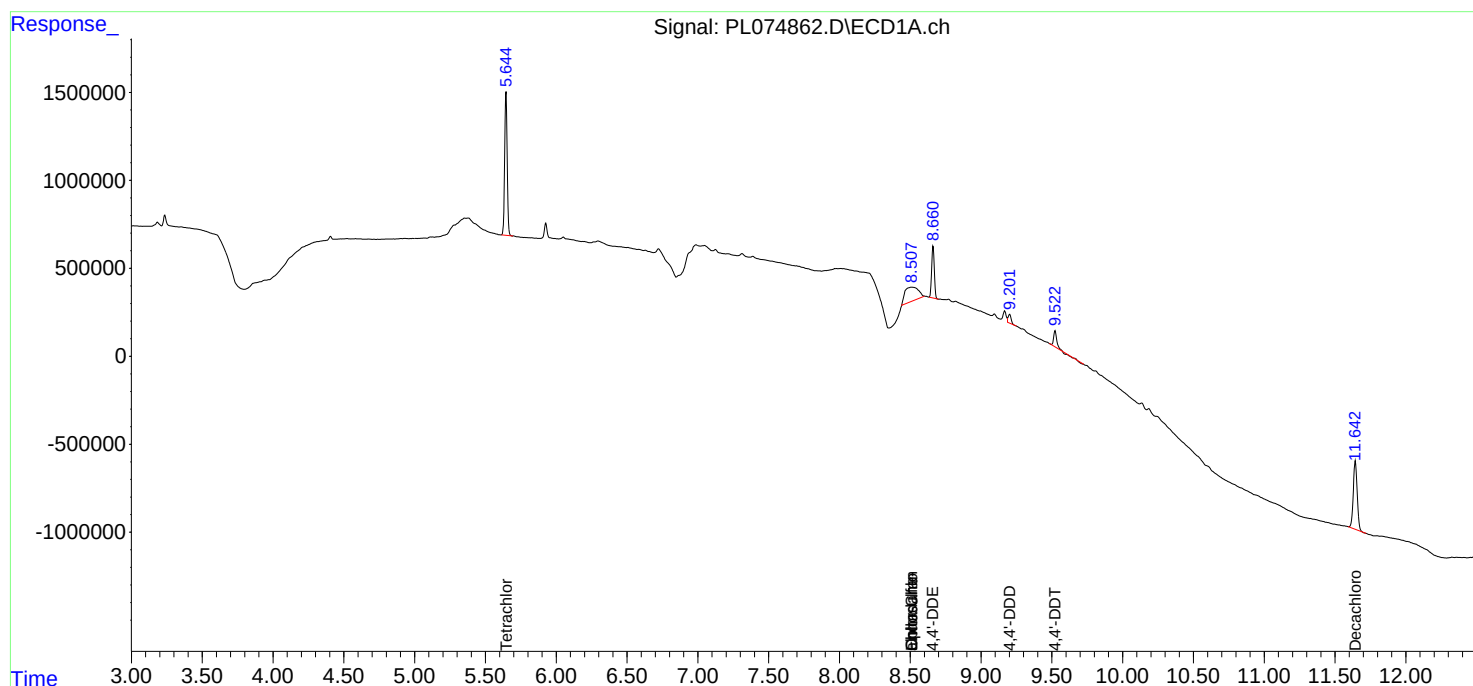


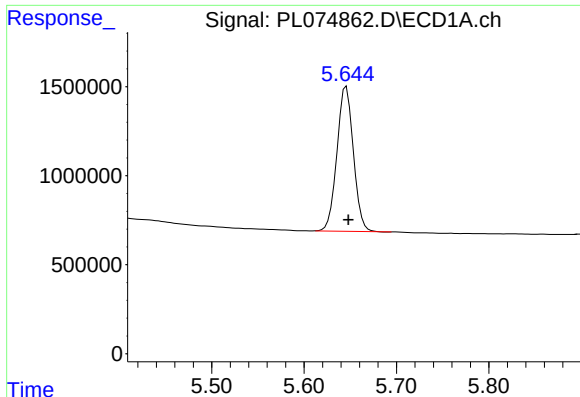

#1 Tetrachloro-m-xylene


R.T.: 5.646 min
Delta R.T.: -0.002 min
Response: 10049589
Conc: 19.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

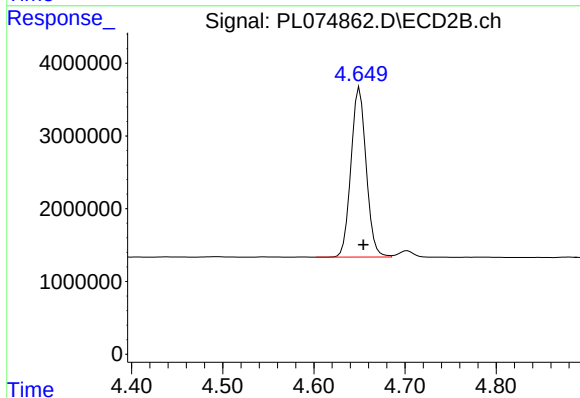


#1 Tetrachloro-m-xylene

R.T.: 4.650 min
Delta R.T.: -0.004 min
Response: 26974968
Conc: 19.65 ng/ml

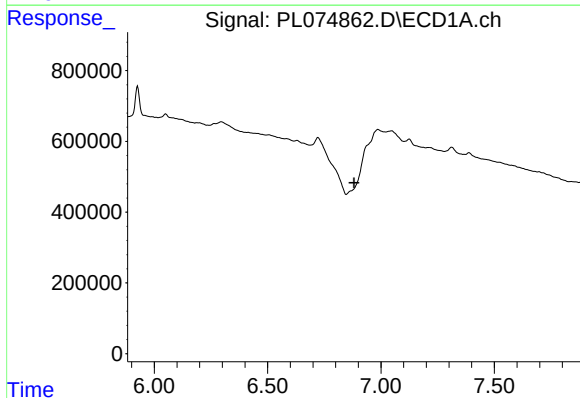


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.882 min
Response: 0
Conc: N.D.

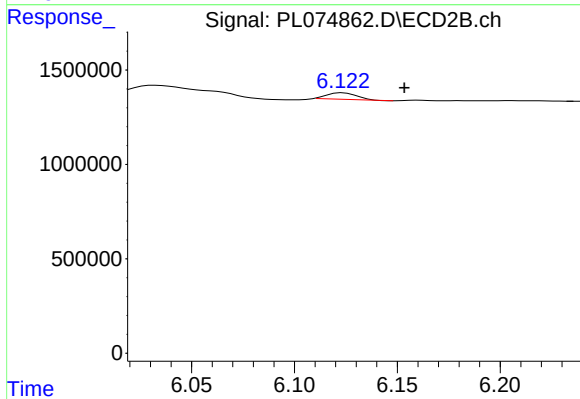

#6 beta-BHC


R.T.: 6.124 min
Delta R.T.: -0.030 min
Response: 344824
Conc: 0.43 ng/ml

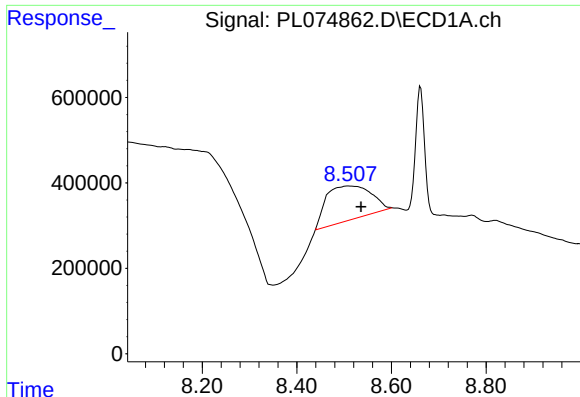

#9 Endosulfan I


R.T.: 8.509 min
Delta R.T.: -0.027 min
Response: 5347843
Conc: 9.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

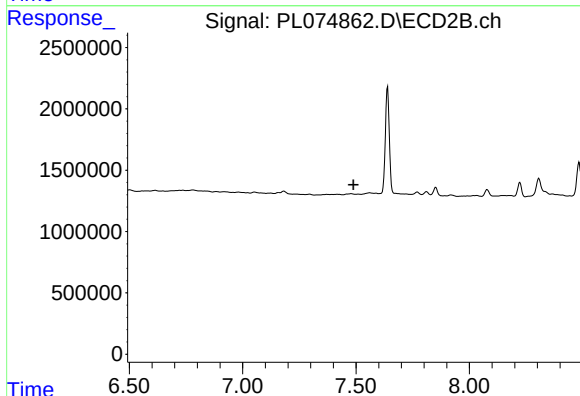


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.489 min
Response: 0
Conc: N.D.

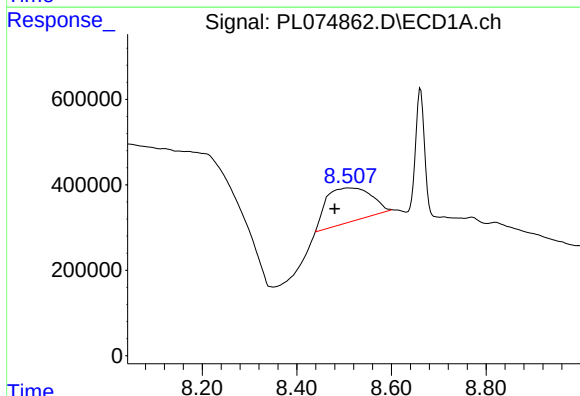


#11 alpha-Chlordane

R.T.: 8.509 min
Delta R.T.: 0.029 min
Response: 5347843
Conc: 8.76 ng/ml

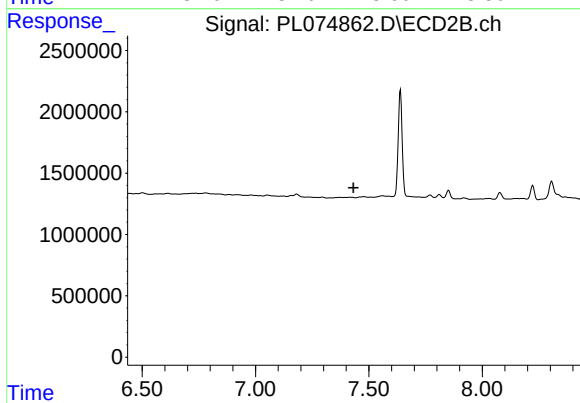

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.433 min
Response: 0
Conc: N.D.

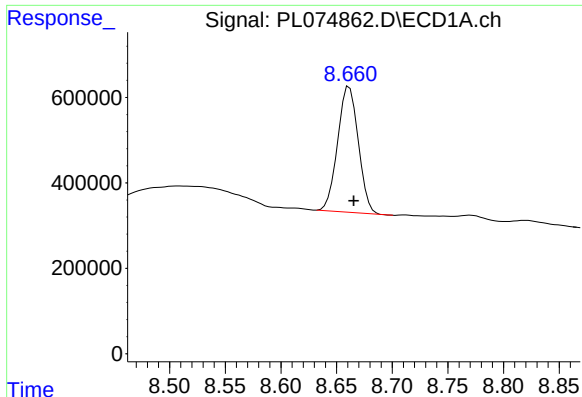

#12 4,4'-DDE


R.T.: 8.661 min
Delta R.T.: -0.004 min
Response: 3789855
Conc: 8.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

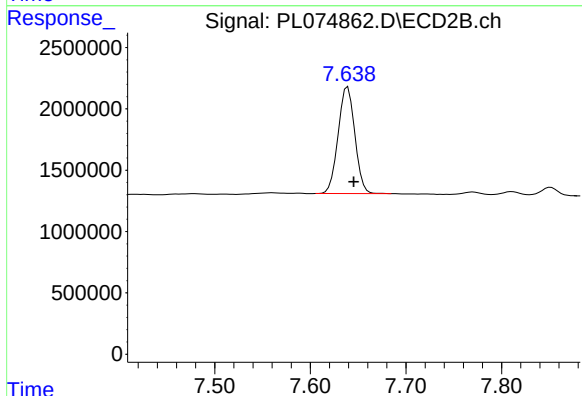


#12 4,4'-DDE

R.T.: 7.639 min
Delta R.T.: -0.006 min
Response: 10571302
Conc: 8.98 ng/ml

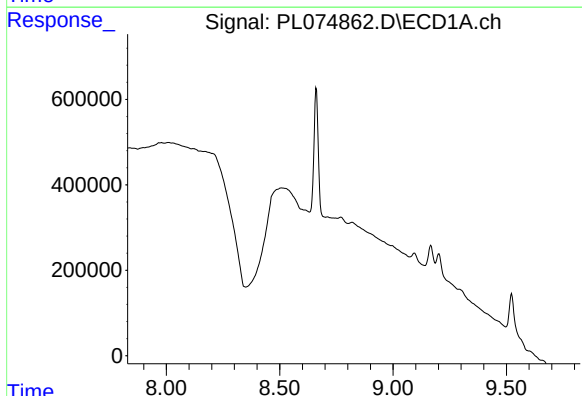


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.827 min
Response: 0
Conc: N.D.

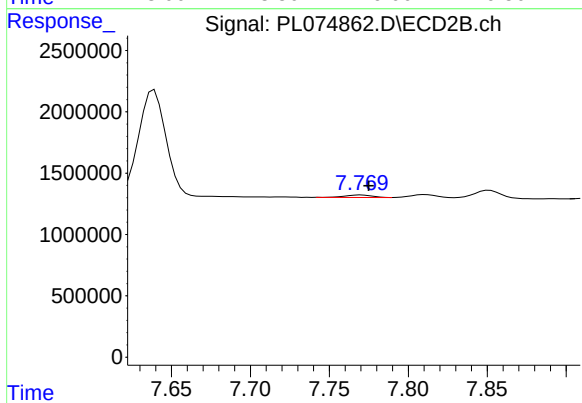

#13 Dieldrin


R.T.: 7.770 min
Delta R.T.: -0.005 min
Response: 229075
Conc: 0.18 ng/ml

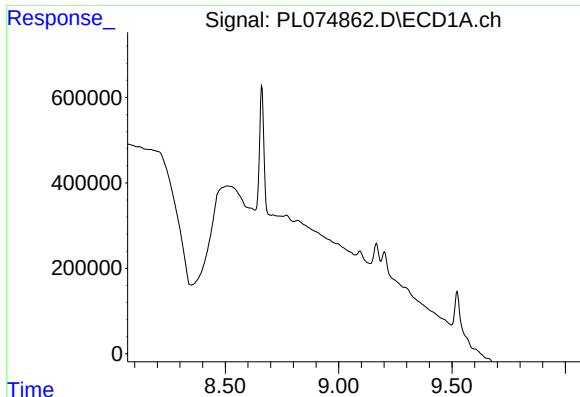

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

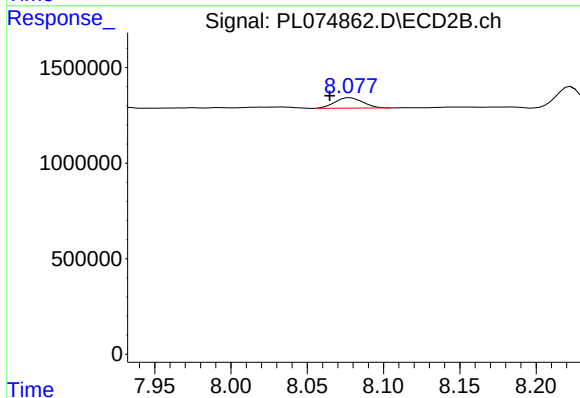


#14 Endrin

R.T.: 8.078 min
Delta R.T.: 0.014 min
Response: 684102
Conc: 0.65 ng/ml

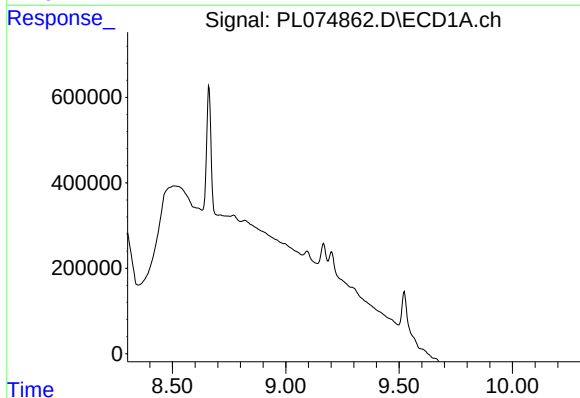


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 9.302 min
Response: 0
Conc: N.D.

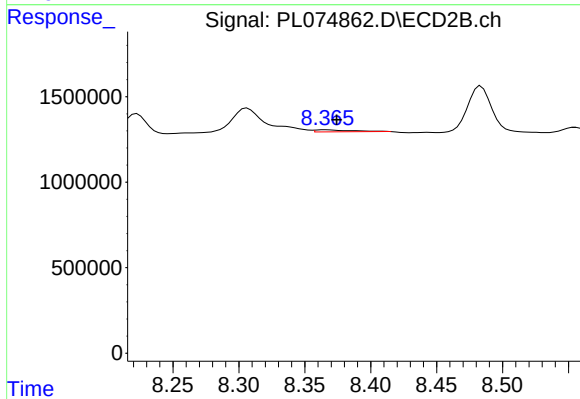

#15 Endosulfan II


R.T.: 8.367 min
Delta R.T.: -0.008 min
Response: 234617
Conc: 0.21 ng/ml

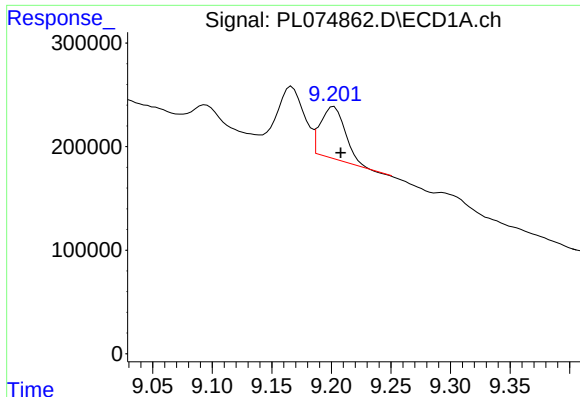

#16 4,4'-DDD


R.T.: 9.202 min
Delta R.T.: -0.006 min
Response: 699661
Conc: 1.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

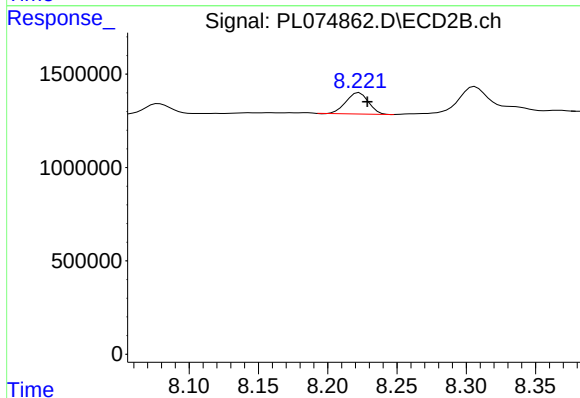


#16 4,4'-DDD

R.T.: 8.223 min
Delta R.T.: -0.006 min
Response: 1287011
Conc: 1.31 ng/ml

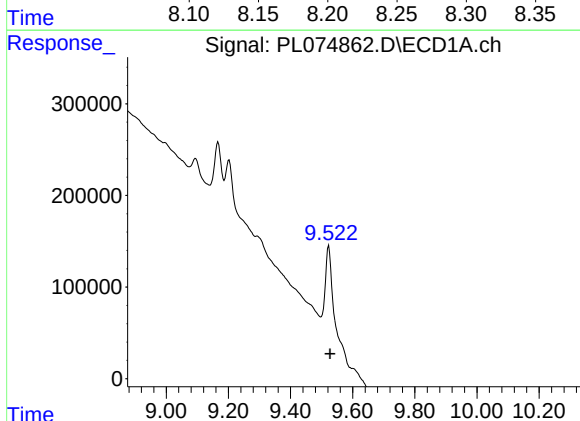


#17 4,4'-DDT

R.T.: 9.523 min
Delta R.T.: -0.004 min
Response: 1167503
Conc: 2.54 ng/ml

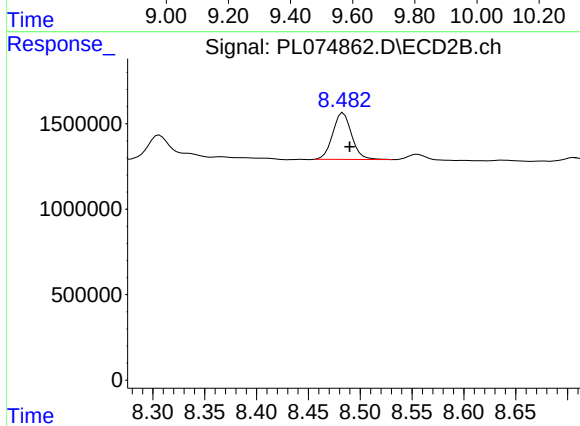

#17 4,4'-DDT


R.T.: 8.484 min
Delta R.T.: -0.006 min
Response: 3447639
Conc: 3.45 ng/ml

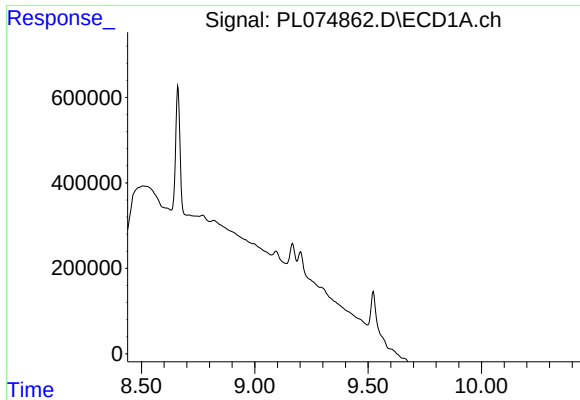

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 9.436 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

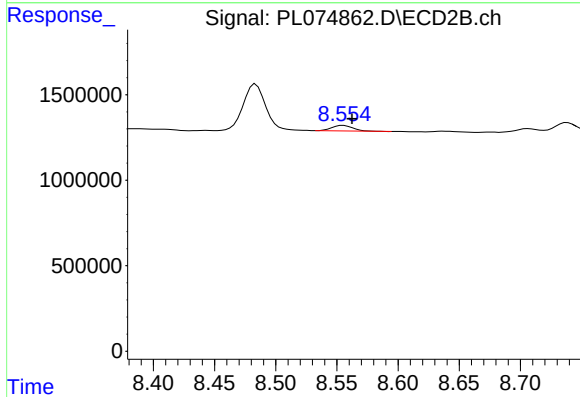


#18 Endrin aldehyde

R.T.: 8.555 min
Delta R.T.: -0.007 min
Response: 394002
Conc: 0.49 ng/ml

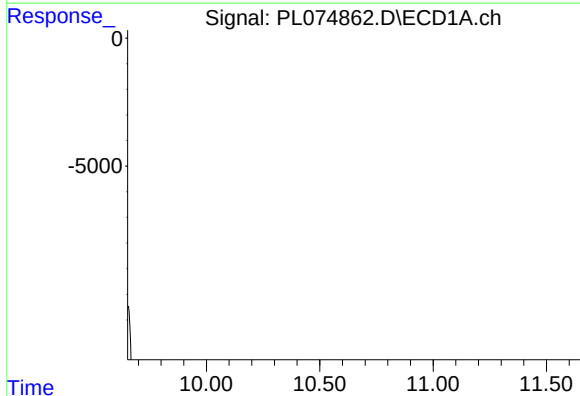


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 10.652 min
Response: 0
Conc: N.D.

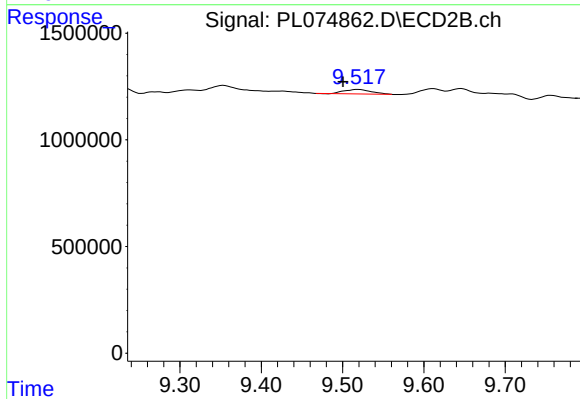

#22 Mirex


R.T.: 9.519 min
Delta R.T.: 0.018 min
Response: 488115
Conc: 0.50 ng/ml

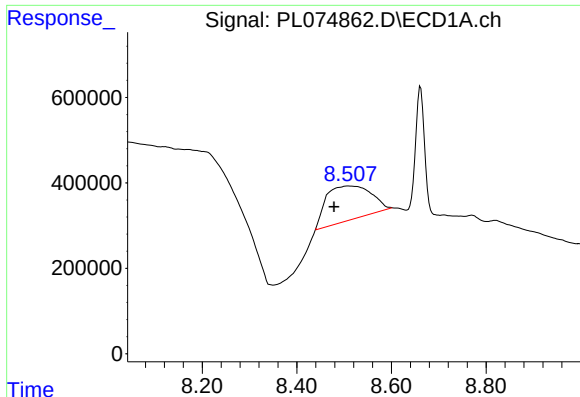

#26 Chlordane-4


R.T.: 8.509 min
Delta R.T.: 0.030 min
Response: 5347843
Conc: 55.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

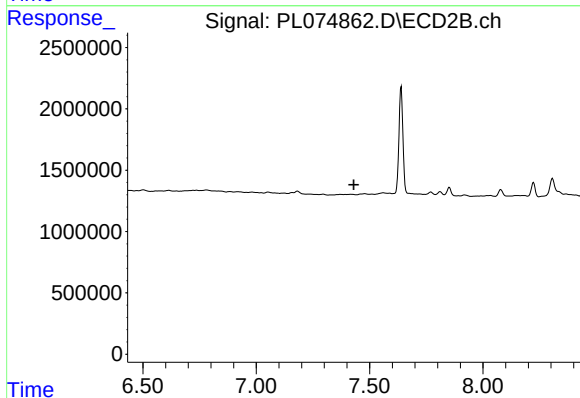


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.430 min
Response: 0
Conc: N.D.

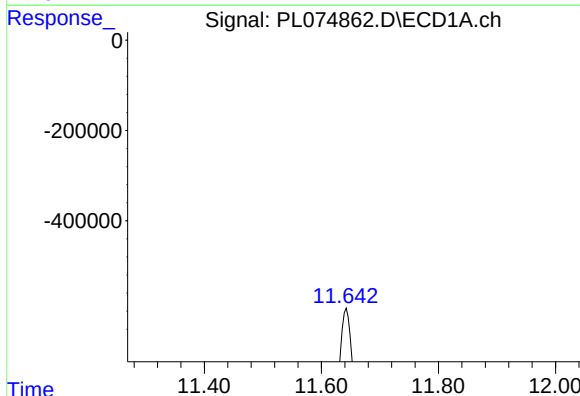

#28 Decachlorobiphenyl

R.T.: 11.643 min
Delta R.T.: -0.008 min
Response: 7429250
Conc: 16.64 ng/ml

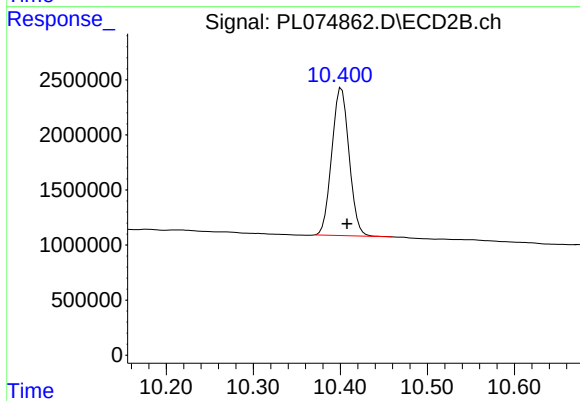

#28 Decachlorobiphenyl

R.T.: 10.401 min
Delta R.T.: -0.006 min
Response: 18514477
Conc: 18.04 ng/ml