

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051922\
 Data File : PL074871.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2022 00:00
 Operator : AR\AJ
 Sample : N2938-01
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 02:54:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.645	4.650	4931457	13038561	9.713	9.500
28)	SA Decachlor...	11.643	10.402	7071382	16460927	15.834	16.037
Target Compounds							
6)	B beta-BHC	0.000	6.125f	0	409174	N.D.	0.515 #
9)	A Endosulfan I	8.513f	0.000	2688151	0	4.663	N.D. #
10)	B gamma-Chl...	0.000	7.341f	0	313370	N.D.	0.226 #
11)	B alpha-Chl...	8.481	0.000	2547070	0	4.172	N.D. #
14)	MA Endrin	0.000	8.082f	0	52532	N.D.	0.050 #
17)	MA 4,4'-DDT	0.000	8.504	0	222374	N.D.	0.222 #
21)	B Endrin ke...	0.000	9.339f	0	293342	N.D.	0.263 #
23)	Chlordane-1	0.000	5.972	0	304950	N.D.	6.729 #
24)	Chlordane-2	0.000	6.658	0	239281	N.D.	4.309 #
25)	Chlordane-3	0.000	7.341f	0	313370	N.D.	2.414 #
26)	Chlordane-4	8.481	0.000	2547070	0	26.438	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051922\
Data File : PL074871.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2022 00:00
Operator : AR\AJ
Sample : N2938-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 02:54:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

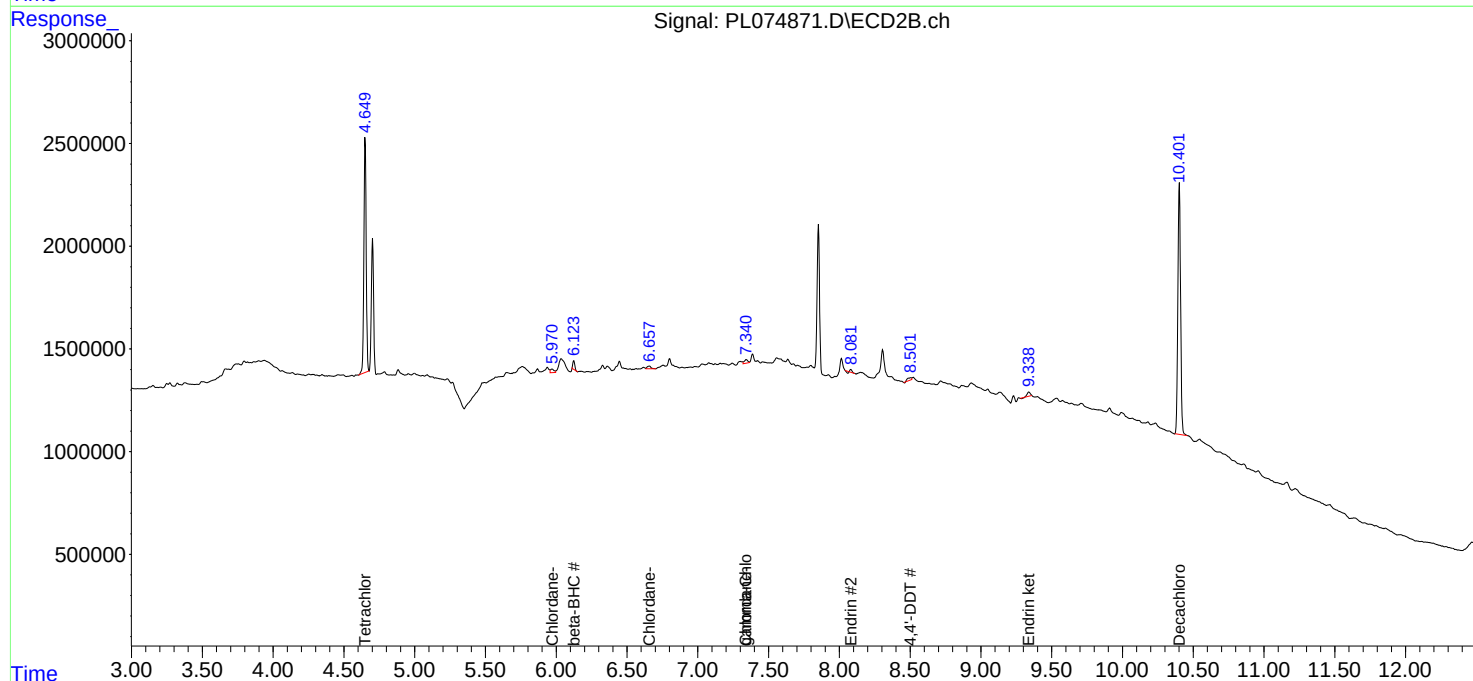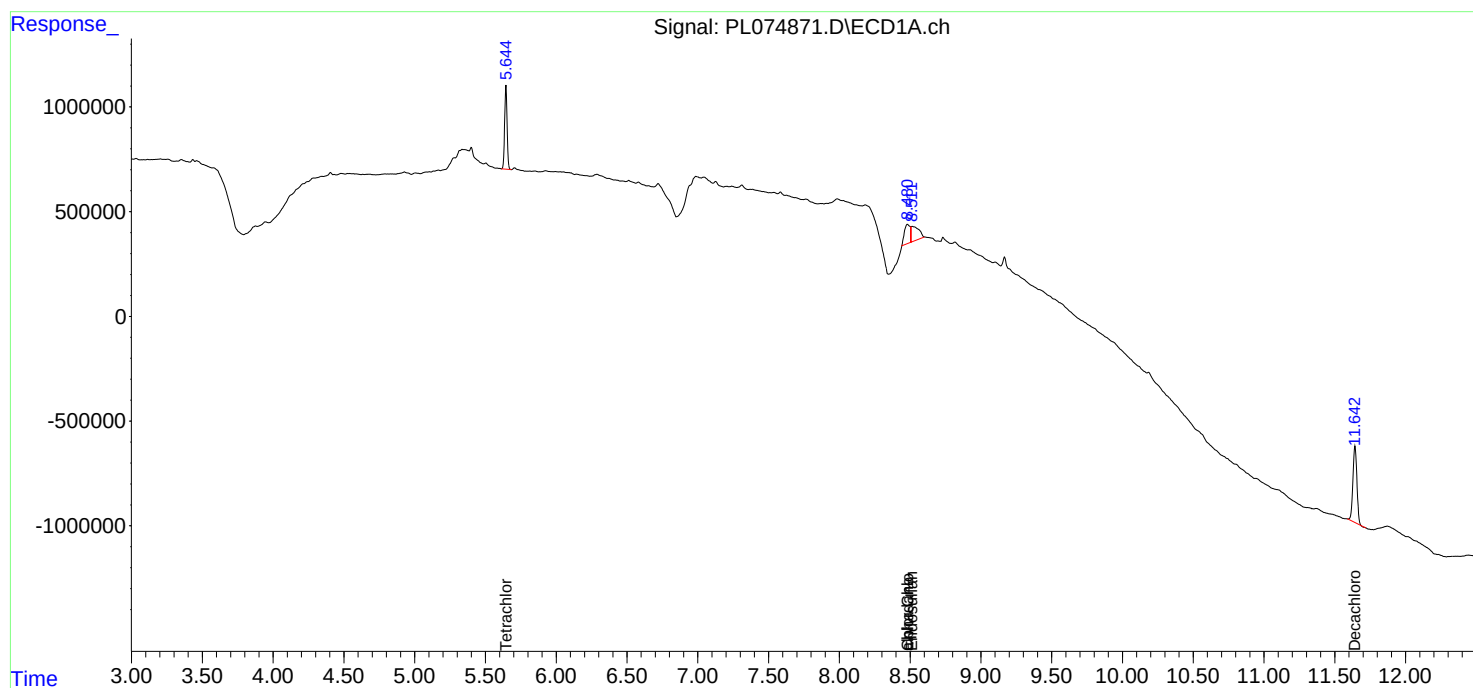


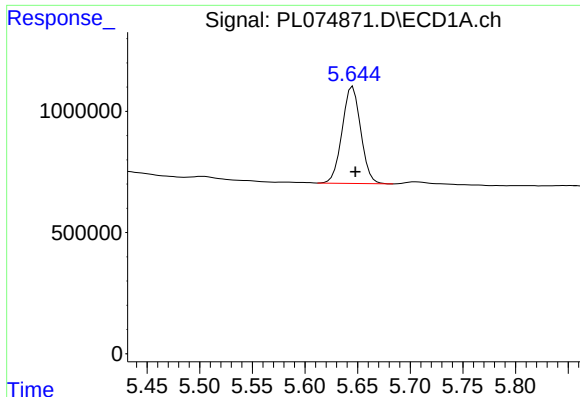

#1 Tetrachloro-m-xylene


R.T.: 5.645 min
Delta R.T.: -0.003 min
Response: 4931457
Conc: 9.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

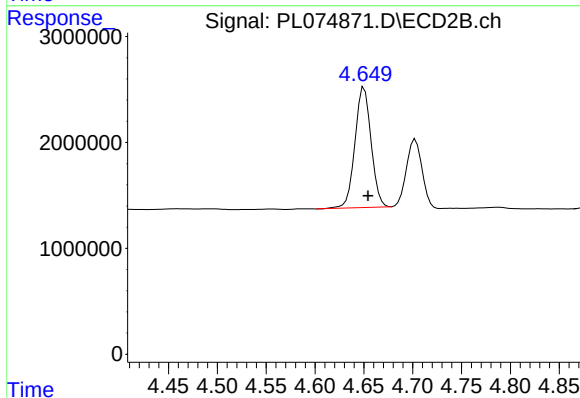


#1 Tetrachloro-m-xylene

R.T.: 4.650 min
Delta R.T.: -0.004 min
Response: 13038561
Conc: 9.50 ng/ml

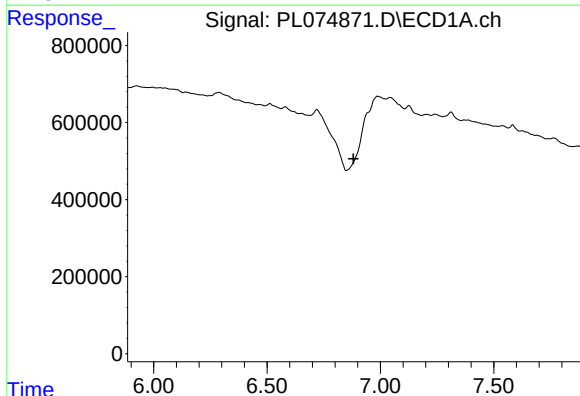


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.882 min
Response: 0
Conc: N.D.

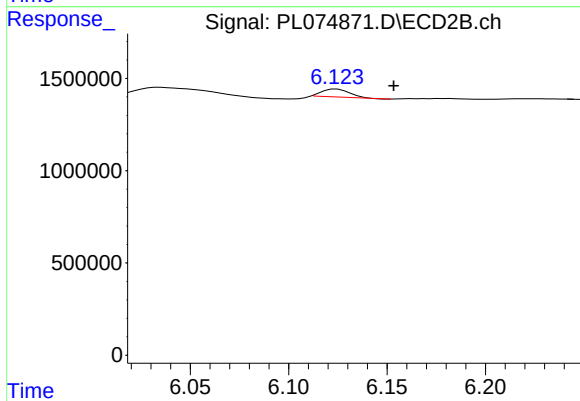

#6 beta-BHC


R.T.: 6.125 min
Delta R.T.: -0.029 min
Response: 409174
Conc: 0.52 ng/ml

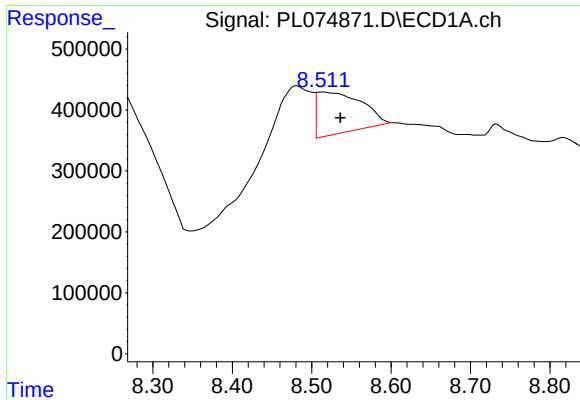

#9 Endosulfan I


R.T.: 8.513 min
Delta R.T.: -0.023 min
Response: 2688151
Conc: 4.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

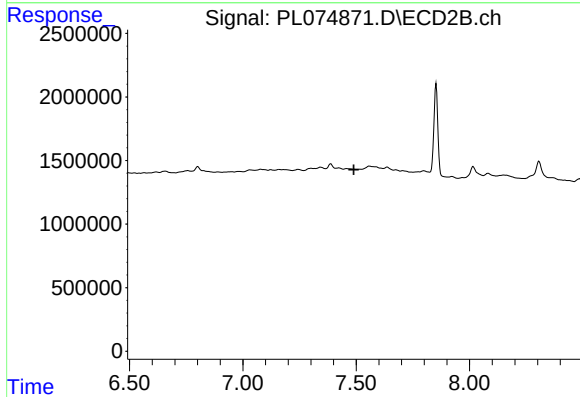


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.489 min
Response: 0
Conc: N.D.

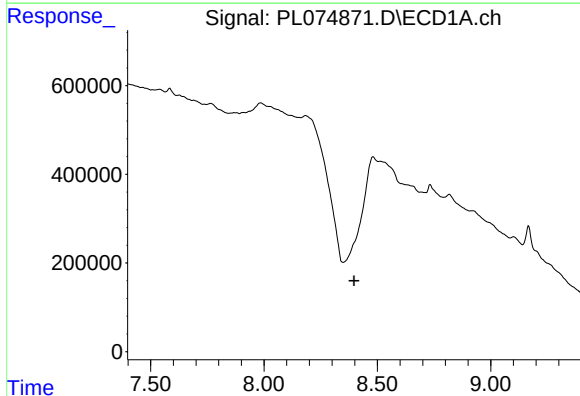


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.398 min
Response: 0
Conc: N.D.

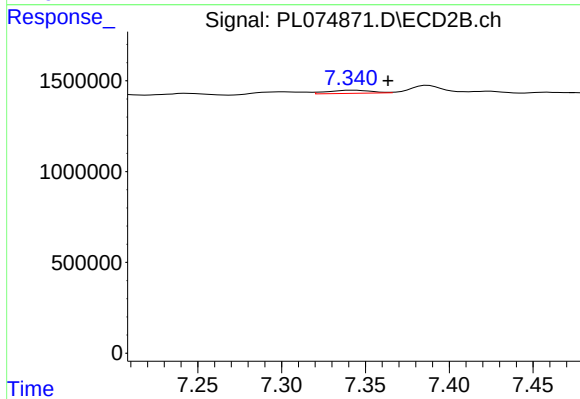

#10 gamma-Chlordane


R.T.: 7.341 min
Delta R.T.: -0.022 min
Response: 313370
Conc: 0.23 ng/ml

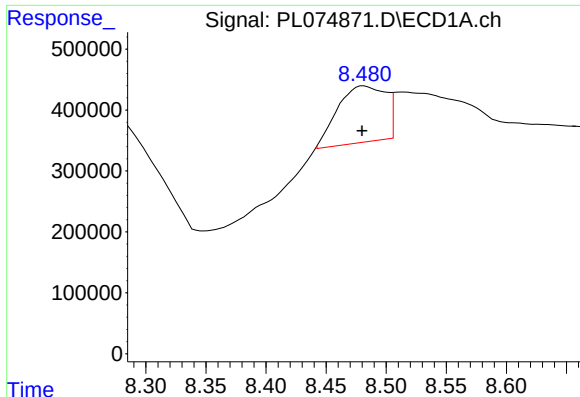

#11 alpha-Chlordane


R.T.: 8.481 min
Delta R.T.: 0.002 min
Response: 2547070
Conc: 4.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

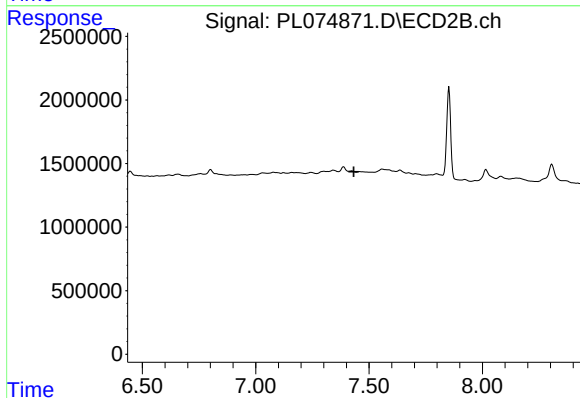


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.433 min
Response: 0
Conc: N.D.

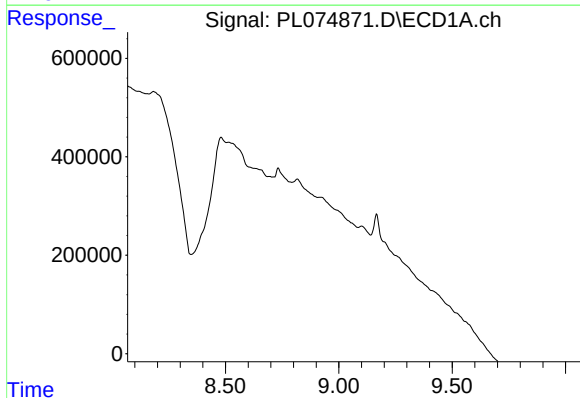


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.068 min
Response: 0
Conc: N.D.

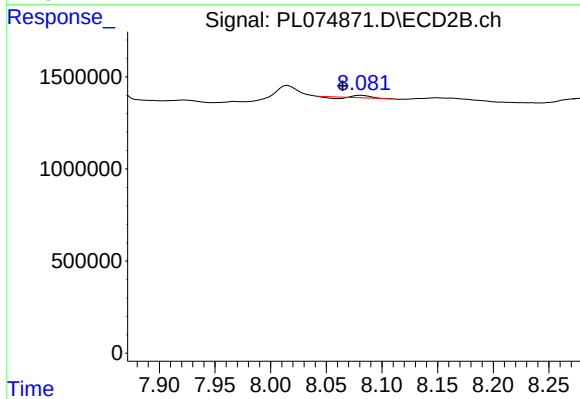

#14 Endrin


R.T.: 8.082 min
Delta R.T.: 0.017 min
Response: 52532
Conc: 0.05 ng/ml

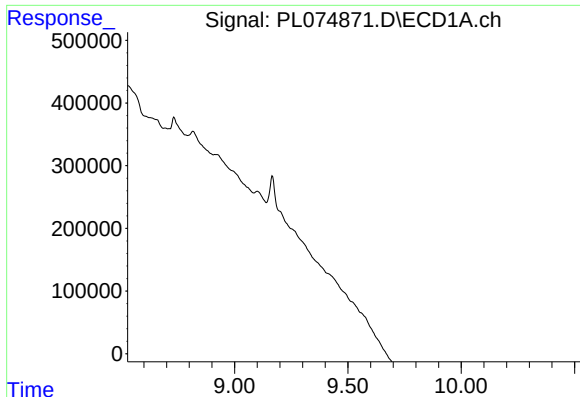

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.527 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

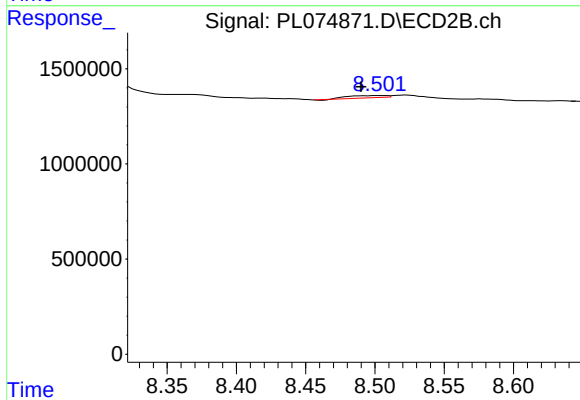


#17 4,4'-DDT

R.T.: 8.504 min
Delta R.T.: 0.014 min
Response: 222374
Conc: 0.22 ng/ml

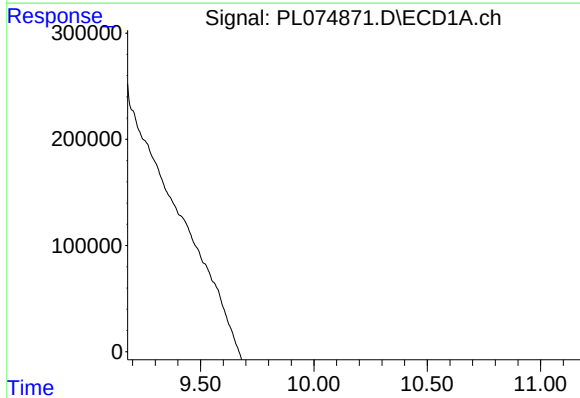


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 10.177 min
Response: 0
Conc: N.D.

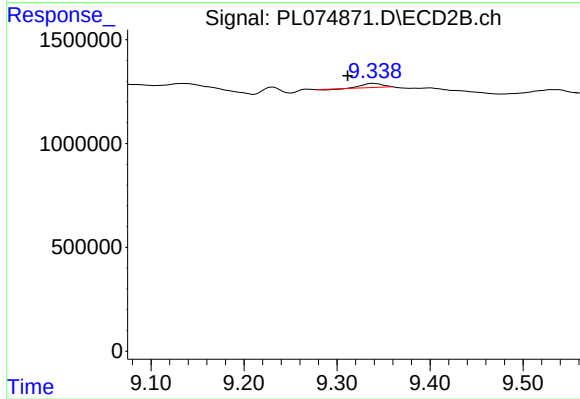

#21 Endrin ketone


R.T.: 9.339 min
Delta R.T.: 0.028 min
Response: 293342
Conc: 0.26 ng/ml

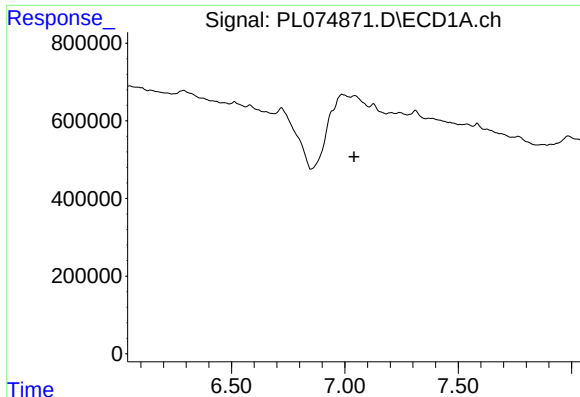

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 7.041 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

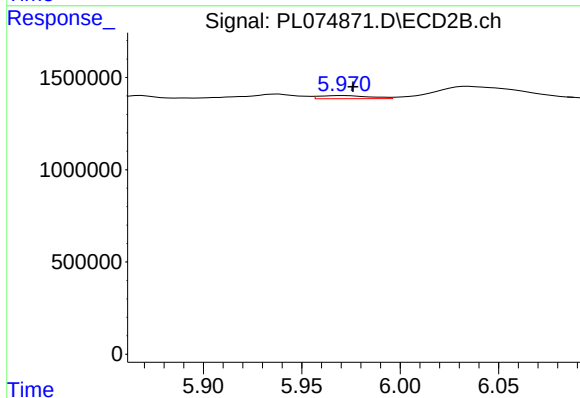


#23 Chlordane-1

R.T.: 5.972 min
Delta R.T.: -0.004 min
Response: 304950
Conc: 6.73 ng/ml

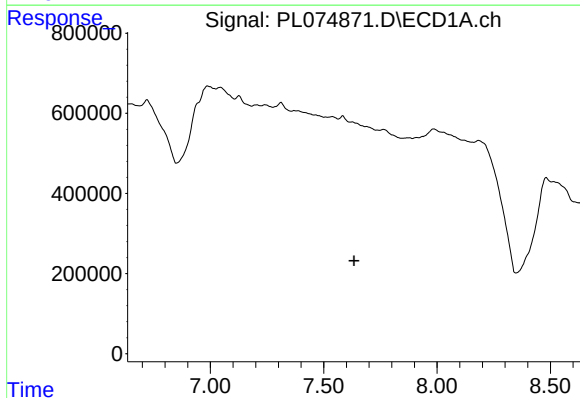


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 7.634 min
Response: 0
Conc: N.D.

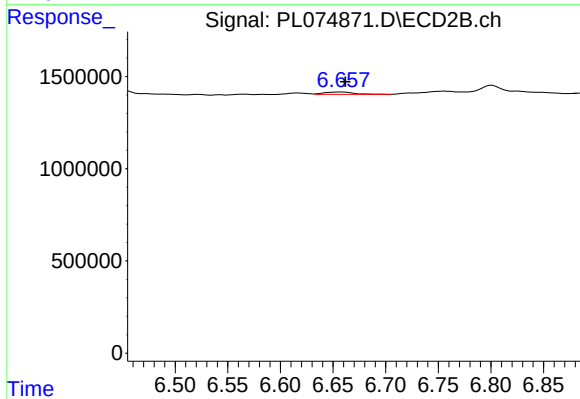

#24 Chlordane-2


R.T.: 6.658 min
Delta R.T.: -0.004 min
Response: 239281
Conc: 4.31 ng/ml

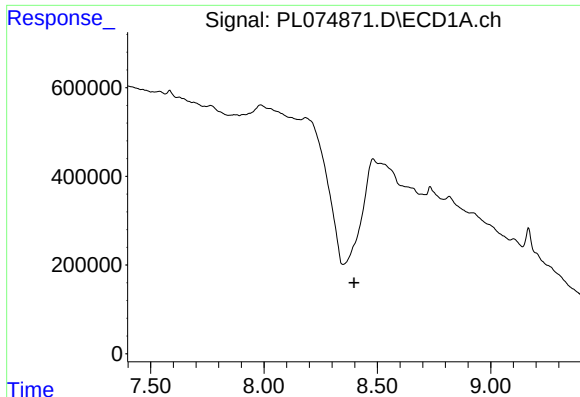

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

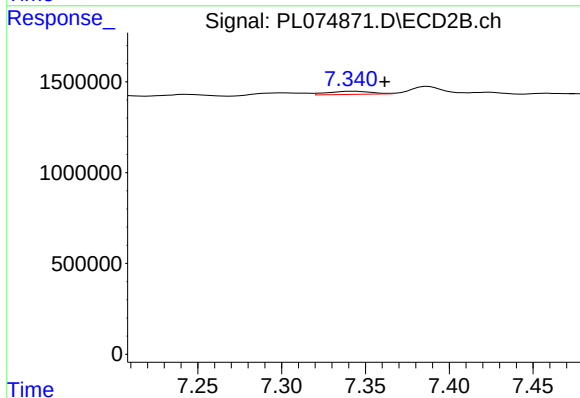


#25 Chlordane-3

R.T.: 7.341 min
Delta R.T.: -0.020 min
Response: 313370
Conc: 2.41 ng/ml

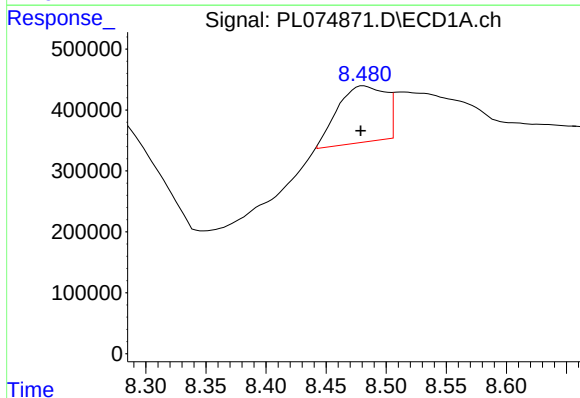


#26 Chlordane-4

R.T.: 8.481 min
Delta R.T.: 0.003 min
Response: 2547070
Conc: 26.44 ng/ml

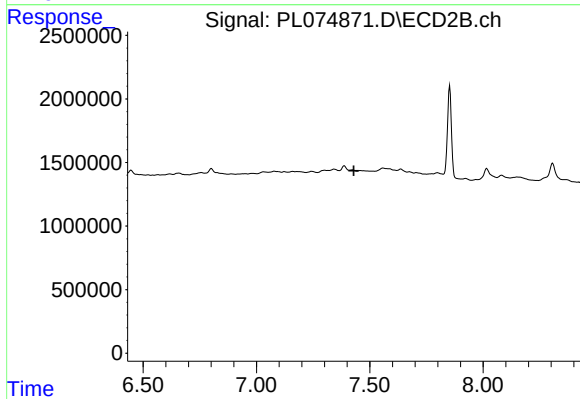

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

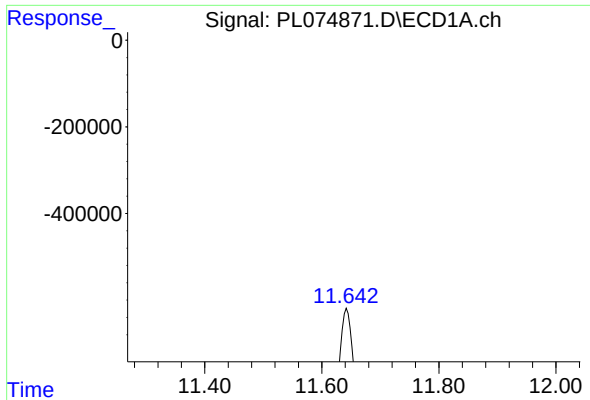

#28 Decachlorobiphenyl

R.T.: 11.643 min
Delta R.T.: -0.008 min
Response: 7071382
Conc: 15.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

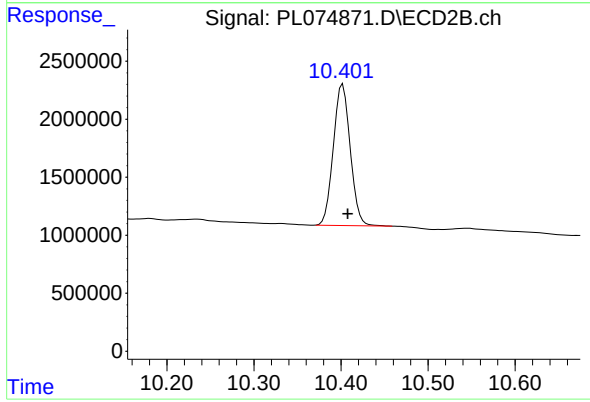

#28 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: -0.006 min
Response: 16460927
Conc: 16.04 ng/ml