

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051922\
 Data File : PL074872.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2022 00:16
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 02:55:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.646	4.651	10406778	27505474	20.496	20.040
28)	SA Decachlor...	11.644	10.402	9865779	23292713	22.092	22.693
Target Compounds							
4)	MA Heptachlor	0.000	6.164f	0	196221	N.D.	0.129 #
6)	B beta-BHC	0.000	6.164	0	196221	N.D.	0.247 #
7)	B delta-BHC	0.000	6.428	0	181545	N.D.	0.116 #
8)	B Heptachlo...	8.129	0.000	1914427	0	3.366	N.D. #
9)	A Endosulfan I	8.508f	0.000	5235655	0	9.082	N.D. #
10)	B gamma-Chl...	0.000	7.341f	0	283456	N.D.	0.205 #
11)	B alpha-Chl...	8.508f	0.000	5235655	0	8.576	N.D. #
13)	MA Dieldrin	0.000	7.772	0	1654114	N.D.	1.298 #
14)	MA Endrin	0.000	8.082f	0	685454	N.D.	0.649 #
17)	MA 4,4'-DDT	0.000	8.494	0	427217	N.D.	0.427 #
25)	Chlordane-3	0.000	7.341f	0	283456	N.D.	2.184 #
26)	Chlordane-4	8.508f	0.000	5235655	0	54.346	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051922\
Data File : PL074872.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2022 00:16
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 02:55:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

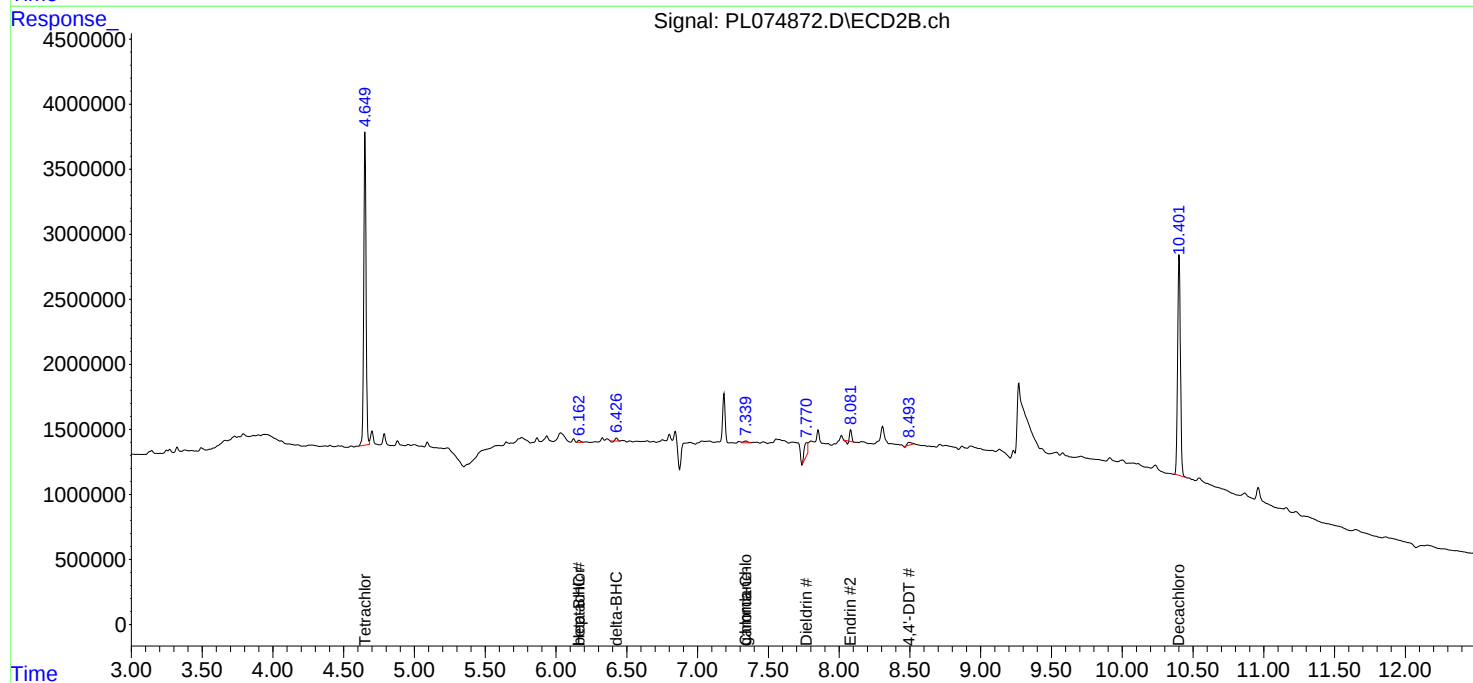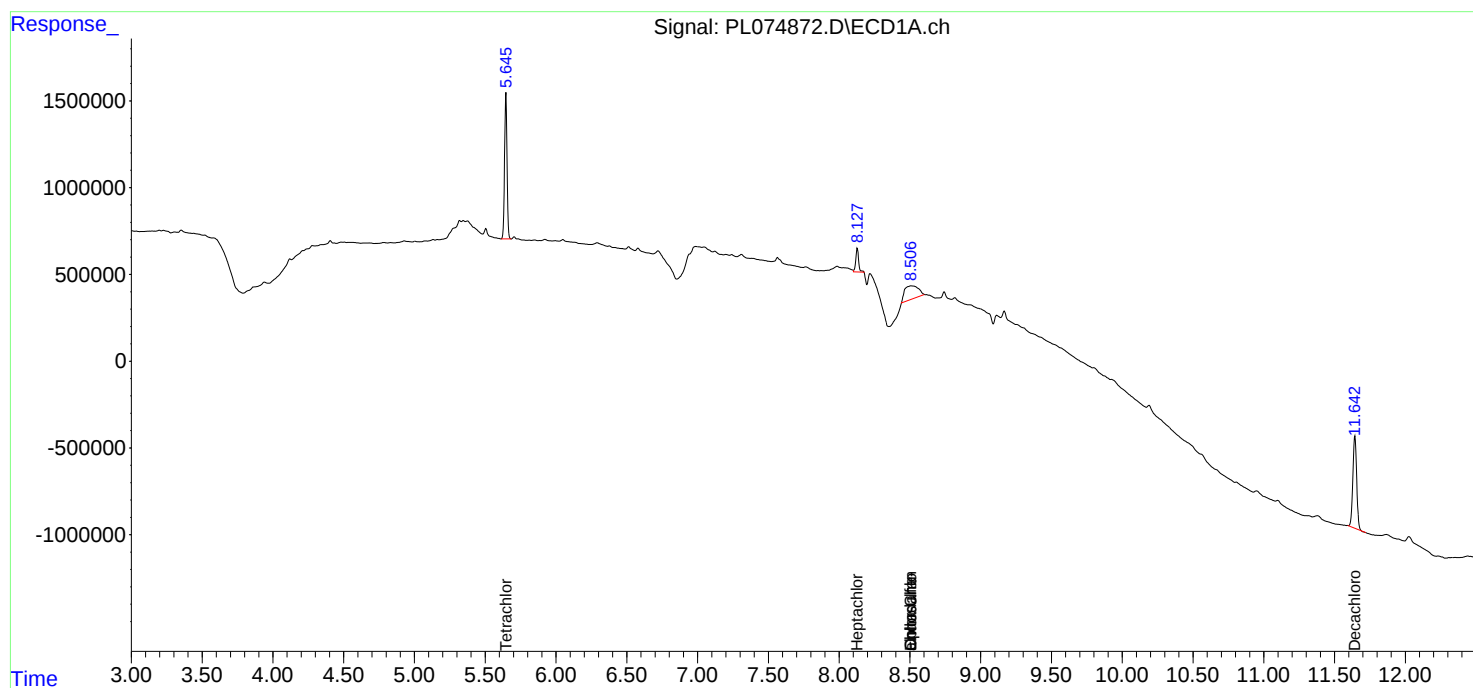


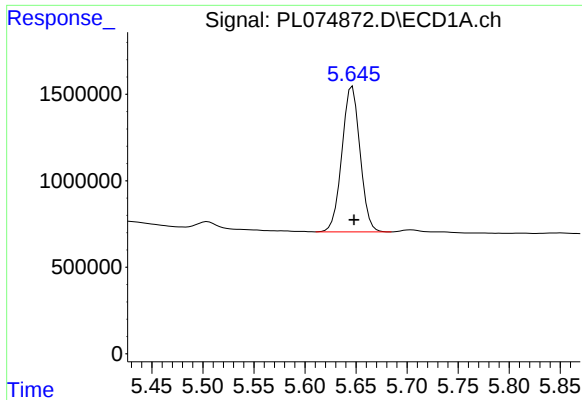

#1 Tetrachloro-m-xylene


R.T.: 5.646 min
Delta R.T.: -0.002 min
Response: 10406778
Conc: 20.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

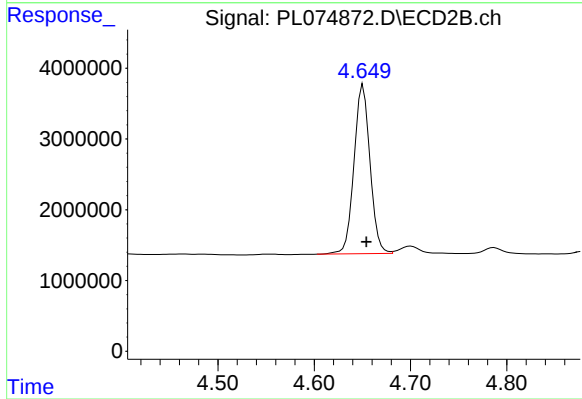


#1 Tetrachloro-m-xylene

R.T.: 4.651 min
Delta R.T.: -0.004 min
Response: 27505474
Conc: 20.04 ng/ml

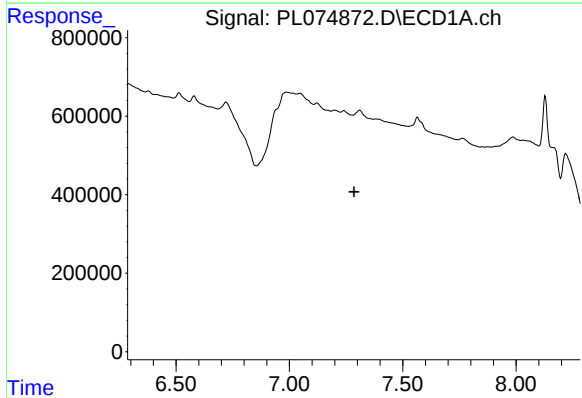


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.286 min
Response: 0
Conc: N.D.

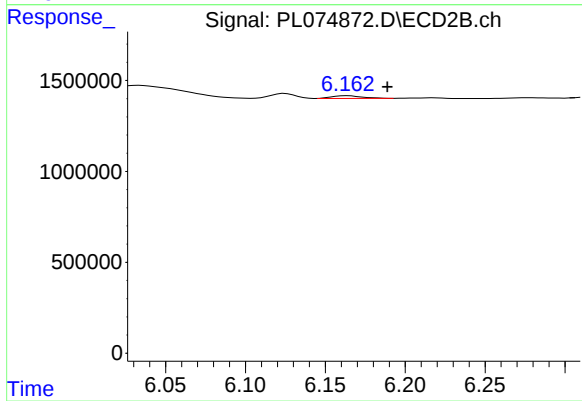

#4 Heptachlor


R.T.: 6.164 min
Delta R.T.: -0.025 min
Response: 196221
Conc: 0.13 ng/ml

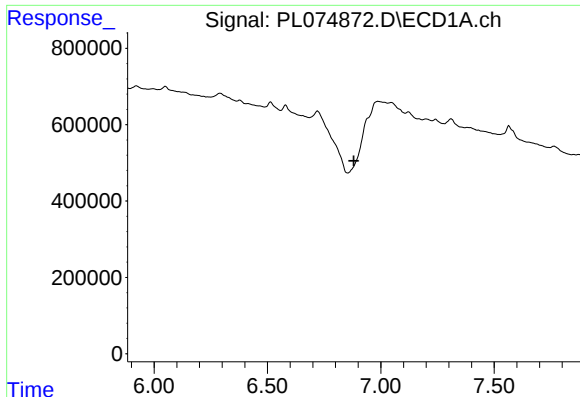

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.882 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

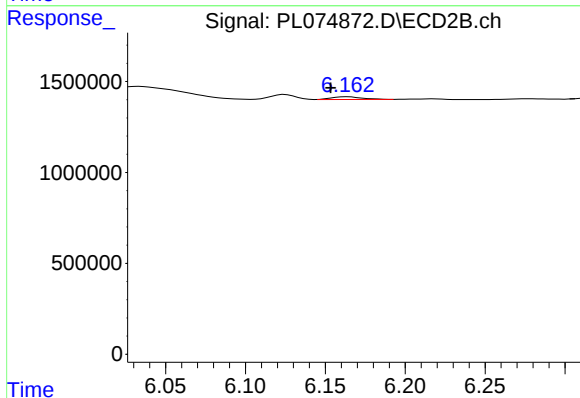


#6 beta-BHC

R.T.: 6.164 min
Delta R.T.: 0.010 min
Response: 196221
Conc: 0.25 ng/ml

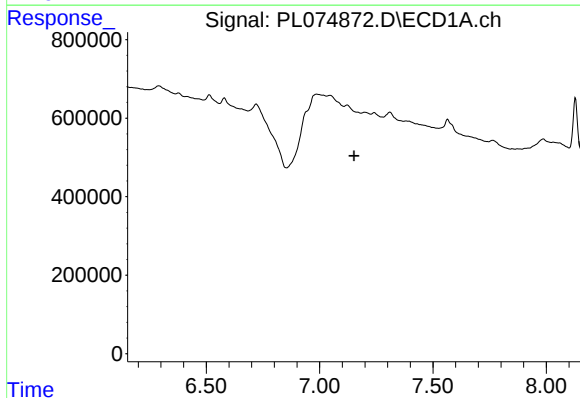


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 7.152 min
Response: 0
Conc: N.D.

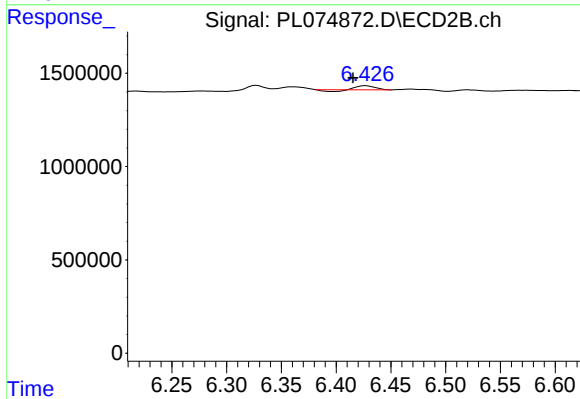

#7 delta-BHC


R.T.: 6.428 min
Delta R.T.: 0.012 min
Response: 181545
Conc: 0.12 ng/ml

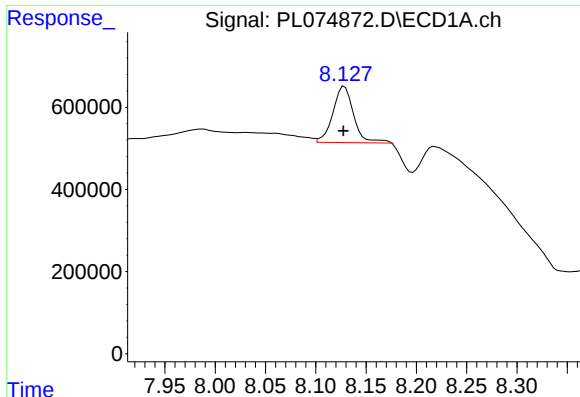

#8 Heptachlor epoxide


R.T.: 8.129 min
Delta R.T.: 0.001 min
Response: 1914427
Conc: 3.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

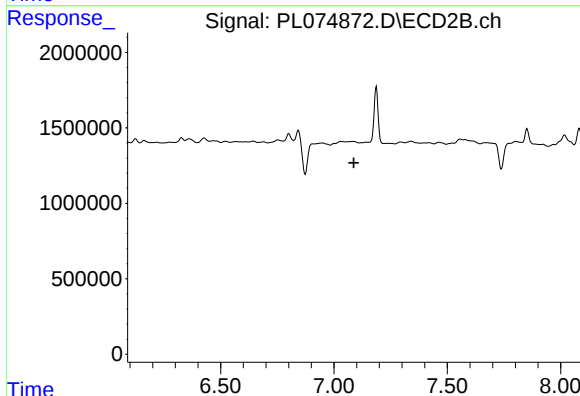


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.087 min
Response: 0
Conc: N.D.

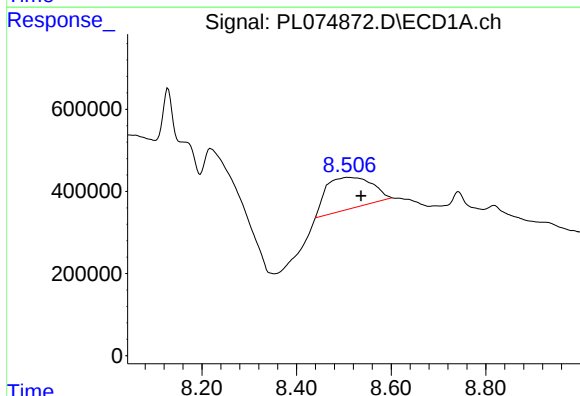


#9 Endosulfan I

R.T.: 8.508 min
Delta R.T.: -0.028 min
Response: 5235655
Conc: 9.08 ng/ml

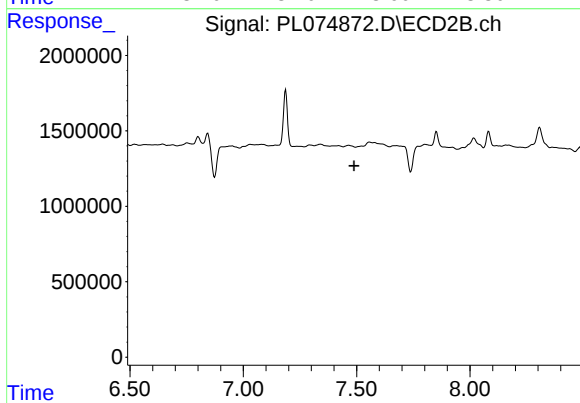

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 7.489 min
Response: 0
Conc: N.D.

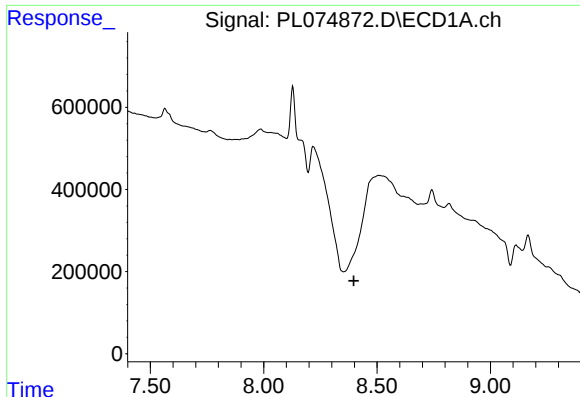

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

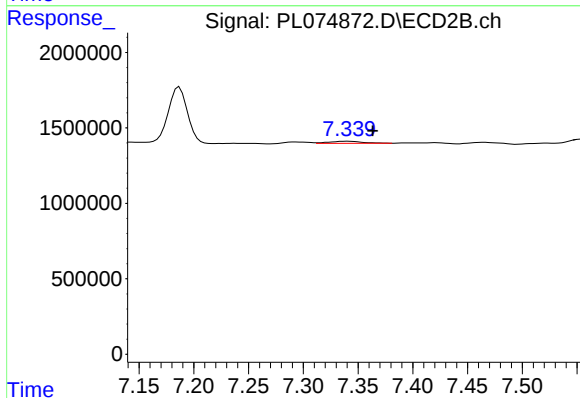


#10 gamma-Chlordane

R.T.: 7.341 min
Delta R.T.: -0.022 min
Response: 283456
Conc: 0.20 ng/ml

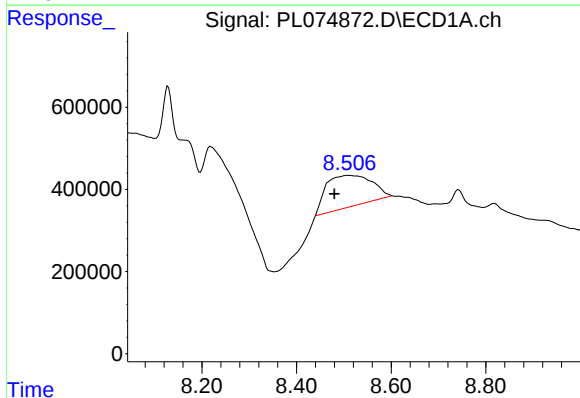


#11 alpha-Chlordane

R.T.: 8.508 min
Delta R.T.: 0.028 min
Response: 5235655
Conc: 8.58 ng/ml

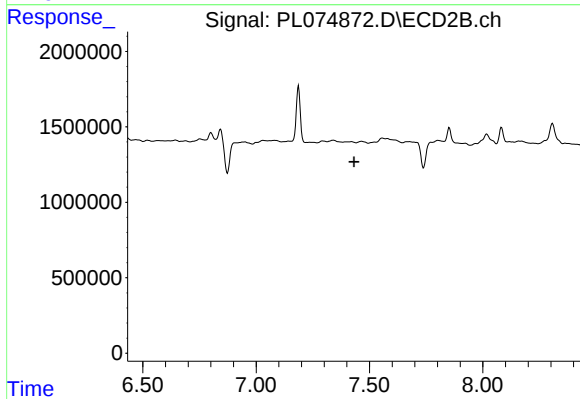

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.433 min
Response: 0
Conc: N.D.

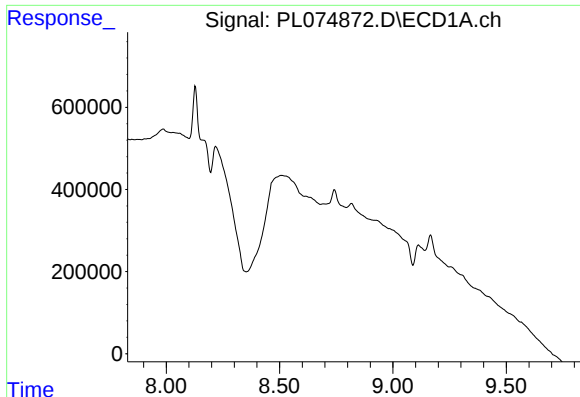

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.827 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

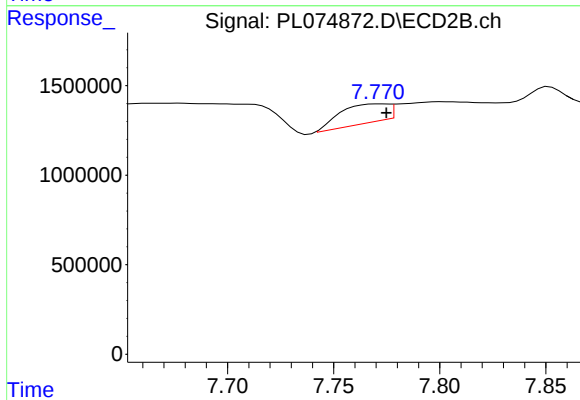


#13 Dieldrin

R.T.: 7.772 min
Delta R.T.: -0.003 min
Response: 1654114
Conc: 1.30 ng/ml

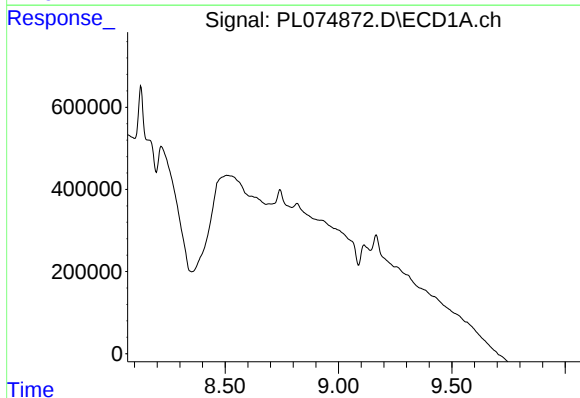


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.068 min
Response: 0
Conc: N.D.

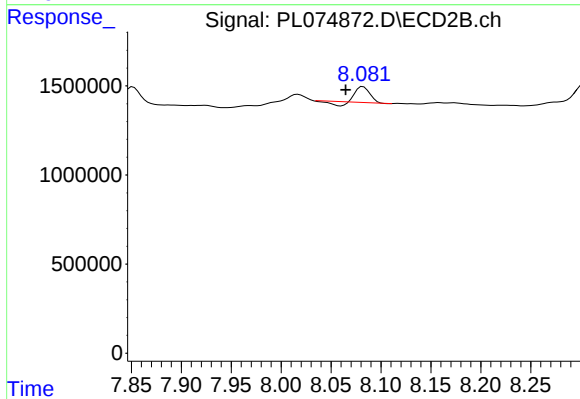

#14 Endrin


R.T.: 8.082 min
Delta R.T.: 0.017 min
Response: 685454
Conc: 0.65 ng/ml

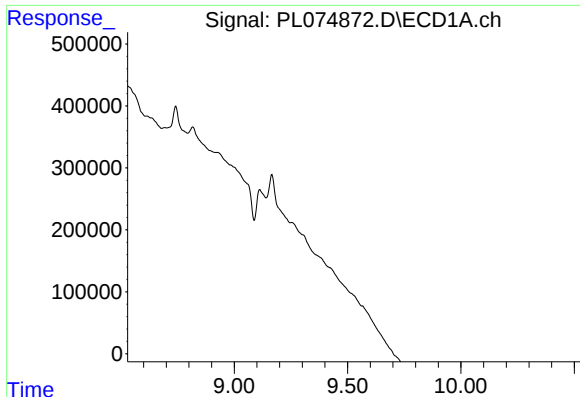

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.527 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

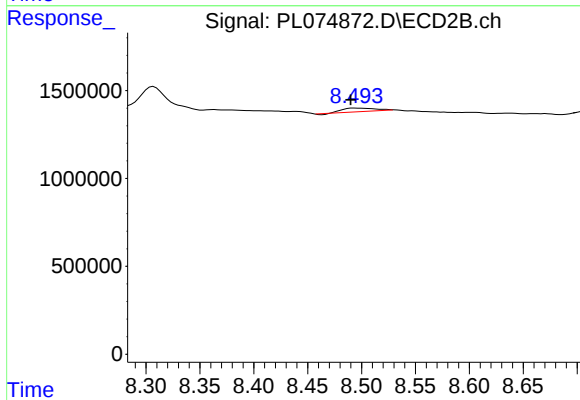


#17 4,4'-DDT

R.T.: 8.494 min
Delta R.T.: 0.004 min
Response: 427217
Conc: 0.43 ng/ml

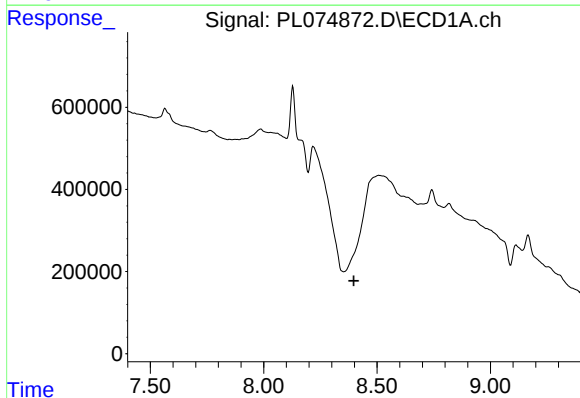


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

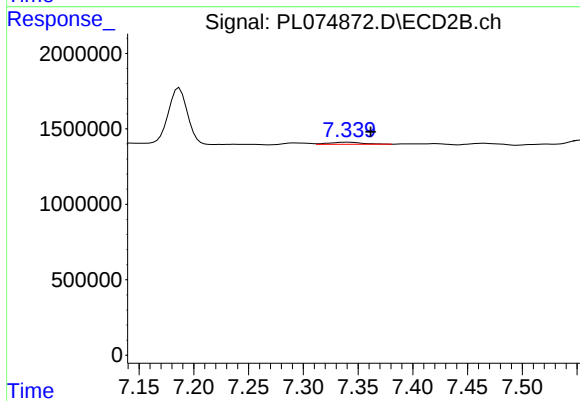

#25 Chlordane-3


R.T.: 7.341 min
Delta R.T.: -0.021 min
Response: 283456
Conc: 2.18 ng/ml

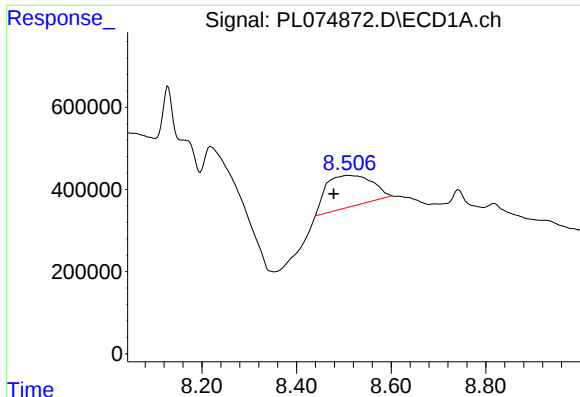

#26 Chlordane-4


R.T.: 8.508 min
Delta R.T.: 0.029 min
Response: 5235655
Conc: 54.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

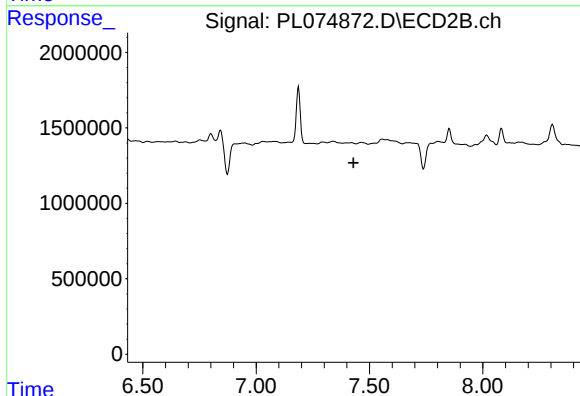


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.430 min
Response: 0
Conc: N.D.

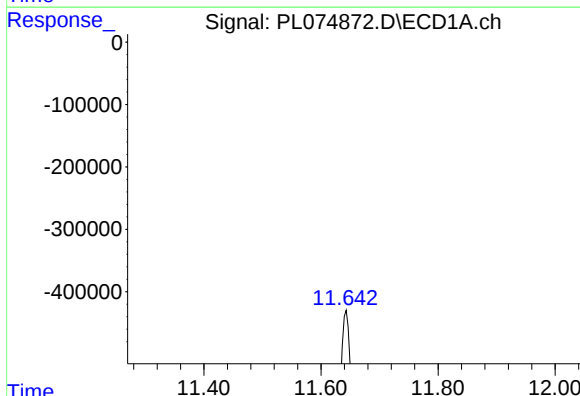

#28 Decachlorobiphenyl

R.T.: 11.644 min
Delta R.T.: -0.007 min
Response: 9865779
Conc: 22.09 ng/ml

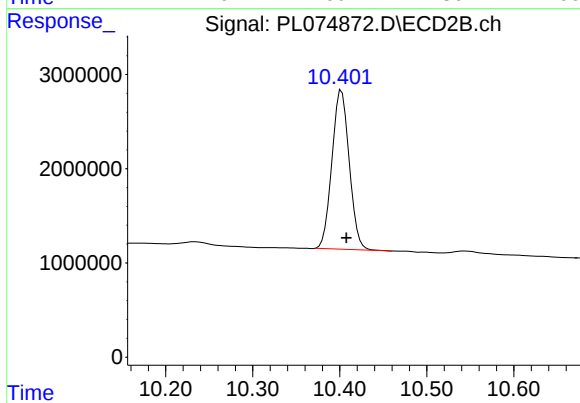

#28 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: -0.006 min
Response: 23292713
Conc: 22.69 ng/ml