

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051922\
 Data File : PL074847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2022 16:43
 Operator : AR\AJ
 Sample : N2906-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CDF-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 02:43:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.646	4.651	10787119	28854248	21.245	21.023
28)	SA Decachlor...	11.645	10.403	8602841	20868749	19.264	20.332
Target Compounds							
12)	B 4,4'-DDE	8.662	7.640	287397	866110	0.621	0.736



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051922\
Data File : PL074847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2022 16:43
Operator : AR\AJ
Sample : N2906-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CDF-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 02:43:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

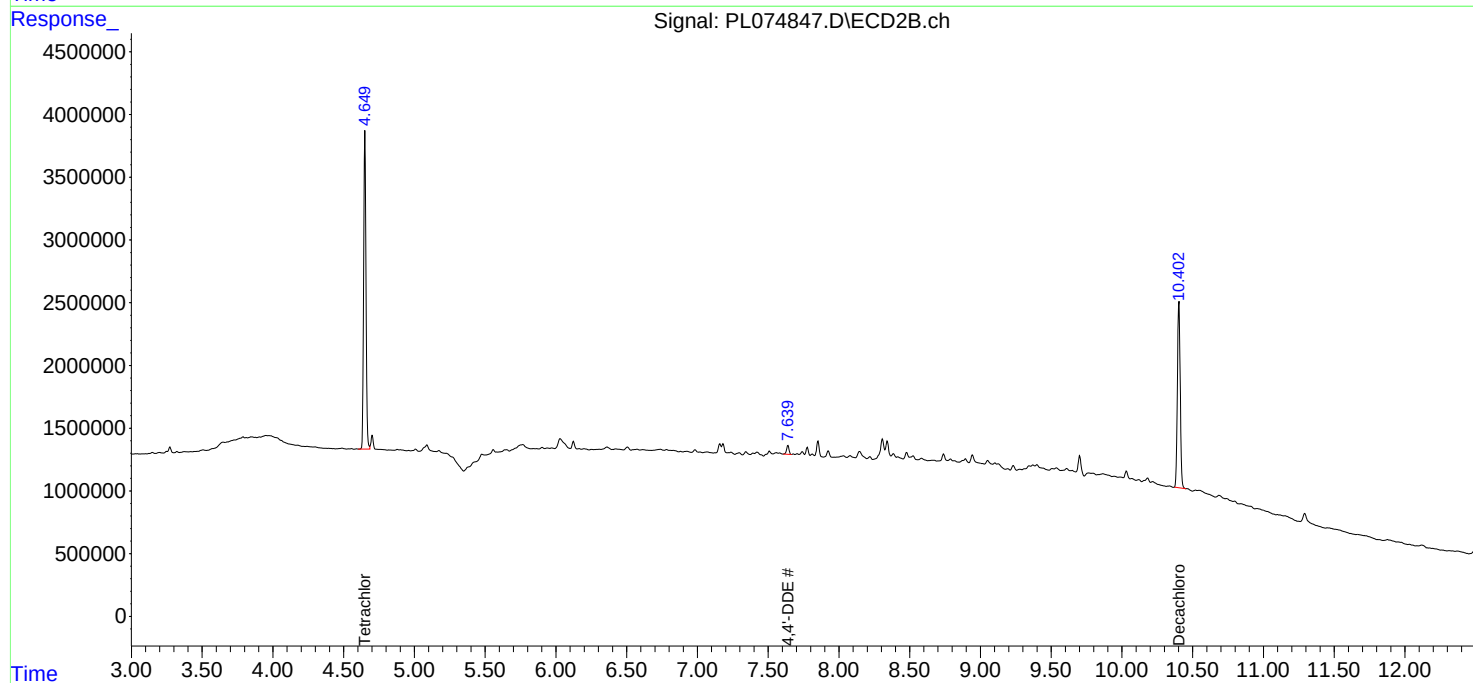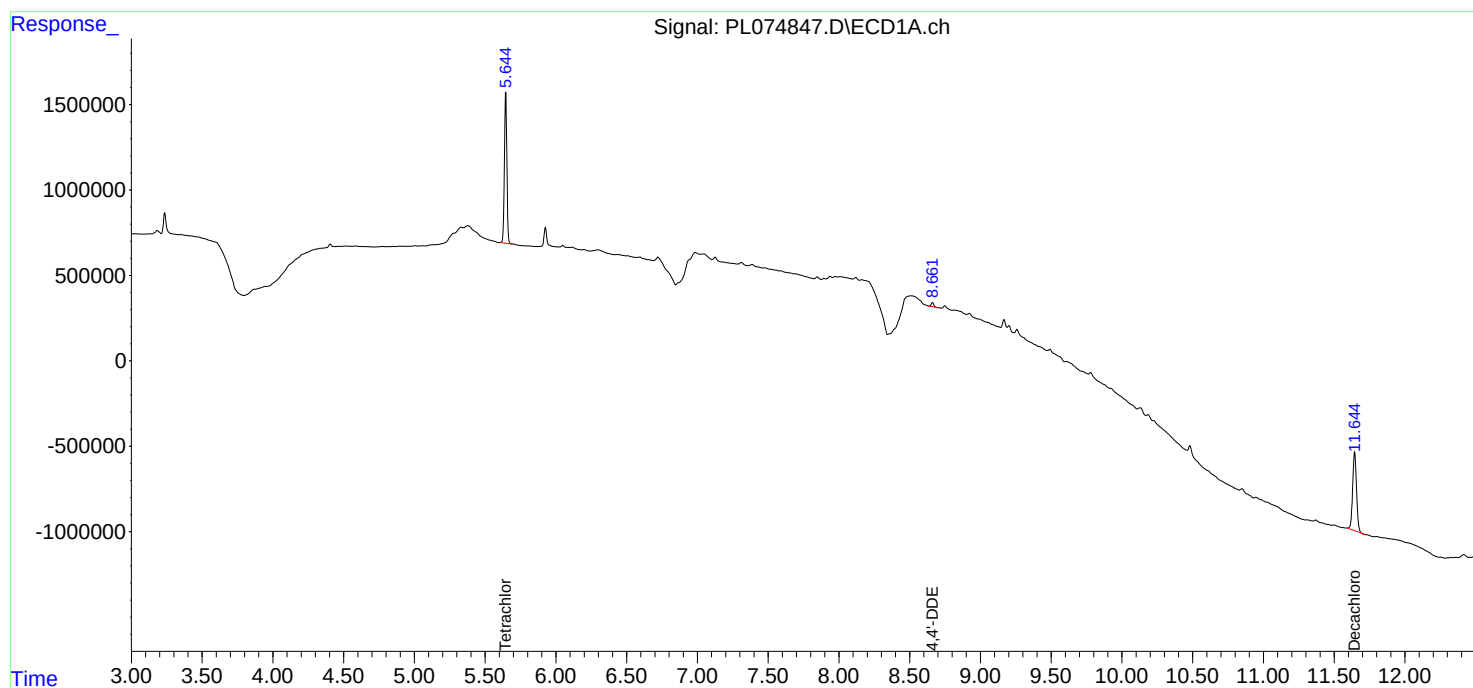


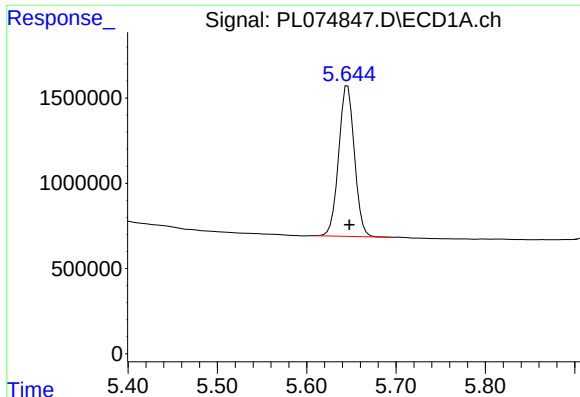

#1 Tetrachloro-m-xylene


R.T.: 5.646 min
Delta R.T.: -0.002 min
Response: 10787119
Conc: 21.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
CDF-1

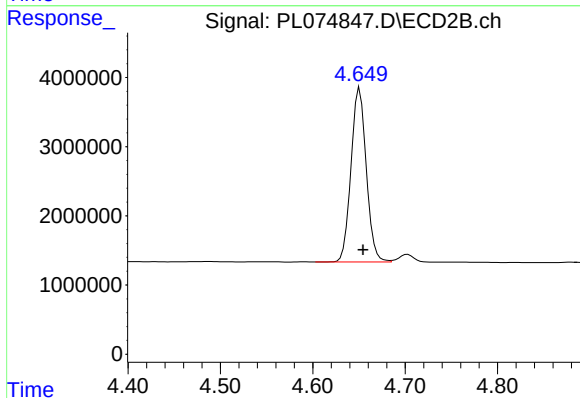


#1 Tetrachloro-m-xylene

R.T.: 4.651 min
Delta R.T.: -0.004 min
Response: 28854248
Conc: 21.02 ng/ml

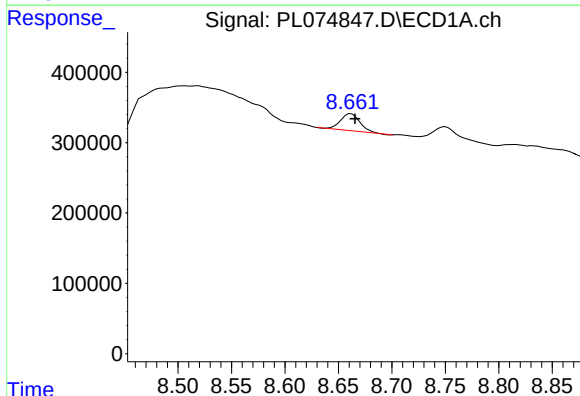


#12 4,4'-DDE

R.T.: 8.662 min
Delta R.T.: -0.004 min
Response: 287397
Conc: 0.62 ng/ml

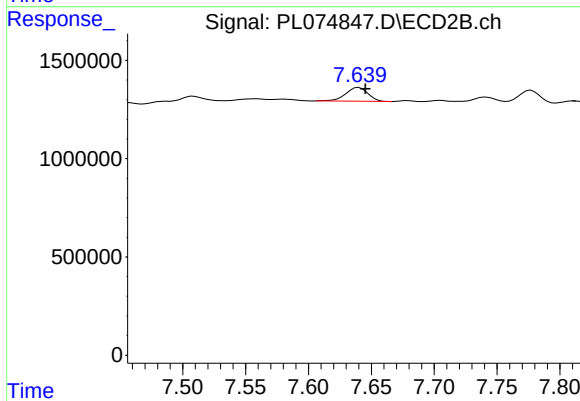

#12 4,4'-DDE


R.T.: 7.640 min
Delta R.T.: -0.005 min
Response: 866110
Conc: 0.74 ng/ml

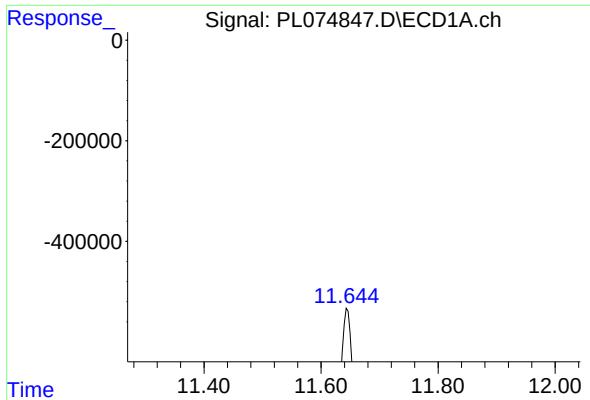

#28 Decachlorobiphenyl

R.T.: 11.645 min
Delta R.T.: -0.006 min
Response: 8602841
Conc: 19.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
CDF-1

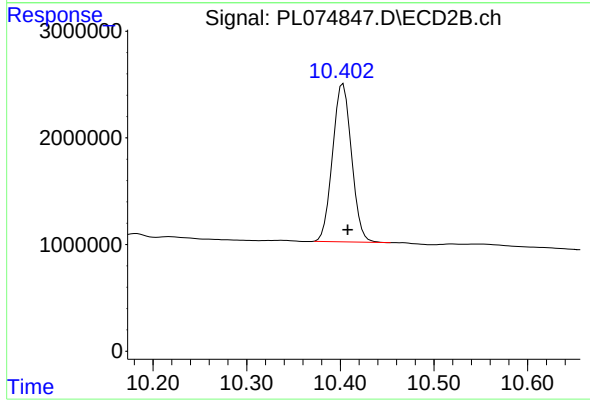

#28 Decachlorobiphenyl

R.T.: 10.403 min
Delta R.T.: -0.005 min
Response: 20868749
Conc: 20.33 ng/ml