

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051922\
 Data File : PL074866.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2022 22:37
 Operator : AR\AJ
 Sample : N2908-03
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-3

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/20/2022
 Supervised By : mohammad ahmed 05/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 02:52:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.646	4.651	2755050	7883757	5.426	5.744
28)	SA Decachlor...	11.644	10.402	5786964	14910395	12.958	14.527
Target Compounds							
12)	B 4,4'-DDE	8.660	7.639	258163	649648	0.558m	0.552

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051922\
Data File : PL074866.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2022 22:37
Operator : AR\AJ
Sample : N2908-03
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BI-3


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/20/2022
Supervised By : mohammad ahmed 05/20/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 02:52:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

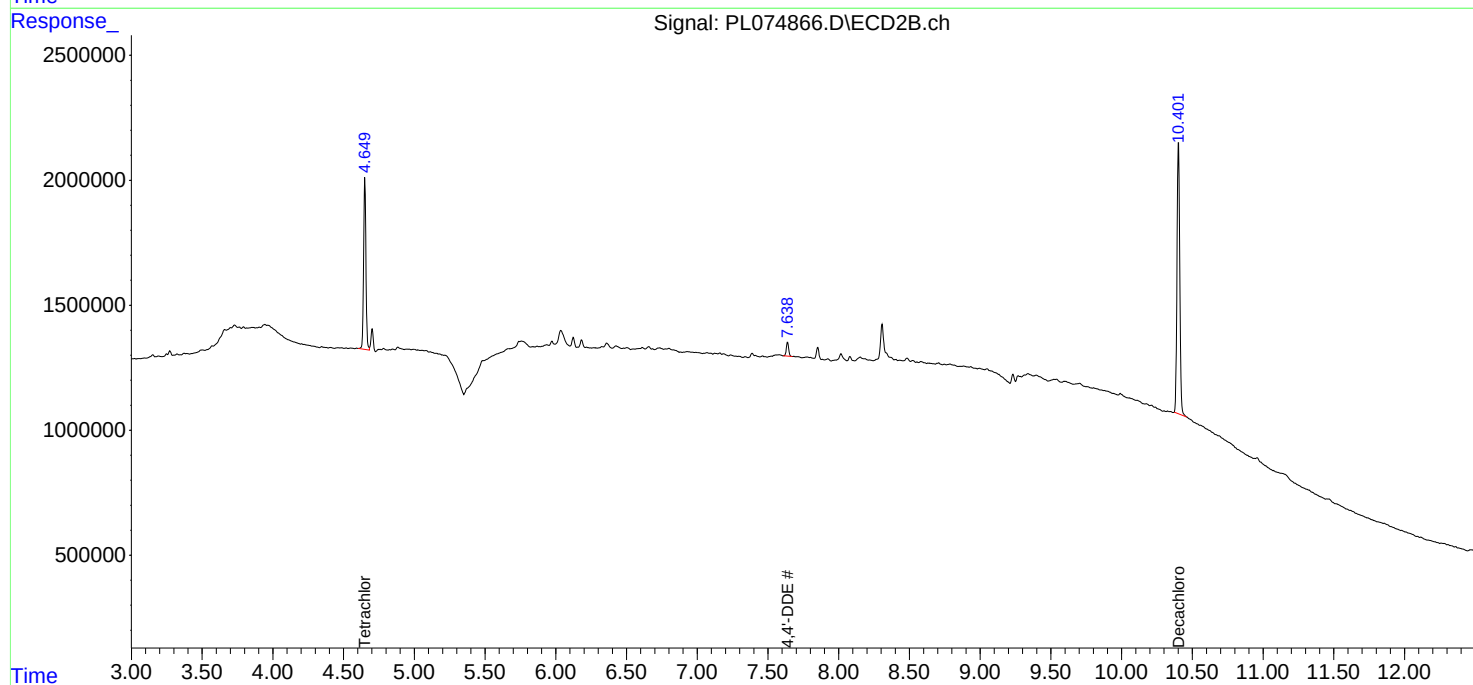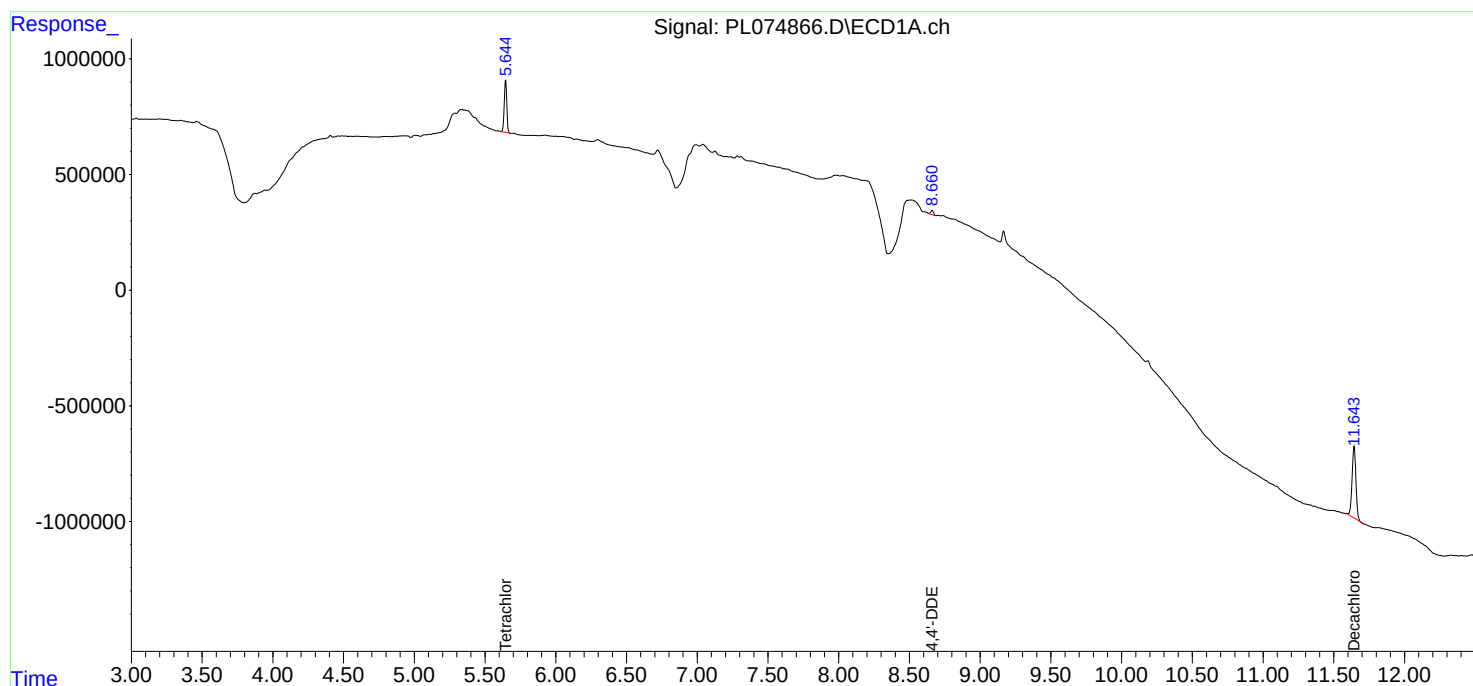

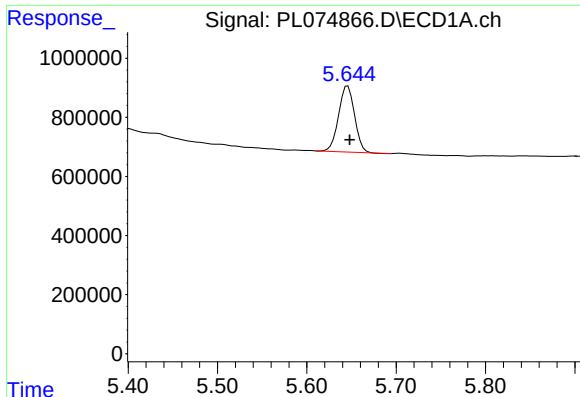


#1 Tetrachloro-m-xylene

R.T.: 5.646 min
Delta R.T.: -0.002 min
Response: 2755050
Conc: 5.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-3


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/20/2022
Supervised By :mohammad ahmed 05/20/2022

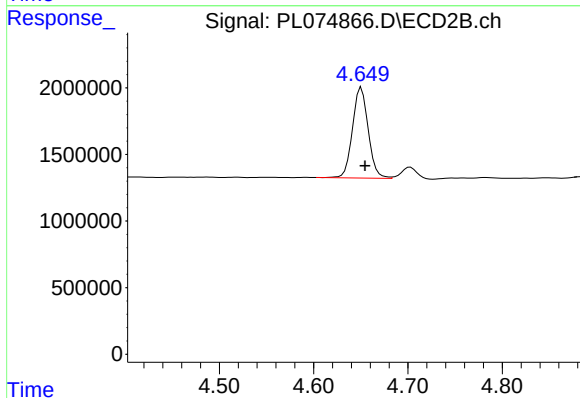


#1 Tetrachloro-m-xylene

R.T.: 4.651 min
Delta R.T.: -0.004 min
Response: 7883757
Conc: 5.74 ng/ml

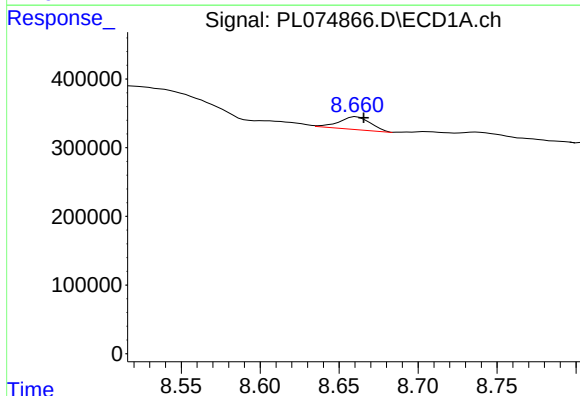


#12 4,4'-DDE

R.T.: 8.660 min
Delta R.T.: -0.006 min
Response: 258163
Conc: 0.56 ng/ml m

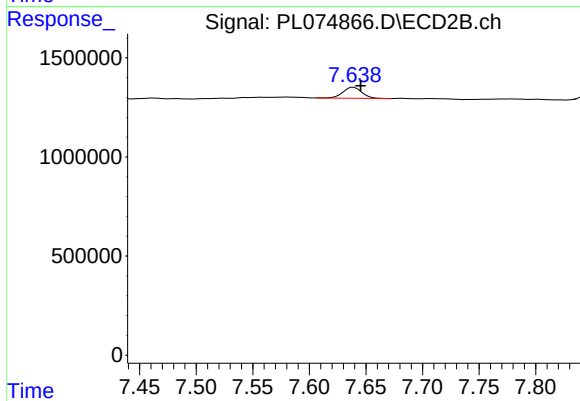

#12 4,4'-DDE

R.T.: 7.639 min
Delta R.T.: -0.006 min
Response: 649648
Conc: 0.55 ng/ml

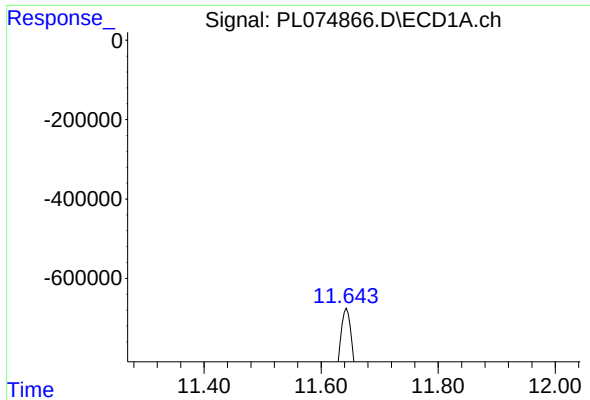


#28 Decachlorobiphenyl

R.T.: 11.644 min
Delta R.T.: -0.007 min
Response: 5786964
Conc: 12.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-3

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/20/2022
Supervised By :mohammad ahmed 05/20/2022

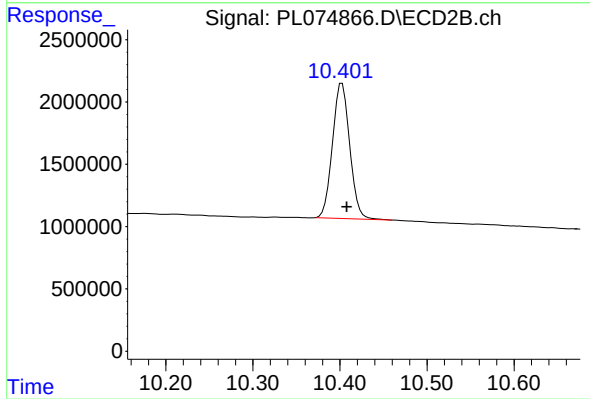

#28 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: -0.005 min
Response: 14910395
Conc: 14.53 ng/ml