

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051923\
 Data File : PL082813.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2023 14:41
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 04:24:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:23:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.317	2.637	180.2E6	205.5E6	76.089	75.623
28)	SA Decachlor...	8.733	7.744	114.5E6	142.5E6	69.577	71.892
Target Compounds							
23)	Chlordane-1	4.459	3.620	78519265	60939864	730.157	744.997
24)	Chlordane-2	4.986	4.193	80877574	64757071	732.912	731.784
25)	Chlordane-3	5.691	4.820	311.4E6	204.6E6	757.318	765.970
26)	Chlordane-4	5.772	4.880	377.7E6	212.9E6	752.526	757.418
27)	Chlordane-5	6.613	5.773	61267290	69804524	738.038	740.585



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051923\
Data File : PL082813.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2023 14:41
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 04:24:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:23:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

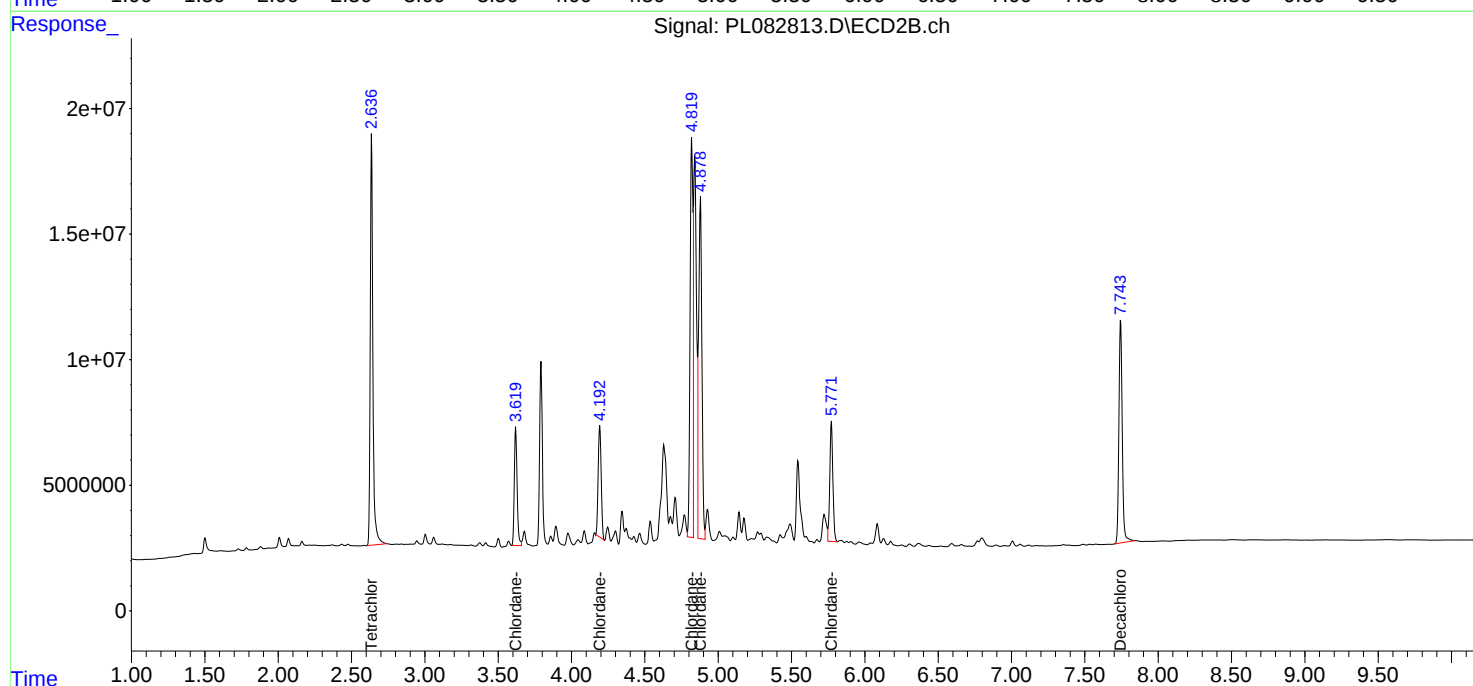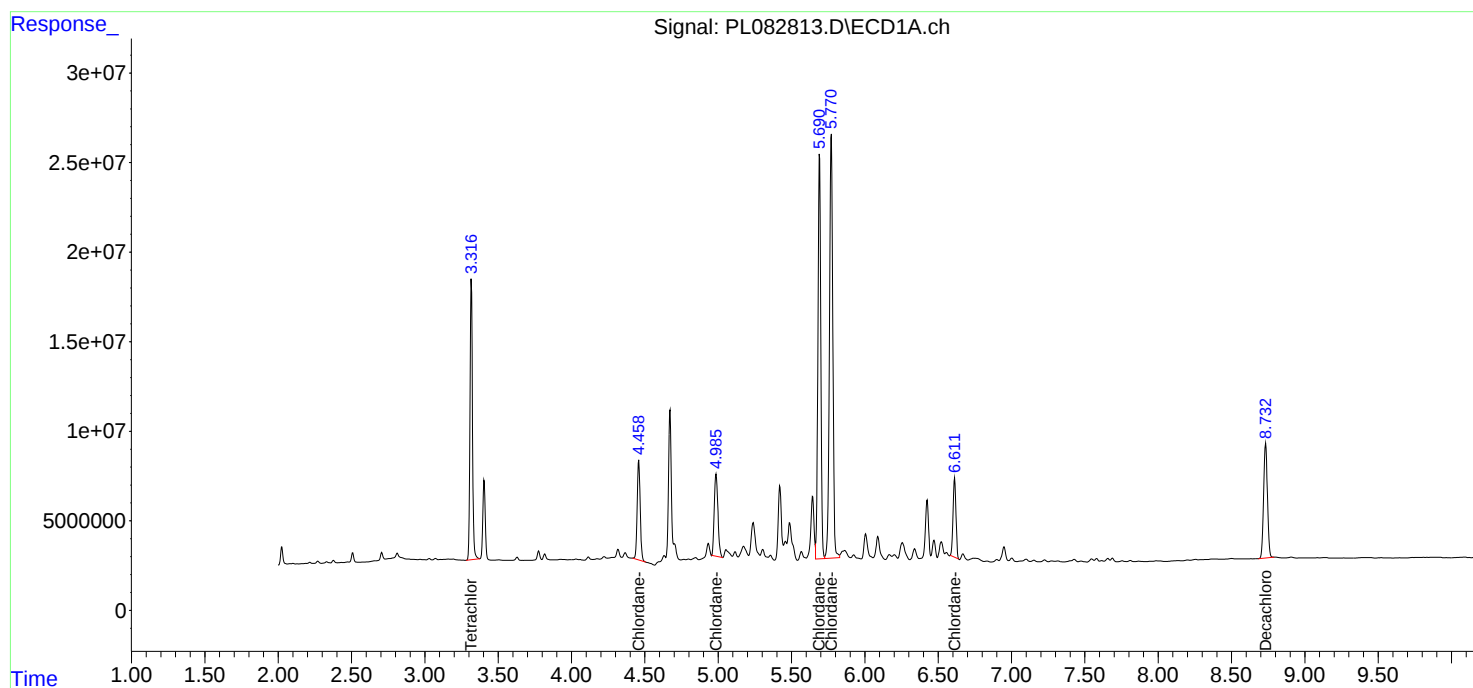


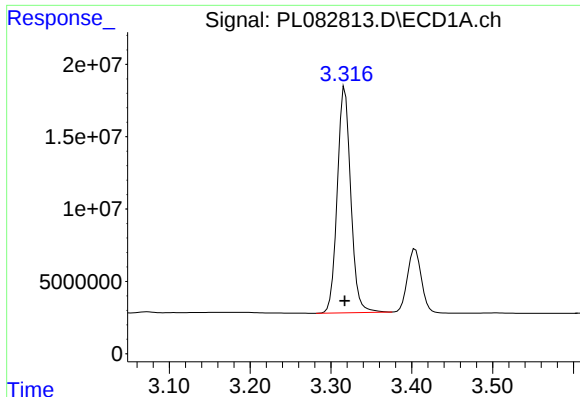

#1 Tetrachloro-m-xylene


R.T.: 3.317 min
Delta R.T.: 0.000 min
Response: 180209834
Conc: 76.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

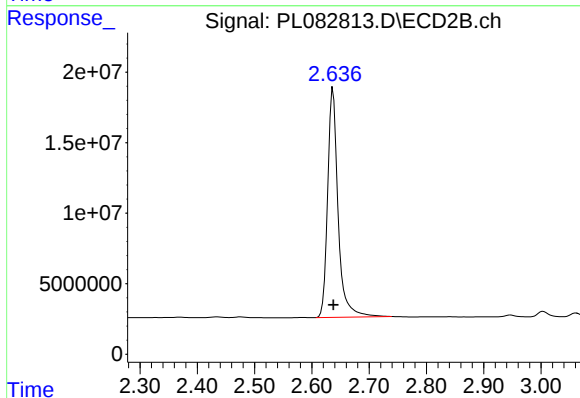


#1 Tetrachloro-m-xylene

R.T.: 2.637 min
Delta R.T.: 0.000 min
Response: 205524300
Conc: 75.62 ng/ml

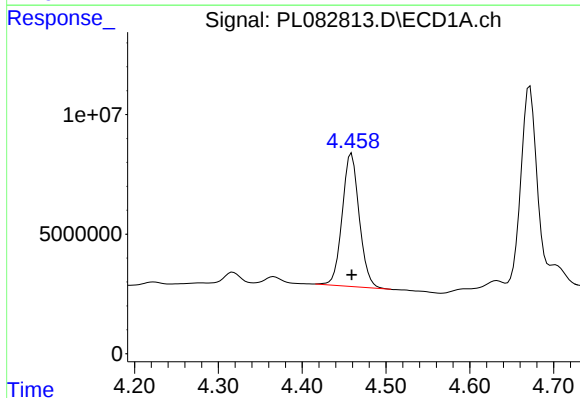


#23 Chlordane-1

R.T.: 4.459 min
Delta R.T.: 0.000 min
Response: 78519265
Conc: 730.16 ng/ml

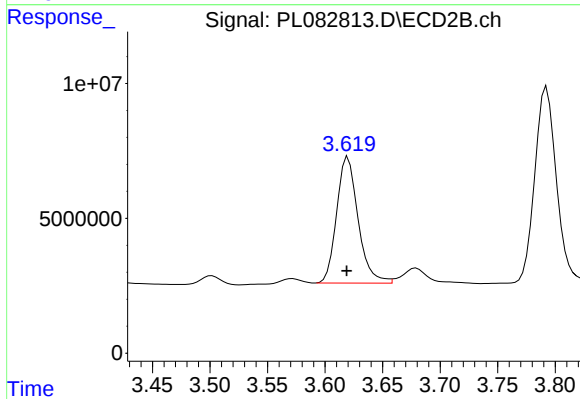

#23 Chlordane-1


R.T.: 3.620 min
Delta R.T.: 0.001 min
Response: 60939864
Conc: 745.00 ng/ml

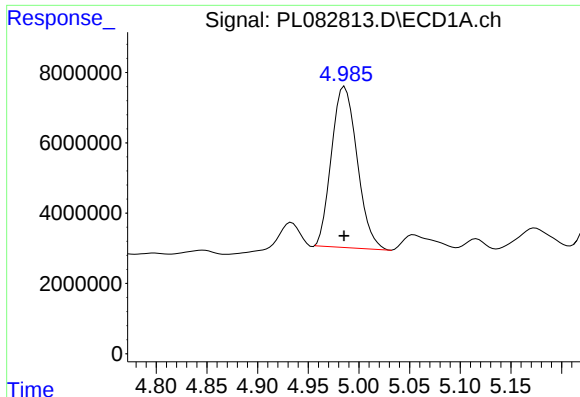

#24 Chlordane-2


R.T.: 4.986 min
Delta R.T.: 0.000 min
Response: 80877574
Conc: 732.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

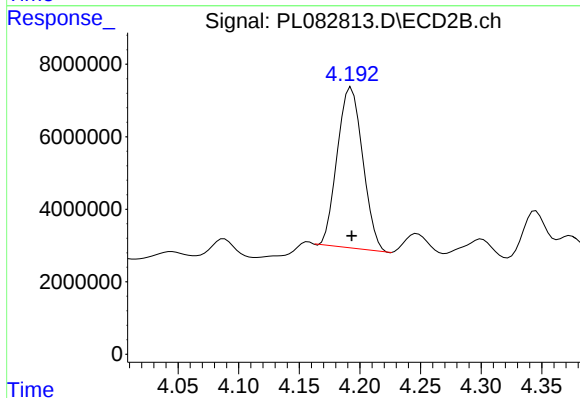


#24 Chlordane-2

R.T.: 4.193 min
Delta R.T.: 0.000 min
Response: 64757071
Conc: 731.78 ng/ml

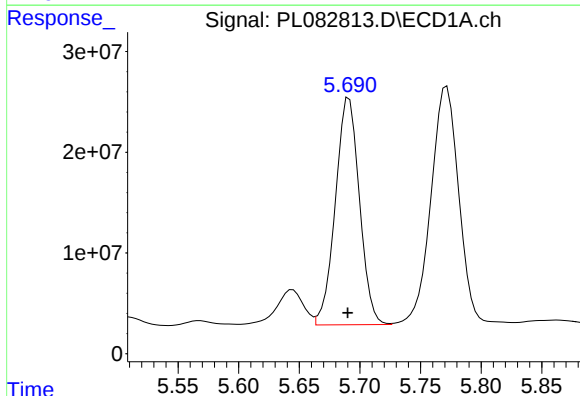


#25 Chlordane-3

R.T.: 5.691 min
Delta R.T.: 0.001 min
Response: 311400857
Conc: 757.32 ng/ml

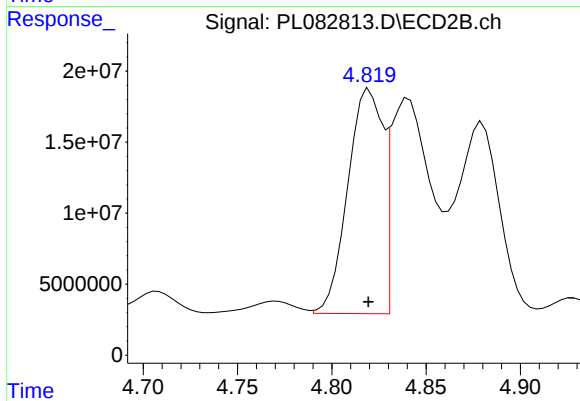

#25 Chlordane-3


R.T.: 4.820 min
Delta R.T.: 0.000 min
Response: 204612594
Conc: 765.97 ng/ml

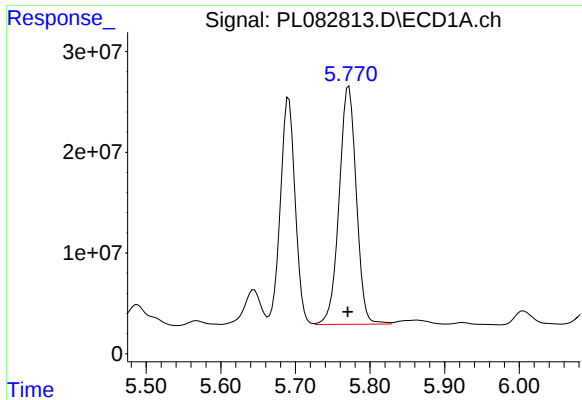

#26 Chlordane-4


R.T.: 5.772 min
Delta R.T.: 0.002 min
Response: 377650698
Conc: 752.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

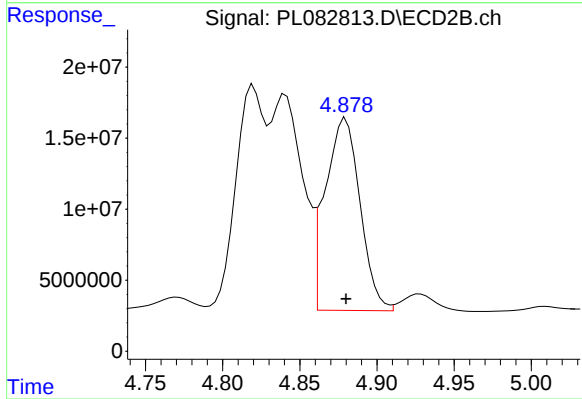


#26 Chlordane-4

R.T.: 4.880 min
Delta R.T.: 0.000 min
Response: 212850085
Conc: 757.42 ng/ml

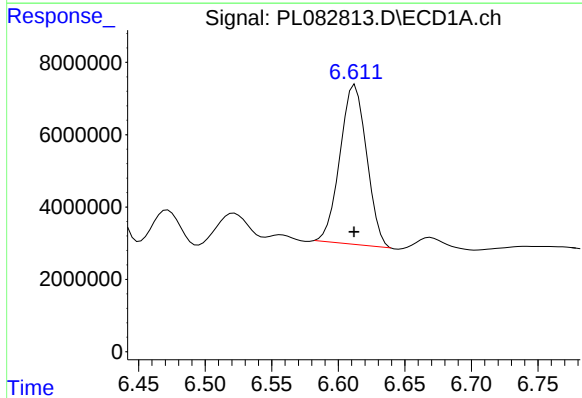


#27 Chlordane-5

R.T.: 6.613 min
Delta R.T.: 0.000 min
Response: 61267290
Conc: 738.04 ng/ml

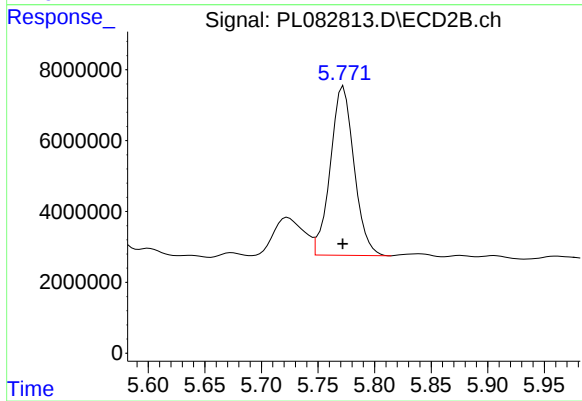

#27 Chlordane-5


R.T.: 5.773 min
Delta R.T.: 0.000 min
Response: 69804524
Conc: 740.59 ng/ml

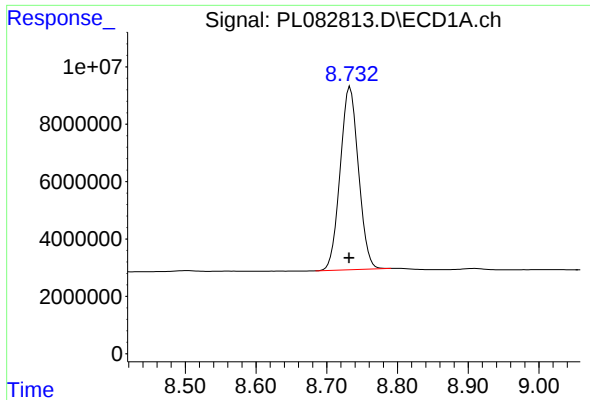

#28 Decachlorobiphenyl

R.T.: 8.733 min
Delta R.T.: 0.001 min
Response: 114545589
Conc: 69.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

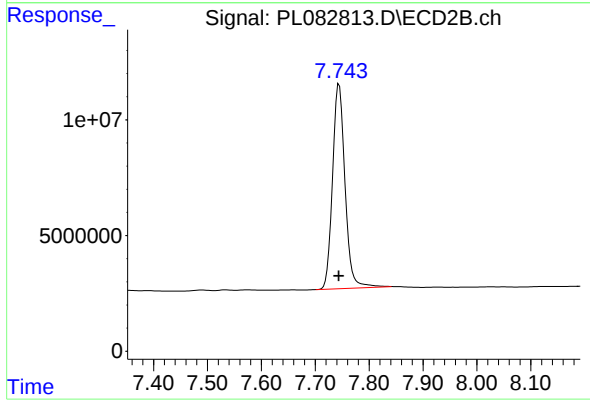

#28 Decachlorobiphenyl

R.T.: 7.744 min
Delta R.T.: 0.000 min
Response: 142547264
Conc: 71.89 ng/ml