

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051923\
 Data File : PL082814.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2023 14:55
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 04:25:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:23:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.317	2.638	118.4E6	135.9E6	50.000	50.000
28)	SA Decachlor...	8.732	7.743	82315292	99140079	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.459	3.620	53768745	40717836	500.000	497.780
24)	Chlordane-2	4.985	4.193	55175476	44246009	500.000	500.000
25)	Chlordane-3	5.690	4.819	205.6E6	133.6E6	500.000	500.000
26)	Chlordane-4	5.770	4.880	250.9E6	140.5E6	500.000	500.000
27)	Chlordane-5	6.612	5.772	41506839	47127932	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051923\
Data File : PL082814.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2023 14:55
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 04:25:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:23:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

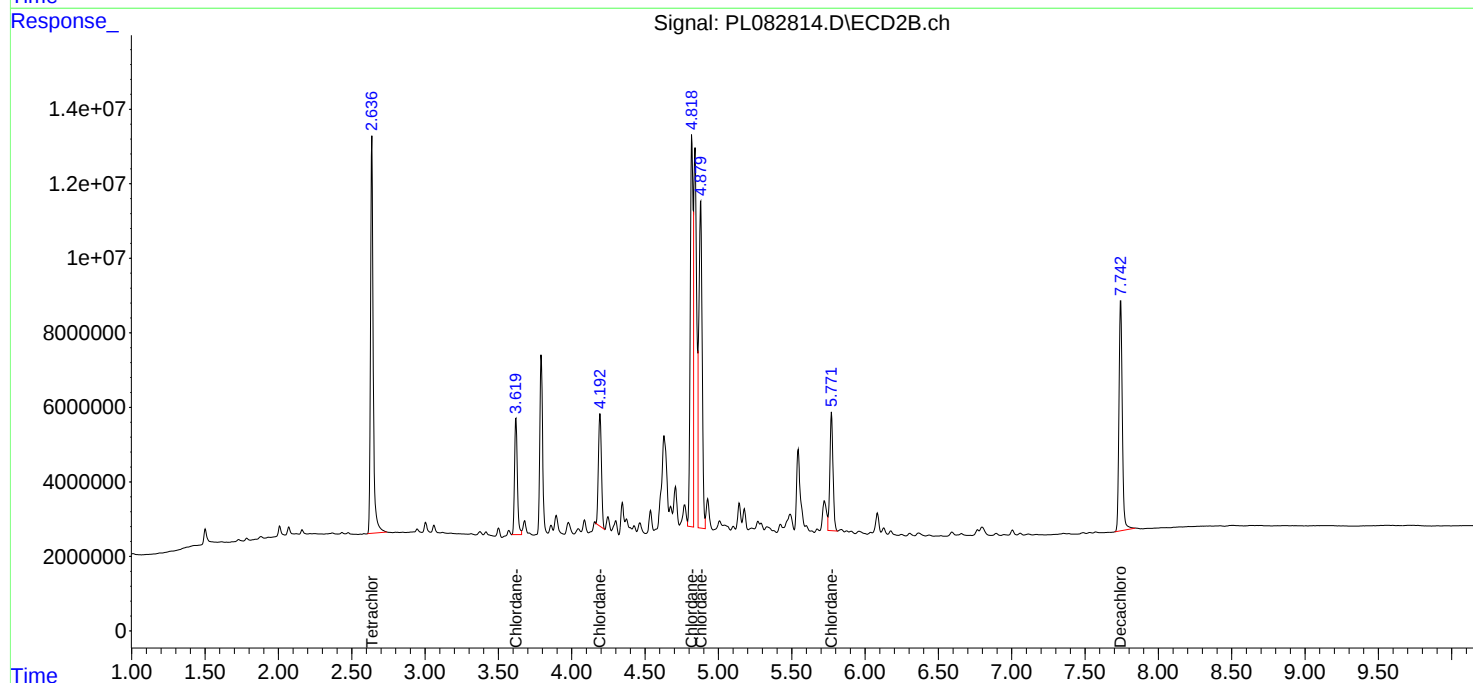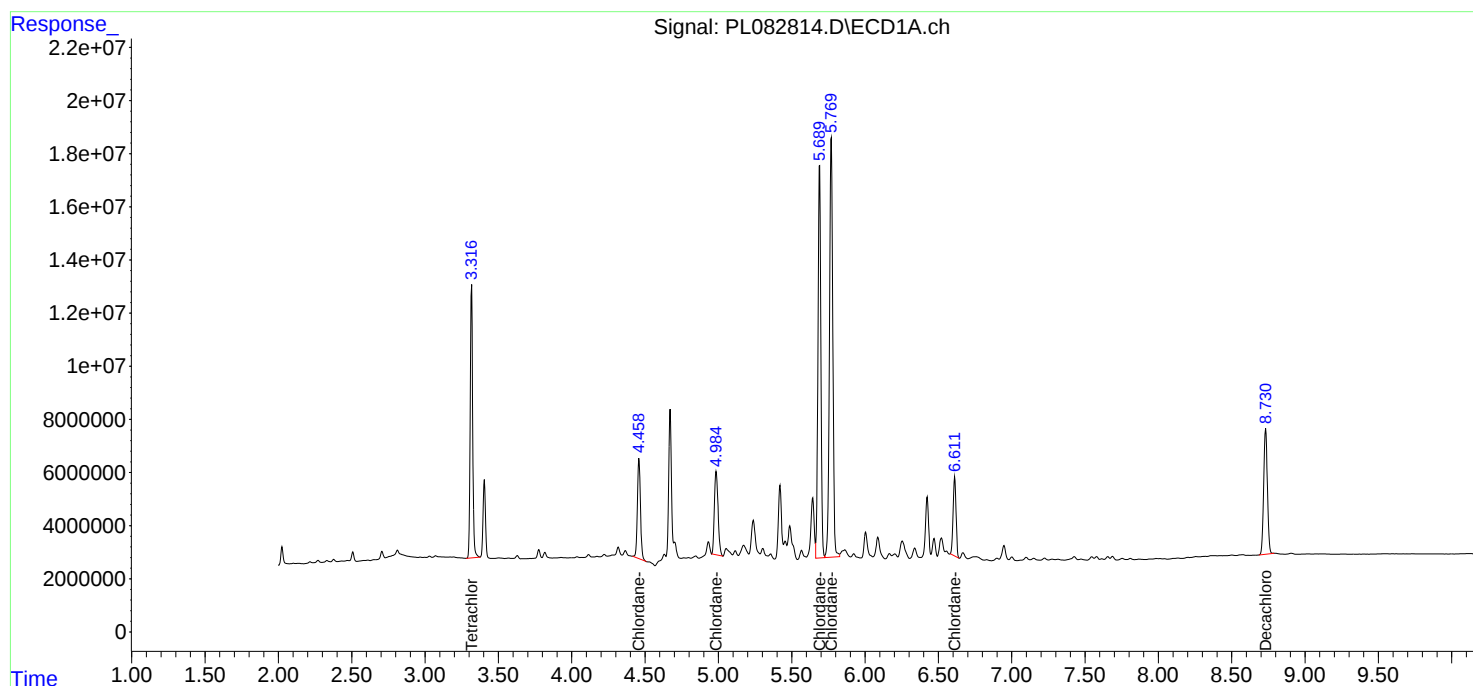


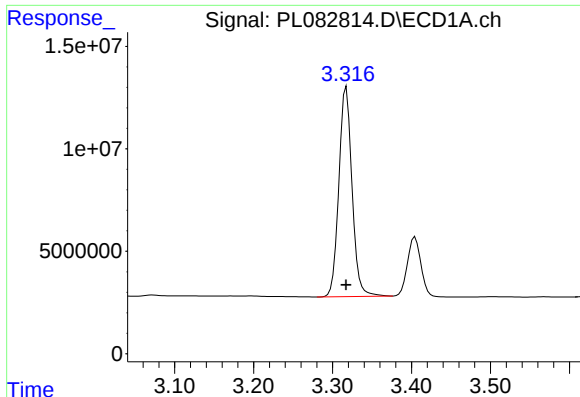

#1 Tetrachloro-m-xylene


R.T.: 3.317 min
Delta R.T.: 0.000 min
Response: 118420377
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

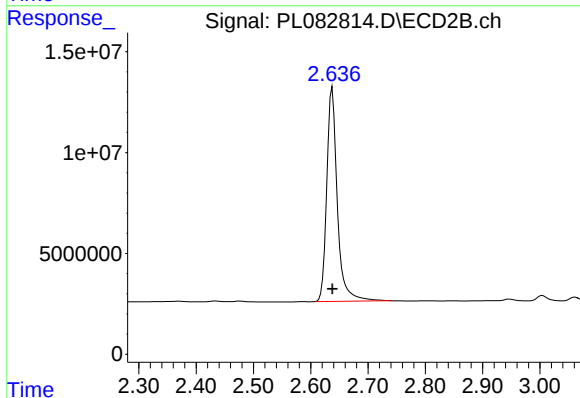


#1 Tetrachloro-m-xylene

R.T.: 2.638 min
Delta R.T.: 0.000 min
Response: 135887759
Conc: 50.00 ng/ml

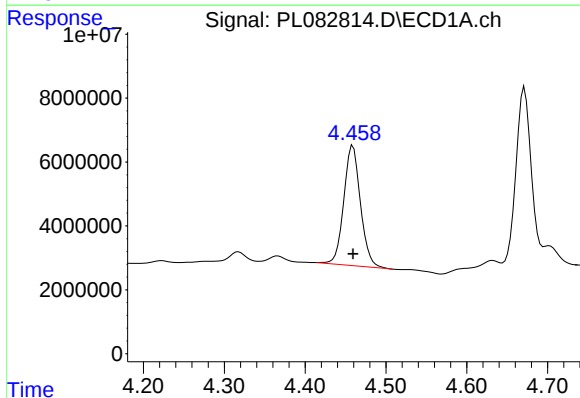


#23 Chlordane-1

R.T.: 4.459 min
Delta R.T.: 0.000 min
Response: 53768745
Conc: 500.00 ng/ml

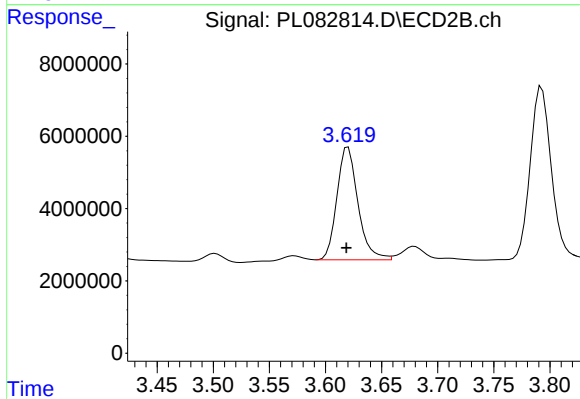

#23 Chlordane-1


R.T.: 3.620 min
Delta R.T.: 0.001 min
Response: 40717836
Conc: 497.78 ng/ml

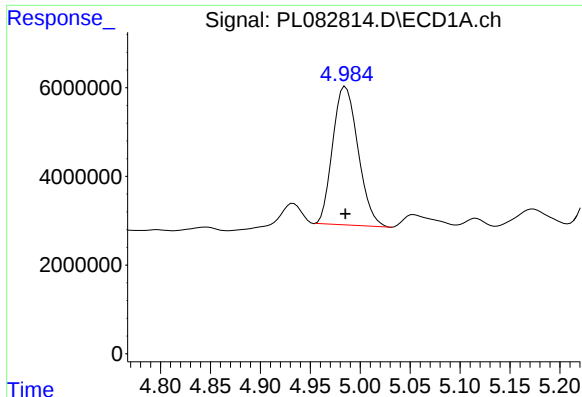

#24 Chlordane-2


R.T.: 4.985 min
Delta R.T.: 0.000 min
Response: 55175476
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

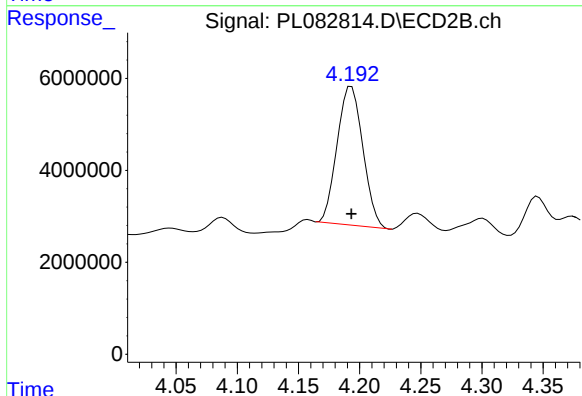


#24 Chlordane-2

R.T.: 4.193 min
Delta R.T.: 0.000 min
Response: 44246009
Conc: 500.00 ng/ml

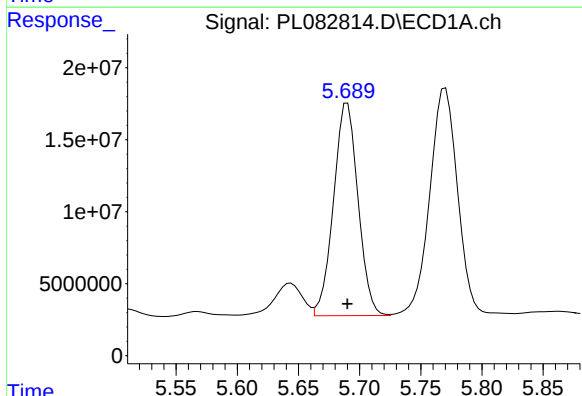


#25 Chlordane-3

R.T.: 5.690 min
Delta R.T.: 0.000 min
Response: 205594622
Conc: 500.00 ng/ml

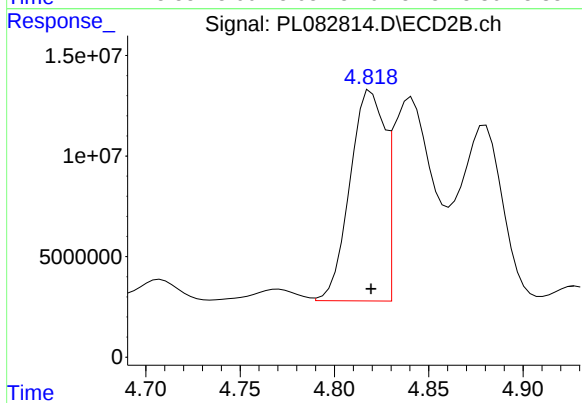

#25 Chlordane-3


R.T.: 4.819 min
Delta R.T.: 0.000 min
Response: 133564322
Conc: 500.00 ng/ml

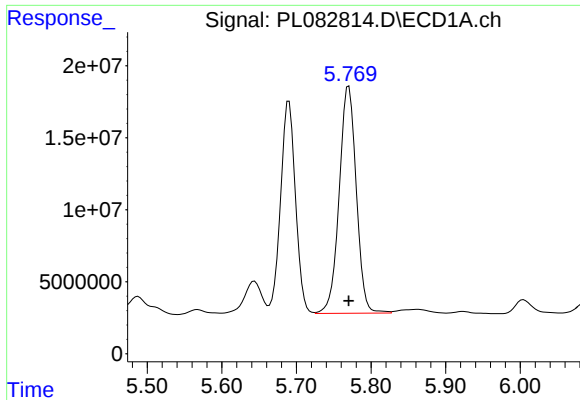

#26 Chlordane-4


R.T.: 5.770 min
Delta R.T.: 0.000 min
Response: 250922139
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

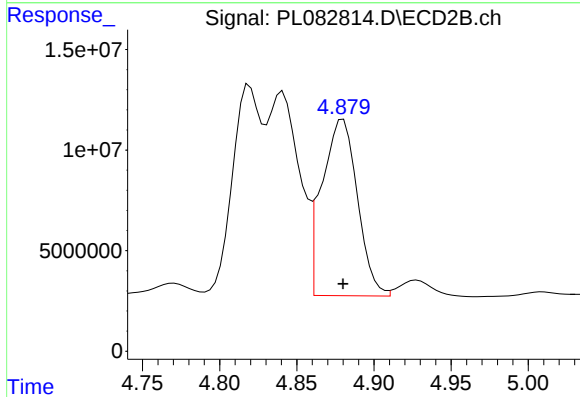


#26 Chlordane-4

R.T.: 4.880 min
Delta R.T.: 0.000 min
Response: 140510343
Conc: 500.00 ng/ml

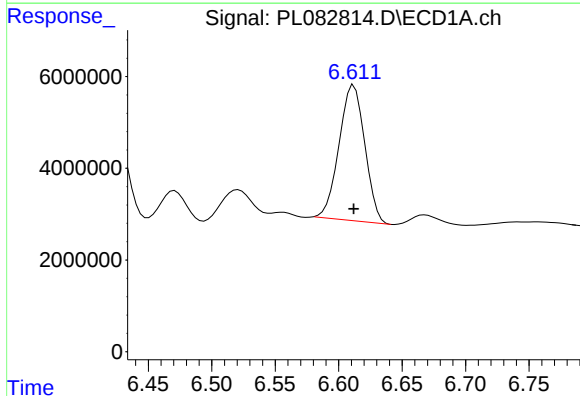


#27 Chlordane-5

R.T.: 6.612 min
Delta R.T.: 0.000 min
Response: 41506839
Conc: 500.00 ng/ml

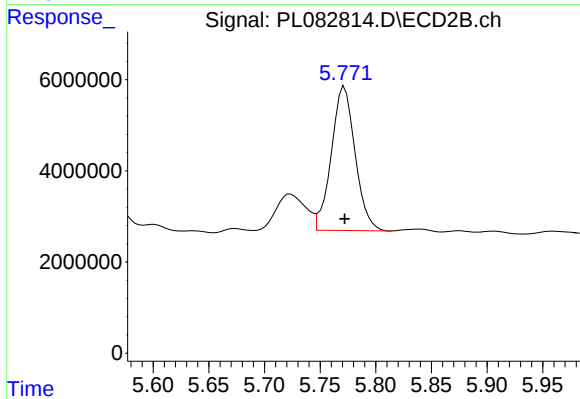

#27 Chlordane-5


R.T.: 5.772 min
Delta R.T.: 0.000 min
Response: 47127932
Conc: 500.00 ng/ml

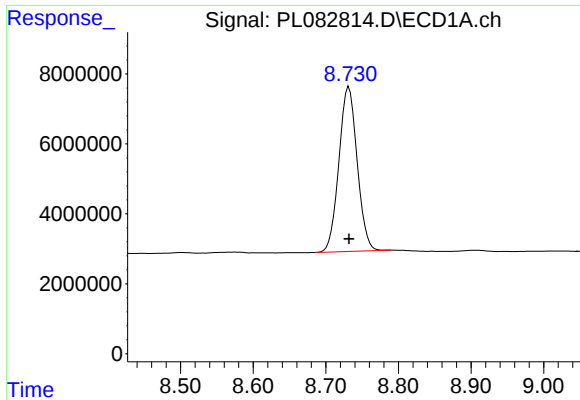

#28 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: 0.000 min
Response: 82315292
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

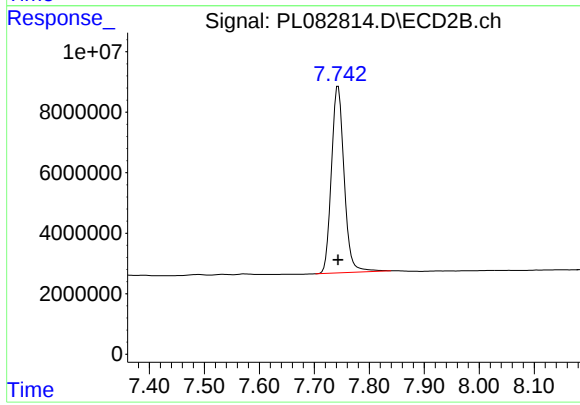

#28 Decachlorobiphenyl

R.T.: 7.743 min
Delta R.T.: 0.000 min
Response: 99140079
Conc: 50.00 ng/ml