

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051923\
 Data File : PL082815.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2023 15:09
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 04:25:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:23:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	2.637	61206757	69214442	25.843	25.468
28)	SA Decachlor...	8.732	7.744	44665104	53389963	27.131	26.927
Target Compounds							
23)	Chlordane-1	4.458	3.620	29529661	21076576	274.599	257.663
24)	Chlordane-2	4.985	4.193	29627759	23310990	268.487	263.425
25)	Chlordane-3	5.689	4.819	104.8E6	65972885	254.822	246.970
26)	Chlordane-4	5.770	4.880	129.4E6	70935104	257.761	252.420
27)	Chlordane-5	6.611	5.772	21938640	24442407	264.277	259.320



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051923\
Data File : PL082815.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2023 15:09
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 04:25:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:23:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

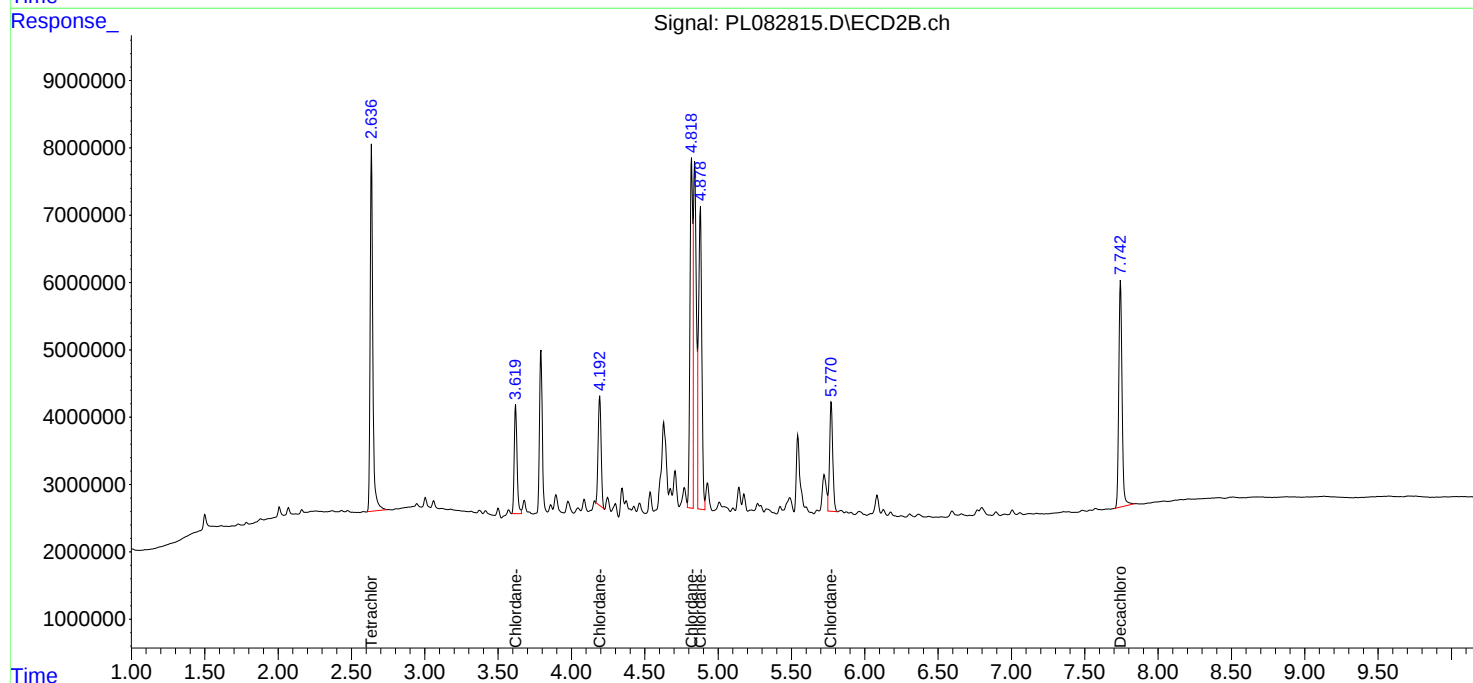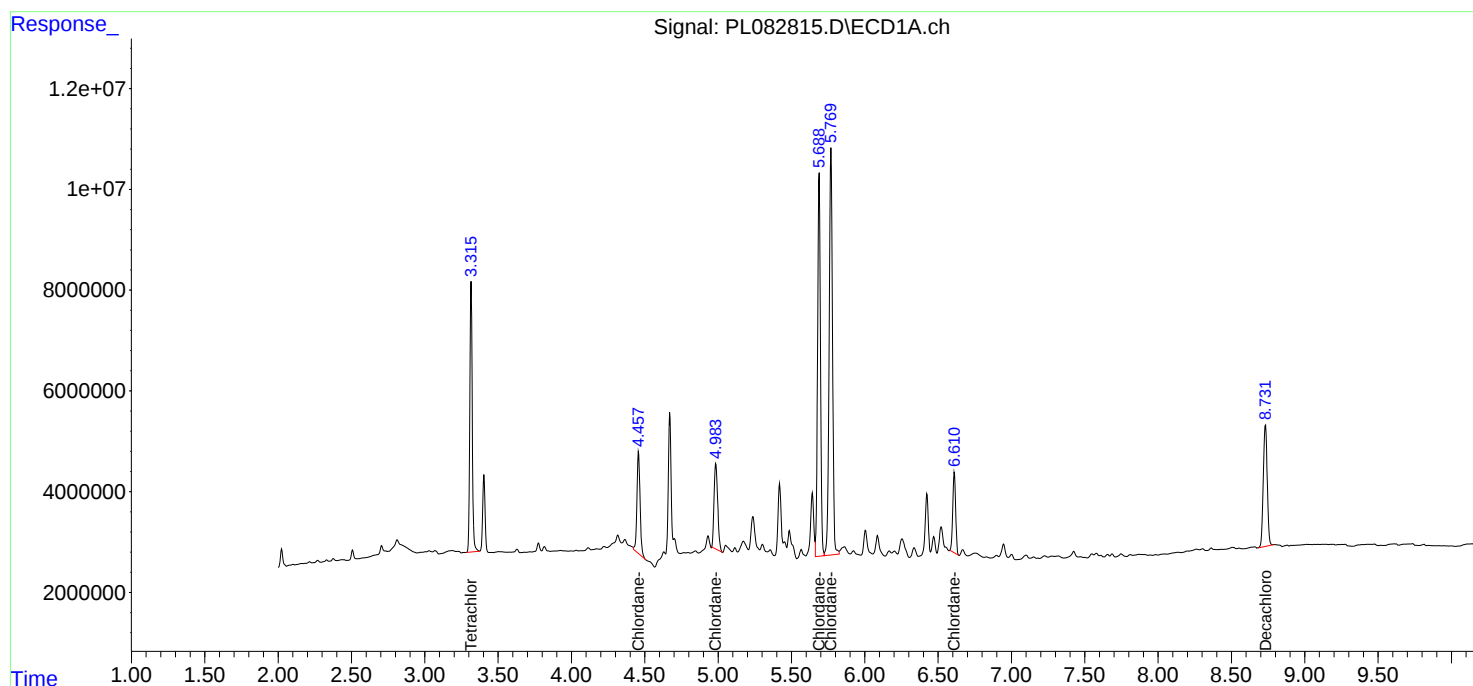


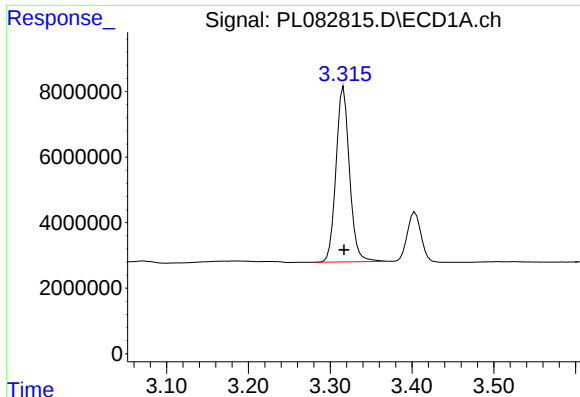

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: 0.000 min
Response: 61206757
Conc: 25.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

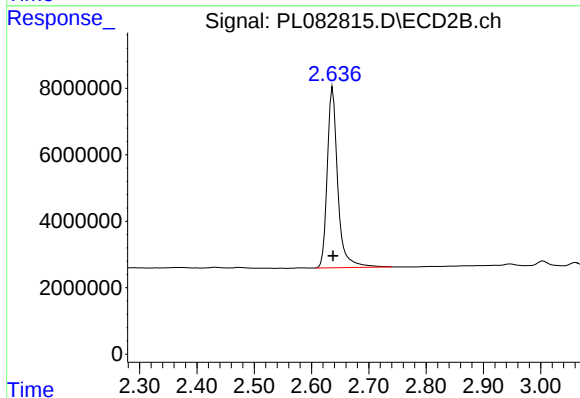


#1 Tetrachloro-m-xylene

R.T.: 2.637 min
Delta R.T.: 0.000 min
Response: 69214442
Conc: 25.47 ng/ml

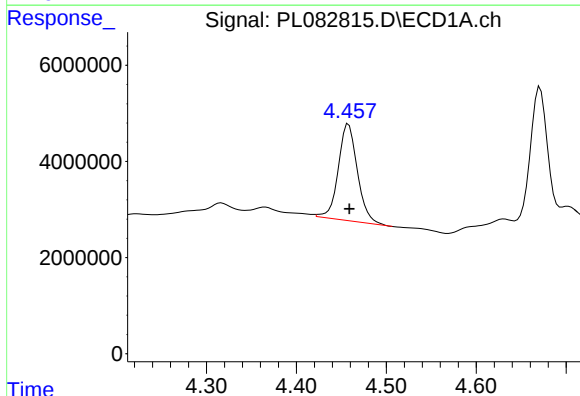


#23 Chlordane-1

R.T.: 4.458 min
Delta R.T.: -0.001 min
Response: 29529661
Conc: 274.60 ng/ml

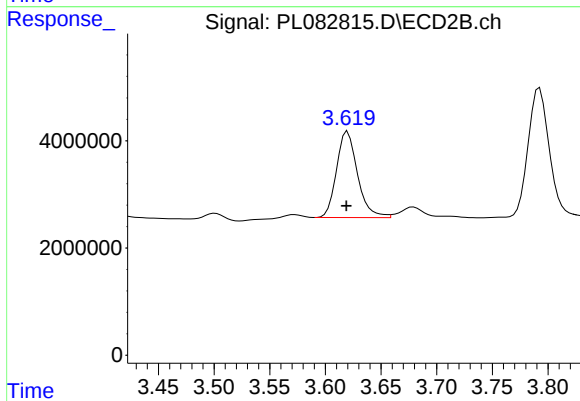

#23 Chlordane-1


R.T.: 3.620 min
Delta R.T.: 0.001 min
Response: 21076576
Conc: 257.66 ng/ml

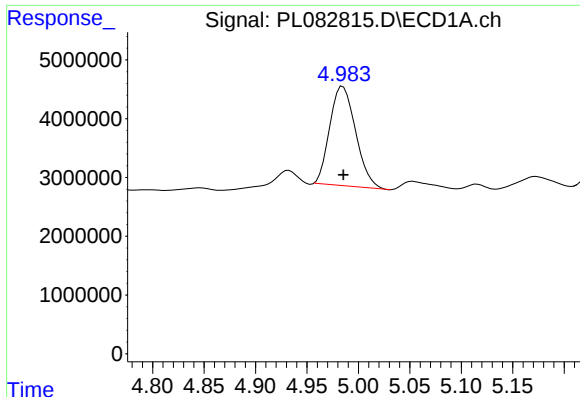

#24 Chlordane-2


R.T.: 4.985 min
Delta R.T.: 0.000 min
Response: 29627759
Conc: 268.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

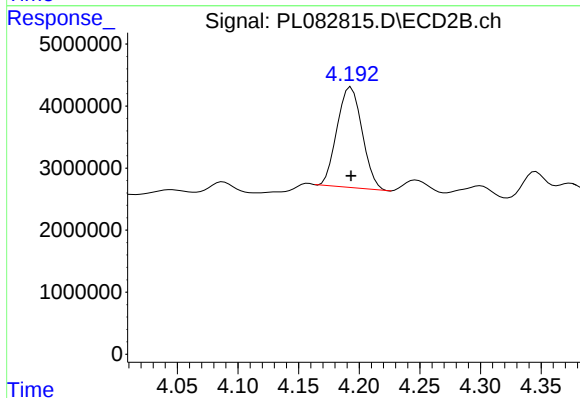


#24 Chlordane-2

R.T.: 4.193 min
Delta R.T.: 0.000 min
Response: 23310990
Conc: 263.42 ng/ml

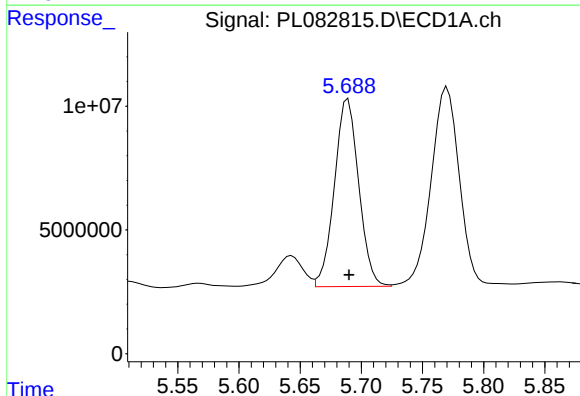


#25 Chlordane-3

R.T.: 5.689 min
Delta R.T.: 0.000 min
Response: 104780237
Conc: 254.82 ng/ml

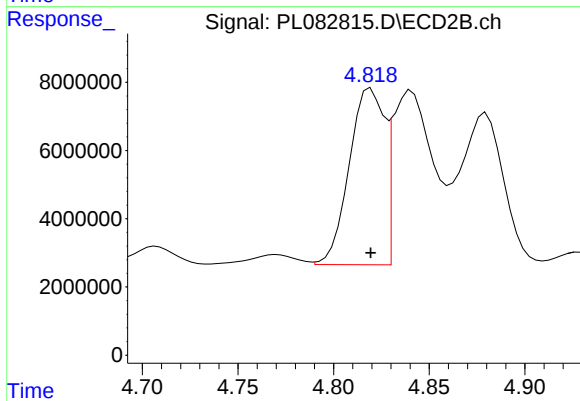

#25 Chlordane-3


R.T.: 4.819 min
Delta R.T.: 0.000 min
Response: 65972885
Conc: 246.97 ng/ml

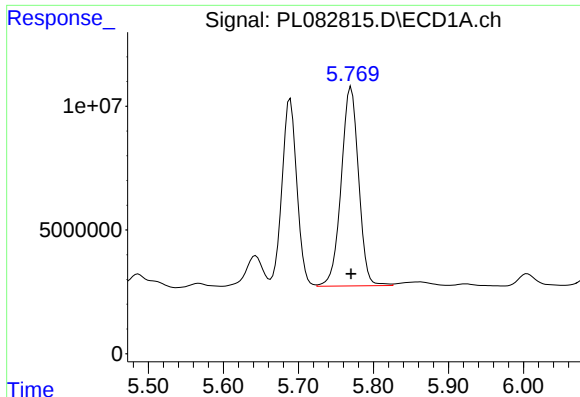

#26 Chlordane-4


R.T.: 5.770 min
Delta R.T.: 0.000 min
Response: 129356128
Conc: 257.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

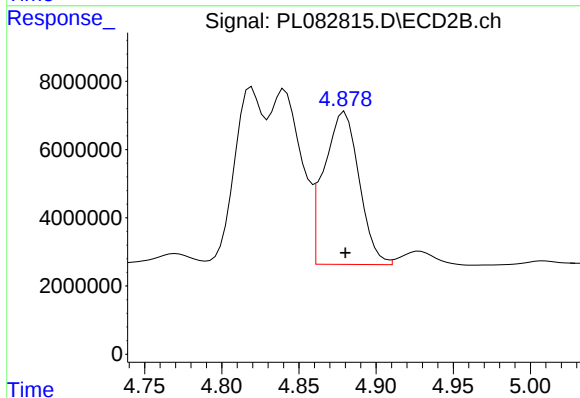


#26 Chlordane-4

R.T.: 4.880 min
Delta R.T.: 0.000 min
Response: 70935104
Conc: 252.42 ng/ml

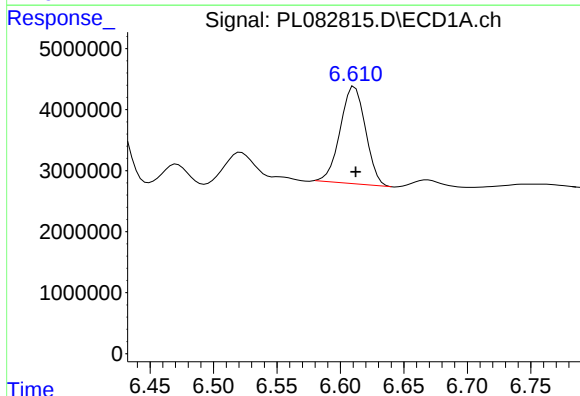


#27 Chlordane-5

R.T.: 6.611 min
Delta R.T.: 0.000 min
Response: 21938640
Conc: 264.28 ng/ml

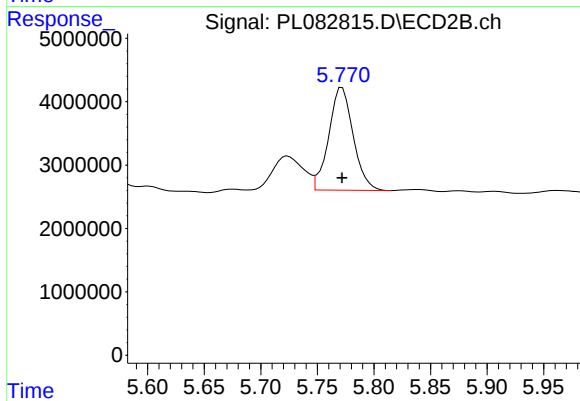

#27 Chlordane-5


R.T.: 5.772 min
Delta R.T.: 0.000 min
Response: 24442407
Conc: 259.32 ng/ml

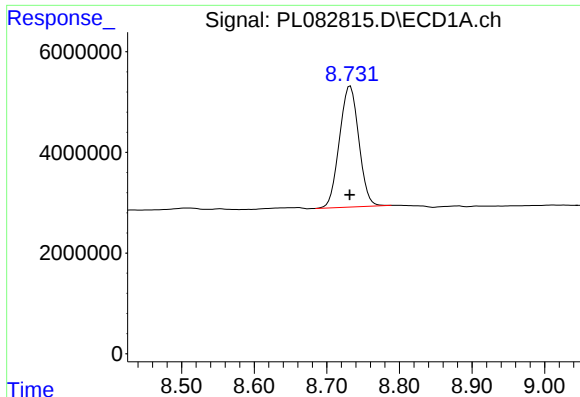

#28 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: 0.000 min
Response: 44665104
Conc: 27.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

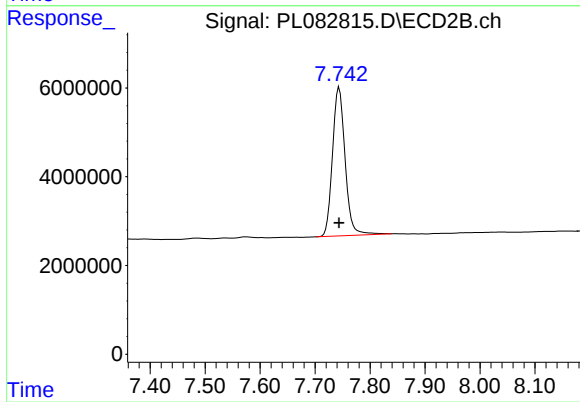

#28 Decachlorobiphenyl

R.T.: 7.744 min
Delta R.T.: 0.000 min
Response: 53389963
Conc: 26.93 ng/ml