

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051923\
 Data File : PL082816.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2023 15:23
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 04:25:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:23:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.317	2.637	11247864	12029572	4.749	4.426
28)	SA Decachlor...	8.731	7.744	9814996	11281285	5.962	5.690
Target Compounds							
23)	Chlordane-1	4.457	3.620	5819052	3922920	54.112	47.958
24)	Chlordane-2	4.985	4.193	5142730	4525366	46.603	51.139
25)	Chlordane-3	5.690	4.819	21258349	11747287	51.700	43.976
26)	Chlordane-4	5.771	4.880	26263529	12692069	52.334	45.164
27)	Chlordane-5	6.611	5.772	3567252	5002215	42.972	53.071



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051923\
Data File : PL082816.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2023 15:23
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 04:25:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:23:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

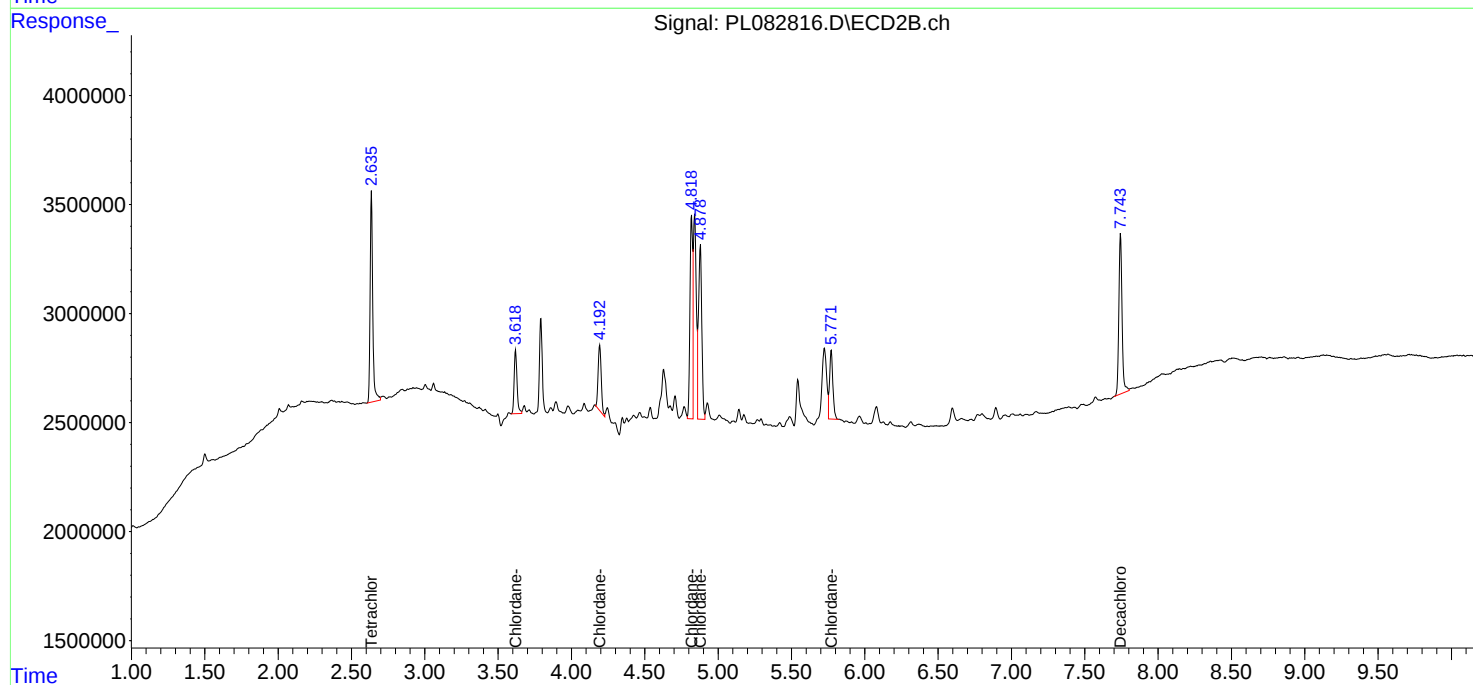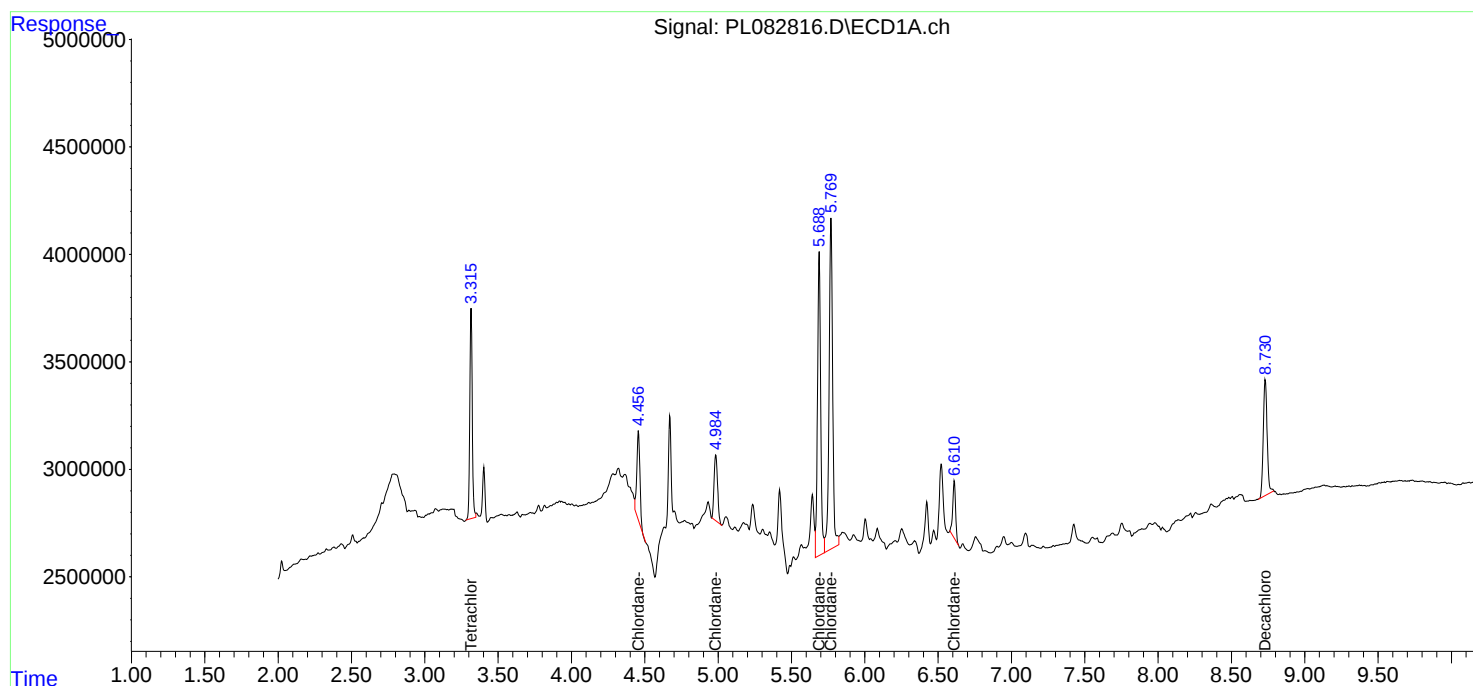


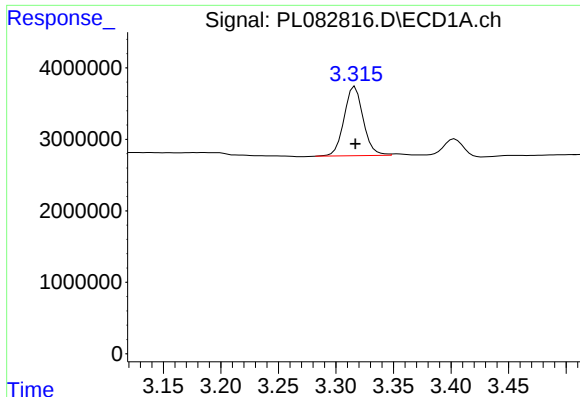

#1 Tetrachloro-m-xylene


R.T.: 3.317 min
Delta R.T.: 0.000 min
Response: 11247864
Conc: 4.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

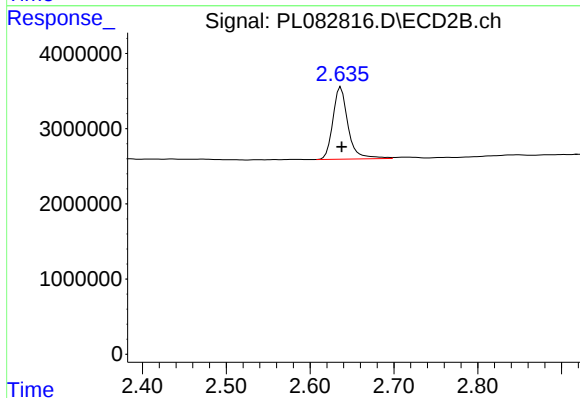


#1 Tetrachloro-m-xylene

R.T.: 2.637 min
Delta R.T.: 0.000 min
Response: 12029572
Conc: 4.43 ng/ml

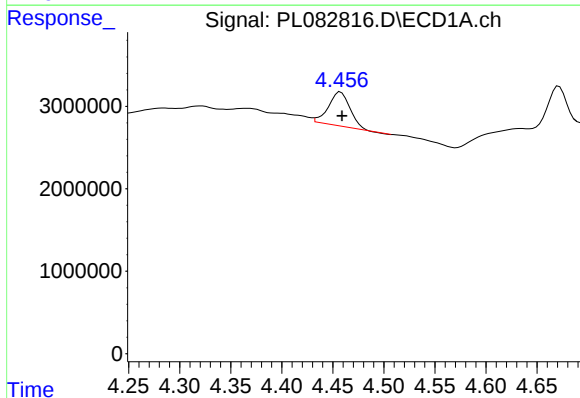


#23 Chlordane-1

R.T.: 4.457 min
Delta R.T.: -0.002 min
Response: 5819052
Conc: 54.11 ng/ml

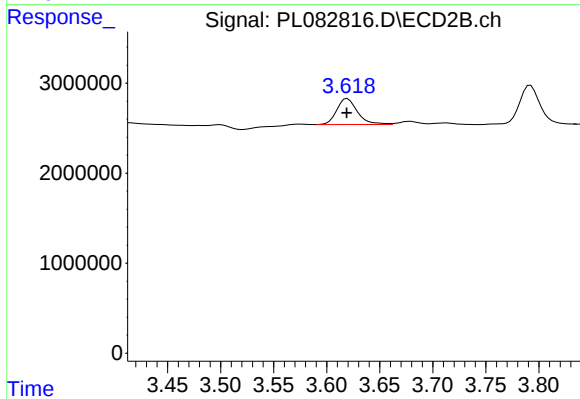

#23 Chlordane-1


R.T.: 3.620 min
Delta R.T.: 0.000 min
Response: 3922920
Conc: 47.96 ng/ml

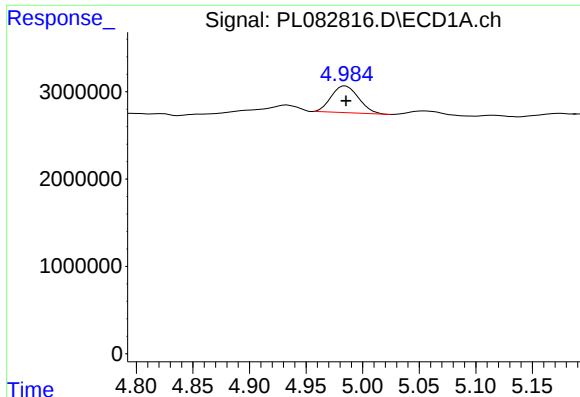

#24 Chlordane-2


R.T.: 4.985 min
Delta R.T.: 0.000 min
Response: 5142730
Conc: 46.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

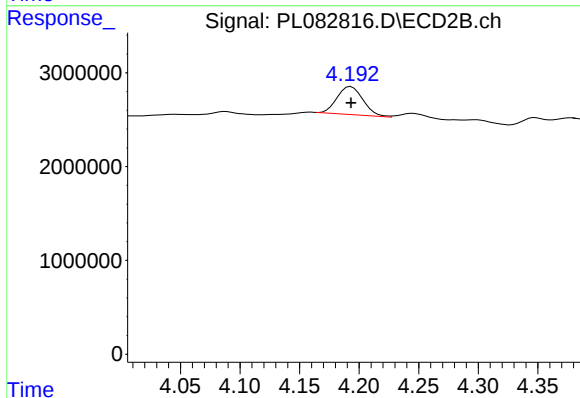


#24 Chlordane-2

R.T.: 4.193 min
Delta R.T.: 0.000 min
Response: 4525366
Conc: 51.14 ng/ml

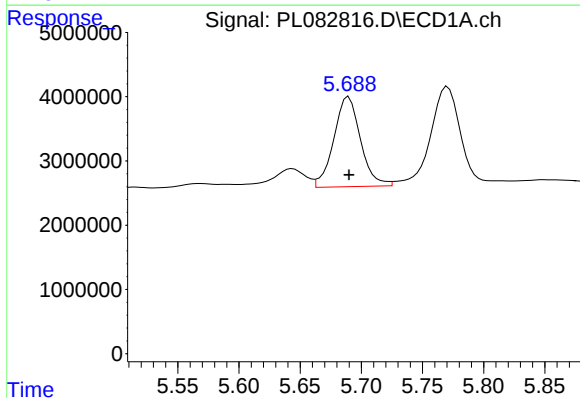


#25 Chlordane-3

R.T.: 5.690 min
Delta R.T.: 0.000 min
Response: 21258349
Conc: 51.70 ng/ml

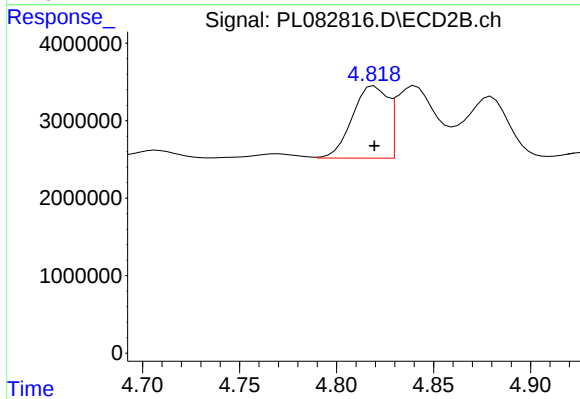

#25 Chlordane-3


R.T.: 4.819 min
Delta R.T.: 0.000 min
Response: 11747287
Conc: 43.98 ng/ml

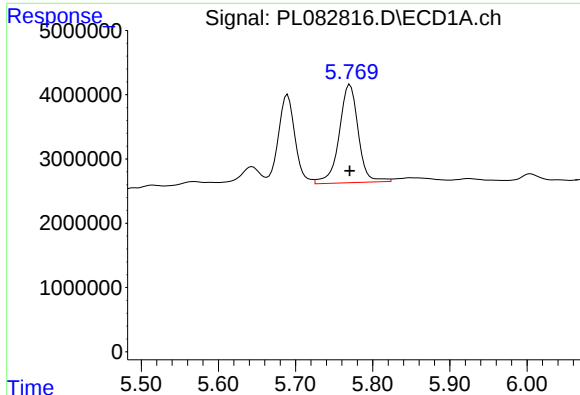

#26 Chlordane-4


R.T.: 5.771 min
Delta R.T.: 0.000 min
Response: 26263529
Conc: 52.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

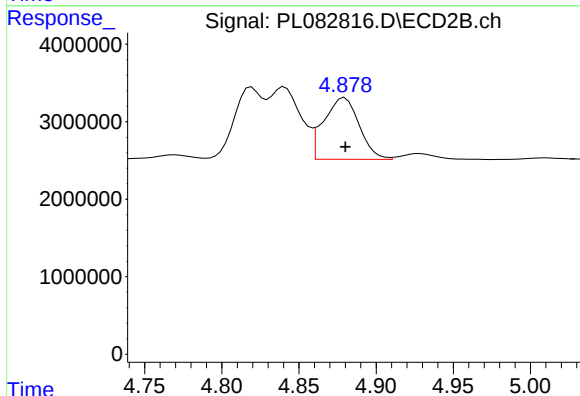


#26 Chlordane-4

R.T.: 4.880 min
Delta R.T.: 0.000 min
Response: 12692069
Conc: 45.16 ng/ml

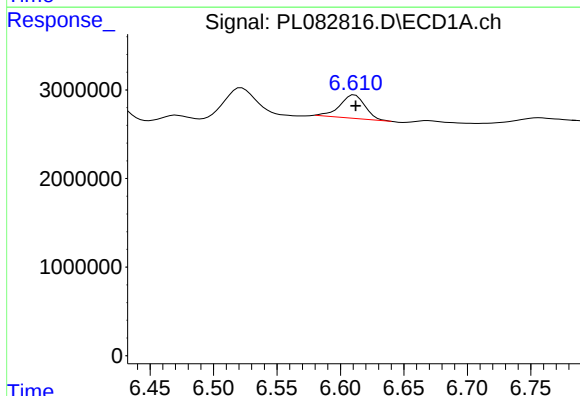


#27 Chlordane-5

R.T.: 6.611 min
Delta R.T.: 0.000 min
Response: 3567252
Conc: 42.97 ng/ml

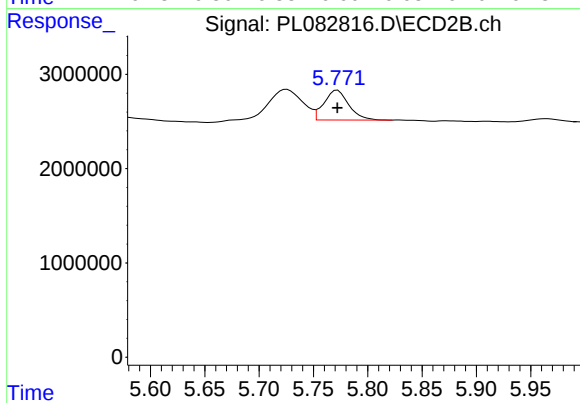

#27 Chlordane-5


R.T.: 5.772 min
Delta R.T.: 0.000 min
Response: 5002215
Conc: 53.07 ng/ml

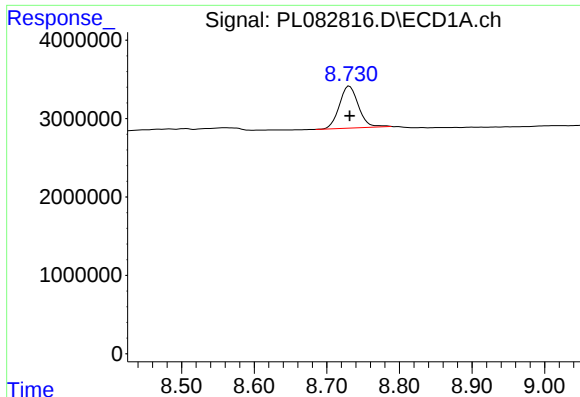

#28 Decachlorobiphenyl

R.T.: 8.731 min
Delta R.T.: 0.000 min
Response: 9814996
Conc: 5.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

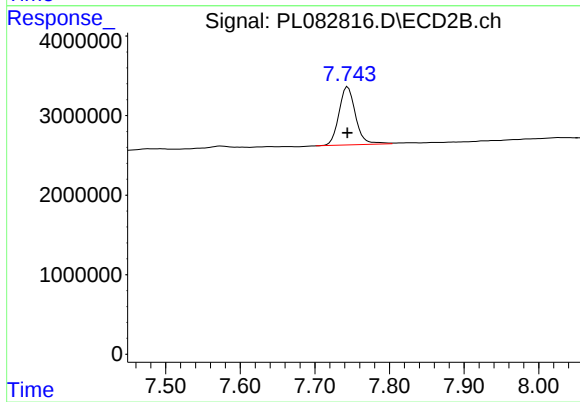

#28 Decachlorobiphenyl

R.T.: 7.744 min
Delta R.T.: 0.000 min
Response: 11281285
Conc: 5.69 ng/ml