

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051923\
 Data File : PL082813.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2023 14:41
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 04:31:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:31:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.317	2.637	180.2E6	205.5E6	73.815	73.388
28) SA Decachlor...	8.733	7.744	114.5E6	142.5E6	71.876	72.848
Target Compounds						
23) Chlordane-1	4.459	3.620	78519265	60939864	728.847	731.860
24) Chlordane-2	4.986	4.193	80877574	64757071	736.534	732.751
25) Chlordane-3	5.691	4.820	311.4E6	204.6E6	736.097	736.294
26) Chlordane-4	5.772	4.880	377.7E6	212.9E6	736.771	732.976
27) Chlordane-5	6.613	5.773	61267290	69804524	731.591	727.339



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051923\
Data File : PL082813.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2023 14:41
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 04:31:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:31:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

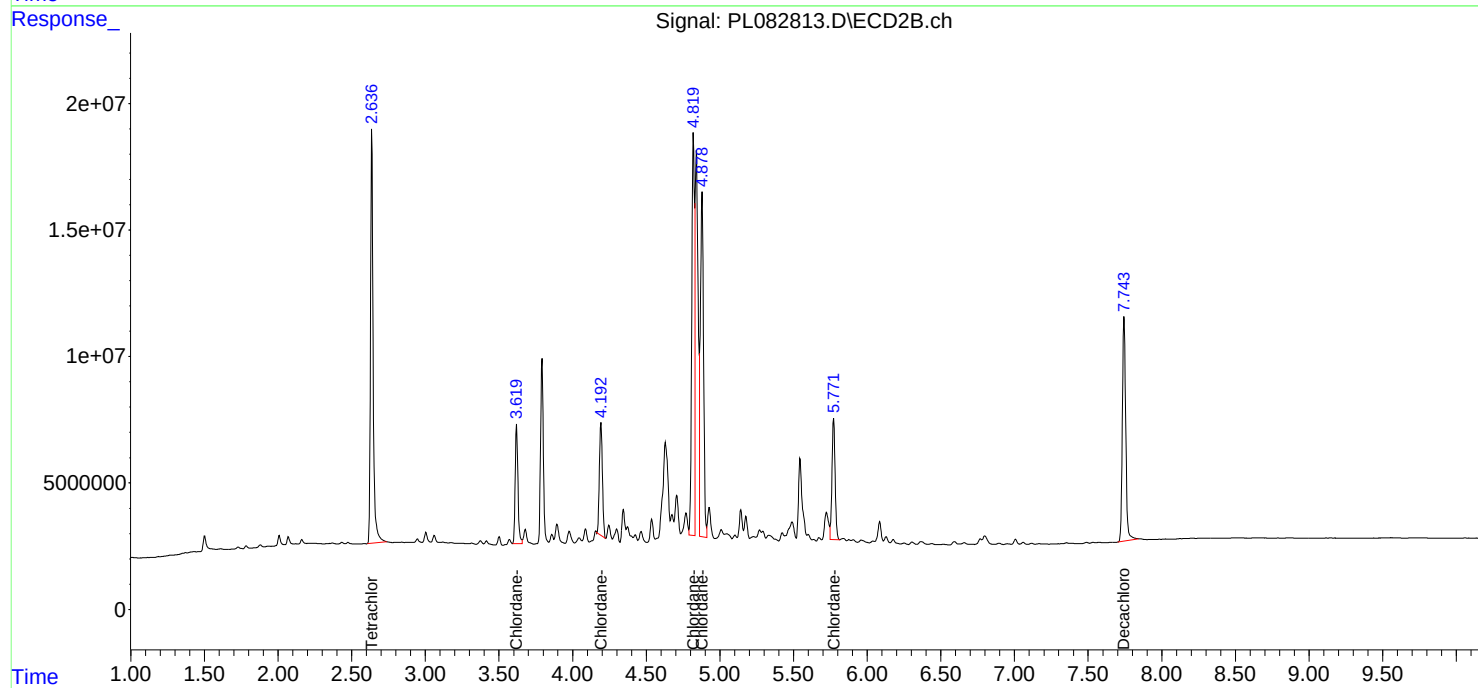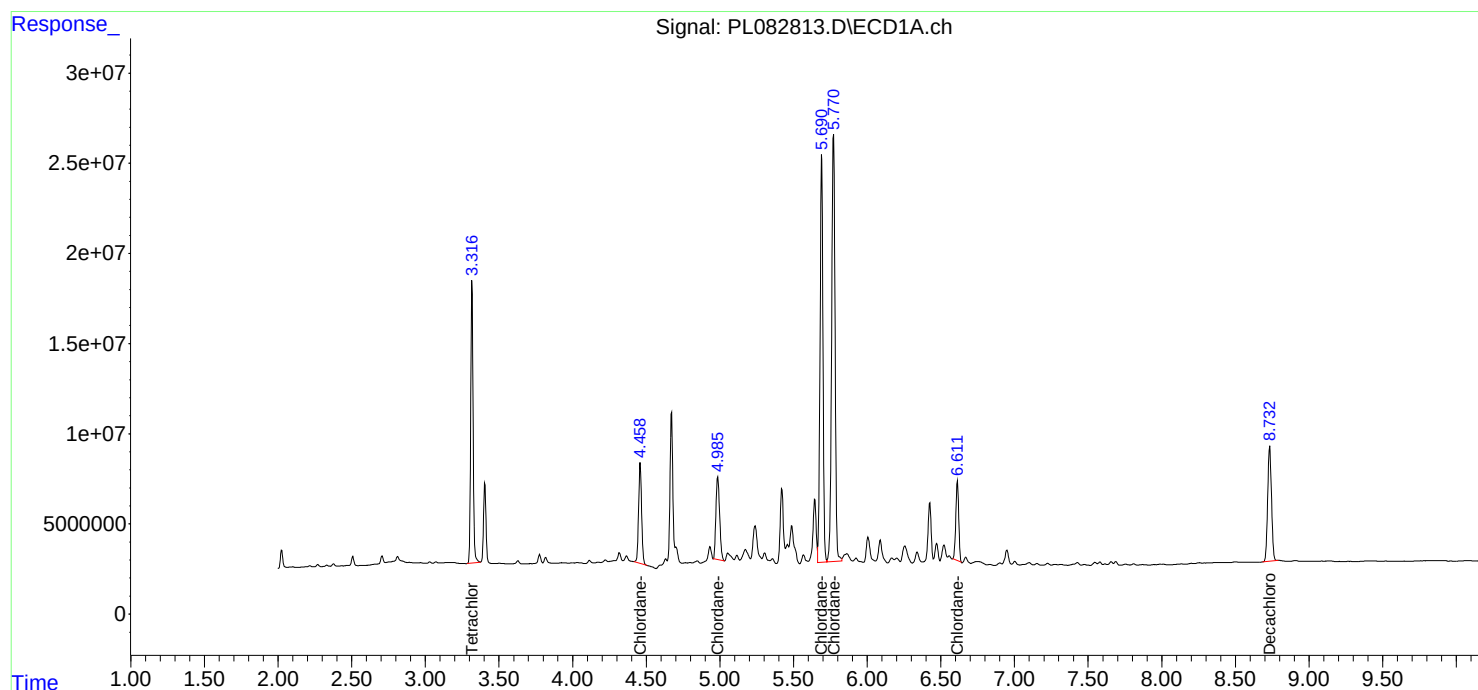


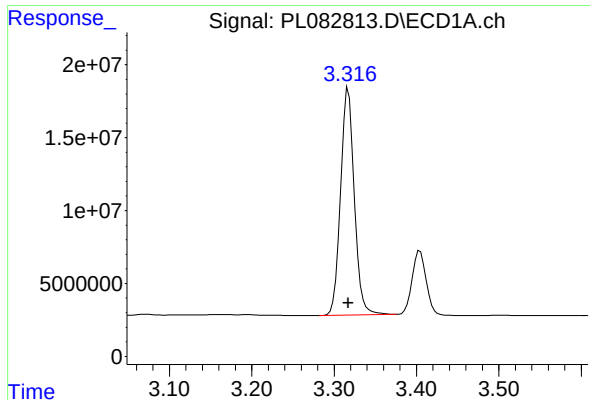

#1 Tetrachloro-m-xylene


R.T.: 3.317 min
Delta R.T.: 0.000 min
Response: 180209834
Conc: 73.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

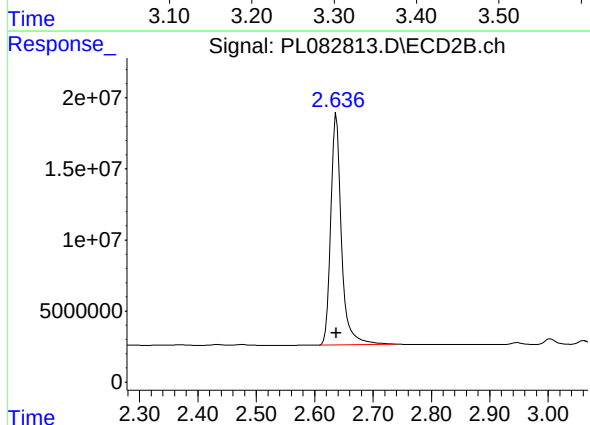


#1 Tetrachloro-m-xylene

R.T.: 2.637 min
Delta R.T.: 0.000 min
Response: 205524300
Conc: 73.39 ng/ml

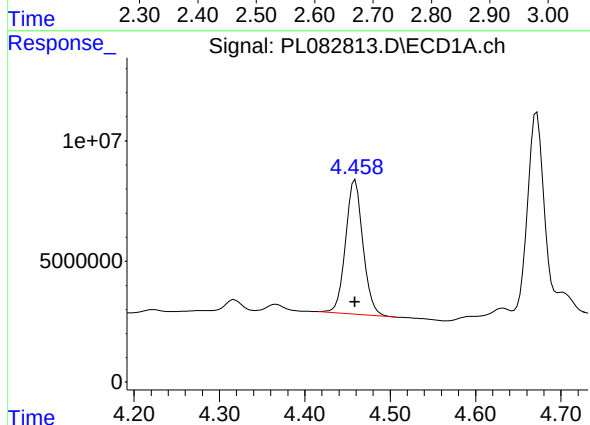


#23 Chlordane-1

R.T.: 4.459 min
Delta R.T.: 0.000 min
Response: 78519265
Conc: 728.85 ng/ml

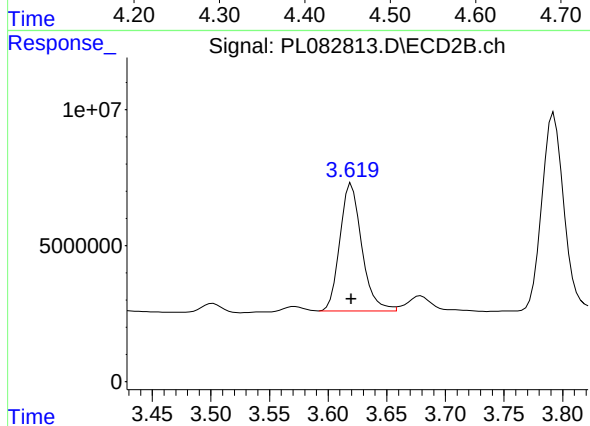

#23 Chlordane-1


R.T.: 3.620 min
Delta R.T.: 0.000 min
Response: 60939864
Conc: 731.86 ng/ml

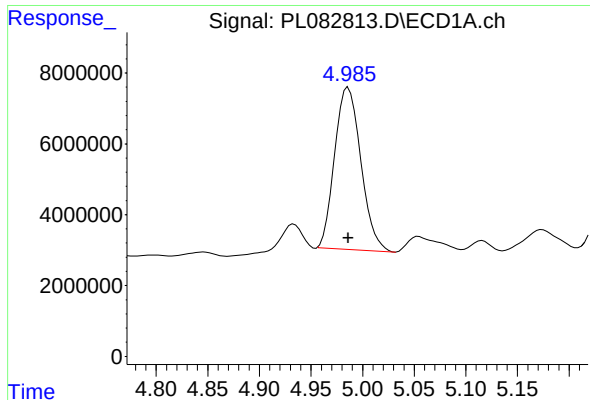

#24 Chlordane-2


R.T.: 4.986 min
Delta R.T.: 0.000 min
Response: 80877574
Conc: 736.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

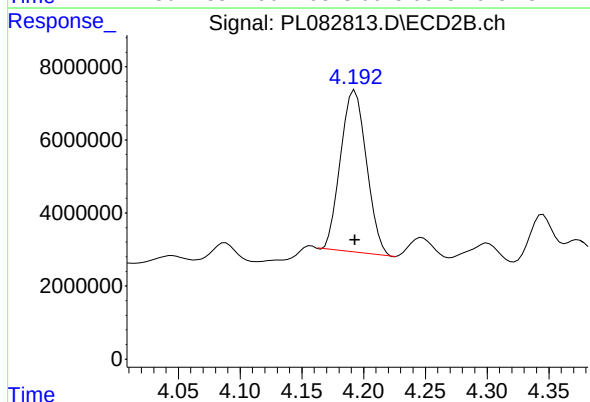


#24 Chlordane-2

R.T.: 4.193 min
Delta R.T.: 0.000 min
Response: 64757071
Conc: 732.75 ng/ml

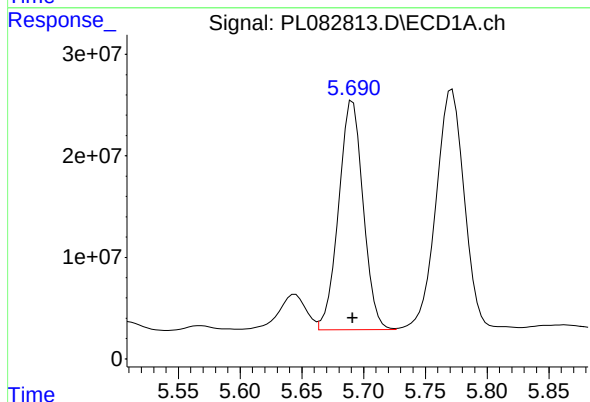


#25 Chlordane-3

R.T.: 5.691 min
Delta R.T.: 0.000 min
Response: 311400857
Conc: 736.10 ng/ml

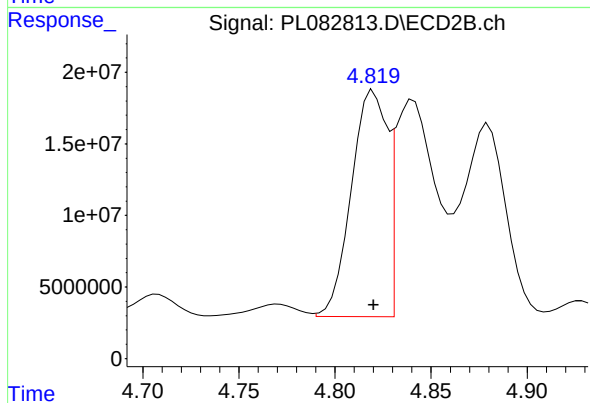

#25 Chlordane-3


R.T.: 4.820 min
Delta R.T.: 0.000 min
Response: 204612594
Conc: 736.29 ng/ml

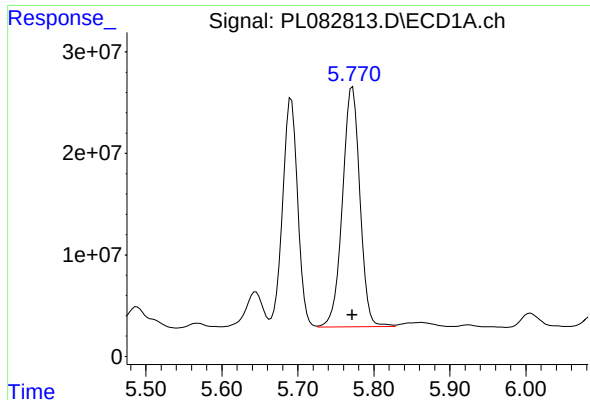

#26 Chlordane-4


R.T.: 5.772 min
Delta R.T.: 0.000 min
Response: 377650698
Conc: 736.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

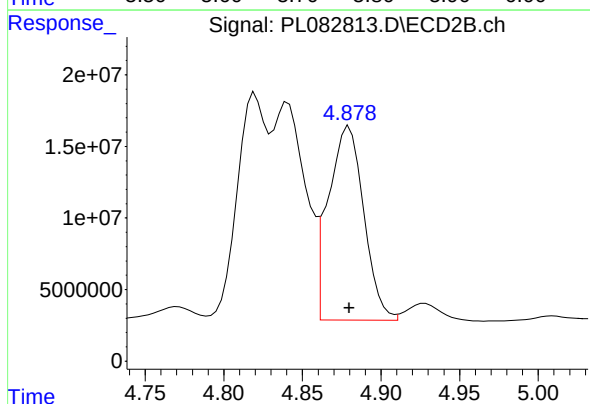


#26 Chlordane-4

R.T.: 4.880 min
Delta R.T.: 0.000 min
Response: 212850085
Conc: 732.98 ng/ml

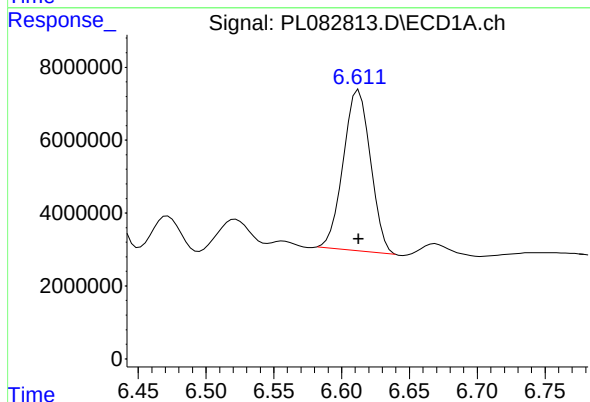


#27 Chlordane-5

R.T.: 6.613 min
Delta R.T.: 0.000 min
Response: 61267290
Conc: 731.59 ng/ml

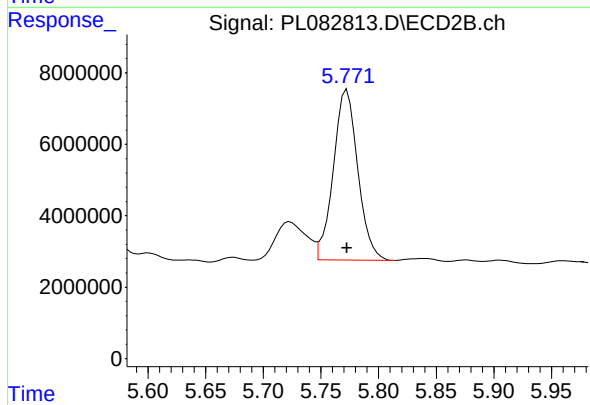

#27 Chlordane-5


R.T.: 5.773 min
Delta R.T.: 0.000 min
Response: 69804524
Conc: 727.34 ng/ml

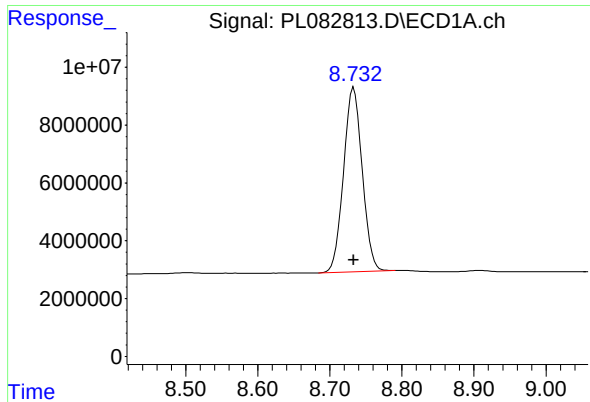

#28 Decachlorobiphenyl

R.T.: 8.733 min
Delta R.T.: 0.000 min
Response: 114545589
Conc: 71.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

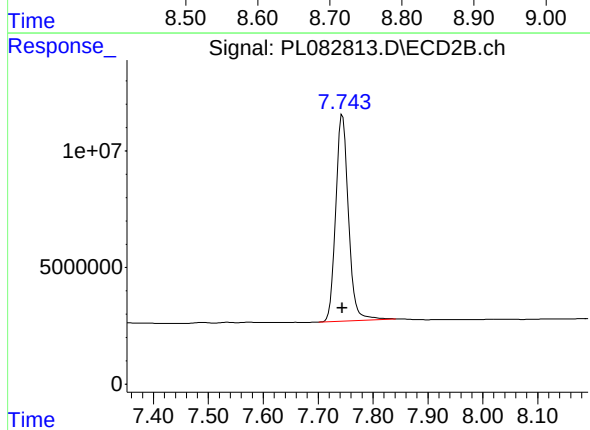

#28 Decachlorobiphenyl

R.T.: 7.744 min
Delta R.T.: 0.000 min
Response: 142547264
Conc: 72.85 ng/ml