

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051923\
 Data File : PL082851.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2023 00:38
 Operator : AR\AJ
 Sample : 02840-06
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 GROUND-WATER

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/22/2023
 Supervised By : Ankita Jodhani 05/22/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 09:36:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.314	2.637	432859	1065091	0.147m	0.410m#
28) SA Decachlor...	8.727	7.738	220410	432390	0.105m	0.174 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051923\
Data File : PL082851.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2023 00:38
Operator : AR\AJ
Sample : 02840-06
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
GROUND-WATER


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/22/2023
Supervised By : Ankita Jodhani 05/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 09:36:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

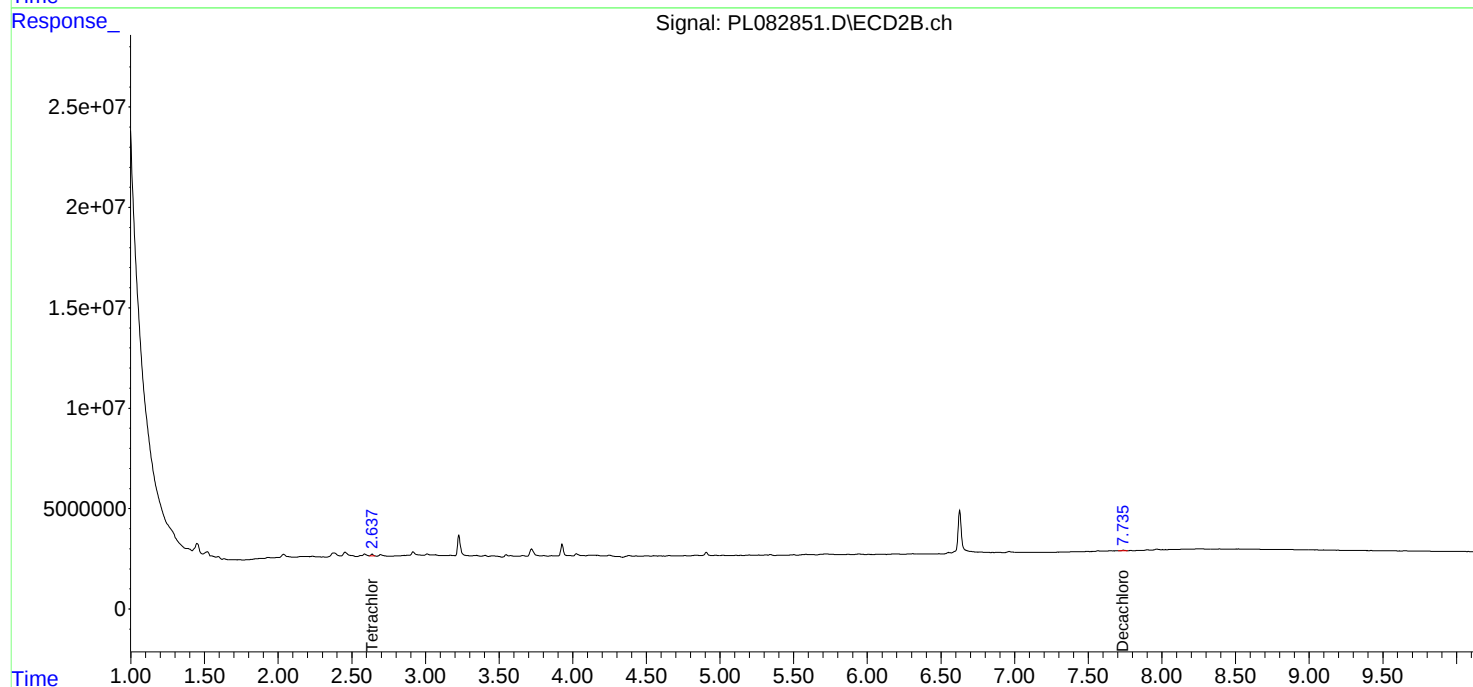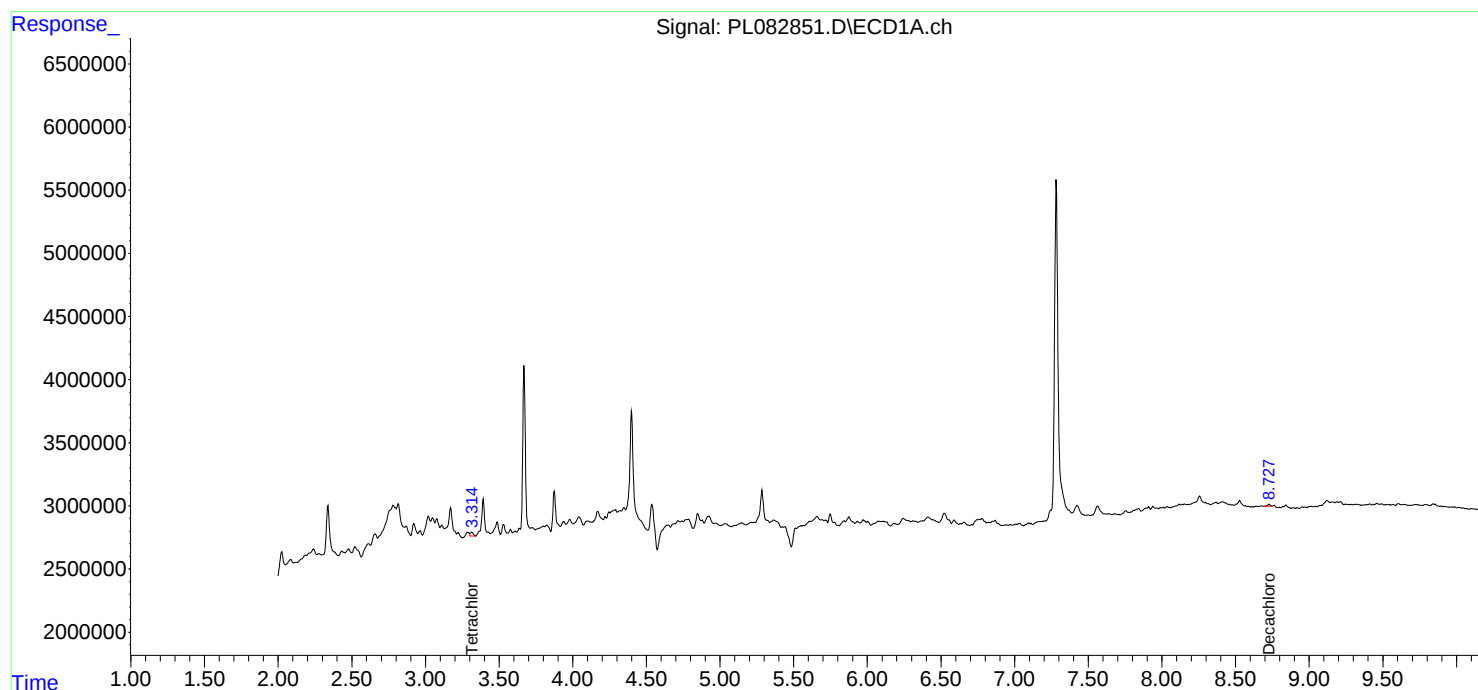

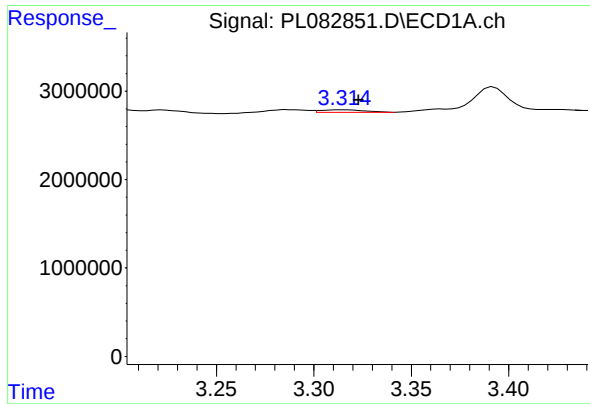


#1 Tetrachloro-m-xylene

R.T.: 3.314 min
Delta R.T.: -0.009 min
Response: 432859
Conc: 0.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
GROUND-WATER


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/22/2023
Supervised By :Ankita Jodhani 05/22/2023

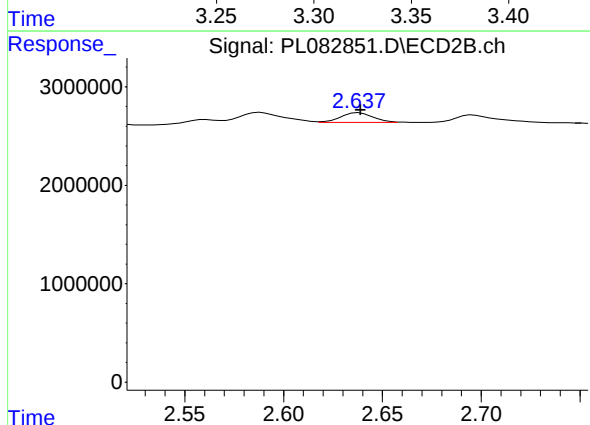


#1 Tetrachloro-m-xylene

R.T.: 2.637 min
Delta R.T.: -0.002 min
Response: 1065091
Conc: 0.41 ng/ml m

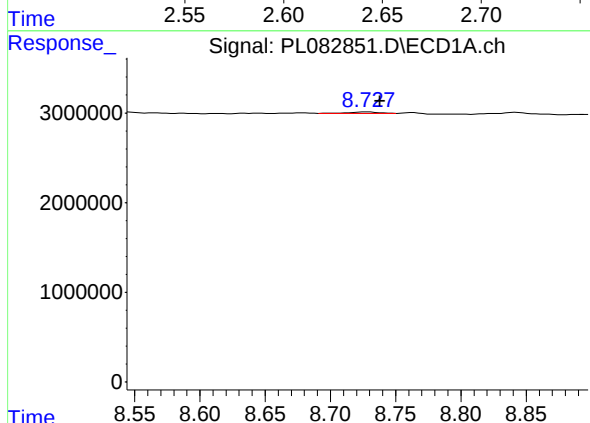

#28 Decachlorobiphenyl

R.T.: 8.727 min
Delta R.T.: -0.011 min
Response: 220410
Conc: 0.11 ng/ml m

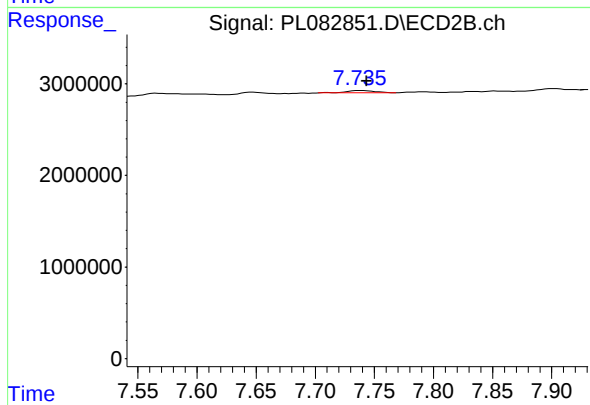

#28 Decachlorobiphenyl

R.T.: 7.738 min
Delta R.T.: -0.005 min
Response: 432390
Conc: 0.17 ng/ml