

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052020\
 Data File : PL058796.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2020 08:20
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 11:29:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.531	4.076	41853282	60599680	22.825	22.375
28)	SA Decachlor...	8.315	9.188	38455034	60686717	22.760	23.020
Target Compounds							
2)	A alpha-BHC	3.984	0.000	2113898	0	0.778	N.D. #
7)	B delta-BHC	0.000	5.118f	0	1814581	N.D.	0.498 #
8)	B Heptachlo...	0.000	5.957	0	12349243	N.D.	3.744 #
9)	A Endosulfan I	0.000	6.308f	0	3541390	N.D.	1.205 #
10)	B gamma-Chl...	0.000	6.173f	0	12235423	N.D.	3.694 #
13)	MA Dieldrin	0.000	6.558f	0	1322513	N.D.	0.437 #
15)	B Endosulfa...	0.000	7.011	0	2407615	N.D.	0.859 #
18)	B Endrin al...	0.000	7.125	0	557494	N.D.	0.236 #
23)	Chlordane-1	0.000	5.058f	0	1499338	N.D.	15.632 #
25)	Chlordane-3	0.000	6.173f	0	12235423	N.D.	32.142 #
27)	Chlordane-5	0.000	7.110f	0	1633653	N.D.	20.621 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052020\
Data File : PL058796.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2020 08:20
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 11:29:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

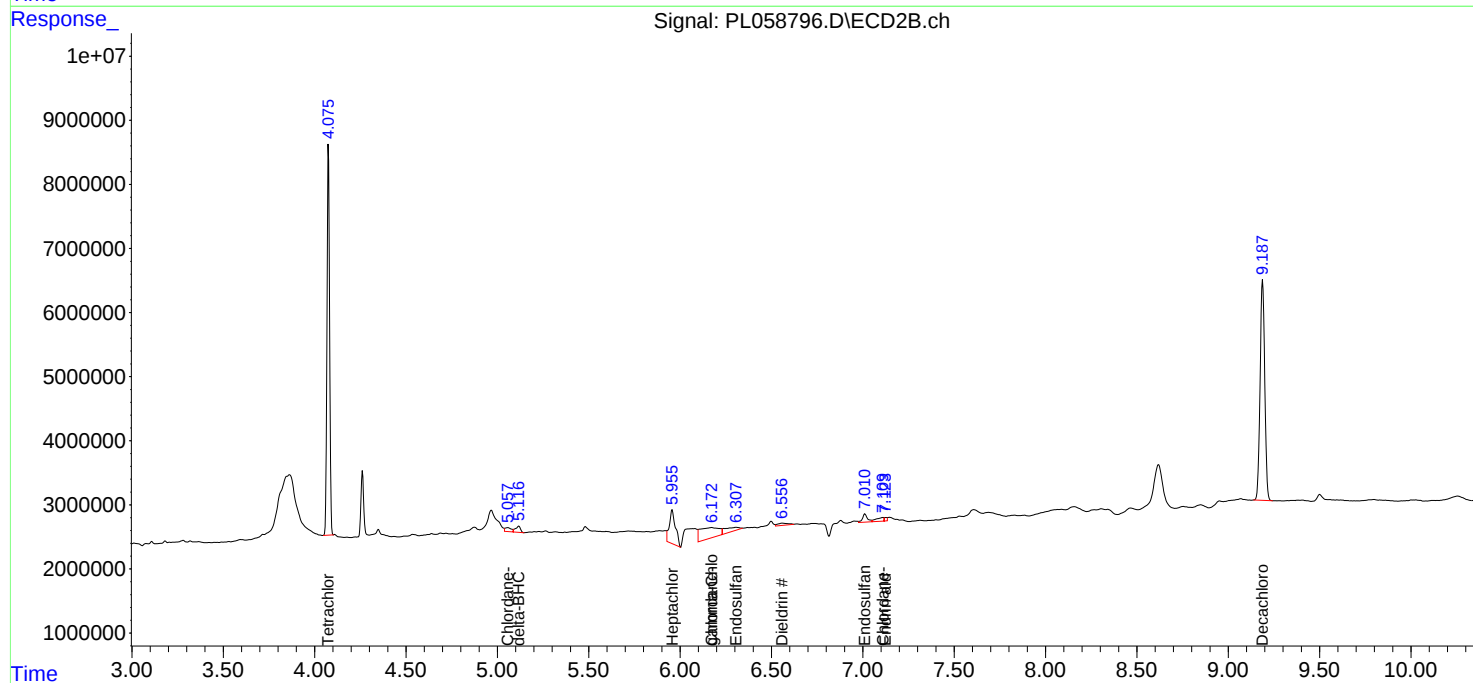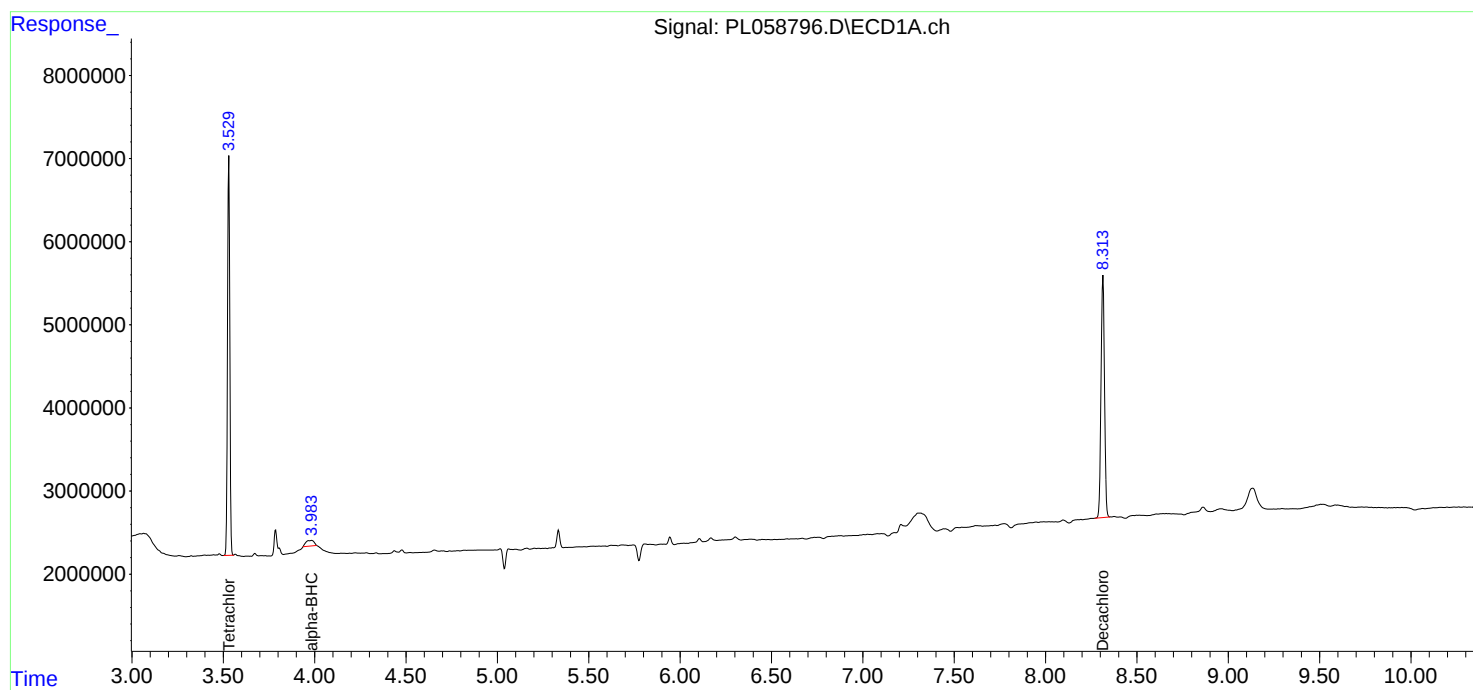


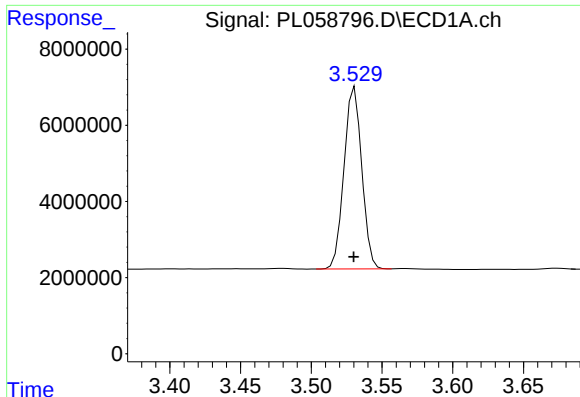

#1 Tetrachloro-m-xylene


R.T.: 3.531 min
Delta R.T.: 0.000 min
Response: 41853282
Conc: 22.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

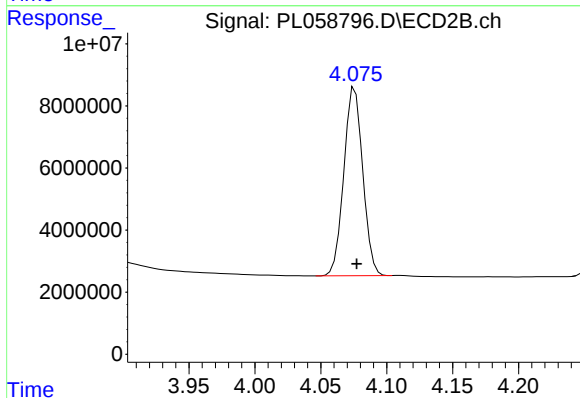


#1 Tetrachloro-m-xylene

R.T.: 4.076 min
Delta R.T.: -0.001 min
Response: 60599680
Conc: 22.37 ng/ml

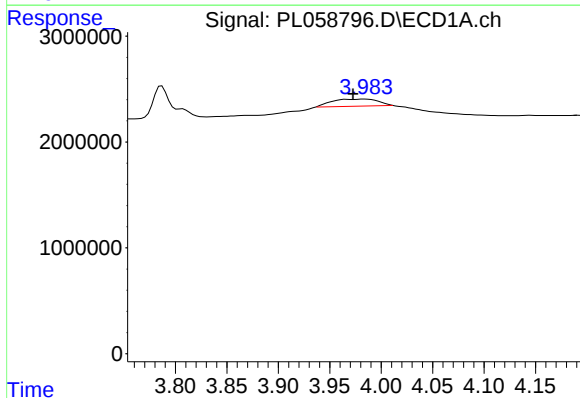


#2 alpha-BHC

R.T.: 3.984 min
Delta R.T.: 0.011 min
Response: 2113898
Conc: 0.78 ng/ml

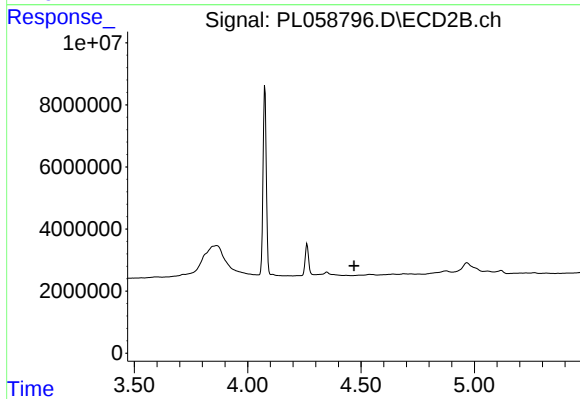

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.469 min
Response: 0
Conc: N.D.

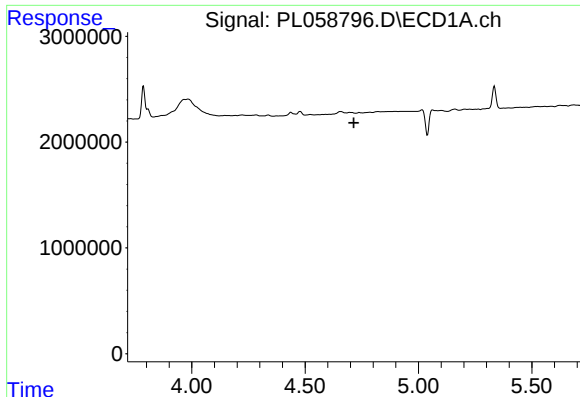

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.715 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

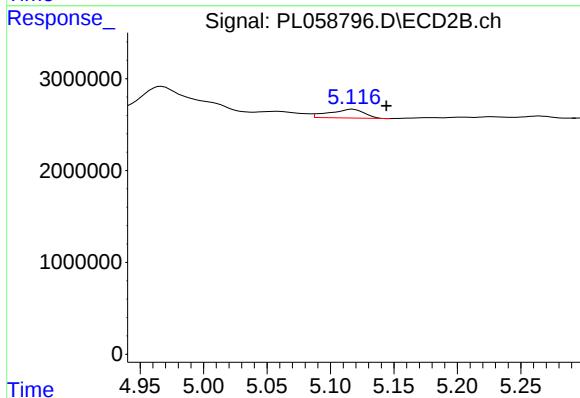


#7 delta-BHC

R.T.: 5.118 min
Delta R.T.: -0.026 min
Response: 1814581
Conc: 0.50 ng/ml

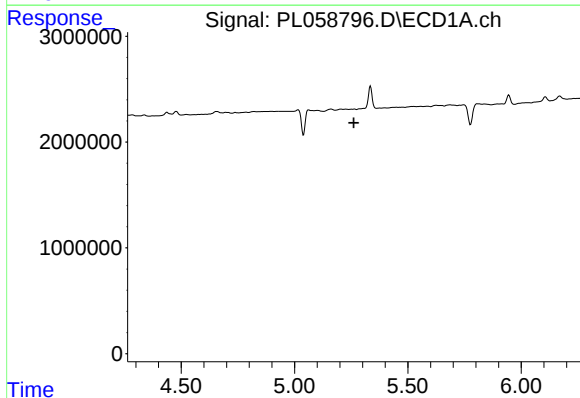


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.261 min
Response: 0
Conc: N.D.

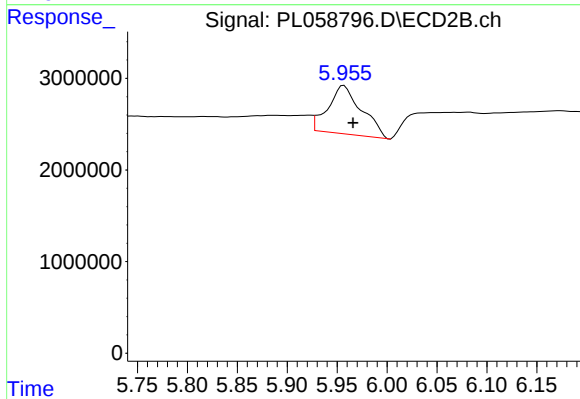

#8 Heptachlor epoxide


R.T.: 5.957 min
Delta R.T.: -0.009 min
Response: 12349243
Conc: 3.74 ng/ml

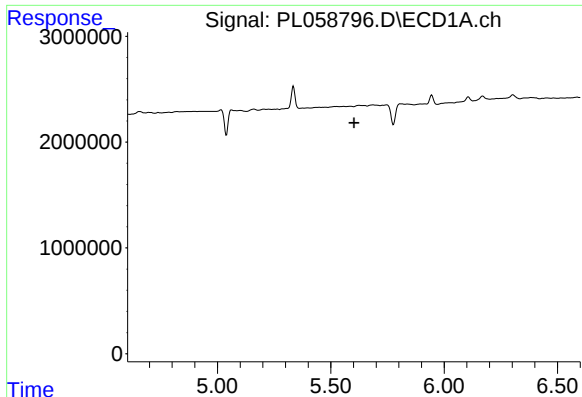

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.603 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

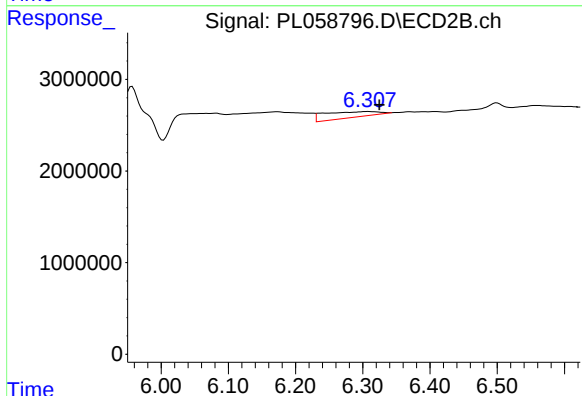


#9 Endosulfan I

R.T.: 6.308 min
Delta R.T.: -0.017 min
Response: 3541390
Conc: 1.20 ng/ml

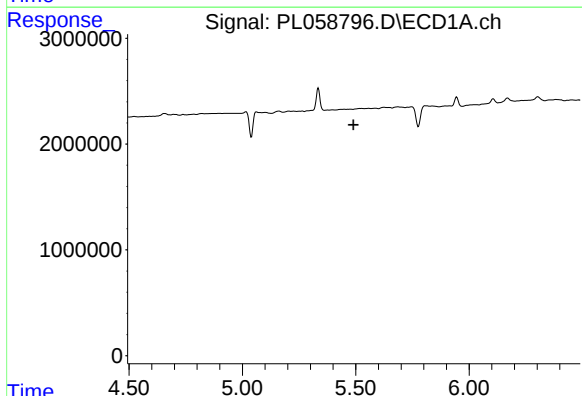


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.490 min
Response: 0
Conc: N.D.

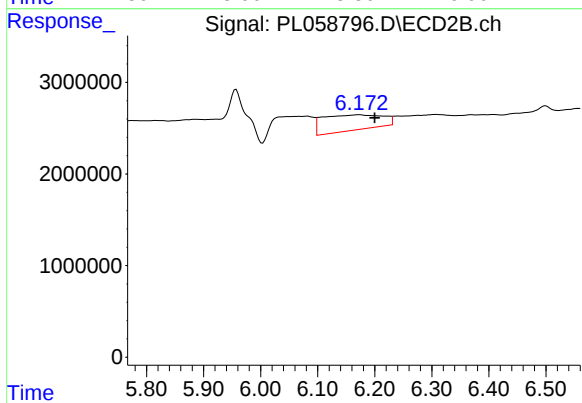

#10 gamma-Chlordane


R.T.: 6.173 min
Delta R.T.: -0.028 min
Response: 12235423
Conc: 3.69 ng/ml

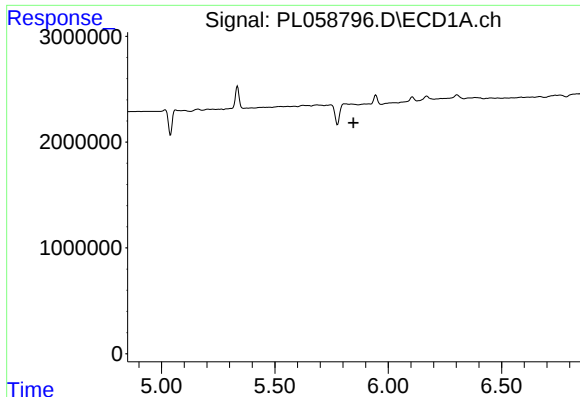

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.847 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

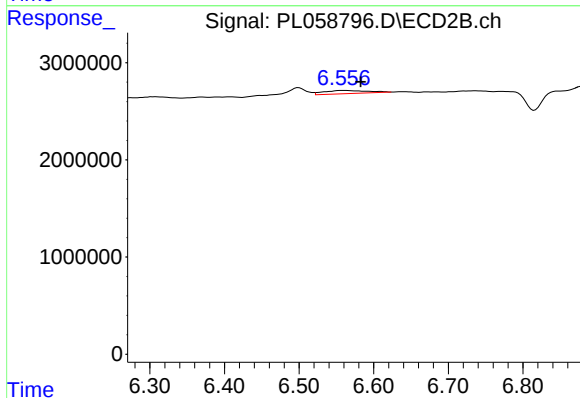


#13 Dieldrin

R.T.: 6.558 min
Delta R.T.: -0.025 min
Response: 1322513
Conc: 0.44 ng/ml

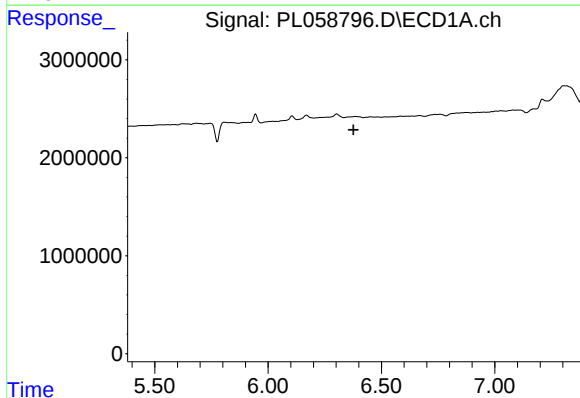


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.377 min
Response: 0
Conc: N.D.

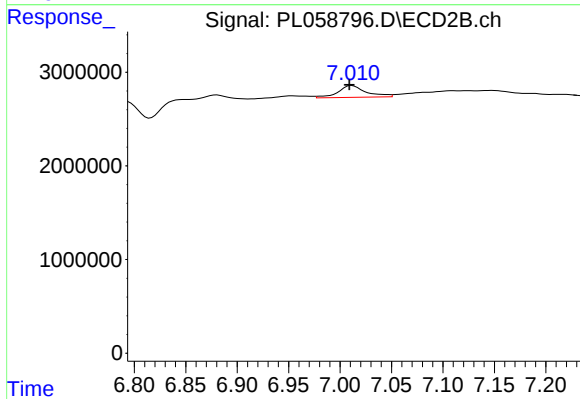

#15 Endosulfan II


R.T.: 7.011 min
Delta R.T.: 0.002 min
Response: 2407615
Conc: 0.86 ng/ml

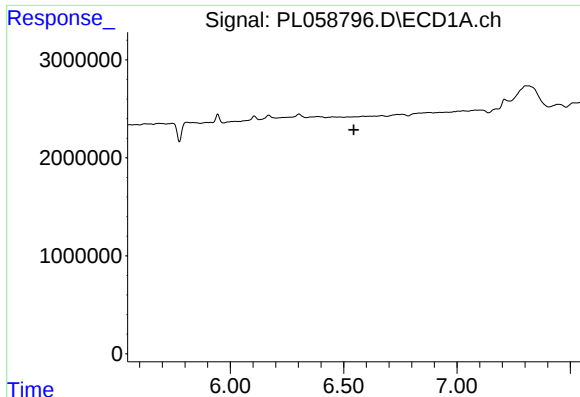

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

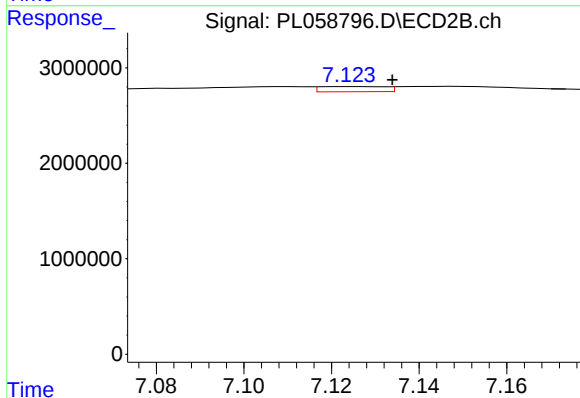


#18 Endrin aldehyde

R.T.: 7.125 min
Delta R.T.: -0.009 min
Response: 557494
Conc: 0.24 ng/ml

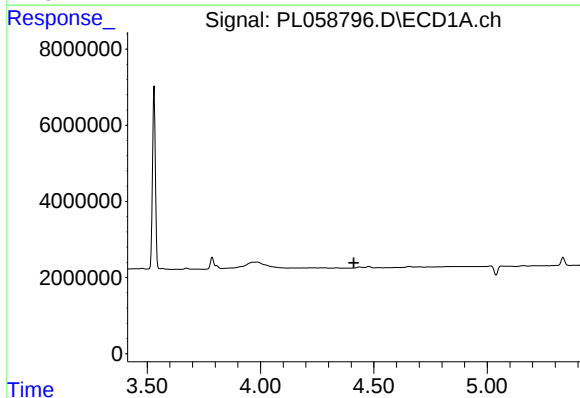


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.412 min
Response: 0
Conc: N.D.

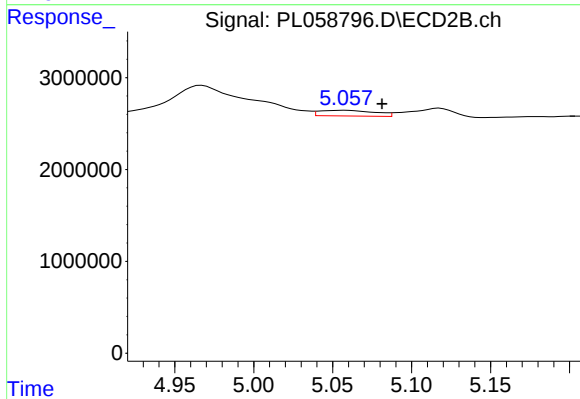

#23 Chlordane-1


R.T.: 5.058 min
Delta R.T.: -0.023 min
Response: 1499338
Conc: 15.63 ng/ml

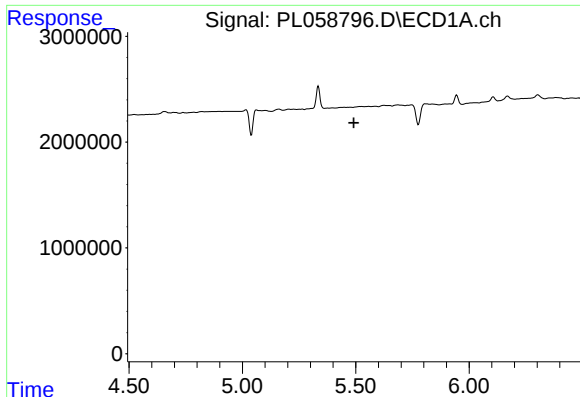

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.491 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

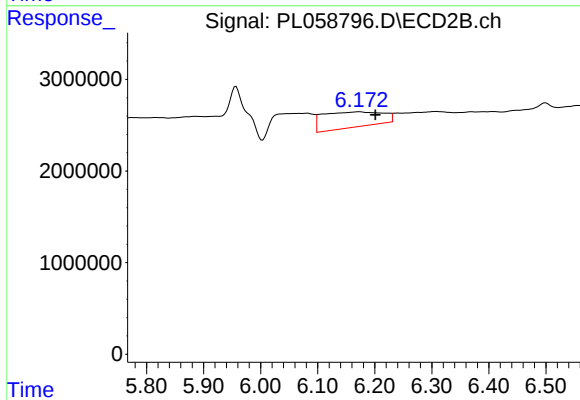


#25 Chlordane-3

R.T.: 6.173 min
Delta R.T.: -0.028 min
Response: 12235423
Conc: 32.14 ng/ml

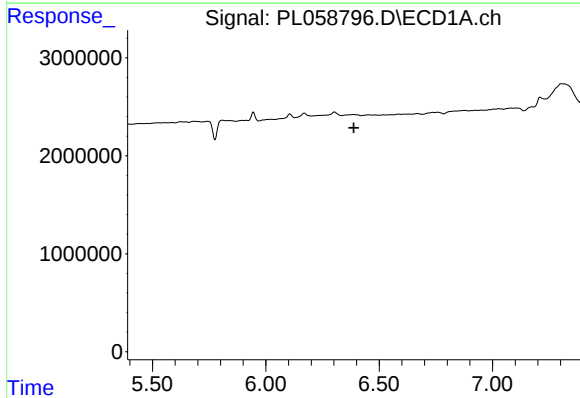


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.389 min
Response: 0
Conc: N.D.

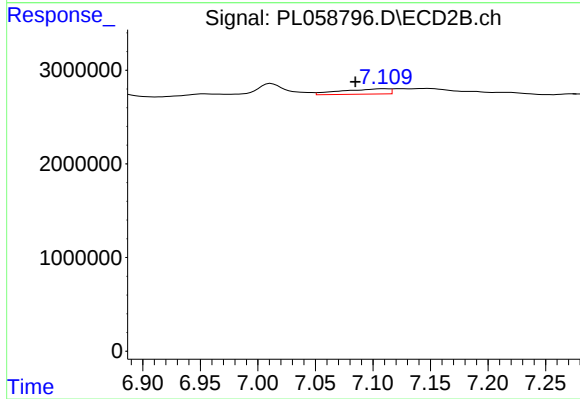

#27 Chlordane-5


R.T.: 7.110 min
Delta R.T.: 0.025 min
Response: 1633653
Conc: 20.62 ng/ml

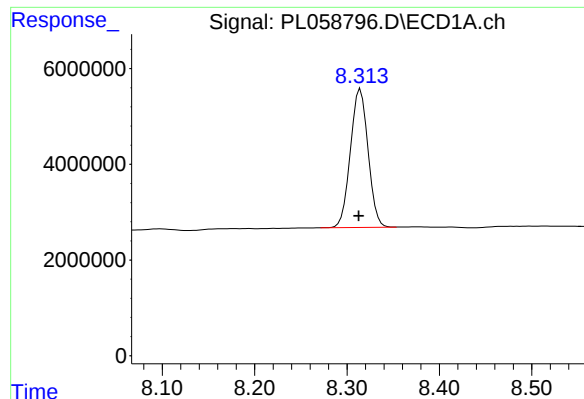

#28 Decachlorobiphenyl

R.T.: 8.315 min
Delta R.T.: 0.002 min
Response: 38455034
Conc: 22.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

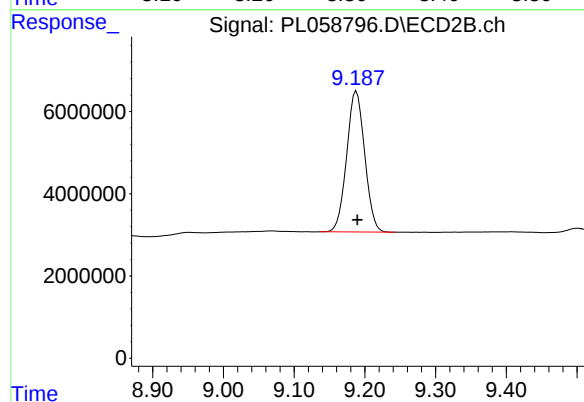

#28 Decachlorobiphenyl

R.T.: 9.188 min
Delta R.T.: -0.001 min
Response: 60686717
Conc: 23.02 ng/ml