

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052020\
 Data File : PL058810.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2020 12:19
 Operator : AJ\MA
 Sample : PB128948TB
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 17:25:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	4.077	35195872	52552510	19.195	19.403
28)	SA Decachlor...	8.319	9.193	36266981	56373393	21.465	21.384
Target Compounds							
3)	MA gamma-BHC...	0.000	4.751	0	660606	N.D.	0.174 #
7)	B delta-BHC	0.000	5.121f	0	594040	N.D.	0.163 #
8)	B Heptachlo...	0.000	5.953	0	444053	N.D.	0.135 #
9)	A Endosulfan I	0.000	6.297f	0	1006056	N.D.	0.342 #
11)	B alpha-Chl...	0.000	6.297f	0	1006056	N.D.	0.310 #
15)	B Endosulfa...	0.000	7.011	0	7474454	N.D.	2.667 #
16)	A 4,4'-DDD	0.000	6.946f	0	853361	N.D.	0.358 #
22)	Mirex	7.459	0.000	867383	0	0.561	N.D. #
26)	Chlordane-4	0.000	6.297f	0	1006056	N.D.	2.209 #
27)	Chlordane-5	0.000	7.070f	0	971984	N.D.	12.269 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052020\
Data File : PL058810.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2020 12:19
Operator : AJ\MA
Sample : PB128948TB
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 17:25:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

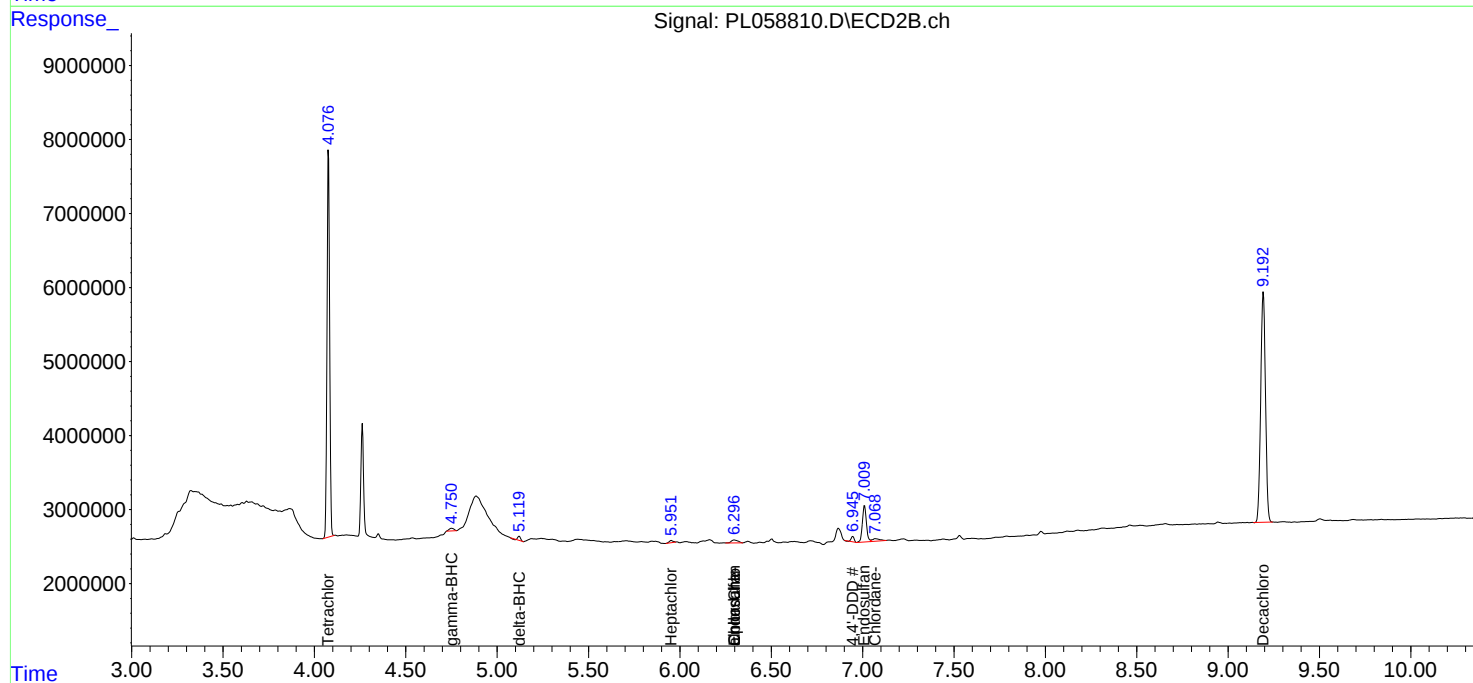


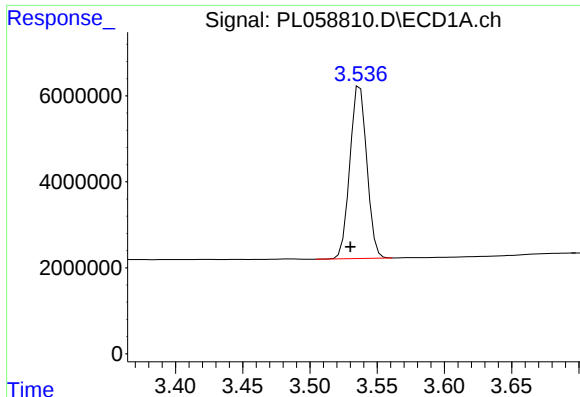

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: 0.007 min
Response: 35195872
Conc: 19.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

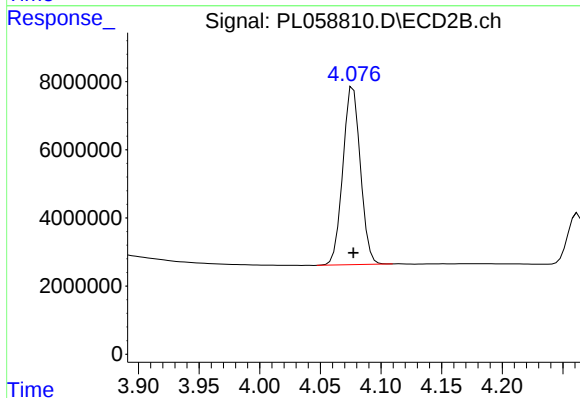


#1 Tetrachloro-m-xylene

R.T.: 4.077 min
Delta R.T.: 0.000 min
Response: 52552510
Conc: 19.40 ng/ml

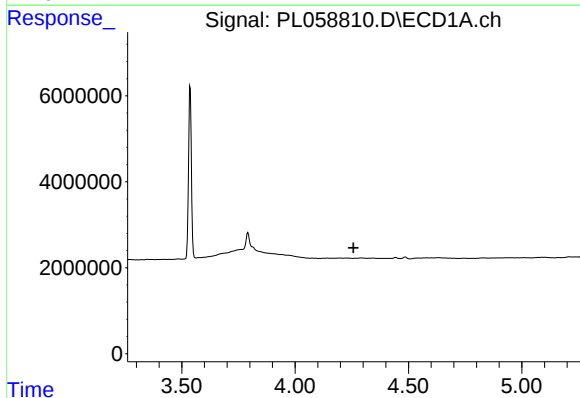


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.258 min
Response: 0
Conc: N.D.

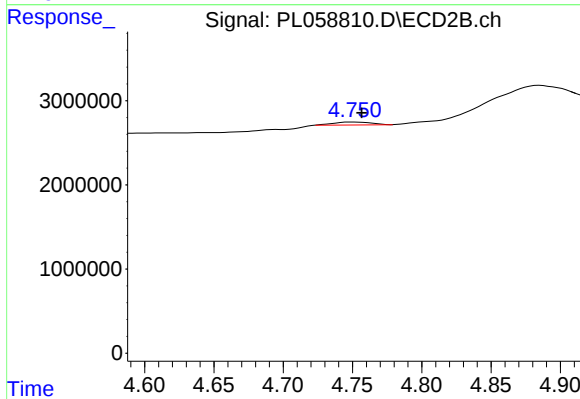

#3 gamma-BHC (Lindane)


R.T.: 4.751 min
Delta R.T.: -0.006 min
Response: 660606
Conc: 0.17 ng/ml

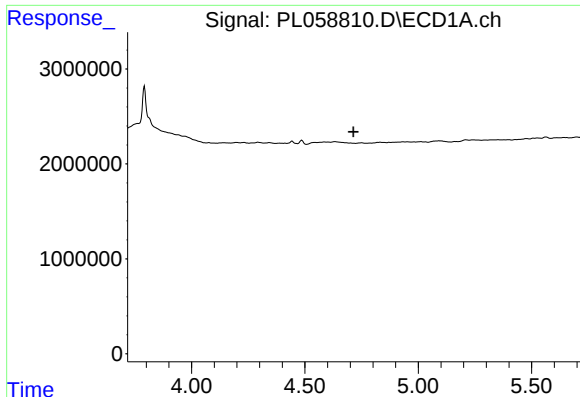

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.715 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

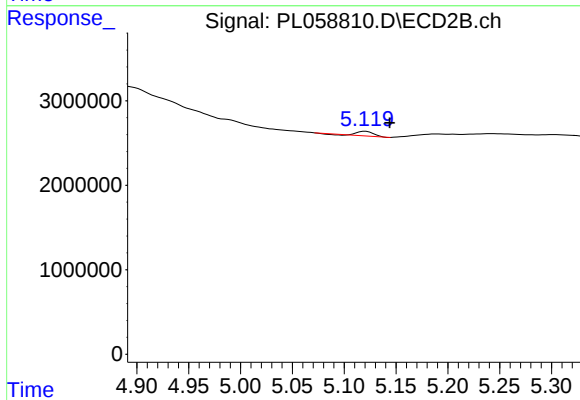


#7 delta-BHC

R.T.: 5.121 min
Delta R.T.: -0.023 min
Response: 594040
Conc: 0.16 ng/ml

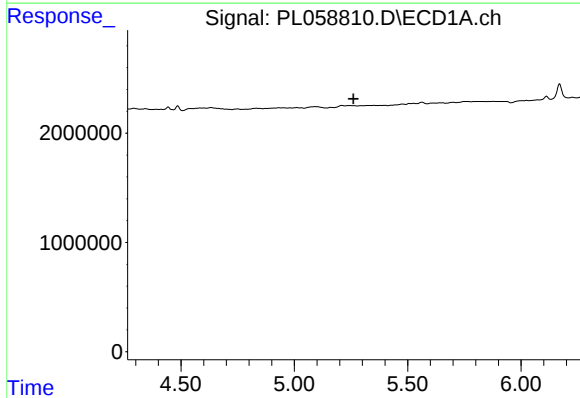


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.261 min
Response: 0
Conc: N.D.

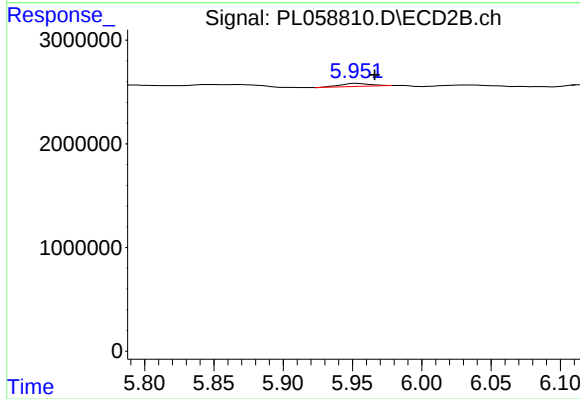

#8 Heptachlor epoxide


R.T.: 5.953 min
Delta R.T.: -0.013 min
Response: 444053
Conc: 0.13 ng/ml

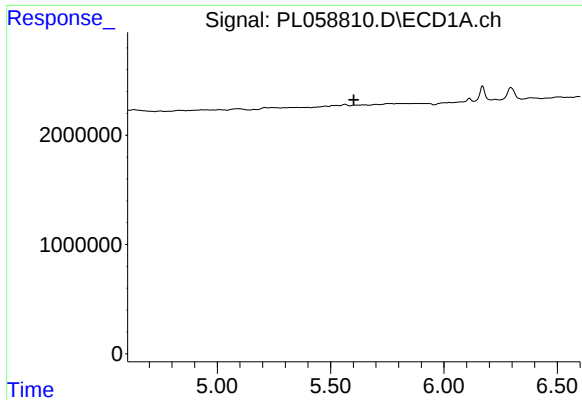

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.603 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

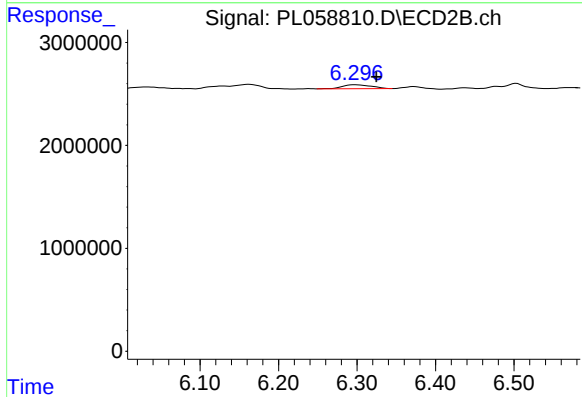


#9 Endosulfan I

R.T.: 6.297 min
Delta R.T.: -0.027 min
Response: 1006056
Conc: 0.34 ng/ml

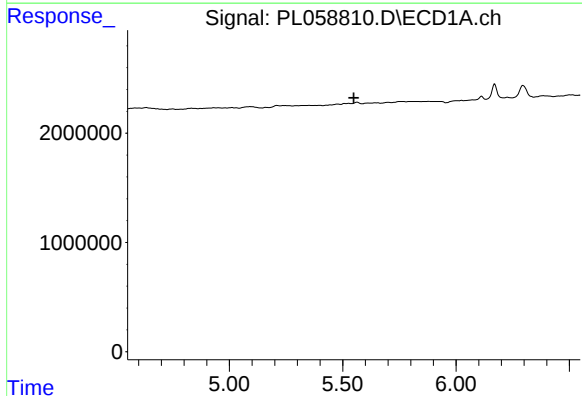


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.549 min
Response: 0
Conc: N.D.

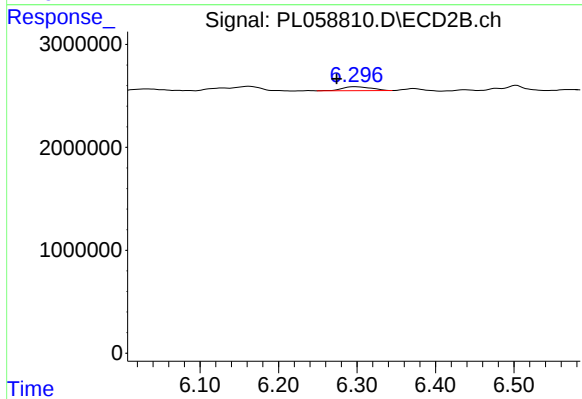

#11 alpha-Chlordane


R.T.: 6.297 min
Delta R.T.: 0.023 min
Response: 1006056
Conc: 0.31 ng/ml

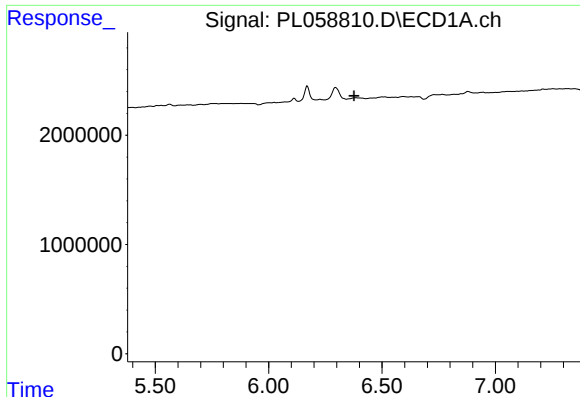

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.377 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

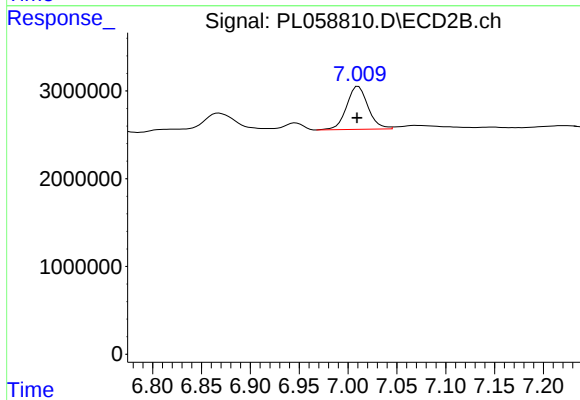


#15 Endosulfan II

R.T.: 7.011 min
Delta R.T.: 0.001 min
Response: 7474454
Conc: 2.67 ng/ml

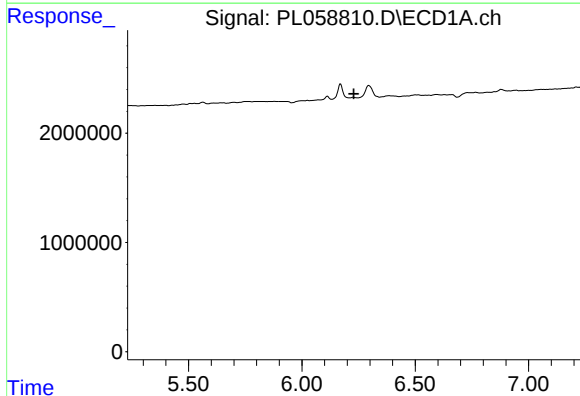


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.229 min
Response: 0
Conc: N.D.

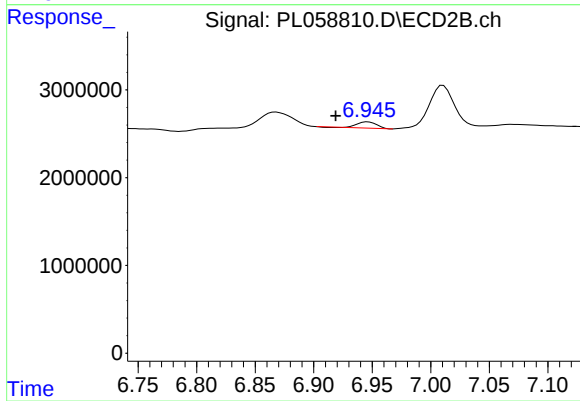

#16 4,4'-DDD


R.T.: 6.946 min
Delta R.T.: 0.027 min
Response: 853361
Conc: 0.36 ng/ml

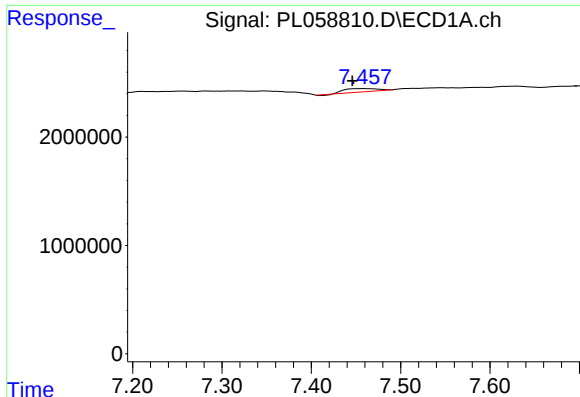

#22 Mirex


R.T.: 7.459 min
Delta R.T.: 0.013 min
Response: 867383
Conc: 0.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

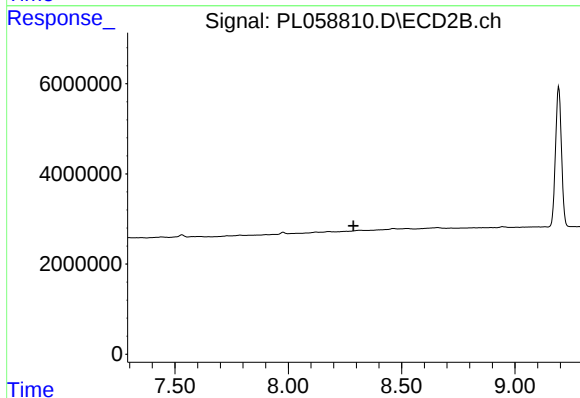


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.288 min
Response: 0
Conc: N.D.

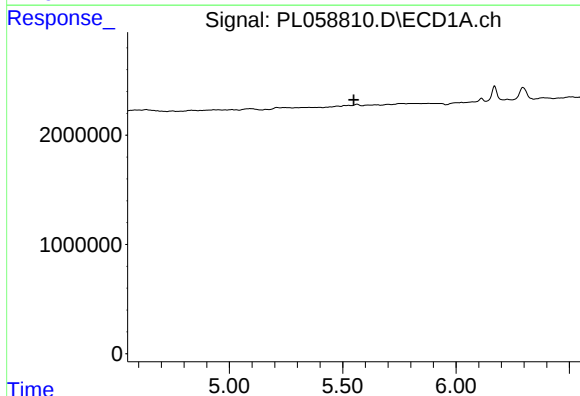


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.549 min
Response: 0
Conc: N.D.

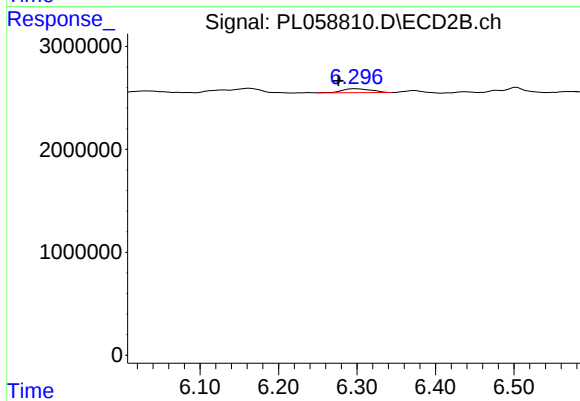

#26 Chlordane-4


R.T.: 6.297 min
Delta R.T.: 0.021 min
Response: 1006056
Conc: 2.21 ng/ml

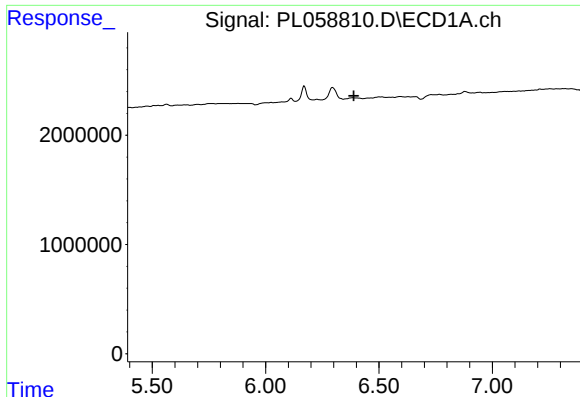

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

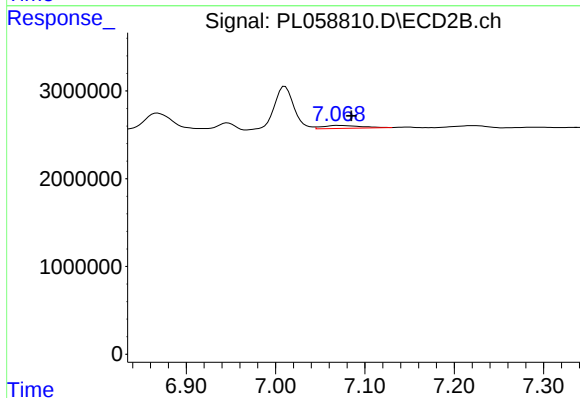


#27 Chlordane-5

R.T.: 7.070 min
Delta R.T.: -0.015 min
Response: 971984
Conc: 12.27 ng/ml

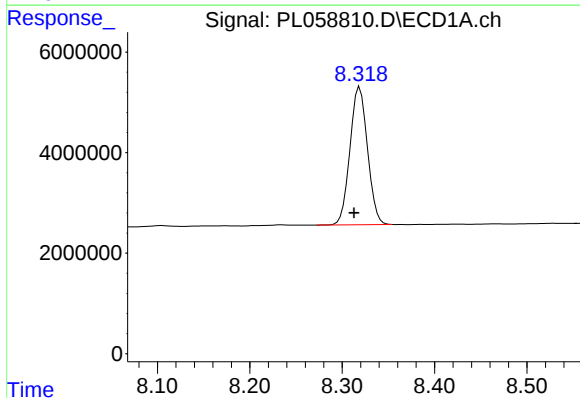

#28 Decachlorobiphenyl

R.T.: 8.319 min
Delta R.T.: 0.006 min
Response: 36266981
Conc: 21.47 ng/ml

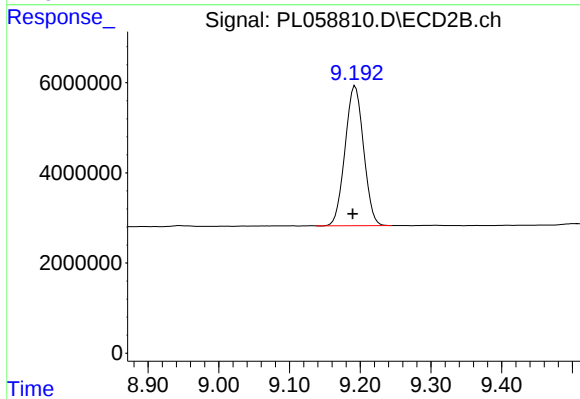

#28 Decachlorobiphenyl

R.T.: 9.193 min
Delta R.T.: 0.004 min
Response: 56373393
Conc: 21.38 ng/ml