

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052020\
 Data File : PL058817.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2020 14:45
 Operator : AJ\MA
 Sample : PB129014BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 17:26:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.529	4.076	35339353	52743314	19.273	19.474
28)	SA Decachlor...	8.312	9.187	34041169	53946990	20.148	20.464
Target Compounds							
4)	MA Heptachlor	0.000	5.262	0	666857	N.D.	0.174 #
7)	B delta-BHC	0.000	5.118f	0	1405345	N.D.	0.385 #
9)	A Endosulfan I	0.000	6.307f	0	209356	N.D.	0.071 #
10)	B gamma-Chl...	0.000	6.174f	0	410554	N.D.	0.124 #
14)	MA Endrin	0.000	6.822f	0	252799	N.D.	0.101 #
15)	B Endosulfa...	0.000	7.011	0	2043567	N.D.	0.729 #
23)	Chlordane-1	0.000	5.059f	0	917386	N.D.	9.565 #
25)	Chlordane-3	0.000	6.174f	0	410554	N.D.	1.079 #
27)	Chlordane-5	0.000	7.072	0	254062	N.D.	3.207 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052020\
Data File : PL058817.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2020 14:45
Operator : AJ\MA
Sample : PB129014BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 17:26:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

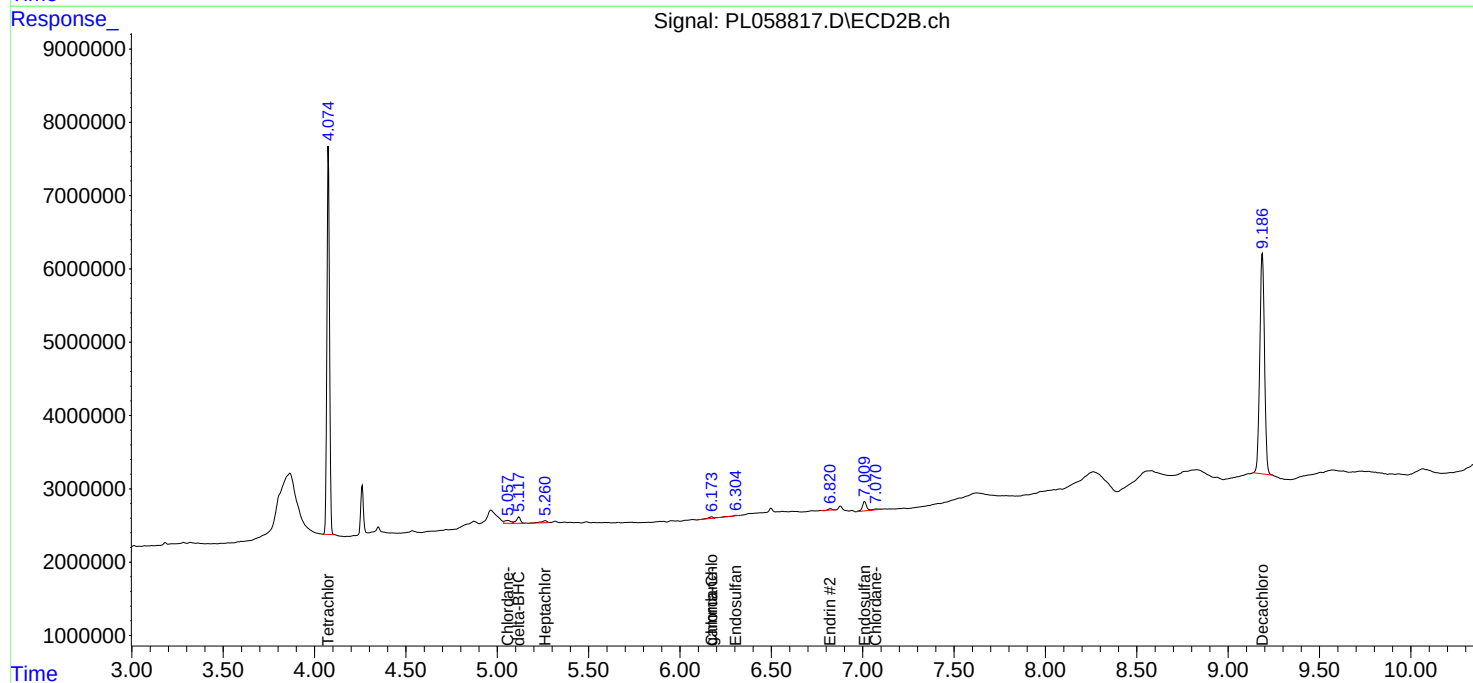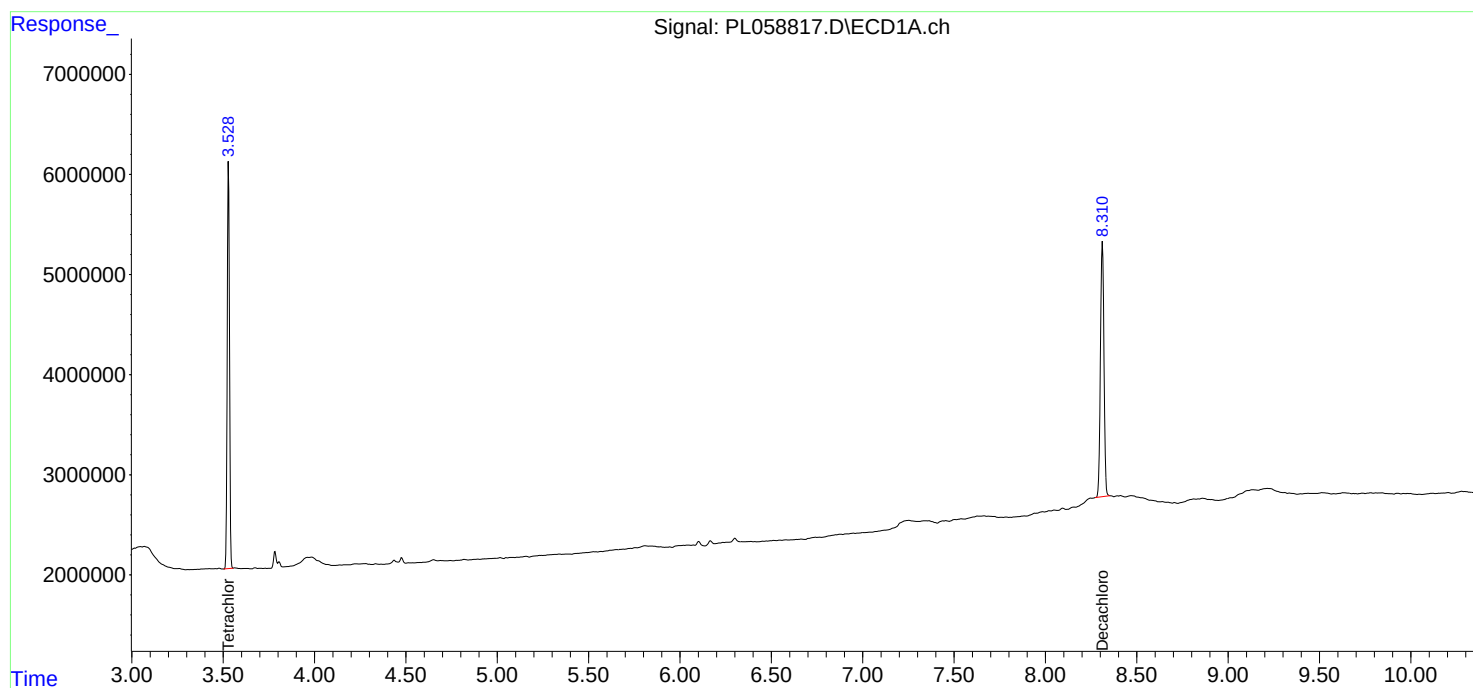


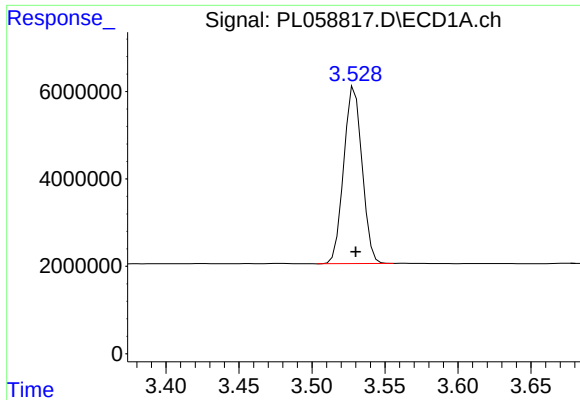

#1 Tetrachloro-m-xylene


R.T.: 3.529 min
Delta R.T.: 0.000 min
Response: 35339353
Conc: 19.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

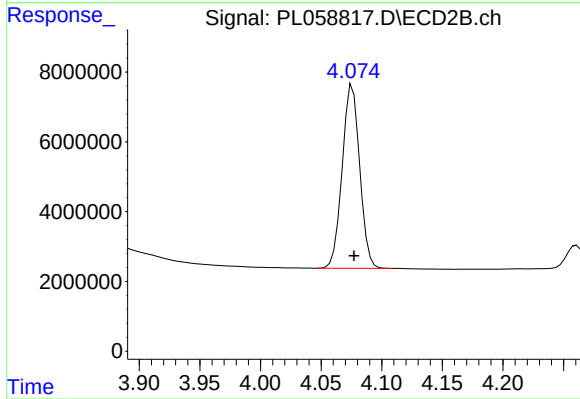


#1 Tetrachloro-m-xylene

R.T.: 4.076 min
Delta R.T.: -0.001 min
Response: 52743314
Conc: 19.47 ng/ml

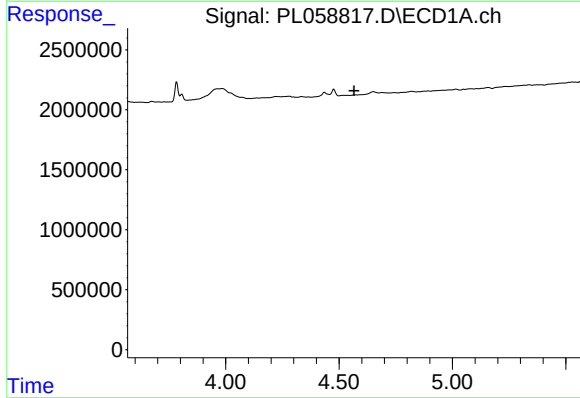


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

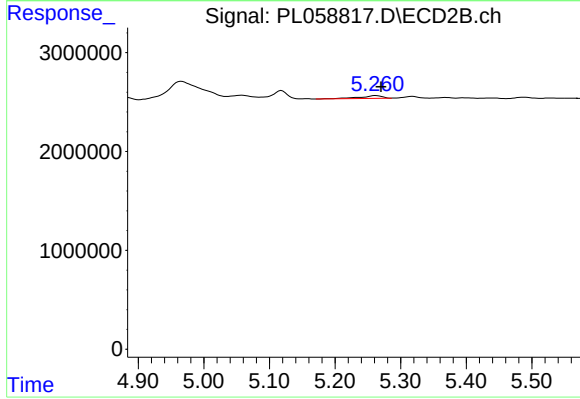

#4 Heptachlor


R.T.: 5.262 min
Delta R.T.: -0.008 min
Response: 666857
Conc: 0.17 ng/ml

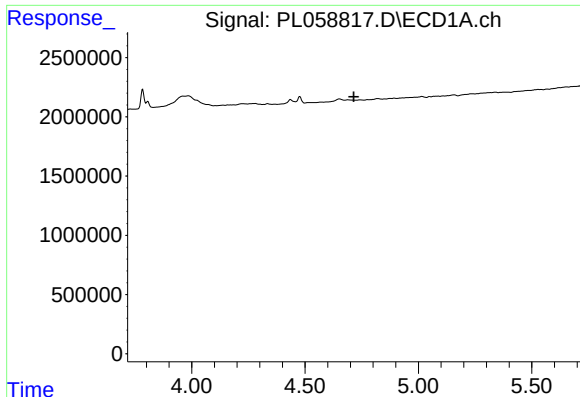

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.715 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

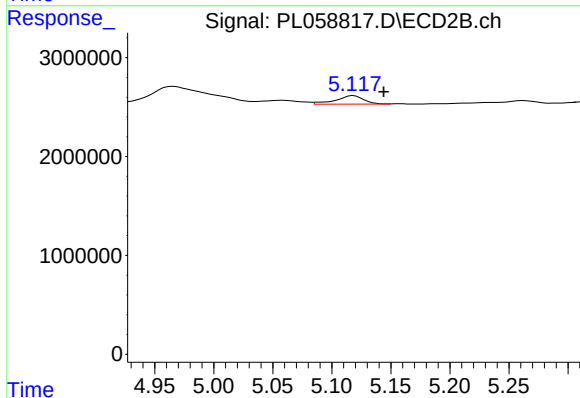


#7 delta-BHC

R.T.: 5.118 min
Delta R.T.: -0.026 min
Response: 1405345
Conc: 0.39 ng/ml

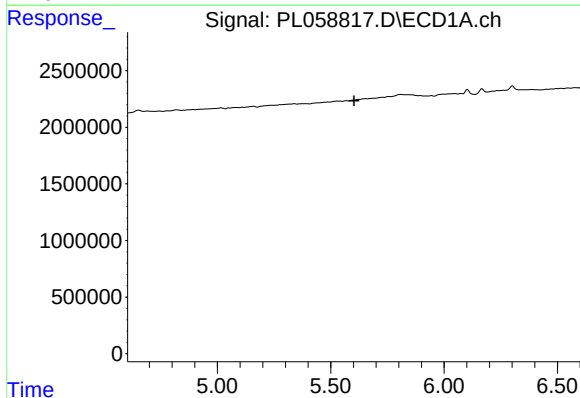


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.603 min
Response: 0
Conc: N.D.

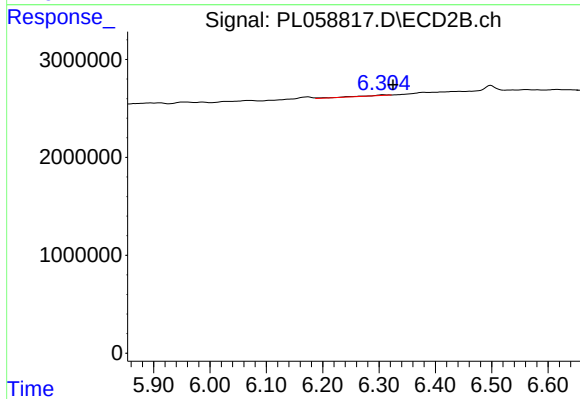

#9 Endosulfan I


R.T.: 6.307 min
Delta R.T.: -0.018 min
Response: 209356
Conc: 0.07 ng/ml

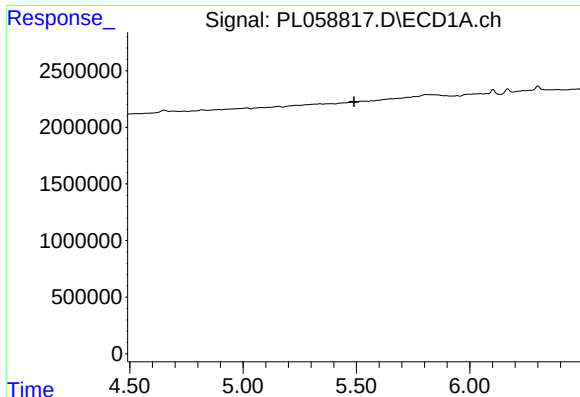

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.490 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

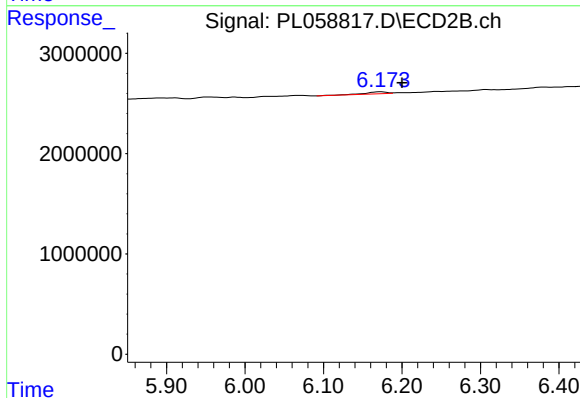


#10 gamma-Chlordane

R.T.: 6.174 min
Delta R.T.: -0.026 min
Response: 410554
Conc: 0.12 ng/ml

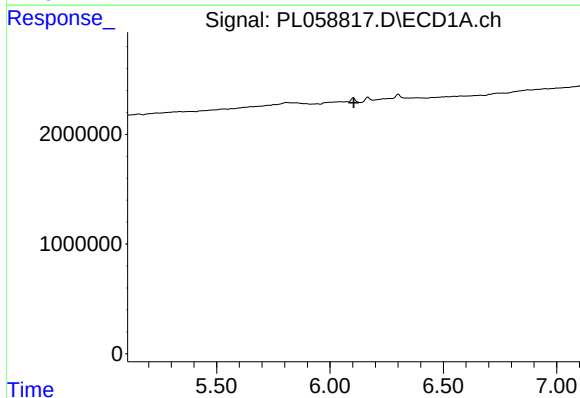


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.105 min
Response: 0
Conc: N.D.

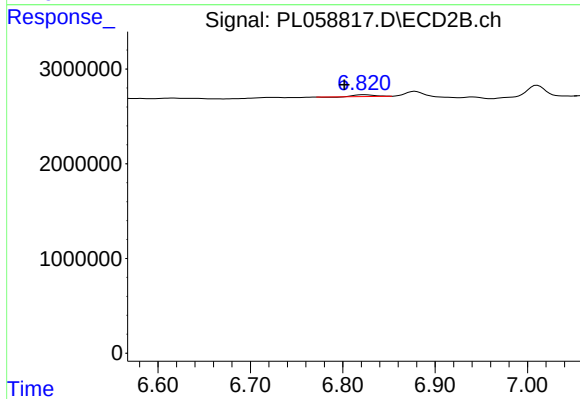

#14 Endrin


R.T.: 6.822 min
Delta R.T.: 0.021 min
Response: 252799
Conc: 0.10 ng/ml

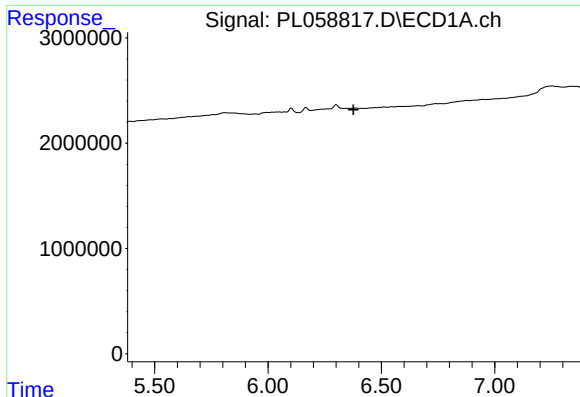

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.377 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

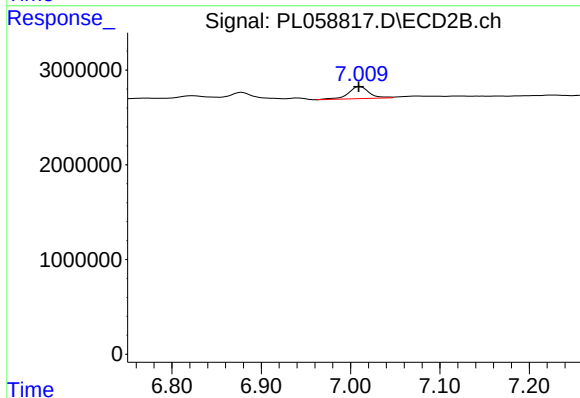


#15 Endosulfan II

R.T.: 7.011 min
Delta R.T.: 0.001 min
Response: 2043567
Conc: 0.73 ng/ml

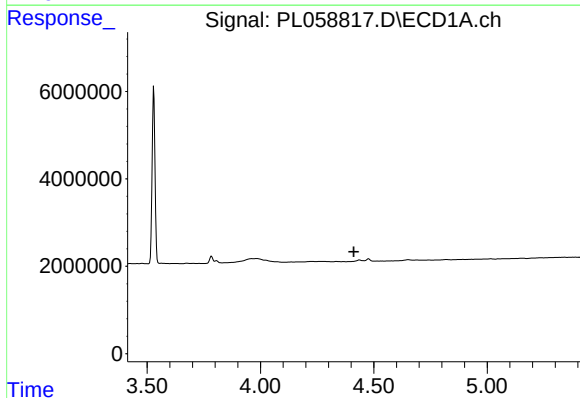


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.412 min
Response: 0
Conc: N.D.

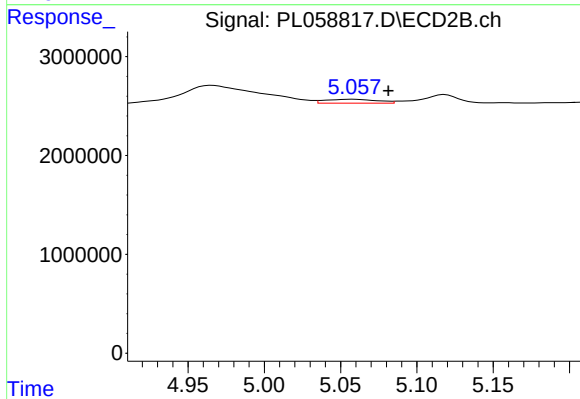

#23 Chlordane-1


R.T.: 5.059 min
Delta R.T.: -0.023 min
Response: 917386
Conc: 9.56 ng/ml

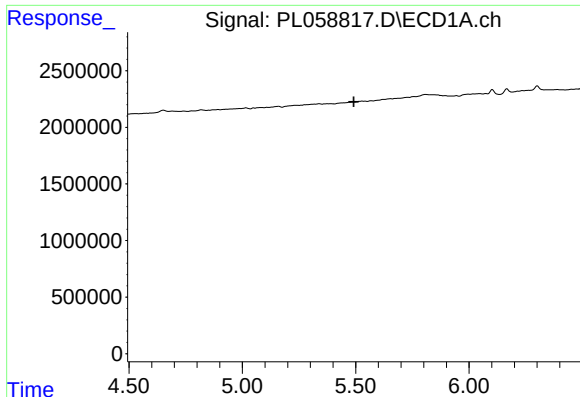

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.491 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

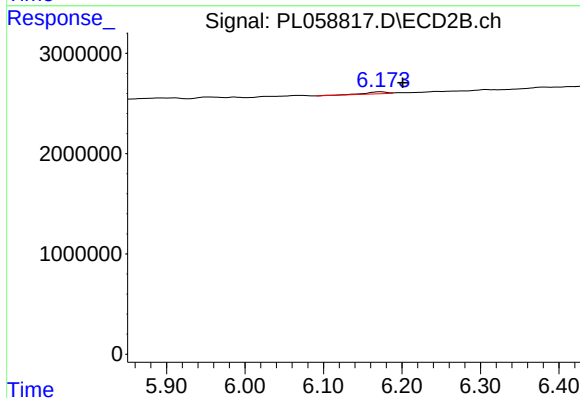


#25 Chlordane-3

R.T.: 6.174 min
Delta R.T.: -0.027 min
Response: 410554
Conc: 1.08 ng/ml

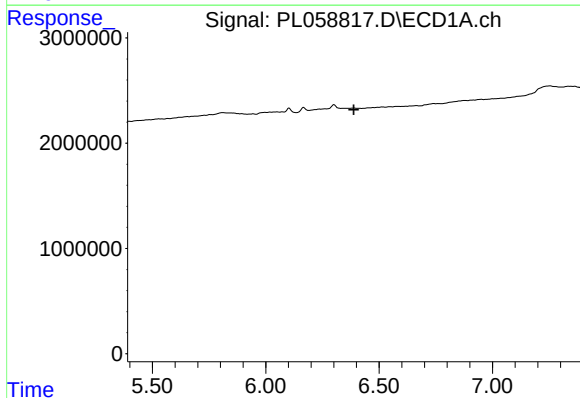


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.389 min
Response: 0
Conc: N.D.

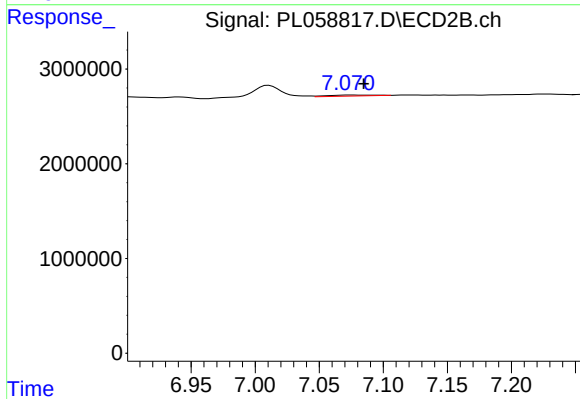

#27 Chlordane-5


R.T.: 7.072 min
Delta R.T.: -0.013 min
Response: 254062
Conc: 3.21 ng/ml

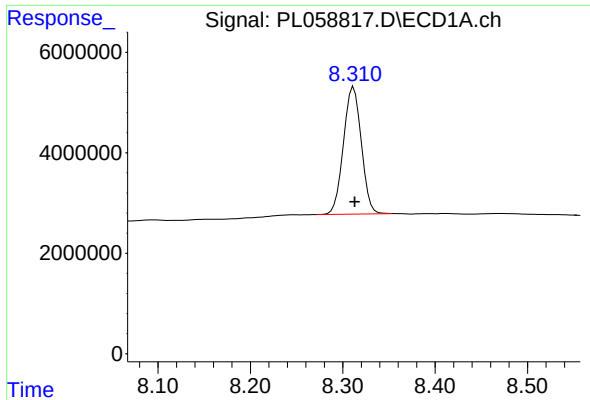

#28 Decachlorobiphenyl

R.T.: 8.312 min
Delta R.T.: -0.001 min
Response: 34041169
Conc: 20.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

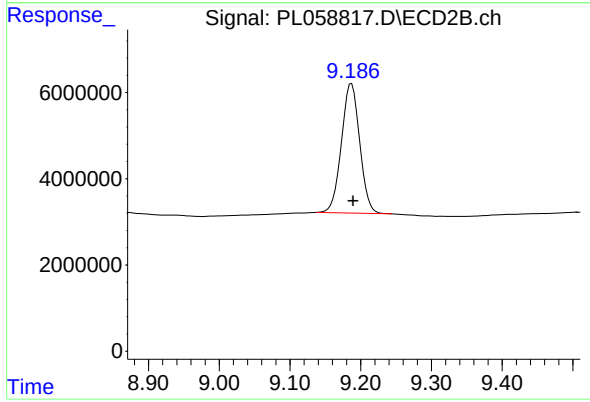

#28 Decachlorobiphenyl

R.T.: 9.187 min
Delta R.T.: -0.002 min
Response: 53946990
Conc: 20.46 ng/ml