

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052020\
 Data File : PL058823.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2020 16:10
 Operator : AJ\MA
 Sample : L2713-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BUS-WASH-SLUDGE-PIT

Manual Integrations
 APPROVED

mohammad
 5/22/2020 12:14:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 17:27:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.528	4.075	26114990	37588018	14.242m	13.878m
28) SA Decachlor...	8.313	9.187	19946223	39037910	11.806	14.808 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052020\
Data File : PL058823.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2020 16:10
Operator : AJ\MA
Sample : L2713-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BUS-WASH-SLUDGE-PIT


Manual Integrations
APPROVED

mohammad
5/22/2020 12:14:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 17:27:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

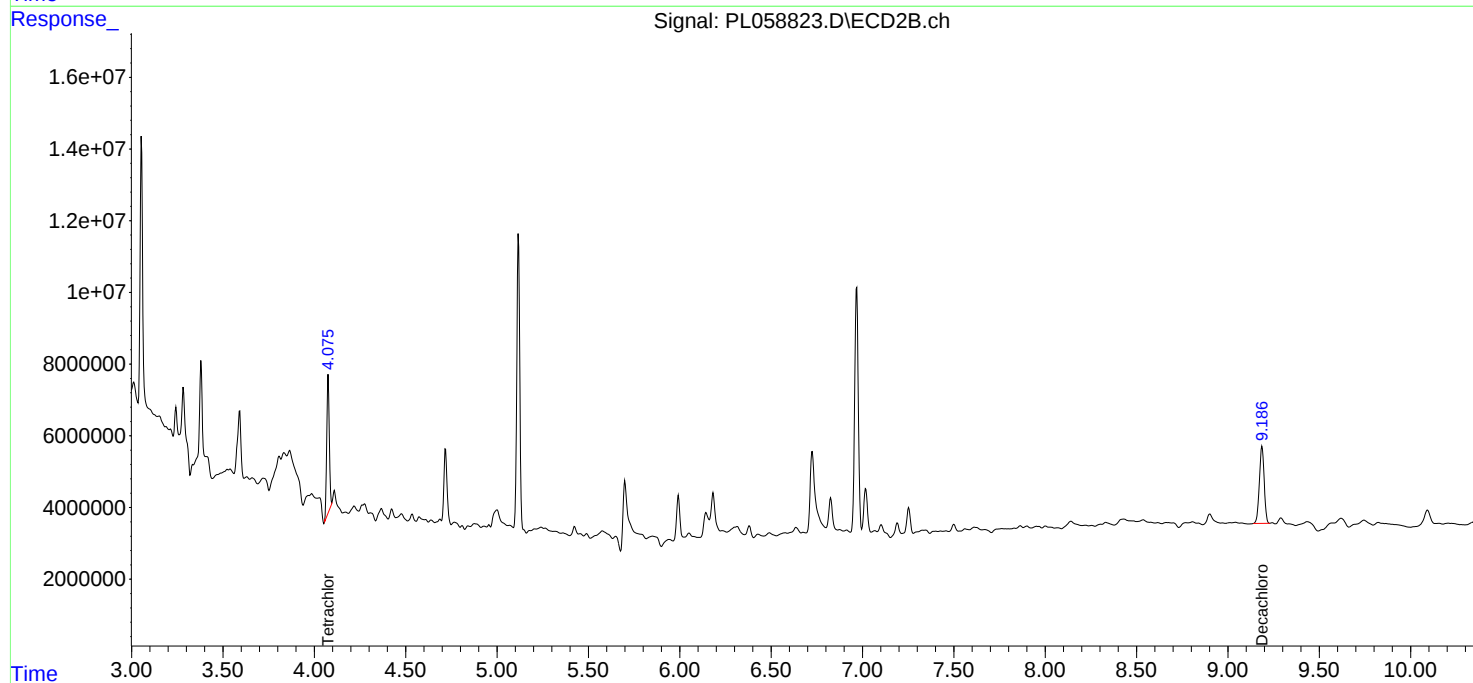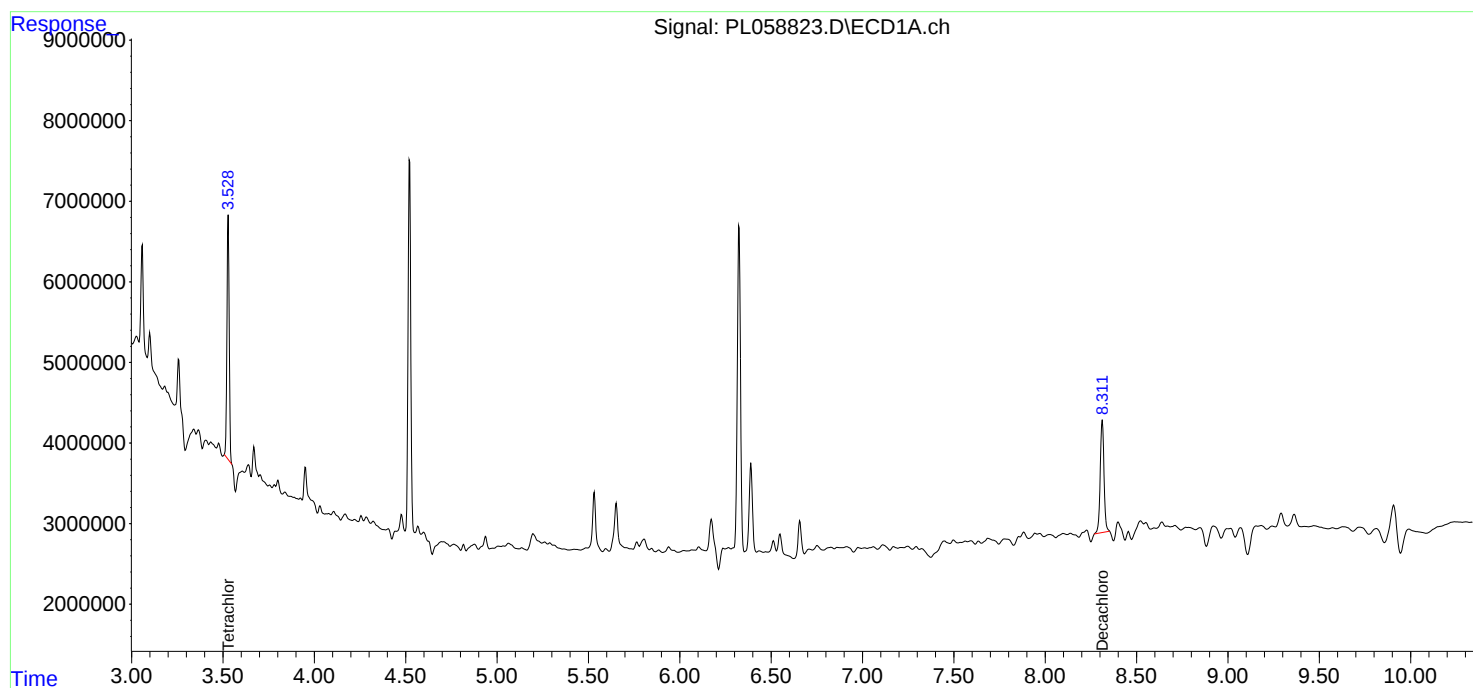

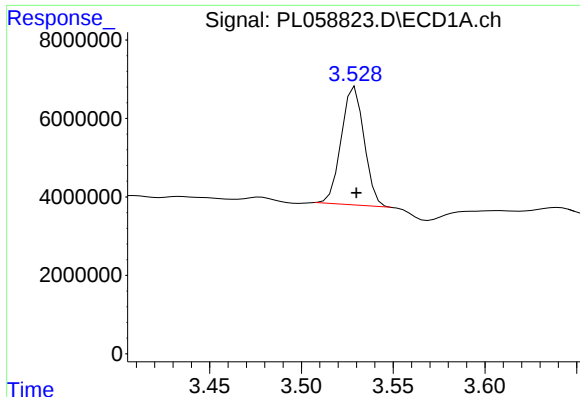


#1 Tetrachloro-m-xylene

R.T.: 3.528 min
Delta R.T.: -0.002 min
Response: 26114990
Conc: 14.24 ng/ml m

Instrument :
ECD_L
ClientSampleId :
BUS-WASH-SLUDGE-PIT


Manual Integrations
APPROVED

mohammad
5/22/2020 12:14:24 PM

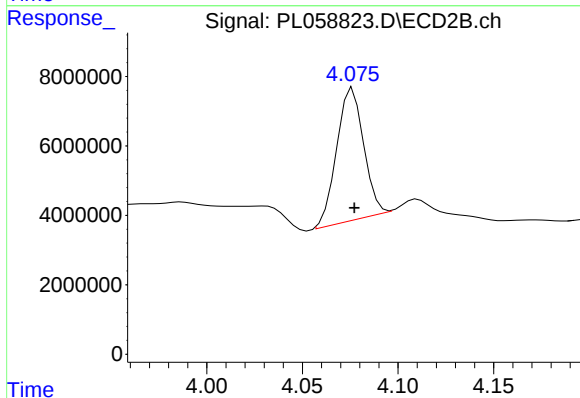


#1 Tetrachloro-m-xylene

R.T.: 4.075 min
Delta R.T.: -0.002 min
Response: 37588018
Conc: 13.88 ng/ml m

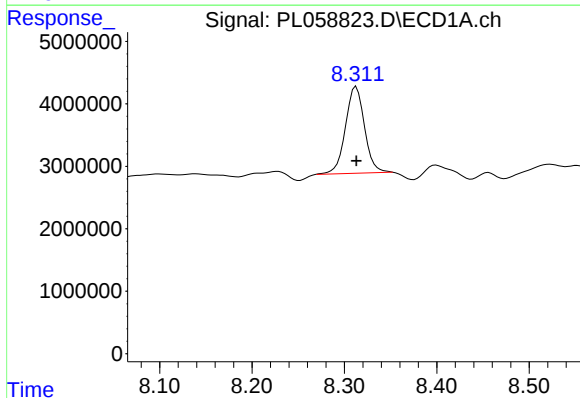

#28 Decachlorobiphenyl

R.T.: 8.313 min
Delta R.T.: 0.000 min
Response: 19946223
Conc: 11.81 ng/ml

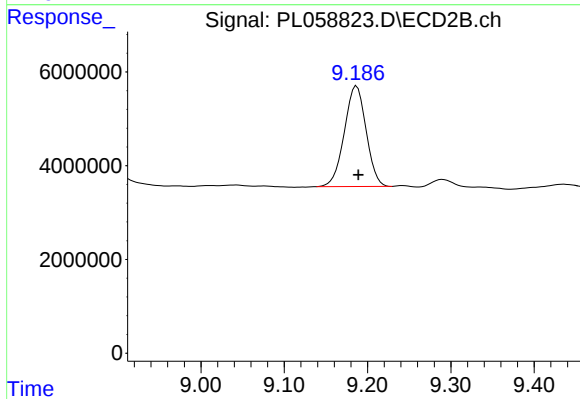

#28 Decachlorobiphenyl

R.T.: 9.187 min
Delta R.T.: -0.002 min
Response: 39037910
Conc: 14.81 ng/ml