

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052022\
 Data File : PL074882.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2022 15:53
 Operator : AR\AJ
 Sample : N2871-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 00:57:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.645	4.650	11719990	29507793	23.083	21.499
28)	SA Decachlor...	11.643	10.400	8889705	21557910	19.906	21.003
Target Compounds							
5)	MB Aldrin	0.000	6.506	0	414447	N.D.	0.276 #
6)	B beta-BHC	0.000	6.124f	0	334622	N.D.	0.421 #
11)	B alpha-Chl...	8.503f	0.000	5103605	0	8.360	N.D. #
15)	B Endosulfa...	0.000	8.385	0	268205	N.D.	0.237 #
17)	MA 4,4'-DDT	0.000	8.501	0	55950	N.D.	0.056 #
22)	Mirex	0.000	9.495	0	1493454	N.D.	1.542 #
26)	Chlordane-4	8.503f	0.000	5103605	0	52.975	N.D. #
27)	Chlordane-5	0.000	8.140	0	653086	N.D.	17.663 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052022\
Data File : PL074882.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2022 15:53
Operator : AR\AJ
Sample : N2871-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 00:57:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

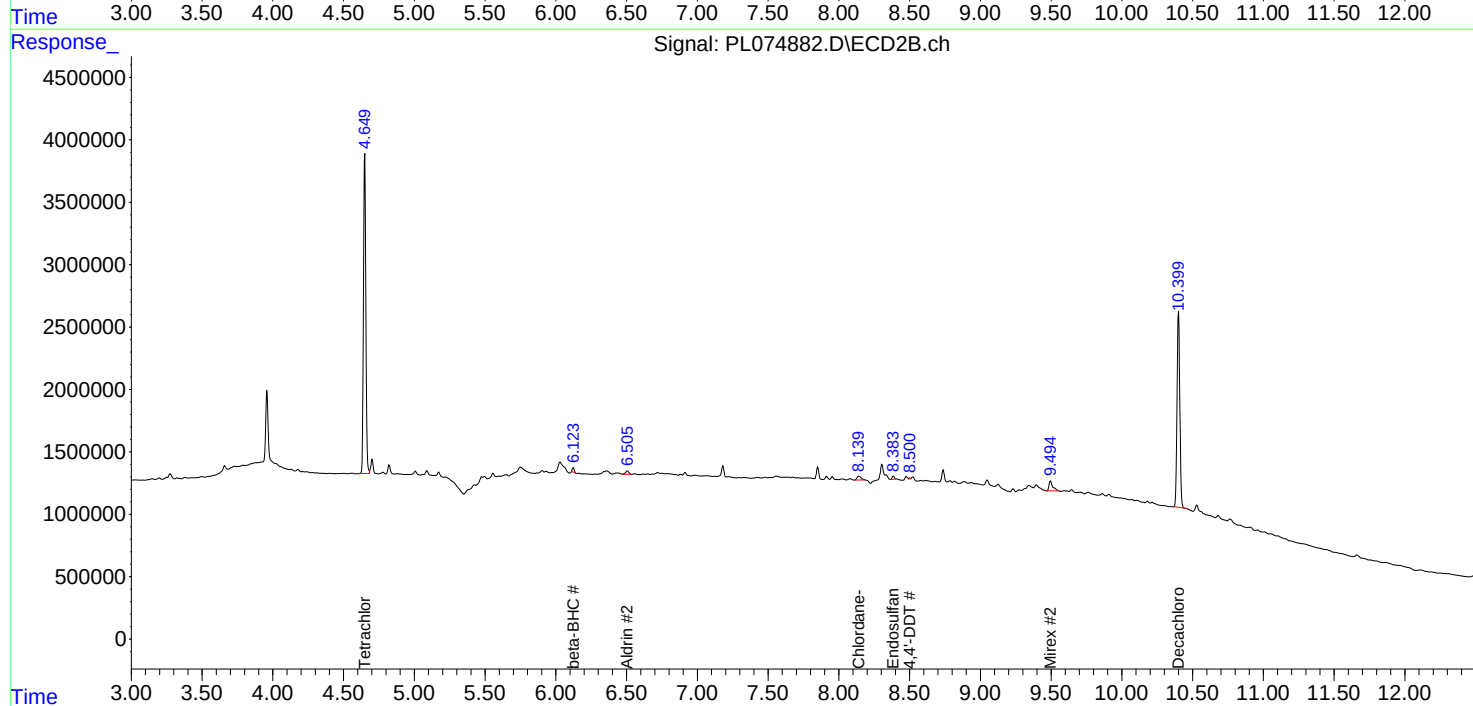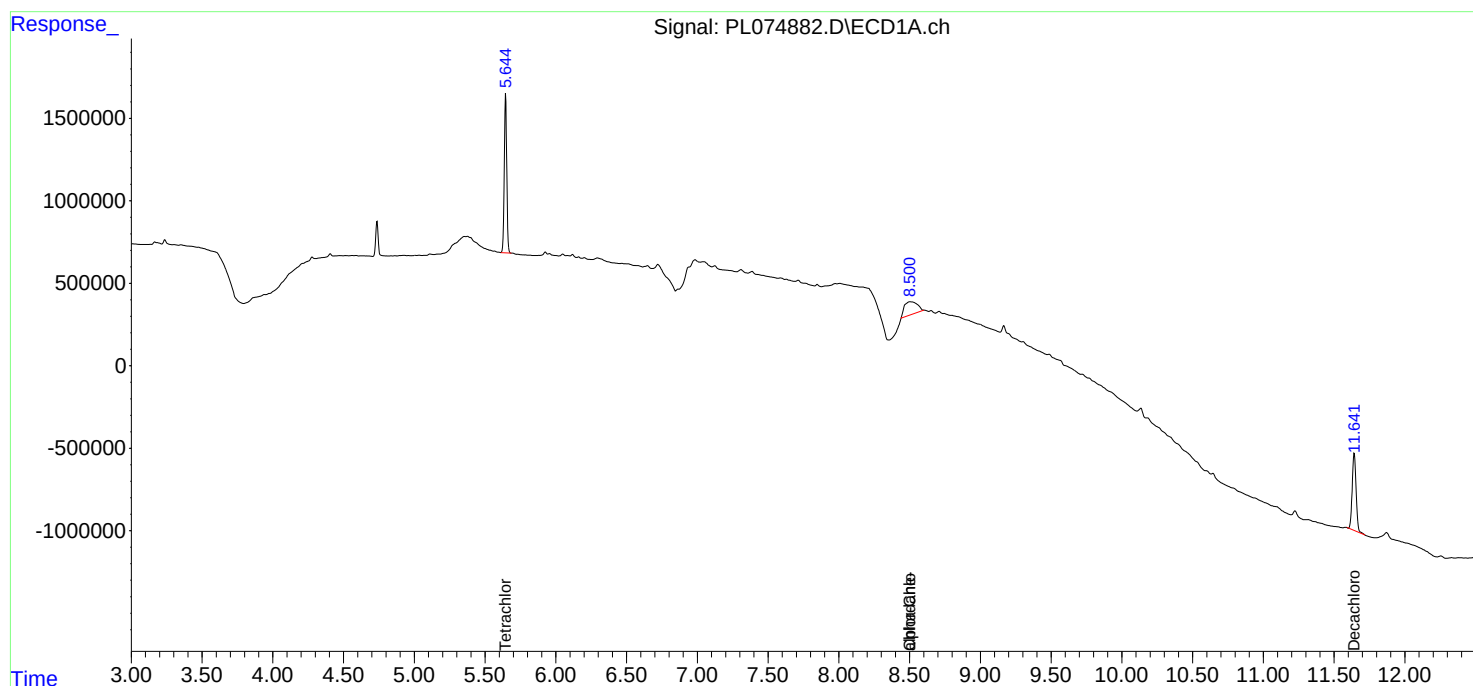


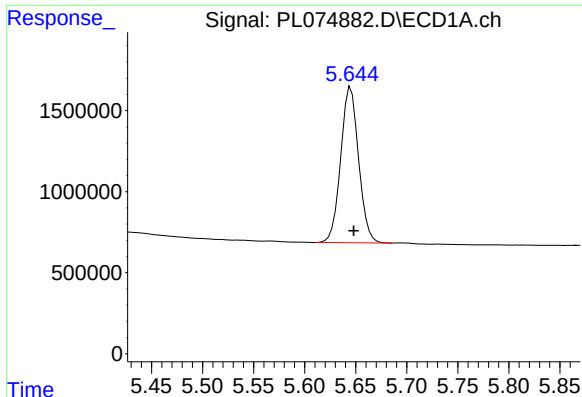

#1 Tetrachloro-m-xylene


R.T.: 5.645 min
Delta R.T.: -0.003 min
Response: 11719990
Conc: 23.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

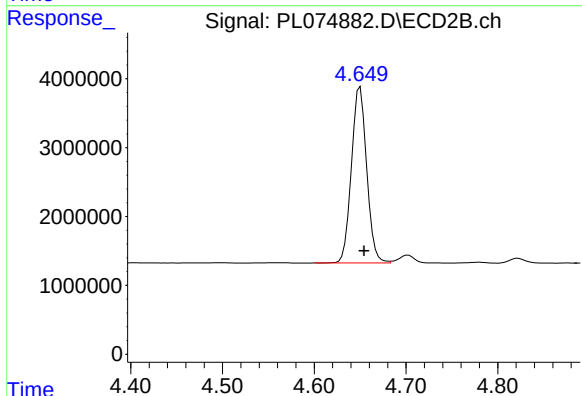


#1 Tetrachloro-m-xylene

R.T.: 4.650 min
Delta R.T.: -0.004 min
Response: 29507793
Conc: 21.50 ng/ml

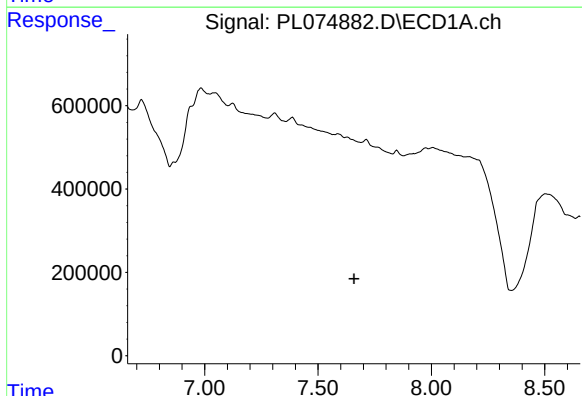


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.660 min
Response: 0
Conc: N.D.

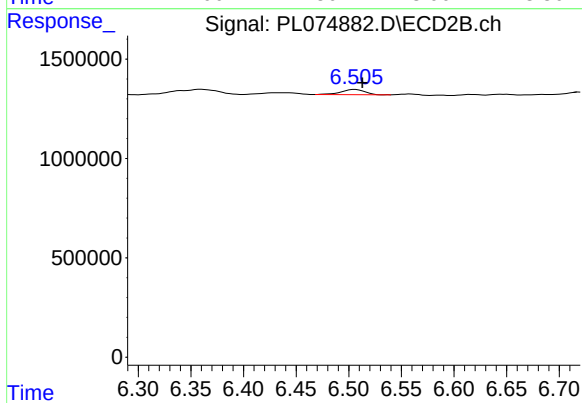

#5 Aldrin


R.T.: 6.506 min
Delta R.T.: -0.007 min
Response: 414447
Conc: 0.28 ng/ml

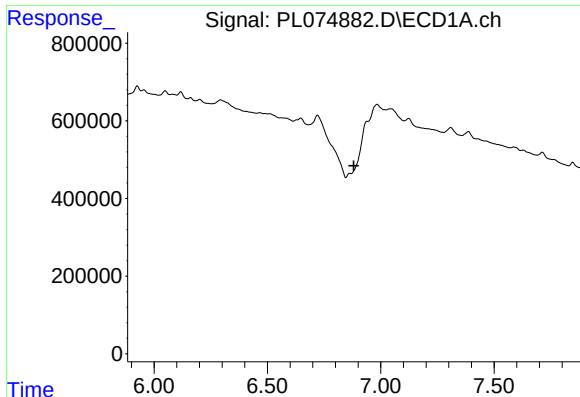

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.882 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

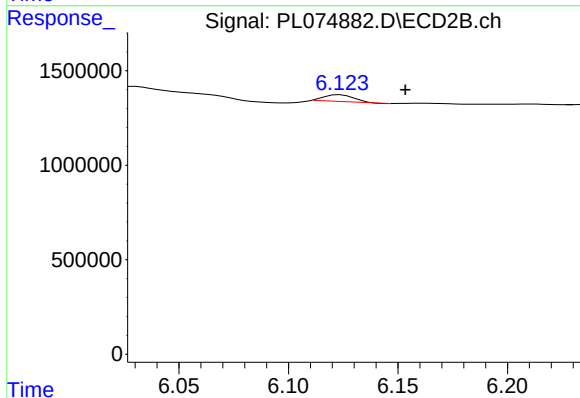


#6 beta-BHC

R.T.: 6.124 min
Delta R.T.: -0.030 min
Response: 334622
Conc: 0.42 ng/ml

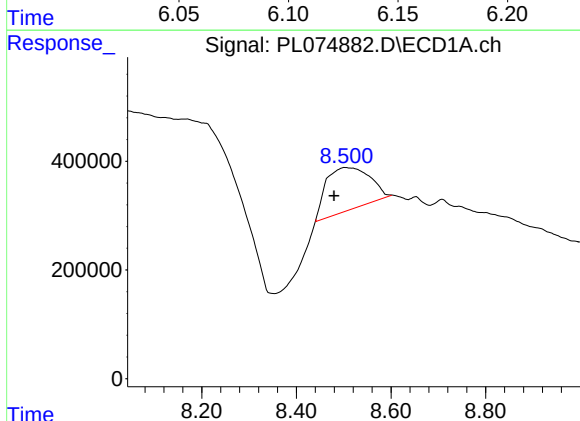


#11 alpha-Chlordane

R.T.: 8.503 min
Delta R.T.: 0.023 min
Response: 5103605
Conc: 8.36 ng/ml

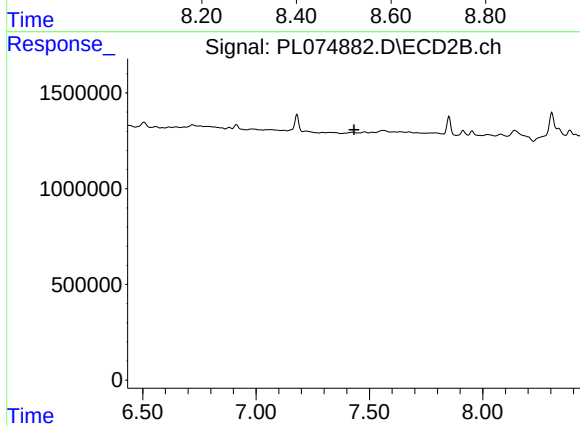

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.433 min
Response: 0
Conc: N.D.

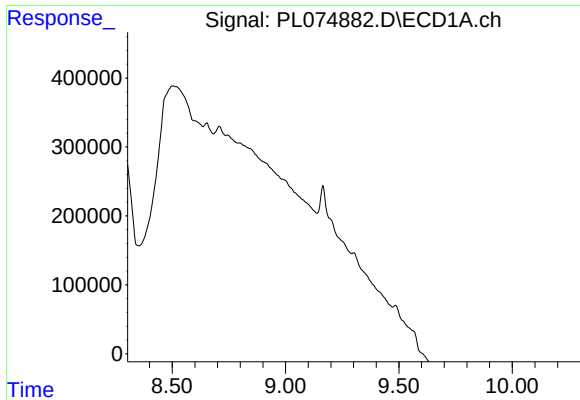

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 9.302 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

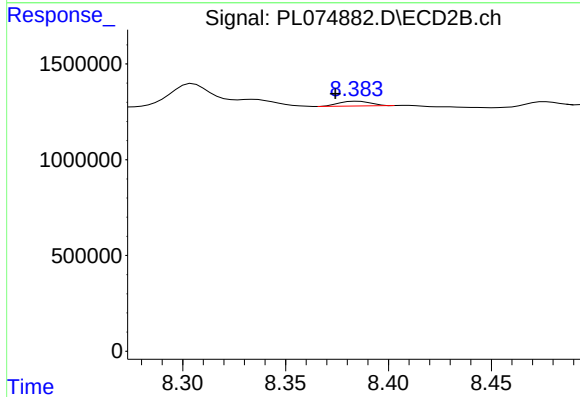


#15 Endosulfan II

R.T.: 8.385 min
Delta R.T.: 0.011 min
Response: 268205
Conc: 0.24 ng/ml

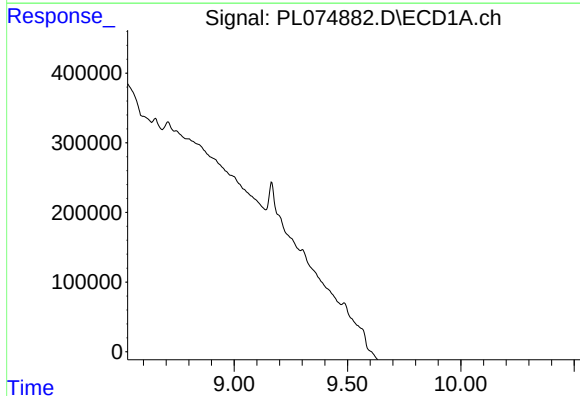


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 9.527 min
Response: 0
Conc: N.D.

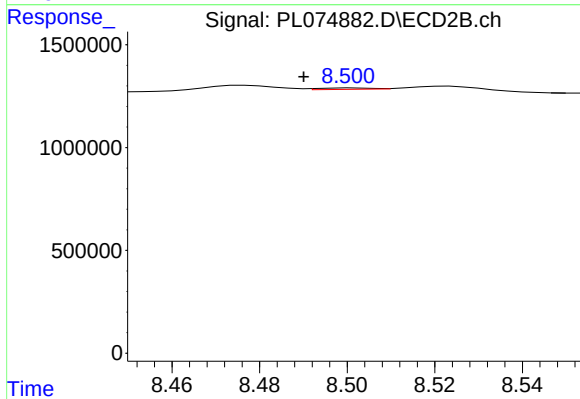

#17 4,4'-DDT


R.T.: 8.501 min
Delta R.T.: 0.011 min
Response: 55950
Conc: 0.06 ng/ml

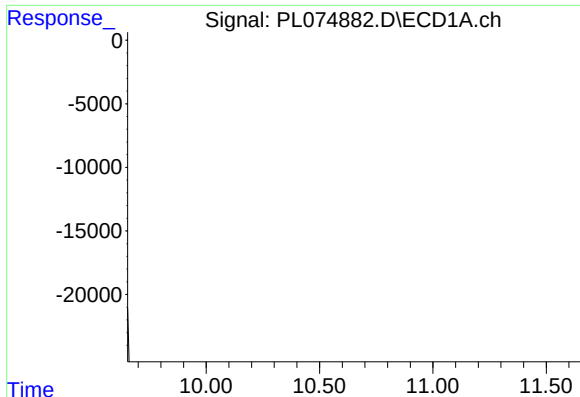

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 10.652 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

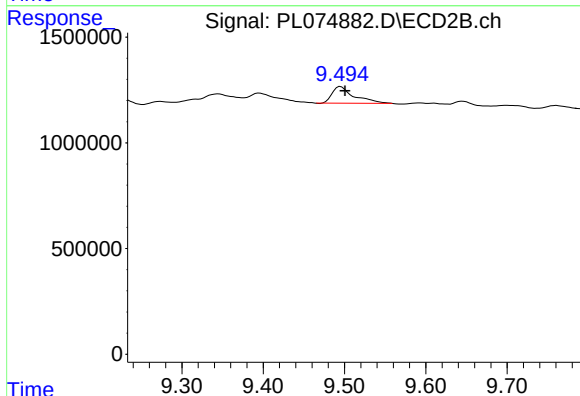


#22 Mirex

R.T.: 9.495 min
Delta R.T.: -0.005 min
Response: 1493454
Conc: 1.54 ng/ml

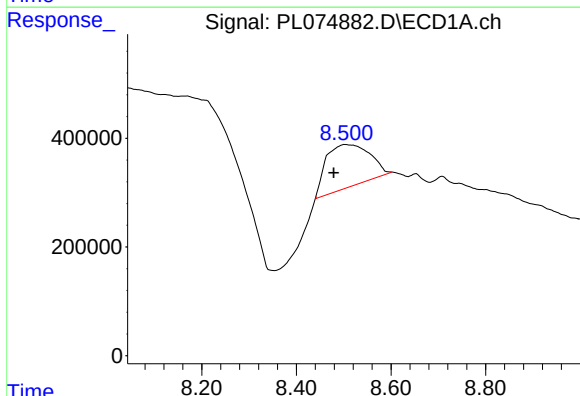


#26 Chlordane-4

R.T.: 8.503 min
Delta R.T.: 0.024 min
Response: 5103605
Conc: 52.97 ng/ml

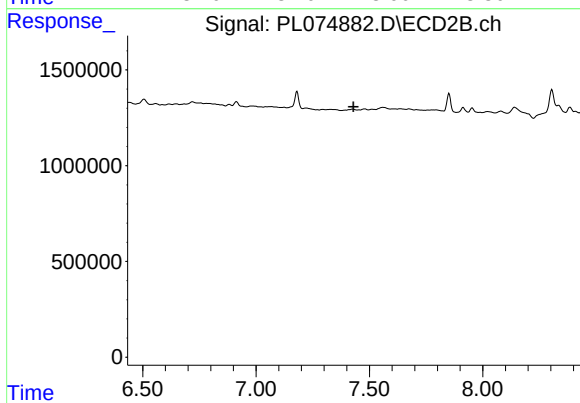

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

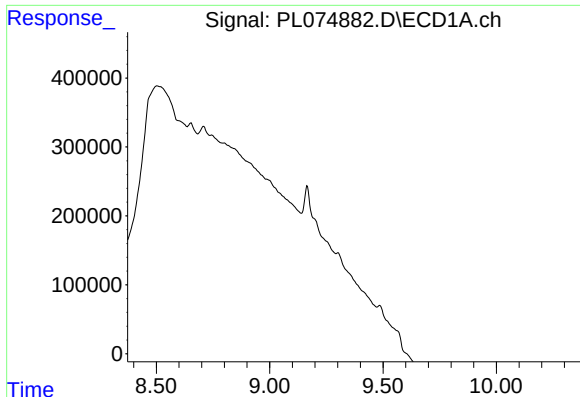

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.371 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

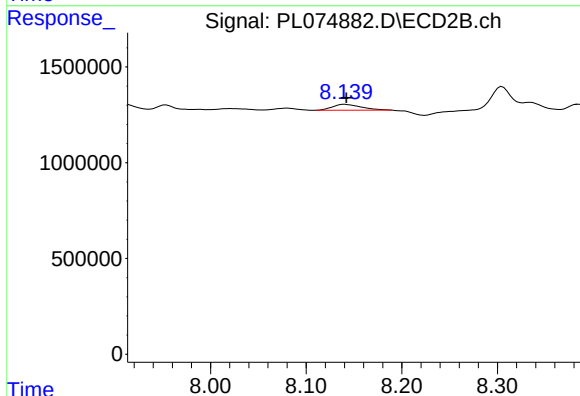


#27 Chlordane-5

R.T.: 8.140 min
Delta R.T.: -0.002 min
Response: 653086
Conc: 17.66 ng/ml

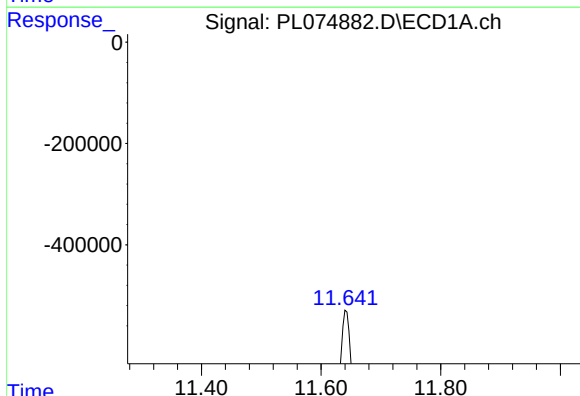

#28 Decachlorobiphenyl

R.T.: 11.643 min
Delta R.T.: -0.008 min
Response: 8889705
Conc: 19.91 ng/ml

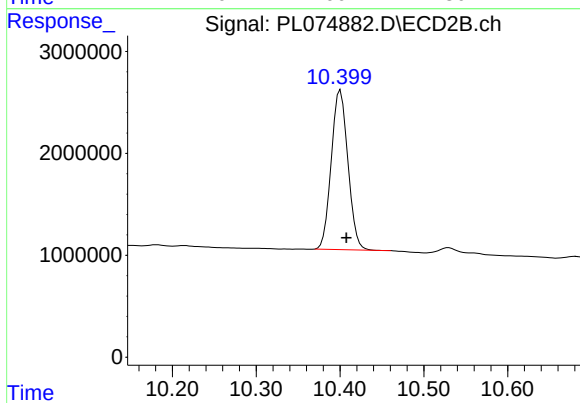

#28 Decachlorobiphenyl

R.T.: 10.400 min
Delta R.T.: -0.007 min
Response: 21557910
Conc: 21.00 ng/ml