

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052022\
 Data File : PL074883.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2022 16:09
 Operator : AR\AJ
 Sample : N2871-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 00:57:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.646	4.650	10726550	28073400	21.126	20.454
28)	SA Decachlor...	11.643	10.401	7761953	18705257	17.381	18.224
Target Compounds							
2)	A alpha-BHC	6.204f	0.000	252294	0	0.369	N.D. #
5)	MB Aldrin	0.000	6.506	0	637684	N.D.	0.425 #
9)	A Endosulfan I	8.510f	0.000	5260442	0	9.125	N.D. #
12)	B 4,4'-DDE	8.653	0.000	331004	0	0.715	N.D. #
13)	MA Dieldrin	0.000	7.768	0	346735	N.D.	0.272 #
15)	B Endosulfa...	0.000	8.385	0	207551	N.D.	0.184 #
17)	MA 4,4'-DDT	0.000	8.477	0	262376	N.D.	0.262 #
21)	B Endrin ke...	0.000	9.340f	0	28781	N.D.	0.026 #
27)	Chlordane-5	0.000	8.153	0	1111134	N.D.	30.052 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052022\
Data File : PL074883.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2022 16:09
Operator : AR\AJ
Sample : N2871-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 00:57:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

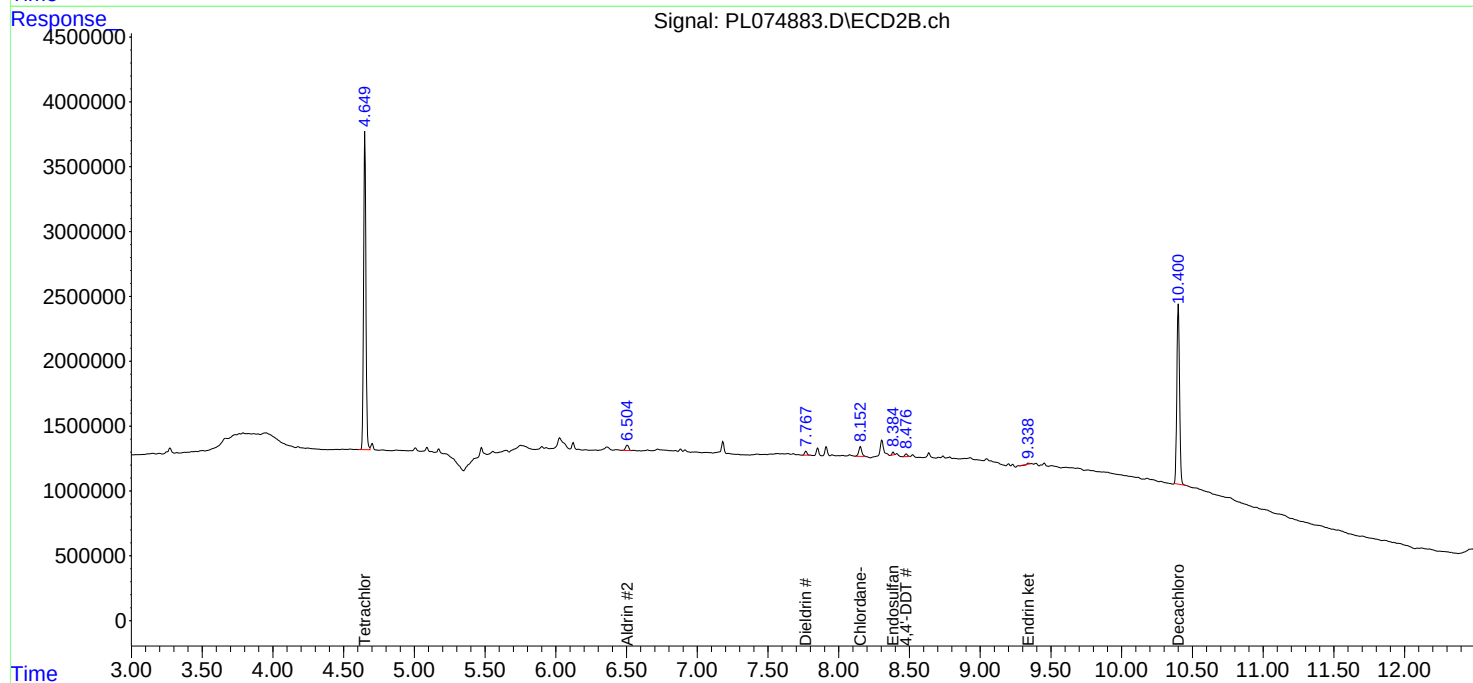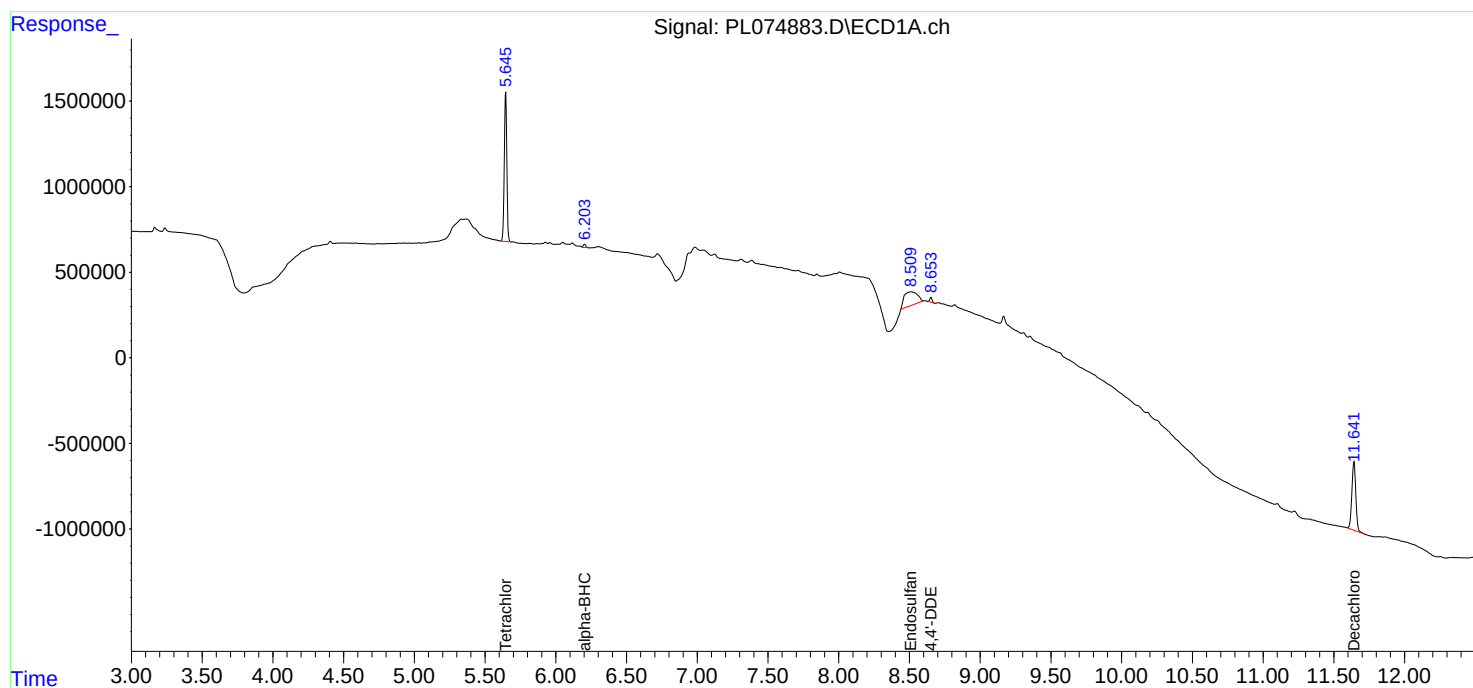


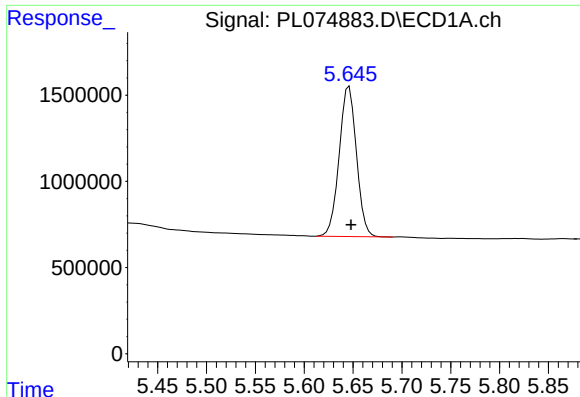

#1 Tetrachloro-m-xylene


R.T.: 5.646 min
Delta R.T.: -0.002 min
Response: 10726550
Conc: 21.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

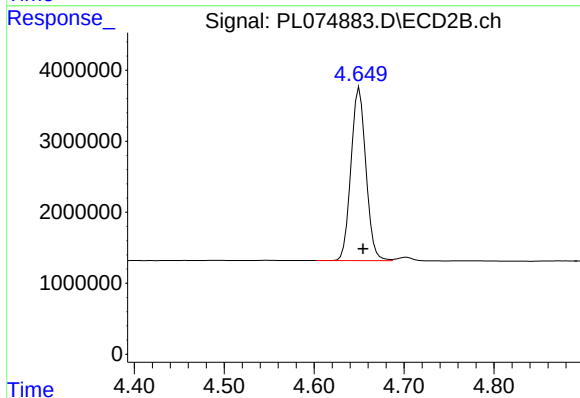


#1 Tetrachloro-m-xylene

R.T.: 4.650 min
Delta R.T.: -0.004 min
Response: 28073400
Conc: 20.45 ng/ml

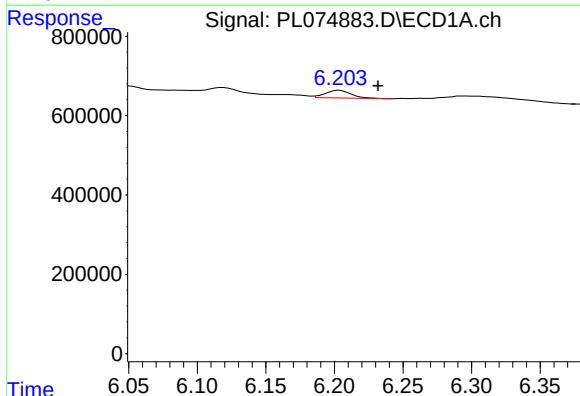


#2 alpha-BHC

R.T.: 6.204 min
Delta R.T.: -0.028 min
Response: 252294
Conc: 0.37 ng/ml

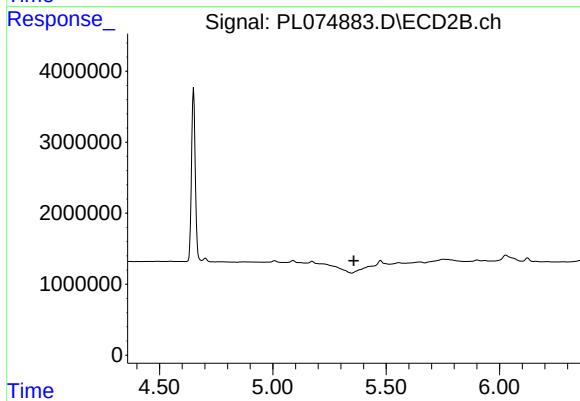

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 5.357 min
Response: 0
Conc: N.D.

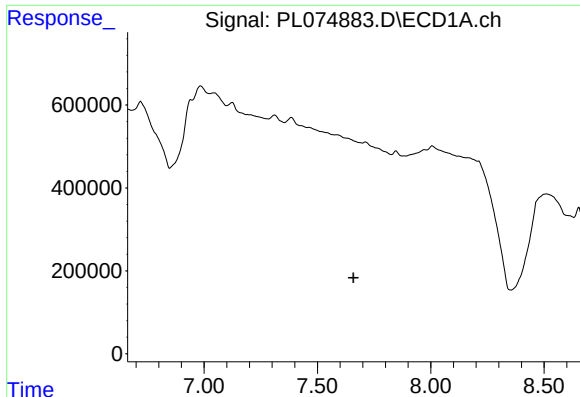

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 7.660 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

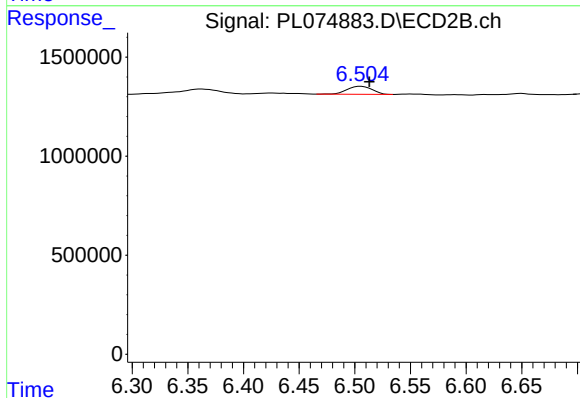


#5 Aldrin

R.T.: 6.506 min
Delta R.T.: -0.007 min
Response: 637684
Conc: 0.42 ng/ml

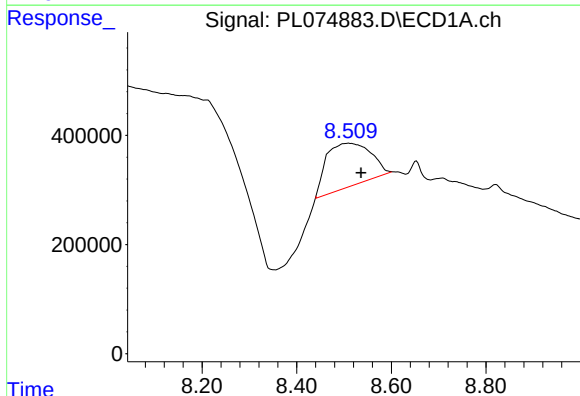


#9 Endosulfan I

R.T.: 8.510 min
Delta R.T.: -0.026 min
Response: 5260442
Conc: 9.12 ng/ml

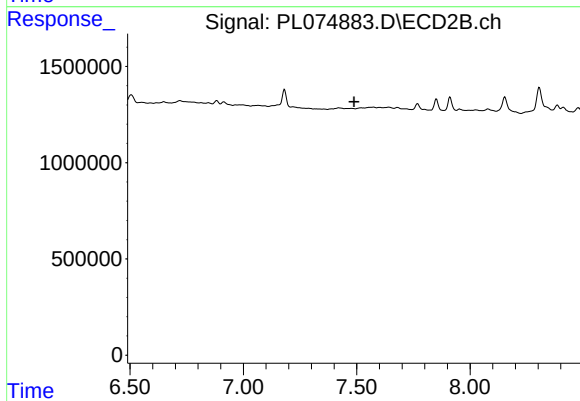

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.489 min
Response: 0
Conc: N.D.

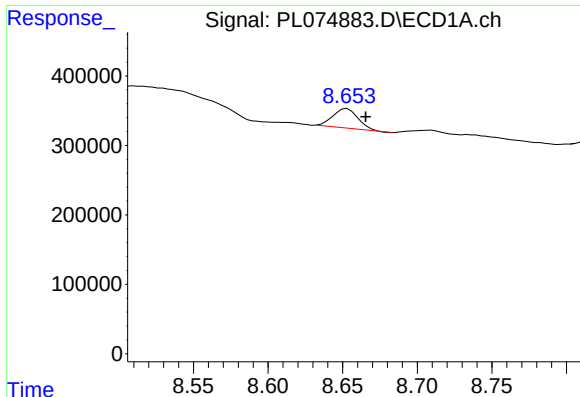

#12 4,4'-DDE


R.T.: 8.653 min
Delta R.T.: -0.012 min
Response: 331004
Conc: 0.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

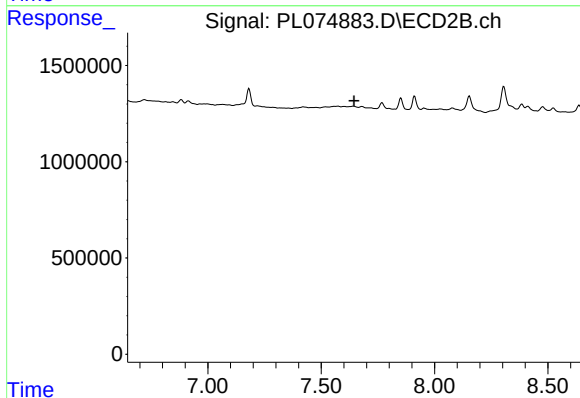


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 7.645 min
Response: 0
Conc: N.D.

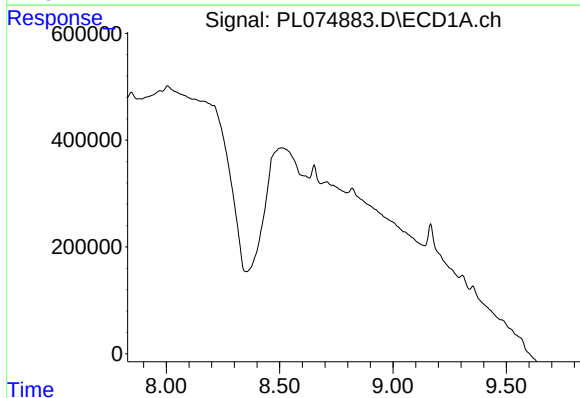


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.827 min
Response: 0
Conc: N.D.

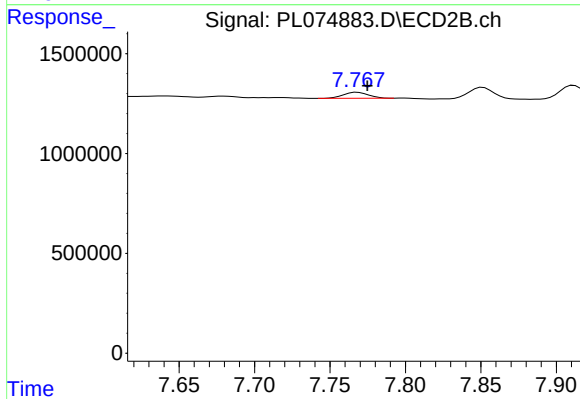

#13 Dieldrin


R.T.: 7.768 min
Delta R.T.: -0.007 min
Response: 346735
Conc: 0.27 ng/ml

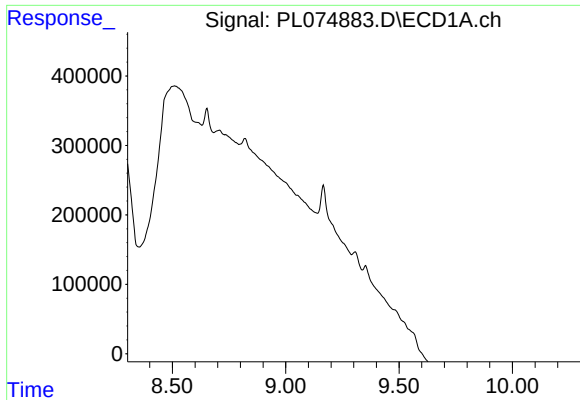

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 9.302 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

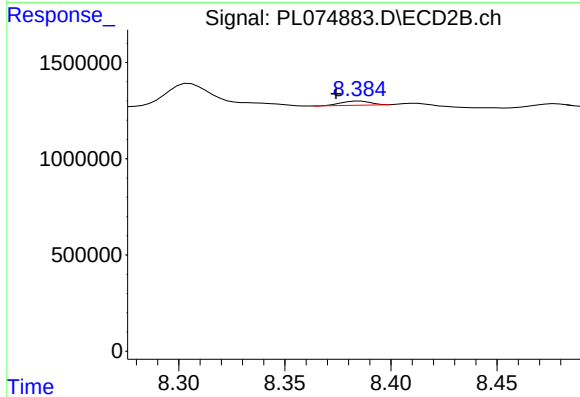


#15 Endosulfan II

R.T.: 8.385 min
Delta R.T.: 0.011 min
Response: 207551
Conc: 0.18 ng/ml

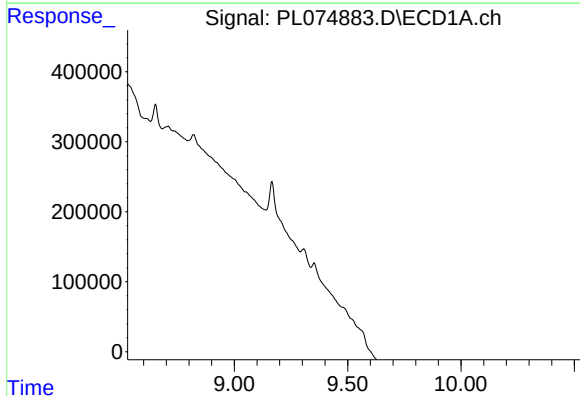


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 9.527 min
Response: 0
Conc: N.D.

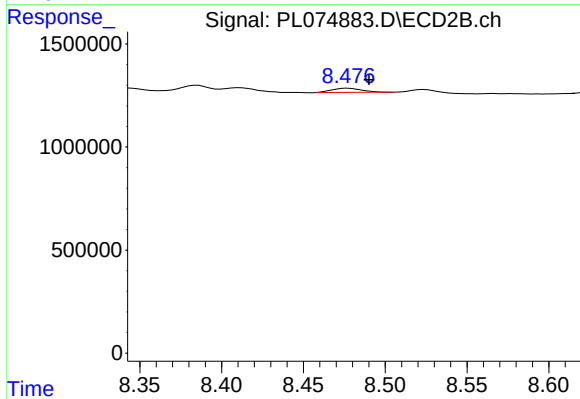

#17 4,4'-DDT


R.T.: 8.477 min
Delta R.T.: -0.013 min
Response: 262376
Conc: 0.26 ng/ml

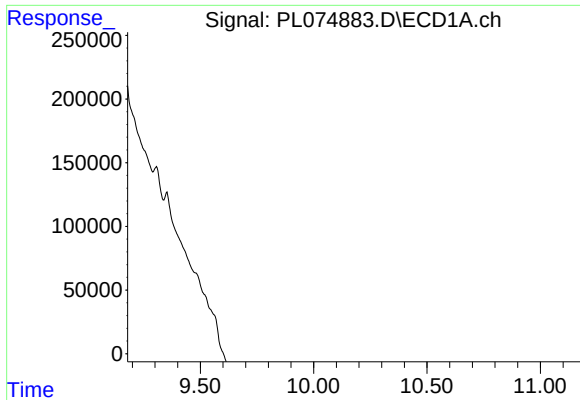

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 10.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

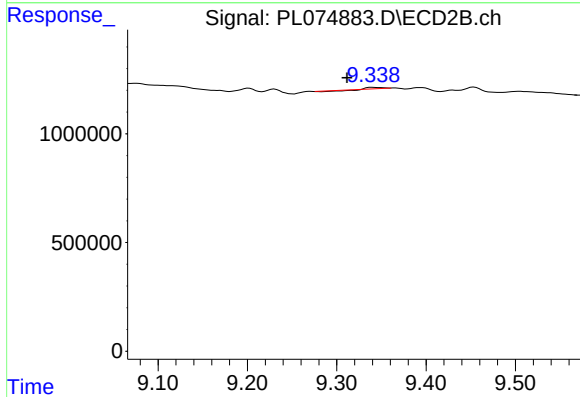


#21 Endrin ketone

R.T.: 9.340 min
Delta R.T.: 0.028 min
Response: 28781
Conc: 0.03 ng/ml

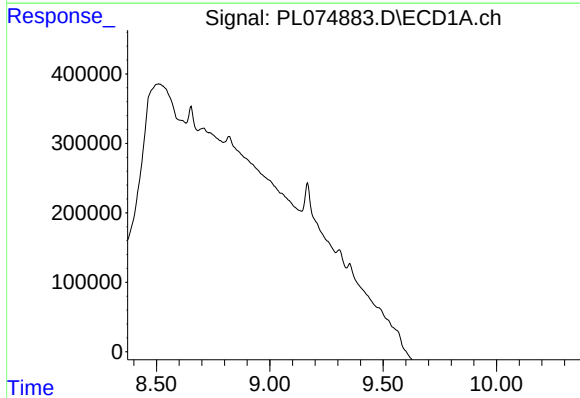


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 9.371 min
Response: 0
Conc: N.D.

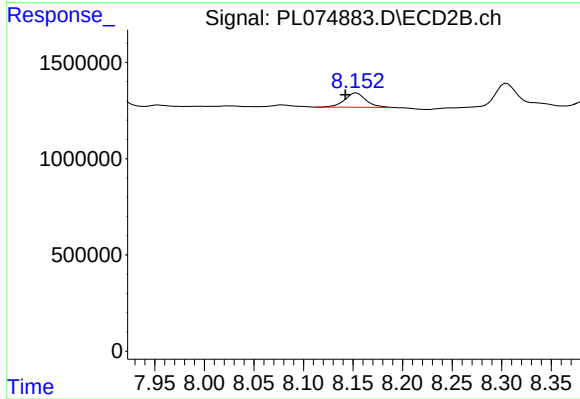

#27 Chlordane-5


R.T.: 8.153 min
Delta R.T.: 0.011 min
Response: 1111134
Conc: 30.05 ng/ml

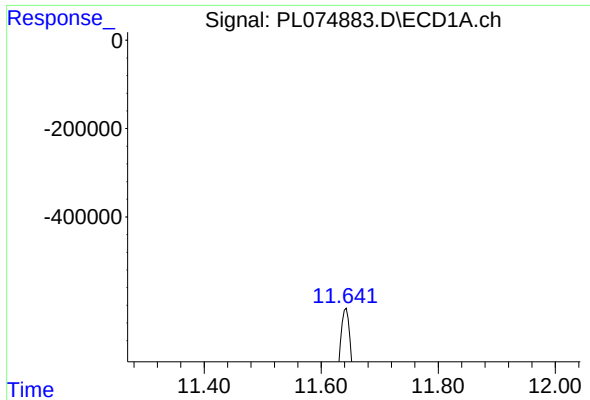

#28 Decachlorobiphenyl

R.T.: 11.643 min
Delta R.T.: -0.008 min
Response: 7761953
Conc: 17.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

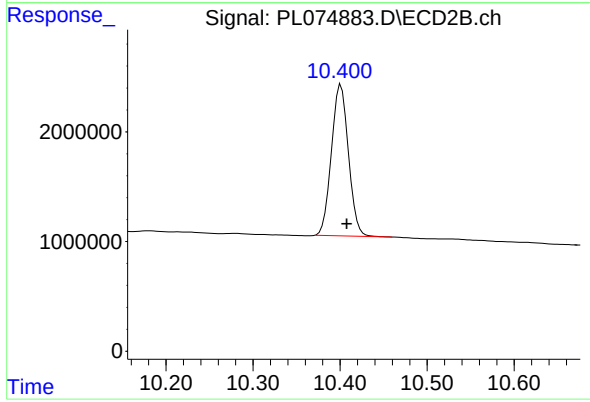

#28 Decachlorobiphenyl

R.T.: 10.401 min
Delta R.T.: -0.007 min
Response: 18705257
Conc: 18.22 ng/ml