

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052022\
 Data File : PL074884.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2022 16:26
 Operator : AR\AJ
 Sample : N2871-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 00:57:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.646	4.650	10879598	28814615	21.428	20.994
28)	SA Decachlor...	11.642	10.401	7729838	18366582	17.309	17.894
Target Compounds							
2)	A alpha-BHC	6.204f	0.000	276600	0	0.404	N.D. #
5)	MB Aldrin	0.000	6.506	0	985927	N.D.	0.657 #
6)	B beta-BHC	0.000	6.123f	0	450000	N.D.	0.567 #
9)	A Endosulfan I	8.516f	0.000	4954658	0	8.594	N.D. #
15)	B Endosulfa...	0.000	8.385	0	274235	N.D.	0.243 #
17)	MA 4,4'-DDT	0.000	8.476	0	309552	N.D.	0.309 #
21)	B Endrin ke...	0.000	9.340f	0	34460	N.D.	0.031 #
22)	Mirex	0.000	9.502	0	244589	N.D.	0.253 #
27)	Chlordane-5	0.000	8.154	0	1608953	N.D.	43.516 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052022\
Data File : PL074884.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2022 16:26
Operator : AR\AJ
Sample : N2871-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 00:57:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

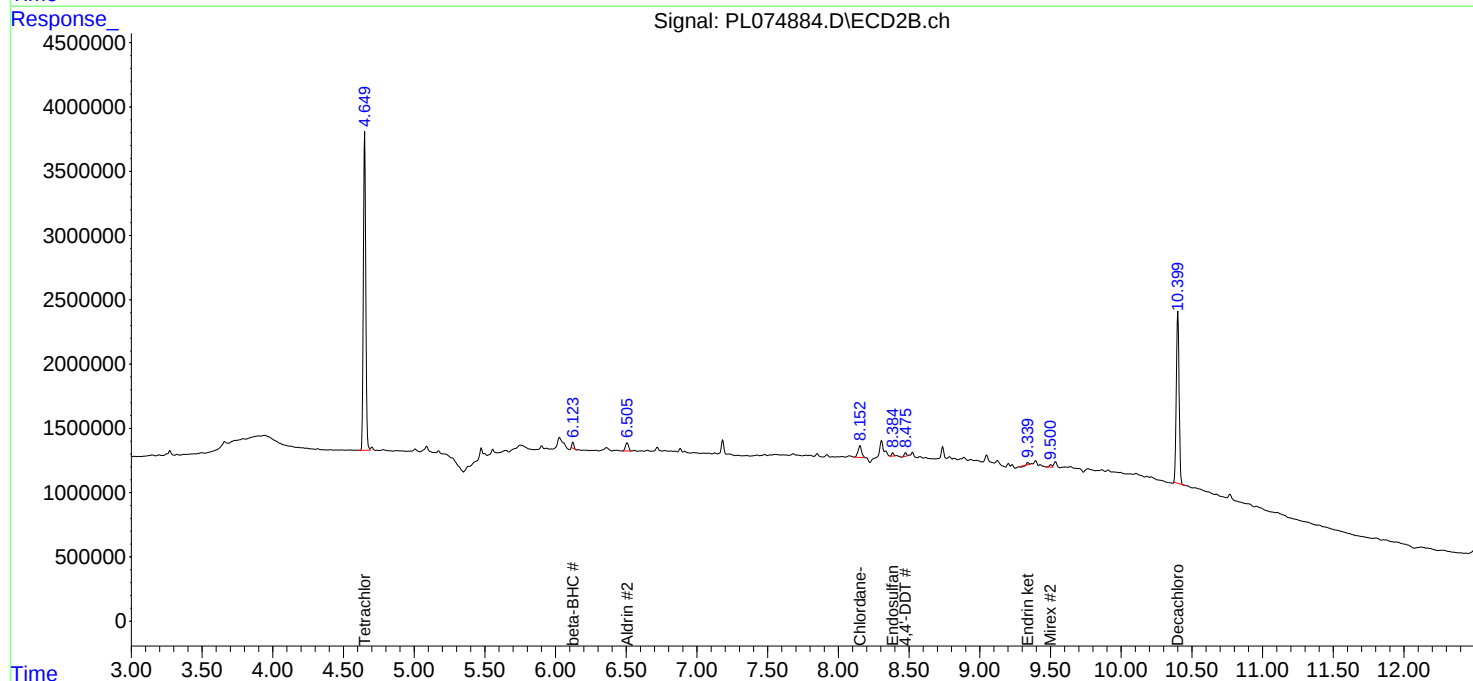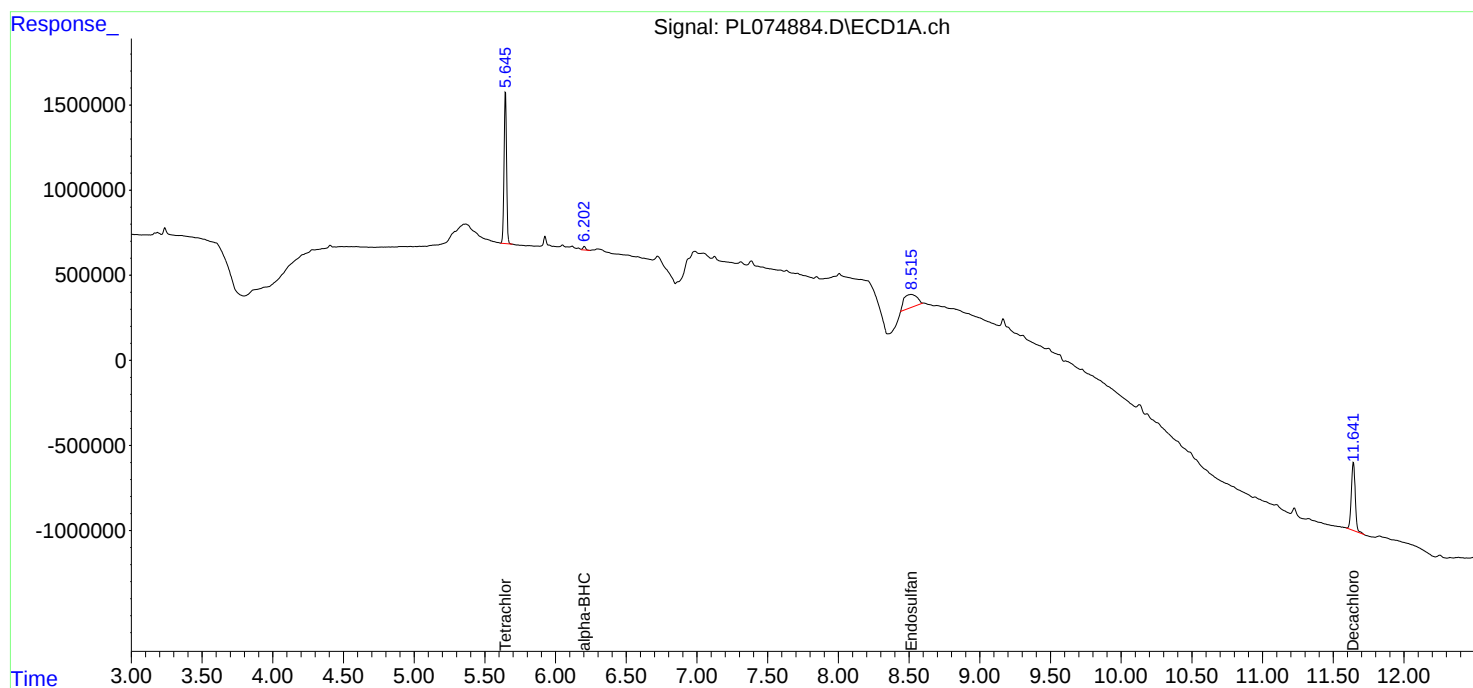


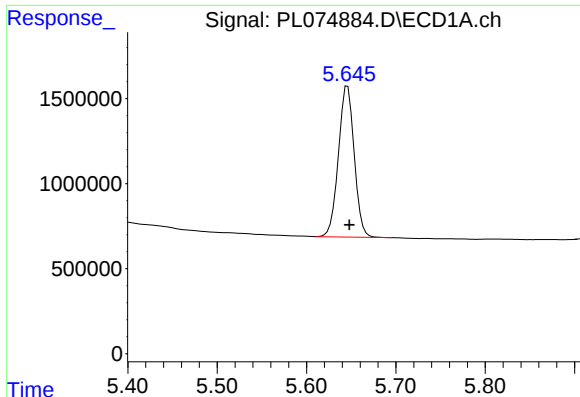

#1 Tetrachloro-m-xylene


R.T.: 5.646 min
Delta R.T.: -0.002 min
Response: 10879598
Conc: 21.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

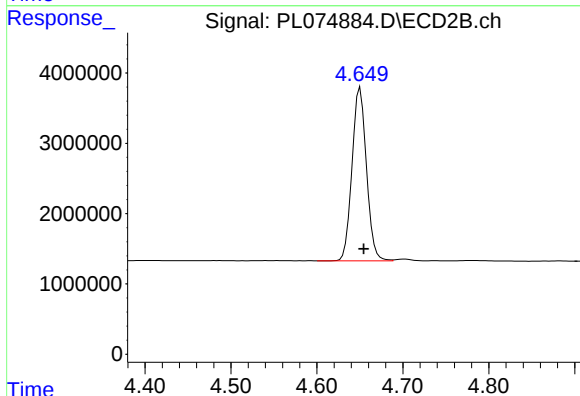


#1 Tetrachloro-m-xylene

R.T.: 4.650 min
Delta R.T.: -0.004 min
Response: 28814615
Conc: 20.99 ng/ml

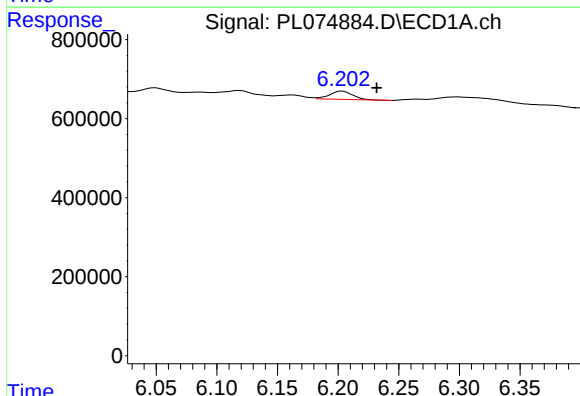


#2 alpha-BHC

R.T.: 6.204 min
Delta R.T.: -0.028 min
Response: 276600
Conc: 0.40 ng/ml

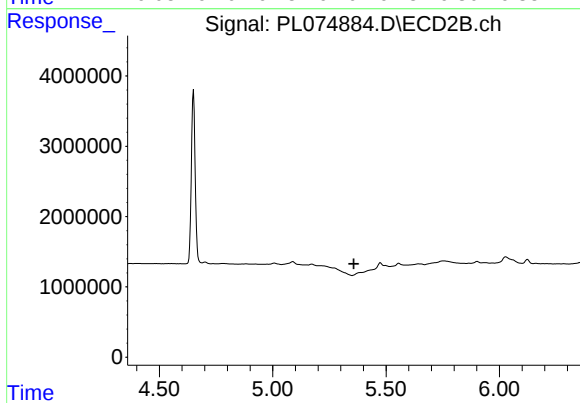

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 5.357 min
Response: 0
Conc: N.D.

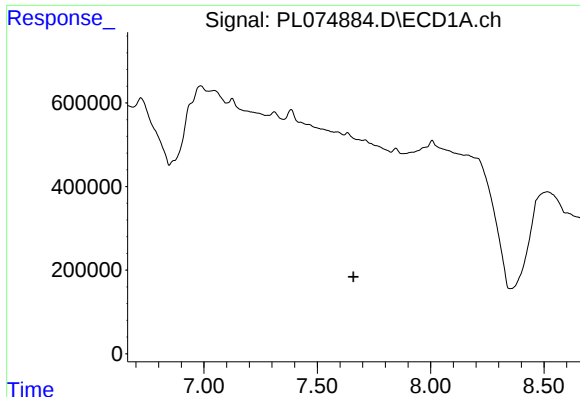

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 7.660 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

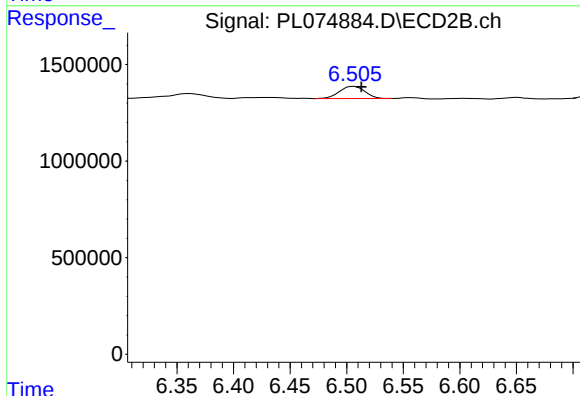


#5 Aldrin

R.T.: 6.506 min
Delta R.T.: -0.007 min
Response: 985927
Conc: 0.66 ng/ml

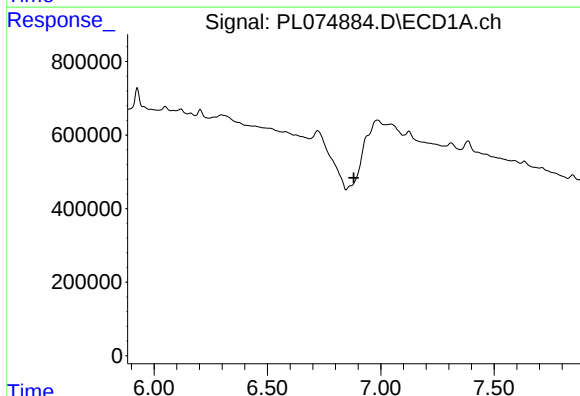


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 6.882 min
Response: 0
Conc: N.D.

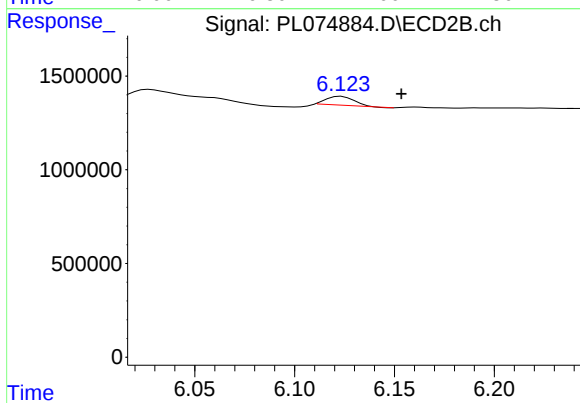

#6 beta-BHC


R.T.: 6.123 min
Delta R.T.: -0.030 min
Response: 450000
Conc: 0.57 ng/ml

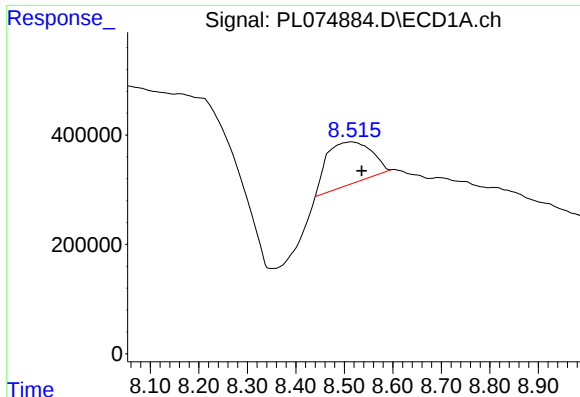

#9 Endosulfan I


R.T.: 8.516 min
Delta R.T.: -0.020 min
Response: 4954658
Conc: 8.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

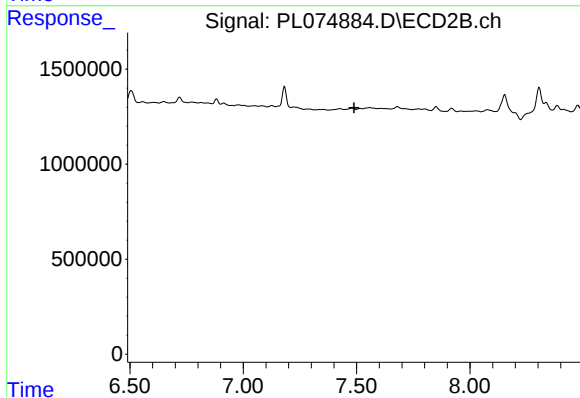


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.489 min
Response: 0
Conc: N.D.

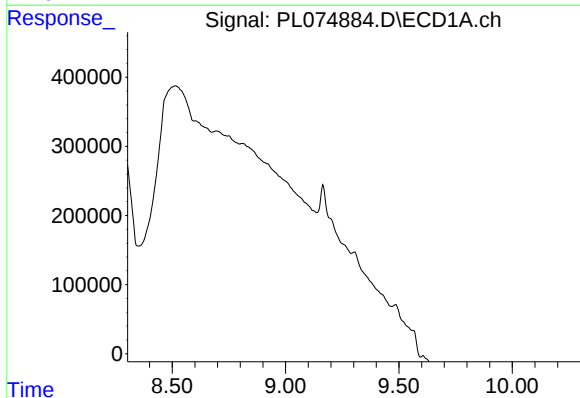


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 9.302 min
Response: 0
Conc: N.D.

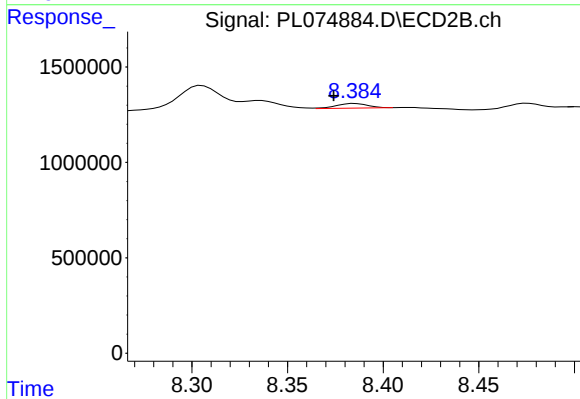

#15 Endosulfan II


R.T.: 8.385 min
Delta R.T.: 0.011 min
Response: 274235
Conc: 0.24 ng/ml

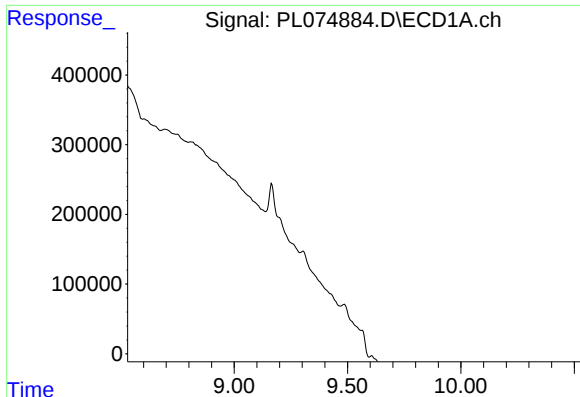

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.527 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

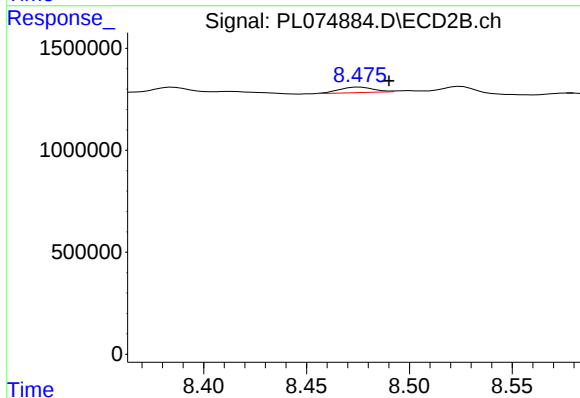


#17 4,4'-DDT

R.T.: 8.476 min
Delta R.T.: -0.014 min
Response: 309552
Conc: 0.31 ng/ml

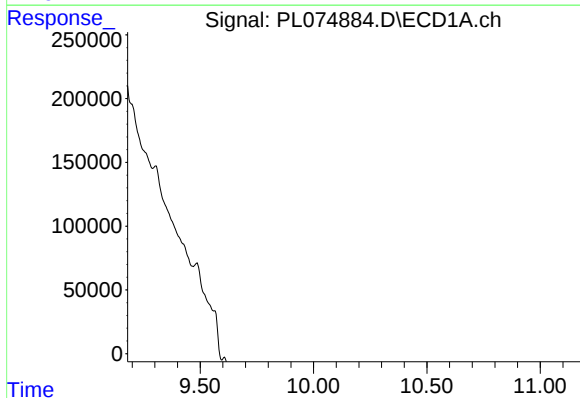


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 10.177 min
Response: 0
Conc: N.D.

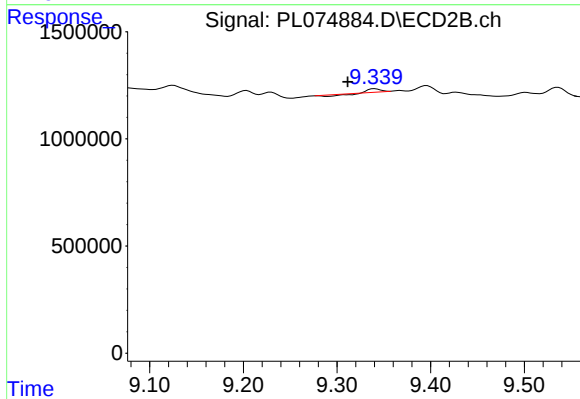

#21 Endrin ketone


R.T.: 9.340 min
Delta R.T.: 0.029 min
Response: 34460
Conc: 0.03 ng/ml

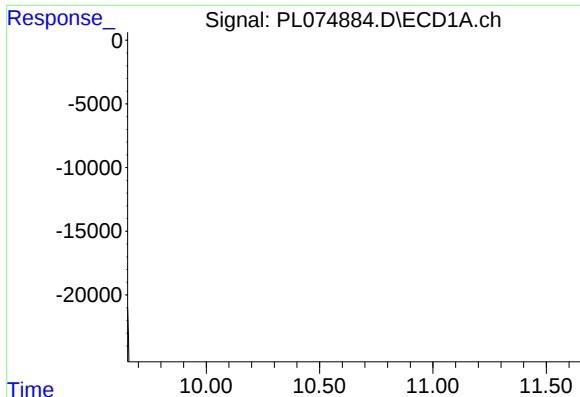

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 10.652 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

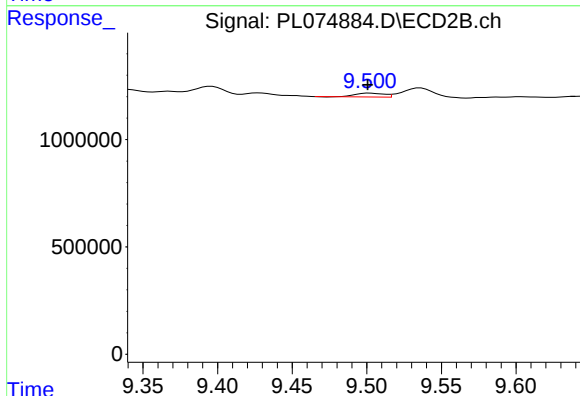


#22 Mirex

R.T.: 9.502 min
Delta R.T.: 0.001 min
Response: 244589
Conc: 0.25 ng/ml

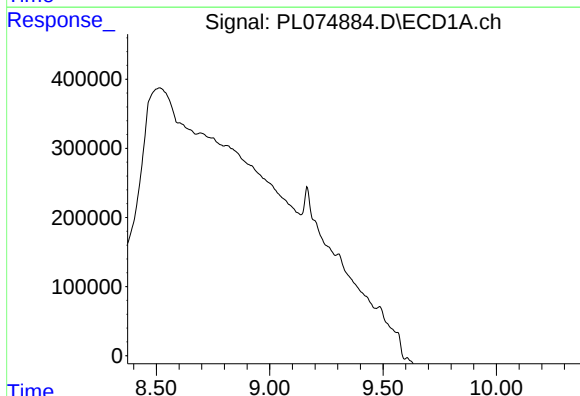


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 9.371 min
Response: 0
Conc: N.D.

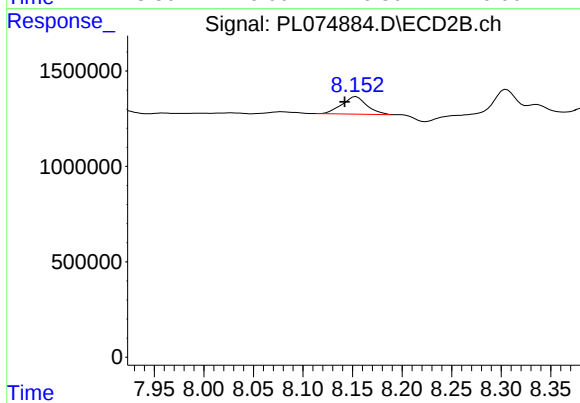

#27 Chlordane-5


R.T.: 8.154 min
Delta R.T.: 0.011 min
Response: 1608953
Conc: 43.52 ng/ml

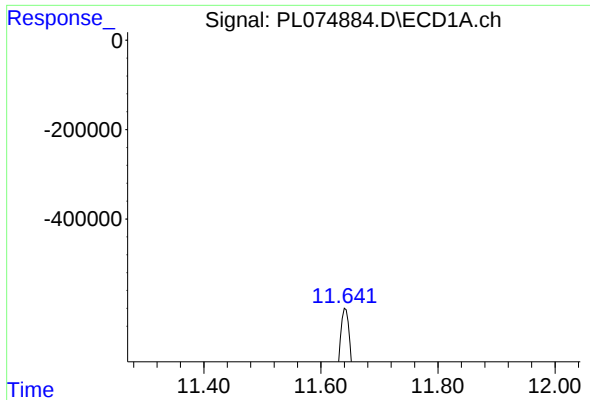

#28 Decachlorobiphenyl

R.T.: 11.642 min
Delta R.T.: -0.009 min
Response: 7729838
Conc: 17.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

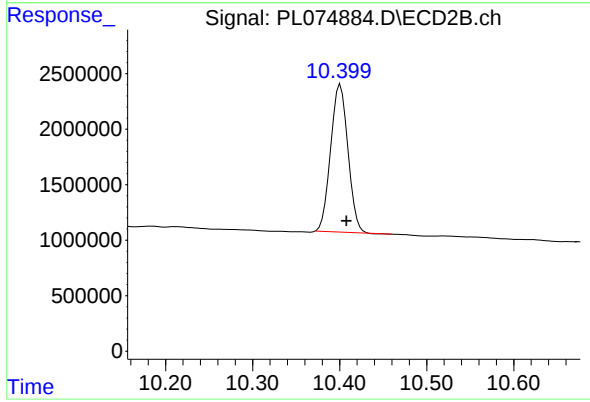

#28 Decachlorobiphenyl

R.T.: 10.401 min
Delta R.T.: -0.007 min
Response: 18366582
Conc: 17.89 ng/ml