

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052022\
 Data File : PL074892.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2022 19:03
 Operator : AR\AJ
 Sample : N2963-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 00:59:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.646	4.650	8093265	21133178	15.940	15.397
28)	SA Decachlor...	11.642	10.401	3161322	7700265	7.079	7.502
Target Compounds							
3)	MA gamma-BHC...	0.000	5.768	0	664627	N.D.	0.402 #
5)	MB Aldrin	0.000	6.505	0	400851	N.D.	0.267 #
9)	A Endosulfan I	8.517f	7.507f	4490214	1259548	7.789	1.007 #
11)	B alpha-Chl...	0.000	7.432	0	503556	N.D.	0.372 #
13)	MA Dieldrin	0.000	7.776	0	651719	N.D.	0.512 #
14)	MA Endrin	0.000	8.078	0	525330	N.D.	0.497 #
15)	B Endosulfa...	0.000	8.381	0	397730	N.D.	0.352 #
17)	MA 4,4'-DDT	9.523	8.483	2265112	2544566	4.928	2.543 #
20)	A Methoxychlor	0.000	9.101f	0	387772	N.D.	0.664 #
26)	Chlordane-4	0.000	7.432	0	503556	N.D.	3.673 #
27)	Chlordane-5	0.000	8.170f	0	2555193	N.D.	69.108 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052022\
Data File : PL074892.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2022 19:03
Operator : AR\AJ
Sample : N2963-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 00:59:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

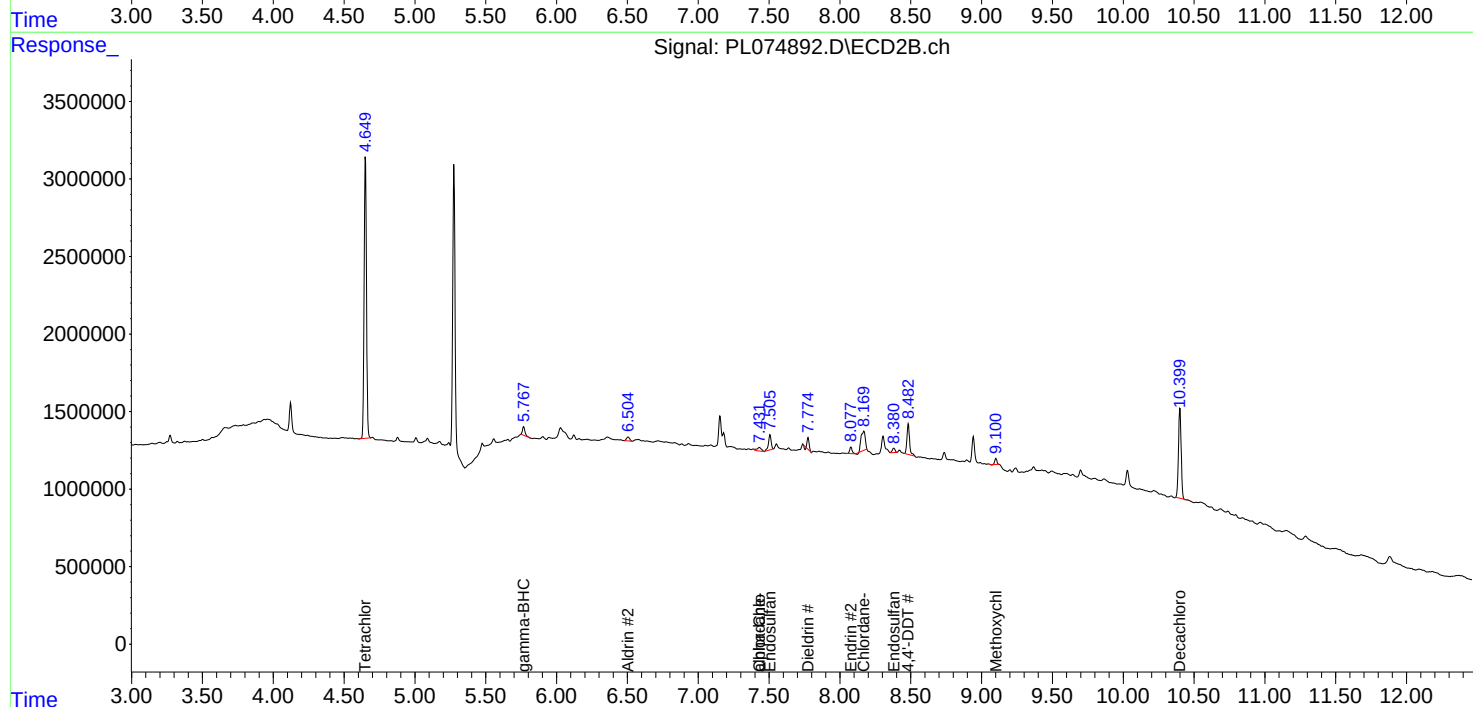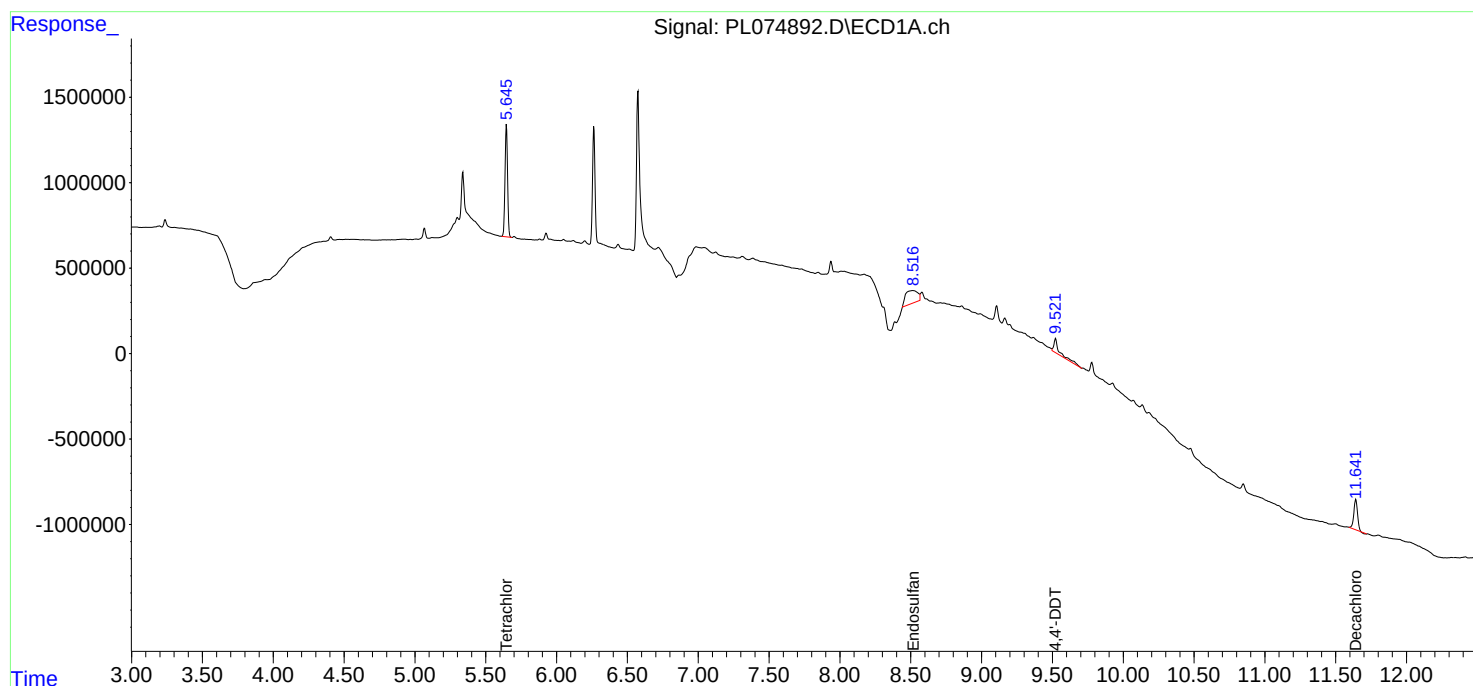


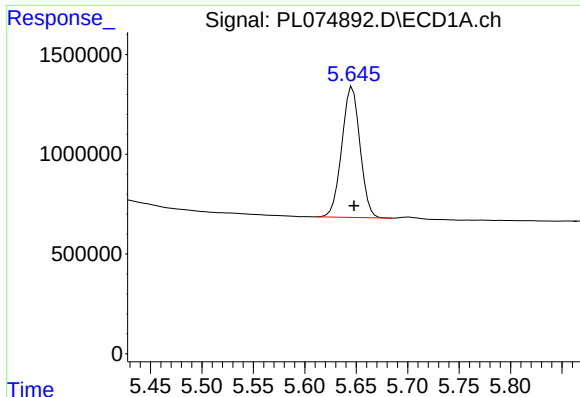

#1 Tetrachloro-m-xylene


R.T.: 5.646 min
Delta R.T.: -0.002 min
Response: 8093265
Conc: 15.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

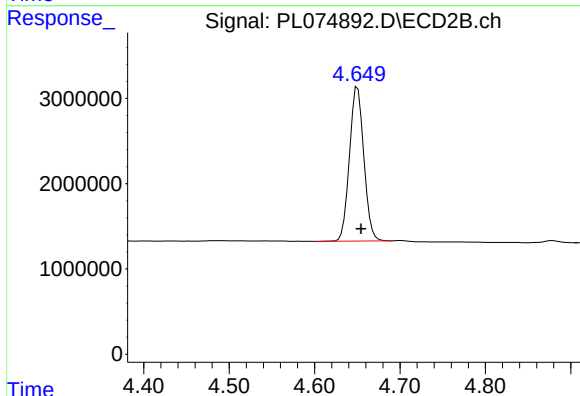


#1 Tetrachloro-m-xylene

R.T.: 4.650 min
Delta R.T.: -0.004 min
Response: 21133178
Conc: 15.40 ng/ml

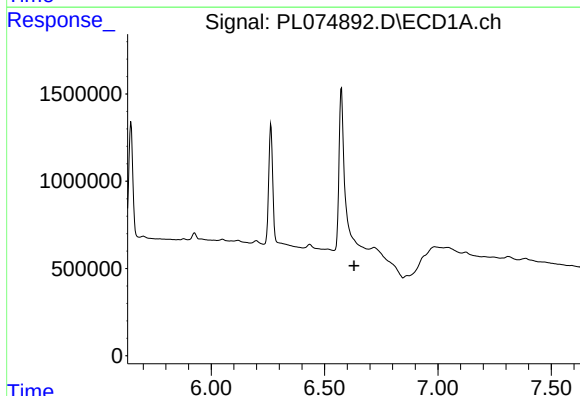


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 6.630 min
Response: 0
Conc: N.D.

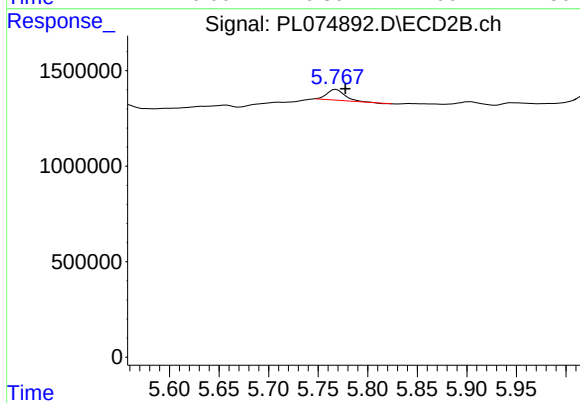

#3 gamma-BHC (Lindane)


R.T.: 5.768 min
Delta R.T.: -0.009 min
Response: 664627
Conc: 0.40 ng/ml

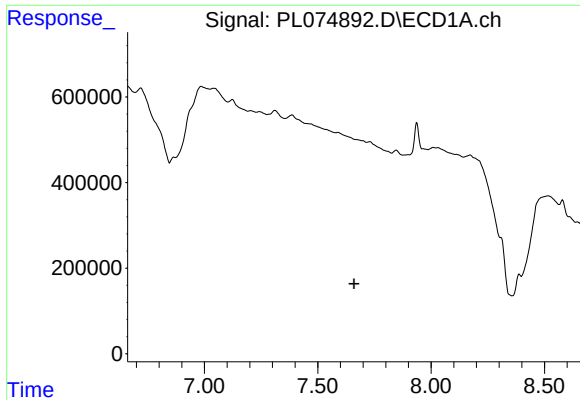

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 7.660 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

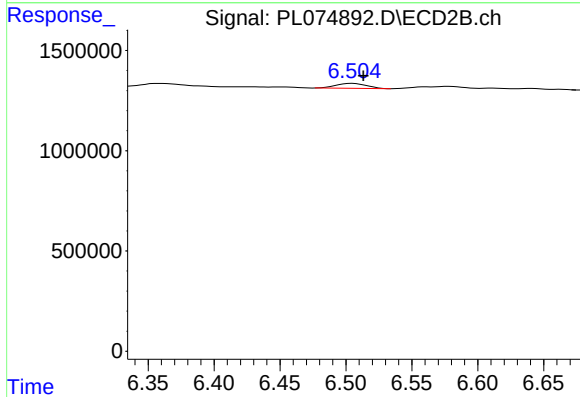


#5 Aldrin

R.T.: 6.505 min
Delta R.T.: -0.008 min
Response: 400851
Conc: 0.27 ng/ml

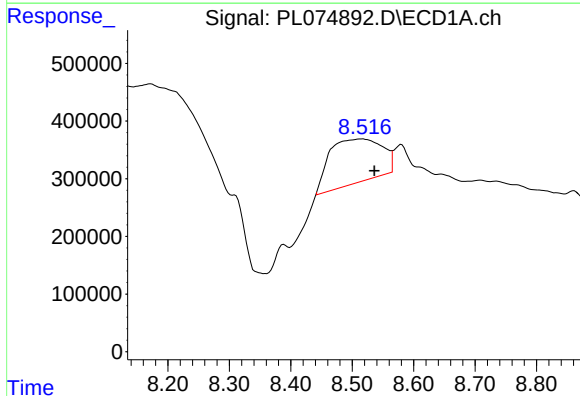


#9 Endosulfan I

R.T.: 8.517 min
Delta R.T.: -0.019 min
Response: 4490214
Conc: 7.79 ng/ml

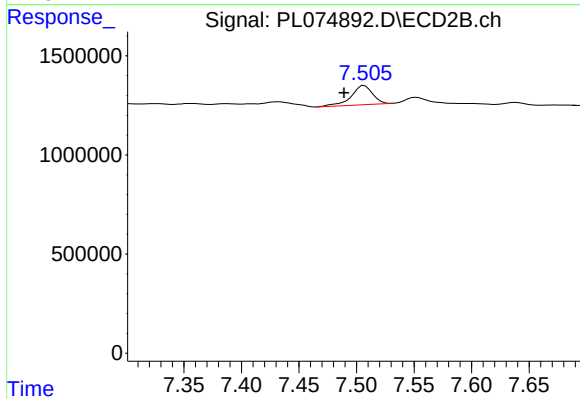

#9 Endosulfan I


R.T.: 7.507 min
Delta R.T.: 0.018 min
Response: 1259548
Conc: 1.01 ng/ml

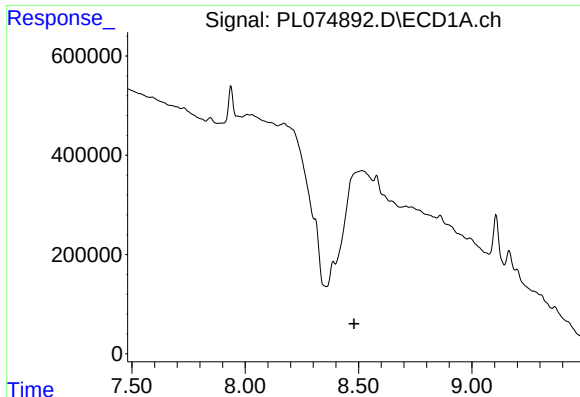

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.480 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

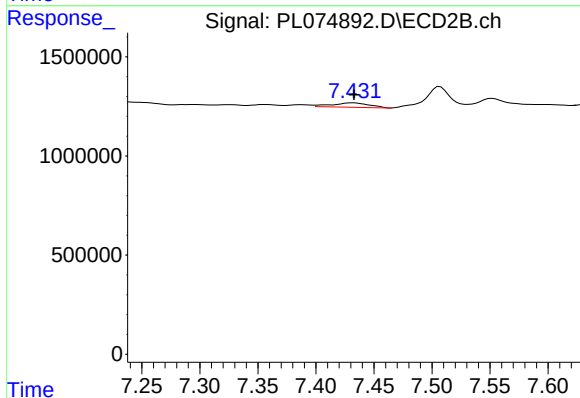


#11 alpha-Chlordane

R.T.: 7.432 min
Delta R.T.: 0.000 min
Response: 503556
Conc: 0.37 ng/ml

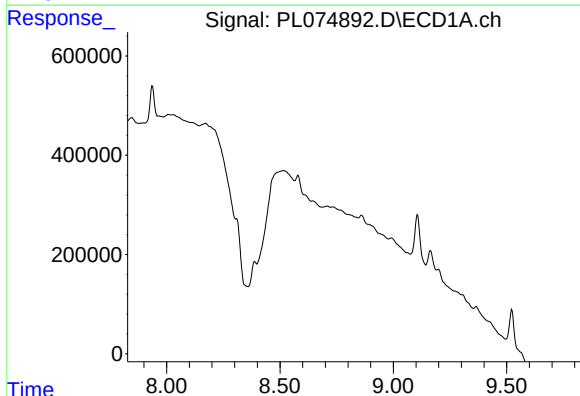


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 8.827 min
Response: 0
Conc: N.D.

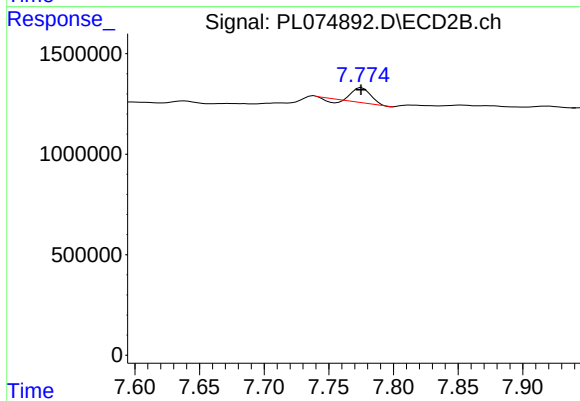

#13 Dieldrin


R.T.: 7.776 min
Delta R.T.: 0.000 min
Response: 651719
Conc: 0.51 ng/ml

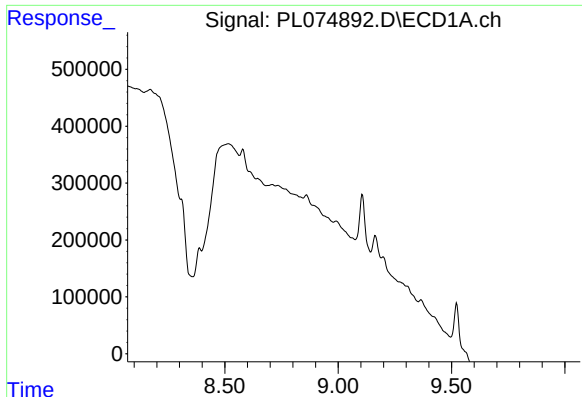

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

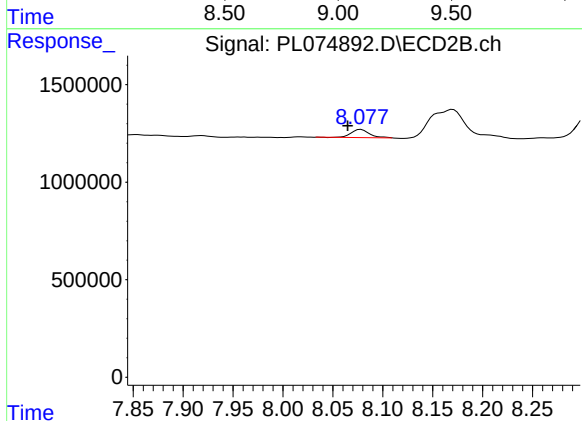


#14 Endrin

R.T.: 8.078 min
Delta R.T.: 0.013 min
Response: 525330
Conc: 0.50 ng/ml

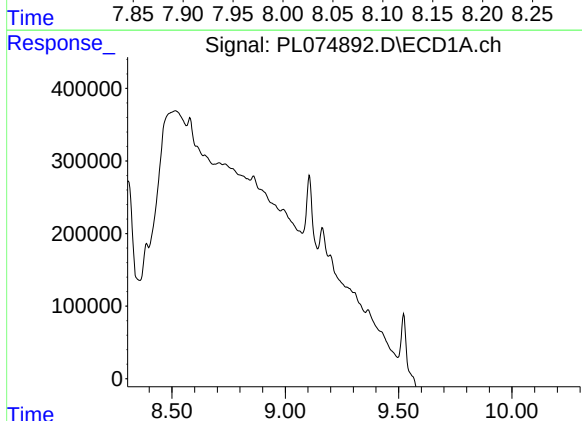


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 9.302 min
Response: 0
Conc: N.D.

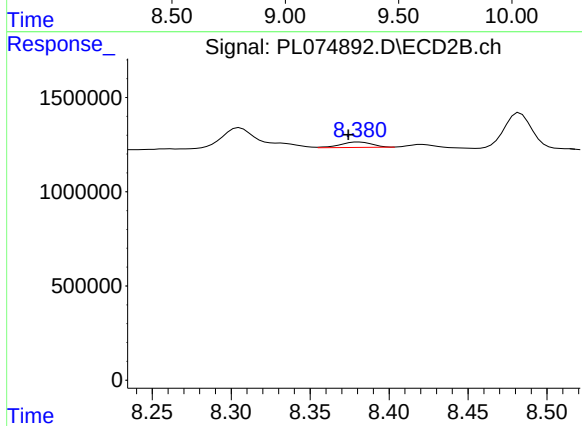

#15 Endosulfan II


R.T.: 8.381 min
Delta R.T.: 0.007 min
Response: 397730
Conc: 0.35 ng/ml

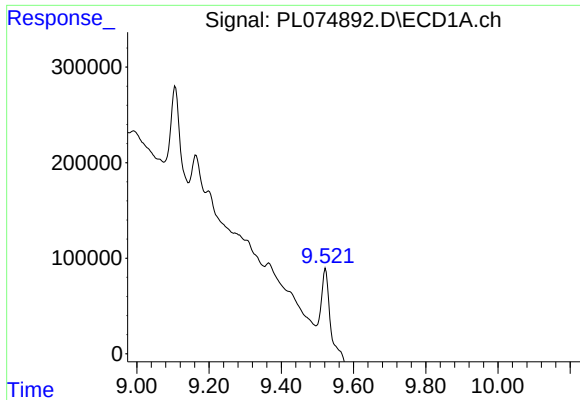

#17 4,4'-DDT


R.T.: 9.523 min
Delta R.T.: -0.005 min
Response: 2265112
Conc: 4.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

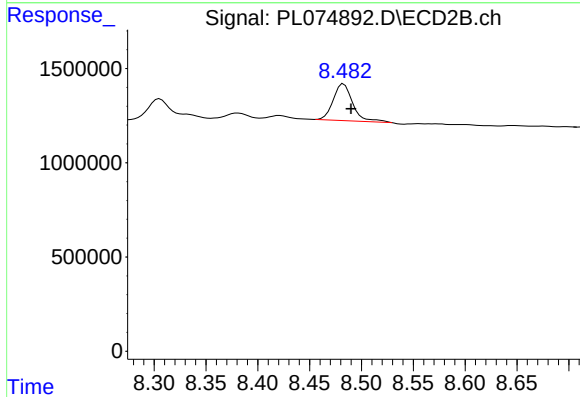


#17 4,4'-DDT

R.T.: 8.483 min
Delta R.T.: -0.007 min
Response: 2544566
Conc: 2.54 ng/ml

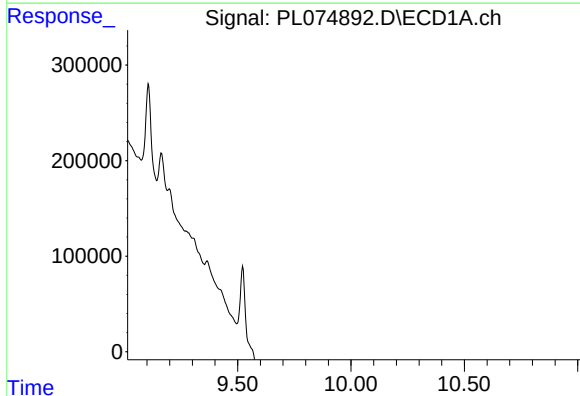


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 10.013 min
Response: 0
Conc: N.D.

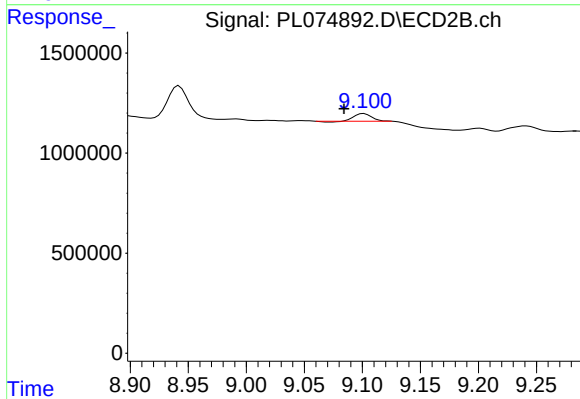

#20 Methoxychlor


R.T.: 9.101 min
Delta R.T.: 0.017 min
Response: 387772
Conc: 0.66 ng/ml

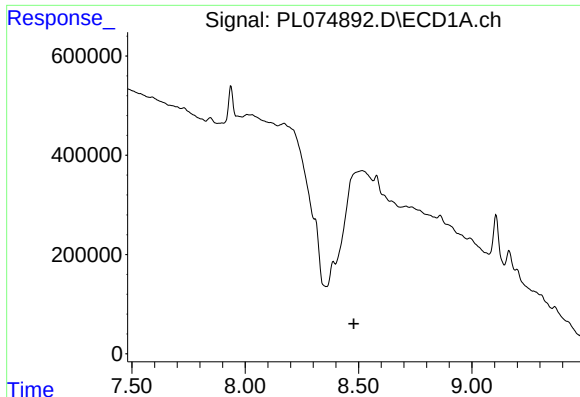

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 8.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

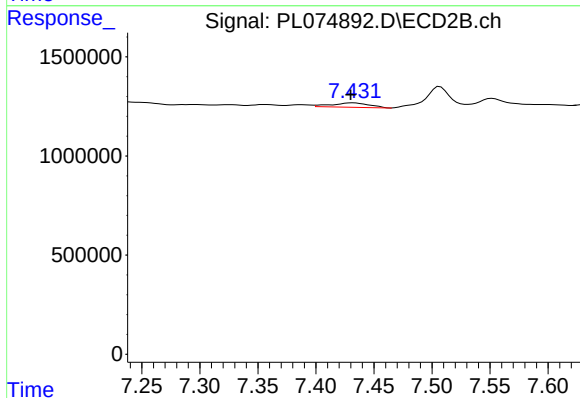


#26 Chlordane-4

R.T.: 7.432 min
Delta R.T.: 0.002 min
Response: 503556
Conc: 3.67 ng/ml

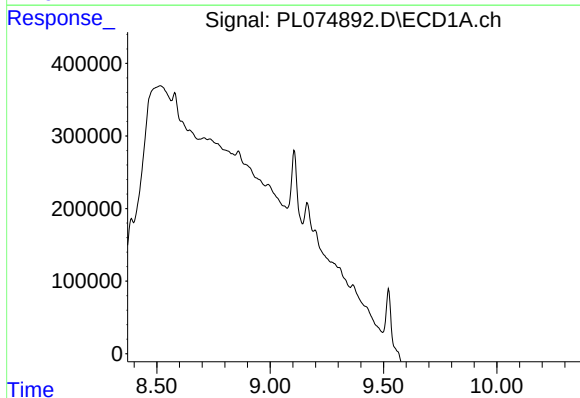


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.371 min
Response: 0
Conc: N.D.

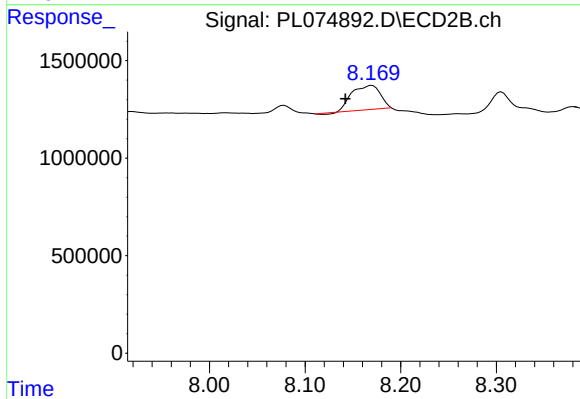

#27 Chlordane-5


R.T.: 8.170 min
Delta R.T.: 0.028 min
Response: 2555193
Conc: 69.11 ng/ml

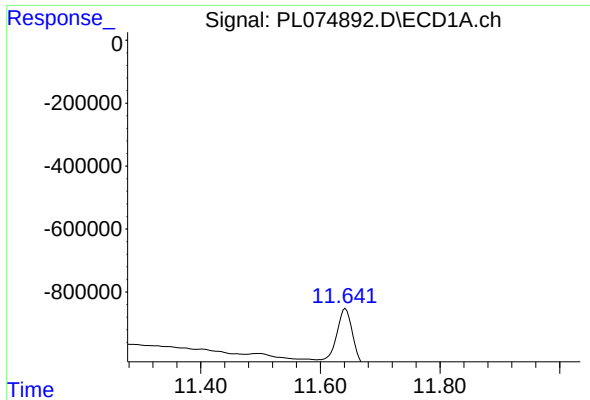

#28 Decachlorobiphenyl

R.T.: 11.642 min
Delta R.T.: -0.009 min
Response: 3161322
Conc: 7.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

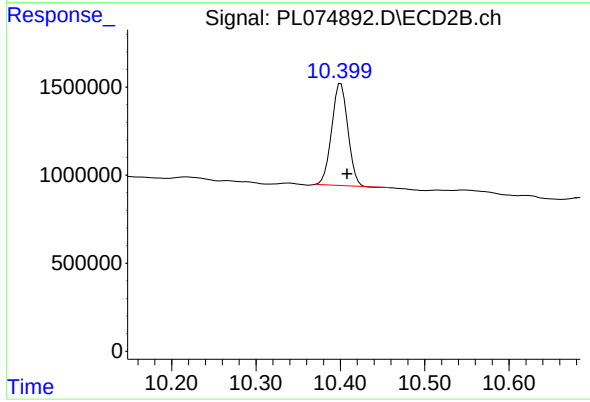

#28 Decachlorobiphenyl

R.T.: 10.401 min
Delta R.T.: -0.007 min
Response: 7700265
Conc: 7.50 ng/ml