

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052022\
 Data File : PL074895.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2022 19:53
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 01:00:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.645	4.650	10293952	27471519	20.274	20.015
28)	SA Decachlor...	11.641	10.400	10065662	23799135	22.539	23.187
Target Compounds							
6)	B beta-BHC	0.000	6.124f	0	175376	N.D.	0.221 #
8)	B Heptachlo...	8.127	0.000	2282994	0	4.014	N.D. #
9)	A Endosulfan I	8.511f	0.000	5273826	0	9.148	N.D. #
13)	MA Dieldrin	0.000	7.773	0	3163597	N.D.	2.483 #
14)	MA Endrin	0.000	8.081f	0	1344121	N.D.	1.272 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052022\
Data File : PL074895.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2022 19:53
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 01:00:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

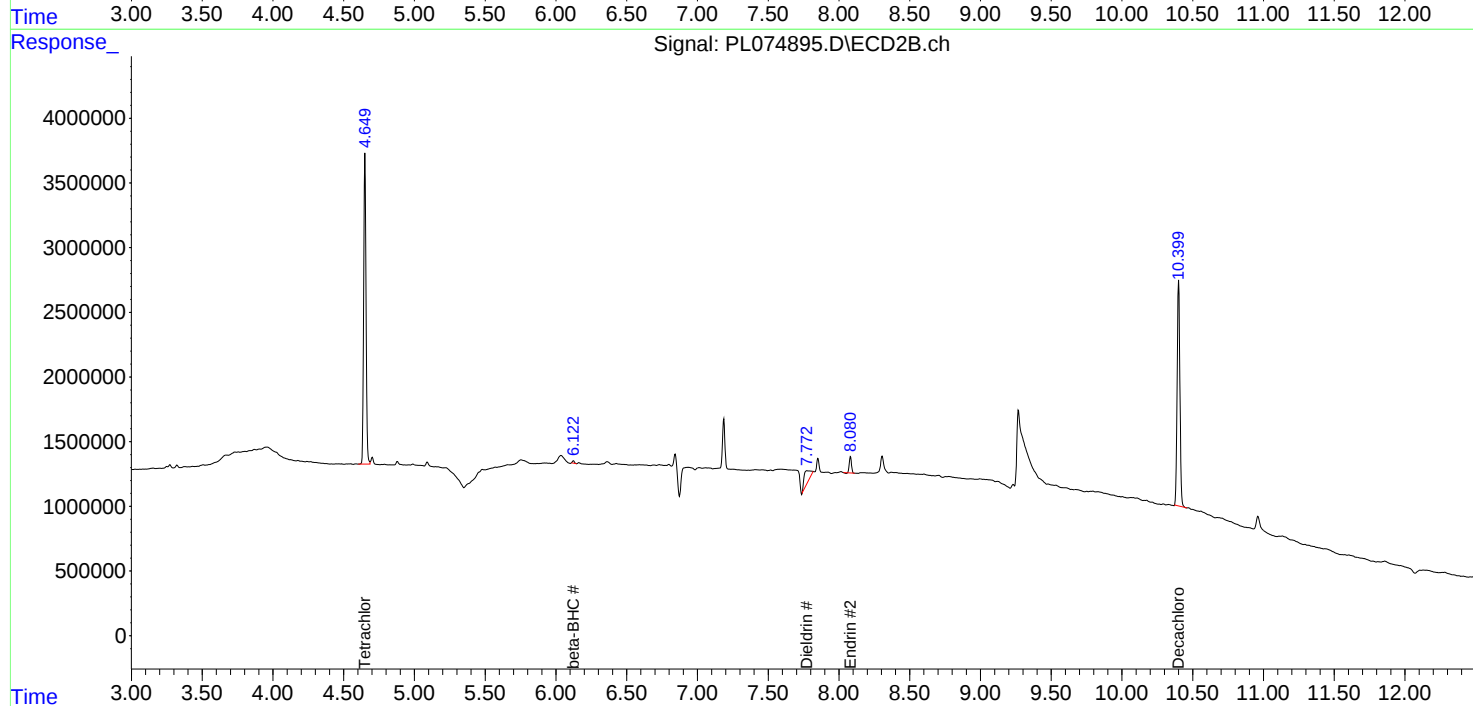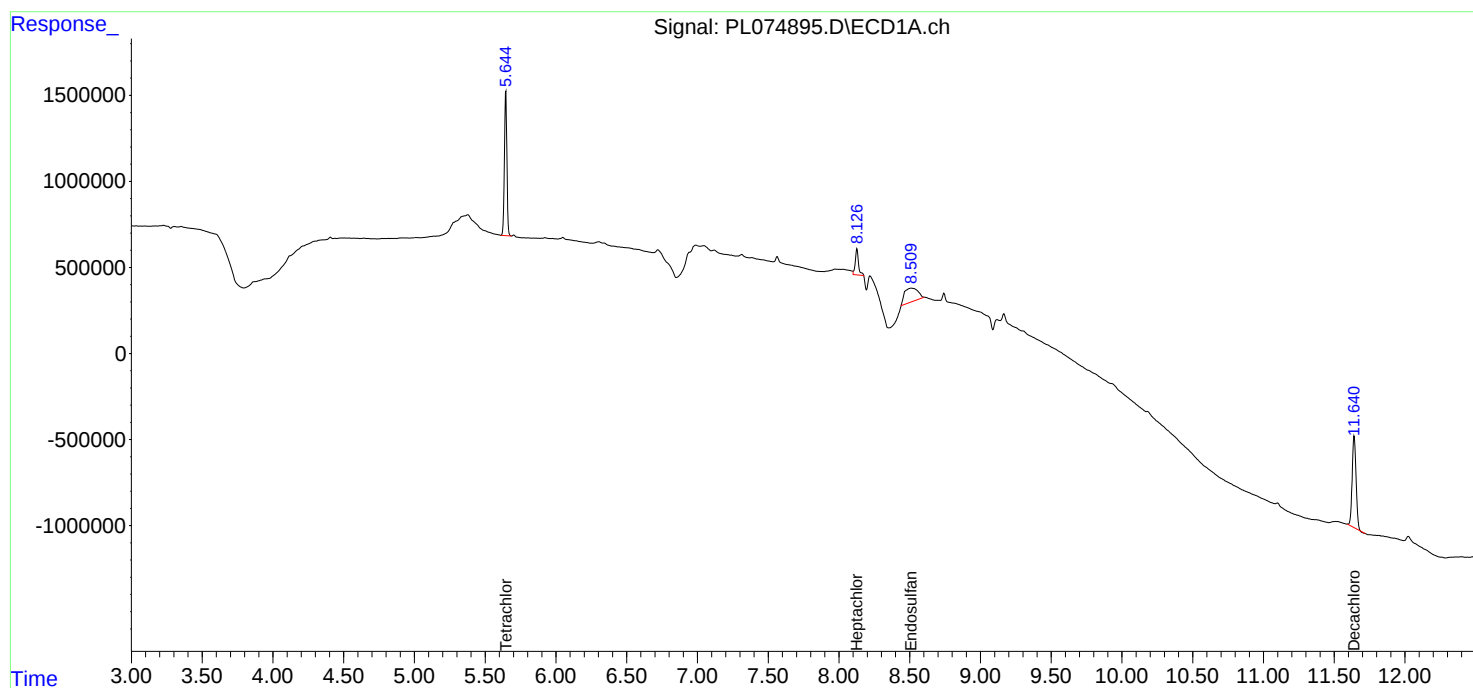


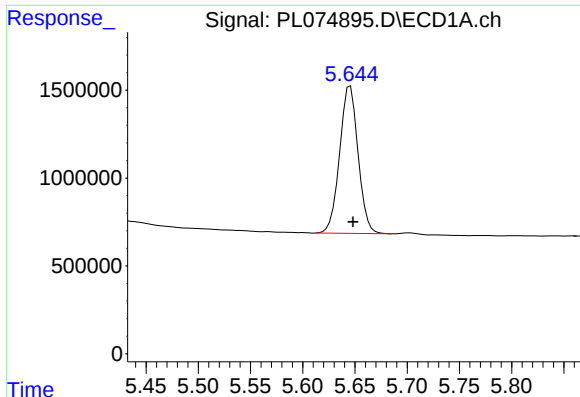

#1 Tetrachloro-m-xylene


R.T.: 5.645 min
Delta R.T.: -0.003 min
Response: 10293952
Conc: 20.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

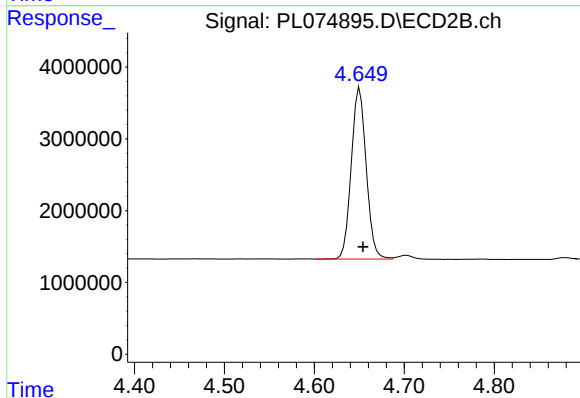


#1 Tetrachloro-m-xylene

R.T.: 4.650 min
Delta R.T.: -0.004 min
Response: 27471519
Conc: 20.02 ng/ml

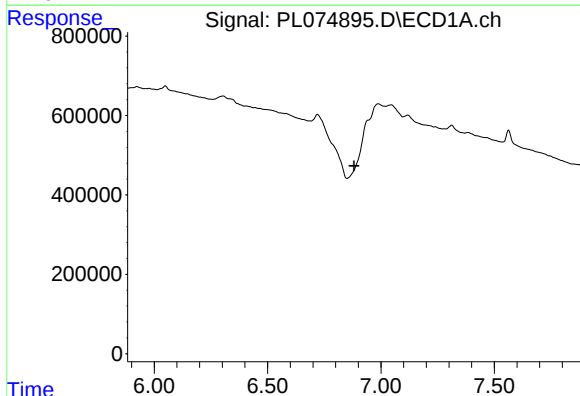


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.882 min
Response: 0
Conc: N.D.

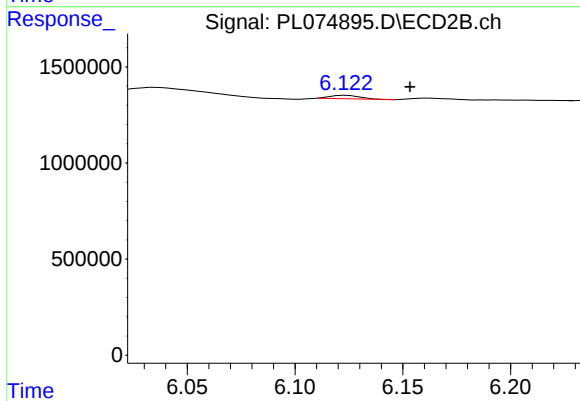

#6 beta-BHC


R.T.: 6.124 min
Delta R.T.: -0.030 min
Response: 175376
Conc: 0.22 ng/ml

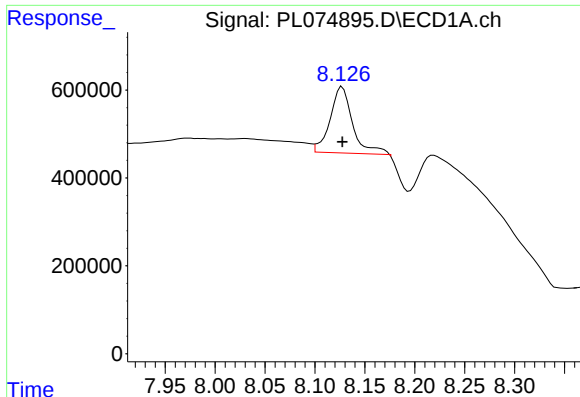

#8 Heptachlor epoxide


R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 2282994
Conc: 4.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

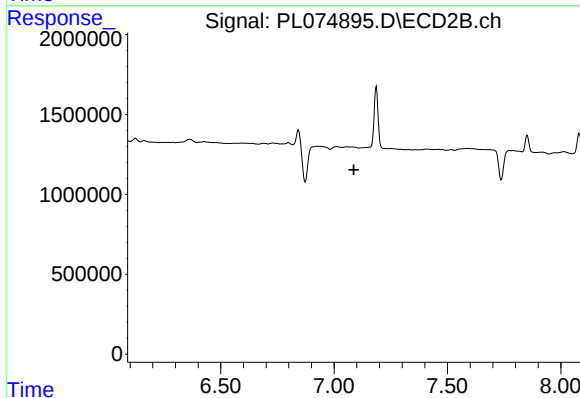


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.087 min
Response: 0
Conc: N.D.

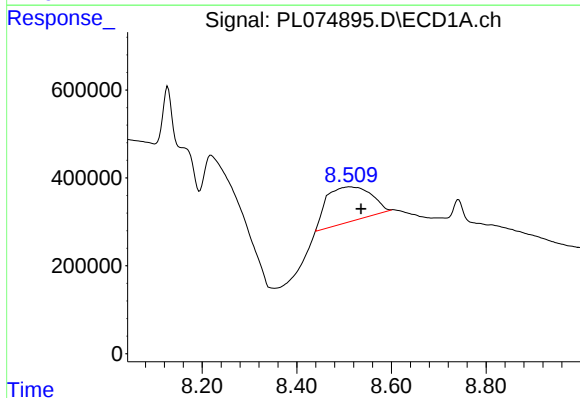


#9 Endosulfan I

R.T.: 8.511 min
Delta R.T.: -0.025 min
Response: 5273826
Conc: 9.15 ng/ml

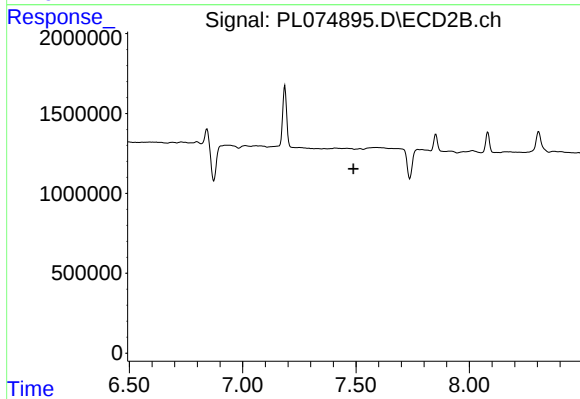

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 7.489 min
Response: 0
Conc: N.D.

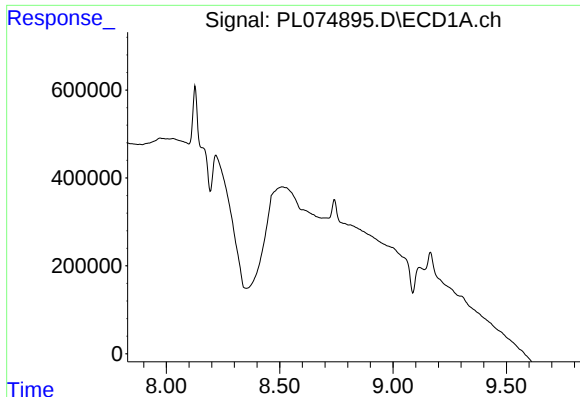

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 8.827 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

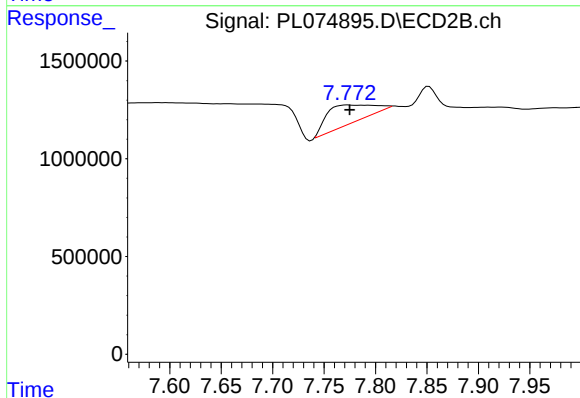


#13 Dieldrin

R.T.: 7.773 min
Delta R.T.: -0.002 min
Response: 3163597
Conc: 2.48 ng/ml

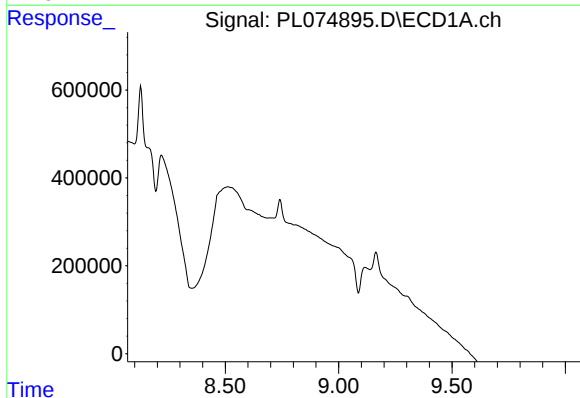


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.068 min
Response: 0
Conc: N.D.

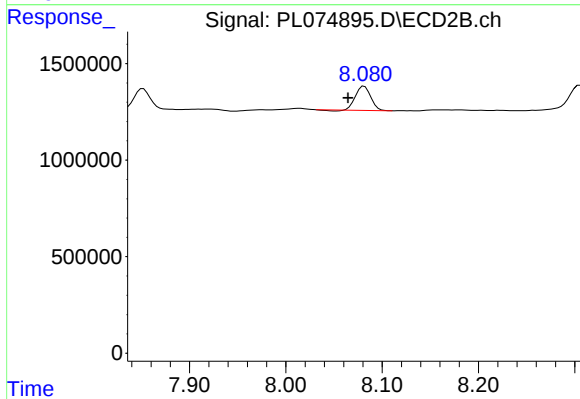

#14 Endrin


R.T.: 8.081 min
Delta R.T.: 0.017 min
Response: 1344121
Conc: 1.27 ng/ml

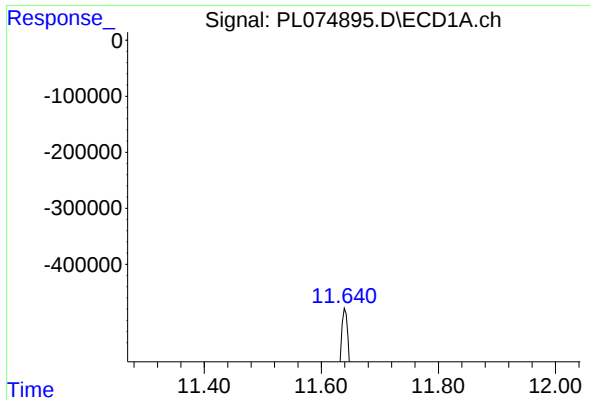

#28 Decachlorobiphenyl

R.T.: 11.641 min
Delta R.T.: -0.010 min
Response: 10065662
Conc: 22.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

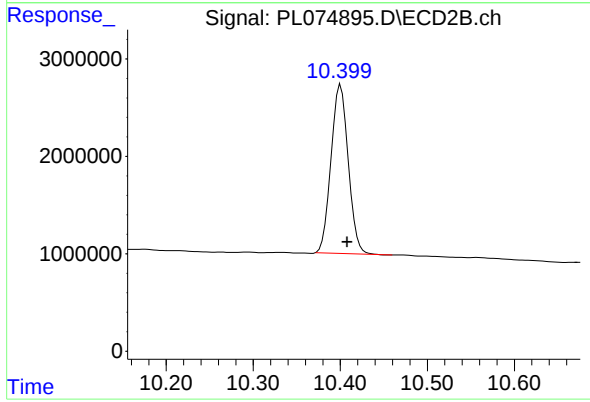

#28 Decachlorobiphenyl

R.T.: 10.400 min
Delta R.T.: -0.007 min
Response: 23799135
Conc: 23.19 ng/ml