

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052022\
 Data File : PL074899.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2022 23:45
 Operator : AR\AJ
 Sample : N2871-11 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 01:02:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.645	4.650	657257	1826281	1.294	1.331
28)	SA Decachlor...	11.640	10.399	846221	2466847	1.895	2.403 #
Target Compounds							
6)	B beta-BHC	0.000	6.124f	0	874435	N.D.	1.101 #
9)	A Endosulfan I	8.523	0.000	5134001	0	8.905	N.D. #
12)	B 4,4'-DDE	8.661	7.638	239429	791056	0.517	0.672 #
13)	MA Dieldrin	0.000	7.801f	0	222277	N.D.	0.174 #
14)	MA Endrin	0.000	8.075	0	293545	N.D.	0.278 #
16)	A 4,4'-DDD	9.203	0.000	541471	0	1.198	N.D. #
17)	MA 4,4'-DDT	0.000	8.476	0	1377195	N.D.	1.376 #
19)	B Endosulfa...	0.000	8.787	0	1253770	N.D.	1.152 #
21)	B Endrin ke...	0.000	9.339f	0	706728	N.D.	0.634 #
27)	Chlordane-5	0.000	8.139	0	1401238	N.D.	37.898 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052022\
Data File : PL074899.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2022 23:45
Operator : AR\AJ
Sample : N2871-11 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 01:02:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

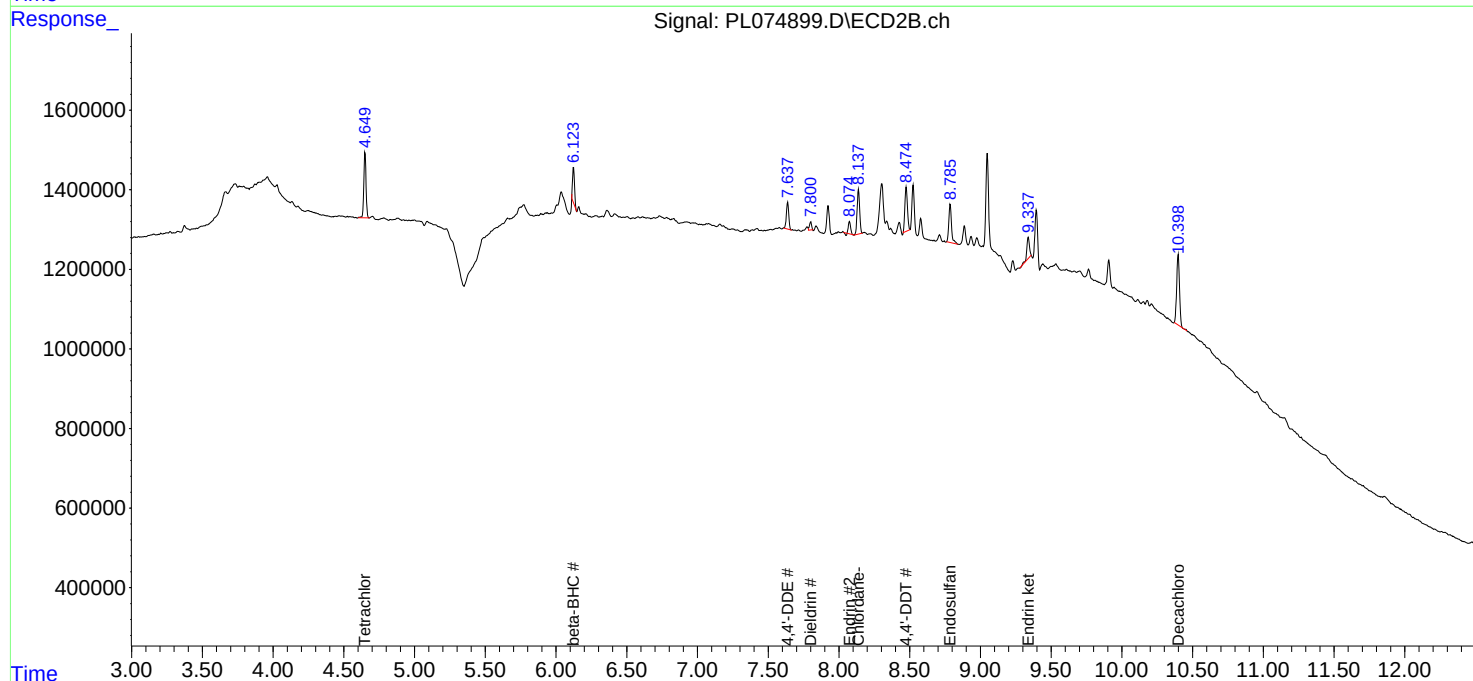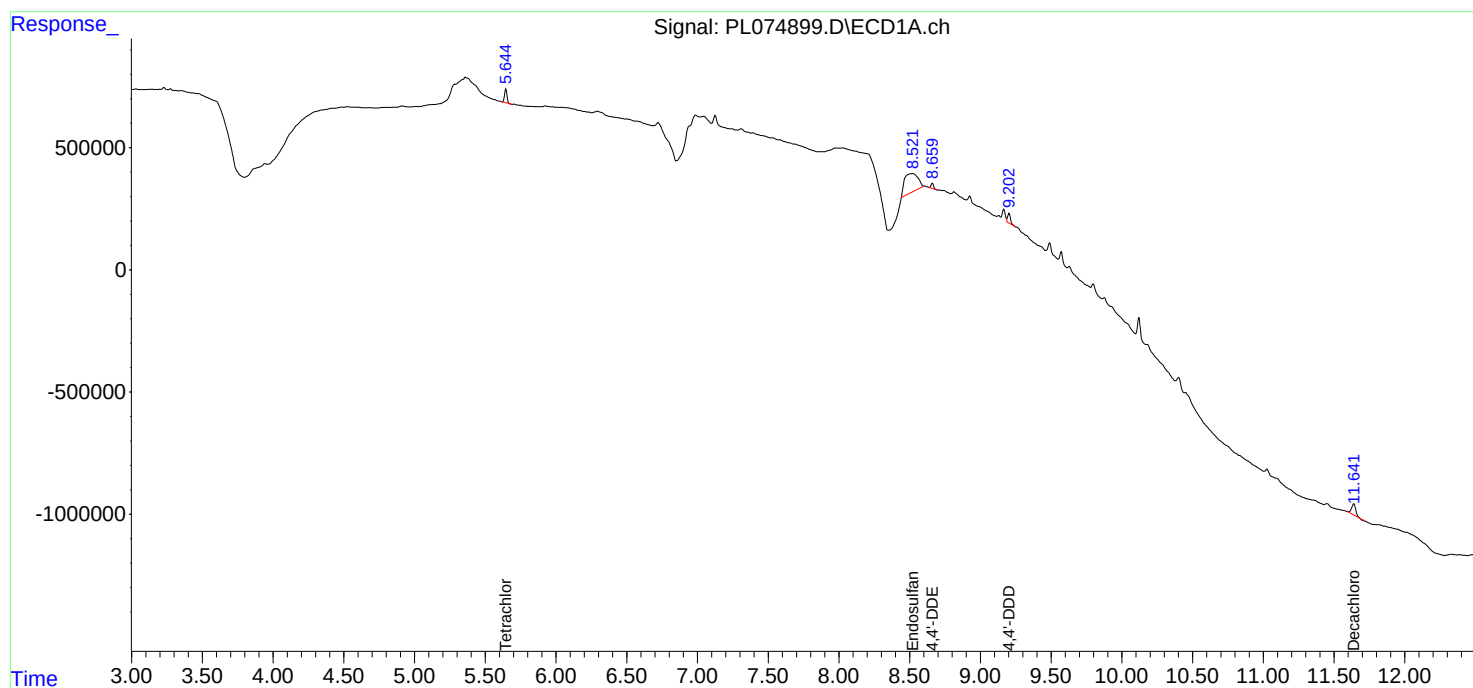


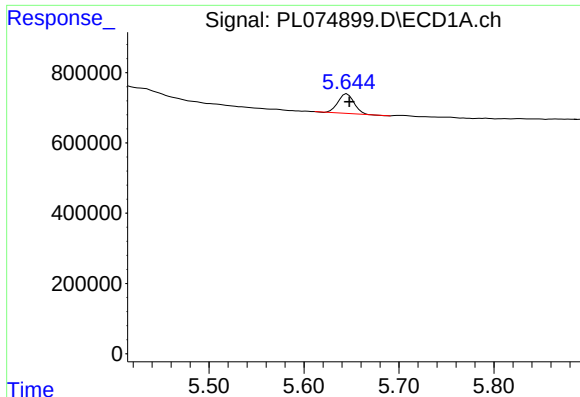

#1 Tetrachloro-m-xylene


R.T.: 5.645 min
Delta R.T.: -0.003 min
Response: 657257
Conc: 1.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

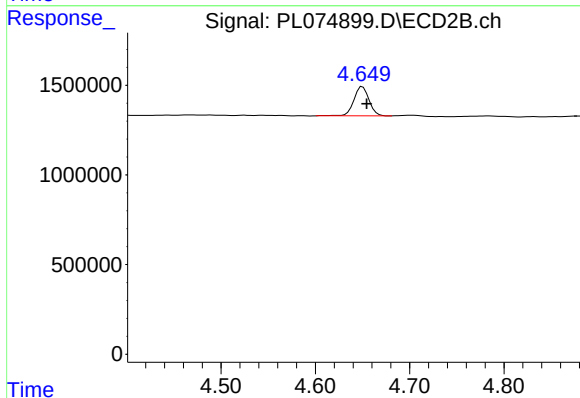


#1 Tetrachloro-m-xylene

R.T.: 4.650 min
Delta R.T.: -0.004 min
Response: 1826281
Conc: 1.33 ng/ml

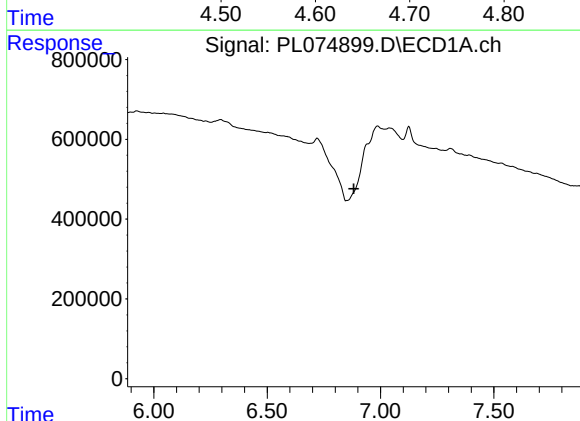


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.882 min
Response: 0
Conc: N.D.

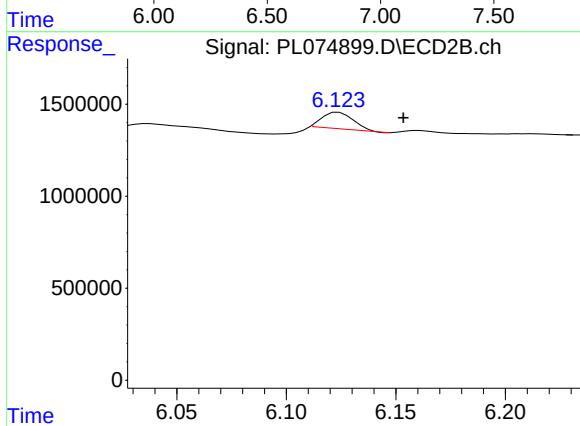

#6 beta-BHC


R.T.: 6.124 min
Delta R.T.: -0.029 min
Response: 874435
Conc: 1.10 ng/ml

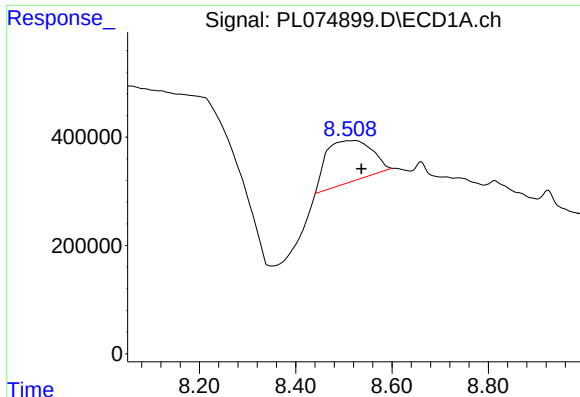

#9 Endosulfan I


R.T.: 8.523 min
Delta R.T.: -0.013 min
Response: 5134001
Conc: 8.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

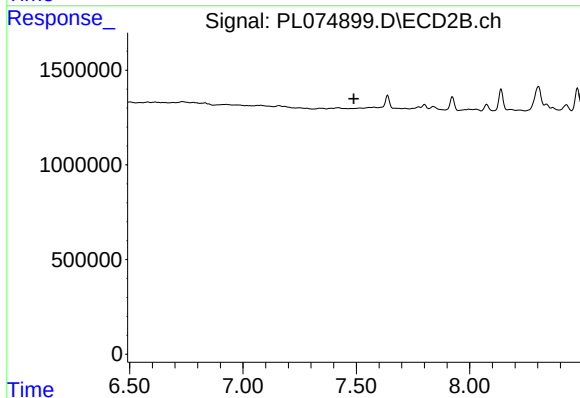


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.489 min
Response: 0
Conc: N.D.

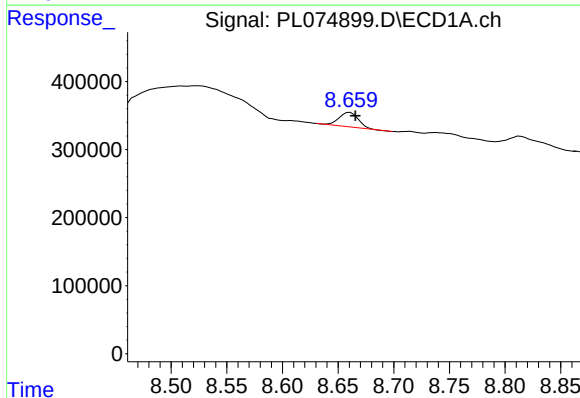


#12 4,4'-DDE

R.T.: 8.661 min
Delta R.T.: -0.005 min
Response: 239429
Conc: 0.52 ng/ml

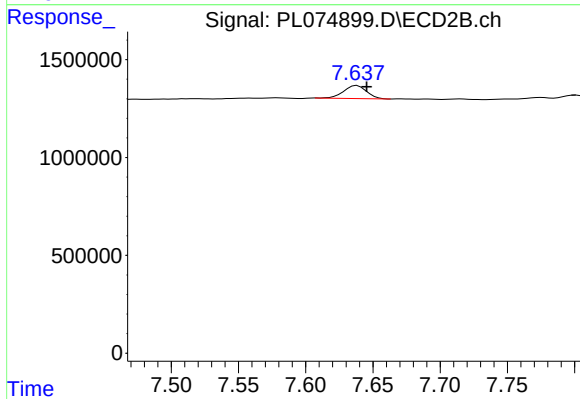

#12 4,4'-DDE


R.T.: 7.638 min
Delta R.T.: -0.007 min
Response: 791056
Conc: 0.67 ng/ml

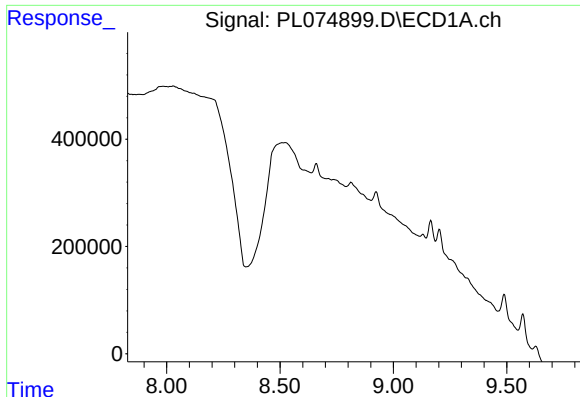

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 8.827 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

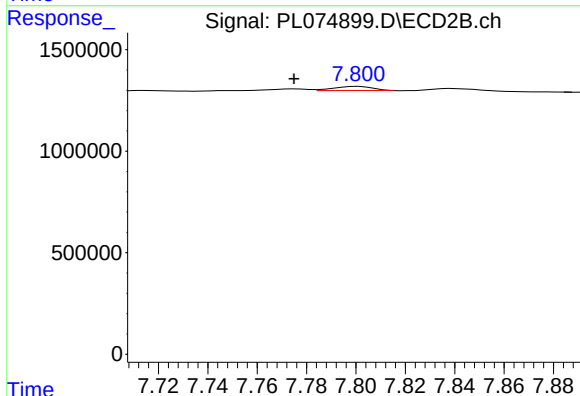


#13 Dieldrin

R.T.: 7.801 min
Delta R.T.: 0.026 min
Response: 222277
Conc: 0.17 ng/ml

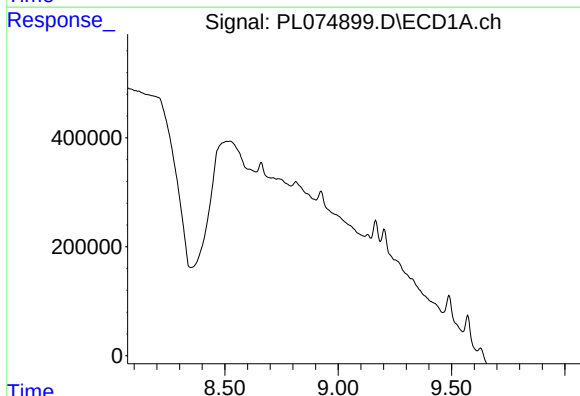


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.068 min
Response: 0
Conc: N.D.

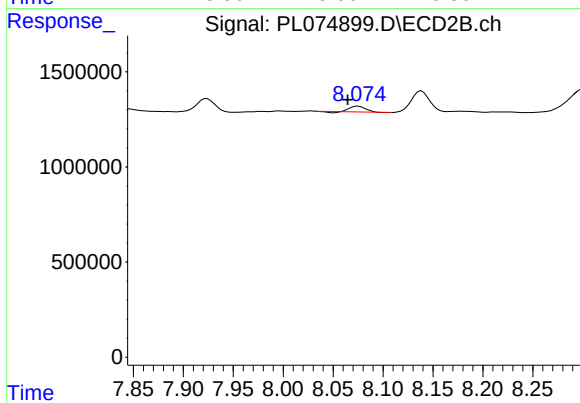

#14 Endrin


R.T.: 8.075 min
Delta R.T.: 0.010 min
Response: 293545
Conc: 0.28 ng/ml

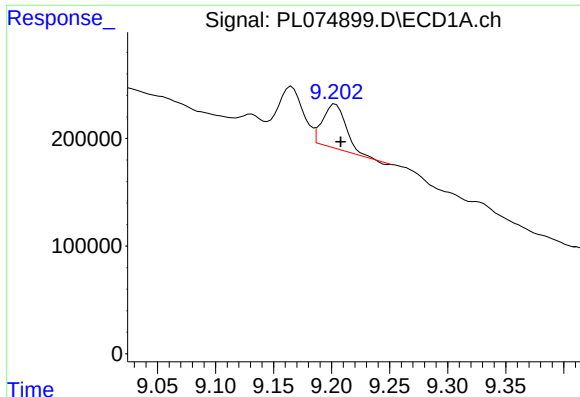

#16 4,4'-DDD


R.T.: 9.203 min
Delta R.T.: -0.005 min
Response: 541471
Conc: 1.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

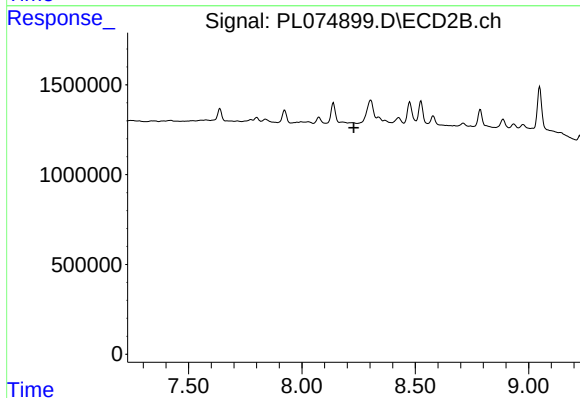


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.229 min
Response: 0
Conc: N.D.

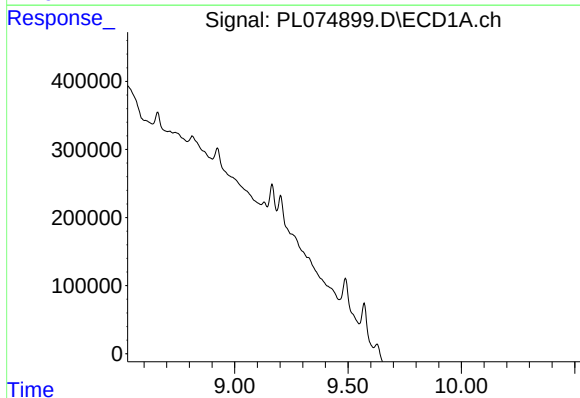


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.527 min
Response: 0
Conc: N.D.

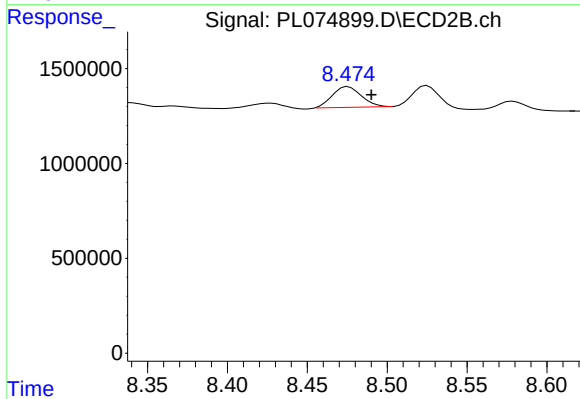

#17 4,4'-DDT


R.T.: 8.476 min
Delta R.T.: -0.014 min
Response: 1377195
Conc: 1.38 ng/ml

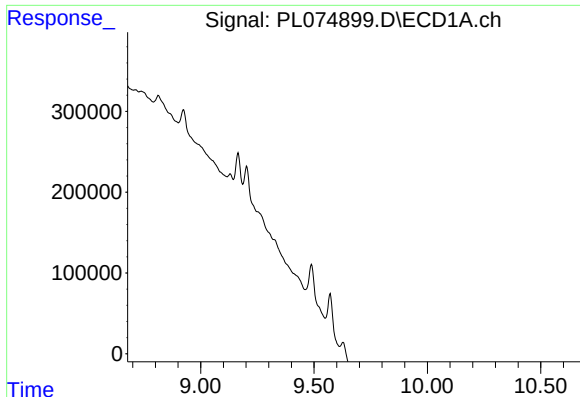

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 9.675 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

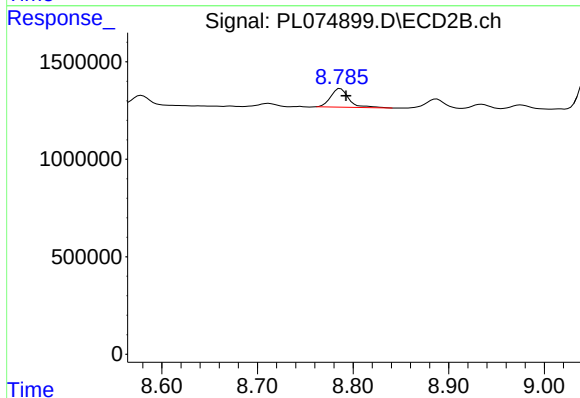


#19 Endosulfan Sulfate

R.T.: 8.787 min
Delta R.T.: -0.006 min
Response: 1253770
Conc: 1.15 ng/ml

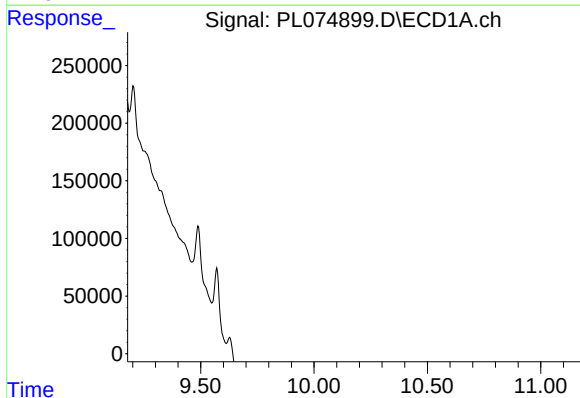


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 10.177 min
Response: 0
Conc: N.D.

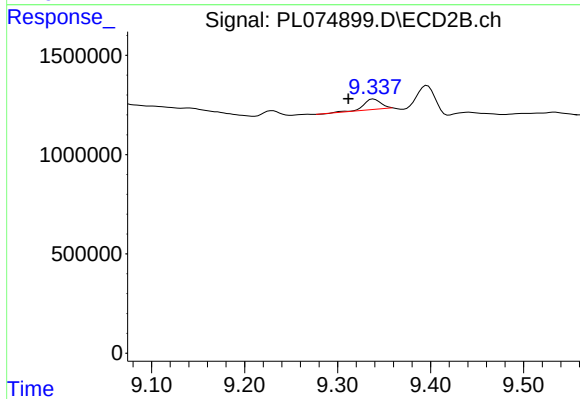

#21 Endrin ketone


R.T.: 9.339 min
Delta R.T.: 0.027 min
Response: 706728
Conc: 0.63 ng/ml

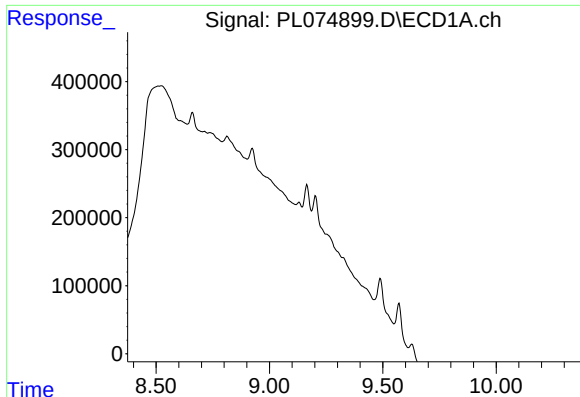

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.371 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

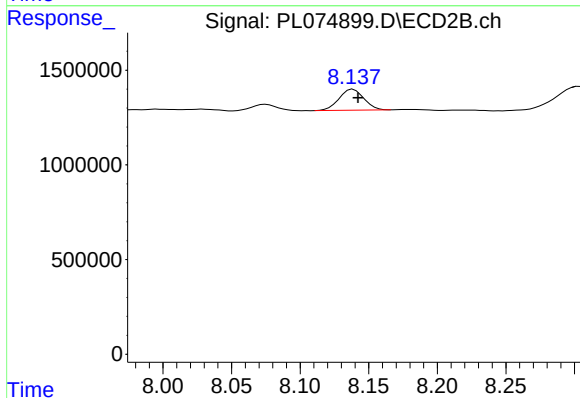


#27 Chlordane-5

R.T.: 8.139 min
Delta R.T.: -0.004 min
Response: 1401238
Conc: 37.90 ng/ml

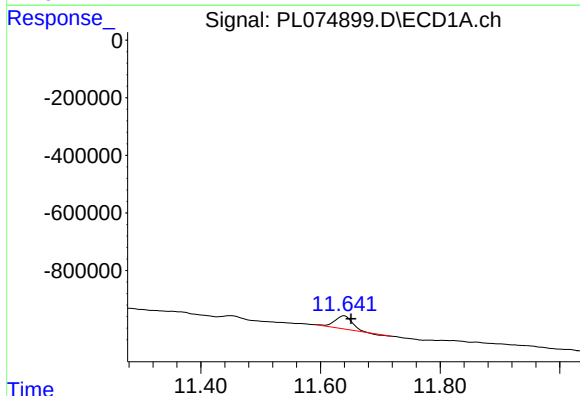

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: -0.011 min
Response: 846221
Conc: 1.89 ng/ml

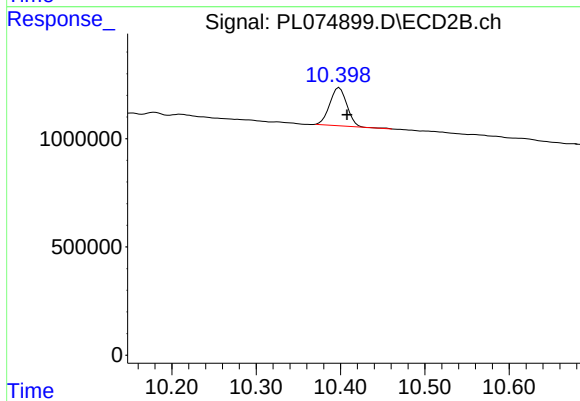

#28 Decachlorobiphenyl

R.T.: 10.399 min
Delta R.T.: -0.009 min
Response: 2466847
Conc: 2.40 ng/ml