

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052022\
 Data File : PL074882.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2022 15:53
 Operator : AR\AJ
 Sample : N2871-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 P017-SS001-0612-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 00:57:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.645	4.650	11719990	29507793	23.083	21.499
28) SA Decachlor...	11.643	10.400	8889705	21557910	19.906	21.003

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052022\
Data File : PL074882.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2022 15:53
Operator : AR\AJ
Sample : N2871-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
P017-SS001-0612-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 00:57:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

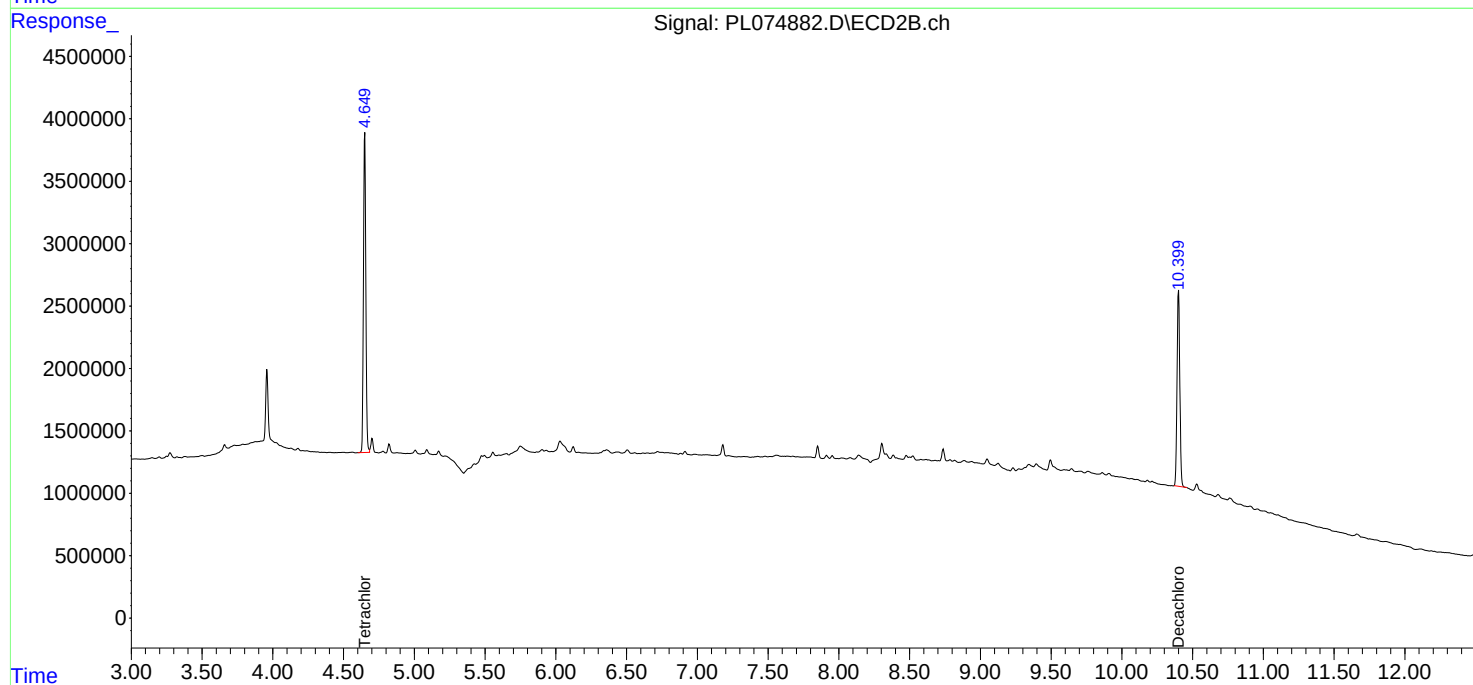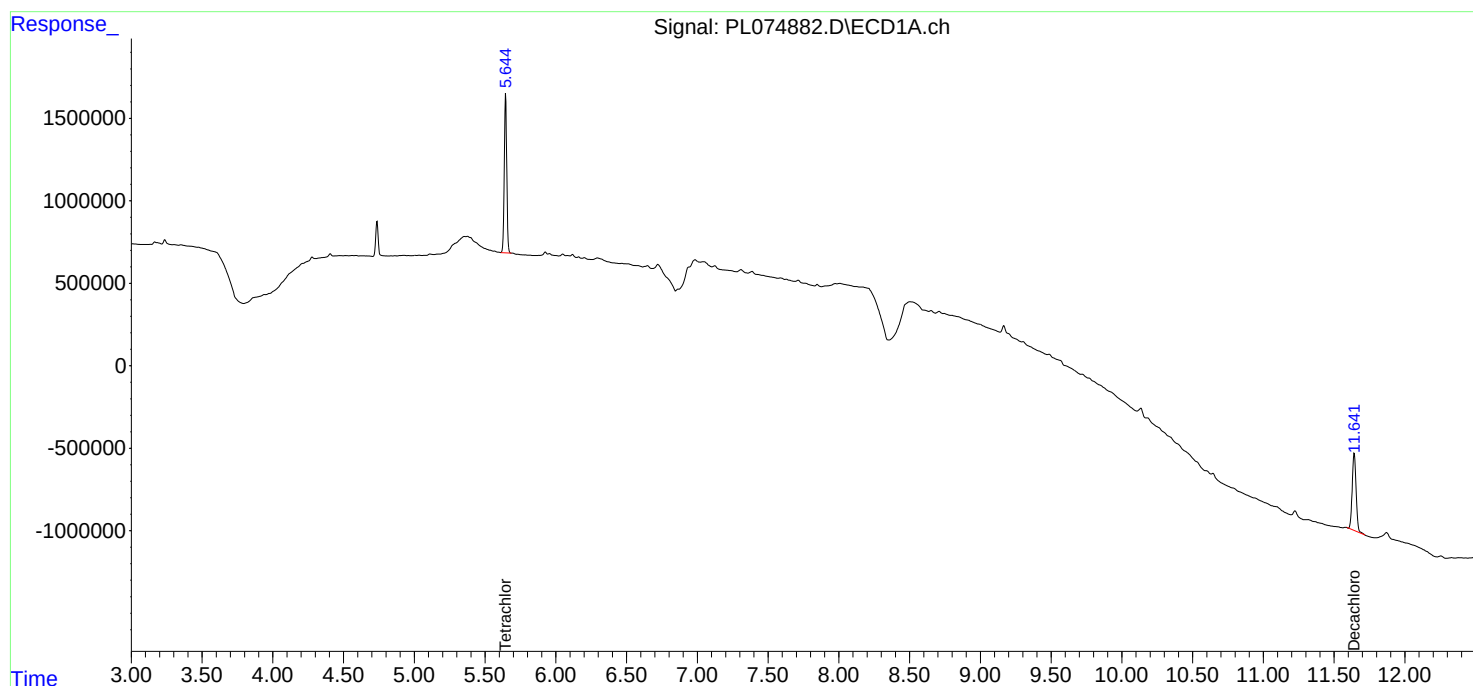


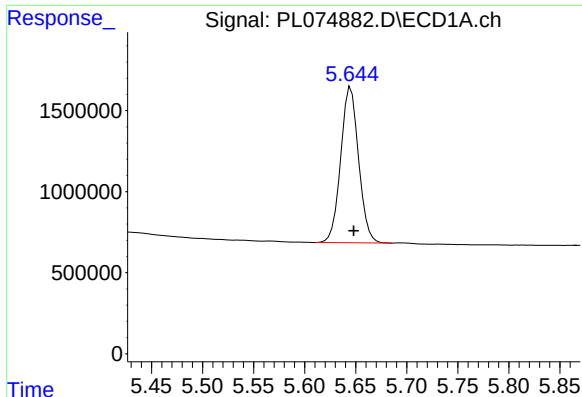

#1 Tetrachloro-m-xylene


R.T.: 5.645 min
Delta R.T.: -0.003 min
Response: 11719990
Conc: 23.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
P017-SS001-0612-01

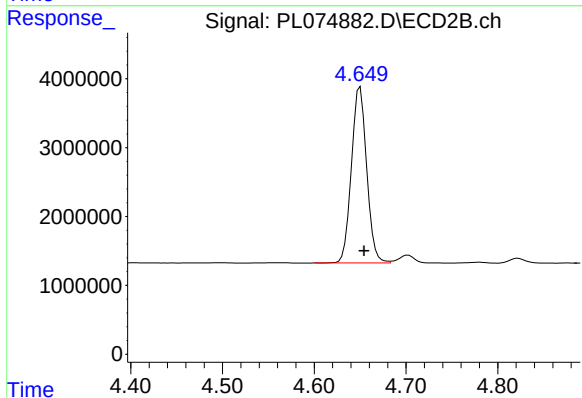


#1 Tetrachloro-m-xylene

R.T.: 4.650 min
Delta R.T.: -0.004 min
Response: 29507793
Conc: 21.50 ng/ml

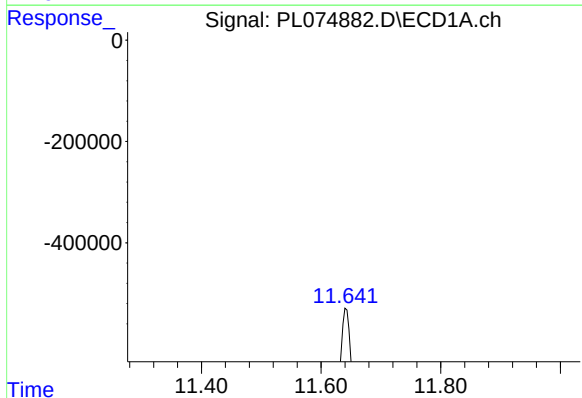

#28 Decachlorobiphenyl

R.T.: 11.643 min
Delta R.T.: -0.008 min
Response: 8889705
Conc: 19.91 ng/ml

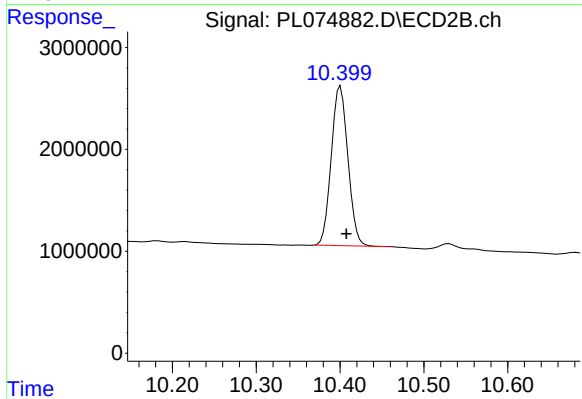

#28 Decachlorobiphenyl

R.T.: 10.400 min
Delta R.T.: -0.007 min
Response: 21557910
Conc: 21.00 ng/ml