

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052024\
 Data File : PL089610.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2024 15:26
 Operator : AR\AJ
 Sample : P2409-02
 Misc : PEST MDL WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-QT2-2024-04

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/21/2024
 Supervised By :Ankita Jodhani 05/21/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 22:15:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 15:59:18 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.795	39828875	24898907	20.480	19.403
27)	SA Decachlor...	9.065	7.945	28803443	26481708	23.454	22.073
Target Compounds							
2)	A alpha-BHC	4.005	3.300	3175812	1422109	1.138	0.790 #
3)	MA gamma-BHC...	4.337	3.630	2884300	1426157	1.097	0.836
4)	MA Heptachlor	4.927	3.972	3051534	1384912	1.284	0.821 #
5)	MB Aldrin	5.269	4.253	3061159	1351758	1.275	0.843 #
6)	B beta-BHC	4.533	3.927	1534353	738368	1.194	0.856m#
7)	B delta-BHC	4.778	4.159	3342979	1289935	1.290m	0.743 #
8)	B Heptachlo...	5.693	4.756	3109296	1353766	1.345m	0.847 #
9)	A Endosulfan I	6.079	5.127	2721066	1274413	1.356m	0.917 #
10)	B trans-Chl...	5.950	5.007	2993176	1426758	1.378	0.924 #
11)	B cis-Chlor...	6.030	5.071	2759593	1440747	1.262	0.906 #
12)	B 4,4'-DDE	6.202	5.260	2539200	1086806	1.387	0.774 #
13)	MA Dieldrin	6.355	5.392	2833453	1301952	1.398	0.851 #
14)	MA Endrin	6.585	5.667	2222170	1152129	1.305	0.837 #
15)	B Endosulfa...	6.801	5.960	2476140	1330475	1.370m	0.977 #
16)	A 4,4'-DDD	6.716	5.815	2029026	981245	1.377m	0.859 #
17)	MA 4,4'-DDT	7.032	6.065	2358685	930979	1.680	0.776 #
18)	B Endrin al...	6.933	6.140	1887595	989452	1.386	0.934 #
19)	B Endosulfa...	7.167	6.363	2236487	1313401	1.387	0.994 #
20)	A Methoxychlor	7.506	6.642	959194	663357	1.401	0.979 #
21)	B Endrin ke...	7.652	6.869	2348991	1329012	1.350	0.904 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052024\
Data File : PL089610.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2024 15:26
Operator : AR\AJ
Sample : P2409-02
Misc : PEST MDL WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 22:15:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051724CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 15:59:18 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

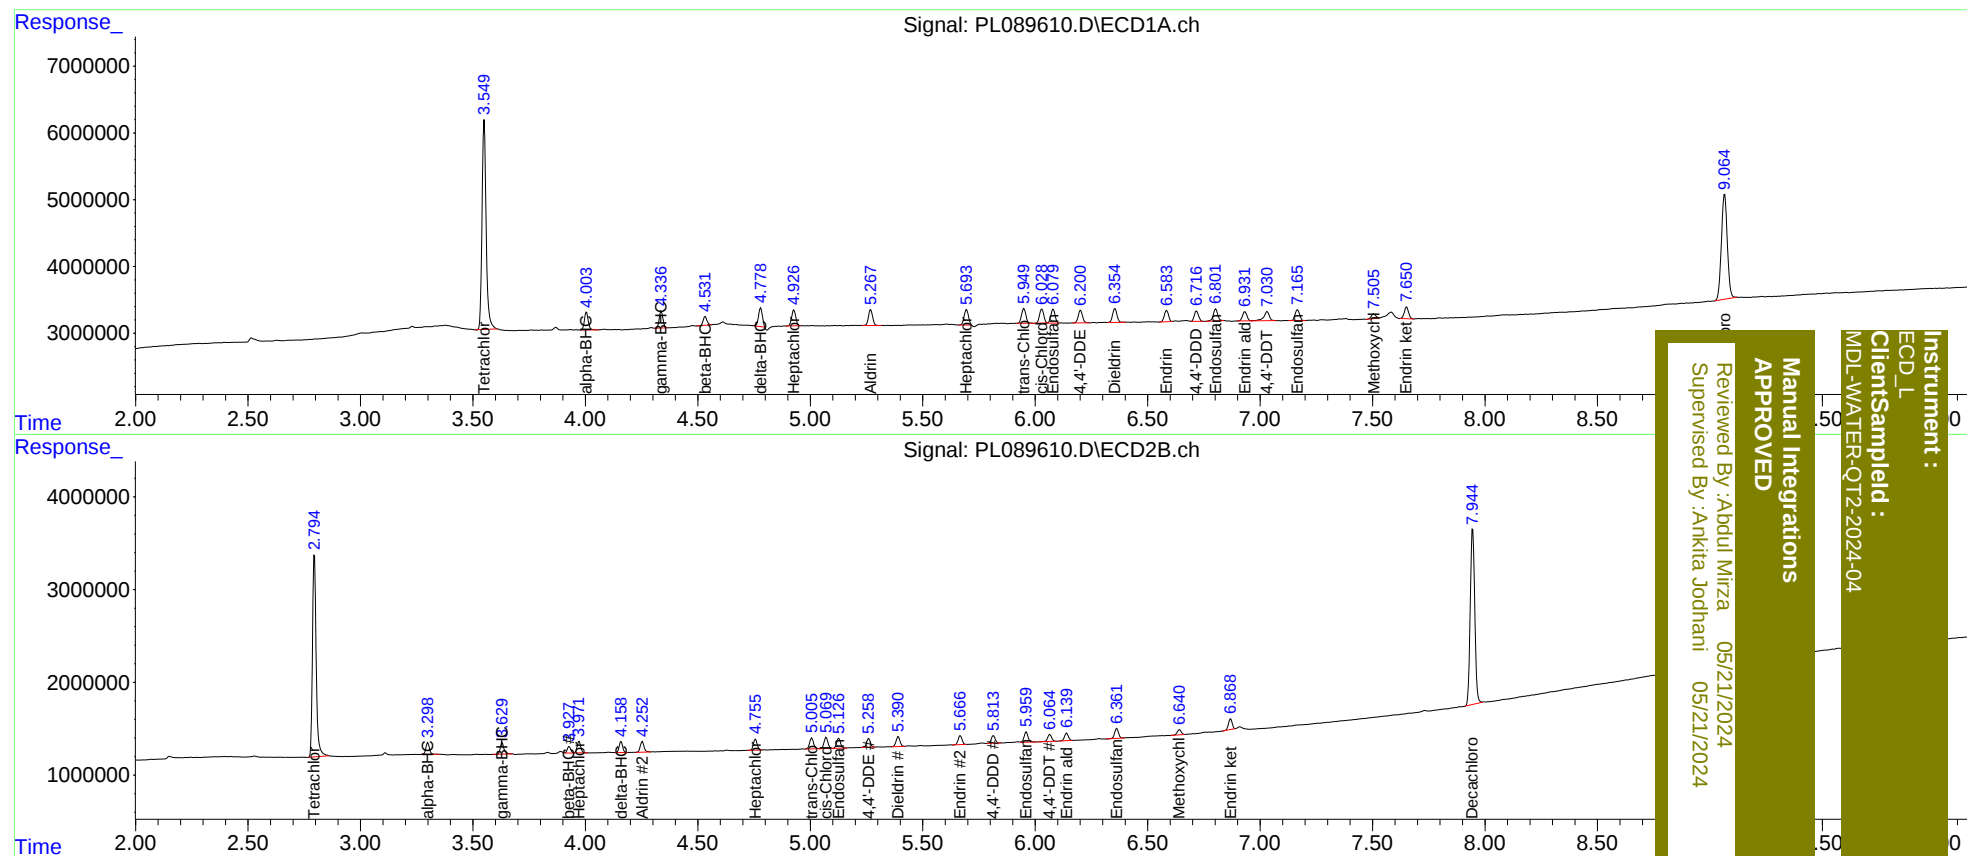

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/21/2024
Supervised By: Ankita Jodhani 05/21/2024

Instrument :
ECD_L
Client Sample :
MDL-WATER-QT2-2024-04